

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090420\
 Data File : PS012136.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Sep 2020 15:39
 Operator : DD\AJ
 Sample : PB131430BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 16:25:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.221	6.912	425.0E6	244.3E6	389.594	456.908
Target Compounds							
2) T	3,5-DICHL...	0.000	6.093	0	98716952	N.D.	120.003
3) T	4-Nitroph...	7.058	0.000	2116686	0	3.593	N.D. #
5) T	DICAMBA	7.399	7.075	15120240	3969724	3.691	1.837 #
6) T	MCP	7.630	0.000	9497530	0	2.973	N.D. #
7) T	MCPA	7.768	0.000	8619413	0	1.895	N.D. #
8) T	DICHLORPROP	0.000	7.736	0	38297940	N.D.	67.828
9) T	2,4-D	8.329	0.000	17167115	0	15.204	N.D. #
10) T	Pentachlo...	8.644	0.000	5985129	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	8.763	0	19055780	N.D.	6.518
12) T	2,4,5-T	9.411	0.000	31910888	0	5.385	N.D. #
15) T	Picloram	11.043	11.019	134.8E6	86916728	17.253	19.177
16) T	DCPA	11.468	10.936	19270859	25528419	2.534	6.943 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090420\
Data File : PS012136.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Sep 2020 15:39
Operator : DD\AJ
Sample : PB131430BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 16:25:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

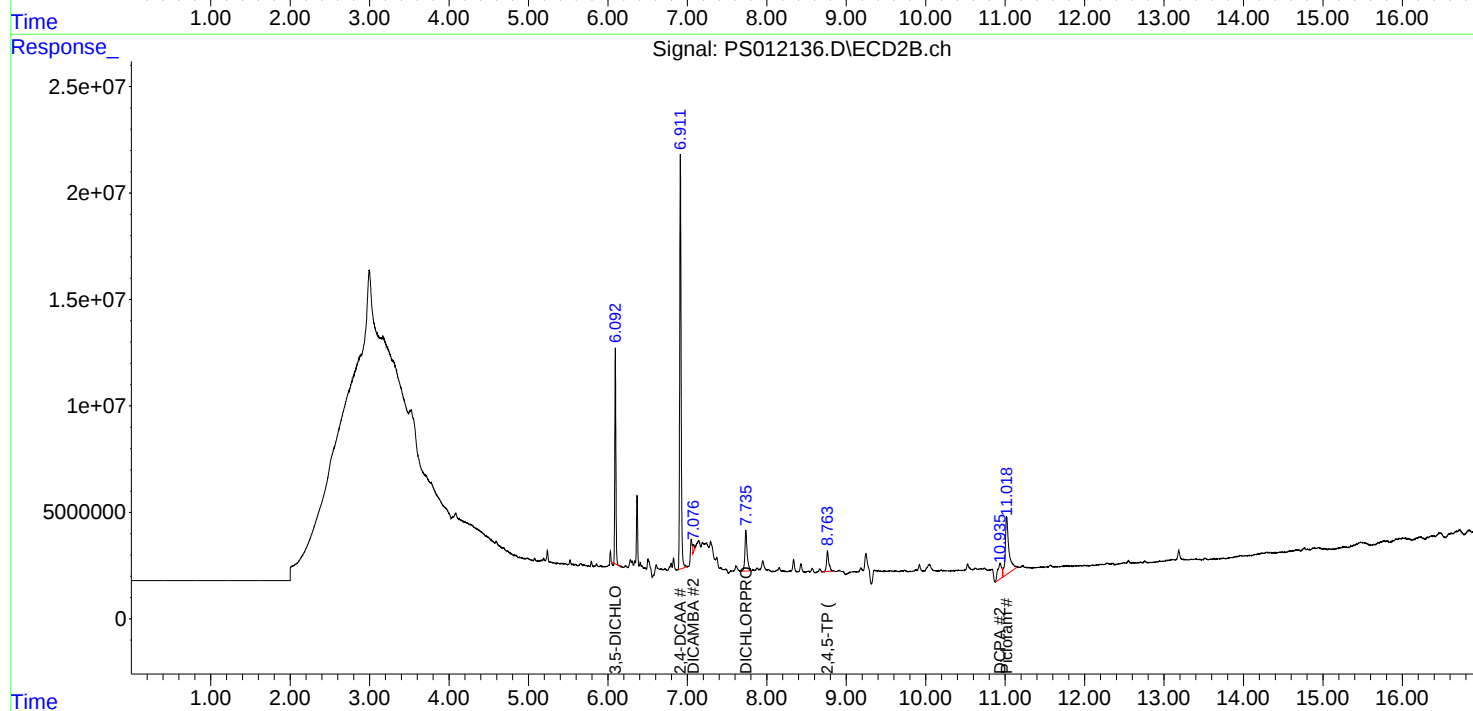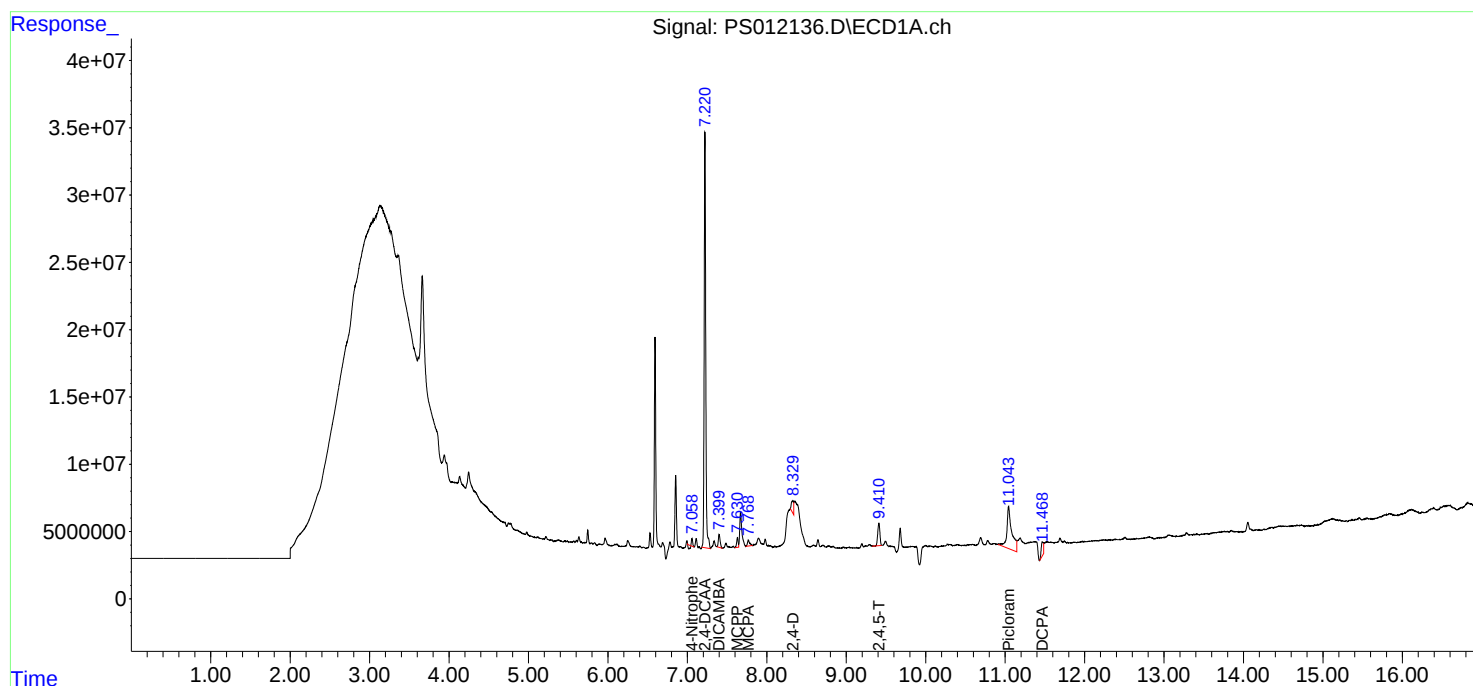


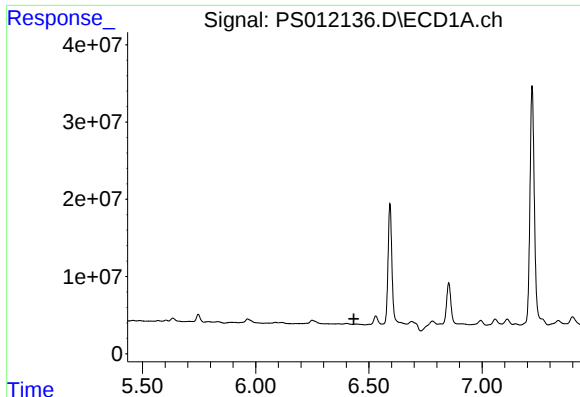

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

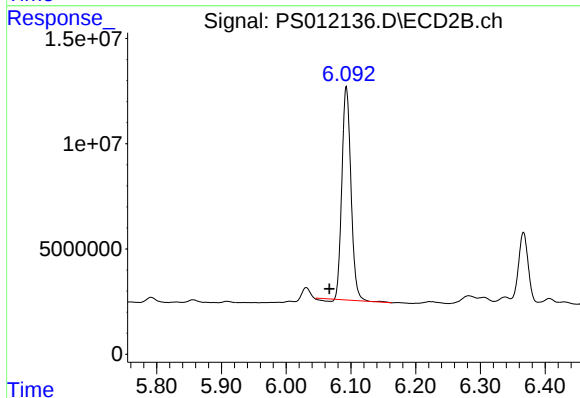


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.093 min
Delta R.T.: 0.026 min
Response: 98716952
Conc: 120.00 ng/ml

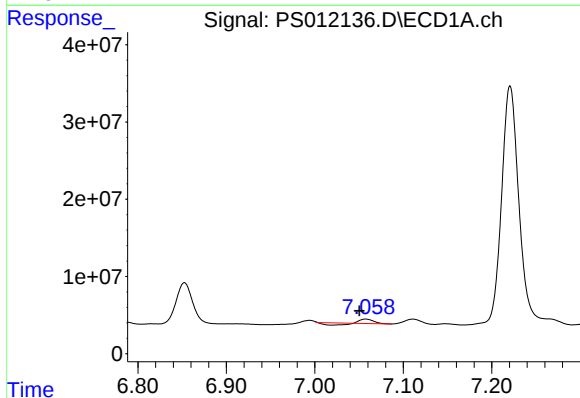


#3 4-Nitrophenol

R.T.: 7.058 min
Delta R.T.: 0.007 min
Response: 2116686
Conc: 3.59 ng/ml

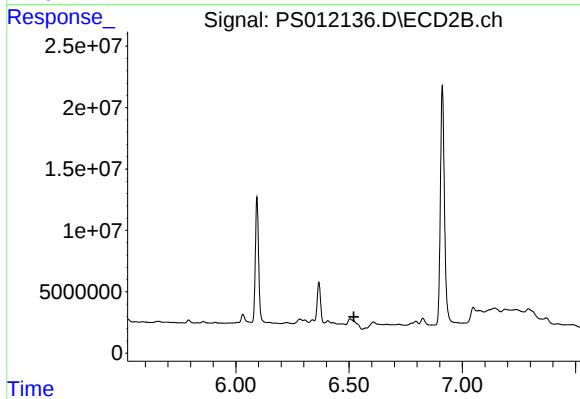

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.521 min
Response: 0
Conc: N.D.

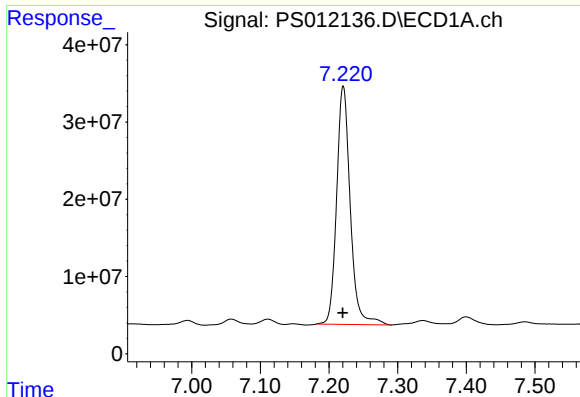

#4 2,4-DCAA


R.T.: 7.221 min
Delta R.T.: 0.000 min
Response: 424957295
Conc: 389.59 ng/ml

Instrument :
ECD_S
ClientSampleId :

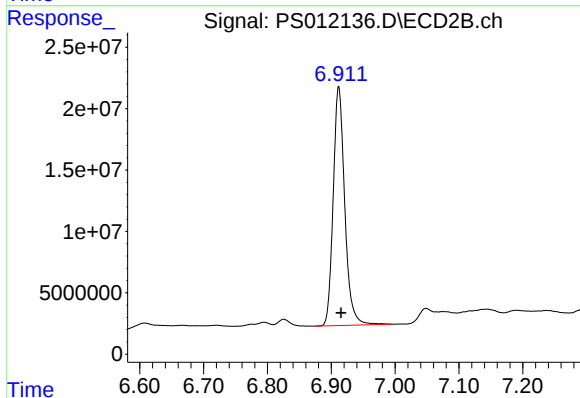


#4 2,4-DCAA

R.T.: 6.912 min
Delta R.T.: -0.003 min
Response: 244348396
Conc: 456.91 ng/ml

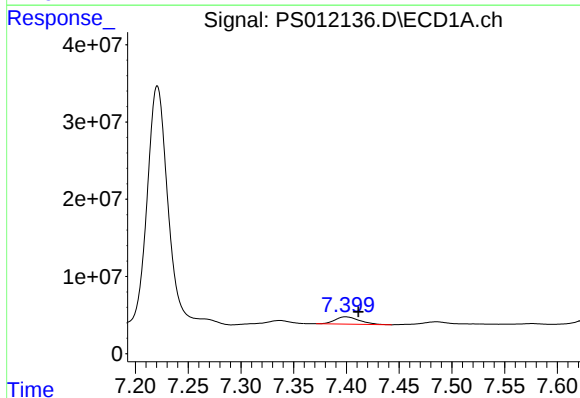


#5 DICAMBA

R.T.: 7.399 min
Delta R.T.: -0.012 min
Response: 15120240
Conc: 3.69 ng/ml

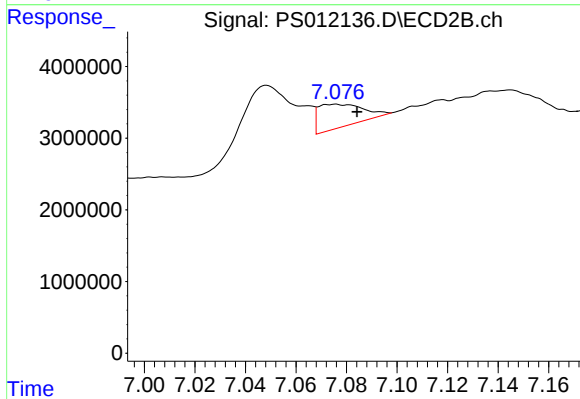

#5 DICAMBA


R.T.: 7.075 min
Delta R.T.: -0.009 min
Response: 3969724
Conc: 1.84 ng/ml

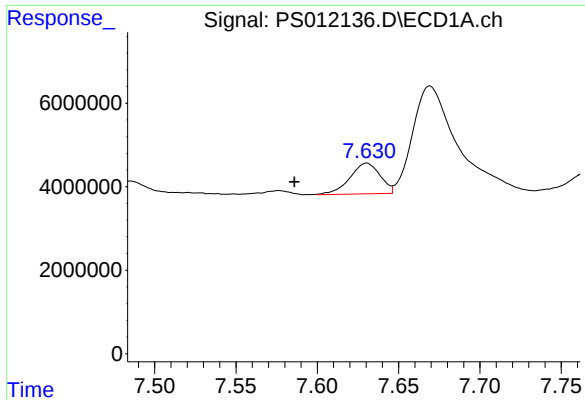

#6 MCPP


R.T.: 7.630 min
Delta R.T.: 0.044 min
Response: 9497530
Conc: 2.97 ug/ml

Instrument :
ECD_S
ClientSampleId :

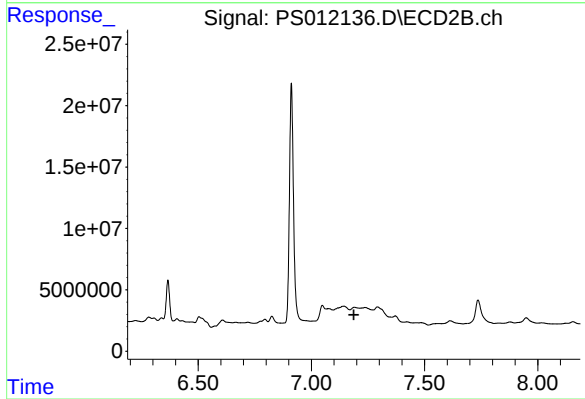


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

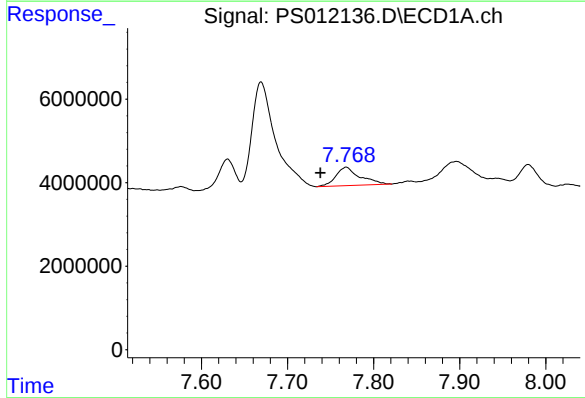


#7 MCPA

R.T.: 7.768 min
Delta R.T.: 0.030 min
Response: 8619413
Conc: 1.90 ug/ml

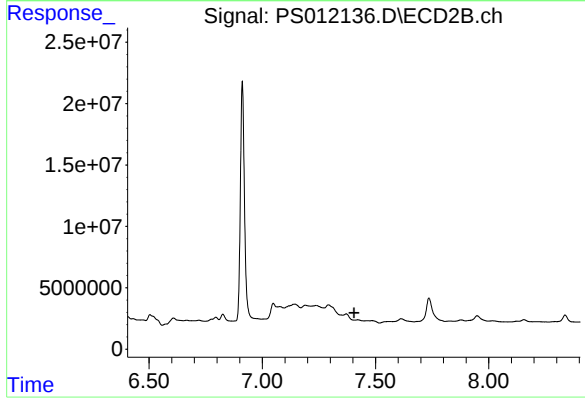

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.405 min
Response: 0
Conc: N.D.

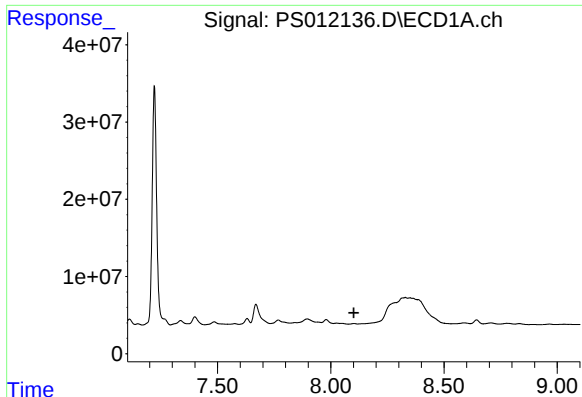

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

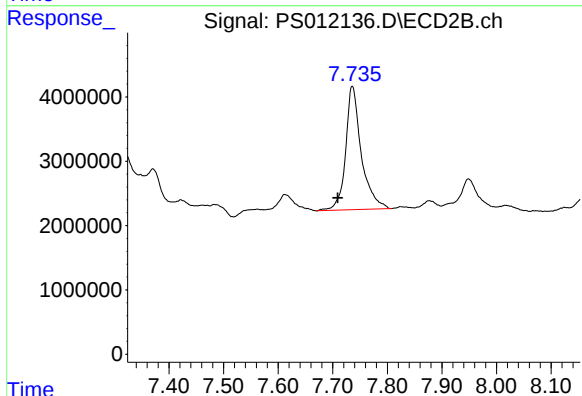


#8 DICHLORPROP

R.T.: 7.736 min
Delta R.T.: 0.026 min
Response: 38297940
Conc: 67.83 ng/ml

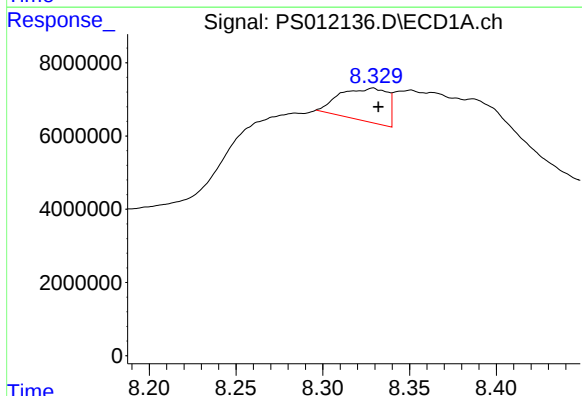


#9 2,4-D

R.T.: 8.329 min
Delta R.T.: -0.003 min
Response: 17167115
Conc: 15.20 ng/ml

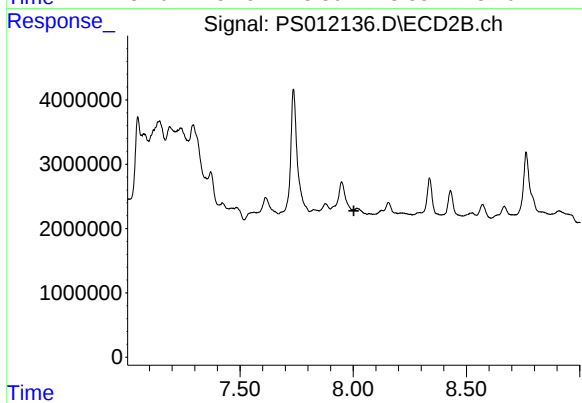

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.003 min
Response: 0
Conc: N.D.

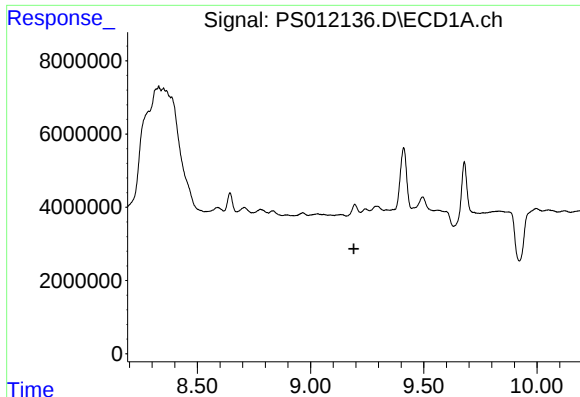

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

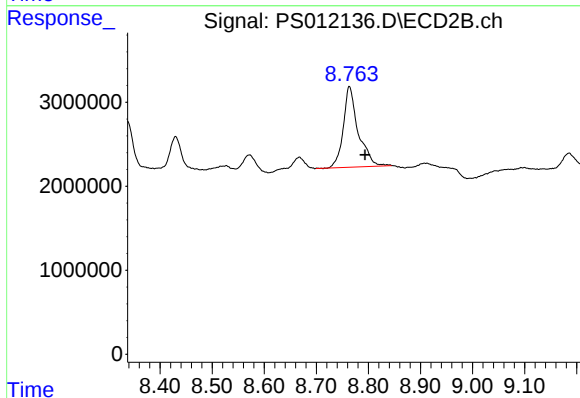


#11 2,4,5-TP (SILVEX)

R.T.: 8.763 min
Delta R.T.: -0.030 min
Response: 19055780
Conc: 6.52 ng/ml

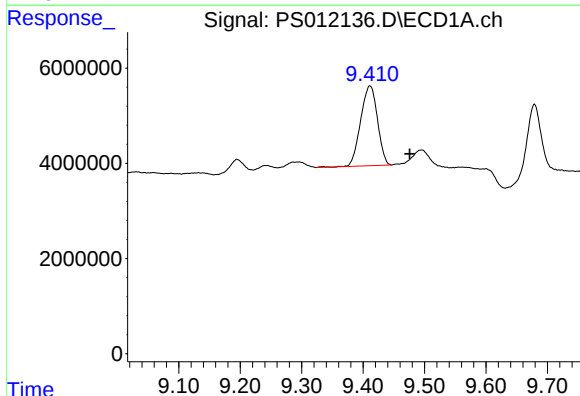


#12 2,4,5-T

R.T.: 9.411 min
Delta R.T.: -0.065 min
Response: 31910888
Conc: 5.39 ng/ml

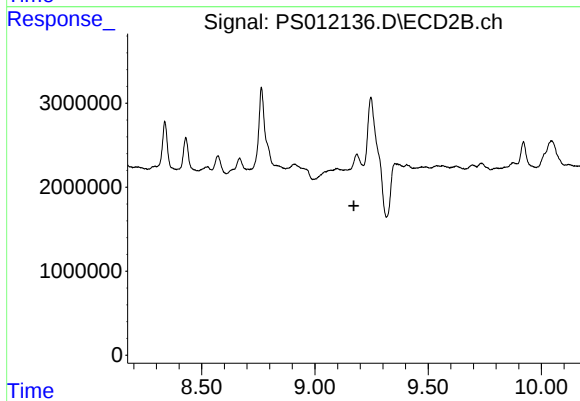

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.172 min
Response: 0
Conc: N.D.

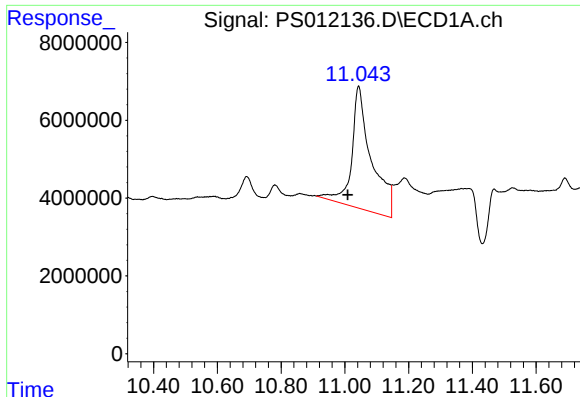

#15 Picloram


R.T.: 11.043 min
Delta R.T.: 0.034 min
Response: 134845296
Conc: 17.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

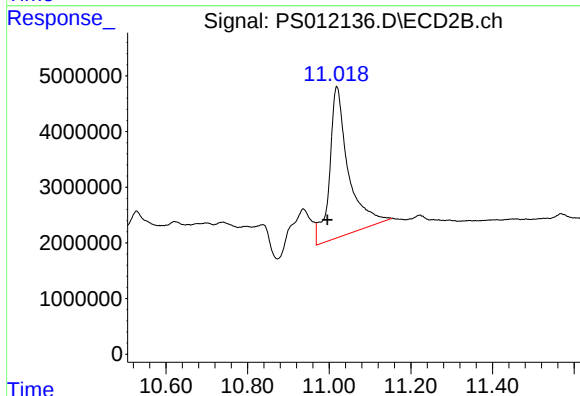


#15 Picloram

R.T.: 11.019 min
Delta R.T.: 0.023 min
Response: 86916728
Conc: 19.18 ng/ml

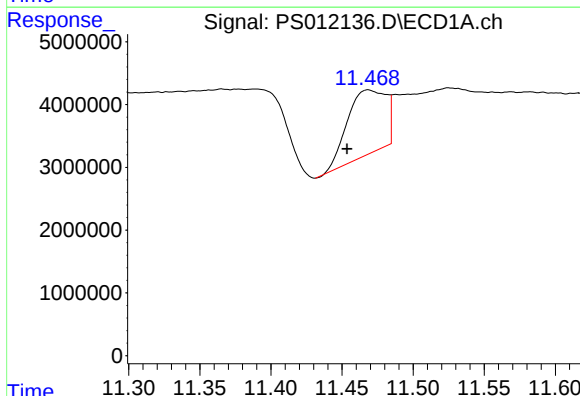

#16 DCPA

R.T.: 11.468 min
Delta R.T.: 0.015 min
Response: 19270859
Conc: 2.53 ng/ml

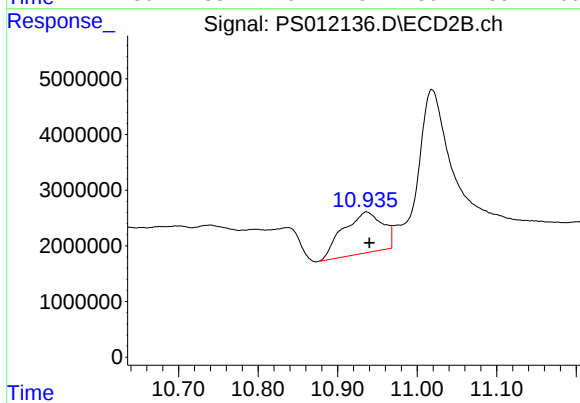

#16 DCPA

R.T.: 10.936 min
Delta R.T.: -0.004 min
Response: 25528419
Conc: 6.94 ng/ml