

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090424\
 Data File : PS027605.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Sep 2024 11:18
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 07:07:32 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090324.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 03 15:23:07 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.147	7.728	1219.6E6	988.1E6	480.965	514.014
Target Compounds							
1) T	Dalapon	0.000	2.721f	0	33252804	N.D.	9.583
3) T	4-Nitroph...	6.939	7.231f	13106133	5340592	8.792	4.145 #
5) T	DICAMBA	0.000	7.923	0	11002681	N.D.	1.239
6) T	MCP	0.000	8.018	0	579950	N.D.	<MDL
8) T	DICHLORPROP	8.044f	8.633	1642062	591214	<MDL	<MDL #
9) T	2,4-D	0.000	8.967	0	208157	N.D.	<MDL
10) T	Pentachlo...	8.534	9.489	1477651	829716	<MDL	<MDL #
11) T	2,4,5-TP ...	9.146f	9.867	2551125	1931780	<MDL	<MDL #
12) T	2,4,5-T	0.000	10.289	0	4093952	N.D.	<MDL
13) T	2,4-DB	9.962	0.000	5085225	0	2.390	N.D. #
14) T	DINOSEB	11.172f	11.226	1085901	381731	<MDL	<MDL #
15) T	Picloram	10.974	12.322	66524864	46764185	3.419	2.536 #
16) T	DCPA	0.000	12.223f	0	2691952	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090424\
Data File : PS027605.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Sep 2024 11:18
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 07:07:32 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090324.M
Quant Title : 8080.M
QLast Update : Tue Sep 03 15:23:07 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

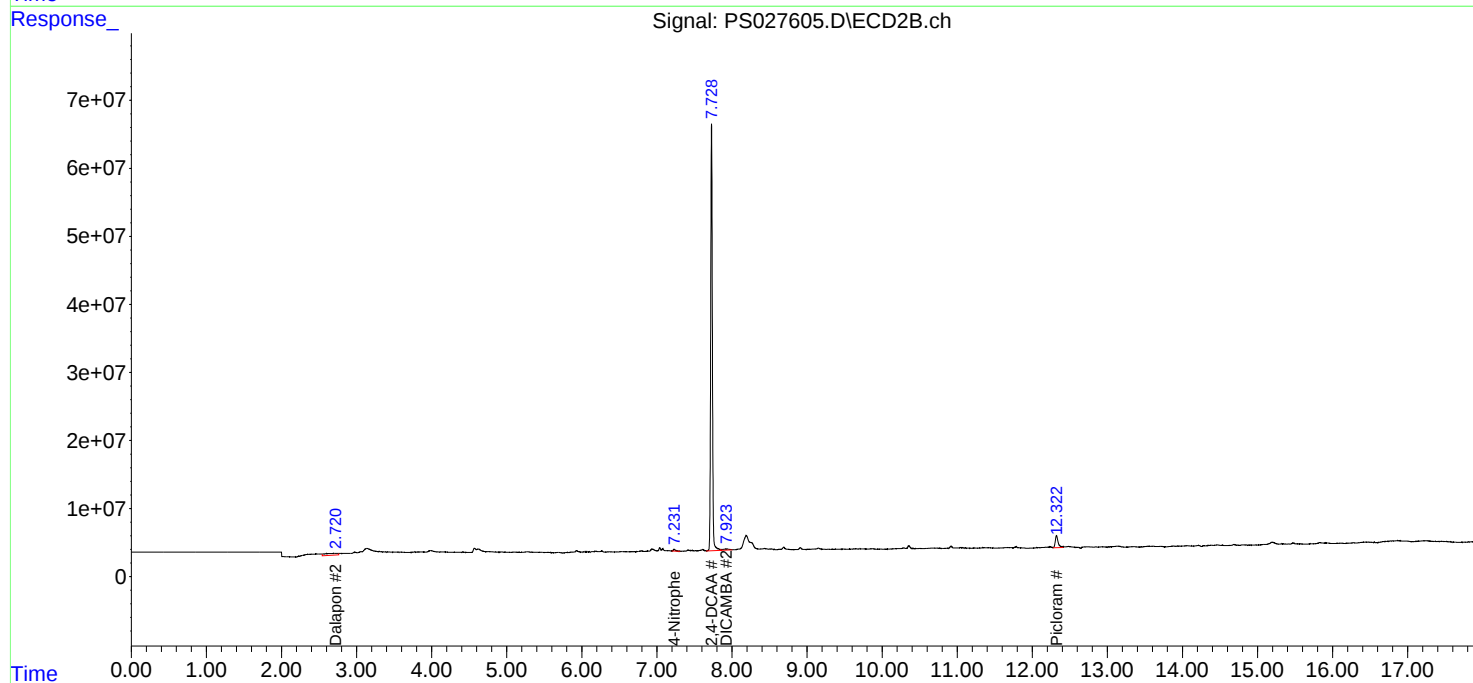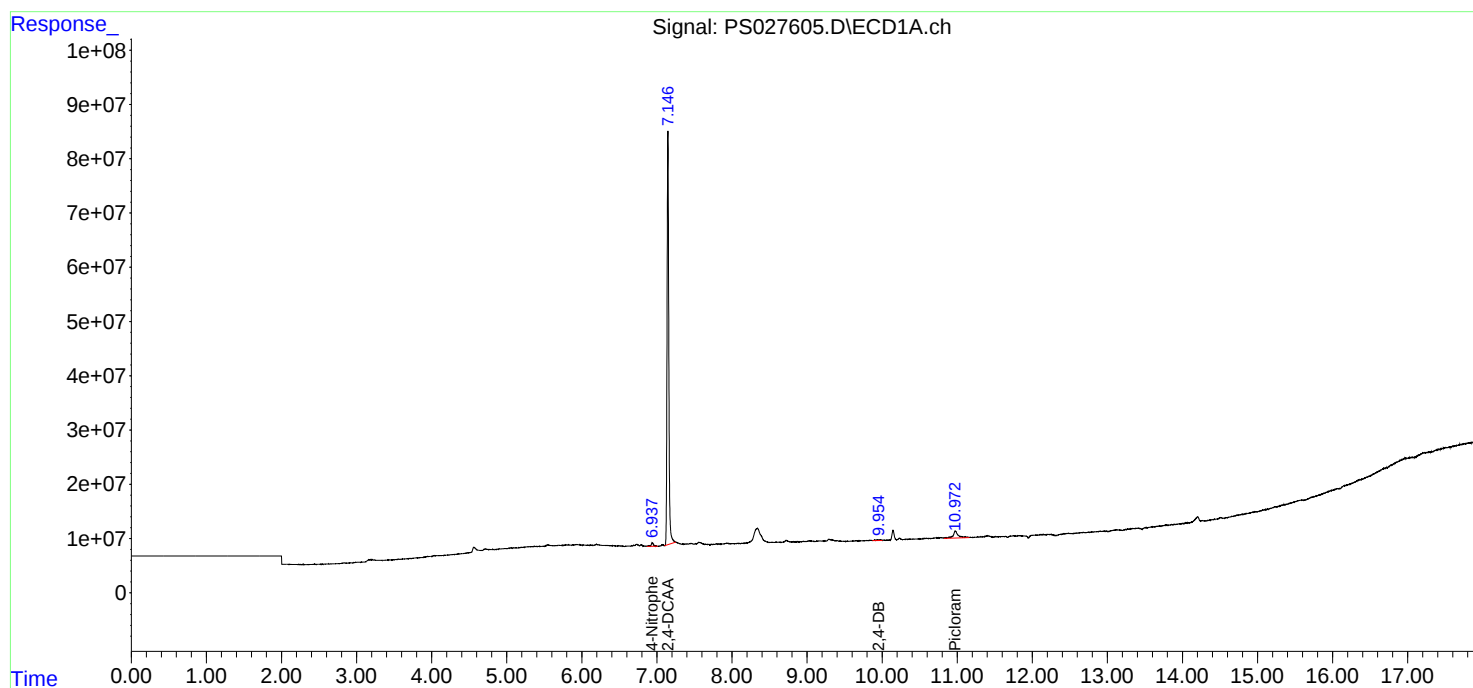


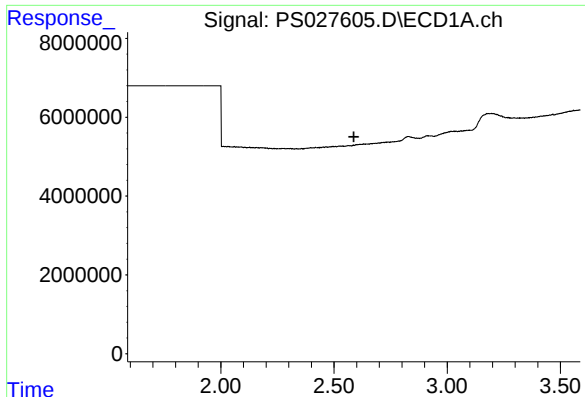

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.588 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

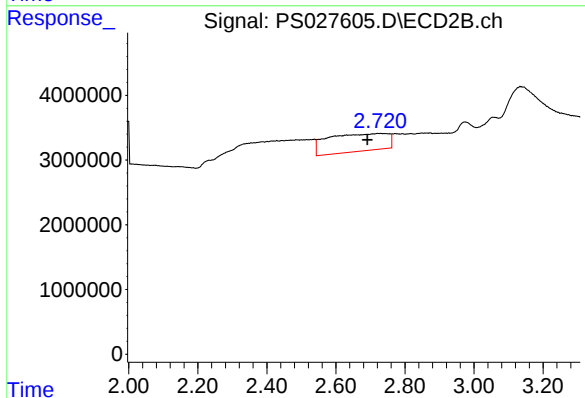


#1 Dalapon

R.T.: 2.721 min
Delta R.T.: 0.030 min
Response: 33252804
Conc: 9.58 ng/ml

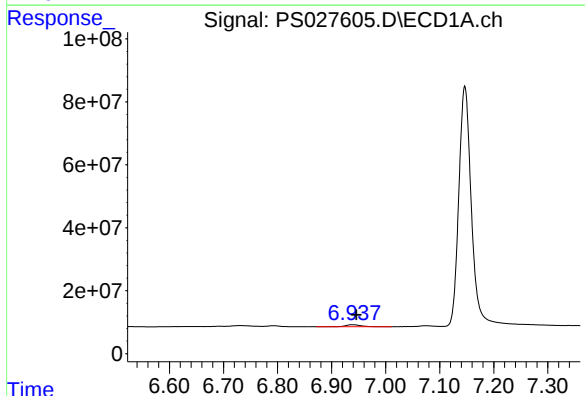


#3 4-Nitrophenol

R.T.: 6.939 min
Delta R.T.: -0.007 min
Response: 13106133
Conc: 8.79 ng/ml

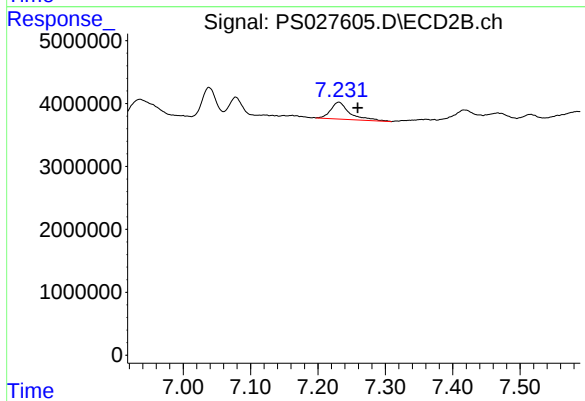

#3 4-Nitrophenol


R.T.: 7.231 min
Delta R.T.: -0.028 min
Response: 5340592
Conc: 4.15 ng/ml

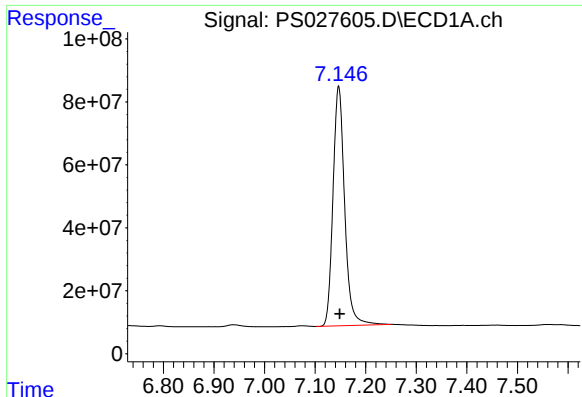

#4 2,4-DCAA


R.T.: 7.147 min
Delta R.T.: -0.002 min
Response: 1219638979
Conc: 480.97 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

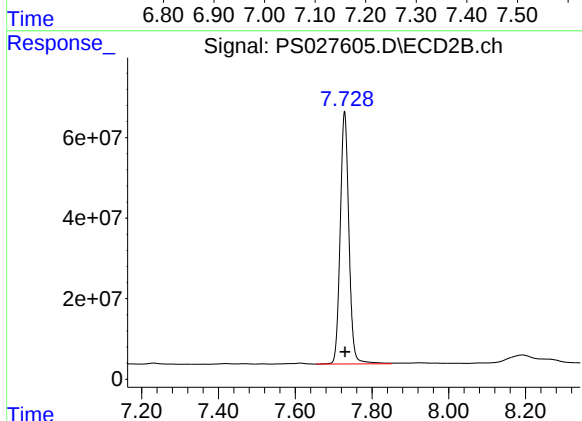


#4 2,4-DCAA

R.T.: 7.728 min
Delta R.T.: -0.001 min
Response: 988103245
Conc: 514.01 ng/ml

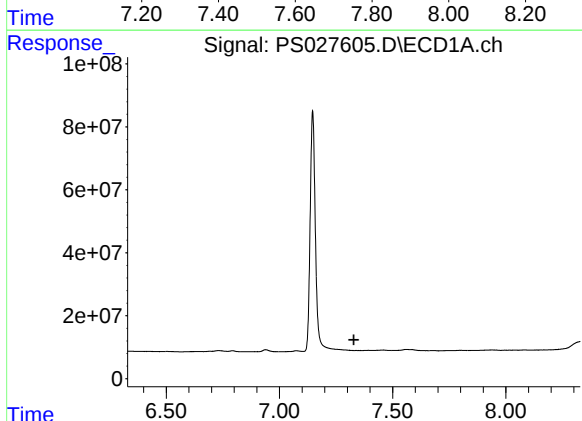


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.329 min
Response: 0
Conc: N.D.

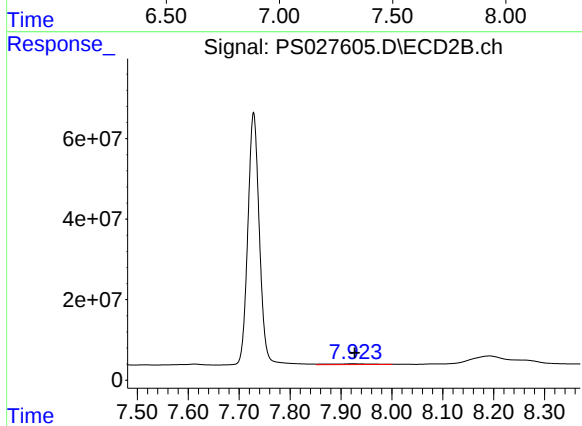

#5 DICAMBA


R.T.: 7.923 min
Delta R.T.: -0.003 min
Response: 11002681
Conc: 1.24 ng/ml

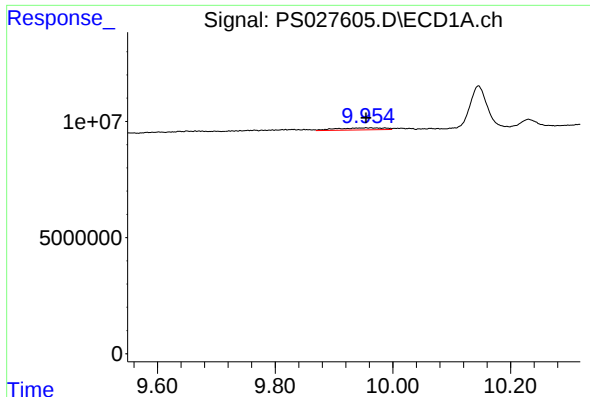

#13 2,4-DB


R.T.: 9.962 min
Delta R.T.: 0.007 min
Response: 5085225
Conc: 2.39 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

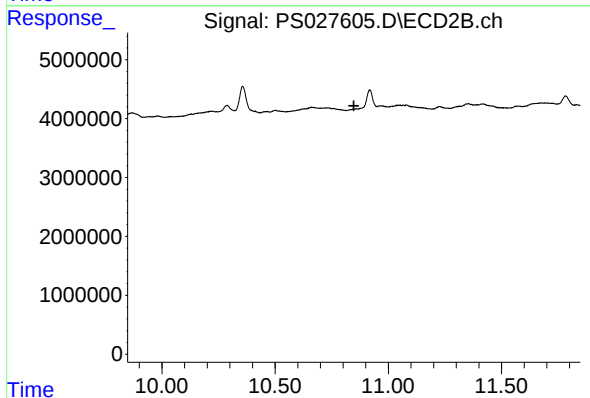


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.848 min
Response: 0
Conc: N.D.

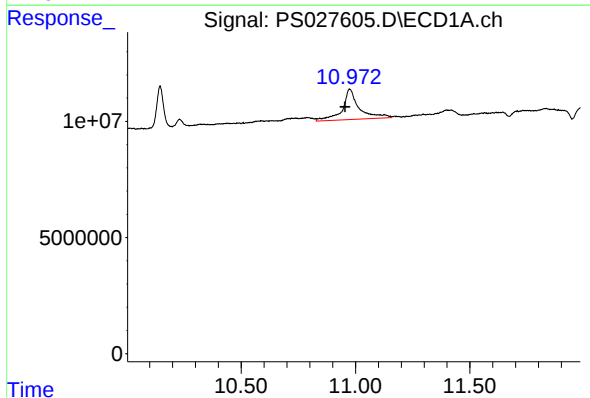

#15 Picloram

R.T.: 10.974 min
Delta R.T.: 0.019 min
Response: 66524864
Conc: 3.42 ng/ml

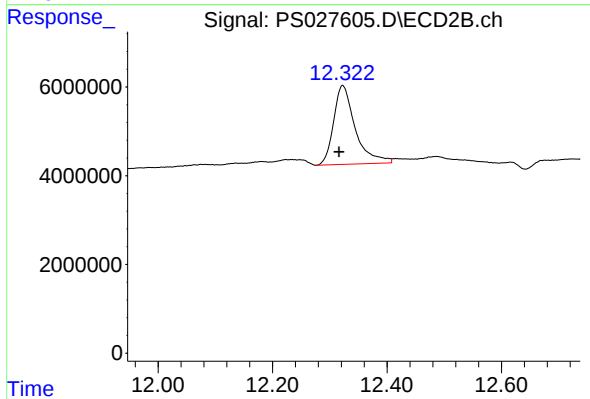

#15 Picloram

R.T.: 12.322 min
Delta R.T.: 0.006 min
Response: 46764185
Conc: 2.54 ng/ml