

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090425\
 Data File : PS031622.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Sep 2025 09:19
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 04:06:18 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
 Quant Title : 8080.M
 QLast Update : Fri Aug 08 03:17:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.287	7.746	1688.3E6	459.2E6	531.933	543.233
Target Compounds							
1) T	Dalapon	0.000	2.653f	0	66894229	N.D.	25.139
2) T	3,5-DICHL...	6.446	0.000	2170596	0	<MDL	N.D. #
7) T	MCPA	7.859f	0.000	426993	0	<MDL	N.D. #
8) T	DICHLORPROP	8.199	0.000	1039240	0	<MDL	N.D. #
10) T	Pentachlo...	8.713	9.515	10427750	13643885	<MDL	<MDL #
11) T	2,4,5-TP ...	9.299	0.000	6169459	0	<MDL	N.D. #
12) T	2,4,5-T	9.592	0.000	2379103	0	<MDL	N.D. #
13) T	2,4-DB	10.166	0.000	1217359	0	<MDL	N.D. #
14) T	DINOSEB	11.361	0.000	5707822	0	<MDL	N.D. #
15) T	Picloram	11.188	0.000	819985	0	<MDL	N.D. #
16) T	DCPA	11.656	12.321	6483491	269701	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090425\
Data File : PS031622.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Sep 2025 09:19
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 04:06:18 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
Quant Title : 8080.M
QLast Update : Fri Aug 08 03:17:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

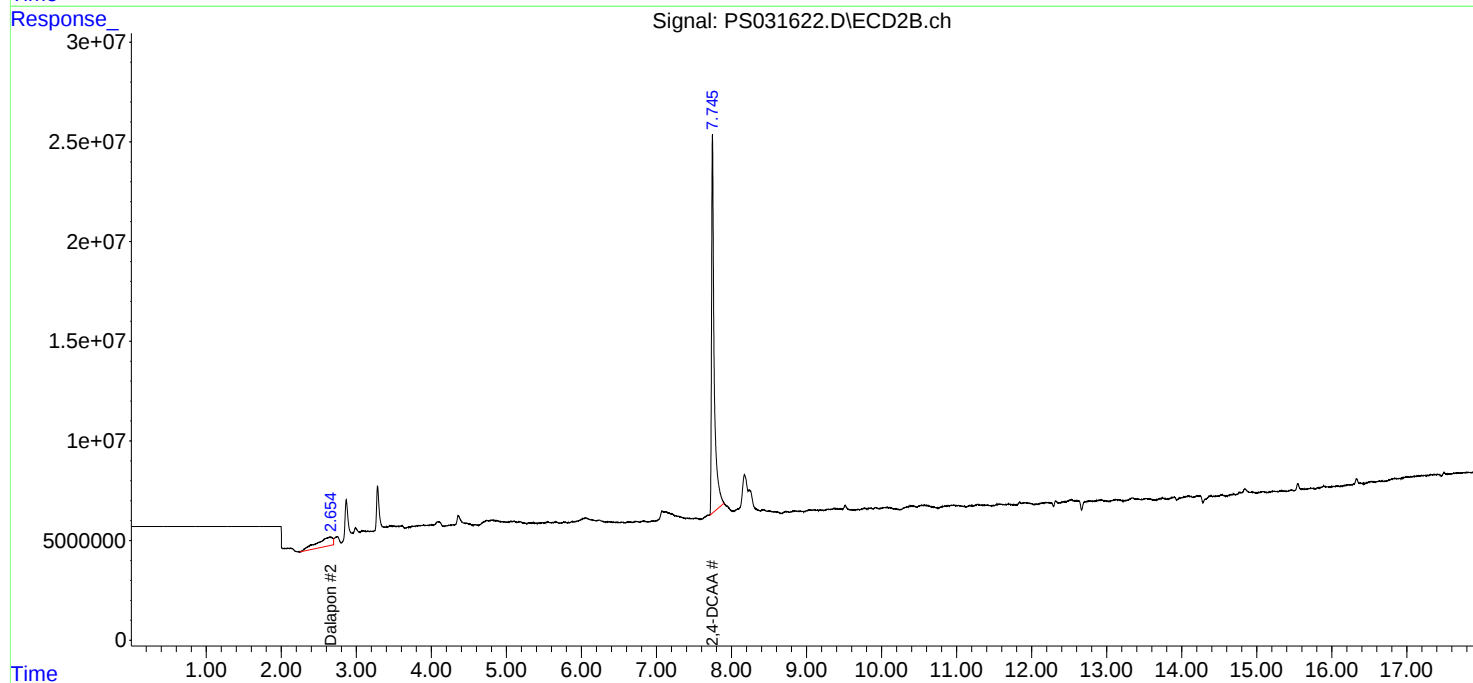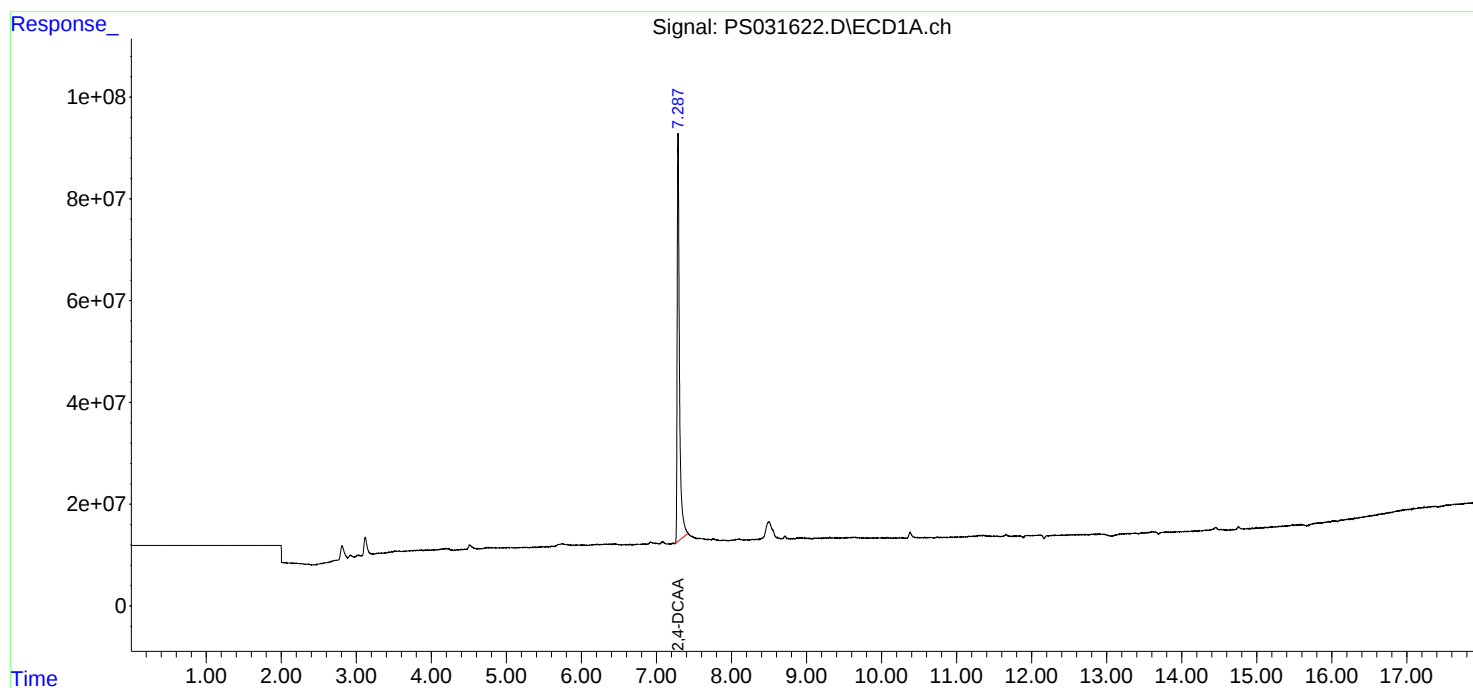


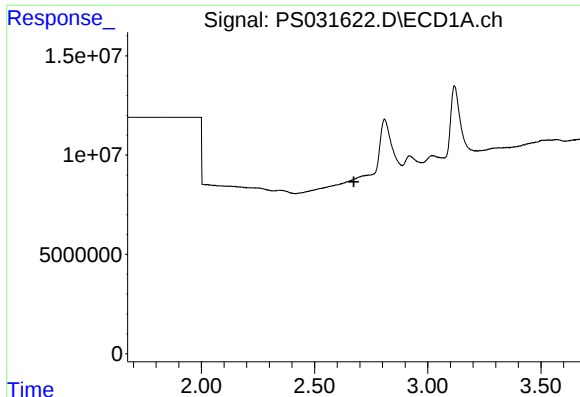

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.674 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

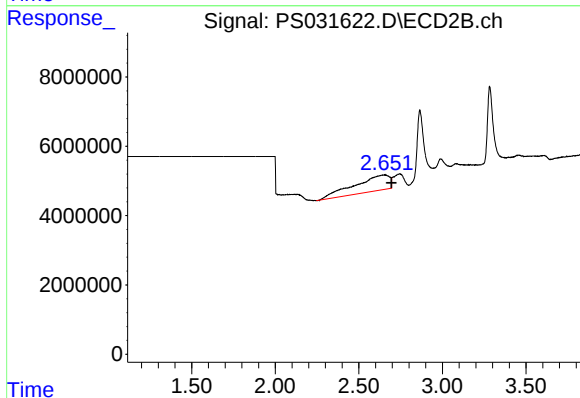


#1 Dalapon

R.T.: 2.653 min
Delta R.T.: -0.042 min
Response: 66894229
Conc: 25.14 ng/ml

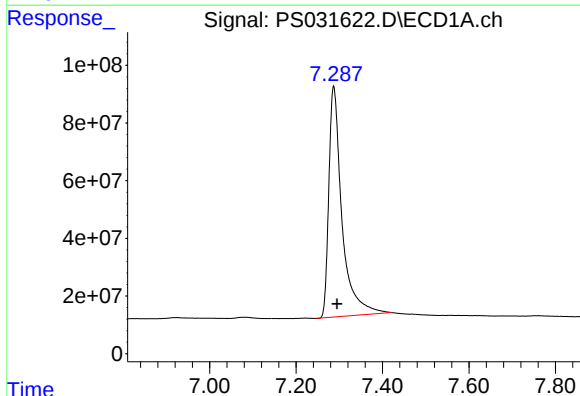

#4 2,4-DCAA

R.T.: 7.287 min
Delta R.T.: -0.008 min
Response: 1688347942
Conc: 531.93 ng/ml

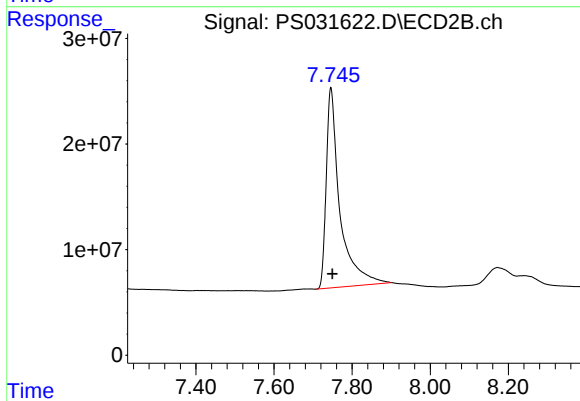

#4 2,4-DCAA

R.T.: 7.746 min
Delta R.T.: -0.003 min
Response: 459216291
Conc: 543.23 ng/ml