

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090525\
 Data File : PS031639.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Sep 2025 15:20
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 23:29:43 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
 Quant Title : 8080.M
 QLast Update : Fri Aug 08 03:17:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.287	7.746	1638.7E6	425.4E6	516.277	503.228
Target Compounds							
1) T	Dalapon	0.000	2.652f	0	72416845	N.D.	27.214
2) T	3,5-DICHL...	6.470	0.000	240030	0	<MDL	N.D. #
3) T	4-Nitroph...	7.083	0.000	430317	0	<MDL	N.D. #
5) T	DICAMBA	7.526f	0.000	65332	0	<MDL	N.D. #
7) T	MCPA	7.787	0.000	1560088	0	<MDL	N.D. #
8) T	DICHLORPROP	8.169	0.000	1903872	0	<MDL	N.D. #
9) T	2,4-D	0.000	9.009	0	1787113	N.D.	1.252
10) T	Pentachlo...	8.711	9.513	8040153	5457240	<MDL	<MDL #
11) T	2,4,5-TP ...	9.302	0.000	2311891	0	<MDL	N.D. #
12) T	2,4,5-T	9.599	0.000	704203	0	<MDL	N.D. #
13) T	2,4-DB	10.179	0.000	2940905	0	1.530	N.D. #
14) T	DINOSEB	11.362	0.000	4799071	0	<MDL	N.D. #
15) T	Picloram	11.204	0.000	265200	0	<MDL	N.D. #
16) T	DCPA	11.657	0.000	5526474	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090525\
Data File : PS031639.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Sep 2025 15:20
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 23:29:43 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
Quant Title : 8080.M
QLast Update : Fri Aug 08 03:17:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

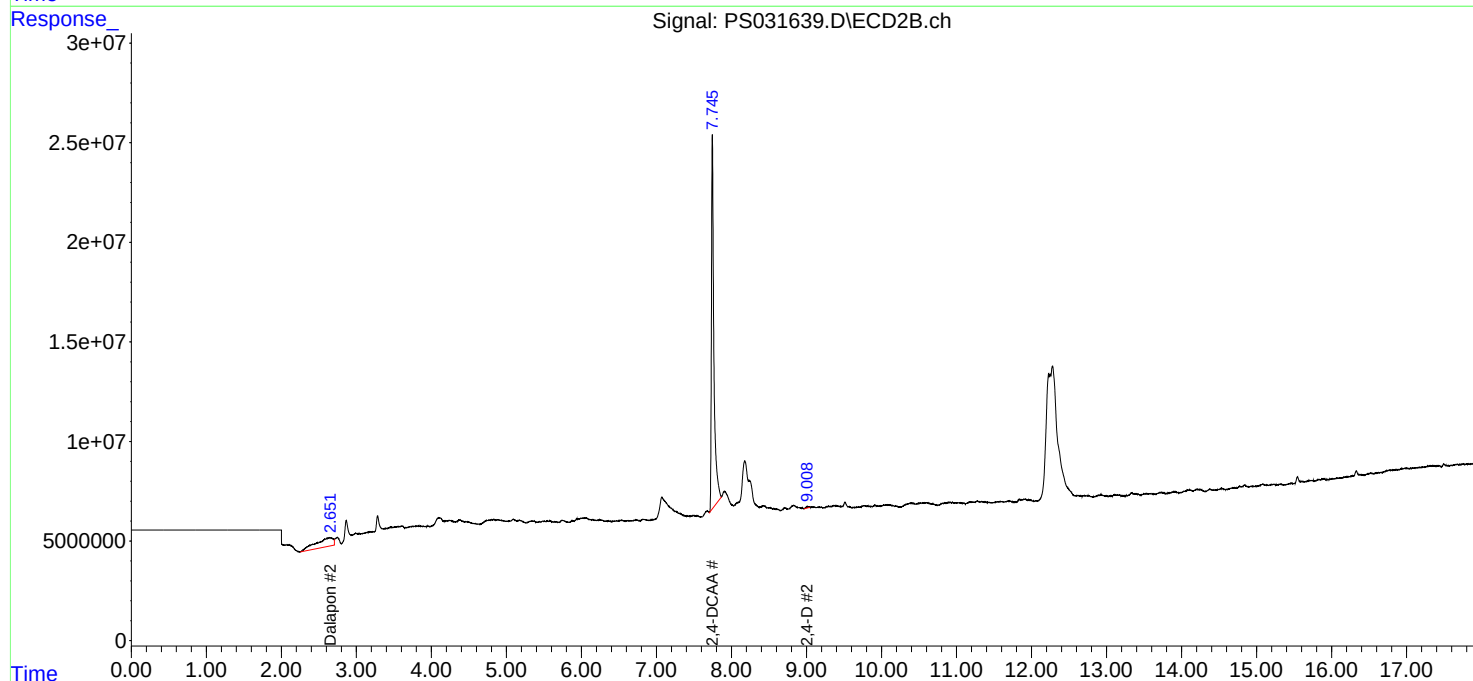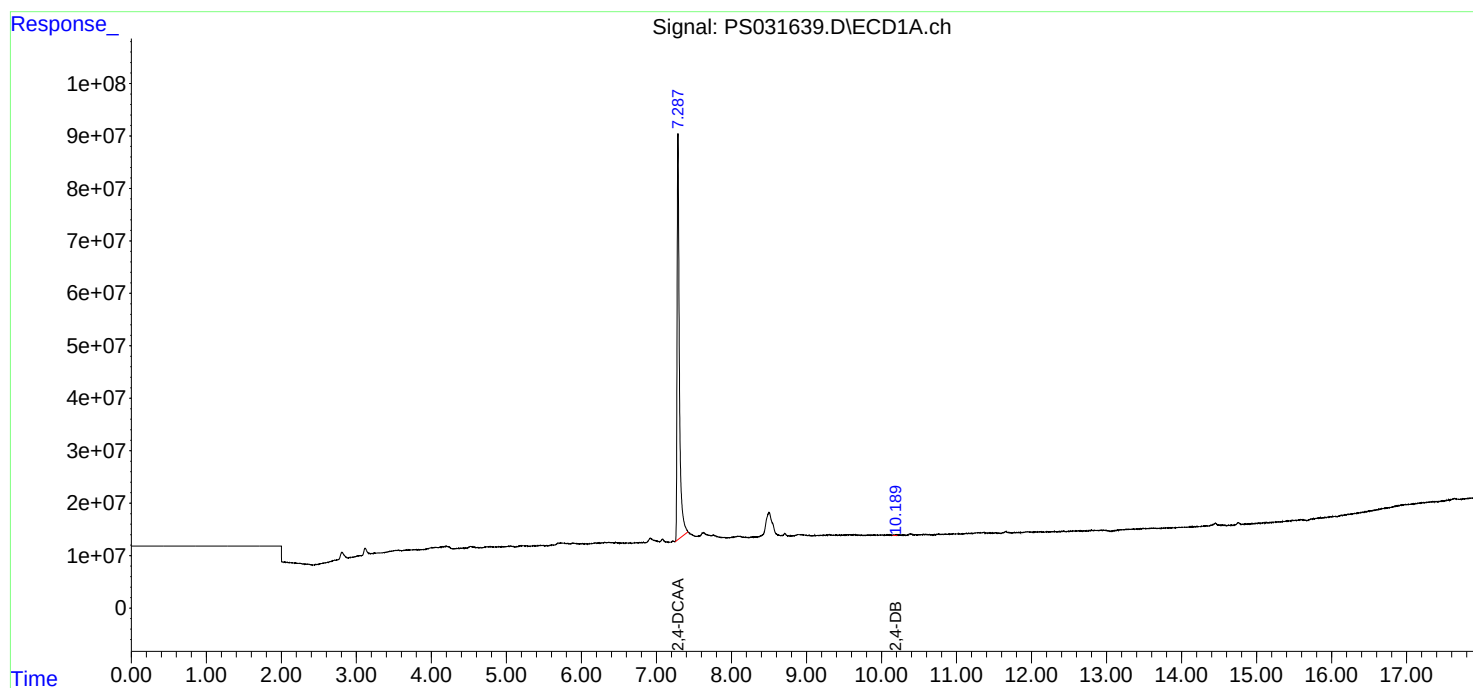


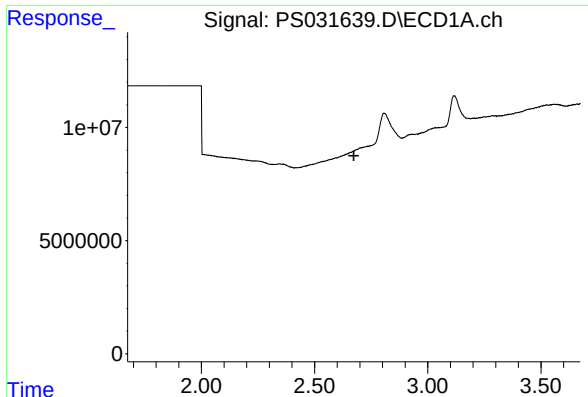

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.674 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

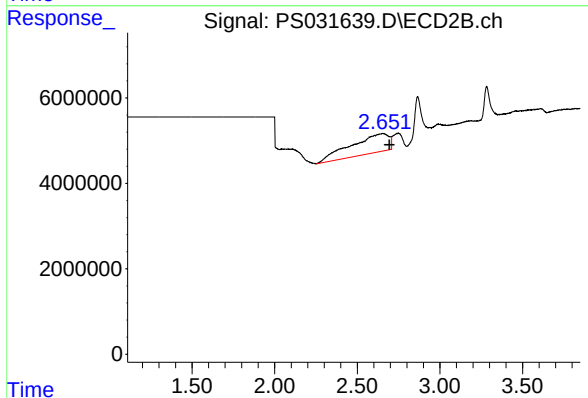


#1 Dalapon

R.T.: 2.652 min
Delta R.T.: -0.043 min
Response: 72416845
Conc: 27.21 ng/ml

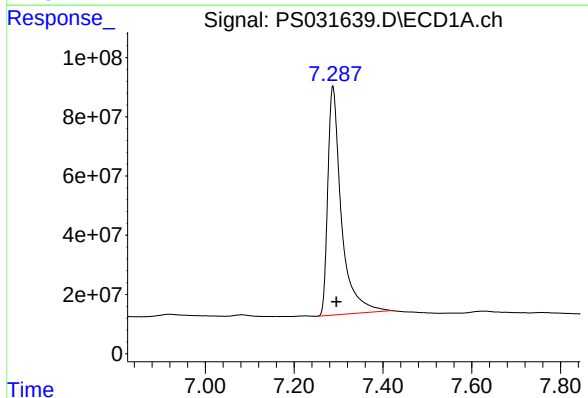


#4 2,4-DCAA

R.T.: 7.287 min
Delta R.T.: -0.008 min
Response: 1638657446
Conc: 516.28 ng/ml

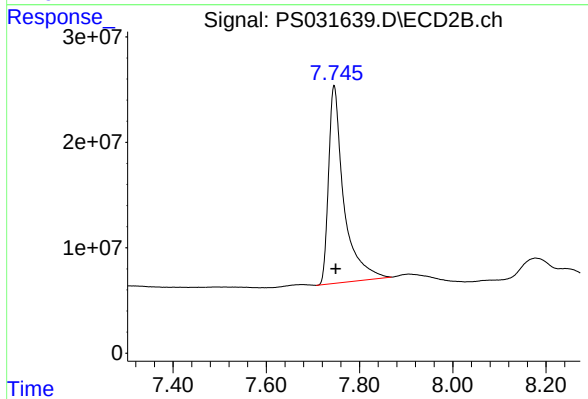

#4 2,4-DCAA


R.T.: 7.746 min
Delta R.T.: -0.004 min
Response: 425398898
Conc: 503.23 ng/ml

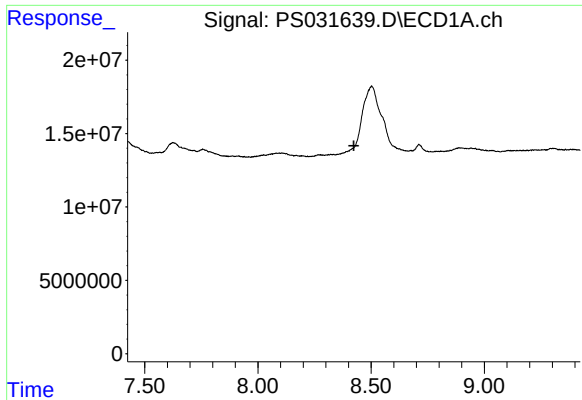

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.424 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

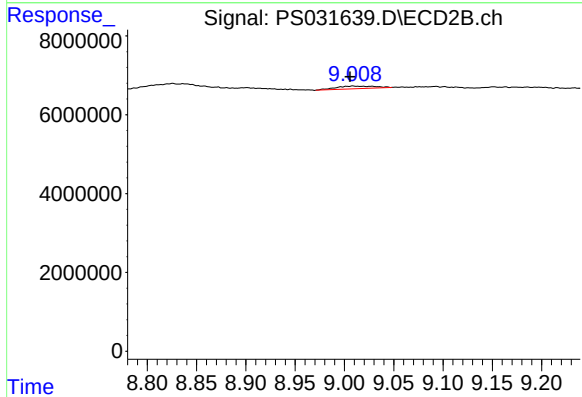


#9 2,4-D

R.T.: 9.009 min
Delta R.T.: 0.003 min
Response: 1787113
Conc: 1.25 ng/ml

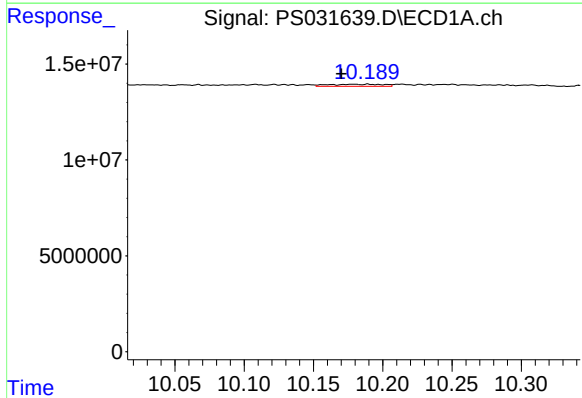

#13 2,4-DB

R.T.: 10.179 min
Delta R.T.: 0.009 min
Response: 2940905
Conc: 1.53 ng/ml

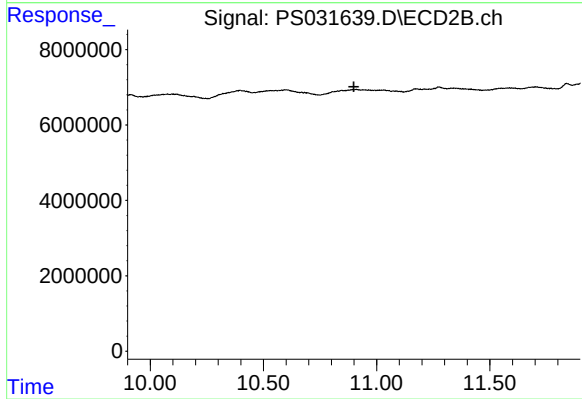

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 10.899 min
Response: 0
Conc: N.D.