

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090619\
 Data File : PS006594.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Sep 2019 22:09
 Operator : SM\AJ
 Sample : K4683-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 07 03:00:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.484	5.213	180.0E6	114.9E6	208.546	233.610
Target Compounds							
1) T	Dalapon	0.000	1.738	0	120.0E6	N.D.	191.256
2) T	3,5-DICHL...	4.864	4.541	205.7E6	30105791	190.824	49.704 #
5) T	DICAMBA	0.000	5.355	0	110.6E6	N.D.	59.974
7) T	MCPA	5.961	5.594	18513883	16098661	5.864	7.877 #
8) T	DICHLORPROP	6.310	0.000	147.5E6	0	194.538	N.D. #
9) T	2,4-D	6.497	0.000	601.9E6	0	738.743	N.D. #
10) T	Pentachlo...	6.742	0.000	25198842	0	2.132	N.D. #
11) T	2,4,5-TP ...	0.000	6.838	0	21310854	N.D.	8.190
13) T	2,4-DB	8.091	0.000	79305341	0	127.340	N.D. #
15) T	Picloram	9.029	0.000	20641756	0	2.774	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090619\
Data File : PS006594.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Sep 2019 22:09
Operator : SM\AJ
Sample : K4683-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 07 03:00:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

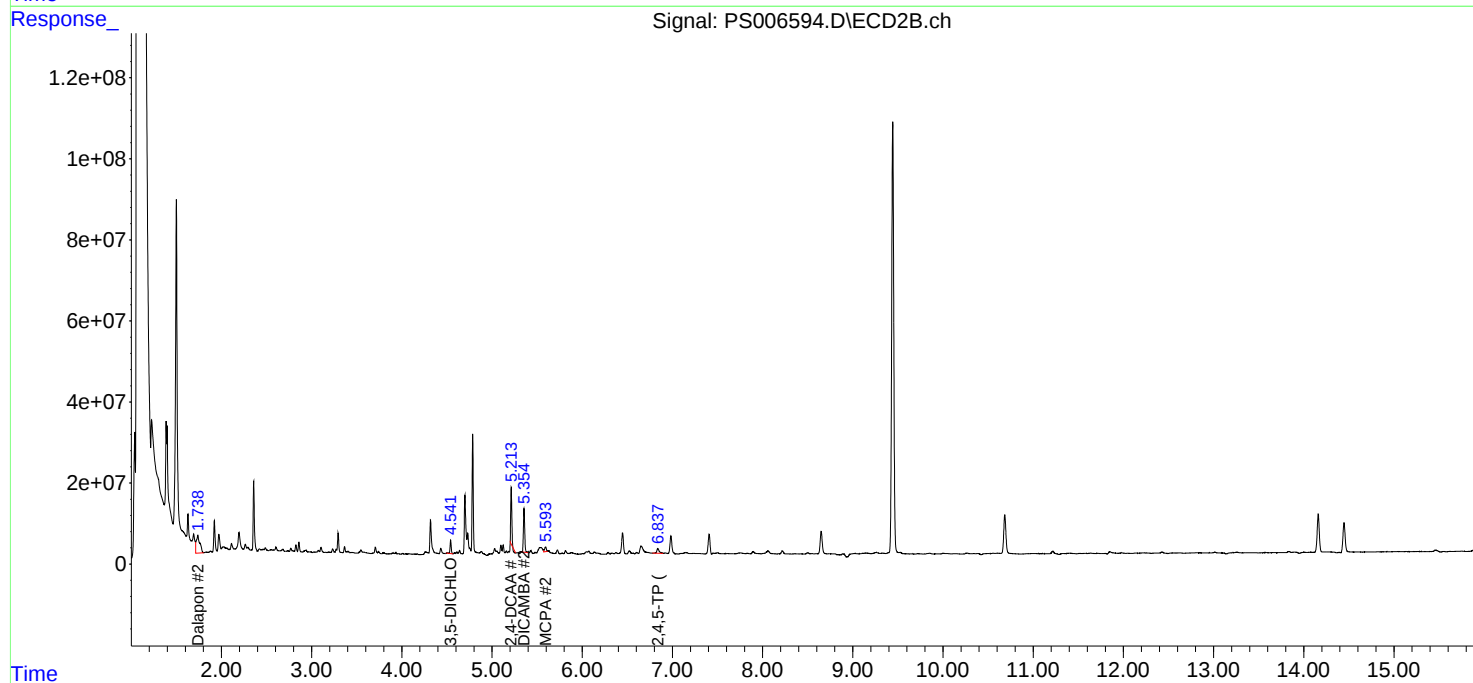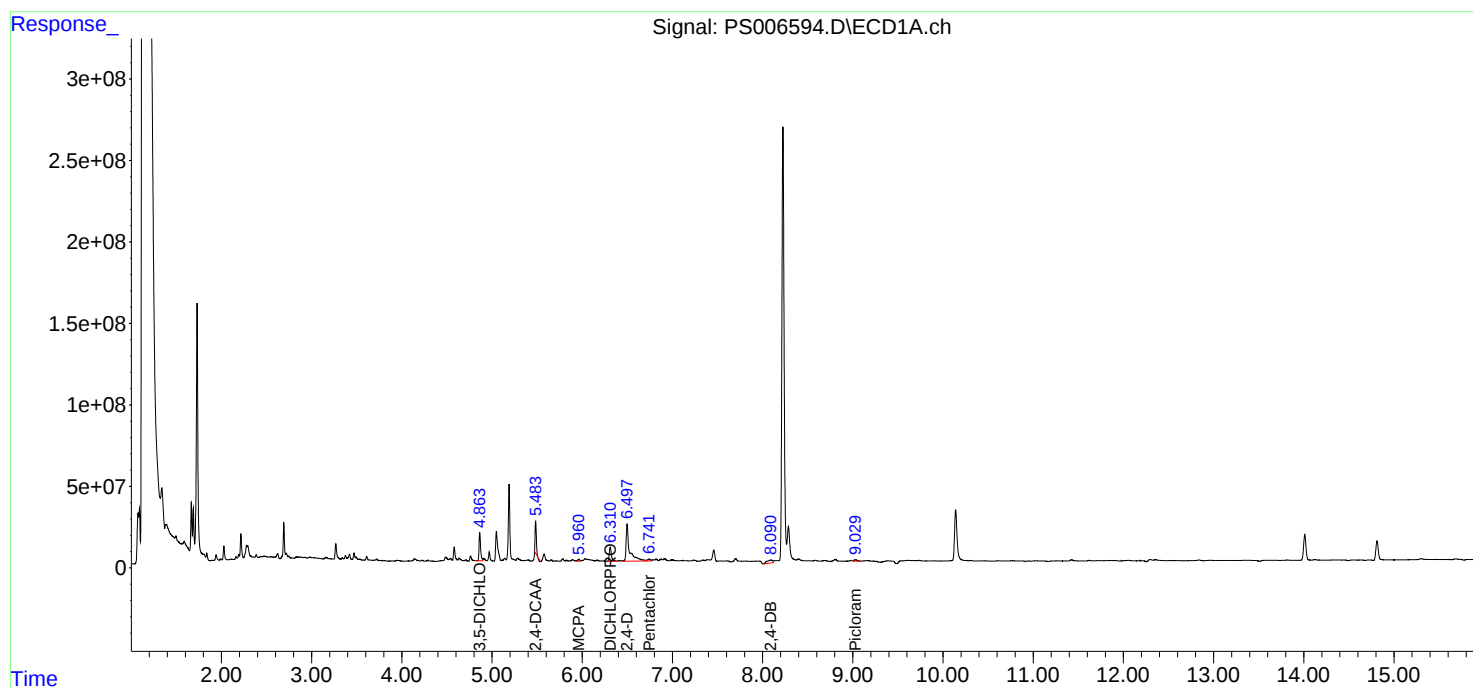


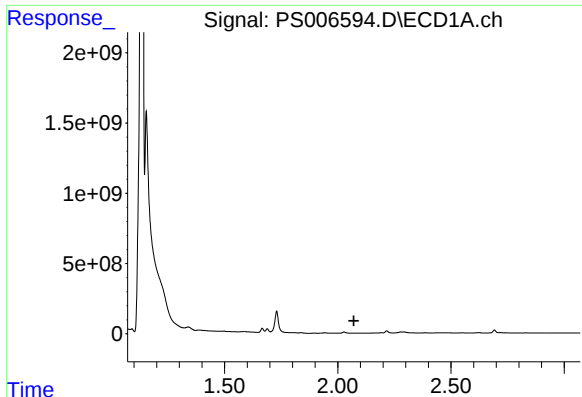

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.071 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

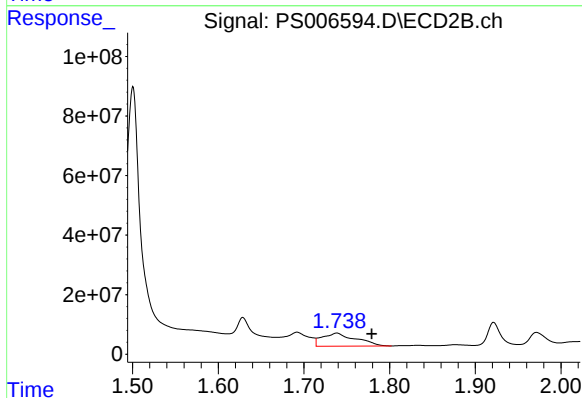


#1 Dalapon

R.T.: 1.738 min
Delta R.T.: -0.041 min
Response: 120012105
Conc: 191.26 ng/ml

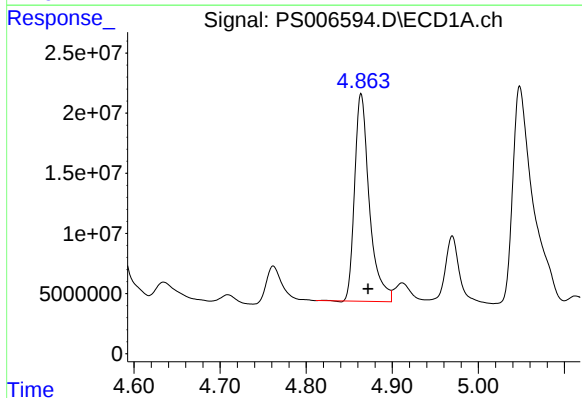


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.864 min
Delta R.T.: -0.008 min
Response: 205733549
Conc: 190.82 ng/ml

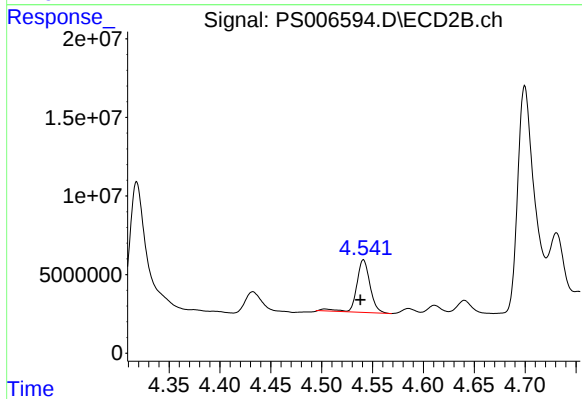

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.541 min
Delta R.T.: 0.003 min
Response: 30105791
Conc: 49.70 ng/ml

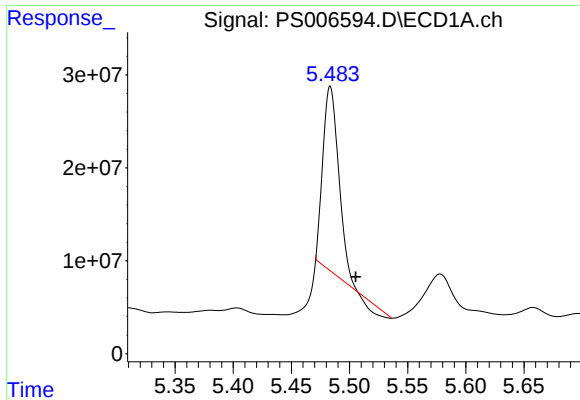

#4 2,4-DCAA


R.T.: 5.484 min
Delta R.T.: -0.022 min
Response: 180017123
Conc: 208.55 ng/ml

Instrument :
ECD_S
ClientSampleId :

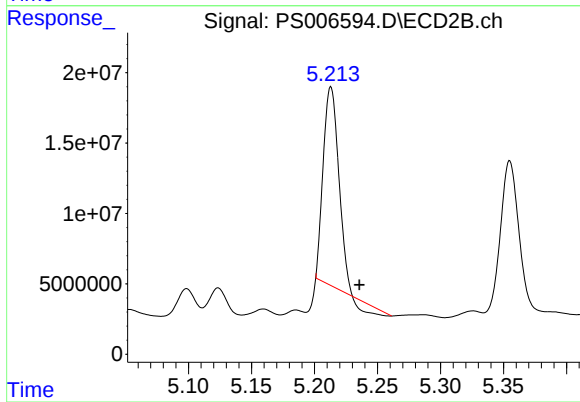


#4 2,4-DCAA

R.T.: 5.213 min
Delta R.T.: -0.023 min
Response: 114901366
Conc: 233.61 ng/ml

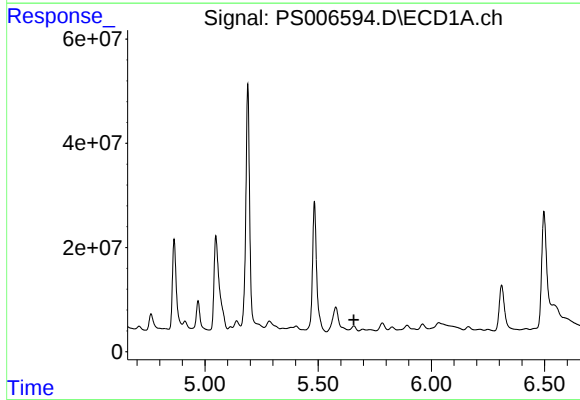


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.658 min
Response: 0
Conc: N.D.

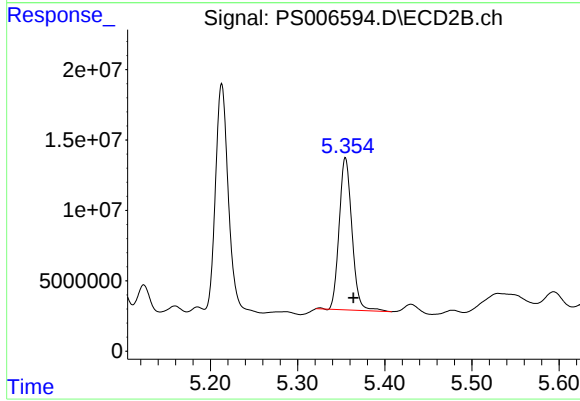

#5 DICAMBA


R.T.: 5.355 min
Delta R.T.: -0.009 min
Response: 110621647
Conc: 59.97 ng/ml

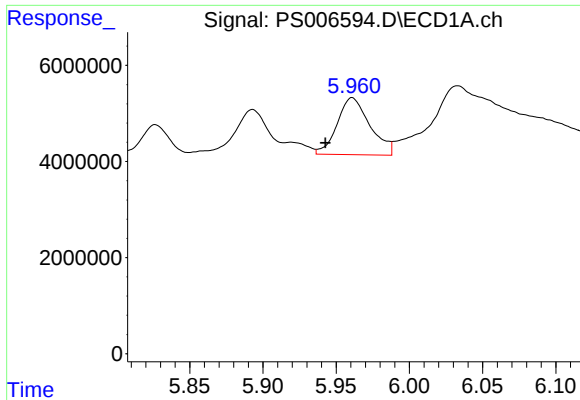

#7 MCPA


R.T.: 5.961 min
Delta R.T.: 0.018 min
Response: 18513883
Conc: 5.86 ug/ml

Instrument :
ECD_S
ClientSampleId :

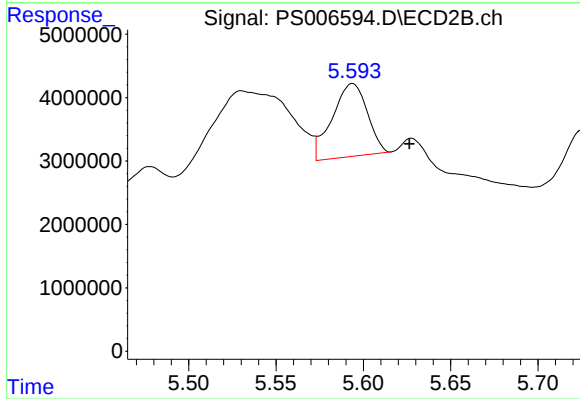


#7 MCPA

R.T.: 5.594 min
Delta R.T.: -0.033 min
Response: 16098661
Conc: 7.88 ug/ml

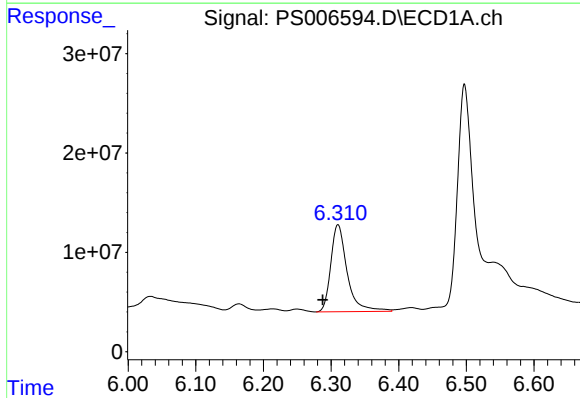


#8 DICHLORPROP

R.T.: 6.310 min
Delta R.T.: 0.022 min
Response: 147532337
Conc: 194.54 ng/ml

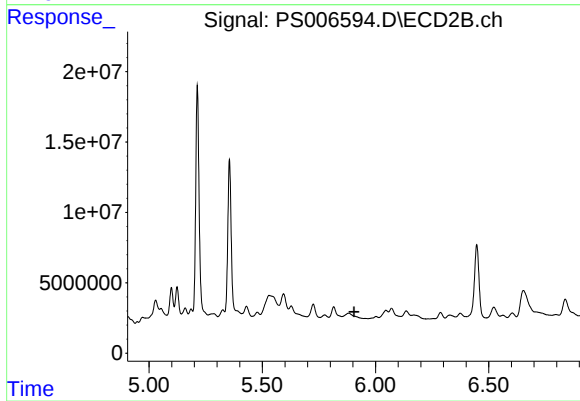

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 5.905 min
Response: 0
Conc: N.D.

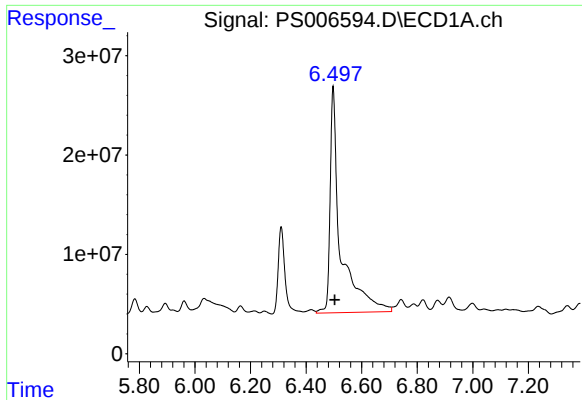

#9 2,4-D


R.T.: 6.497 min
Delta R.T.: -0.005 min
Response: 601915983
Conc: 738.74 ng/ml

Instrument :
ECD_S
ClientSampleId :

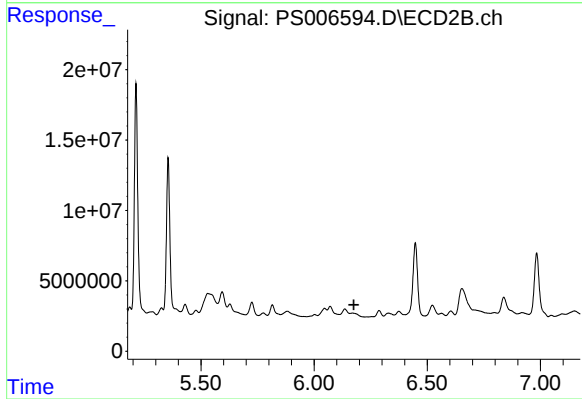


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.176 min
Response: 0
Conc: N.D.

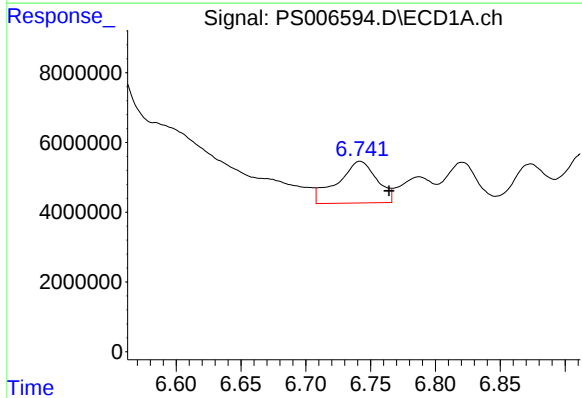


#10 Pentachlorophenol

R.T.: 6.742 min
Delta R.T.: -0.022 min
Response: 25198842
Conc: 2.13 ng/ml

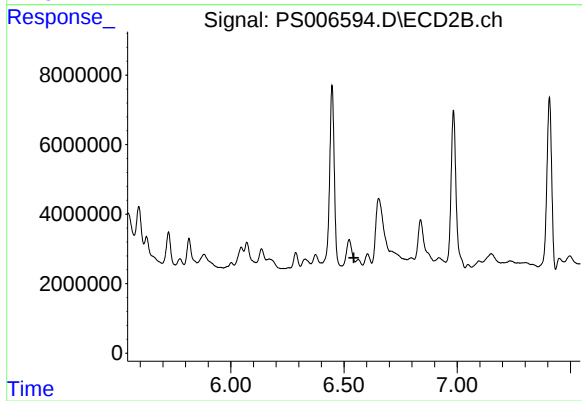

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 6.544 min
Response: 0
Conc: N.D.

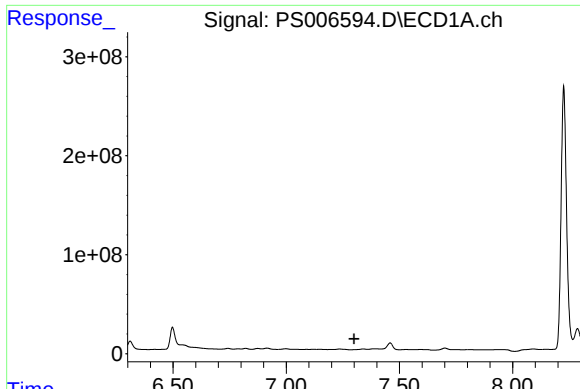

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.299 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

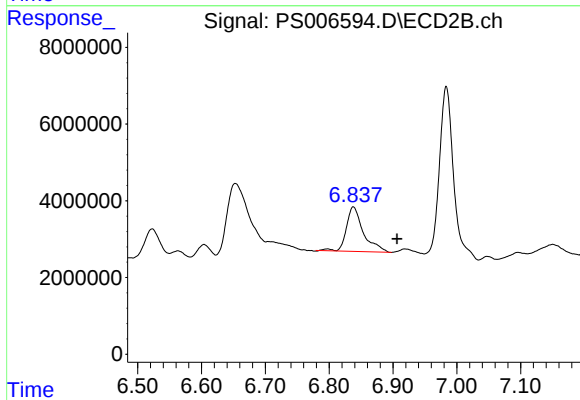


#11 2,4,5-TP (SILVEX)

R.T.: 6.838 min
Delta R.T.: -0.069 min
Response: 21310854
Conc: 8.19 ng/ml

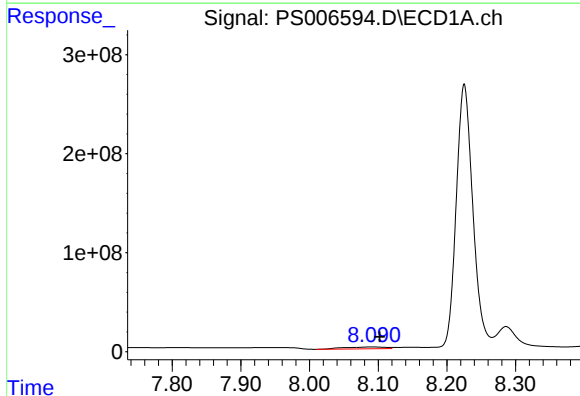


#13 2,4-DB

R.T.: 8.091 min
Delta R.T.: -0.012 min
Response: 79305341
Conc: 127.34 ng/ml

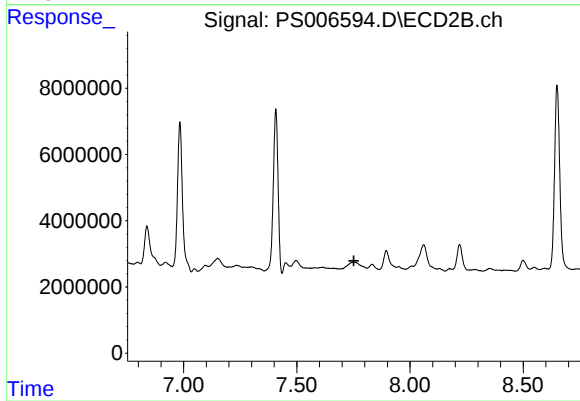

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 7.752 min
Response: 0
Conc: N.D.

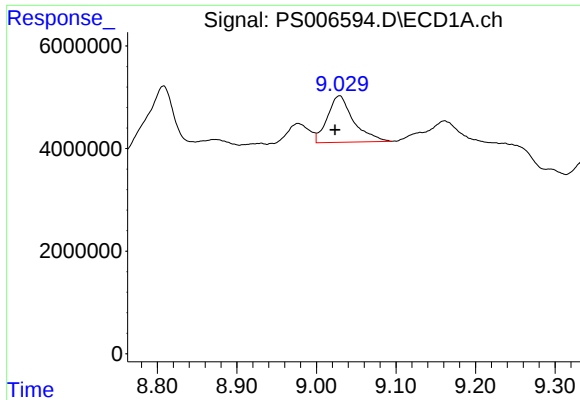

#15 Picloram


R.T.: 9.029 min

Delta R.T.: 0.005 min

Response: 20641756

Conc: 2.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

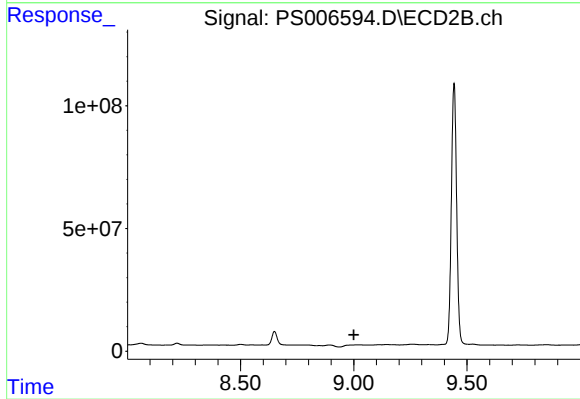

#15 Picloram

R.T.: 0.000 min

Exp R.T. : 9.000 min

Response: 0

Conc: N.D.