

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090619\
 Data File : PS006595.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Sep 2019 22:31
 Operator : SM\AJ
 Sample : K4683-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 07 03:00:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

1) T	Dalapon	0.000	1.736	0	81756984	N.D.	130.291
2) T	3,5-DICHL...	4.862	4.539	233.9E6	30079960	216.937	49.661 #
5) T	DICAMBA	0.000	5.353	0	139.0E6	N.D.	75.363
7) T	MCPA	5.959	5.590	13760992	32670023	4.359	15.986 #
8) T	DICHLORPROP	6.307	0.000	267.6E6	0	352.886	N.D. #
9) T	2,4-D	6.494	0.000	500.9E6	0	614.728	N.D. #
11) T	2,4,5-TP ...	7.339	0.000	30376420	0	6.659	N.D. #
13) T	2,4-DB	8.087	0.000	81915679	0	131.531	N.D. #
14) T	DINOSEB	0.000	8.057	0	23636989	N.D.	12.306
15) T	Picloram	9.024	0.000	48252408	0	6.485	N.D. #
16) T	DCPA	9.440	0.000	87389790	0	15.079	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090619\
Data File : PS006595.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Sep 2019 22:31
Operator : SM\AJ
Sample : K4683-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 07 03:00:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

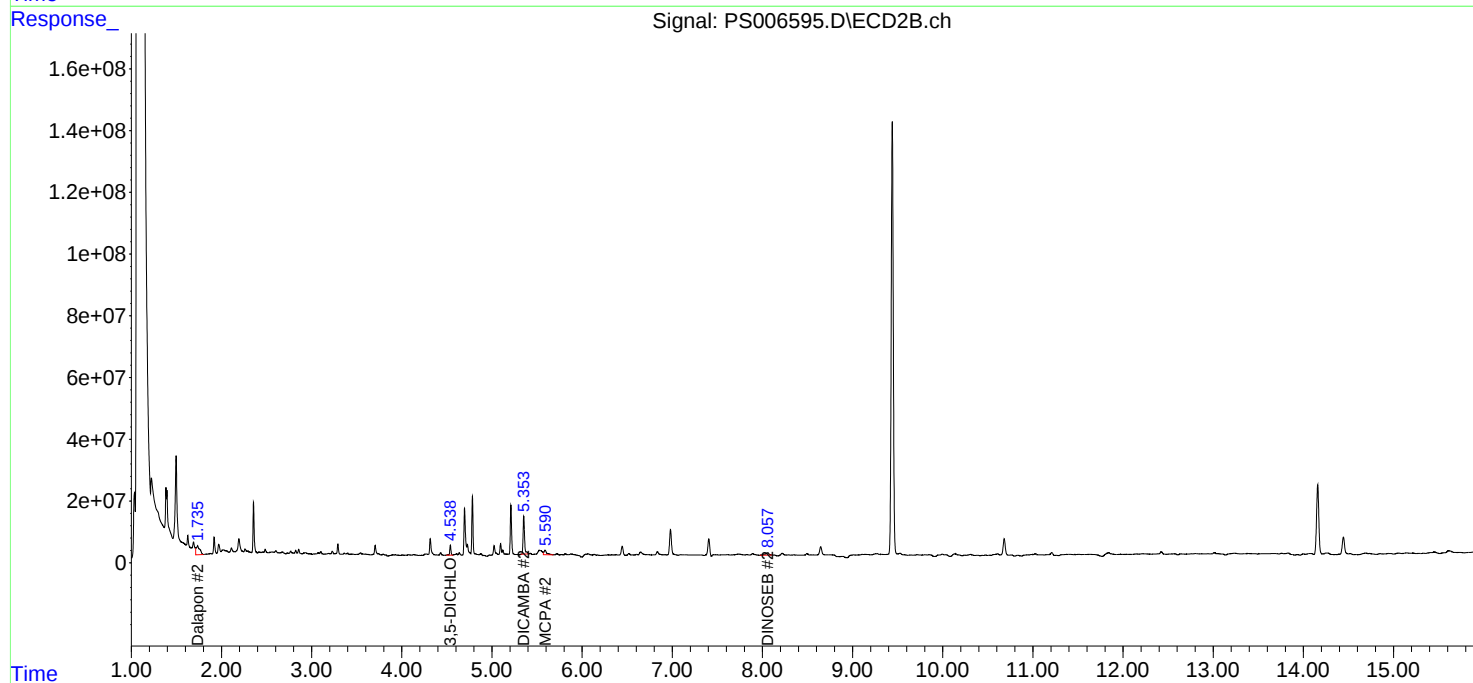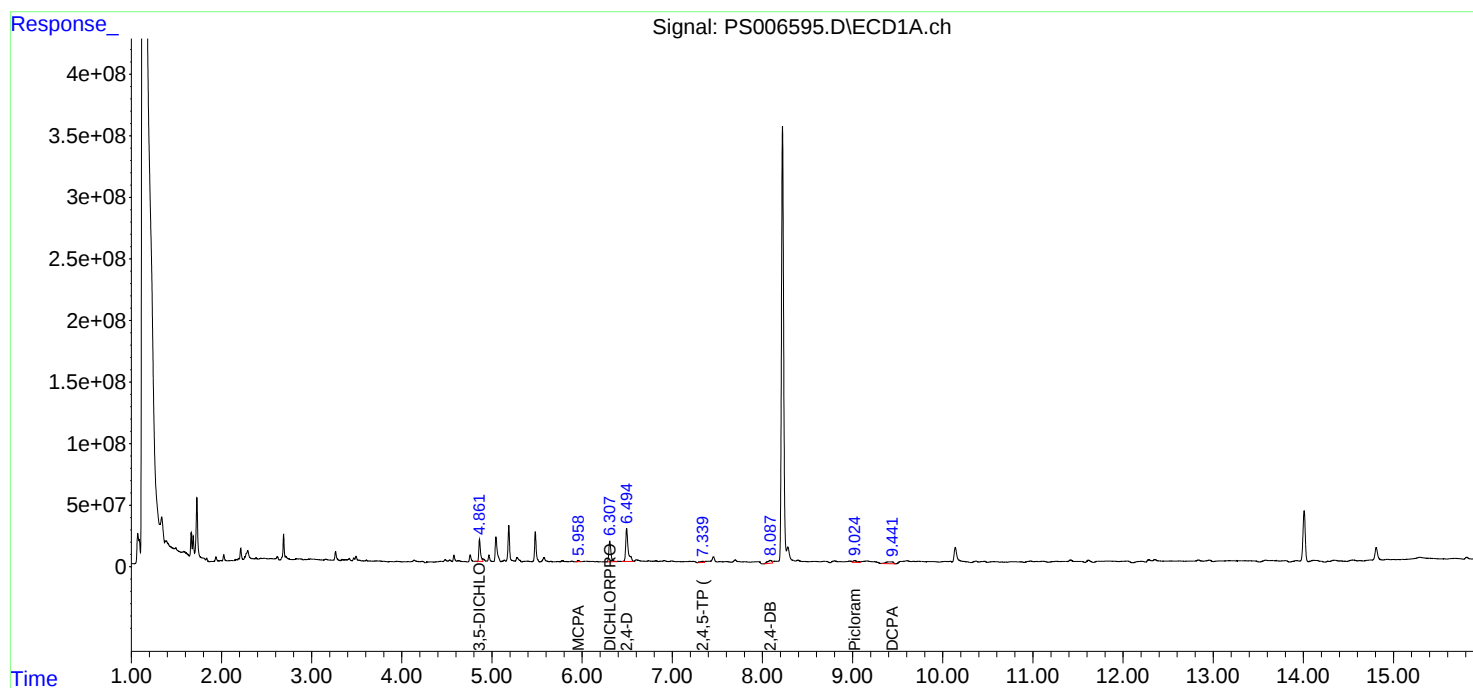


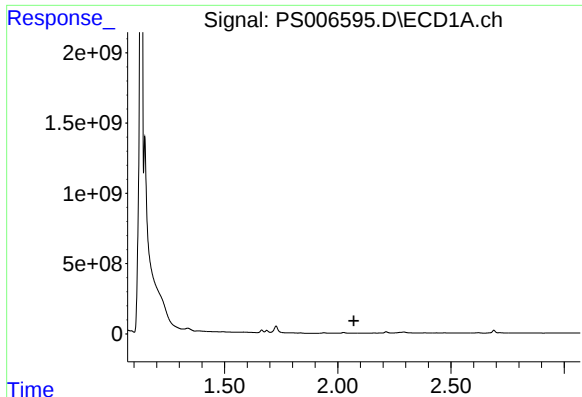

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.071 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

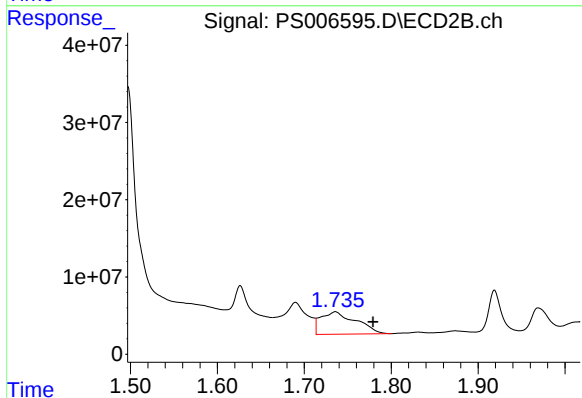


#1 Dalapon

R.T.: 1.736 min
Delta R.T.: -0.043 min
Response: 81756984
Conc: 130.29 ng/ml

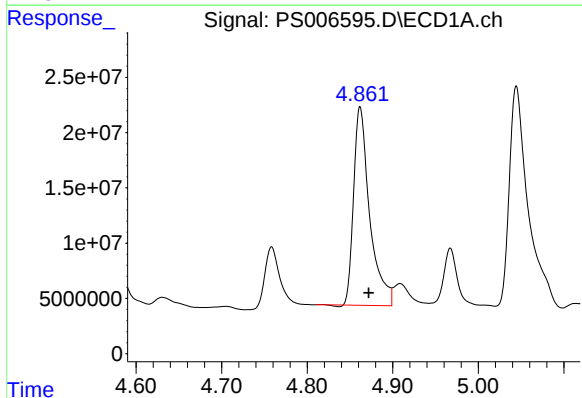


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.862 min
Delta R.T.: -0.010 min
Response: 233886899
Conc: 216.94 ng/ml

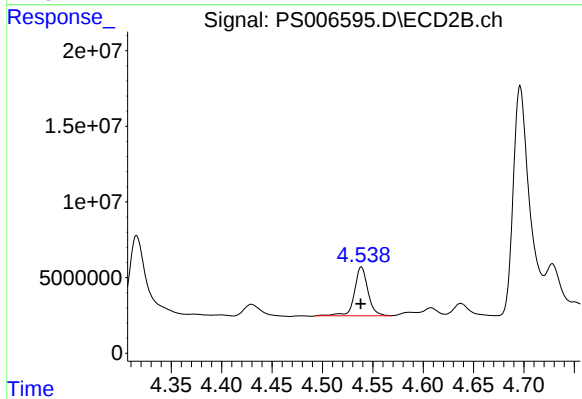

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.539 min
Delta R.T.: 0.000 min
Response: 30079960
Conc: 49.66 ng/ml

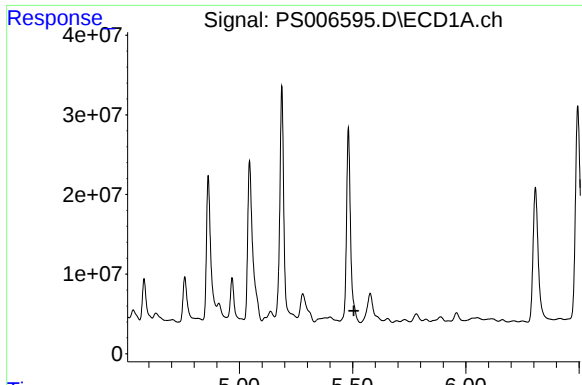

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 5.505 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

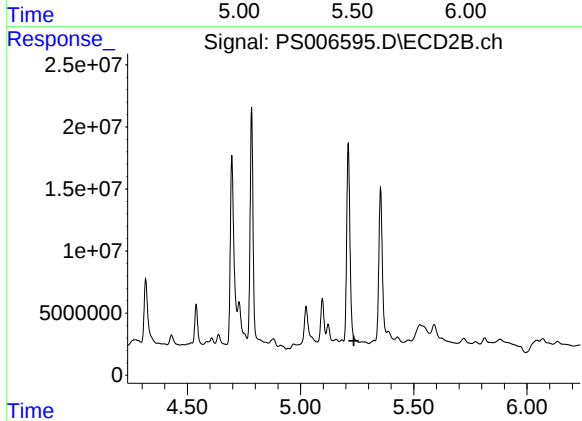


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 5.236 min
Response: 0
Conc: N.D.

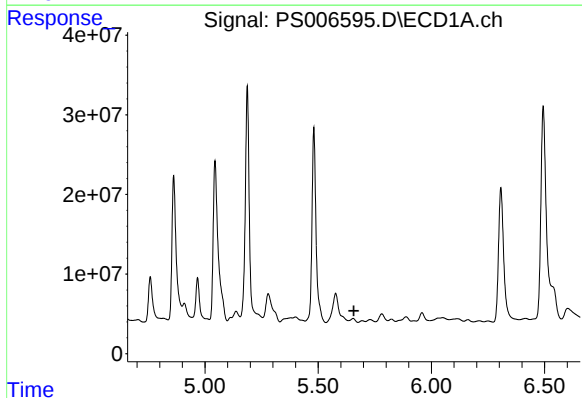


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.658 min
Response: 0
Conc: N.D.

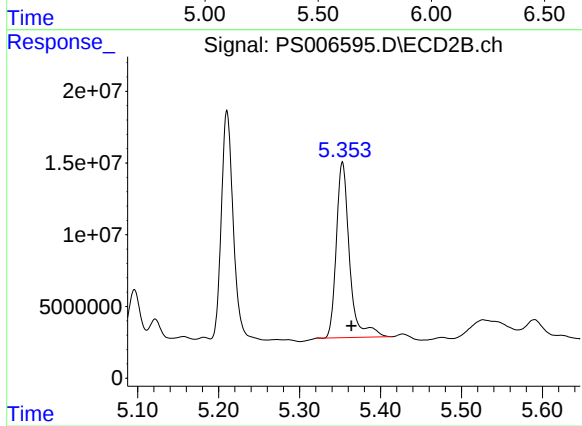

#5 DICAMBA


R.T.: 5.353 min
Delta R.T.: -0.011 min
Response: 139008289
Conc: 75.36 ng/ml

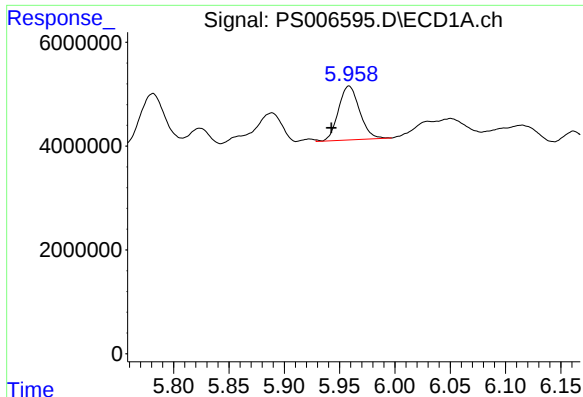

#7 MCPA


R.T.: 5.959 min
Delta R.T.: 0.016 min
Response: 13760992
Conc: 4.36 ug/ml

Instrument :
ECD_S
ClientSampleId :

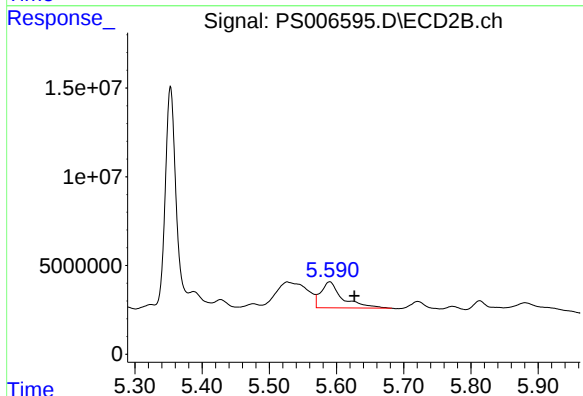


#7 MCPA

R.T.: 5.590 min
Delta R.T.: -0.037 min
Response: 32670023
Conc: 15.99 ug/ml

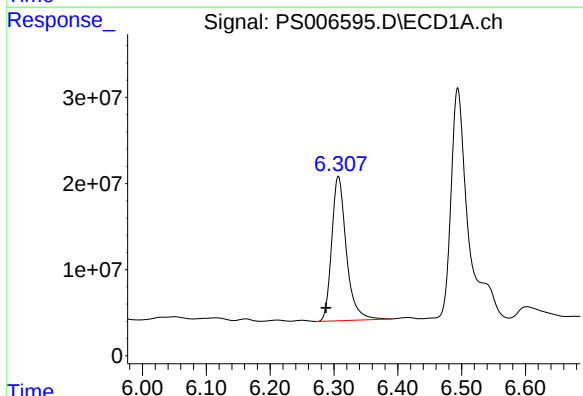


#8 DICHLORPROP

R.T.: 6.307 min
Delta R.T.: 0.019 min
Response: 267619952
Conc: 352.89 ng/ml

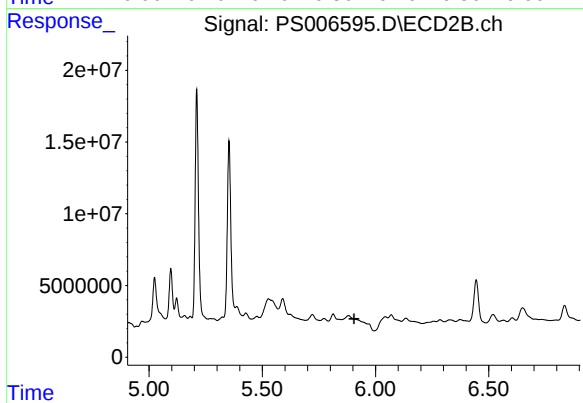

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 5.905 min
Response: 0
Conc: N.D.

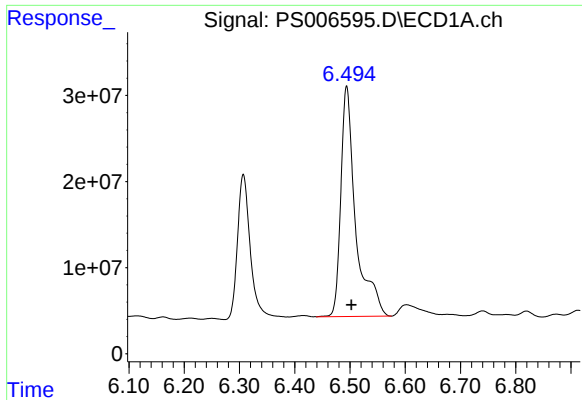

#9 2,4-D


R.T.: 6.494 min
Delta R.T.: -0.009 min
Response: 500870504
Conc: 614.73 ng/ml

Instrument :
ECD_S
ClientSampleId :

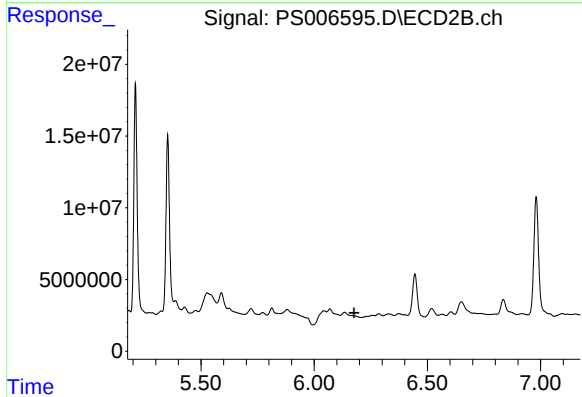


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.176 min
Response: 0
Conc: N.D.

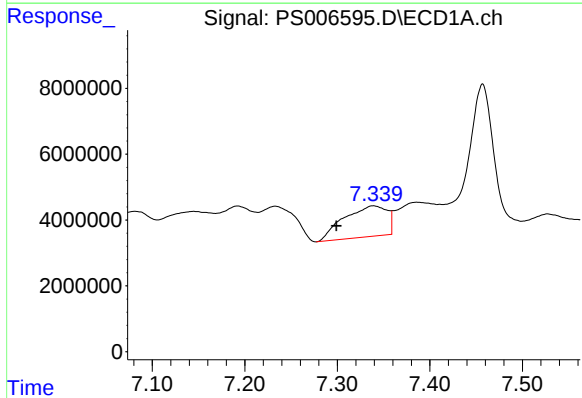


#11 2,4,5-TP (SILVEX)

R.T.: 7.339 min
Delta R.T.: 0.040 min
Response: 30376420
Conc: 6.66 ng/ml

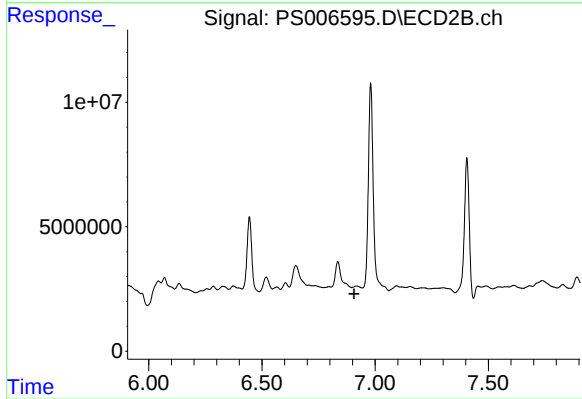

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 6.907 min
Response: 0
Conc: N.D.

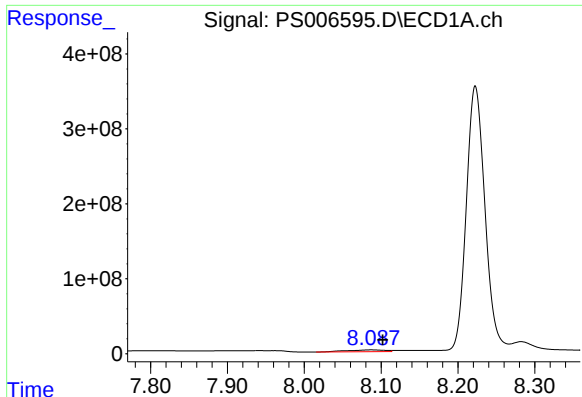

#13 2,4-DB


R.T.: 8.087 min
Delta R.T.: -0.015 min
Response: 81915679
Conc: 131.53 ng/ml

Instrument :
ECD_S
ClientSampleId :

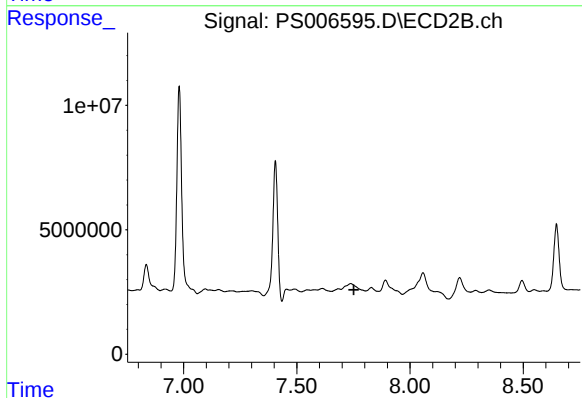


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 7.752 min
Response: 0
Conc: N.D.

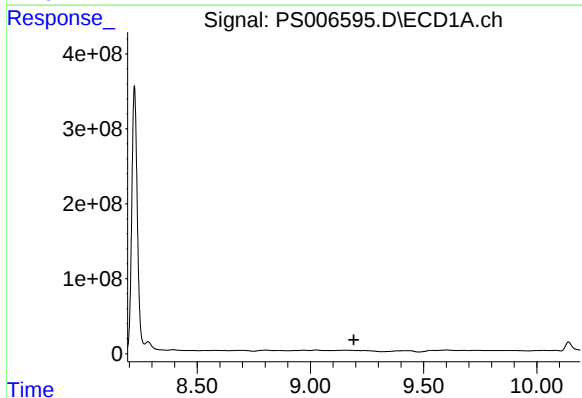


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.192 min
Response: 0
Conc: N.D.

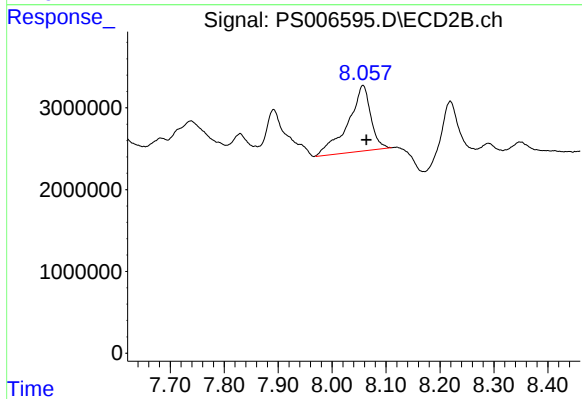

#14 DINOSEB


R.T.: 8.057 min
Delta R.T.: -0.006 min
Response: 23636989
Conc: 12.31 ng/ml

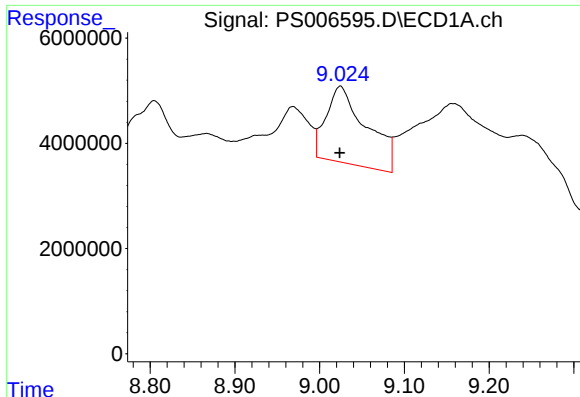

#15 Picloram


R.T.: 9.024 min
Delta R.T.: 0.000 min
Response: 48252408
Conc: 6.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

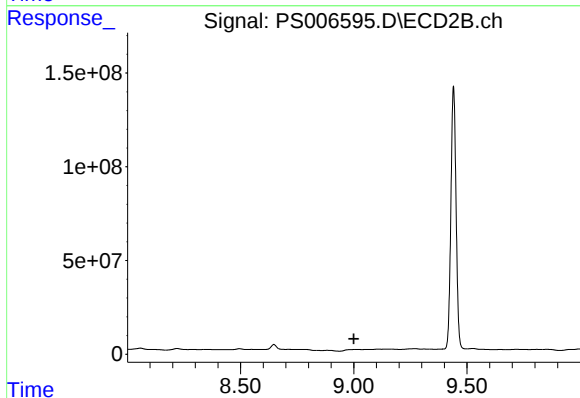


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.000 min
Response: 0
Conc: N.D.

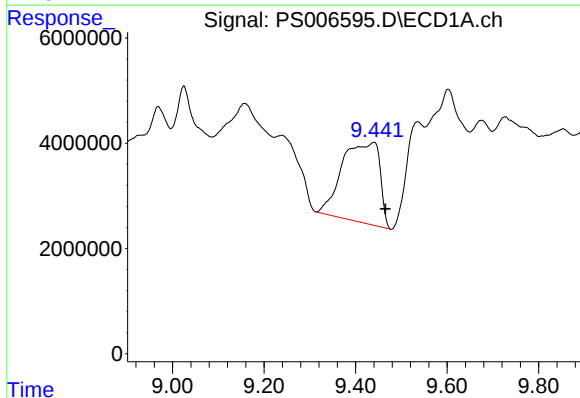

#16 DCPA

R.T.: 9.440 min
Delta R.T.: -0.025 min
Response: 87389790
Conc: 15.08 ng/ml

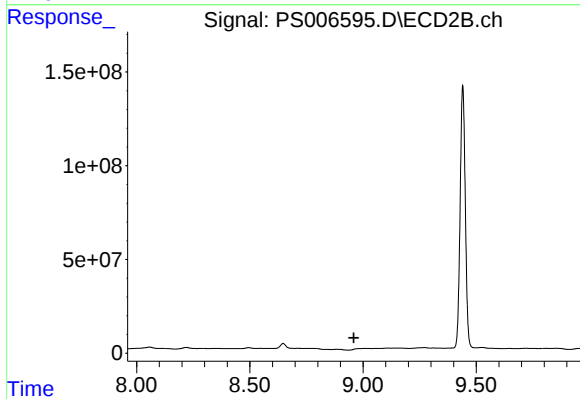

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 8.959 min
Response: 0
Conc: N.D.