

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090619\
 Data File : PS006606.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Sep 2019 02:33
 Operator : SM\AJ
 Sample : K4650-11
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 07 04:16:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.500	5.228	220.2E6	100.1E6	255.133	203.424
Target Compounds							
1) T	Dalapon	2.043	1.756	70194939	195.4E6	64.421	311.388 #
2) T	3,5-DICHL...	0.000	4.558	0	26214078	N.D.	43.278
5) T	DICAMBA	5.597	0.000	23900078	0	7.442	N.D. #
7) T	MCPA	5.976	5.628	22551564	12616646	7.143	6.173
9) T	2,4-D	6.565	0.000	79124192	0	97.111	N.D. #
10) T	Pentachlo...	6.746	6.504	39978233	33951229	3.382	5.022 #
11) T	2,4,5-TP ...	0.000	6.853	0	18365372	N.D.	7.058
13) T	2,4-DB	8.104	0.000	85013220	0	136.505	N.D. #
15) T	Picloram	8.984	0.000	18824121	0	2.530	N.D. #
16) T	DCPA	9.400	0.000	33739795	0	5.822	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090619\
Data File : PS006606.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Sep 2019 02:33
Operator : SM\AJ
Sample : K4650-11
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 07 04:16:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

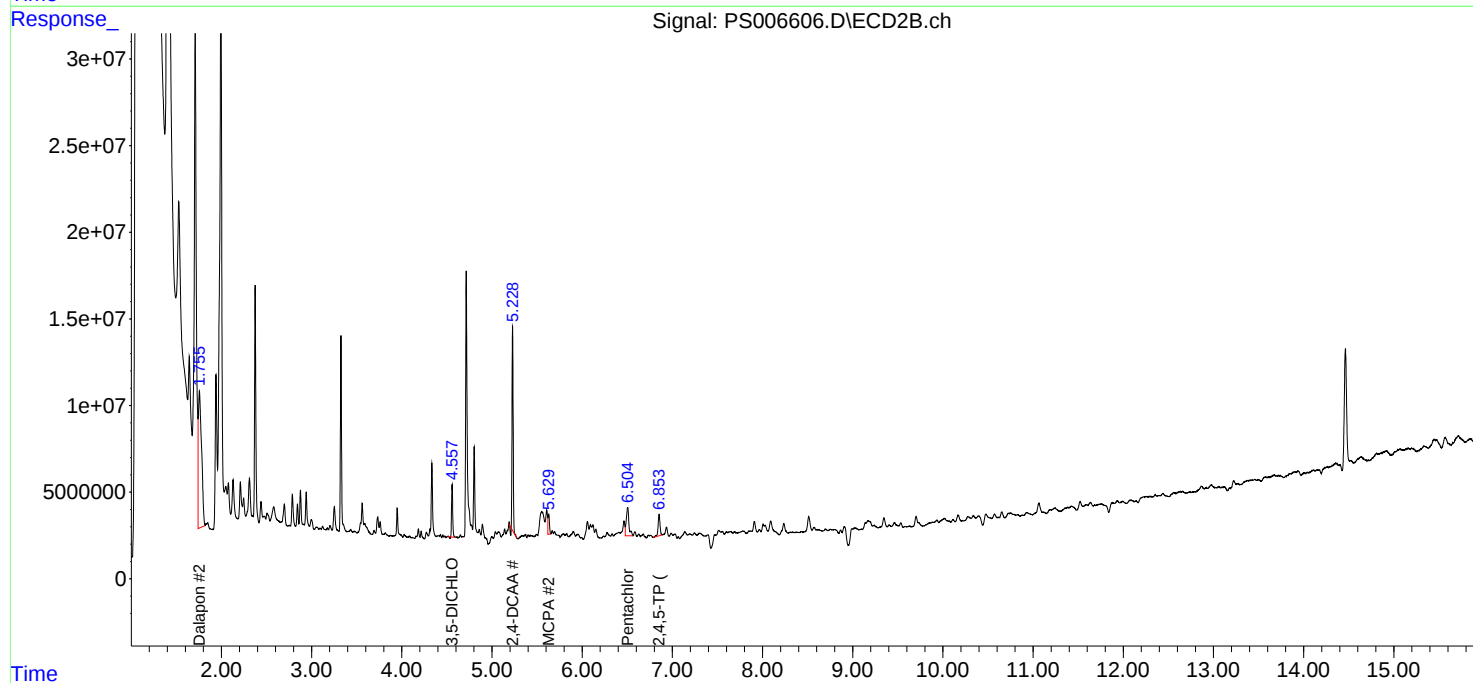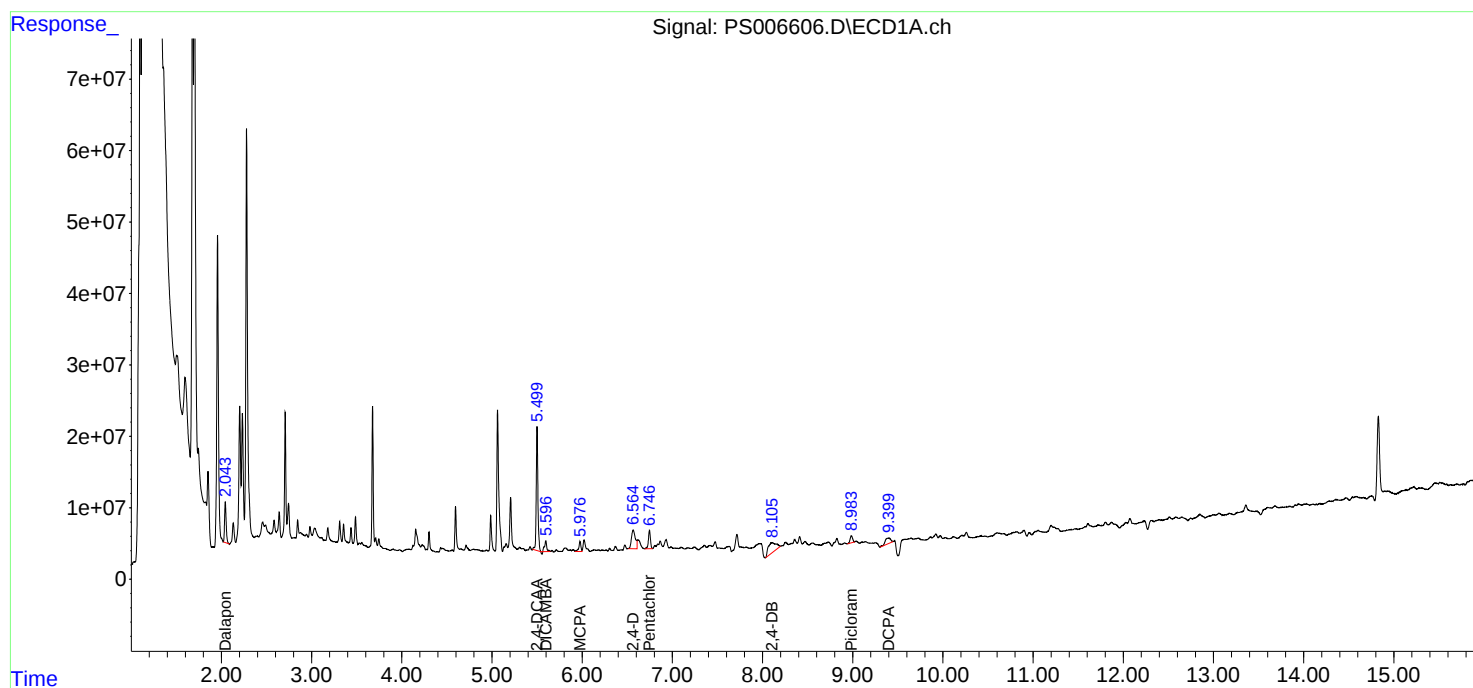


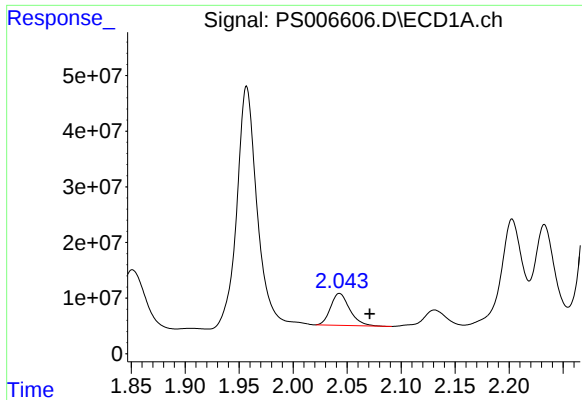

#1 Dalapon


R.T.: 2.043 min
Delta R.T.: -0.028 min
Response: 70194939
Conc: 64.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

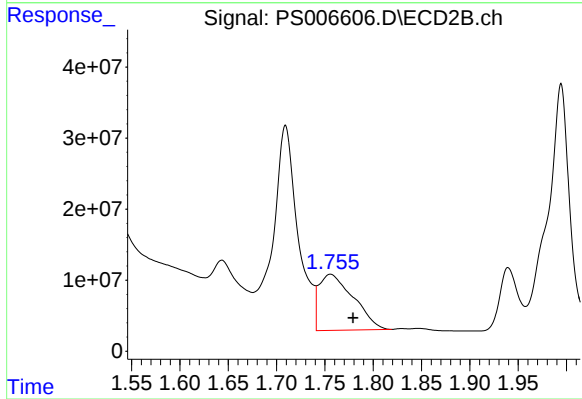


#1 Dalapon

R.T.: 1.756 min
Delta R.T.: -0.023 min
Response: 195393596
Conc: 311.39 ng/ml

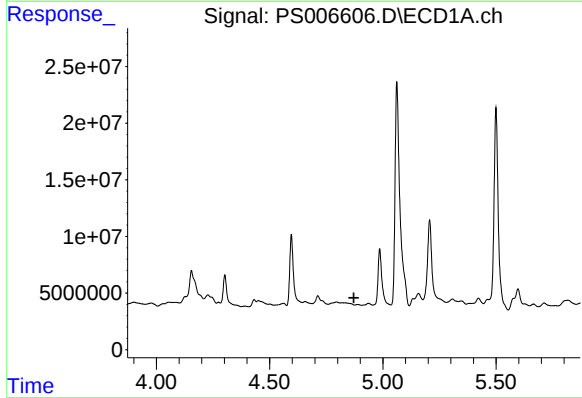


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.872 min
Response: 0
Conc: N.D.

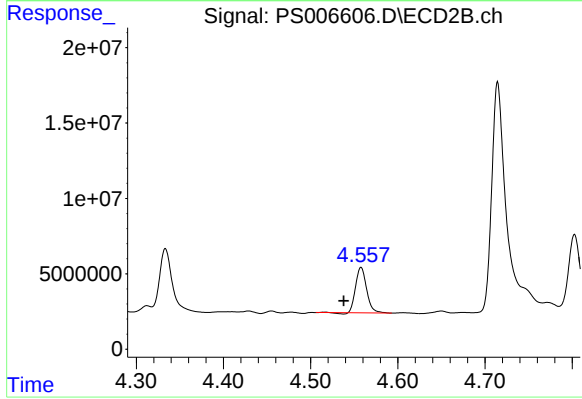

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.558 min
Delta R.T.: 0.020 min
Response: 26214078
Conc: 43.28 ng/ml

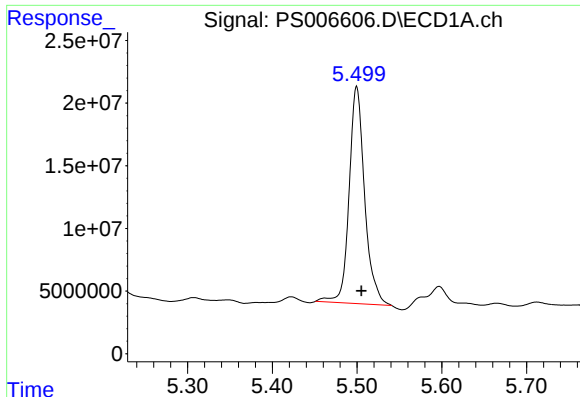

#4 2,4-DCAA


R.T.: 5.500 min
Delta R.T.: -0.006 min
Response: 220231007
Conc: 255.13 ng/ml

Instrument :
ECD_S
ClientSampleId :

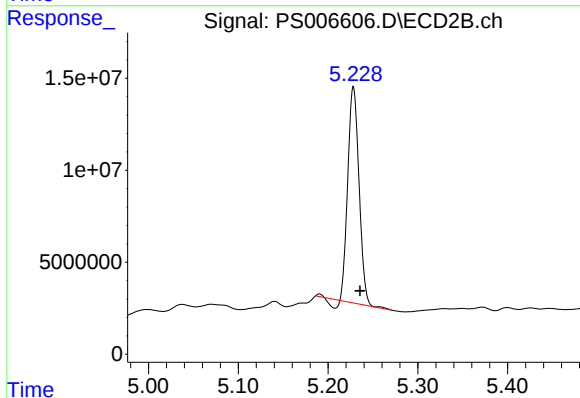


#4 2,4-DCAA

R.T.: 5.228 min
Delta R.T.: -0.007 min
Response: 100054500
Conc: 203.42 ng/ml

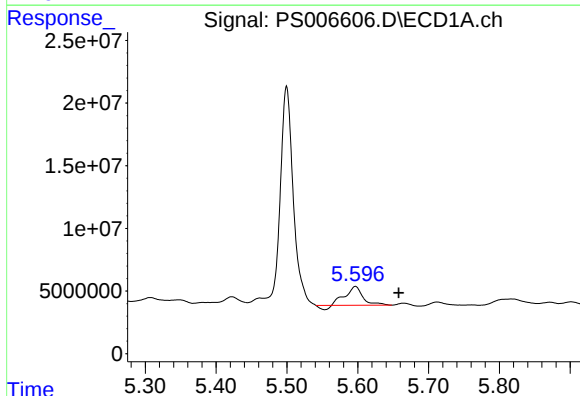


#5 DICAMBA

R.T.: 5.597 min
Delta R.T.: -0.061 min
Response: 23900078
Conc: 7.44 ng/ml

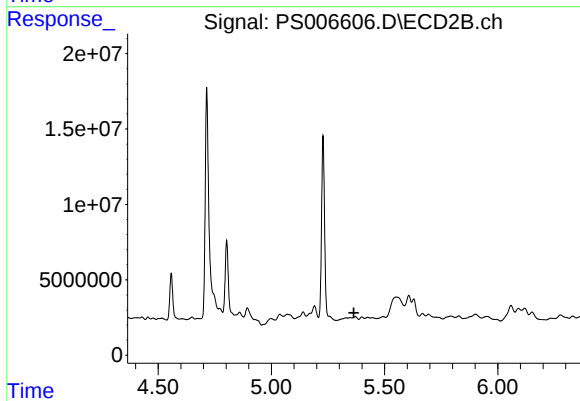

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.364 min
Response: 0
Conc: N.D.

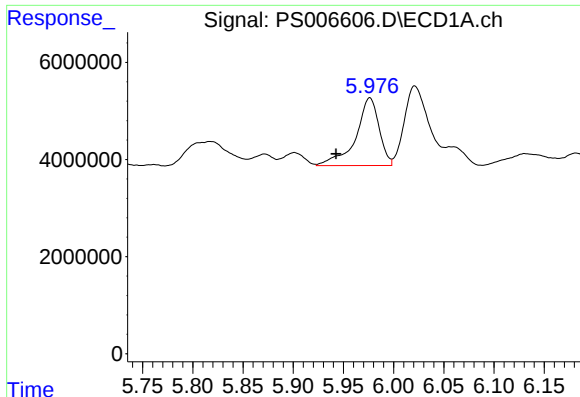

#7 MCPA


R.T.: 5.976 min
Delta R.T.: 0.034 min
Response: 22551564
Conc: 7.14 ug/ml

Instrument :
ECD_S
ClientSampleId :

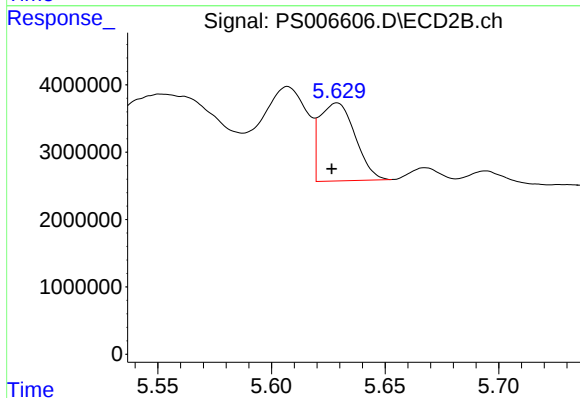


#7 MCPA

R.T.: 5.628 min
Delta R.T.: 0.002 min
Response: 12616646
Conc: 6.17 ug/ml

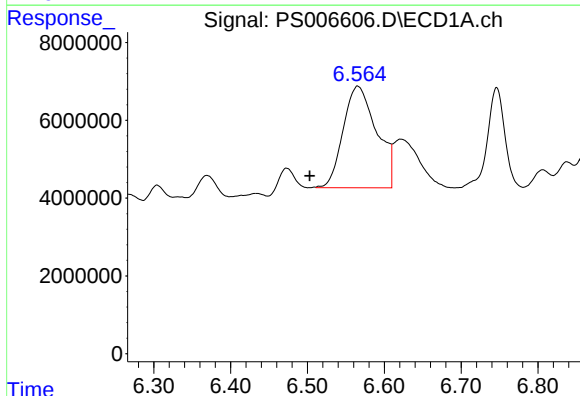


#9 2,4-D

R.T.: 6.565 min
Delta R.T.: 0.063 min
Response: 79124192
Conc: 97.11 ng/ml

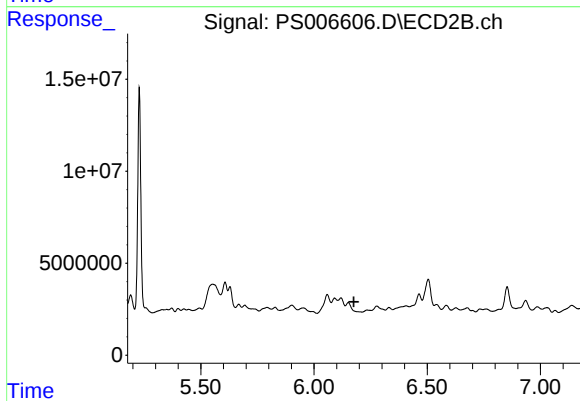

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.176 min
Response: 0
Conc: N.D.

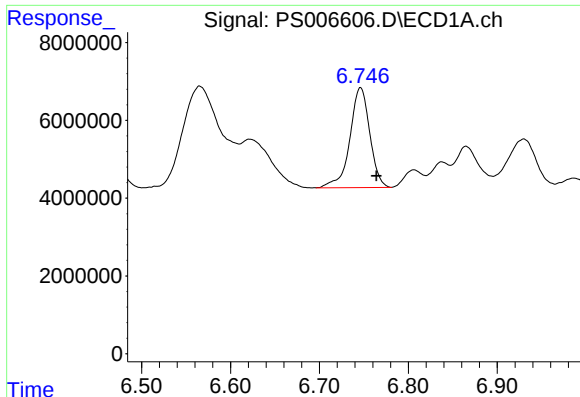

#10 Pentachlorophenol


R.T.: 6.746 min
Delta R.T.: -0.018 min
Response: 39978233
Conc: 3.38 ng/ml

Instrument :
ECD_S
ClientSampleId :

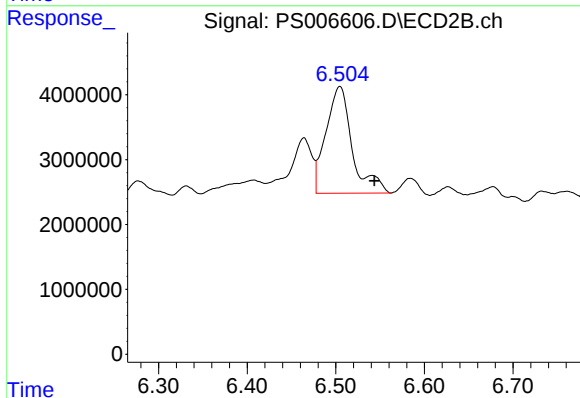


#10 Pentachlorophenol

R.T.: 6.504 min
Delta R.T.: -0.039 min
Response: 33951229
Conc: 5.02 ng/ml

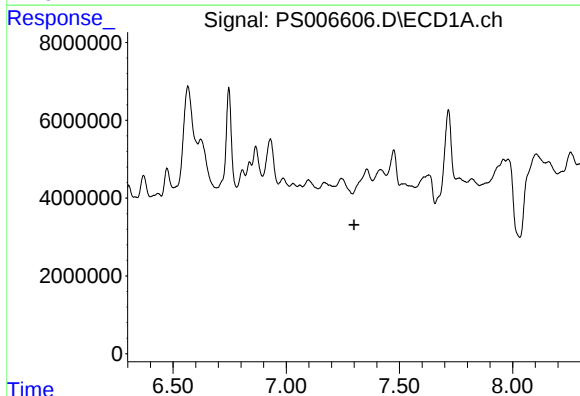


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.299 min
Response: 0
Conc: N.D.

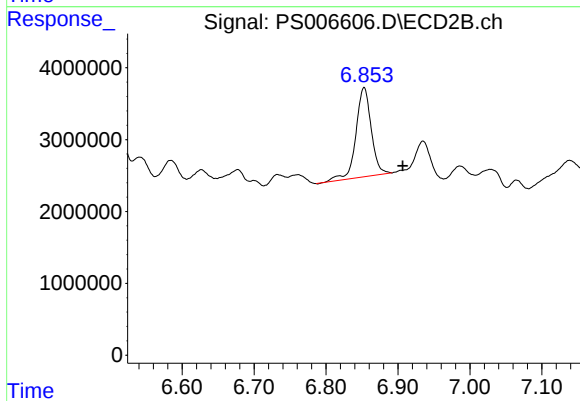

#11 2,4,5-TP (SILVEX)


R.T.: 6.853 min
Delta R.T.: -0.054 min
Response: 18365372
Conc: 7.06 ng/ml

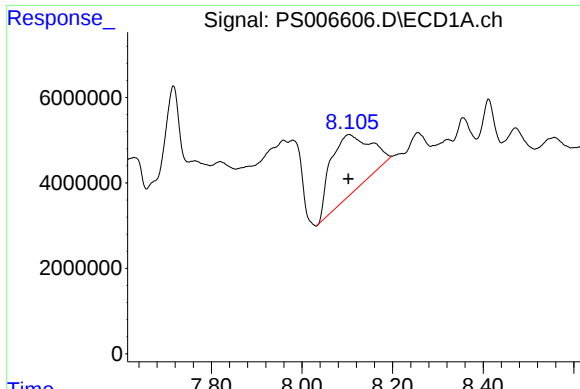

#13 2,4-DB


R.T.: 8.104 min
Delta R.T.: 0.002 min
Response: 85013220
Conc: 136.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

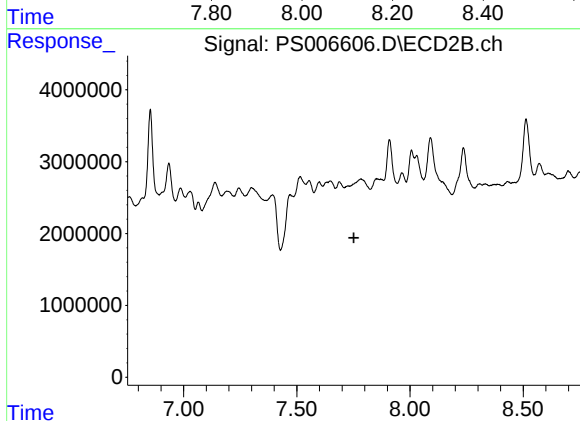


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 7.752 min
Response: 0
Conc: N.D.

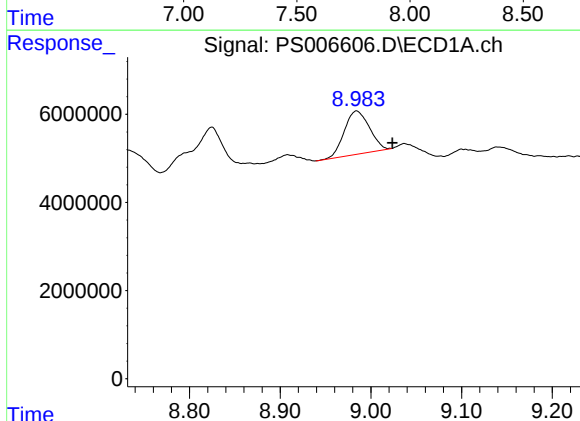


#15 Picloram

R.T.: 8.984 min
Delta R.T.: -0.039 min
Response: 18824121
Conc: 2.53 ng/ml

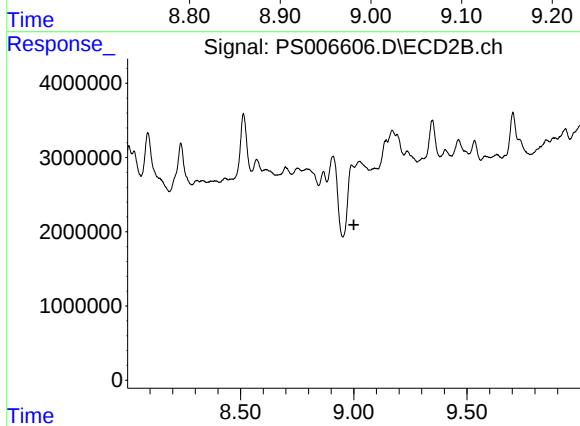

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 9.000 min
Response: 0
Conc: N.D.

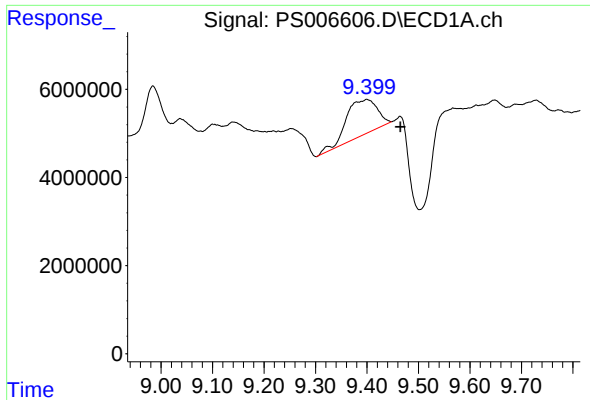

#16 DCPA

R.T.: 9.400 min
Delta R.T.: -0.065 min
Response: 33739795
Conc: 5.82 ng/ml

Instrument :
ECD_S
ClientSampleId :

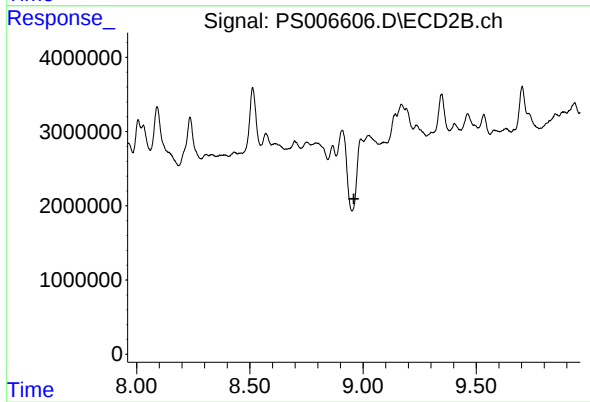

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 8.959 min
Response: 0
Conc: N.D.