

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090619\
 Data File : PS006608.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Sep 2019 03:17
 Operator : SM\AJ
 Sample : K4650-15
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 07 04:16:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.516	5.246	30695104	28970665	35.560	58.901 #
Target Compounds							
1) T	Dalapon	2.061	1.773	68497311	188.4E6	62.863	300.180 #
2) T	3,5-DICHL...	0.000	4.574	0	46373648	N.D.	76.561
5) T	DICAMBA	5.613	0.000	21097448	0	6.569	N.D. #
7) T	MCPA	5.993	5.623	52691916	16411973	16.690	8.030 #
9) T	2,4-D	6.524	6.106	15998353	8479226	19.635	15.425
10) T	Pentachlo...	0.000	6.496	0	44642218	N.D.	6.604
11) T	2,4,5-TP ...	0.000	6.868	0	19147150	N.D.	7.358
13) T	2,4-DB	8.142	7.764	153.0E6	44946678	245.660	135.055 #
14) T	DINOSEB	0.000	8.095	0	14936356	N.D.	7.776
15) T	Picloram	8.996	0.000	56221701	0	7.556	N.D. #
16) T	DCPA	9.484	0.000	96288715	0	16.614	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090619\
Data File : PS006608.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Sep 2019 03:17
Operator : SM\AJ
Sample : K4650-15
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 07 04:16:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

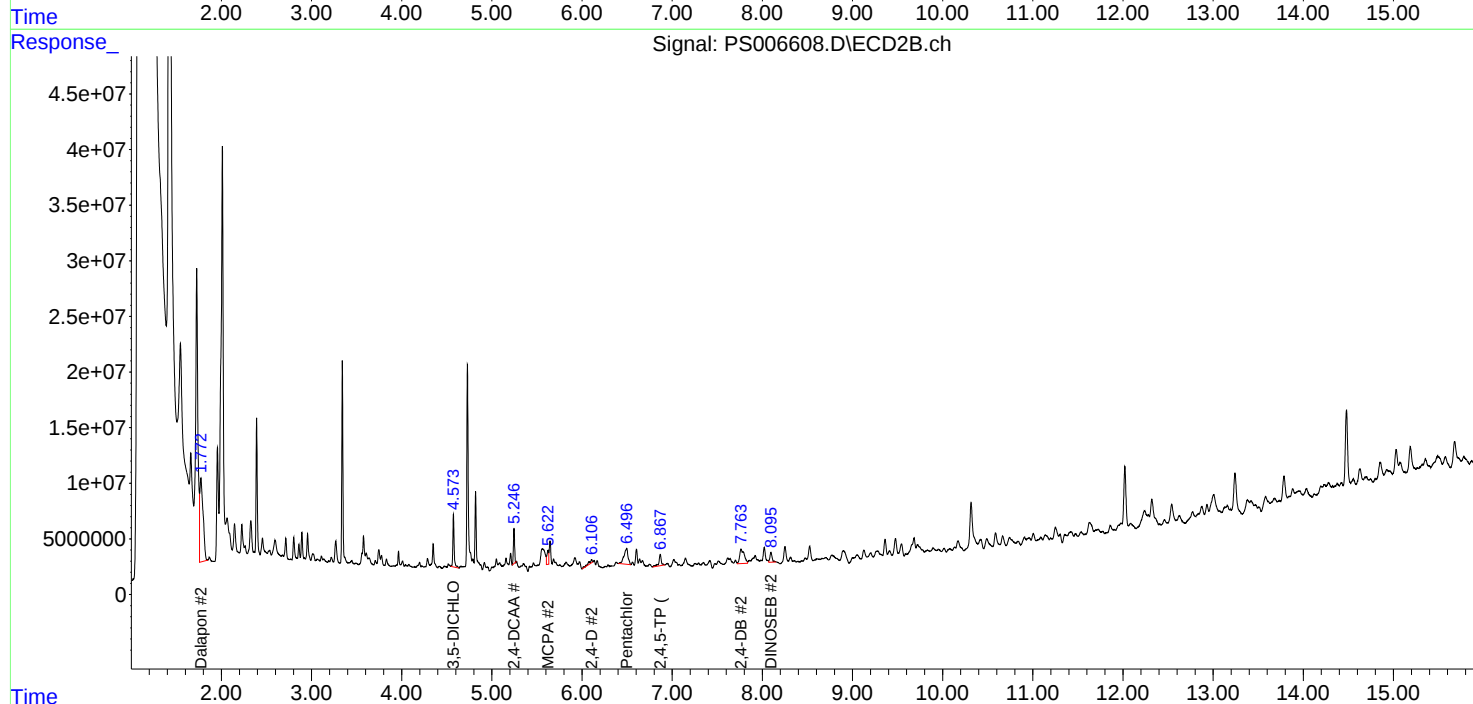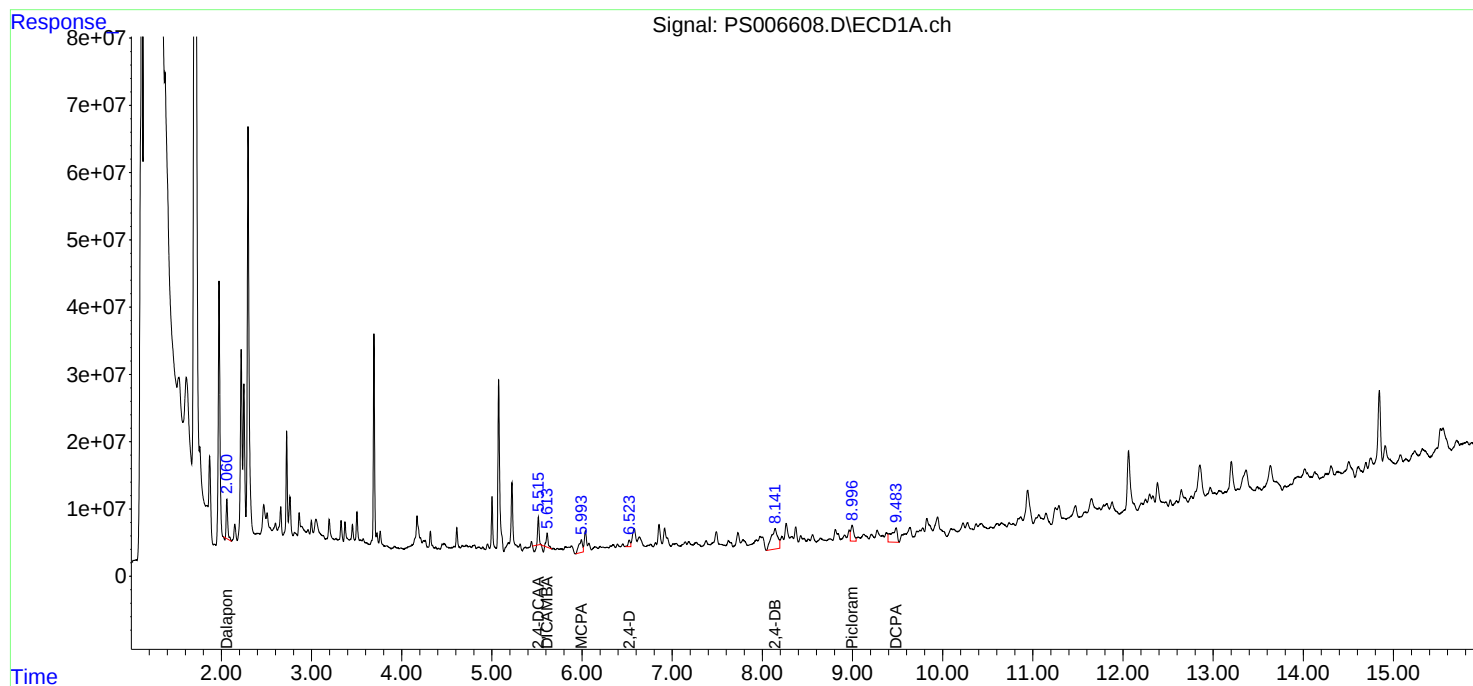


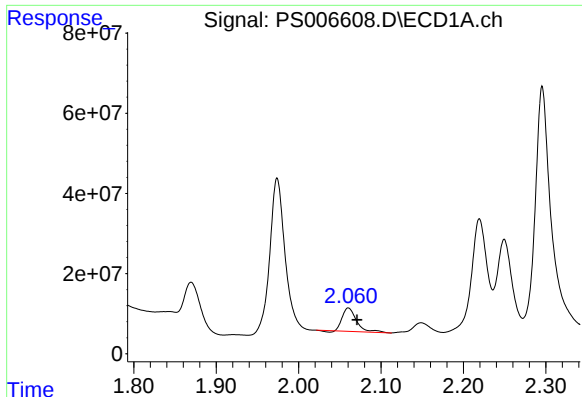

#1 Dalapon


R.T.: 2.061 min
Delta R.T.: -0.010 min
Response: 68497311
Conc: 62.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

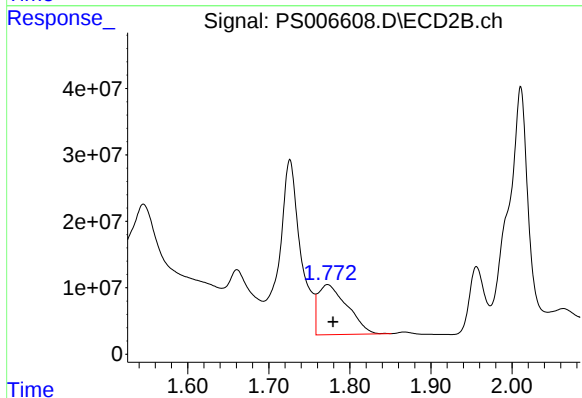


#1 Dalapon

R.T.: 1.773 min
Delta R.T.: -0.006 min
Response: 188361027
Conc: 300.18 ng/ml

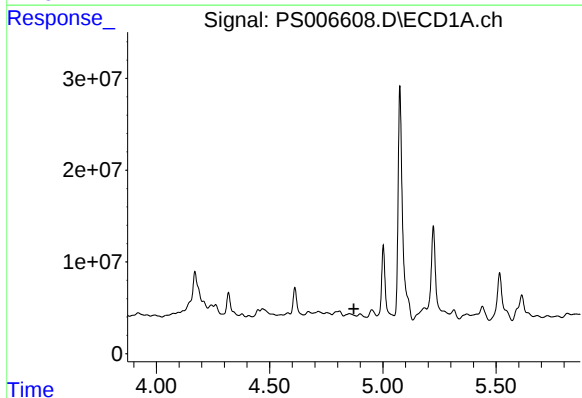


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.872 min
Response: 0
Conc: N.D.

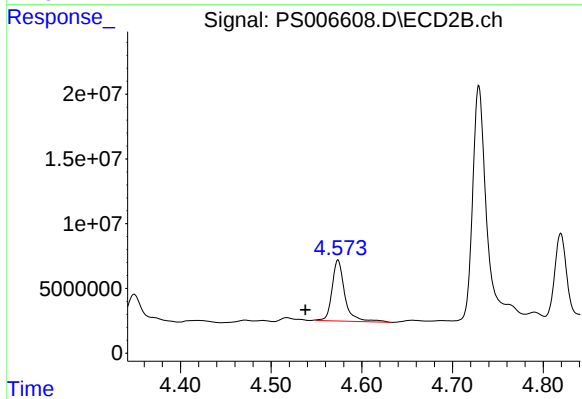

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.574 min
Delta R.T.: 0.036 min
Response: 46373648
Conc: 76.56 ng/ml

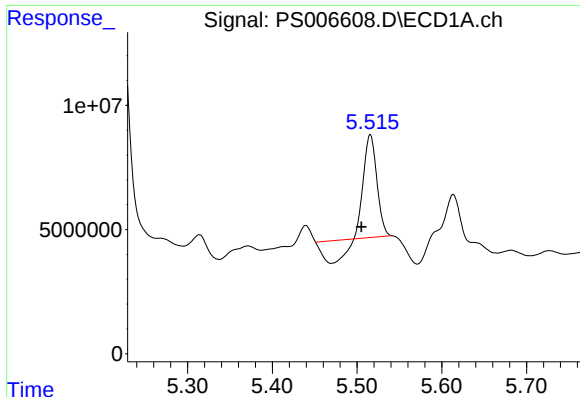

#4 2,4-DCAA


R.T.: 5.516 min
Delta R.T.: 0.010 min
Response: 30695104
Conc: 35.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

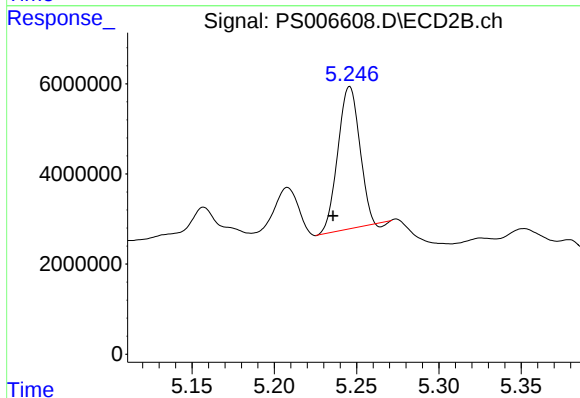


#4 2,4-DCAA

R.T.: 5.246 min
Delta R.T.: 0.010 min
Response: 28970665
Conc: 58.90 ng/ml

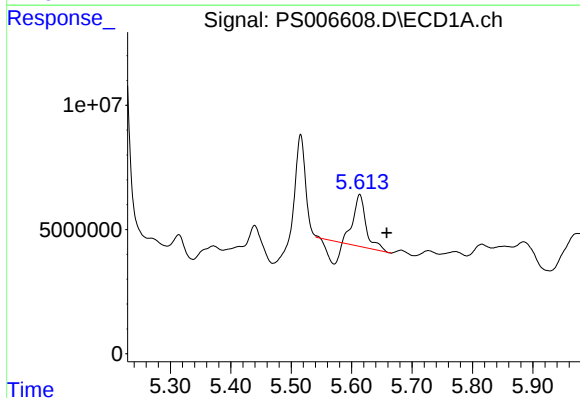


#5 DICAMBA

R.T.: 5.613 min
Delta R.T.: -0.045 min
Response: 21097448
Conc: 6.57 ng/ml

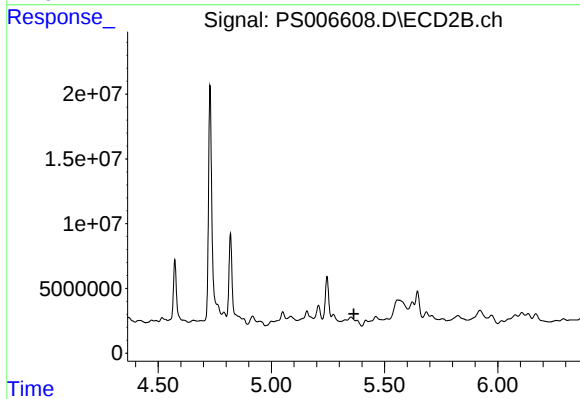

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.364 min
Response: 0
Conc: N.D.

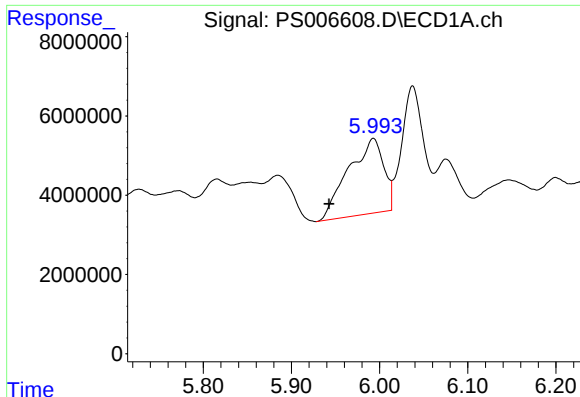

#7 MCPA


R.T.: 5.993 min
Delta R.T.: 0.050 min
Response: 52691916
Conc: 16.69 ug/ml

Instrument :
ECD_S
ClientSampleId :

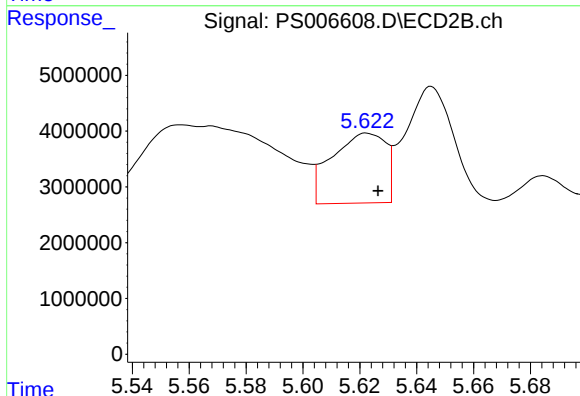


#7 MCPA

R.T.: 5.623 min
Delta R.T.: -0.004 min
Response: 16411973
Conc: 8.03 ug/ml

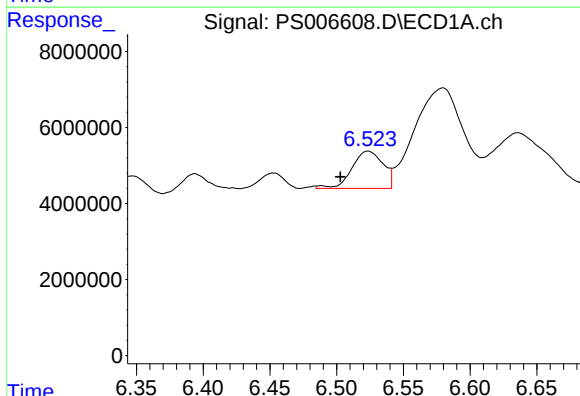


#9 2,4-D

R.T.: 6.524 min
Delta R.T.: 0.021 min
Response: 15998353
Conc: 19.64 ng/ml

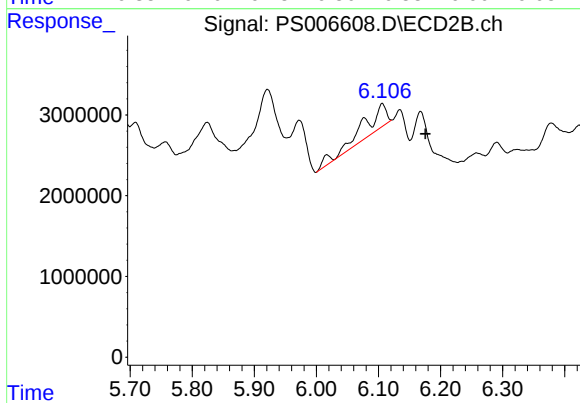

#9 2,4-D


R.T.: 6.106 min
Delta R.T.: -0.070 min
Response: 8479226
Conc: 15.42 ng/ml

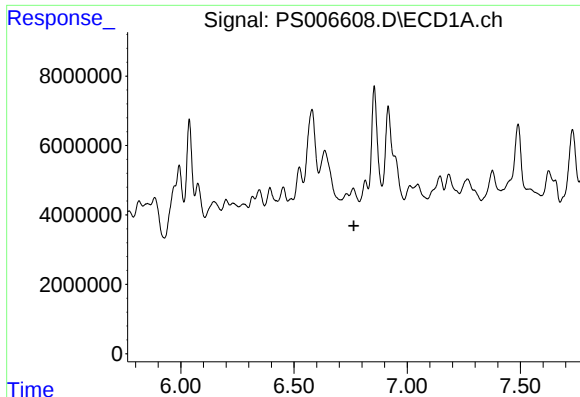

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.764 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

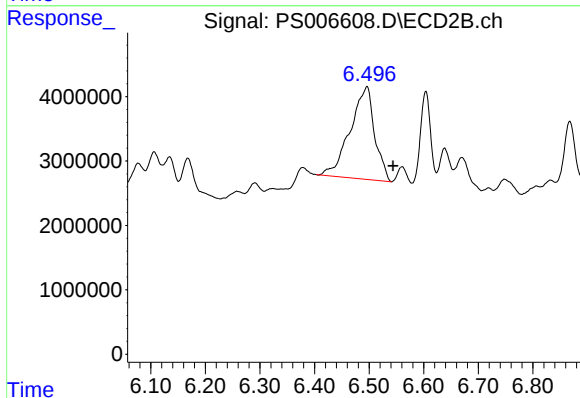


#10 Pentachlorophenol

R.T.: 6.496 min
Delta R.T.: -0.048 min
Response: 44642218
Conc: 6.60 ng/ml

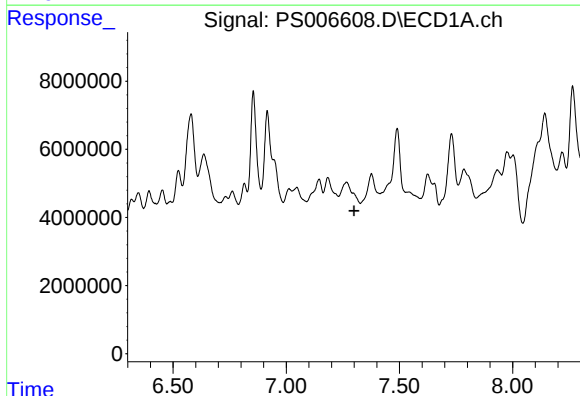


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.299 min
Response: 0
Conc: N.D.

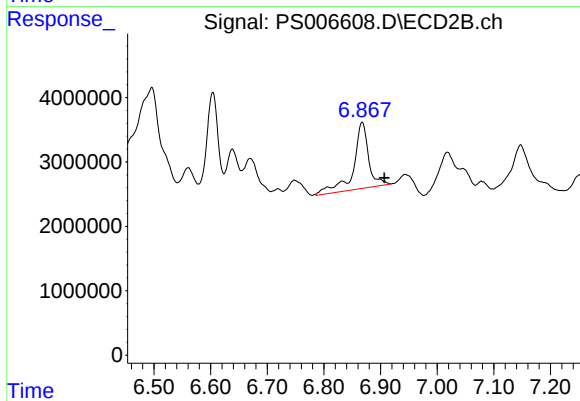

#11 2,4,5-TP (SILVEX)


R.T.: 6.868 min
Delta R.T.: -0.039 min
Response: 19147150
Conc: 7.36 ng/ml

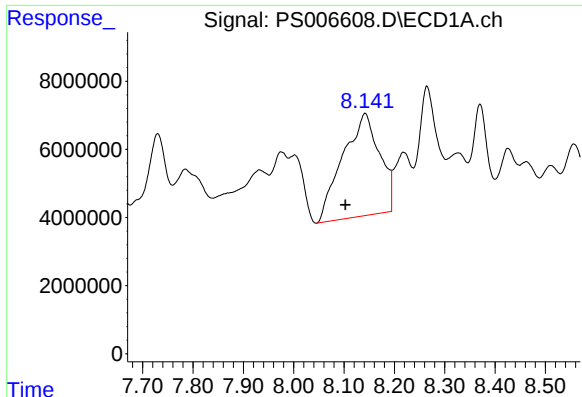

#13 2,4-DB


R.T.: 8.142 min
Delta R.T.: 0.039 min
Response: 152993494
Conc: 245.66 ng/ml

Instrument :
ECD_S
ClientSampleId :

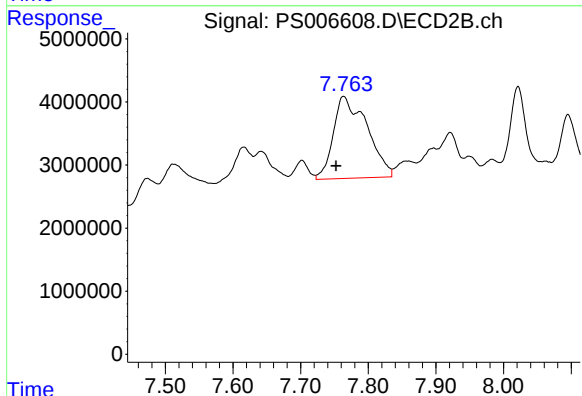


#13 2,4-DB

R.T.: 7.764 min
Delta R.T.: 0.011 min
Response: 44946678
Conc: 135.05 ng/ml

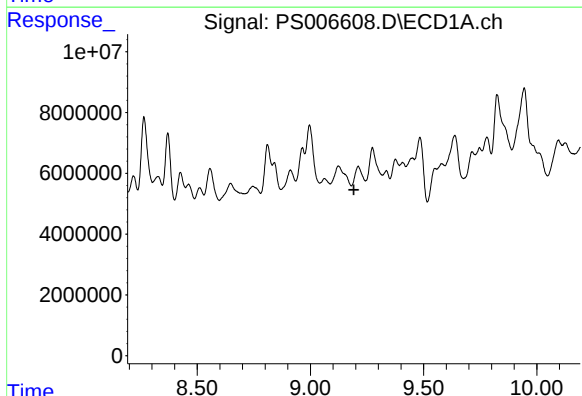


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.192 min
Response: 0
Conc: N.D.

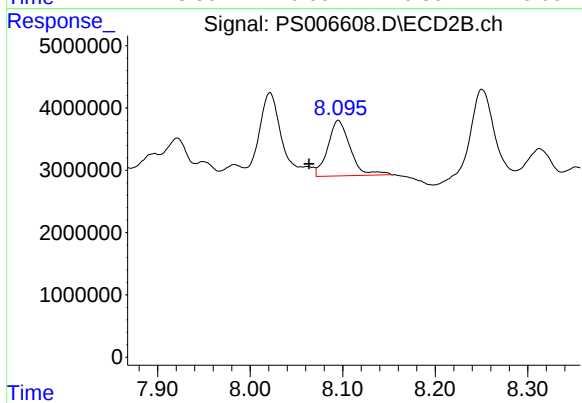

#14 DINOSEB


R.T.: 8.095 min
Delta R.T.: 0.032 min
Response: 14936356
Conc: 7.78 ng/ml

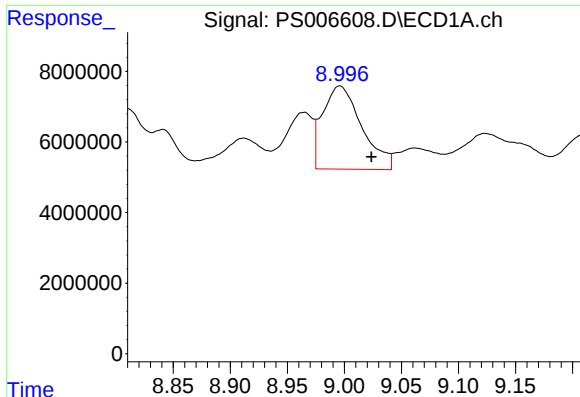

#15 Picloram


R.T.: 8.996 min
Delta R.T.: -0.028 min
Response: 56221701
Conc: 7.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

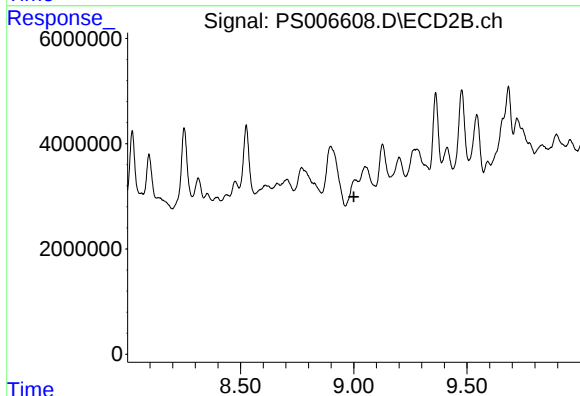


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.000 min
Response: 0
Conc: N.D.

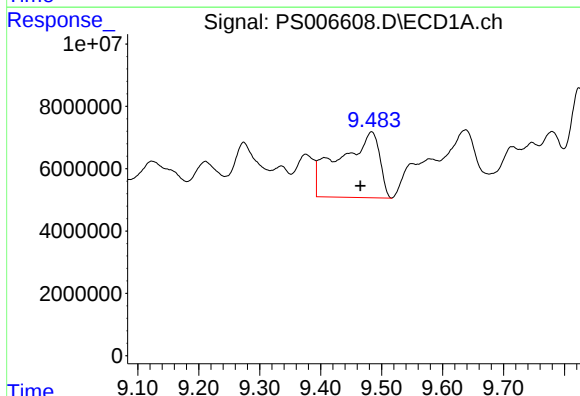

#16 DCPA

R.T.: 9.484 min
Delta R.T.: 0.018 min
Response: 96288715
Conc: 16.61 ng/ml

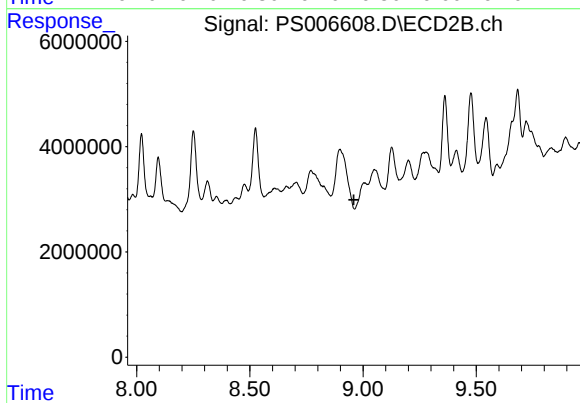

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 8.959 min
Response: 0
Conc: N.D.