

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090619\
 Data File : PS006596.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Sep 2019 22:53
 Operator : SM\AJ
 Sample : K4683-04
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 20190666-FIELD-DUPLICATE

Manual Integrations
 APPROVED

Ankita
 9/9/2019 11:24:25 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 07 03:49:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	5.499	5.211	218.6E6	113.2E6	253.295	230.159m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090619\
Data File : PS006596.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Sep 2019 22:53
Operator : SM\AJ
Sample : K4683-04
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
20190666-FIELD-DUPLICATE


Manual Integrations
APPROVED

Ankita
9/9/2019 11:24:25 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 07 03:49:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

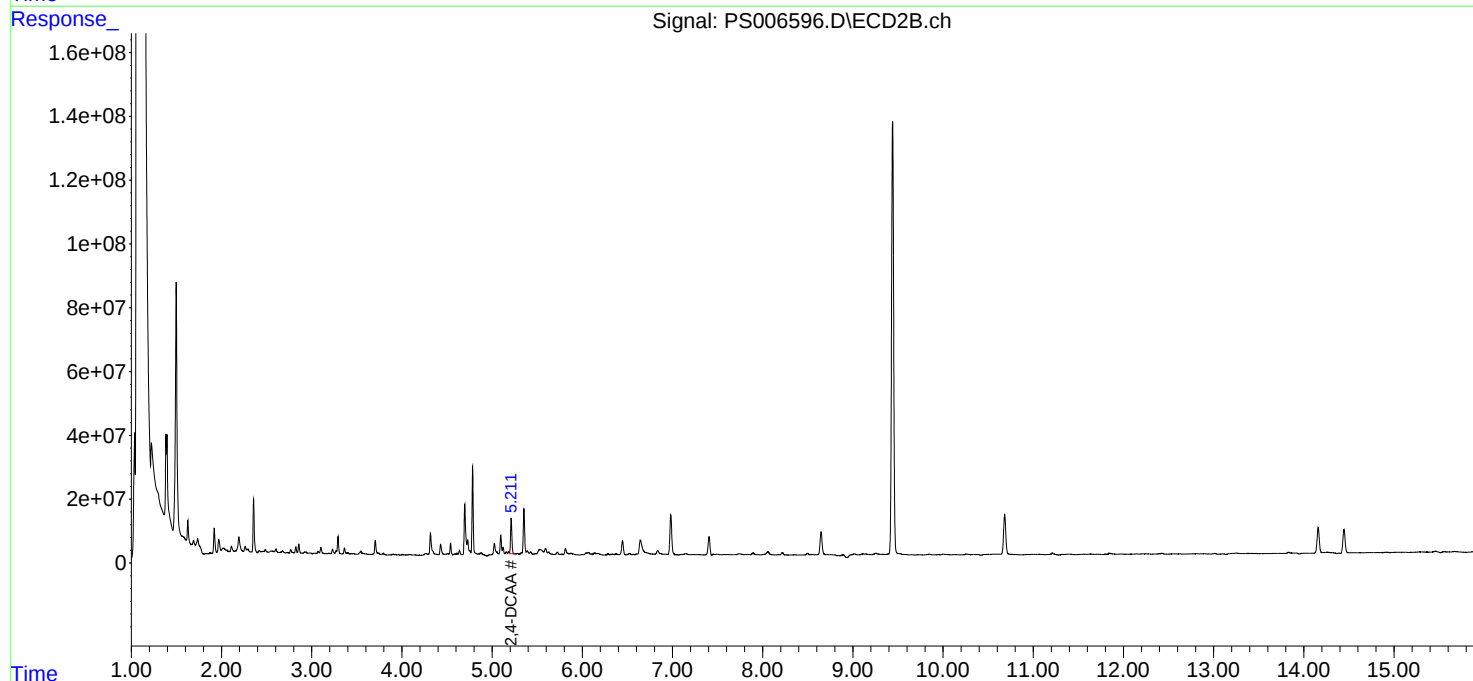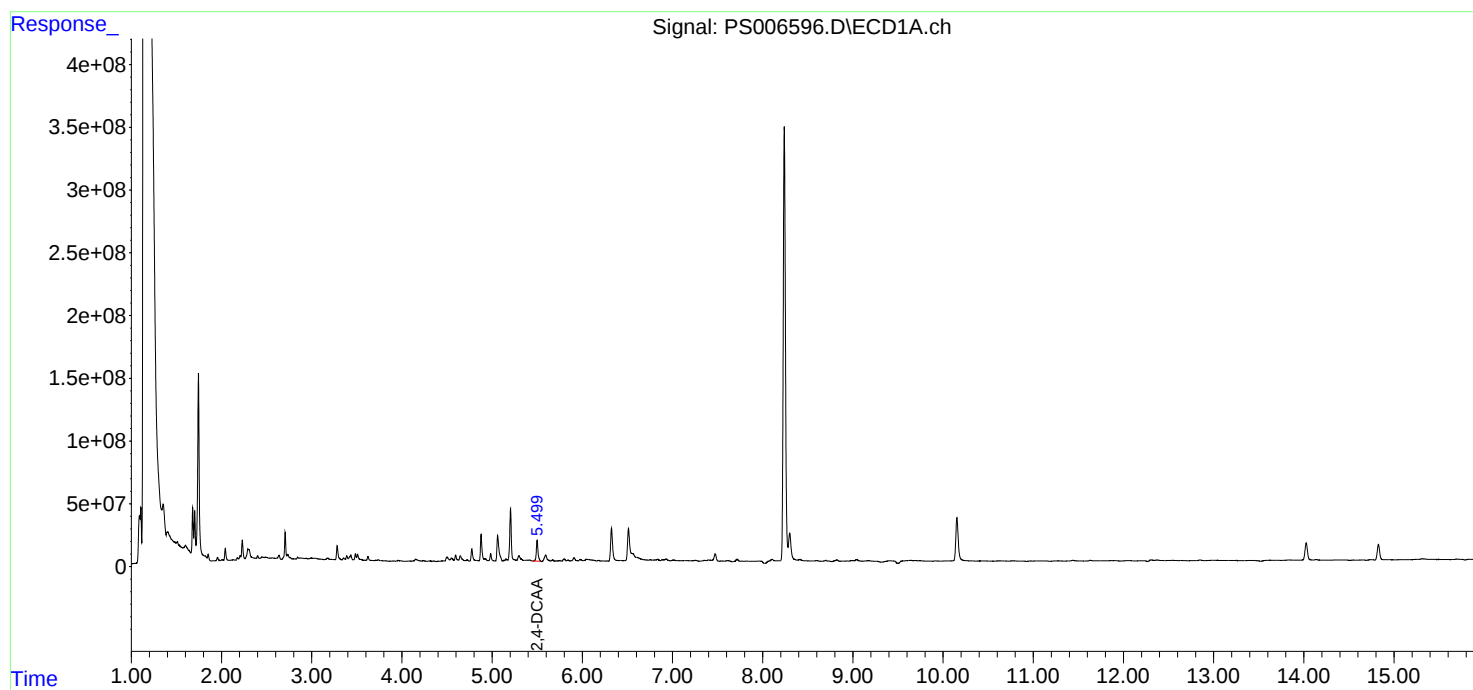

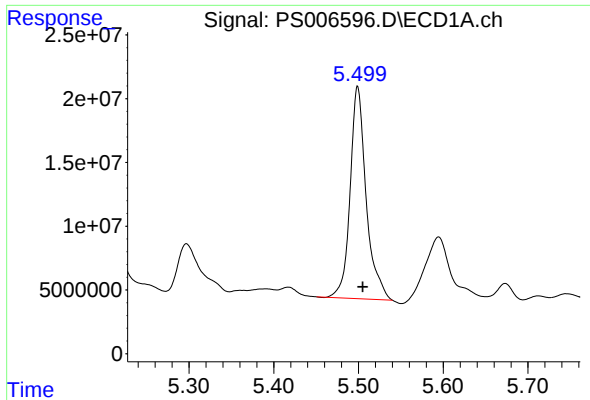


#4 2,4-DCAA

R.T.: 5.499 min
Delta R.T.: -0.006 min
Response: 218644884
Conc: 253.30 ng/ml

Instrument :
ECD_S
ClientSampleId :
20190666-FIELD-DUPLICATE

Manual Integrations
APPROVED

Ankita
9/9/2019 11:24:25 AM

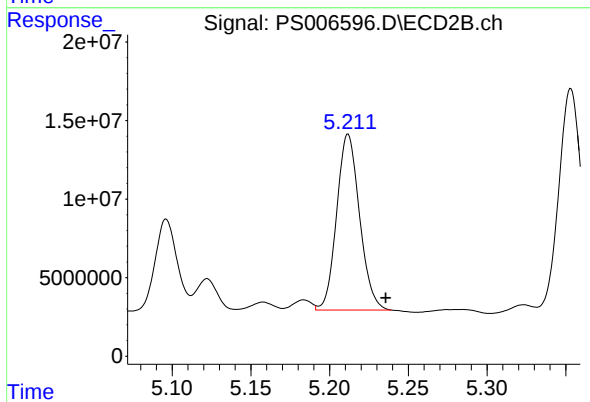

#4 2,4-DCAA

R.T.: 5.211 min
Delta R.T.: -0.024 min
Response: 113204245
Conc: 230.16 ng/ml m