

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090622\
 Data File : PS020454.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Sep 2022 09:41
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 06 11:16:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090222.M
 Quant Title : 8080.M
 QLast Update : Sat Sep 03 01:06:55 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
4) S	2,4-DCAA	7.193	6.798f	252097	3397007	<MDL	3.194 #
Target Compounds							
2) T	3,5-DICHL...	6.366	0.000	458484	0	<MDL	N.D. #
3) T	4-Nitroph...	7.011	0.000	985522	0	<MDL	N.D. #
5) T	DICAMBA	7.381	6.975f	3513662	3935692	<MDL	<MDL #
6) T	MCP	7.520	7.051	-36098	1896969	N.D.	<MDL
7) T	MCPA	7.672	0.000	10435298	0	<MDL	N.D. #
8) T	DICHLORPROP	8.040	0.000	6311915	0	1.910	N.D. #
9) T	2,4-D	8.324	0.000	36231821	0	7.723	N.D. #
10) T	Pentachlo...	8.596	0.000	2654291	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.152	0.000	709209	0	<MDL	N.D. #
12) T	2,4,5-T	9.447	9.053f	472120	5708745	<MDL	<MDL #
14) T	DINOSEB	11.117	0.000	4089019	0	<MDL	N.D. #
15) T	Picloram	10.973	10.807	209.5E6	39082101	5.059	3.805
16) T	DCPA	11.404	10.807f	3162899	39082101	<MDL	4.388 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090622\
Data File : PS020454.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Sep 2022 09:41
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 06 11:16:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090222.M
Quant Title : 8080.M
QLast Update : Sat Sep 03 01:06:55 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

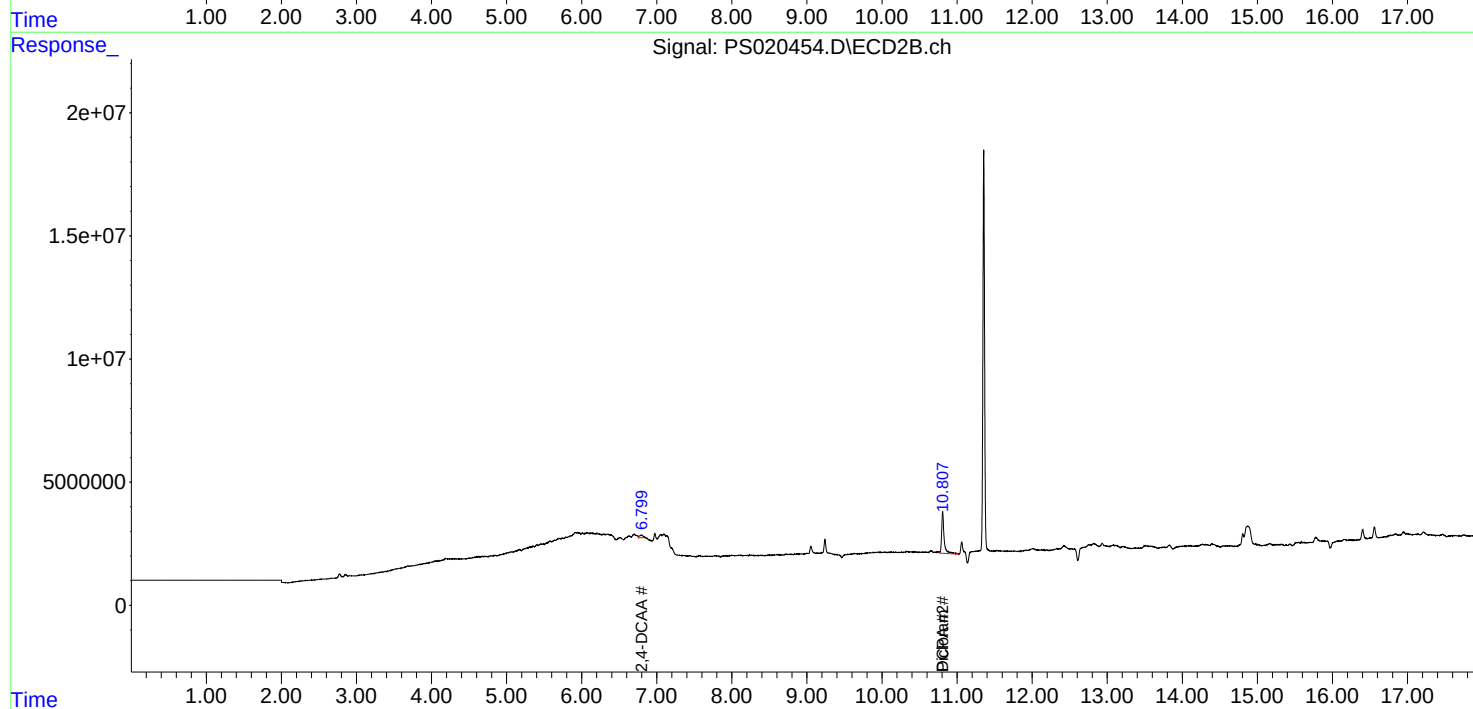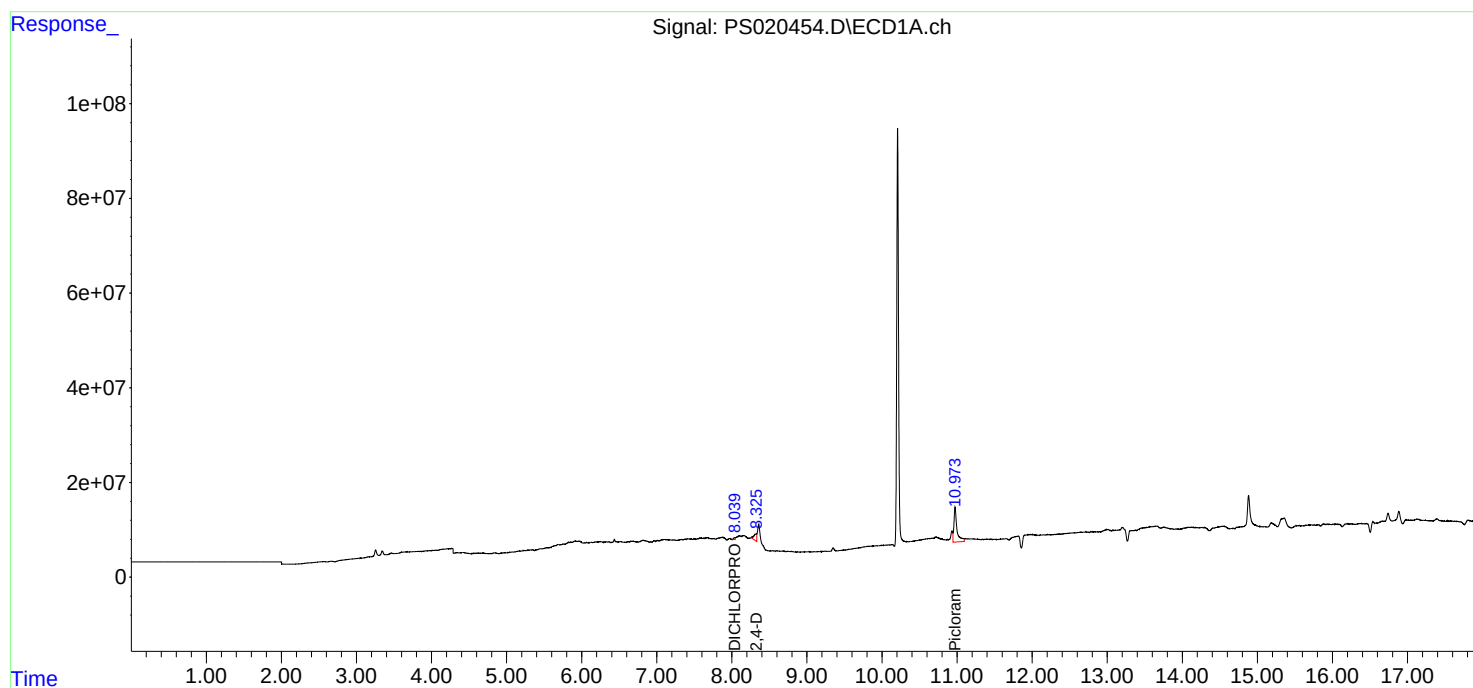

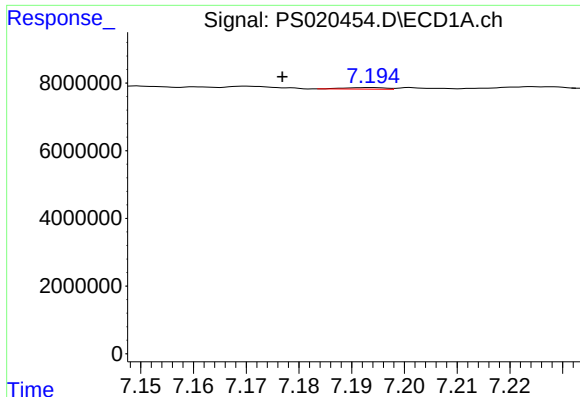


#4 2,4-DCAA

R.T.: 7.193 min
Delta R.T.: 0.016 min
Response: 252097
Conc: N.D.

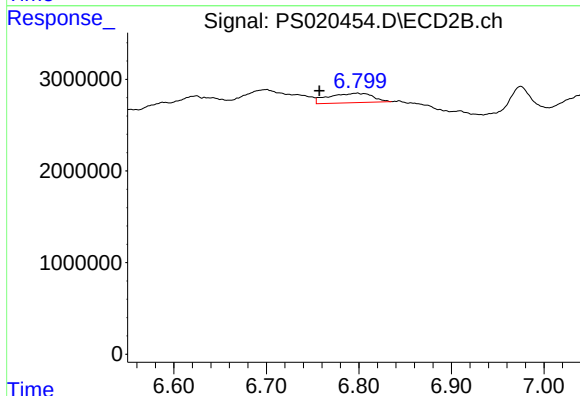


#4 2,4-DCAA

R.T.: 6.798 min
Delta R.T.: 0.041 min
Response: 3397007
Conc: 3.19 ng/ml

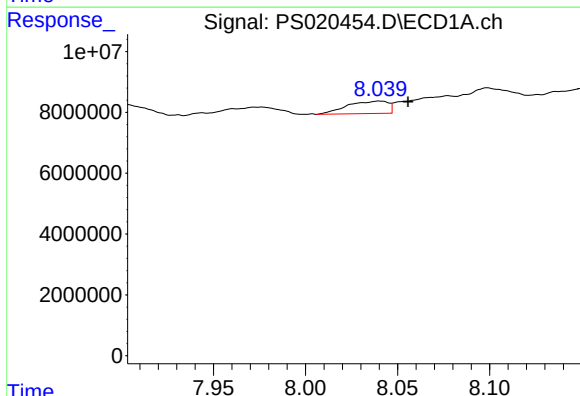


#8 DICHLORPROP

R.T.: 8.040 min
Delta R.T.: -0.016 min
Response: 6311915
Conc: 1.91 ng/ml

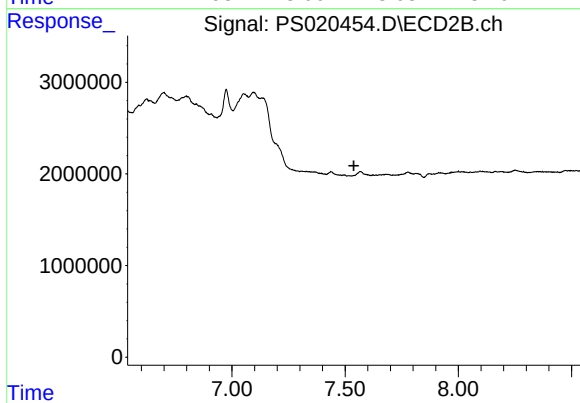


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.539 min
Response: 0
Conc: N.D.

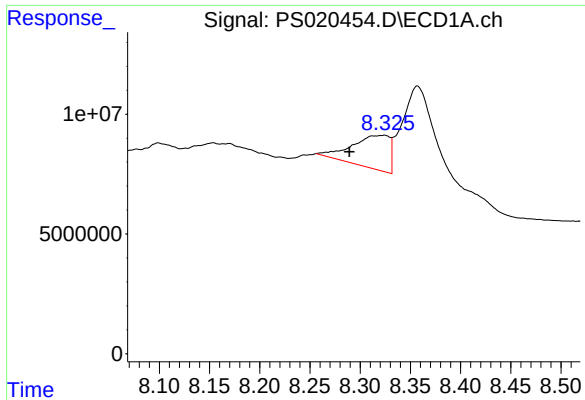


#9 2,4-D

R.T.: 8.324 min
Delta R.T.: 0.035 min
Response: 36231821
Conc: 7.72 ng/ml

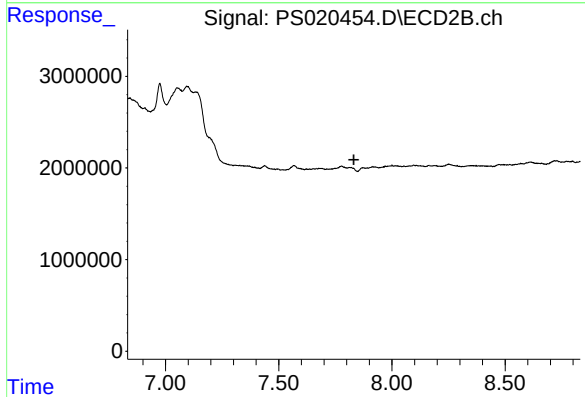


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 7.832 min
Response: 0
Conc: N.D.

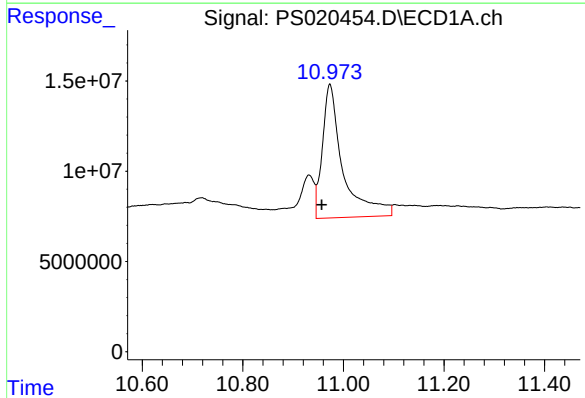


#15 Picloram

R.T.: 10.973 min
Delta R.T.: 0.016 min
Response: 209469923
Conc: 5.06 ng/ml

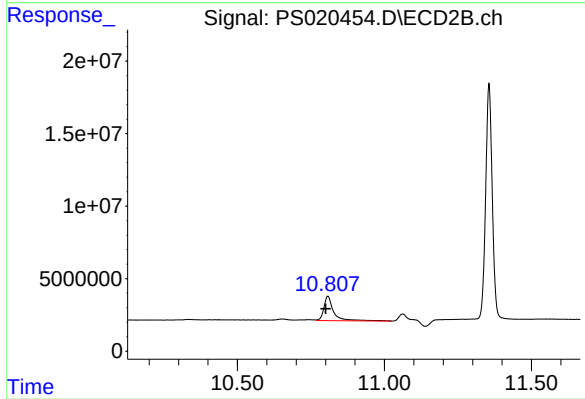


#15 Picloram

R.T.: 10.807 min
Delta R.T.: 0.007 min
Response: 39082101
Conc: 3.81 ng/ml

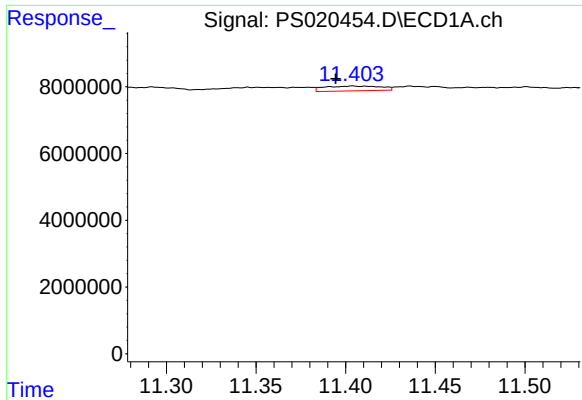

#16 DCPA

R.T.: 11.404 min
Delta R.T.: 0.010 min
Response: 3162899
Conc: N.D.

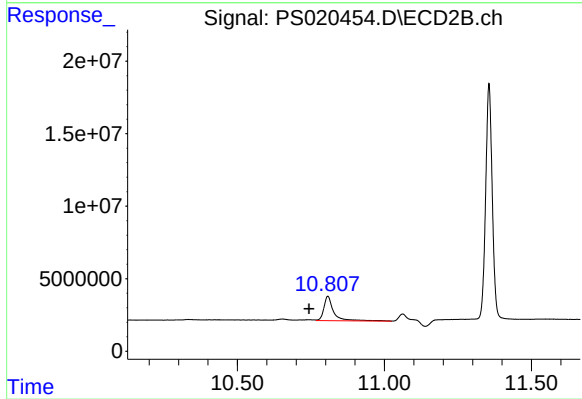

#16 DCPA

R.T.: 10.807 min
Delta R.T.: 0.063 min
Response: 39082101
Conc: 4.39 ng/ml