

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090622\
 Data File : PS020459.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Sep 2022 12:47
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 06 16:34:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090222.M
 Quant Title : 8080.M
 QLast Update : Sat Sep 03 01:06:55 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
4) S	2,4-DCAA	7.178	6.757	1234.8E6	433.4E6	350.329	407.468
Target Compounds							
2) T	3,5-DICHL...	6.333f	0.000	844330	0	<MDL	N.D. #
6) T	MCP	7.539	0.000	3804385	0	<MDL	N.D. #
7) T	MCPA	7.640f	7.200	1137413	15983411	<MDL	2.947 #
10) T	Pentachlo...	8.593	0.000	289434	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.106	0.000	3189871	0	<MDL	N.D. #
14) T	DINOSEB	11.120	0.000	20005427	0	<MDL	N.D. #
15) T	Picloram	10.900f	10.850f	10785138	22639839	<MDL	2.204 #
16) T	DCPA	11.415	0.000	1664743	0	<MDL	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090622\
Data File : PS020459.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Sep 2022 12:47
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 06 16:34:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090222.M
Quant Title : 8080.M
QLast Update : Sat Sep 03 01:06:55 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

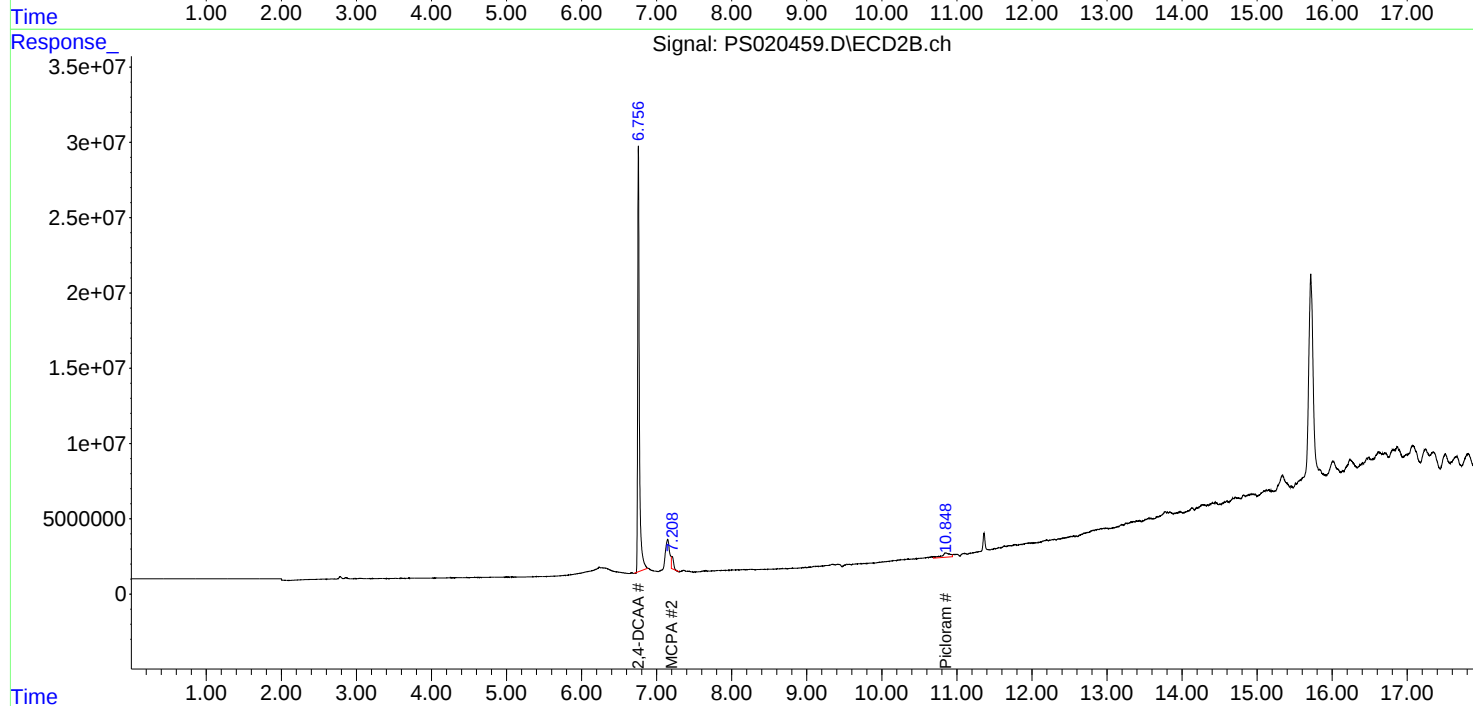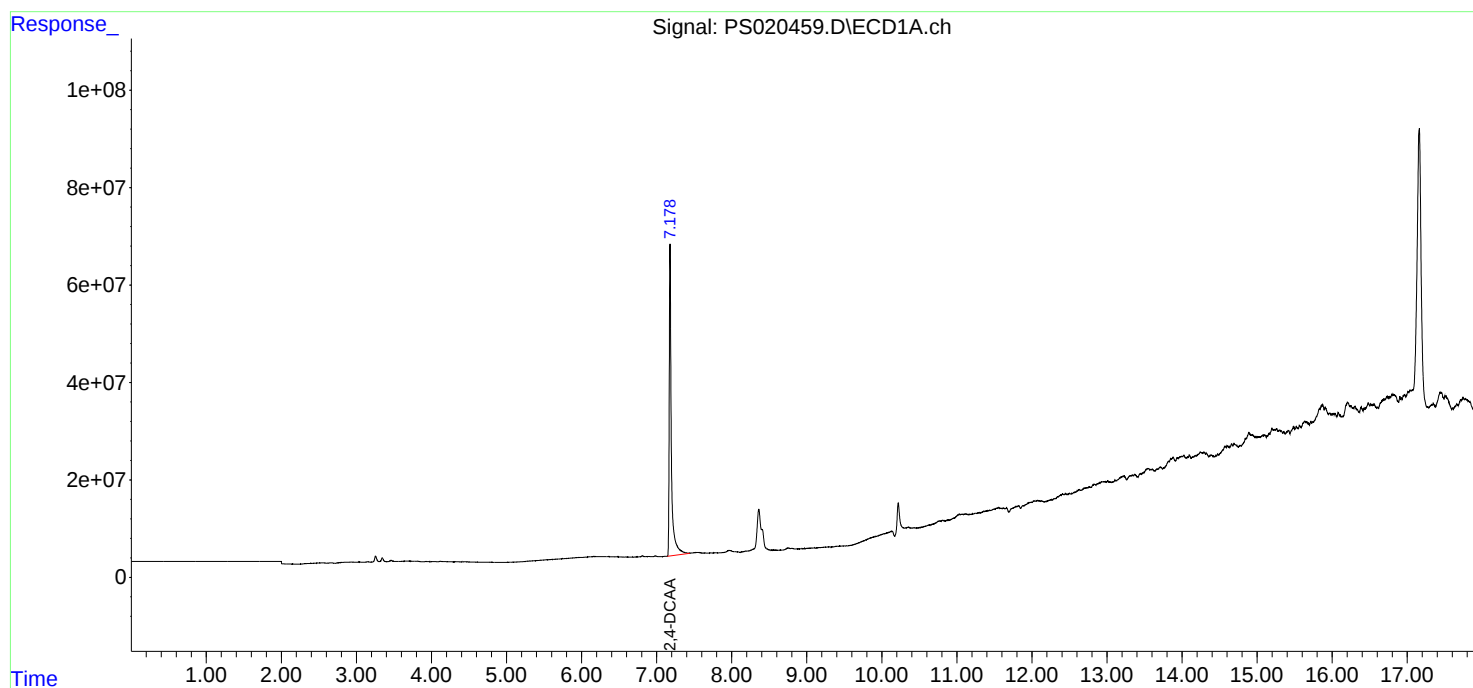

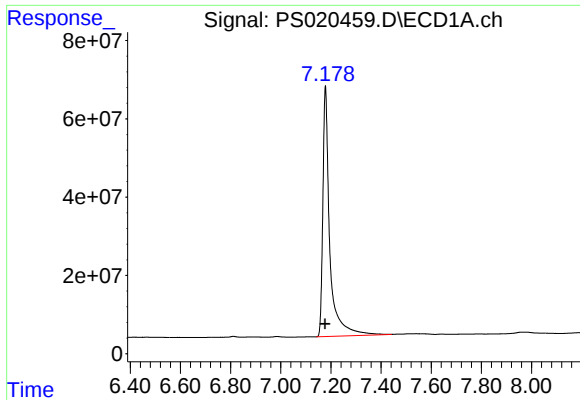


#4 2,4-DCAA

R.T.: 7.178 min
Delta R.T.: 0.001 min
Response: 1234792408
Conc: 350.33 ng/ml

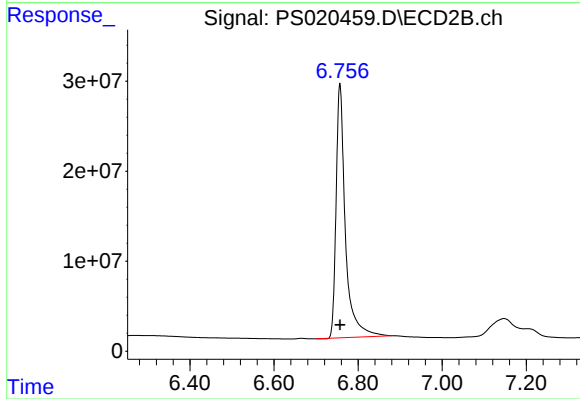


#4 2,4-DCAA

R.T.: 6.757 min
Delta R.T.: 0.000 min
Response: 433419923
Conc: 407.47 ng/ml

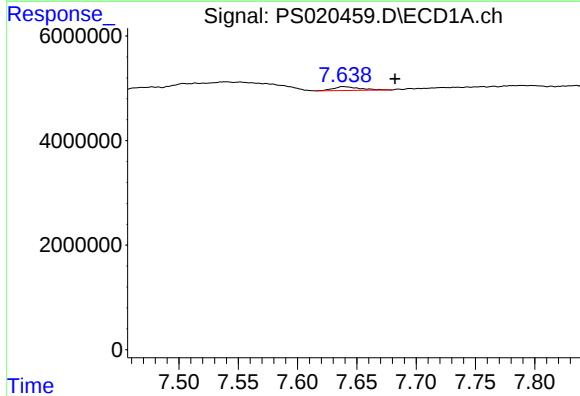


#7 MCPA

R.T.: 7.640 min
Delta R.T.: -0.043 min
Response: 1137413
Conc: N.D.

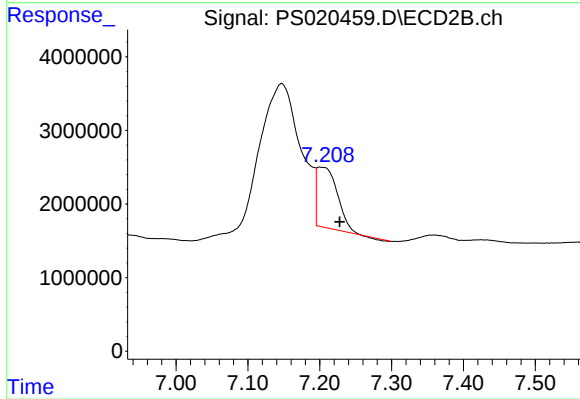


#7 MCPA

R.T.: 7.200 min
Delta R.T.: -0.028 min
Response: 15983411
Conc: 2.95 ug/ml

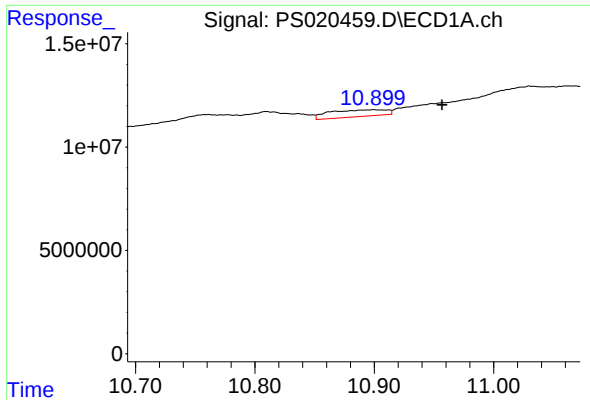

#15 Picloram

R.T.: 10.900 min
Delta R.T.: -0.057 min
Response: 10785138
Conc: N.D.

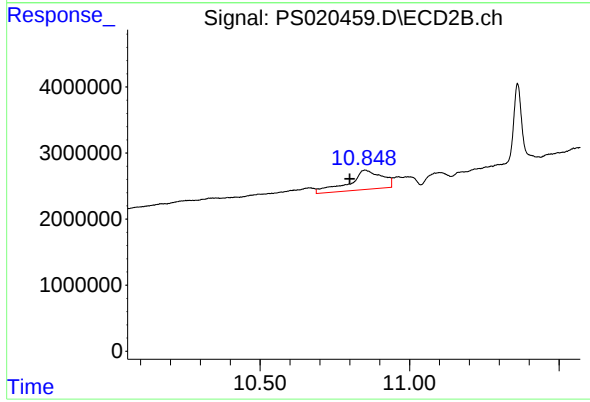

#15 Picloram

R.T.: 10.850 min
Delta R.T.: 0.049 min
Response: 22639839
Conc: 2.20 ng/ml