

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090622\
 Data File : PS020466.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Sep 2022 18:30
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 06 18:57:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090222.M
 Quant Title : 8080.M
 QLast Update : Sat Sep 03 01:06:55 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
4) S	2,4-DCAA	7.179	6.759	1317.1E6	439.2E6	373.675	412.898
Target Compounds							
2) T	3,5-DICHL...	6.454f	0.000	2048435	0	<MDL	N.D. #
6) T	MCP	7.512	0.000	436674	0	<MDL	N.D. #
7) T	MCPA	7.640f	0.000	2355948	0	<MDL	N.D. #
9) T	2,4-D	8.359f	0.000	149.0E6	0	31.749	N.D. #
10) T	Pentachlo...	8.597	8.256	3832768	2037786	<MDL	<MDL #
11) T	2,4,5-TP ...	9.160	0.000	3668486	0	<MDL	N.D. #
12) T	2,4,5-T	9.422	0.000	30359028	0	1.309	N.D. #
13) T	2,4-DB	9.963	0.000	475851	0	<MDL	N.D. #
15) T	Picloram	0.000	10.854f	0	39789437	N.D.	3.874
16) T	DCPA	11.396	10.746	11398657	1775276	<MDL	<MDL #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090622\
Data File : PS020466.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Sep 2022 18:30
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 06 18:57:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090222.M
Quant Title : 8080.M
QLast Update : Sat Sep 03 01:06:55 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

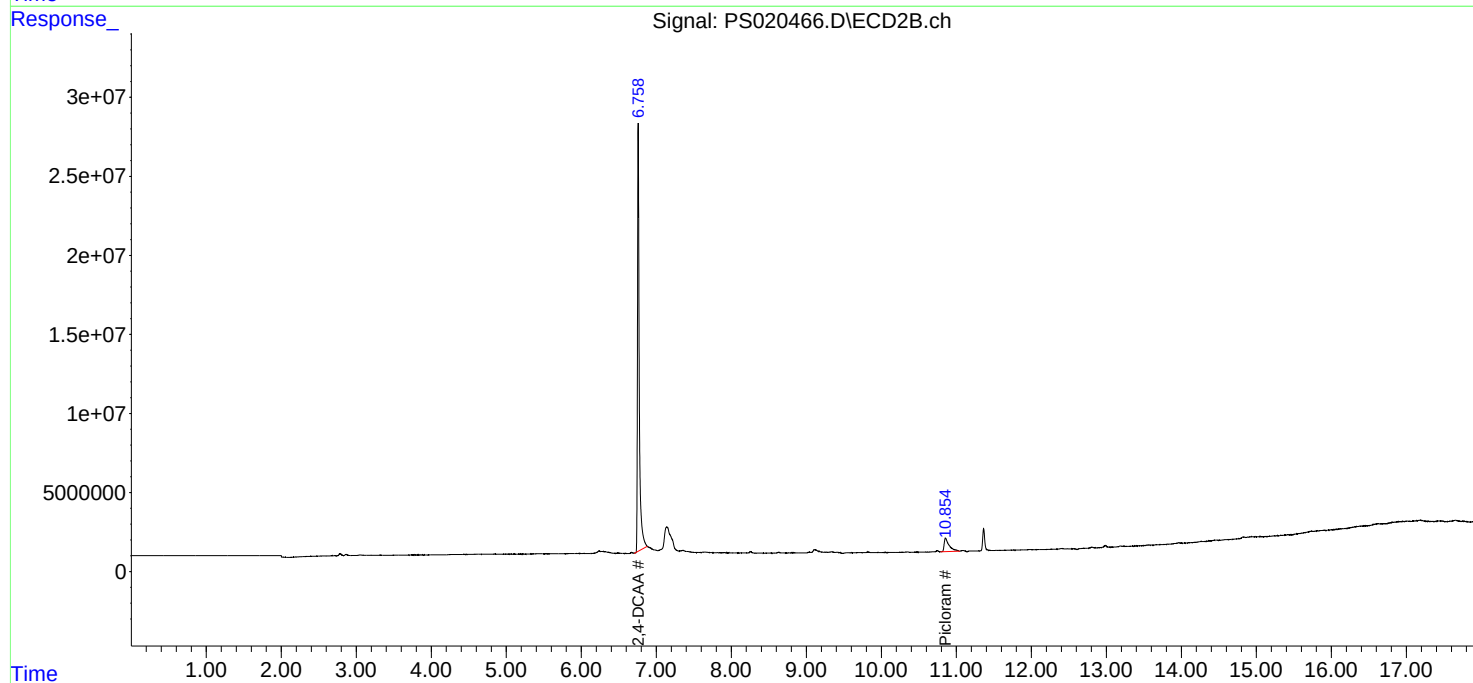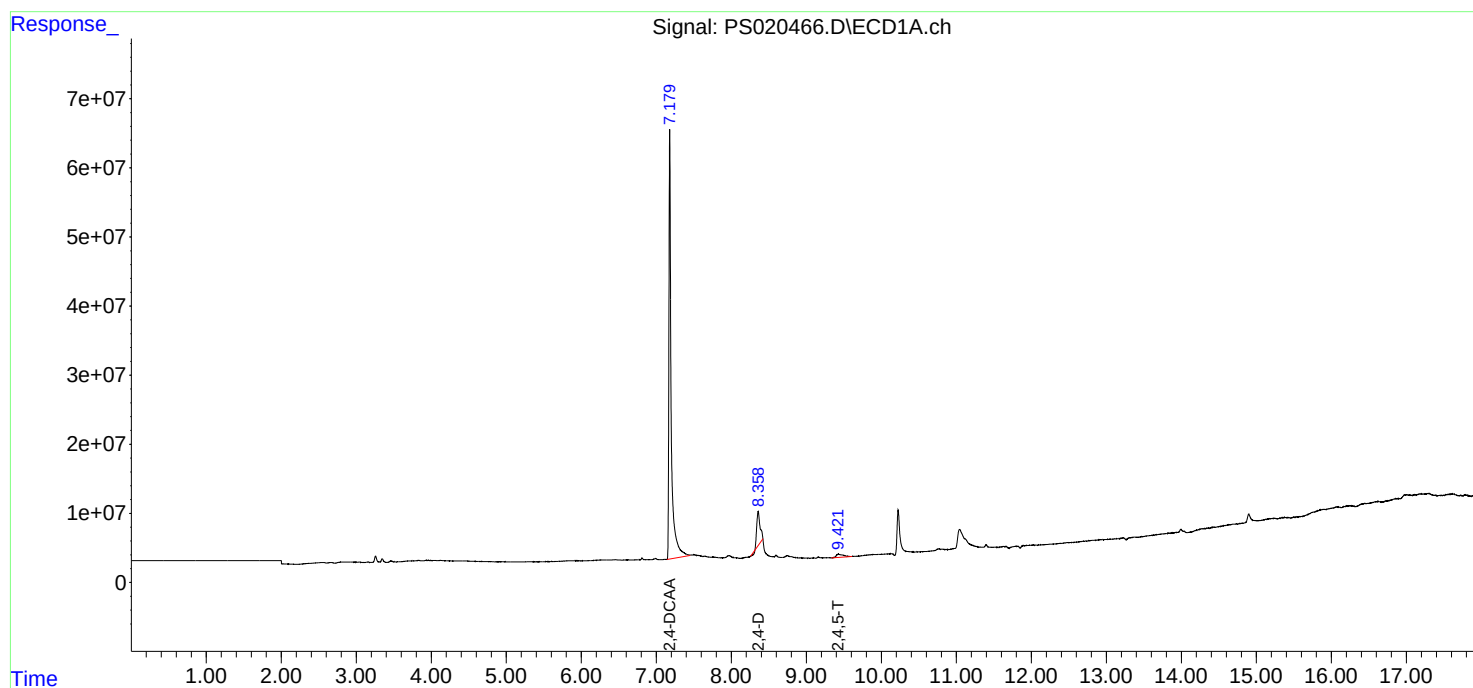

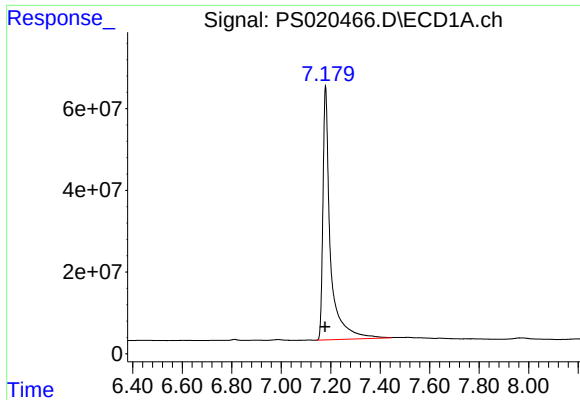


#4 2,4-DCAA

R.T.: 7.179 min
Delta R.T.: 0.002 min
Response: 1317079917
Conc: 373.68 ng/ml

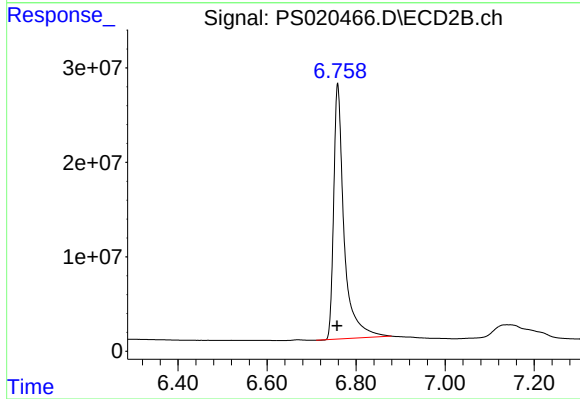


#4 2,4-DCAA

R.T.: 6.759 min
Delta R.T.: 0.001 min
Response: 439195830
Conc: 412.90 ng/ml

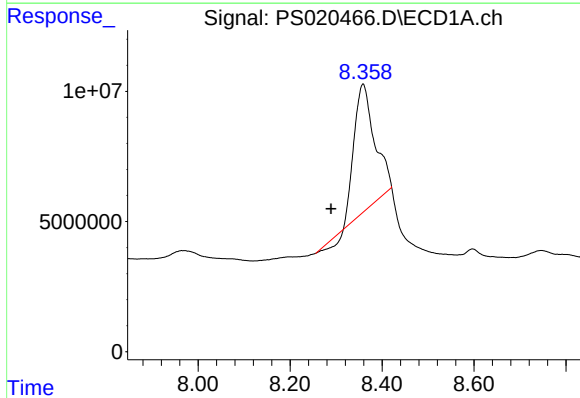


#9 2,4-D

R.T.: 8.359 min
Delta R.T.: 0.069 min
Response: 148950196
Conc: 31.75 ng/ml

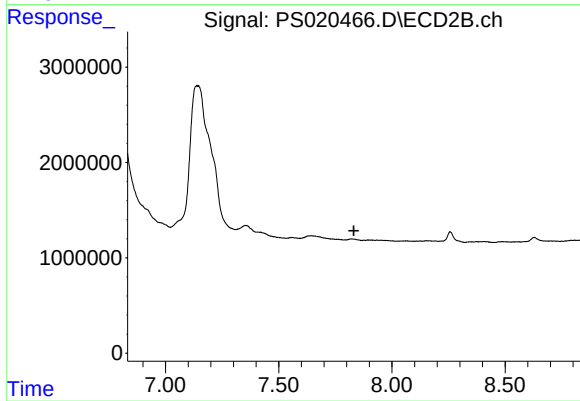


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 7.832 min
Response: 0
Conc: N.D.

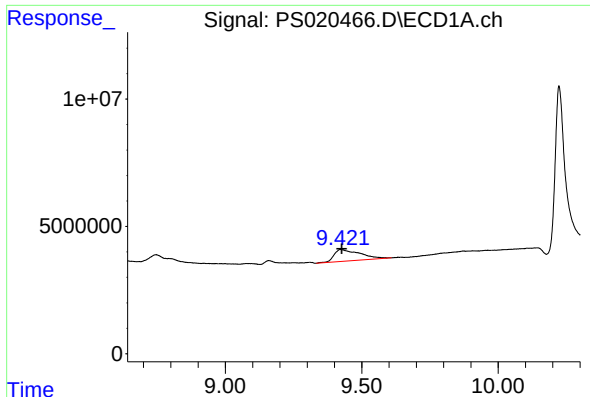


#12 2,4,5-T

R.T.: 9.422 min
Delta R.T.: -0.005 min
Response: 30359028
Conc: 1.31 ng/ml

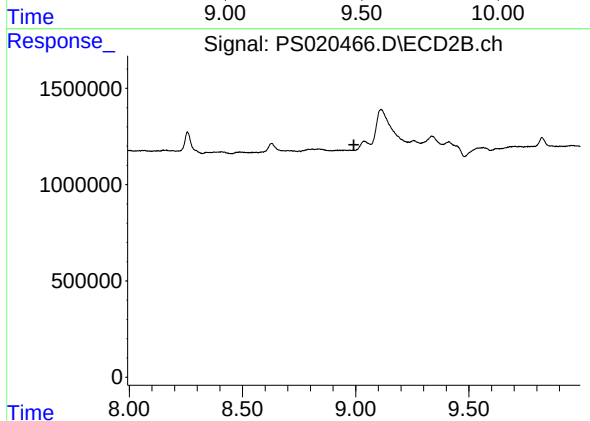


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 8.992 min
Response: 0
Conc: N.D.

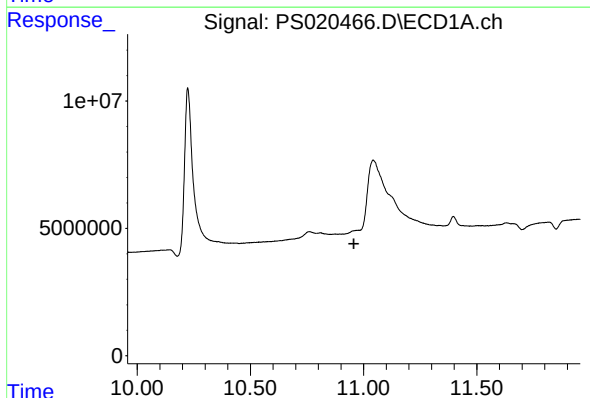

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 10.957 min
Response: 0
Conc: N.D.

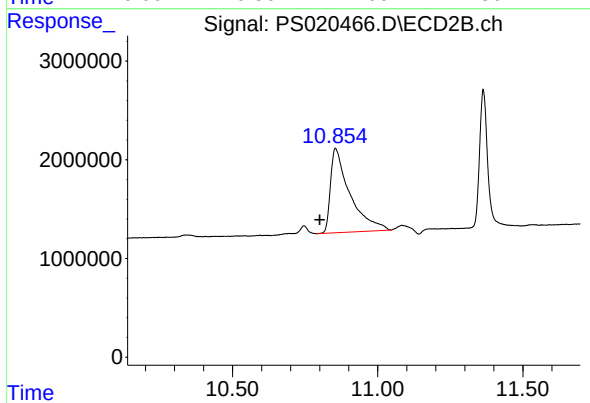

#15 Picloram

R.T.: 10.854 min
Delta R.T.: 0.054 min
Response: 39789437
Conc: 3.87 ng/ml