

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090623\
 Data File : PS024249.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Sep 2023 14:07
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 06 20:47:14 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082823.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 28 16:48:10 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.333	6.784	12447283	1643994	6.248	2.448 #
Target Compounds							
1) T	Dalapon	2.518	2.574	8566939	4413227	3.942	4.185
2) T	3,5-DICHL...	0.000	5.926f	0	1077780	N.D.	1.034
3) T	4-Nitroph...	6.200	6.364f	16912257	275744	13.613	<MDL #
5) T	DICAMBA	6.575f	6.996f	584073	263.8E6	<MDL	91.607 #
6) T	MCPD	6.683	7.085	712595	457341	<MDL	<MDL #
7) T	MCPA	6.753	7.199f	-605378	8829147	N.D.	3.021
8) T	DICHLORPROP	7.089	7.578	2308141	2655193	1.015	3.654 #
9) T	2,4-D	7.257	7.797f	2966.3E6	1110400	1115.210	1.246 #
10) T	Pentachlo...	7.520	8.272	1140983	873359	<MDL	<MDL #
11) T	2,4,5-TP ...	8.050	8.632	4193814	1622618	<MDL	<MDL #
12) T	2,4,5-T	8.304	9.006	3306393	428988	<MDL	<MDL #
13) T	2,4-DB	8.796	0.000	535498	0	<MDL	N.D. #
14) T	DINOSEB	9.853	9.838	3379871	50218	<MDL	<MDL #
15) T	Picloram	9.666	10.793	194.7E6	44110171	11.921	7.427 #
16) T	DCPA	10.167f	10.793	-1301416	44110171	N.D.	8.599



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090623\
Data File : PS024249.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Sep 2023 14:07
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 06 20:47:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082823.M
Quant Title : 8080.M
QLast Update : Mon Aug 28 16:48:10 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

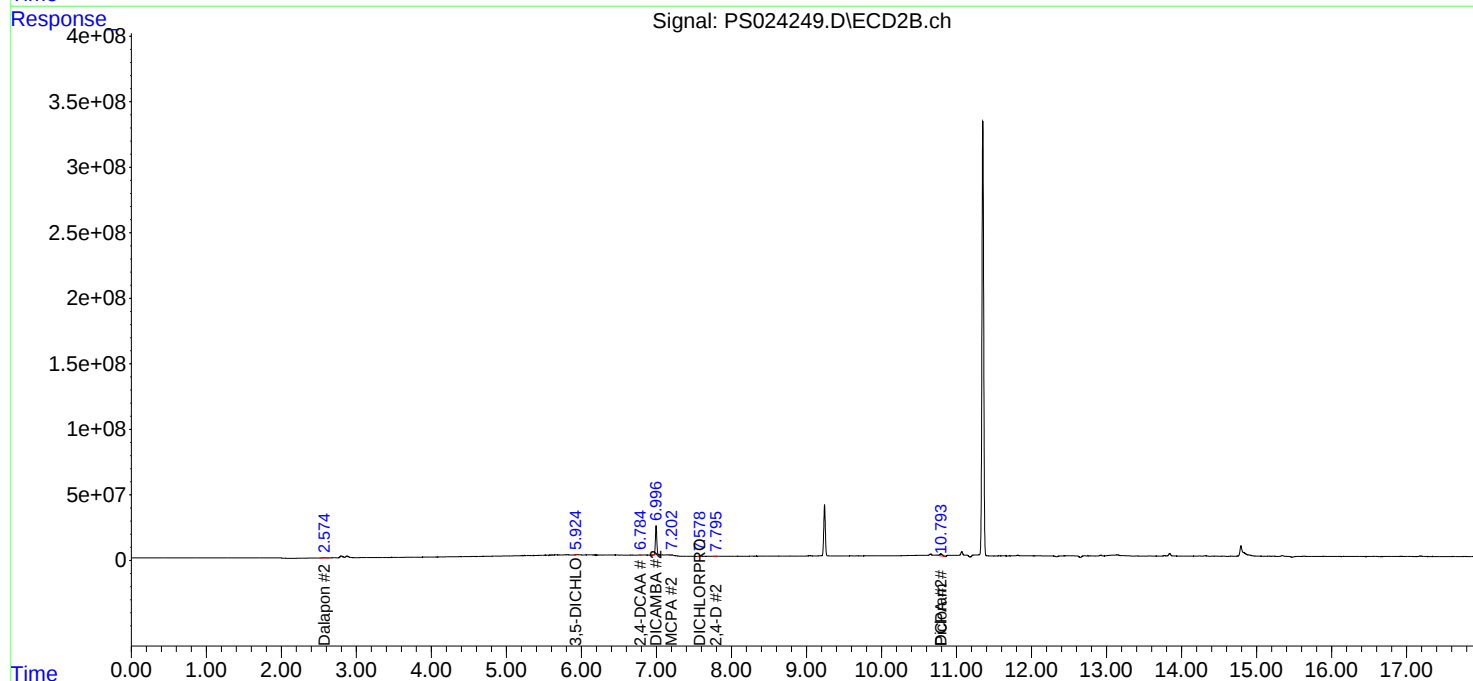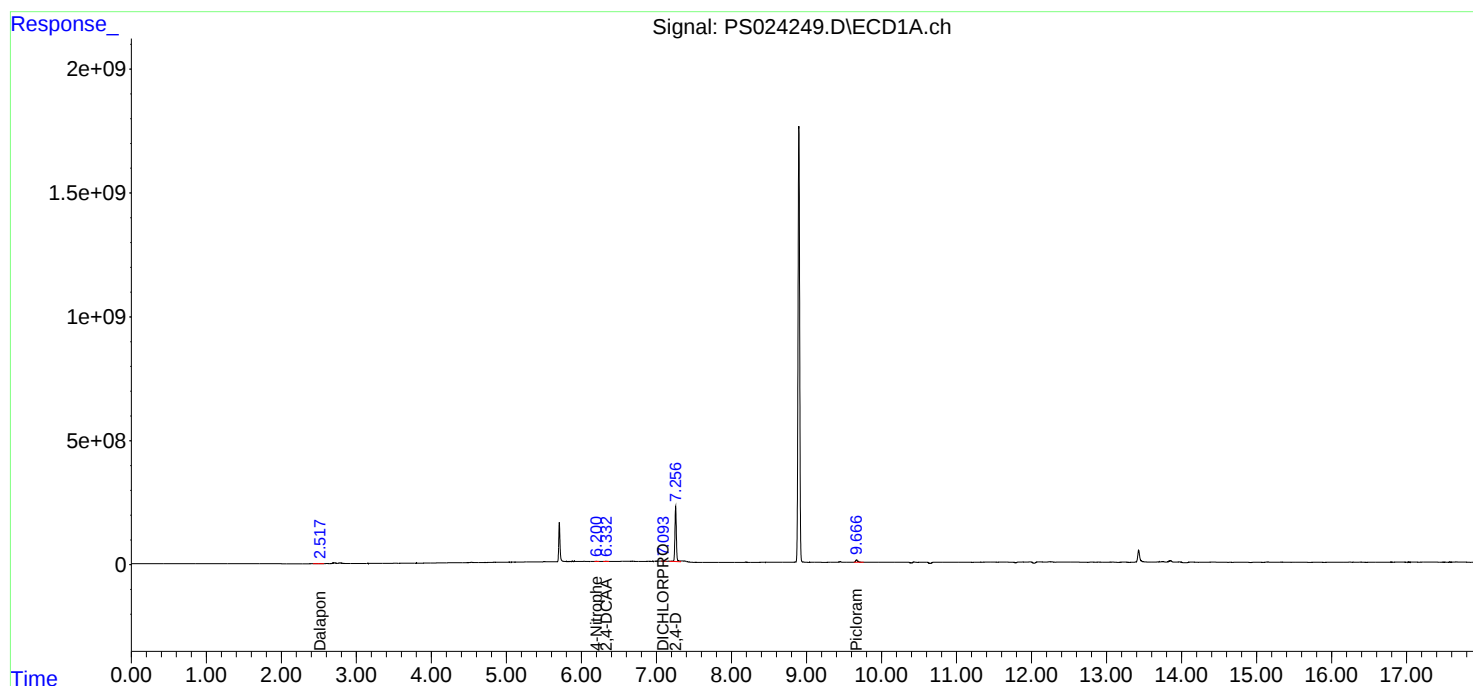


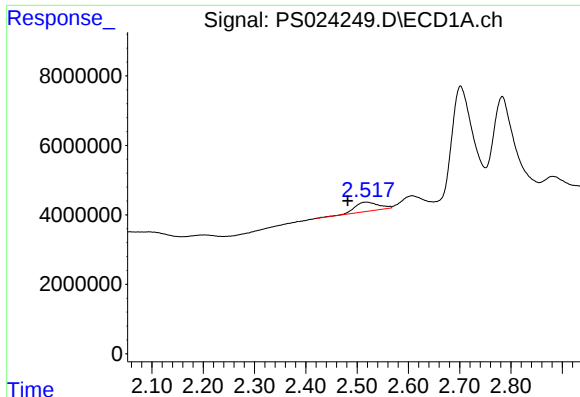

#1 Dalapon


R.T.: 2.518 min
Delta R.T.: 0.036 min
Response: 8566939
Conc: 3.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

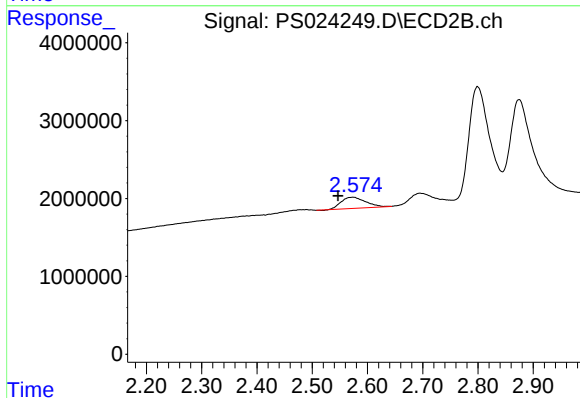


#1 Dalapon

R.T.: 2.574 min
Delta R.T.: 0.027 min
Response: 4413227
Conc: 4.19 ng/ml

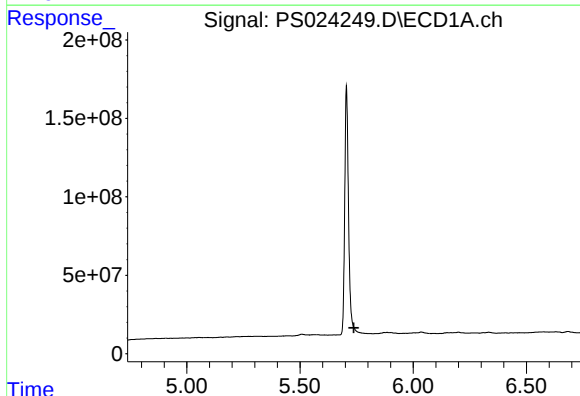


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.738 min
Response: 0
Conc: N.D.

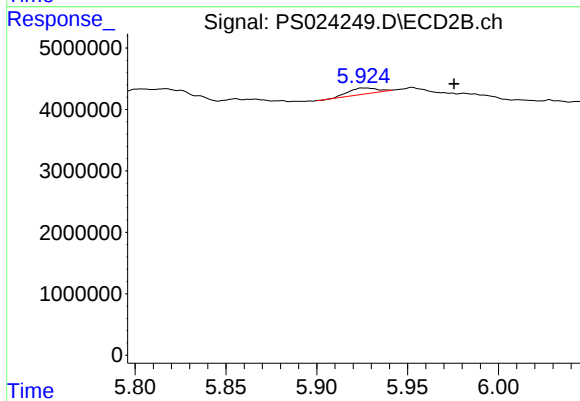

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.926 min
Delta R.T.: -0.049 min
Response: 1077780
Conc: 1.03 ng/ml

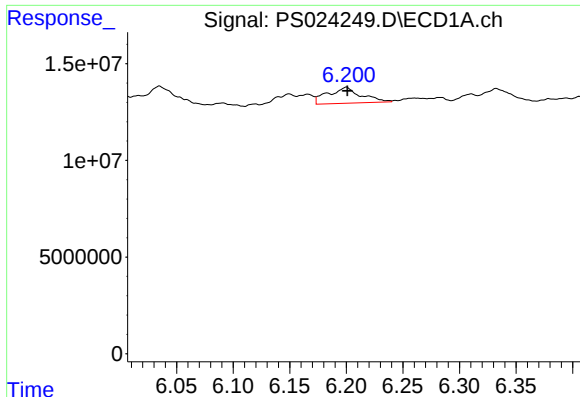

#3 4-Nitrophenol


R.T.: 6.200 min
Delta R.T.: -0.001 min
Response: 16912257
Conc: 13.61 ng/ml

Instrument :
ECD_S
ClientSampleId :

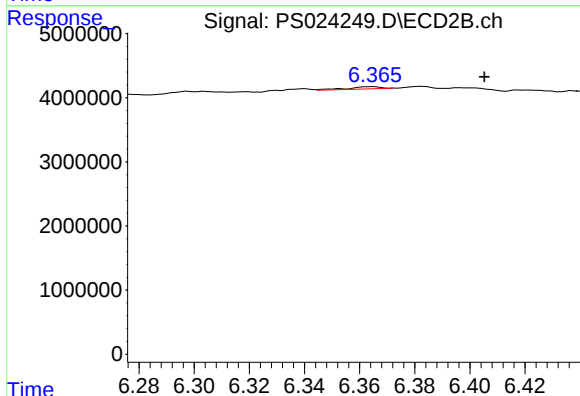


#3 4-Nitrophenol

R.T.: 6.364 min
Delta R.T.: -0.041 min
Response: 275744
Conc: N.D.

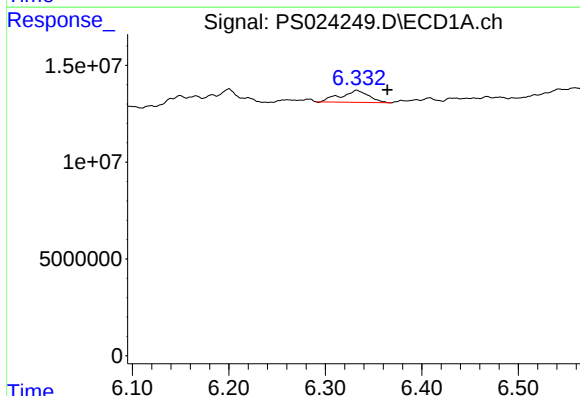


#4 2,4-DCAA

R.T.: 6.333 min
Delta R.T.: -0.032 min
Response: 12447283
Conc: 6.25 ng/ml

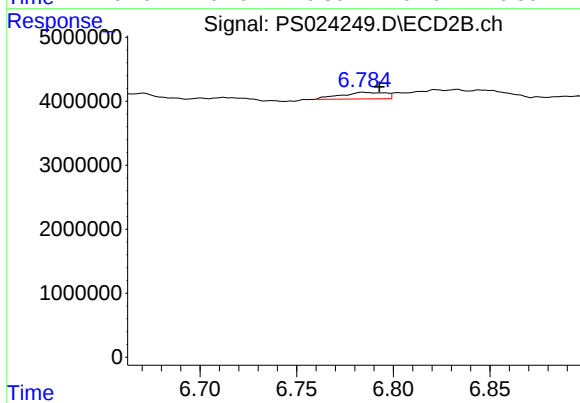

#4 2,4-DCAA


R.T.: 6.784 min
Delta R.T.: -0.009 min
Response: 1643994
Conc: 2.45 ng/ml

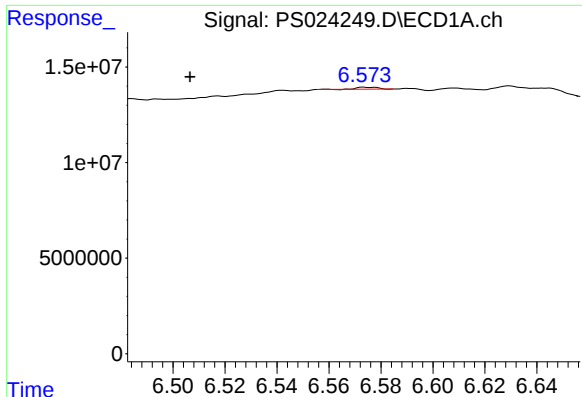

#5 DICAMBA


R.T.: 6.575 min
Delta R.T.: 0.069 min
Response: 584073
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

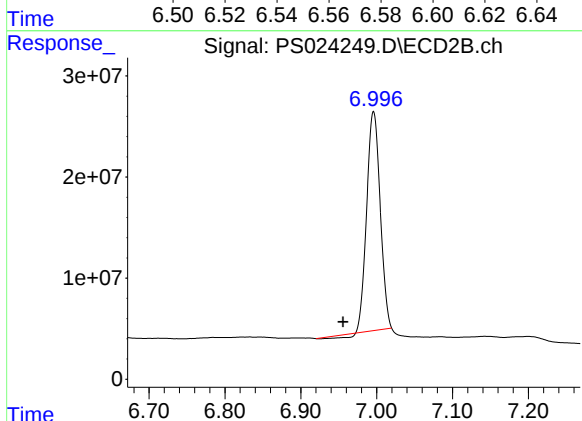


#5 DICAMBA

R.T.: 6.996 min
Delta R.T.: 0.040 min
Response: 263843739
Conc: 91.61 ng/ml

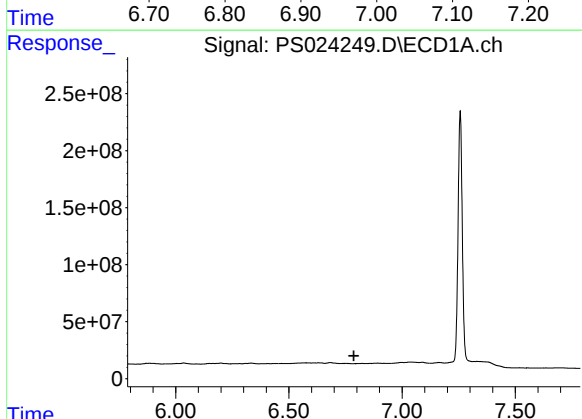


#7 MCPA

R.T.: 6.753 min
Delta R.T.: -0.033 min
Response: -605378
Conc: N.D.

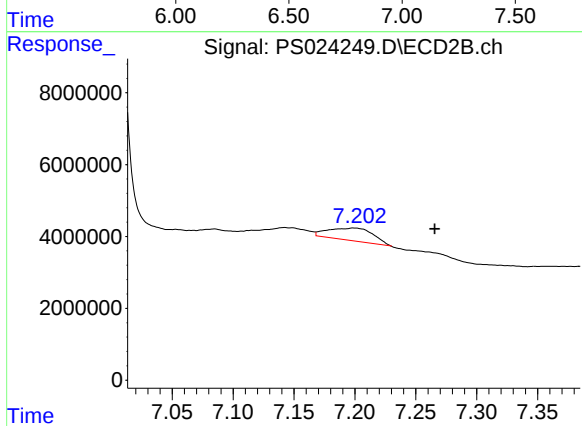

#7 MCPA


R.T.: 7.199 min
Delta R.T.: -0.066 min
Response: 8829147
Conc: 3.02 ug/ml

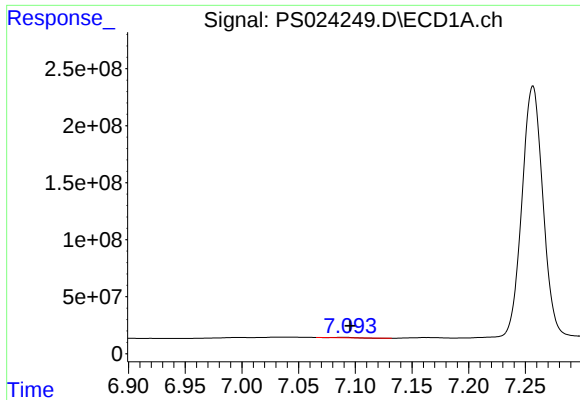

#8 DICHLORPROP


R.T.: 7.089 min
Delta R.T.: -0.006 min
Response: 2308141
Conc: 1.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

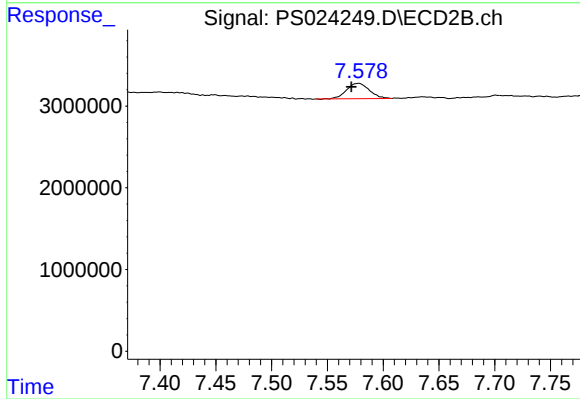


#8 DICHLORPROP

R.T.: 7.578 min
Delta R.T.: 0.006 min
Response: 2655193
Conc: 3.65 ng/ml

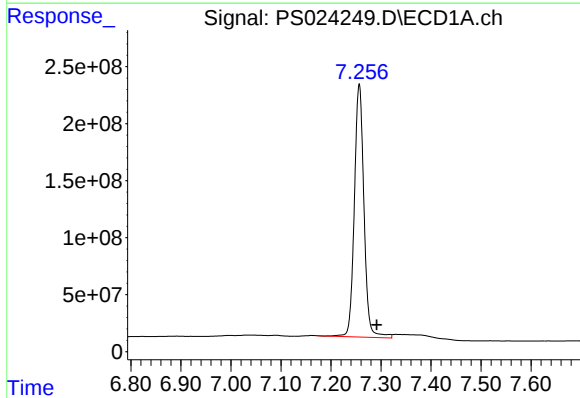


#9 2,4-D

R.T.: 7.257 min
Delta R.T.: -0.035 min
Response: 2966329382
Conc: 1115.21 ng/ml

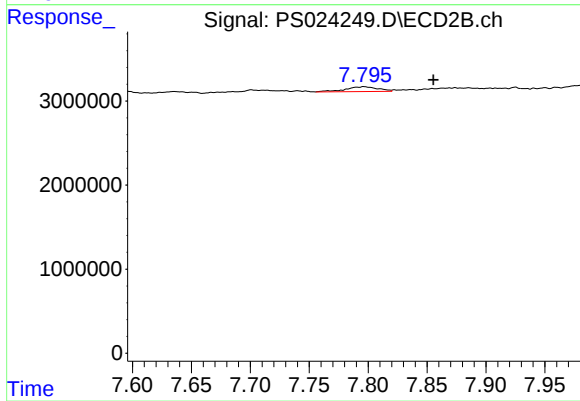

#9 2,4-D


R.T.: 7.797 min
Delta R.T.: -0.059 min
Response: 1110400
Conc: 1.25 ng/ml

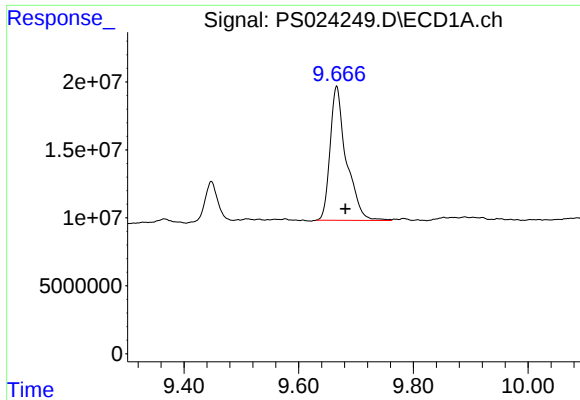

#15 Picloram


R.T.: 9.666 min
Delta R.T.: -0.016 min
Response: 194677658
Conc: 11.92 ng/ml

Instrument :
ECD_S
ClientSampleId :

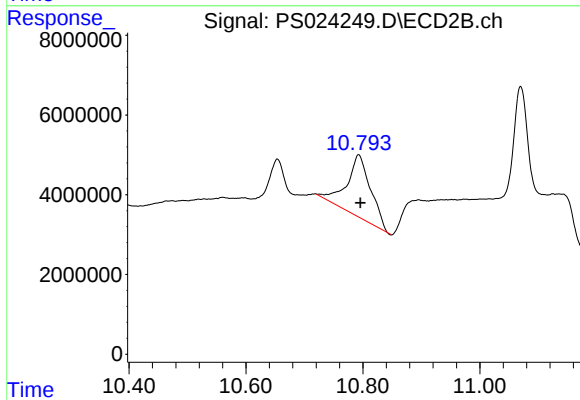


#15 Picloram

R.T.: 10.793 min
Delta R.T.: -0.003 min
Response: 44110171
Conc: 7.43 ng/ml

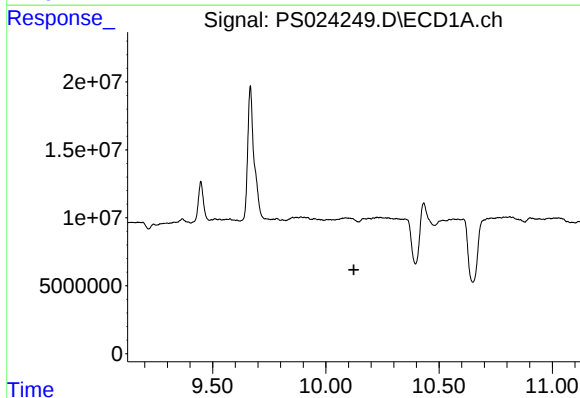

#16 DCPA

R.T.: 10.167 min
Delta R.T.: 0.044 min
Response: -1301416
Conc: N.D.

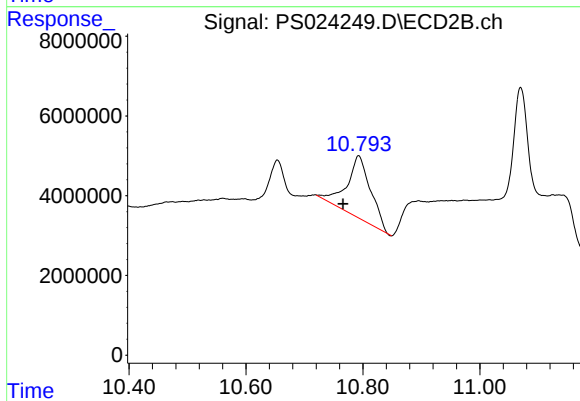

#16 DCPA

R.T.: 10.793 min
Delta R.T.: 0.026 min
Response: 44110171
Conc: 8.60 ng/ml