

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090623\
 Data File : PS024250.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Sep 2023 15:45
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 06 20:47:42 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082823.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 28 16:48:10 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.364	6.791	1057.9E6	358.8E6	530.972	534.304
Target Compounds							
1) T	Dalapon	2.514	2.573	5192177	1339326	2.389	1.270 #
3) T	4-Nitroph...	6.204	0.000	9246230	0	7.442	N.D. #
5) T	DICAMBA	6.496	6.949	961731	1035219	<MDL	<MDL #
6) T	MCP	6.684	6.998f	2481750	11237439	<MDL	5.866 #
7) T	MCPA	6.851f	7.253	742012	7275591	<MDL	2.489 #
8) T	DICHLORPROP	7.047f	7.582	840966	1496462	<MDL	2.060 #
9) T	2,4-D	7.255	7.799f	90088948	807674	33.870	<MDL #
10) T	Pentachlo...	0.000	8.282	0	615691	N.D.	<MDL
11) T	2,4,5-TP ...	8.044	8.634	1176940	1104583	<MDL	<MDL #
12) T	2,4,5-T	8.299	9.052f	1296568	1460467	<MDL	<MDL #
13) T	2,4-DB	8.747f	9.509	94043	981628	<MDL	2.136 #
14) T	DINOSEB	9.856	0.000	1509328	0	<MDL	N.D. #
15) T	Picloram	9.660	10.797	38199587	10495561	2.339	1.767
16) T	DCPA	10.117	10.797	1368268	10495561	<MDL	2.046 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090623\
Data File : PS024250.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Sep 2023 15:45
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 06 20:47:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082823.M
Quant Title : 8080.M
QLast Update : Mon Aug 28 16:48:10 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

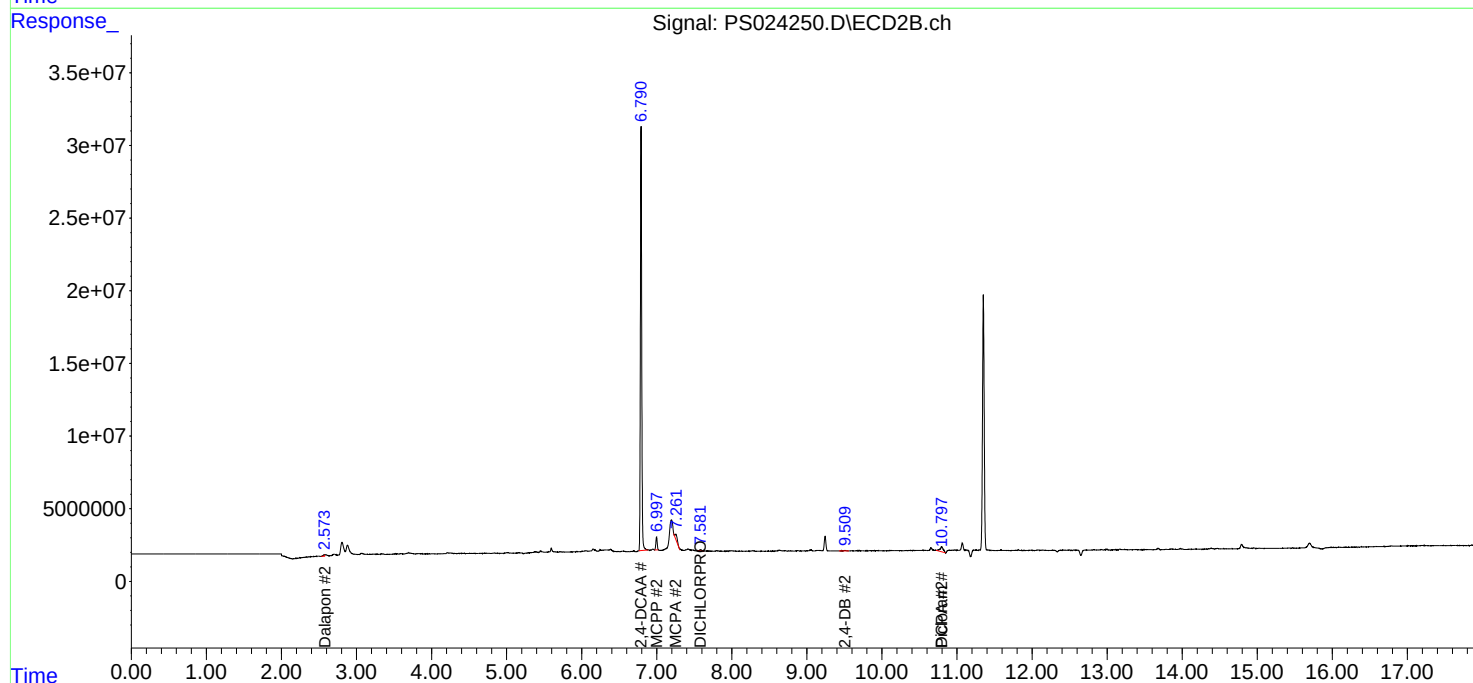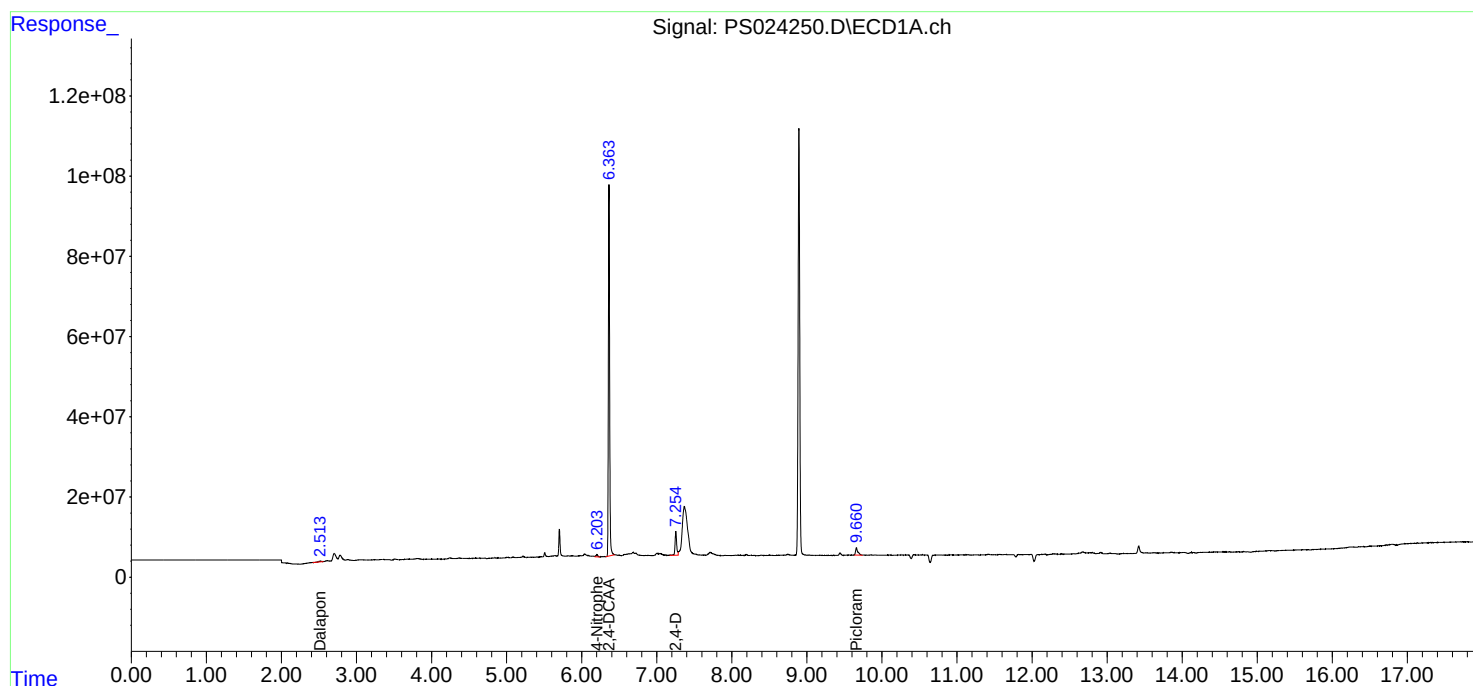


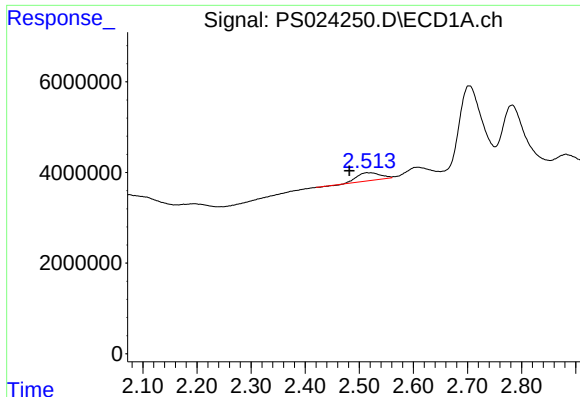

#1 Dalapon


R.T.: 2.514 min
Delta R.T.: 0.032 min
Response: 5192177
Conc: 2.39 ng/ml

Instrument :
ECD_S
ClientSampleId :

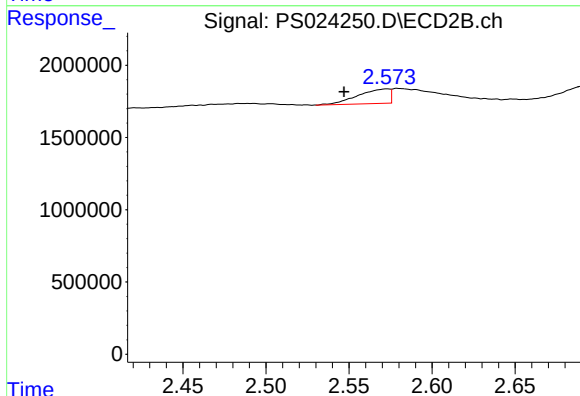


#1 Dalapon

R.T.: 2.573 min
Delta R.T.: 0.026 min
Response: 1339326
Conc: 1.27 ng/ml

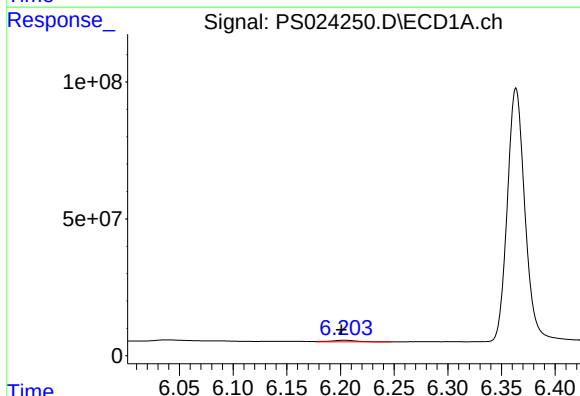


#3 4-Nitrophenol

R.T.: 6.204 min
Delta R.T.: 0.003 min
Response: 9246230
Conc: 7.44 ng/ml

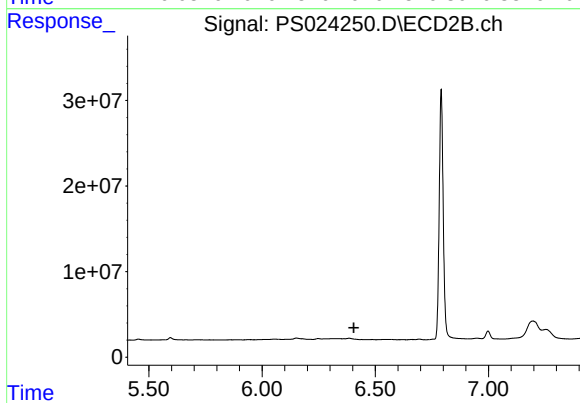

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.405 min
Response: 0
Conc: N.D.

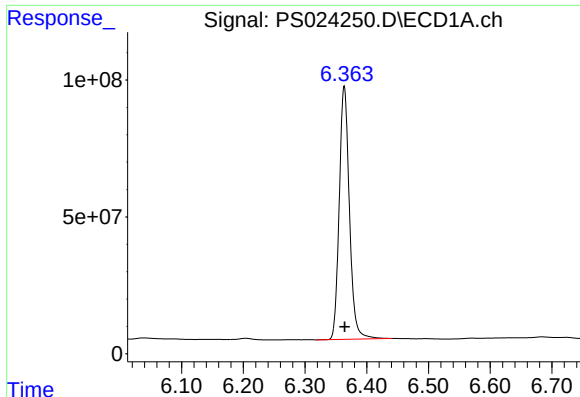

#4 2,4-DCAA


R.T.: 6.364 min
Delta R.T.: 0.000 min
Response: 1057867486
Conc: 530.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

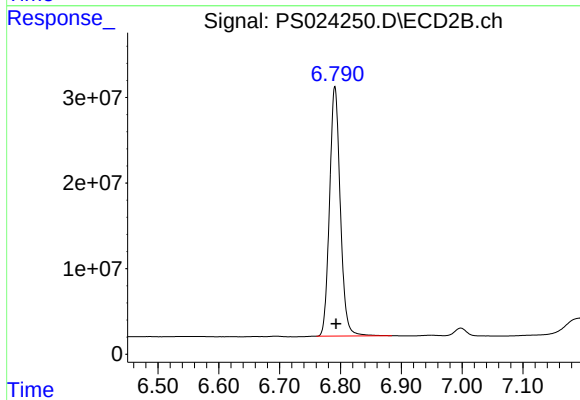


#4 2,4-DCAA

R.T.: 6.791 min
Delta R.T.: -0.002 min
Response: 358834122
Conc: 534.30 ng/ml

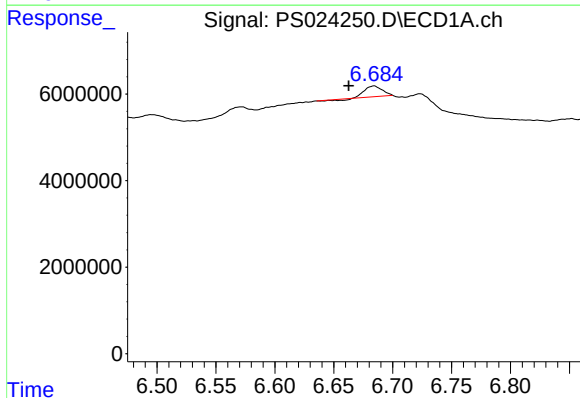


#6 MCP

R.T.: 6.684 min
Delta R.T.: 0.021 min
Response: 2481750
Conc: N.D.

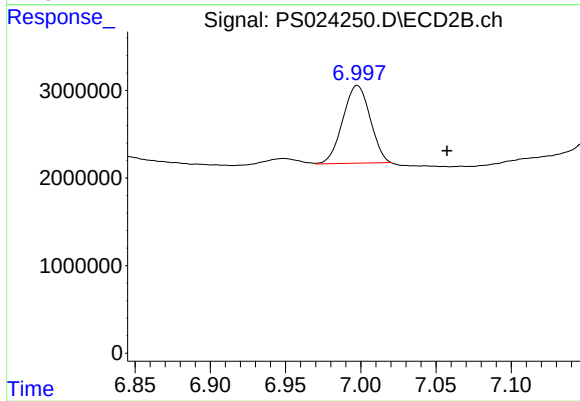

#6 MCP


R.T.: 6.998 min
Delta R.T.: -0.060 min
Response: 11237439
Conc: 5.87 ug/ml

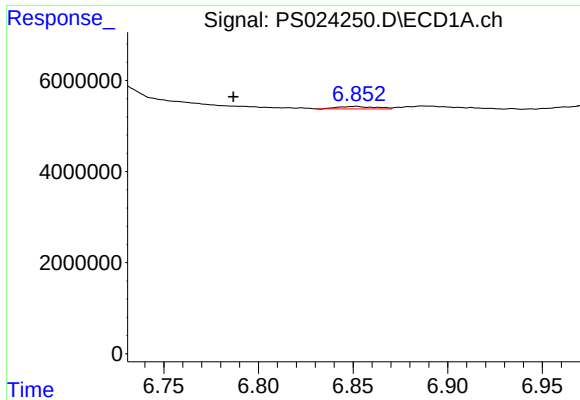

#7 MCPA


R.T.: 6.851 min
Delta R.T.: 0.064 min
Response: 742012
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

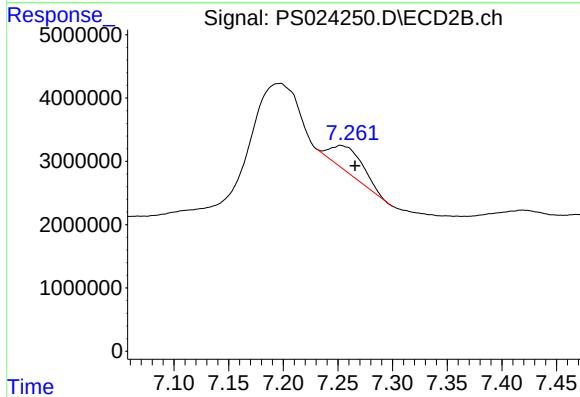


#7 MCPA

R.T.: 7.253 min
Delta R.T.: -0.013 min
Response: 7275591
Conc: 2.49 ug/ml

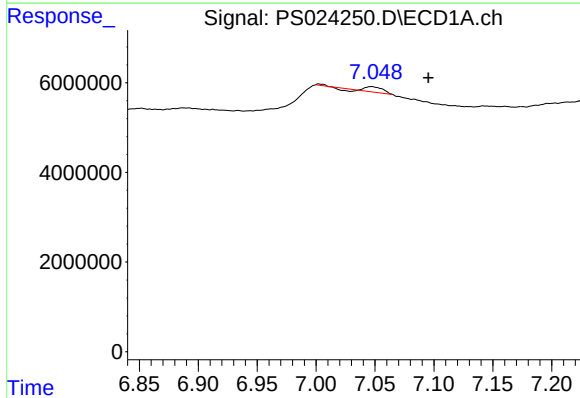


#8 DICHLORPROP

R.T.: 7.047 min
Delta R.T.: -0.048 min
Response: 840966
Conc: N.D.

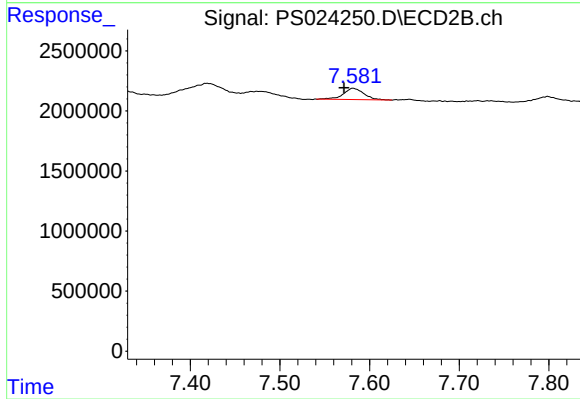

#8 DICHLORPROP


R.T.: 7.582 min
Delta R.T.: 0.010 min
Response: 1496462
Conc: 2.06 ng/ml

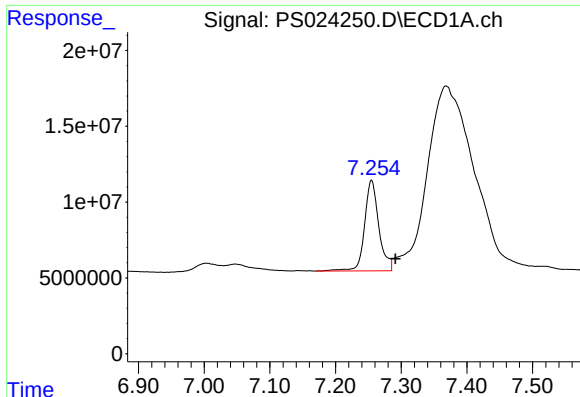

#9 2,4-D


R.T.: 7.255 min
Delta R.T.: -0.037 min
Response: 90088948
Conc: 33.87 ng/ml

Instrument :
ECD_S
ClientSampleId :

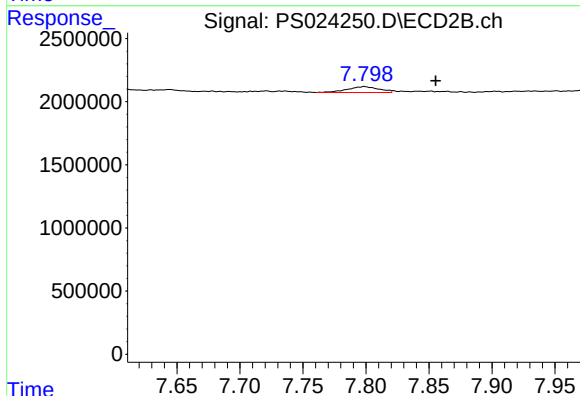


#9 2,4-D

R.T.: 7.799 min
Delta R.T.: -0.056 min
Response: 807674
Conc: N.D.

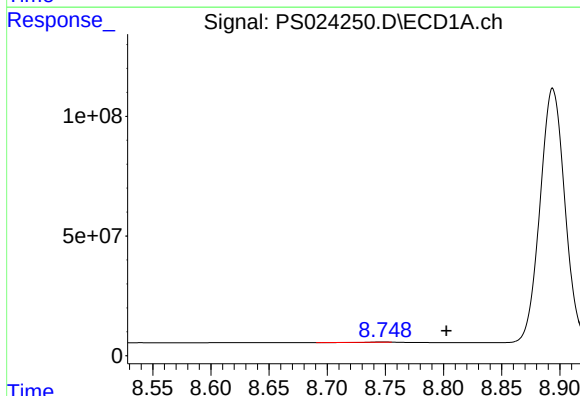


#13 2,4-DB

R.T.: 8.747 min
Delta R.T.: -0.055 min
Response: 94043
Conc: N.D.

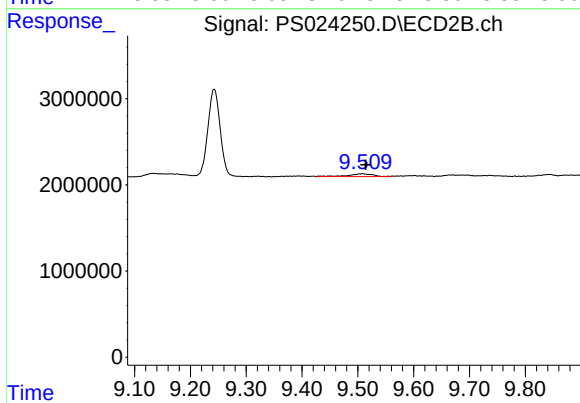

#13 2,4-DB


R.T.: 9.509 min
Delta R.T.: -0.005 min
Response: 981628
Conc: 2.14 ng/ml

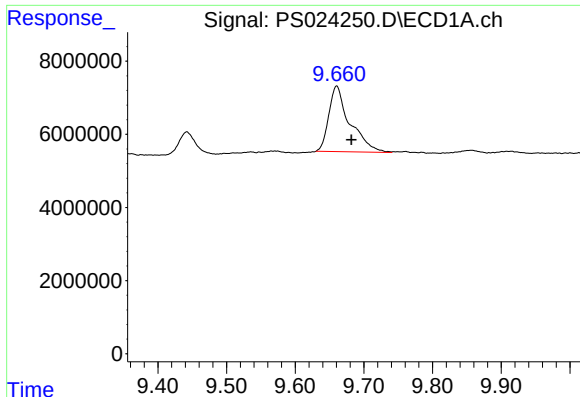

#15 Picloram


R.T.: 9.660 min
Delta R.T.: -0.021 min
Response: 38199587
Conc: 2.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

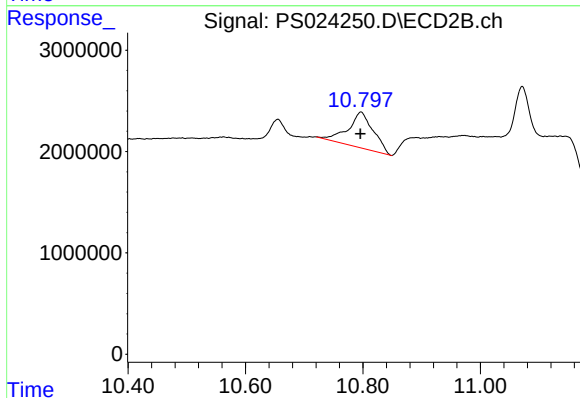


#15 Picloram

R.T.: 10.797 min
Delta R.T.: 0.000 min
Response: 10495561
Conc: 1.77 ng/ml

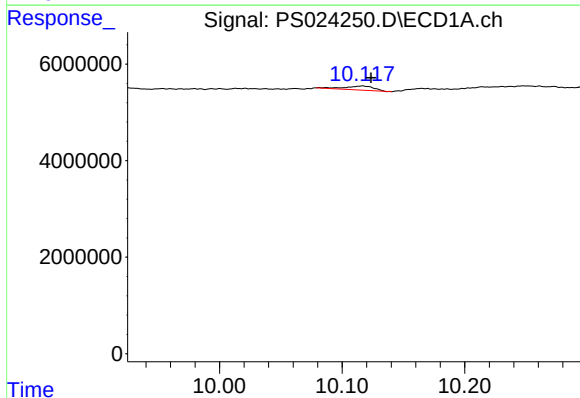

#16 DCPA

R.T.: 10.117 min
Delta R.T.: -0.007 min
Response: 1368268
Conc: N.D.

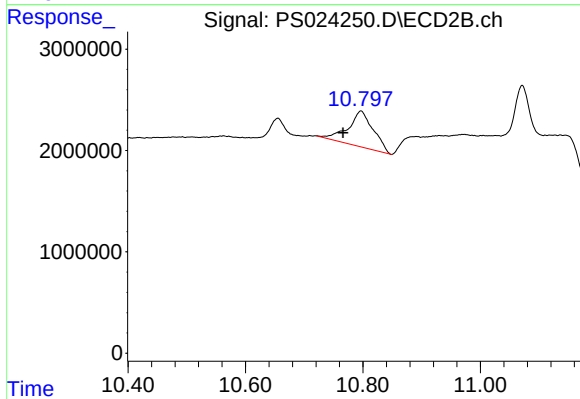

#16 DCPA

R.T.: 10.797 min
Delta R.T.: 0.030 min
Response: 10495561
Conc: 2.05 ng/ml