

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090722\
 Data File : PS020469.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Sep 2022 09:40
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 07:49:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090222.M
 Quant Title : 8080.M
 QLast Update : Sat Sep 03 01:06:55 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.180	6.759	1328.4E6	436.7E6	376.898	410.592
Target Compounds							
2) T	3,5-DICHL...	6.446f	0.000	162.3E6	0	34.035	N.D. #
3) T	4-Nitroph...	6.969f	0.000	650674	0	<MDL	N.D. #
5) T	DICAMBA	0.000	6.983f	0	49800371	N.D.	10.406
6) T	MCP	0.000	6.983	0	49800371	N.D.	13.548
7) T	MCPA	7.640f	0.000	1194000	0	<MDL	N.D. #
9) T	2,4-D	8.224f	0.000	45034	0	<MDL	N.D. #
10) T	Pentachlo...	8.597	0.000	141921	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.158	0.000	3702026	0	<MDL	N.D. #
12) T	2,4,5-T	9.426	0.000	34026891	0	1.467	N.D. #
15) T	Picloram	10.940	10.854f	362.3E6	49553450	8.750	4.825 #
16) T	DCPA	11.399	10.746	15471382	2273849	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090722\
Data File : PS020469.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Sep 2022 09:40
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 07:49:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090222.M
Quant Title : 8080.M
QLast Update : Sat Sep 03 01:06:55 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

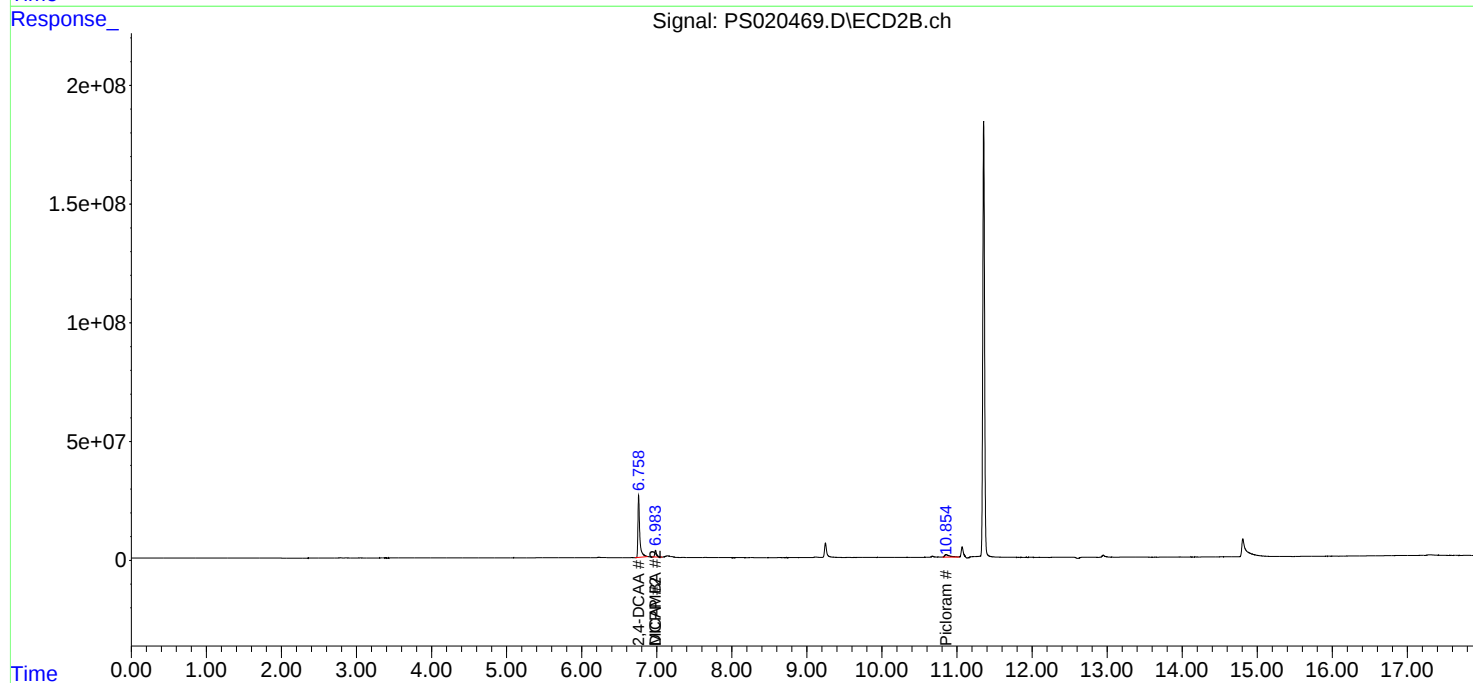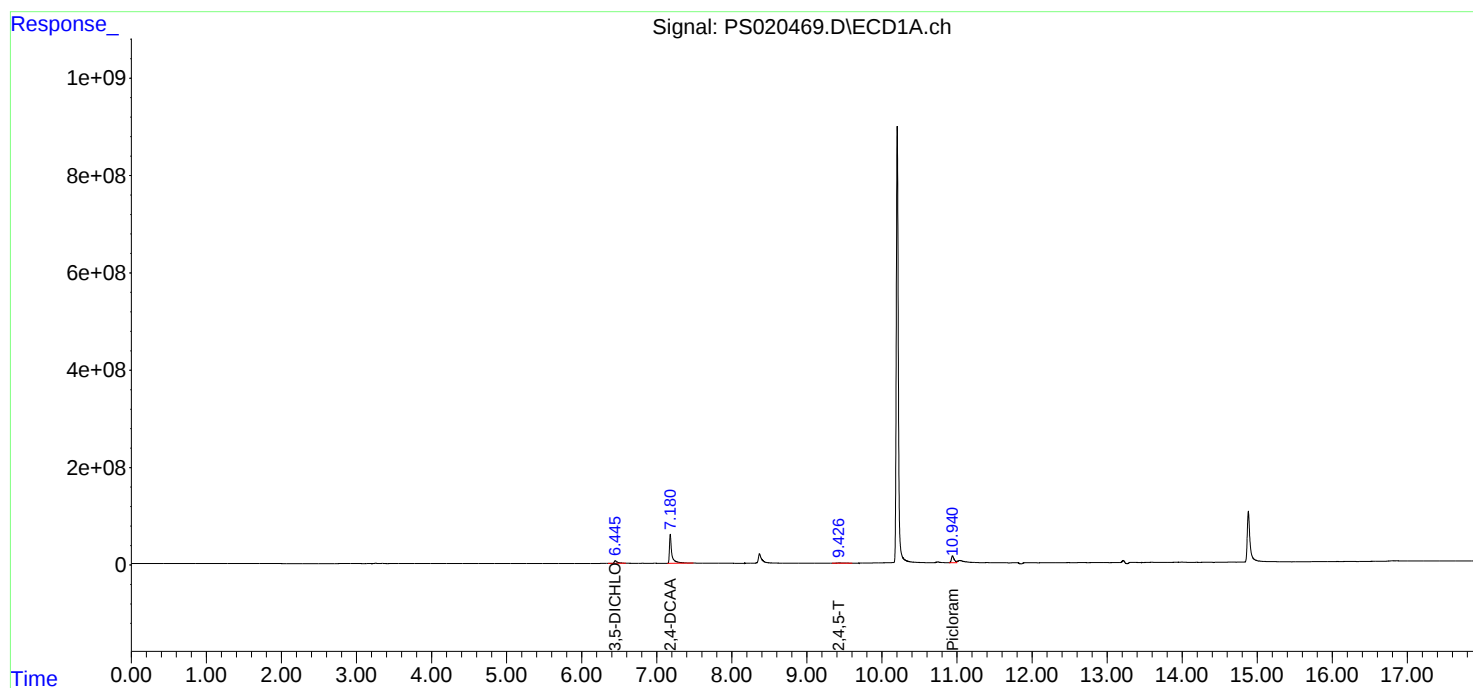


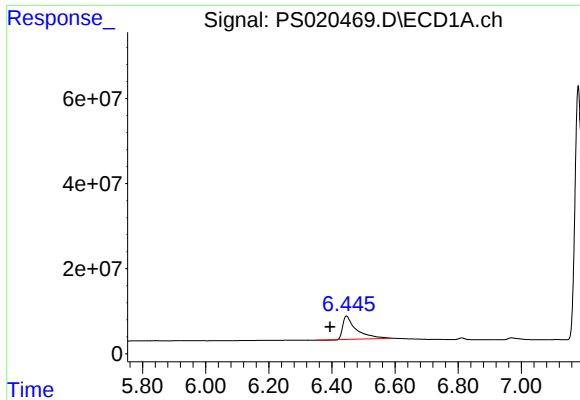

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.446 min
Delta R.T.: 0.052 min
Response: 162295840
Conc: 34.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

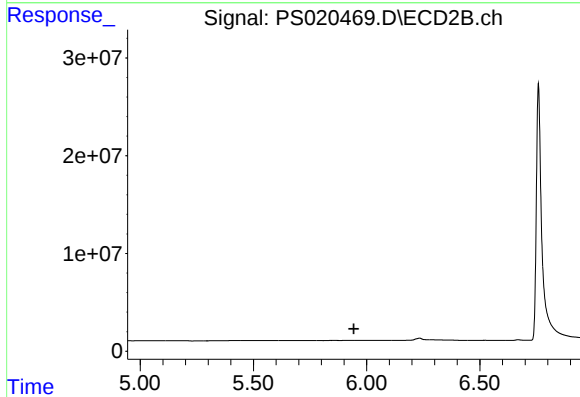


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.944 min
Response: 0
Conc: N.D.

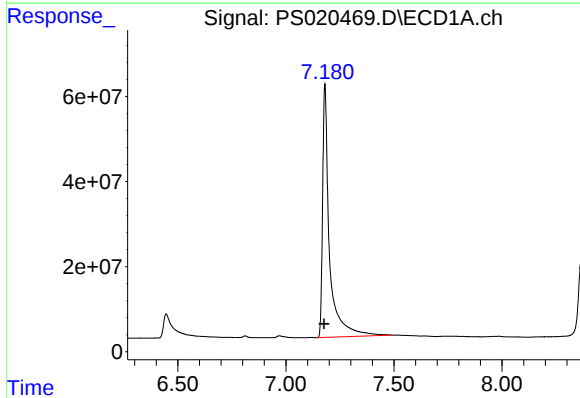


#4 2,4-DCAA

R.T.: 7.180 min
Delta R.T.: 0.004 min
Response: 1328437255
Conc: 376.90 ng/ml

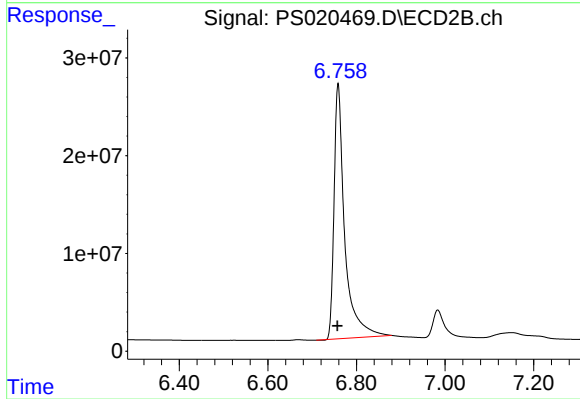

#4 2,4-DCAA


R.T.: 6.759 min
Delta R.T.: 0.001 min
Response: 436742003
Conc: 410.59 ng/ml

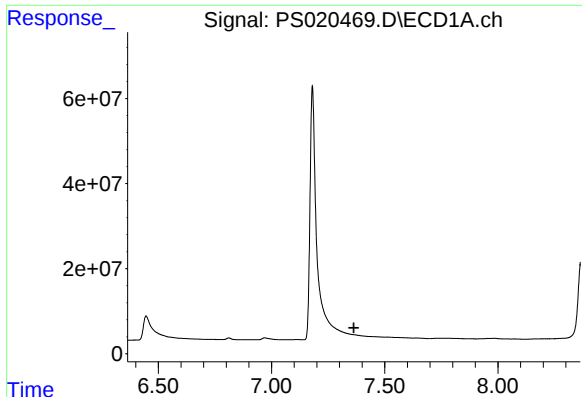

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.364 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

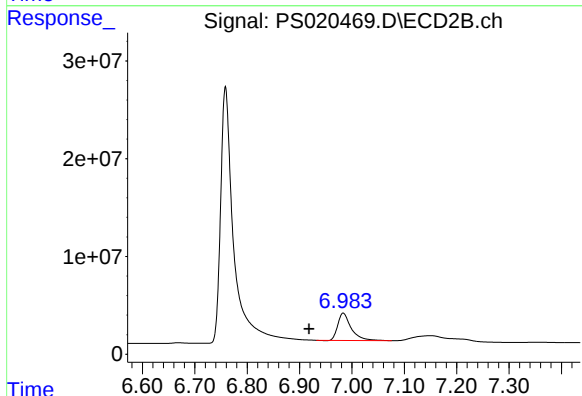


#5 DICAMBA

R.T.: 6.983 min
Delta R.T.: 0.065 min
Response: 49800371
Conc: 10.41 ng/ml

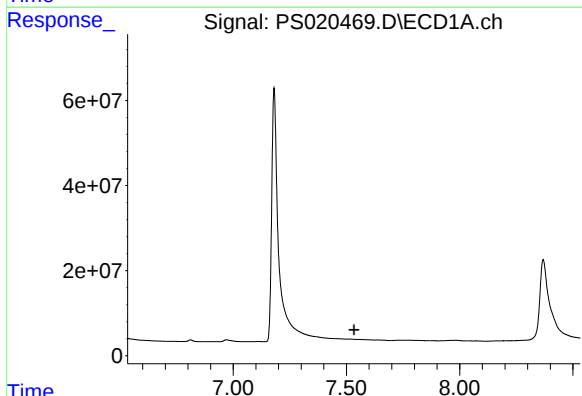


#6 MCP

R.T.: 0.000 min
Exp R.T.: 7.533 min
Response: 0
Conc: N.D.

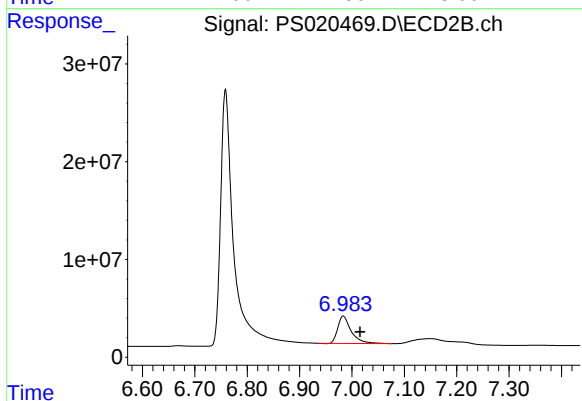

#6 MCP


R.T.: 6.983 min
Delta R.T.: -0.032 min
Response: 49800371
Conc: 13.55 ug/ml

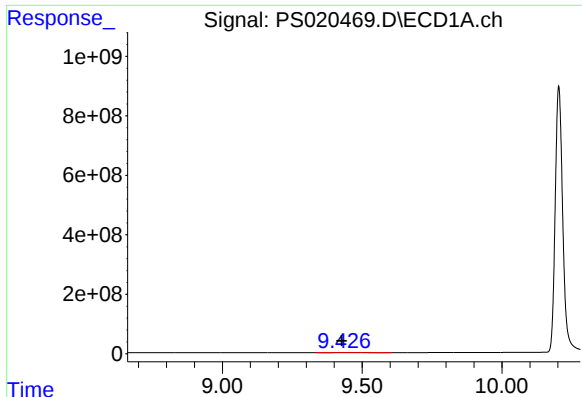

#12 2,4,5-T


R.T.: 9.426 min
Delta R.T.: -0.001 min
Response: 34026891
Conc: 1.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

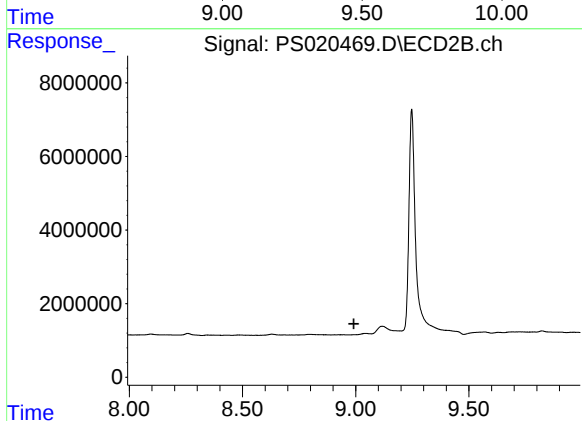


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 8.992 min
Response: 0
Conc: N.D.

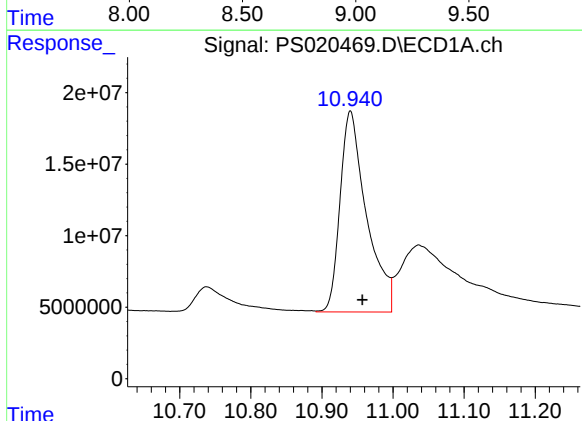

#15 Picloram

R.T.: 10.940 min
Delta R.T.: -0.017 min
Response: 362346892
Conc: 8.75 ng/ml

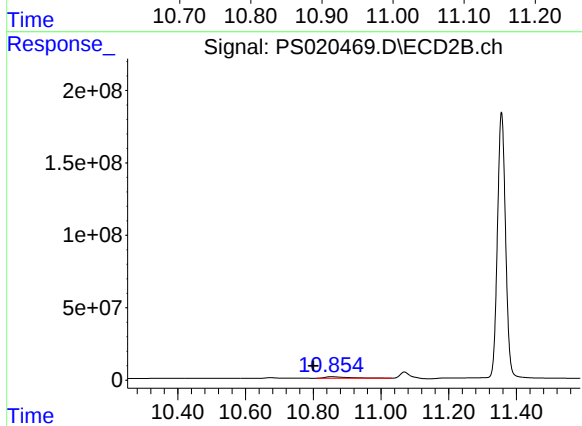

#15 Picloram

R.T.: 10.854 min
Delta R.T.: 0.054 min
Response: 49553450
Conc: 4.83 ng/ml