

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090722\
 Data File : PS020481.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Sep 2022 18:20
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 07:53:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090222.M
 Quant Title : 8080.M
 QLast Update : Sat Sep 03 01:06:55 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.178	6.758	1281.7E6	461.0E6	363.646	433.386
Target Compounds							
2) T	3,5-DICHL...	6.437f	0.000	306.9E6	0	64.365	N.D. #
3) T	4-Nitroph...	6.967f	0.000	1920600	0	1.243	N.D. #
5) T	DICAMBA	0.000	6.979f	0	89825097	N.D.	18.769
6) T	MCP	7.509	6.979	2159049	89825097	<MDL	24.437 #
7) T	MCPA	7.690	0.000	25487495	0	1.655	N.D. #
8) T	DICHLORPROP	0.000	7.607f	0	7290570	N.D.	5.834
11) T	2,4,5-TP ...	9.158	8.586	2048954	524572	<MDL	<MDL #
12) T	2,4,5-T	9.405	9.022	16002829	2318605	<MDL	<MDL #
13) T	2,4-DB	0.000	9.536	0	2813685	N.D.	3.107
14) T	DINOSEB	11.175f	0.000	28086399	0	1.219	N.D. #
15) T	Picloram	10.931	10.847f	413.2E6	9288821	9.979	<MDL #
16) T	DCPA	11.405	10.746	9613365	2615810	<MDL	<MDL #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090722\
Data File : PS020481.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Sep 2022 18:20
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 07:53:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090222.M
Quant Title : 8080.M
QLast Update : Sat Sep 03 01:06:55 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

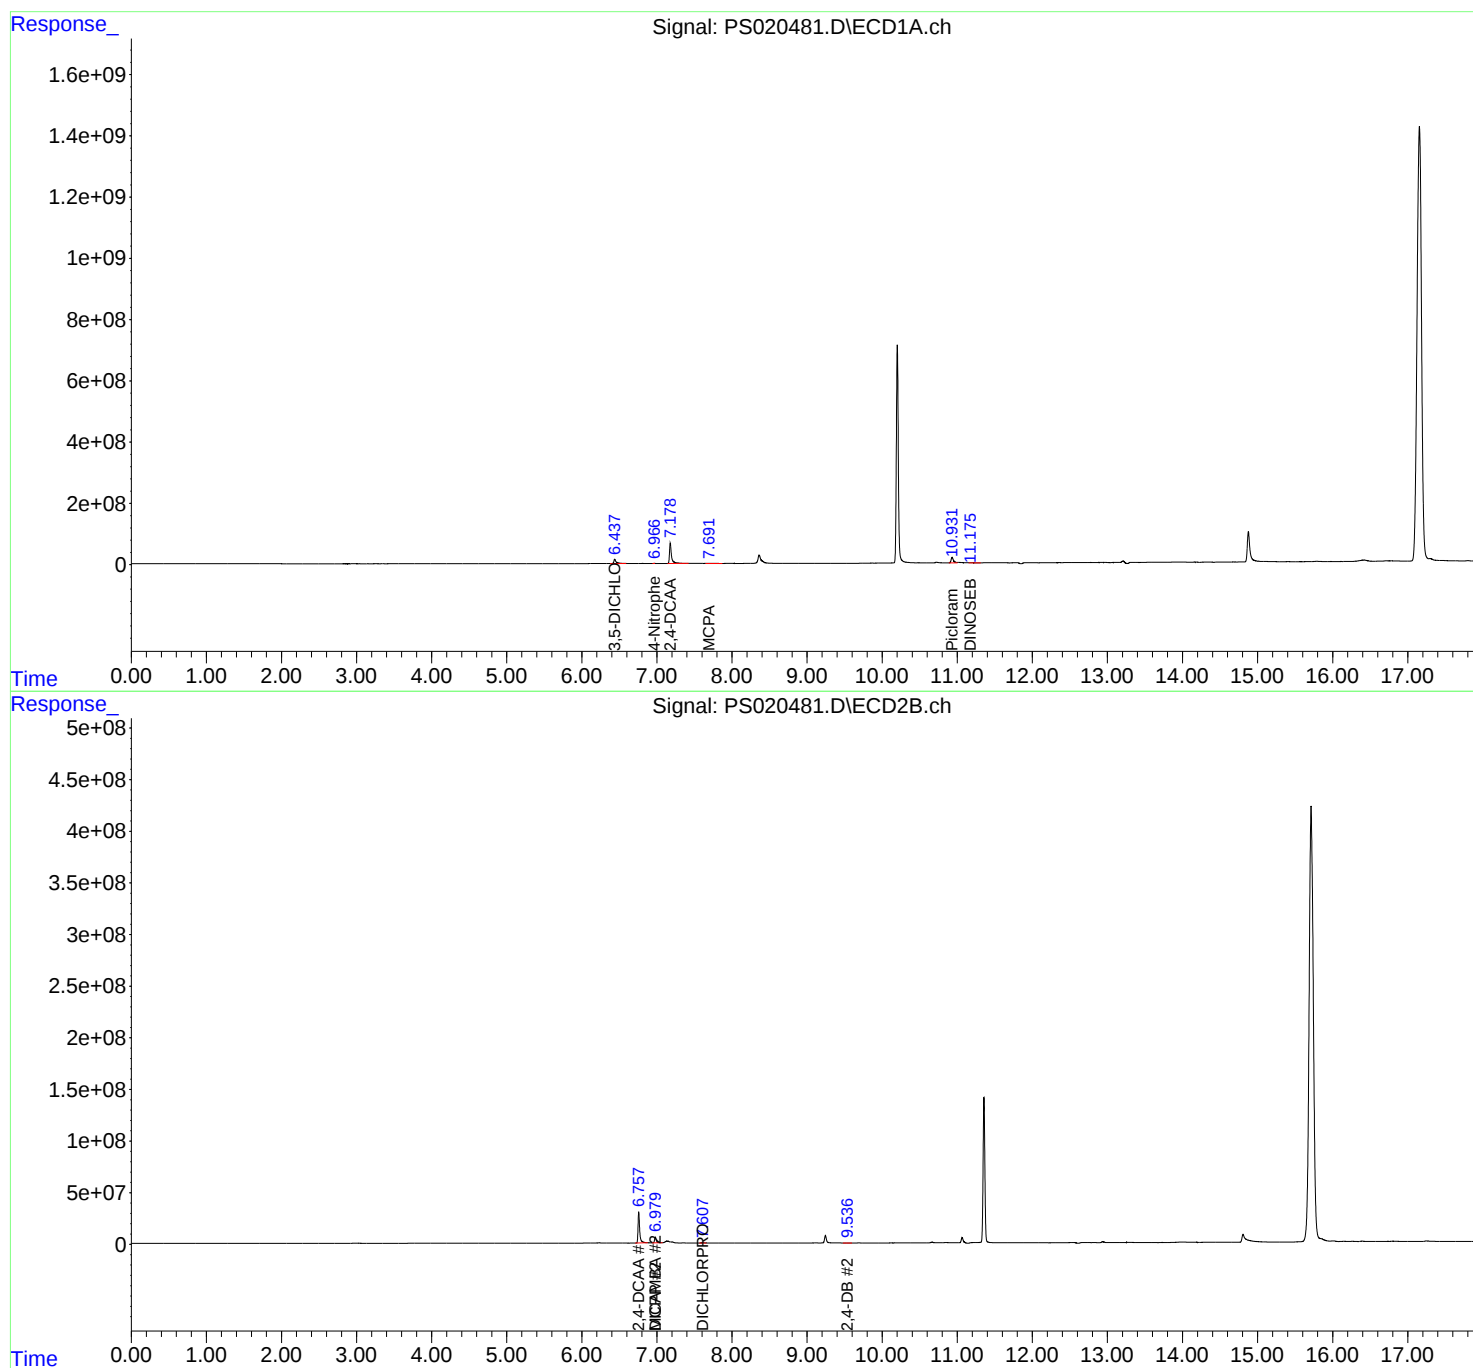


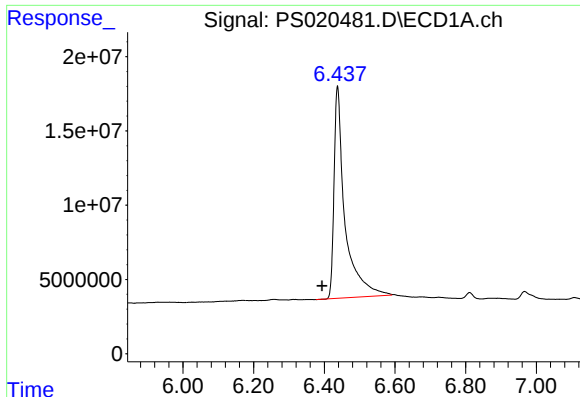

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.437 min
Delta R.T.: 0.043 min
Response: 306917880
Conc: 64.36 ng/ml

Instrument :
ECD_S
ClientSampleId :

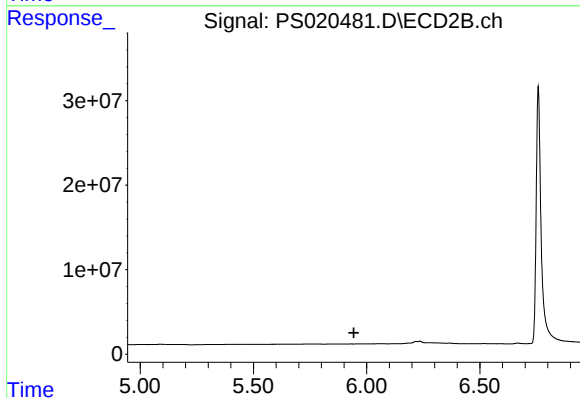


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.944 min
Response: 0
Conc: N.D.

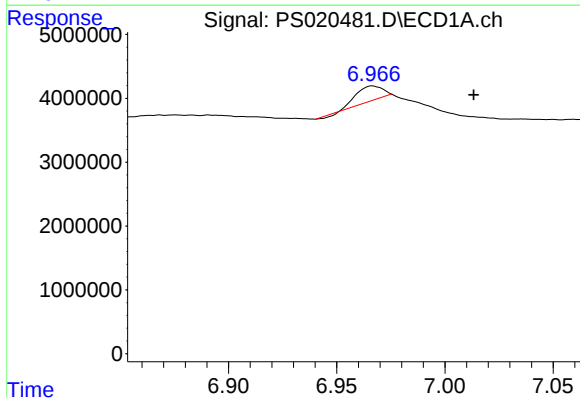


#3 4-Nitrophenol

R.T.: 6.967 min
Delta R.T.: -0.047 min
Response: 1920600
Conc: 1.24 ng/ml

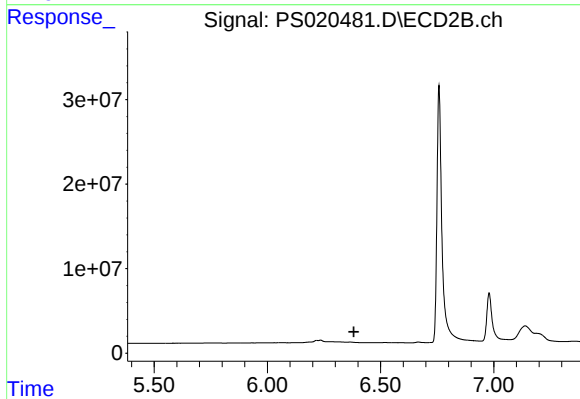

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.382 min
Response: 0
Conc: N.D.

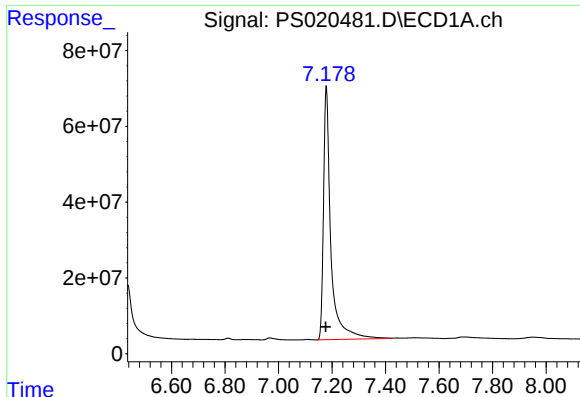

#4 2,4-DCAA


R.T.: 7.178 min
Delta R.T.: 0.002 min
Response: 1281728297
Conc: 363.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

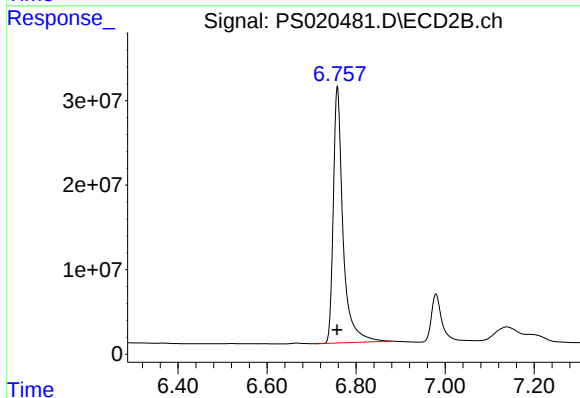


#4 2,4-DCAA

R.T.: 6.758 min
Delta R.T.: 0.000 min
Response: 460988158
Conc: 433.39 ng/ml

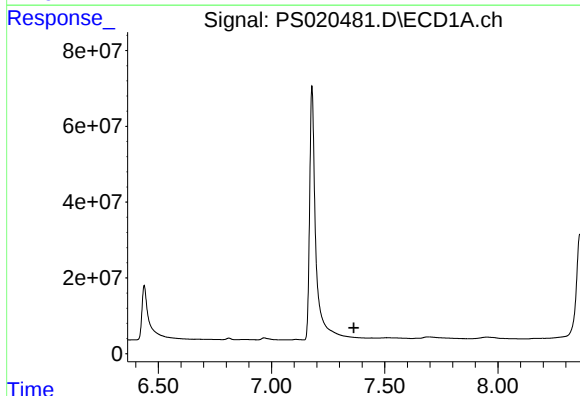


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.364 min
Response: 0
Conc: N.D.

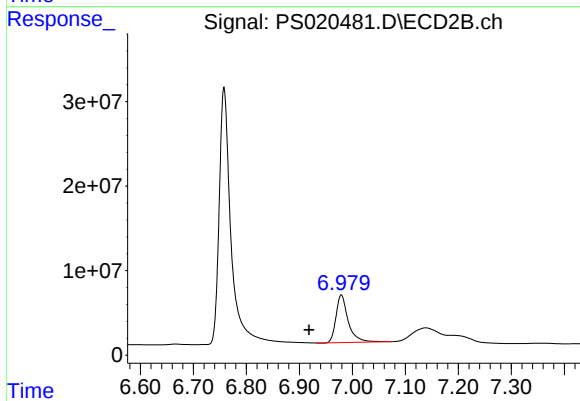

#5 DICAMBA


R.T.: 6.979 min
Delta R.T.: 0.061 min
Response: 89825097
Conc: 18.77 ng/ml

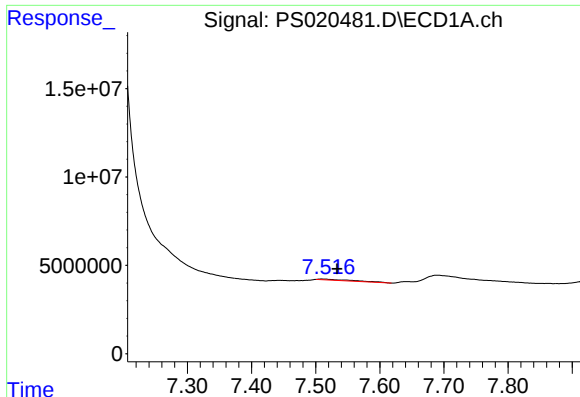

#6 MCPP


R.T.: 7.509 min
Delta R.T.: -0.024 min
Response: 2159049
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

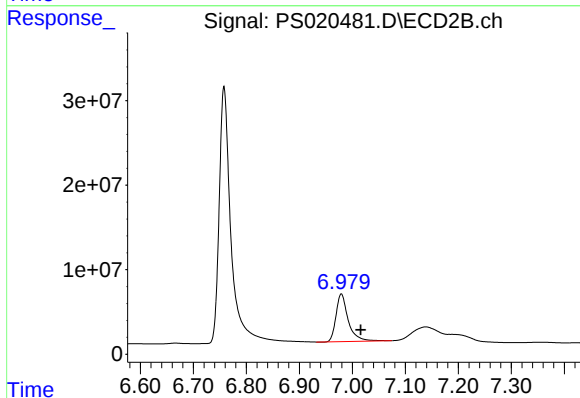


#6 MCPP

R.T.: 6.979 min
Delta R.T.: -0.036 min
Response: 89825097
Conc: 24.44 ug/ml

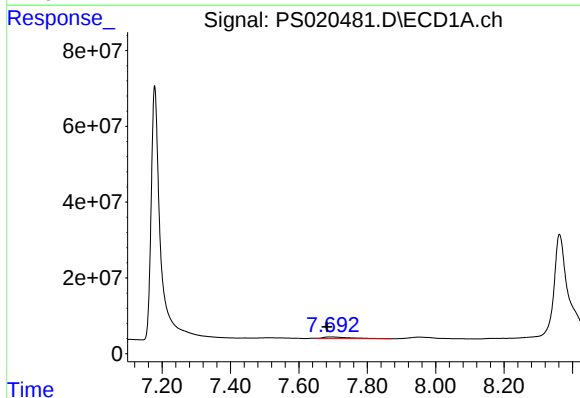


#7 MCPA

R.T.: 7.690 min
Delta R.T.: 0.008 min
Response: 25487495
Conc: 1.65 ug/ml

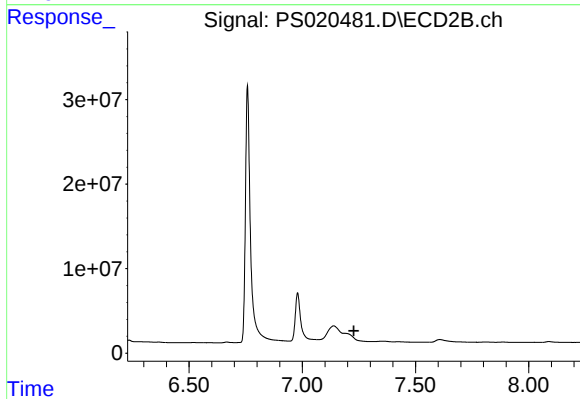

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.228 min
Response: 0
Conc: N.D.

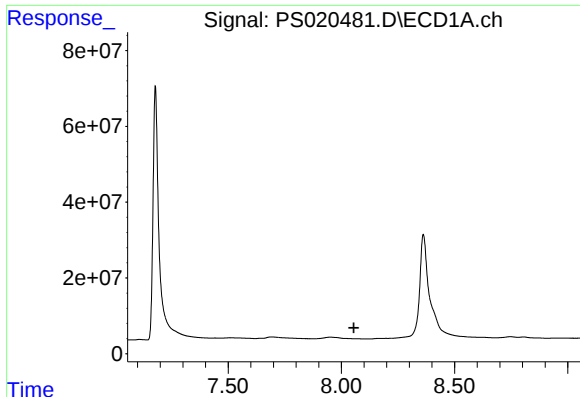

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.056 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

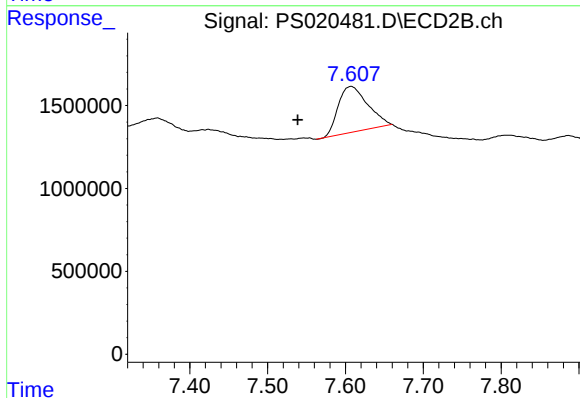


#8 DICHLORPROP

R.T.: 7.607 min
Delta R.T.: 0.069 min
Response: 7290570
Conc: 5.83 ng/ml

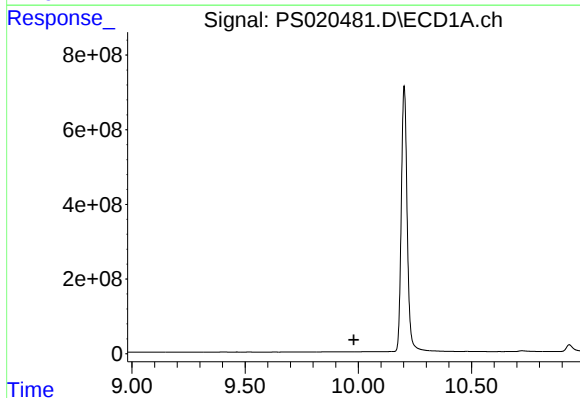


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 9.980 min
Response: 0
Conc: N.D.

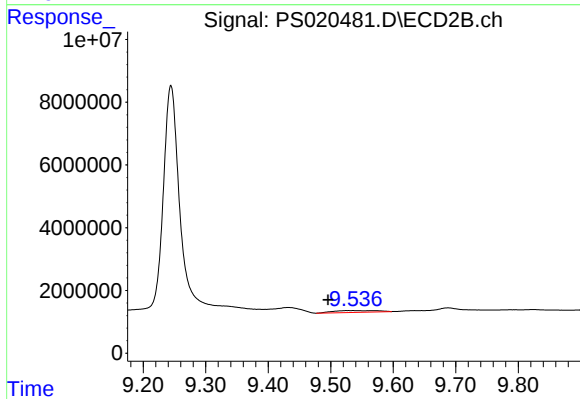

#13 2,4-DB


R.T.: 9.536 min
Delta R.T.: 0.040 min
Response: 2813685
Conc: 3.11 ng/ml

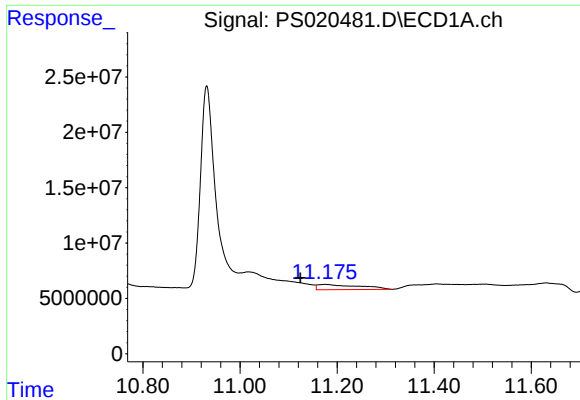

#14 DINOSEB


R.T.: 11.175 min
Delta R.T.: 0.050 min
Response: 28086399
Conc: 1.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

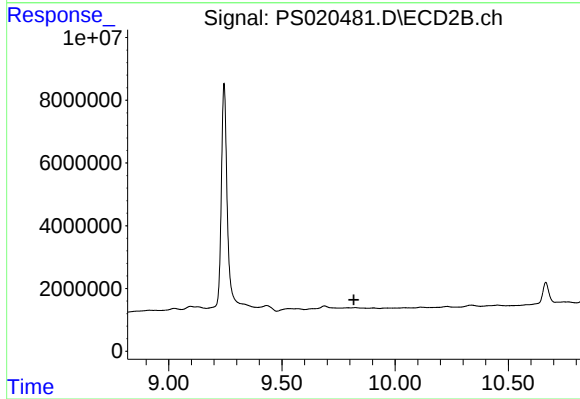


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.818 min
Response: 0
Conc: N.D.

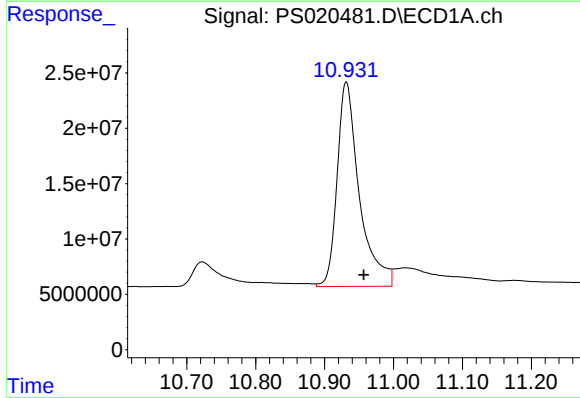

#15 Picloram

R.T.: 10.931 min
Delta R.T.: -0.025 min
Response: 413228201
Conc: 9.98 ng/ml

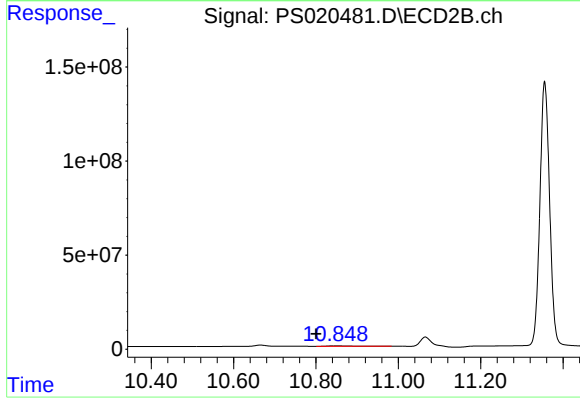

#15 Picloram

R.T.: 10.847 min
Delta R.T.: 0.047 min
Response: 9288821
Conc: N.D.