

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090723\
 Data File : PS024261.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Sep 2023 11:53
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 03:27:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082823.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 28 16:48:10 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.333	6.738f	31972950	776962	16.048	1.157 #
Target Compounds							
1) T	Dalapon	2.513	2.570	7467119	3155774	3.436	2.993
3) T	4-Nitroph...	6.201	6.363f	6867143	255259	5.527	<MDL #
5) T	DICAMBA	6.506	6.996f	367205	1514.5E6	<MDL	525.846 #
6) T	MCP	6.683	6.996f	10980340	1514.5E6	1.763	790.598 #
7) T	MCPA	6.791	0.000	1339570	0	<MDL	N.D. #
8) T	DICHLORPROP	7.089	7.577	23337466	5430481	10.266	7.474 #
9) T	2,4-D	7.257	7.888	10904.3E6	260279	4099.524	<MDL #
10) T	Pentachlo...	7.522	8.270	2410525	1212521	<MDL	<MDL #
11) T	2,4,5-TP ...	8.053	8.630	9338777	1789087	<MDL	<MDL #
12) T	2,4,5-T	8.305	9.012	3191248	280777	<MDL	<MDL #
13) T	2,4-DB	0.000	9.502	0	577676	N.D.	1.257
14) T	DINOSEB	9.863	9.875	1985678	181255	<MDL	<MDL #
15) T	Picloram	9.665	10.793	429.1E6	67198974	26.277	11.315 #
16) T	DCPA	10.106	10.793	2682170	67198974	<MDL	13.099 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090723\
Data File : PS024261.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Sep 2023 11:53
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 03:27:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082823.M
Quant Title : 8080.M
QLast Update : Mon Aug 28 16:48:10 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

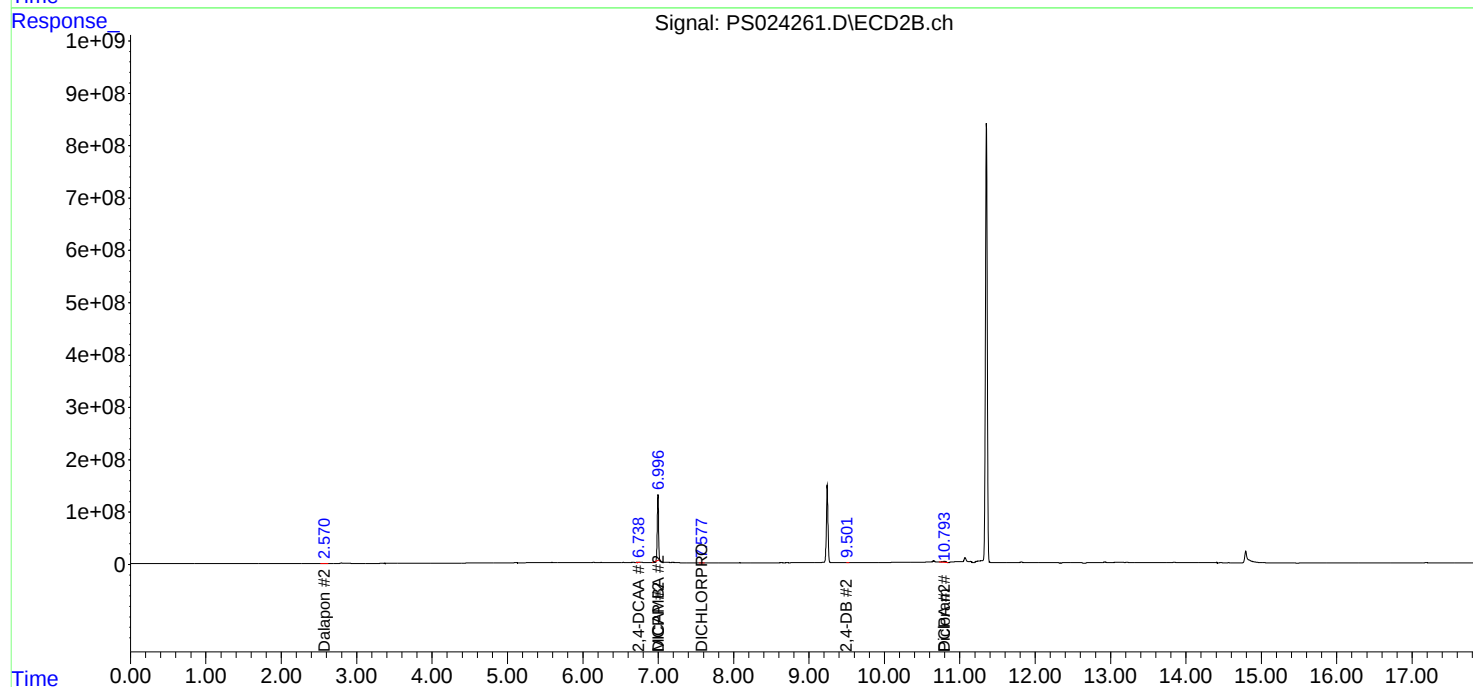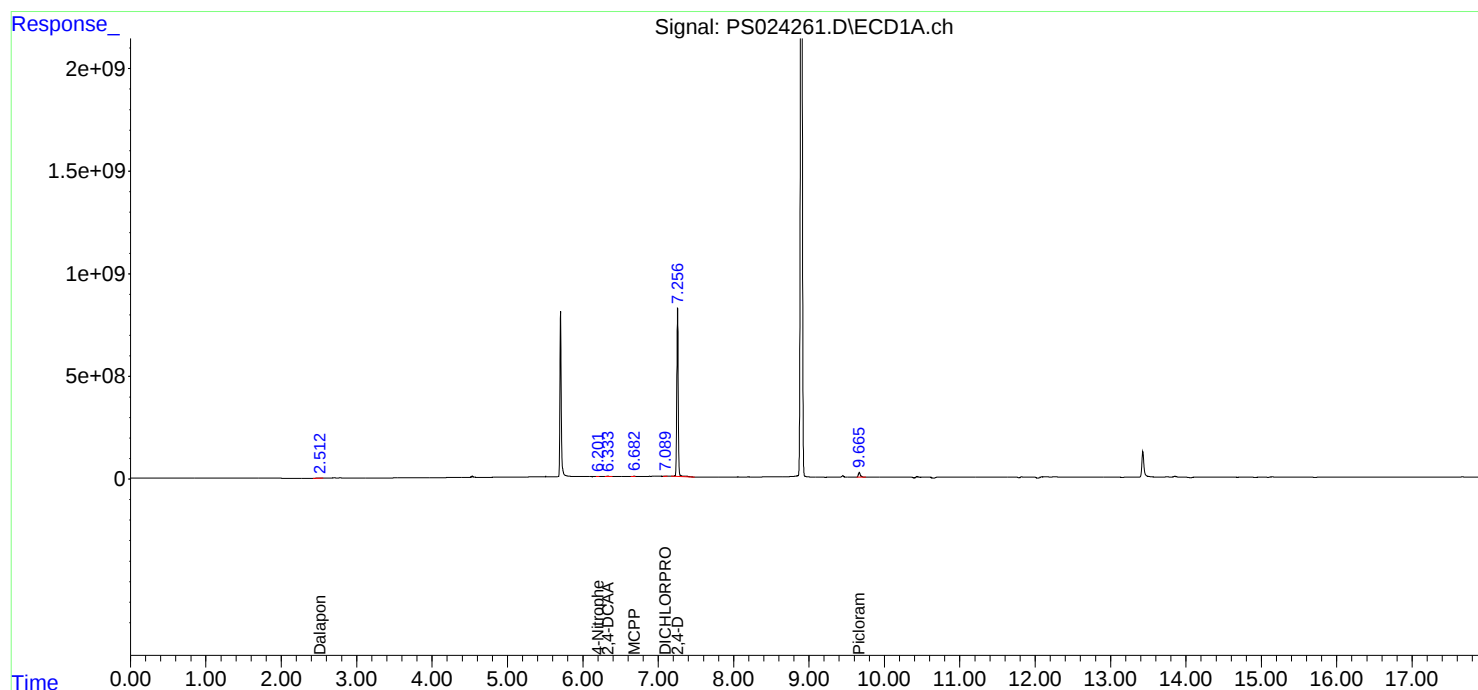


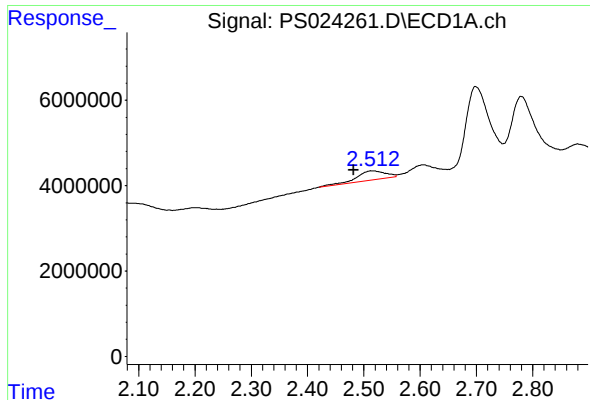

#1 Dalapon


R.T.: 2.513 min
Delta R.T.: 0.031 min
Response: 7467119
Conc: 3.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

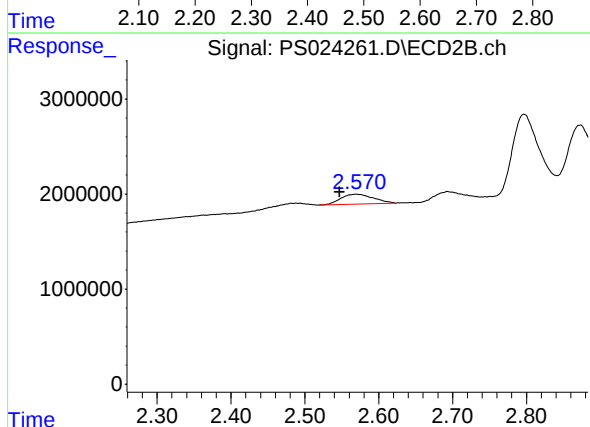


#1 Dalapon

R.T.: 2.570 min
Delta R.T.: 0.024 min
Response: 3155774
Conc: 2.99 ng/ml

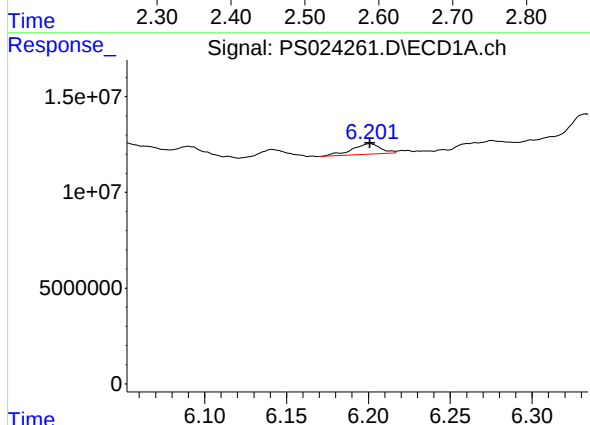


#3 4-Nitrophenol

R.T.: 6.201 min
Delta R.T.: 0.000 min
Response: 6867143
Conc: 5.53 ng/ml

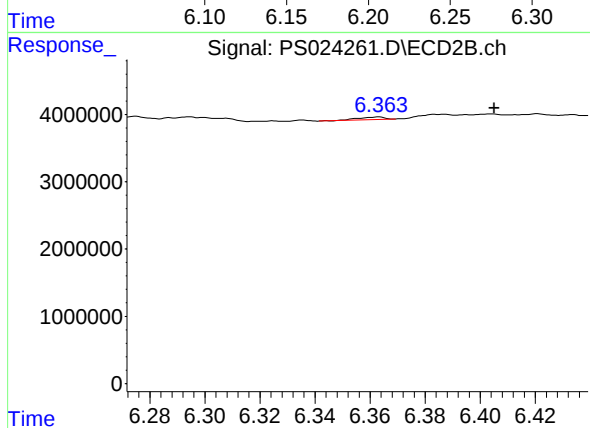

#3 4-Nitrophenol


R.T.: 6.363 min
Delta R.T.: -0.042 min
Response: 255259
Conc: N.D.

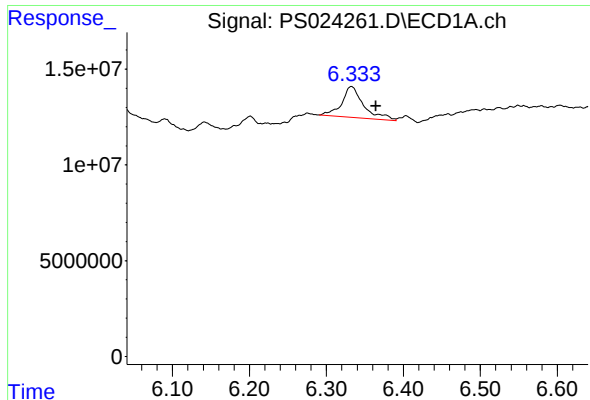

#4 2,4-DCAA


R.T.: 6.333 min
Delta R.T.: -0.032 min
Response: 31972950
Conc: 16.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

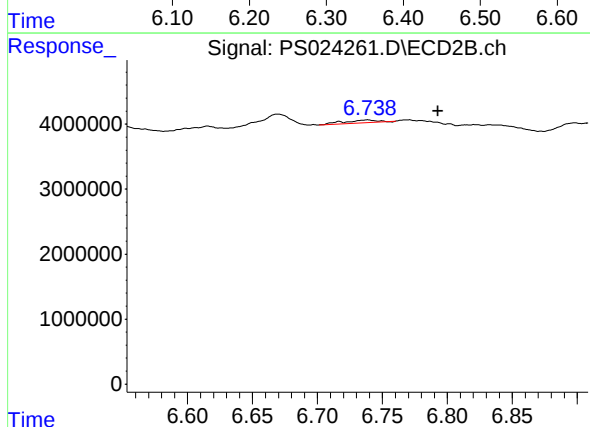


#4 2,4-DCAA

R.T.: 6.738 min
Delta R.T.: -0.054 min
Response: 776962
Conc: 1.16 ng/ml

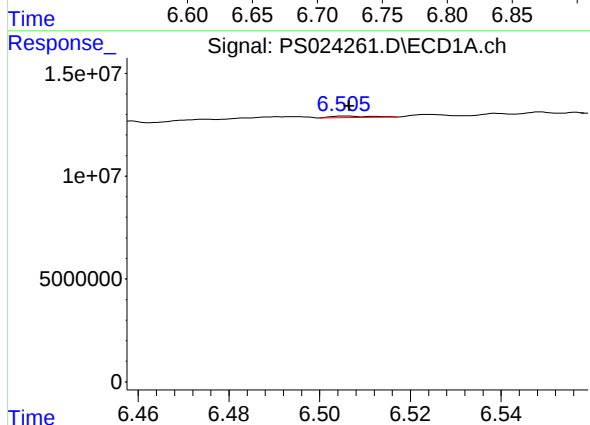


#5 DICAMBA

R.T.: 6.506 min
Delta R.T.: 0.000 min
Response: 367205
Conc: N.D.

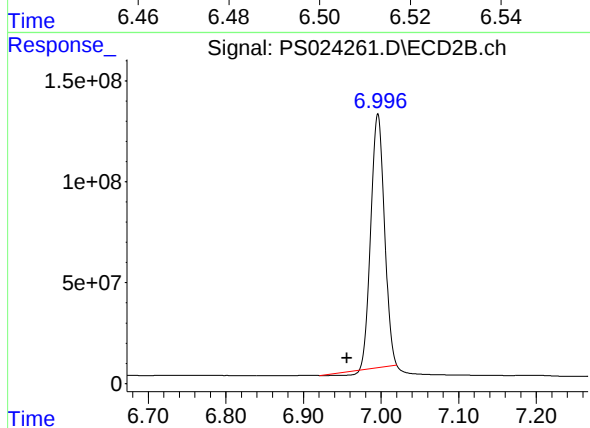

#5 DICAMBA


R.T.: 6.996 min
Delta R.T.: 0.040 min
Response: 1514519429
Conc: 525.85 ng/ml

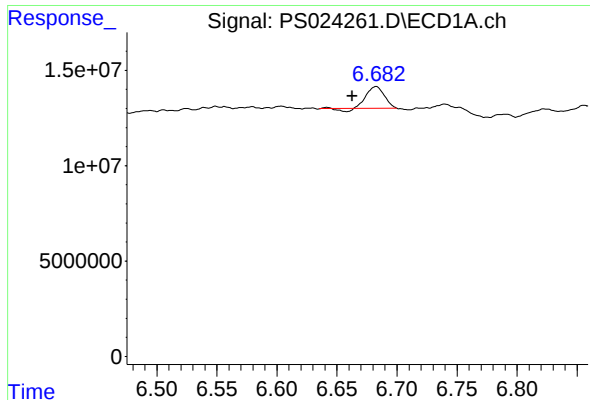

#6 MCPP


R.T.: 6.683 min
Delta R.T.: 0.020 min
Response: 10980340
Conc: 1.76 ug/ml

Instrument :
ECD_S
ClientSampleId :

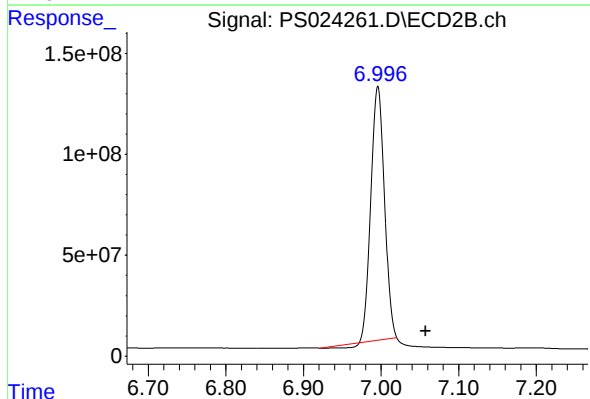


#6 MCPP

R.T.: 6.996 min
Delta R.T.: -0.061 min
Response: 1514519429
Conc: 790.60 ug/ml

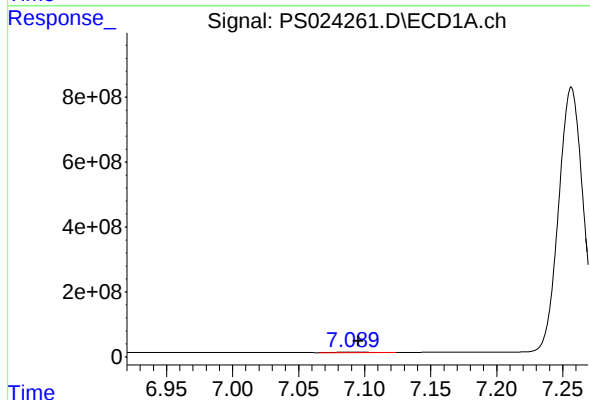


#8 DICHLORPROP

R.T.: 7.089 min
Delta R.T.: -0.007 min
Response: 23337466
Conc: 10.27 ng/ml

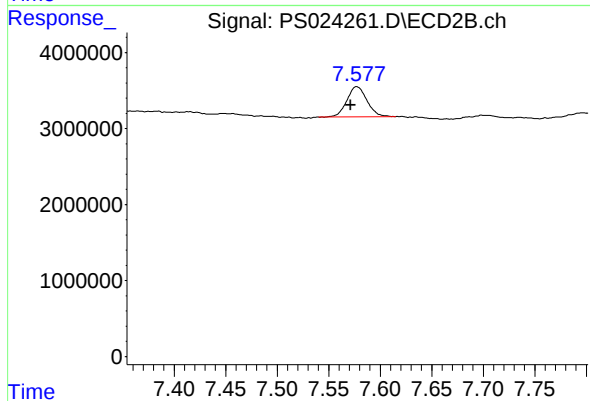

#8 DICHLORPROP

R.T.: 7.577 min
Delta R.T.: 0.006 min
Response: 5430481
Conc: 7.47 ng/ml

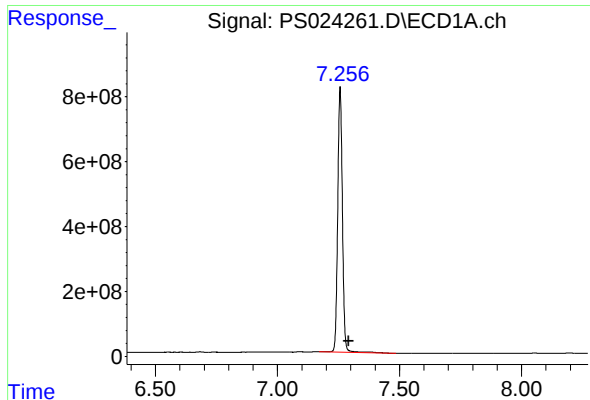


#9 2,4-D

R.T.: 7.257 min
Delta R.T.: -0.035 min
Response: 10904253991
Conc: 4099.52 ng/ml

Instrument :


ECD_S

ClientSampleId :

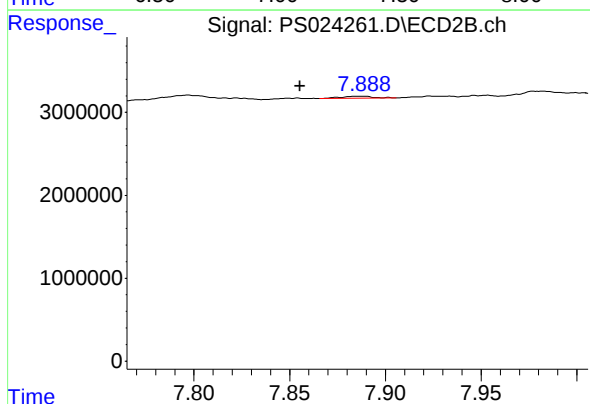


#9 2,4-D

R.T.: 7.888 min
Delta R.T.: 0.033 min
Response: 260279
Conc: N.D.

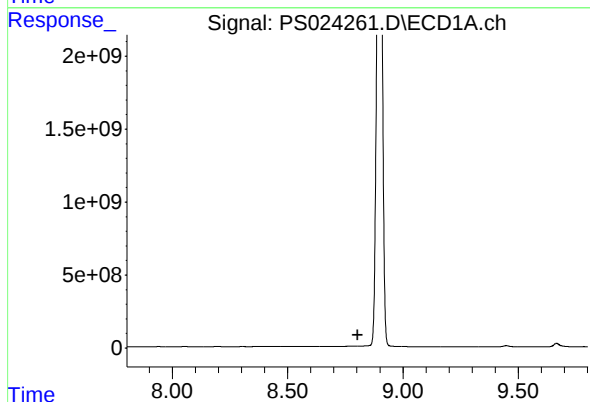


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 8.803 min
Response: 0
Conc: N.D.

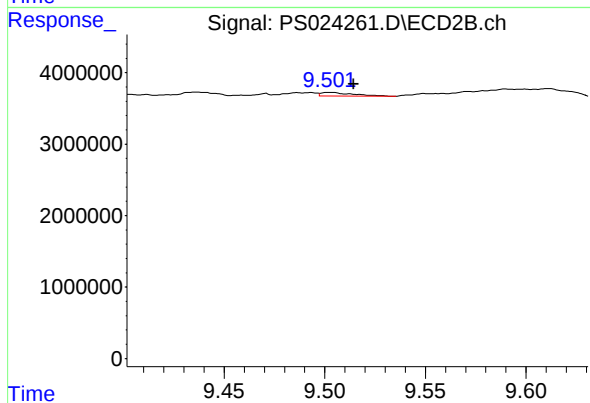

#13 2,4-DB


R.T.: 9.502 min
Delta R.T.: -0.012 min
Response: 577676
Conc: 1.26 ng/ml

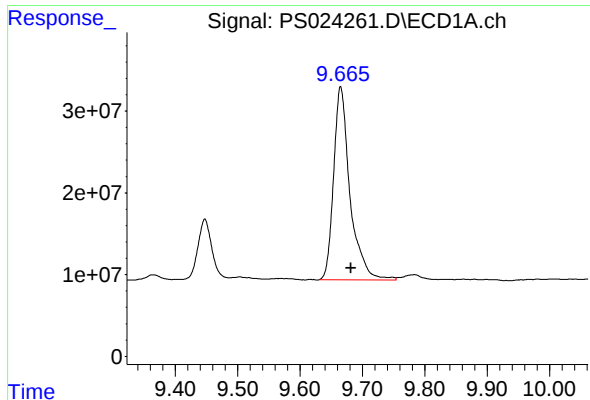

#15 Picloram


R.T.: 9.665 min
Delta R.T.: -0.017 min
Response: 429138473
Conc: 26.28 ng/ml

Instrument :
ECD_S
ClientSampleId :

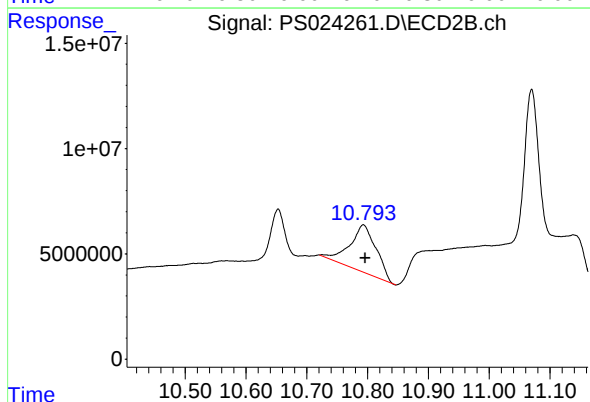


#15 Picloram

R.T.: 10.793 min
Delta R.T.: -0.003 min
Response: 67198974
Conc: 11.32 ng/ml

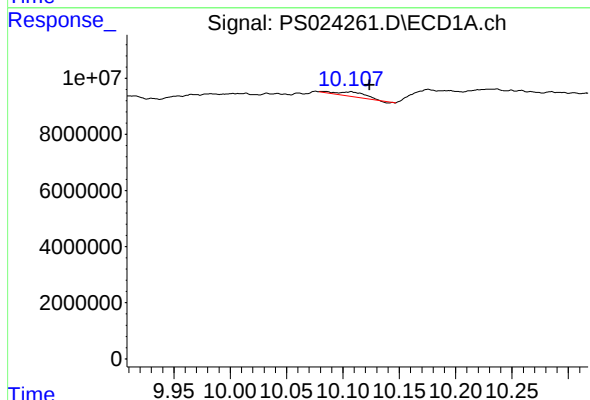

#16 DCPA

R.T.: 10.106 min
Delta R.T.: -0.017 min
Response: 2682170
Conc: N.D.

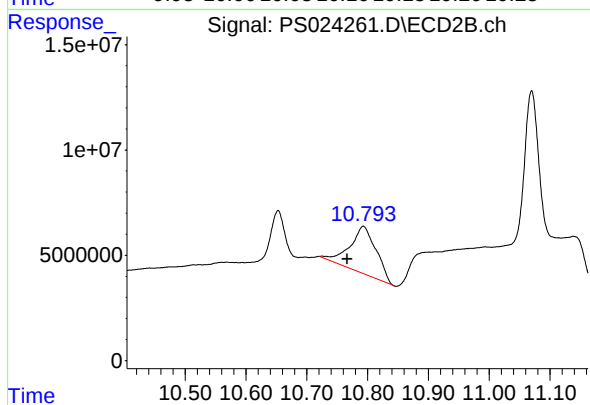

#16 DCPA

R.T.: 10.793 min
Delta R.T.: 0.027 min
Response: 67198974
Conc: 13.10 ng/ml