

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090723\
 Data File : PS024262.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Sep 2023 12:17
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 03:27:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082823.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 28 16:48:10 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.363	6.790	959.6E6	322.0E6	481.649	479.449
Target Compounds							
1) T	Dalapon	2.519	2.576	6020377	1860460	2.770	1.764 #
2) T	3,5-DICHL...	5.702	0.000	10632514	0	3.498	N.D. #
3) T	4-Nitroph...	6.203	6.340f	9412585	402193	7.576	<MDL #
5) T	DICAMBA	6.494	6.946	840642	494943	<MDL	<MDL #
6) T	MCP	6.684	6.996f	2293951	9534964	<MDL	4.977 #
7) T	MCPA	6.814	0.000	57992	0	<MDL	N.D. #
8) T	DICHLORPROP	7.143f	7.580	310117	1264808	<MDL	1.741 #
9) T	2,4-D	7.254	7.796f	72382097	344833	27.213	<MDL #
10) T	Pentachlo...	7.560	0.000	1240917	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.039	8.633	852257	837743	<MDL	<MDL #
12) T	2,4,5-T	8.302	9.050	1243861	3339541	<MDL	<MDL #
14) T	DINOSEB	9.855	0.000	1006445	0	<MDL	N.D. #
15) T	Picloram	9.685	10.794	42783340	18102966	2.620	3.048
16) T	DCPA	10.167f	10.794	671978	18102966	<MDL	3.529 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090723\
Data File : PS024262.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Sep 2023 12:17
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 03:27:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082823.M
Quant Title : 8080.M
QLast Update : Mon Aug 28 16:48:10 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

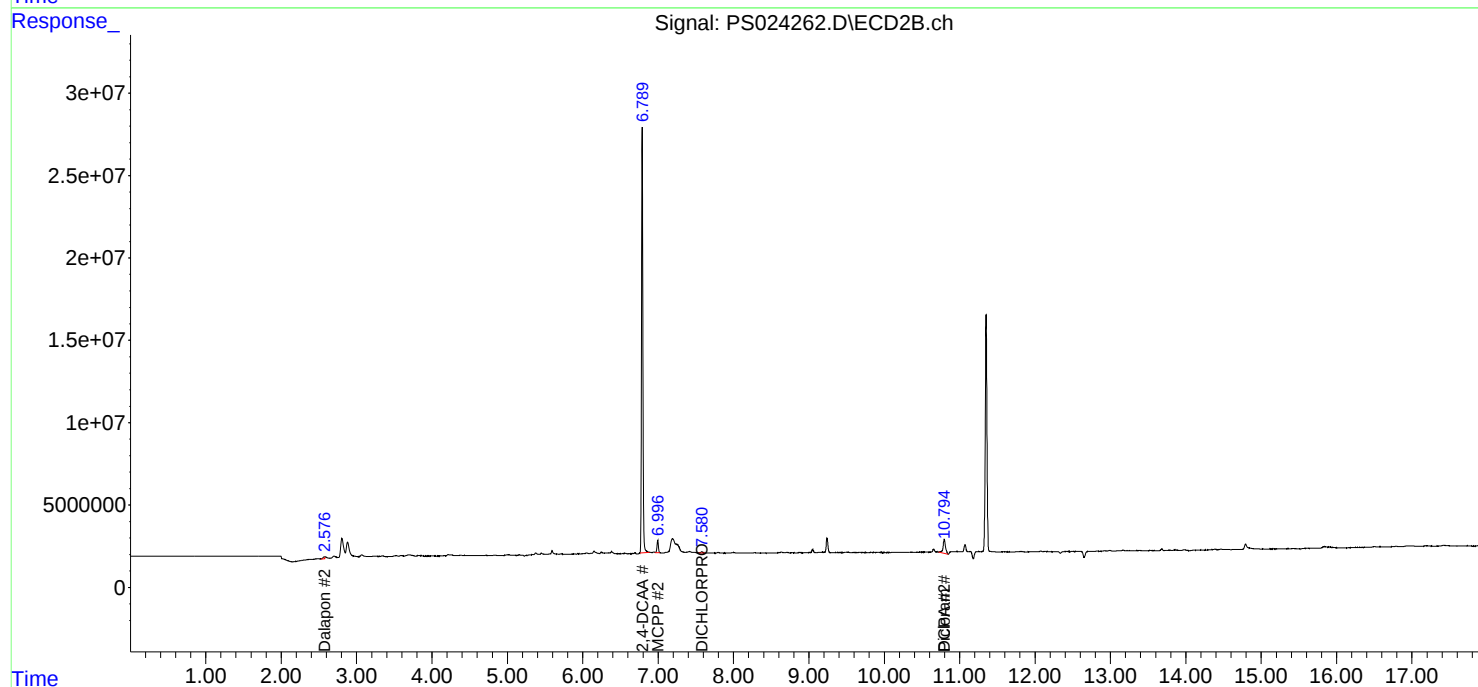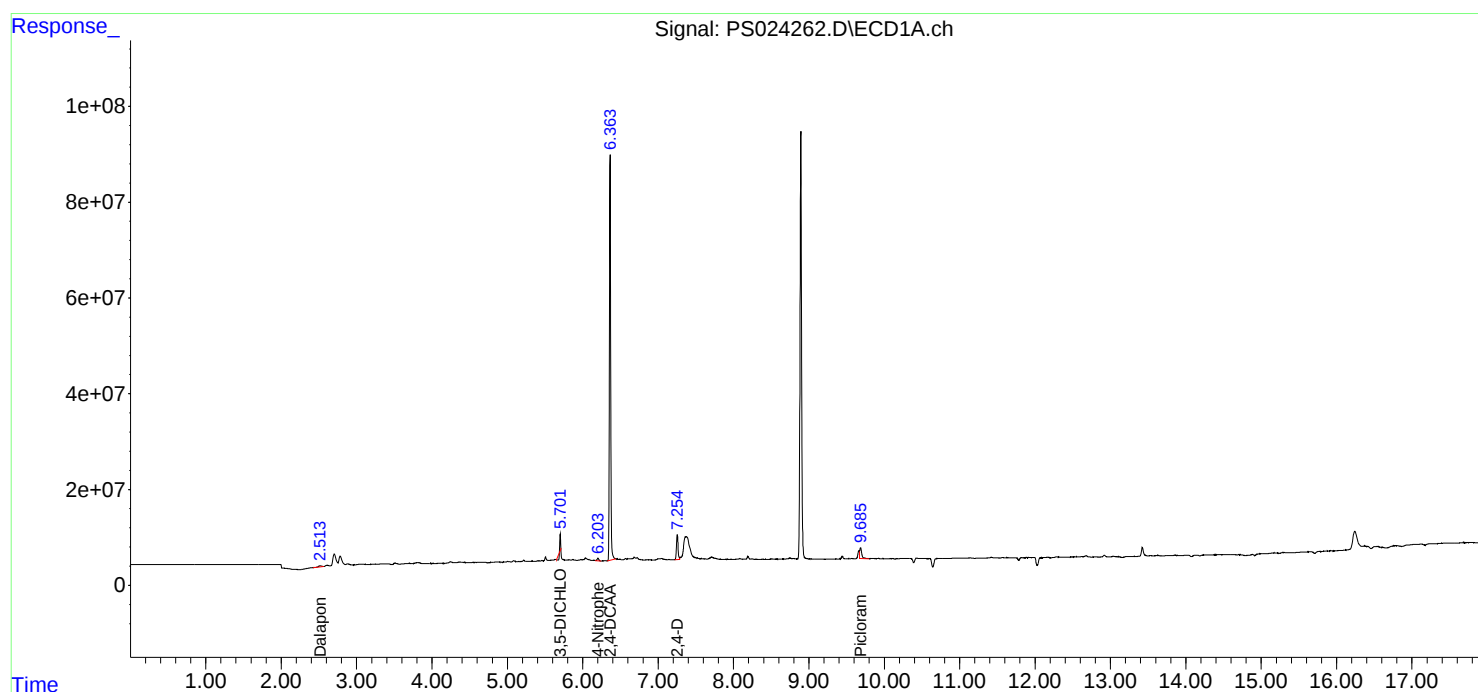


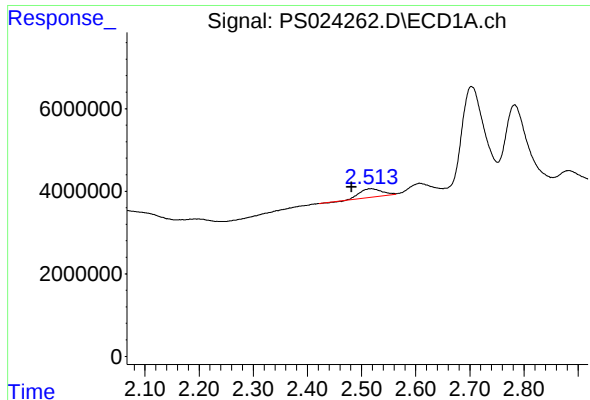

#1 Dalapon


R.T.: 2.519 min
Delta R.T.: 0.037 min
Response: 6020377
Conc: 2.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

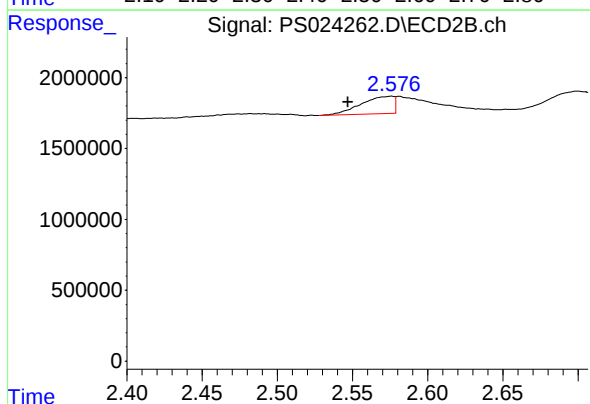


#1 Dalapon

R.T.: 2.576 min
Delta R.T.: 0.029 min
Response: 1860460
Conc: 1.76 ng/ml

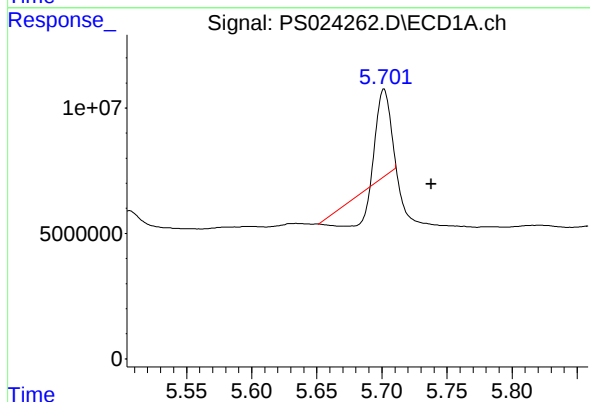


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.702 min
Delta R.T.: -0.036 min
Response: 10632514
Conc: 3.50 ng/ml

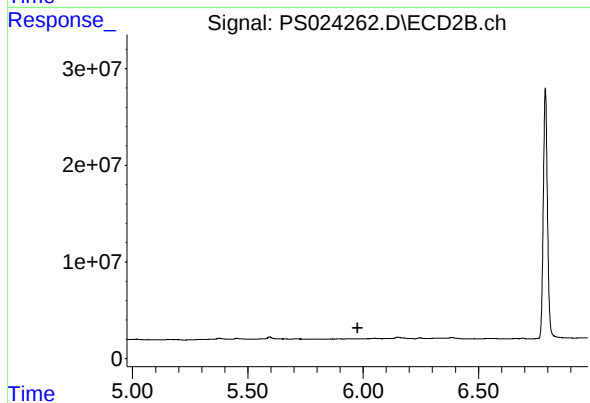

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 5.976 min
Response: 0
Conc: N.D.

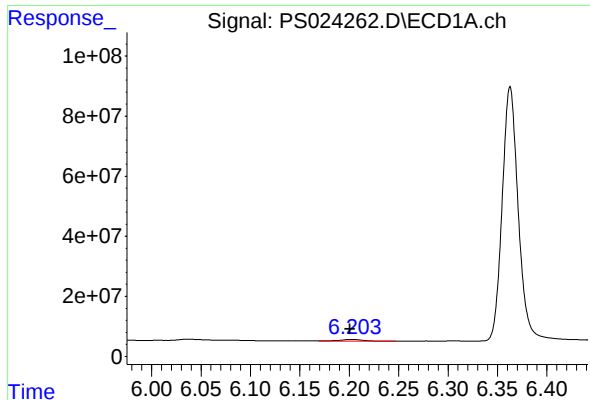

#3 4-Nitrophenol


R.T.: 6.203 min
Delta R.T.: 0.002 min
Response: 9412585
Conc: 7.58 ng/ml

Instrument :
ECD_S
ClientSampleId :

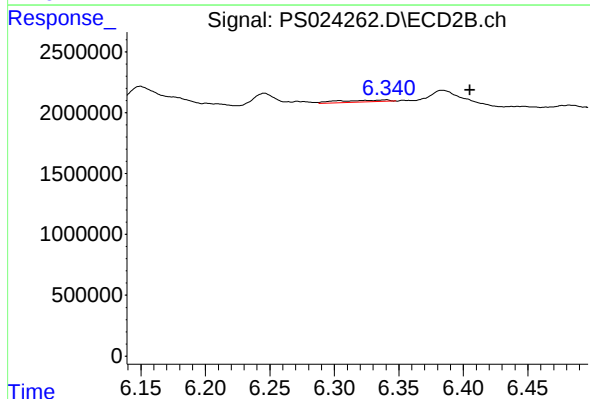


#3 4-Nitrophenol

R.T.: 6.340 min
Delta R.T.: -0.065 min
Response: 402193
Conc: N.D.

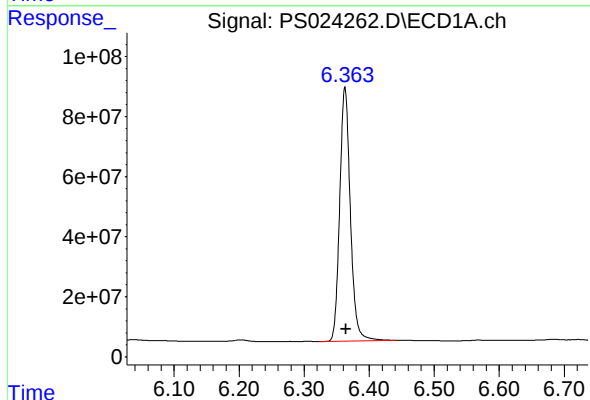


#4 2,4-DCAA

R.T.: 6.363 min
Delta R.T.: -0.002 min
Response: 959599788
Conc: 481.65 ng/ml

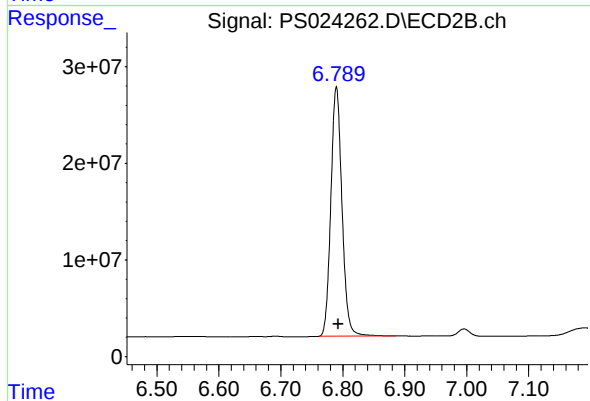

#4 2,4-DCAA


R.T.: 6.790 min
Delta R.T.: -0.003 min
Response: 321994328
Conc: 479.45 ng/ml

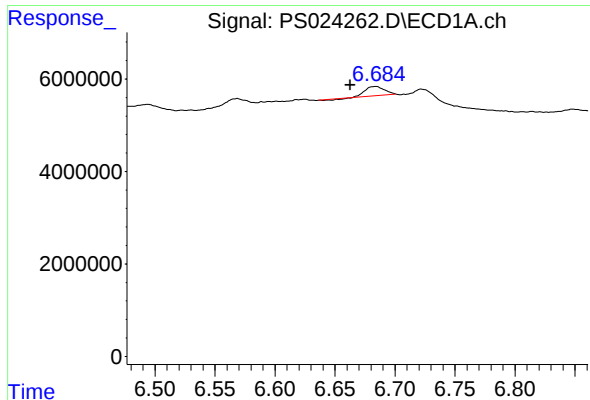

#6 MCPP


R.T.: 6.684 min
Delta R.T.: 0.021 min
Response: 2293951
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

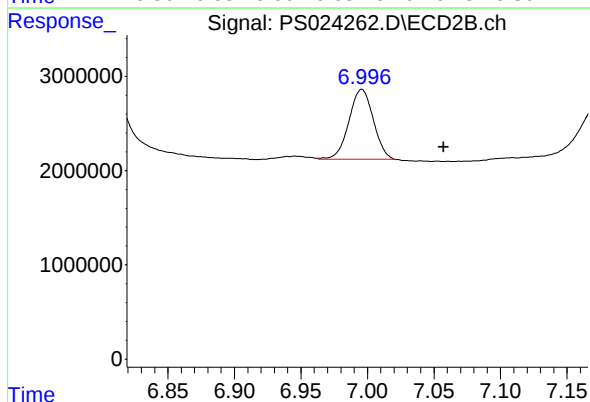


#6 MCPP

R.T.: 6.996 min
Delta R.T.: -0.061 min
Response: 9534964
Conc: 4.98 ug/ml

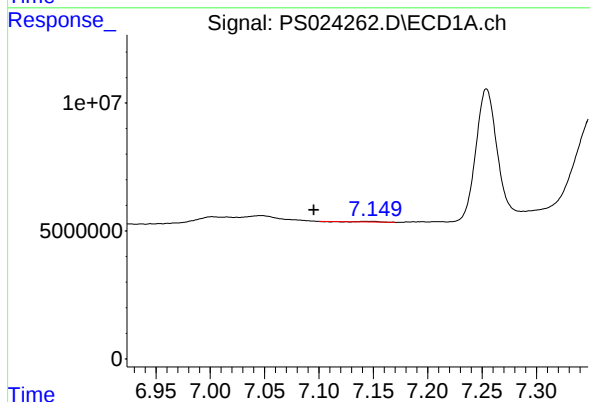


#8 DICHLORPROP

R.T.: 7.143 min
Delta R.T.: 0.047 min
Response: 310117
Conc: N.D.

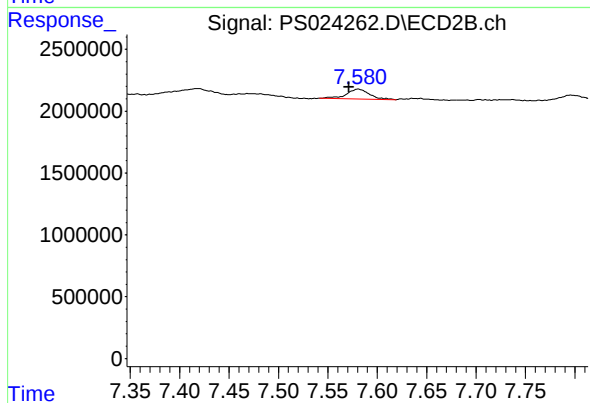

#8 DICHLORPROP


R.T.: 7.580 min
Delta R.T.: 0.009 min
Response: 1264808
Conc: 1.74 ng/ml

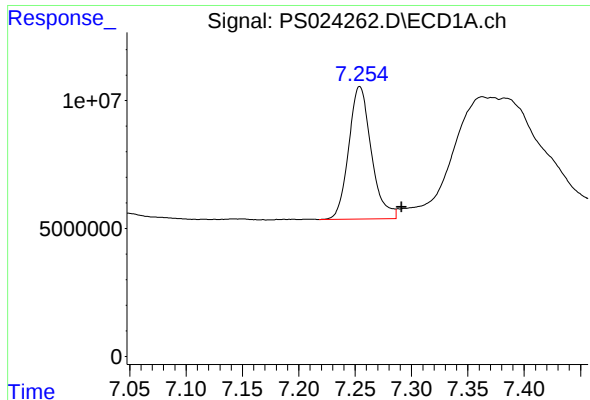

#9 2,4-D


R.T.: 7.254 min
Delta R.T.: -0.037 min
Response: 72382097
Conc: 27.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

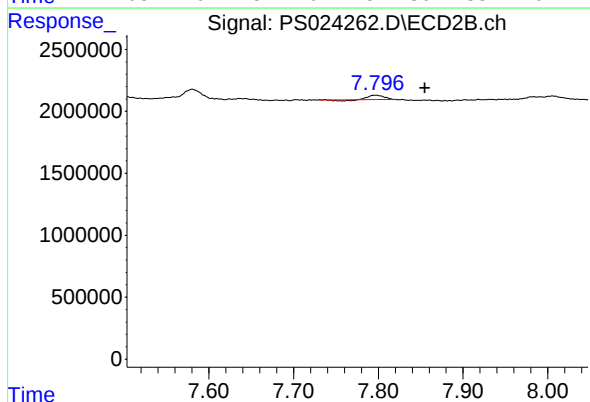


#9 2,4-D

R.T.: 7.796 min
Delta R.T.: -0.059 min
Response: 344833
Conc: N.D.

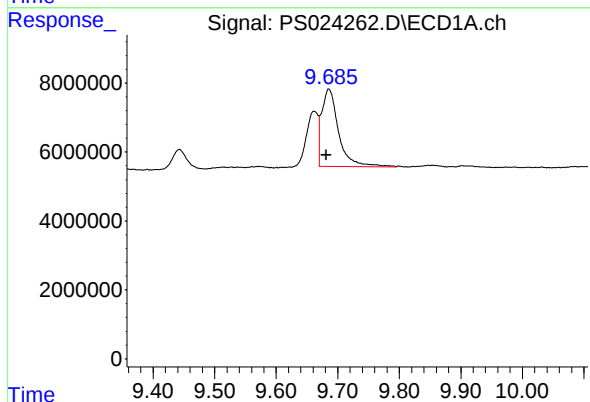


#15 Picloram

R.T.: 9.685 min
Delta R.T.: 0.004 min
Response: 42783340
Conc: 2.62 ng/ml

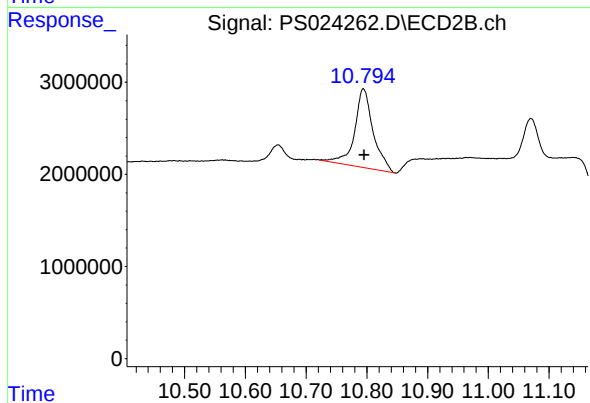

#15 Picloram


R.T.: 10.794 min
Delta R.T.: -0.001 min
Response: 18102966
Conc: 3.05 ng/ml

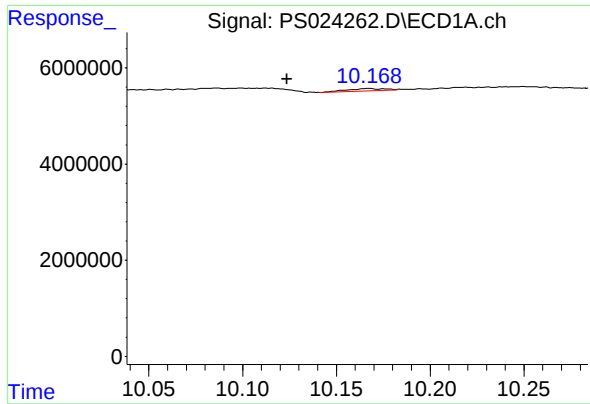

#16 DCPA

R.T.: 10.167 min
Delta R.T.: 0.043 min
Response: 671978
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

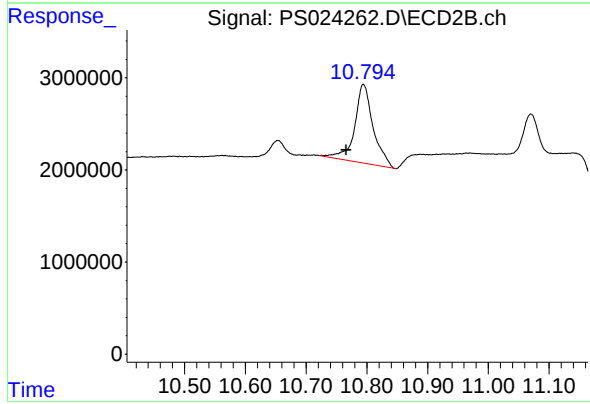

#16 DCPA

R.T.: 10.794 min
Delta R.T.: 0.028 min
Response: 18102966
Conc: 3.53 ng/ml