

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090723\
 Data File : PS024265.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Sep 2023 13:55
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 03:28:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082823.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 28 16:48:10 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.363	6.791	962.3E6	322.5E6	483.004	480.179
Target Compounds							
1) T	Dalapon	2.517	2.576	4729073	3265402	2.176	3.097 #
2) T	3,5-DICHL...	5.702	5.942	5722013	13292	1.882	<MDL #
3) T	4-Nitroph...	6.204	0.000	7898609	0	6.358	N.D. #
5) T	DICAMBA	6.495	6.946	714603	426838	<MDL	<MDL #
6) T	MCP	6.683	6.997f	2725330	12067995	<MDL	6.300 #
7) T	MCPA	6.849f	0.000	1128593	0	<MDL	N.D. #
8) T	DICHLORPROP	7.123	7.582	-217626	1252570	N.D.	1.724
9) T	2,4-D	7.254	7.800f	96824701	535059	36.402	<MDL #
11) T	2,4,5-TP ...	8.044	8.636	1094769	904843	<MDL	<MDL #
12) T	2,4,5-T	8.299	9.052f	1245116	1177859	<MDL	<MDL #
13) T	2,4-DB	8.842	0.000	41801	0	<MDL	N.D. #
14) T	DINOSEB	9.851	0.000	1094151	0	<MDL	N.D. #
15) T	Picloram	9.660	10.796	34560660	9268982	2.116	1.561 #
16) T	DCPA	10.116	10.796	440261	9268982	<MDL	1.807 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090723\
Data File : PS024265.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Sep 2023 13:55
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 03:28:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082823.M
Quant Title : 8080.M
QLast Update : Mon Aug 28 16:48:10 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

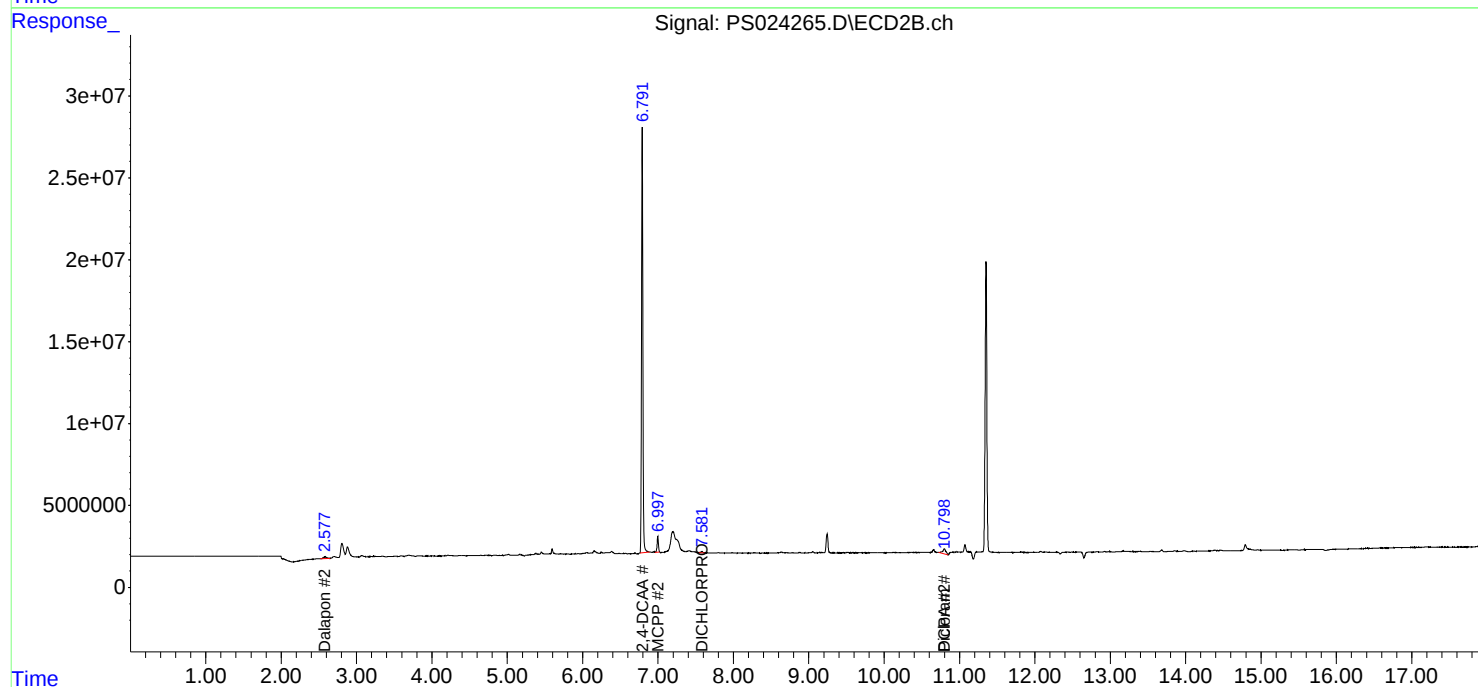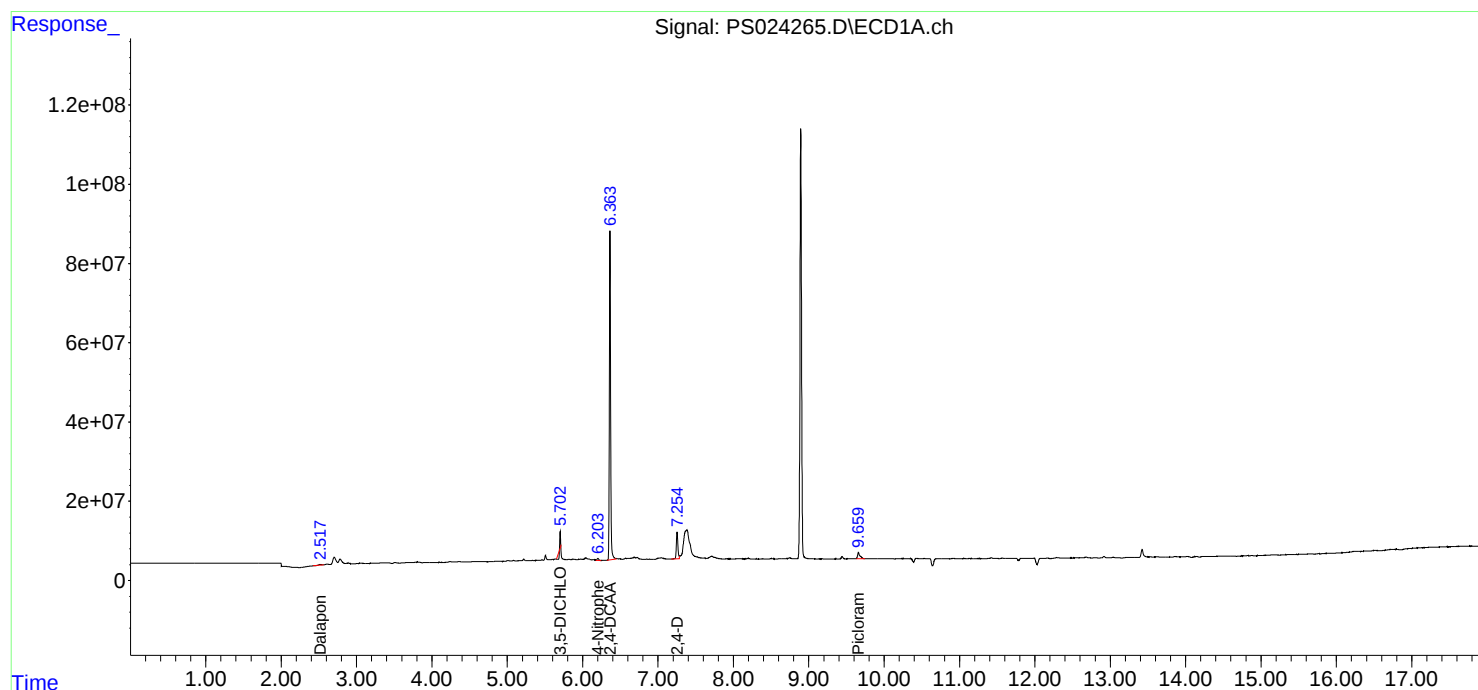


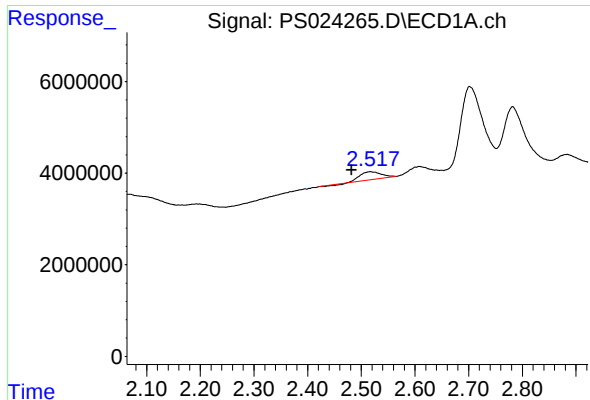

#1 Dalapon


R.T.: 2.517 min
Delta R.T.: 0.035 min
Response: 4729073
Conc: 2.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

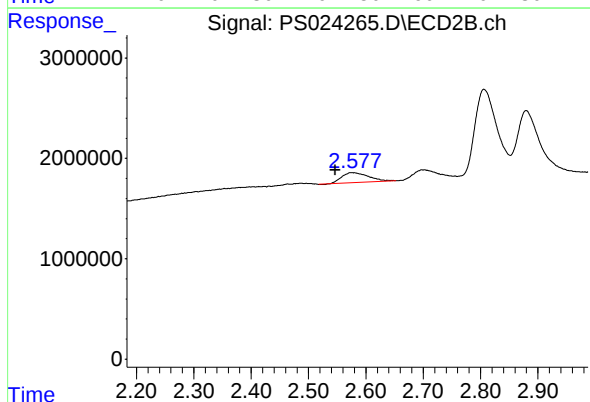


#1 Dalapon

R.T.: 2.576 min
Delta R.T.: 0.029 min
Response: 3265402
Conc: 3.10 ng/ml

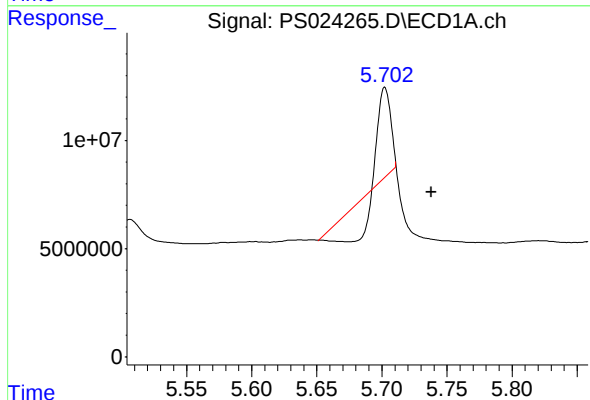


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.702 min
Delta R.T.: -0.036 min
Response: 5722013
Conc: 1.88 ng/ml

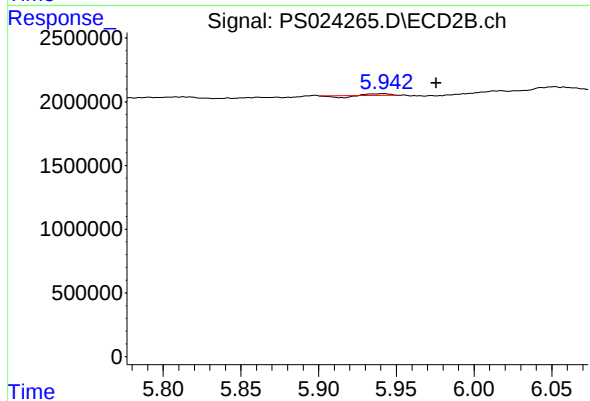

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.942 min
Delta R.T.: -0.034 min
Response: 13292
Conc: N.D.

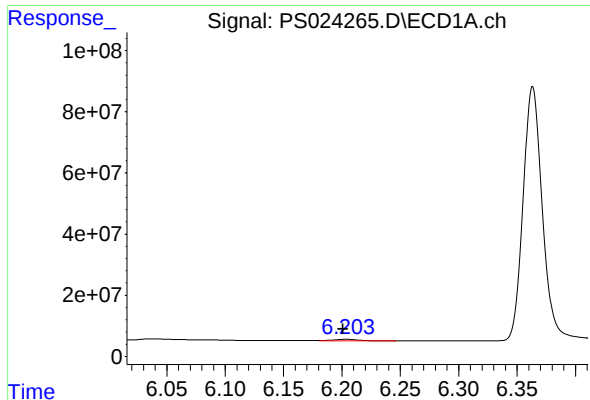

#3 4-Nitrophenol


R.T.: 6.204 min
Delta R.T.: 0.003 min
Response: 7898609
Conc: 6.36 ng/ml

Instrument :
ECD_S
ClientSampleId :

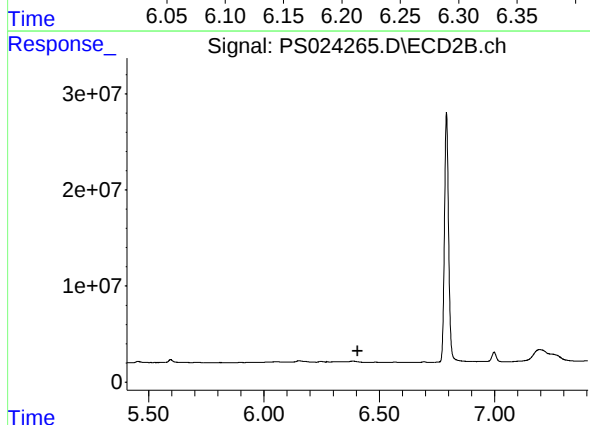


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.405 min
Response: 0
Conc: N.D.

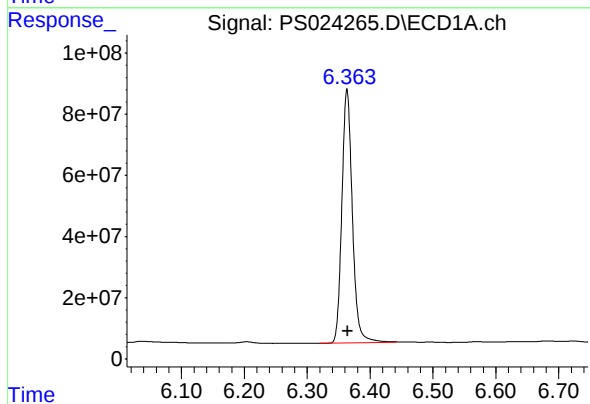


#4 2,4-DCAA

R.T.: 6.363 min
Delta R.T.: -0.001 min
Response: 962299734
Conc: 483.00 ng/ml

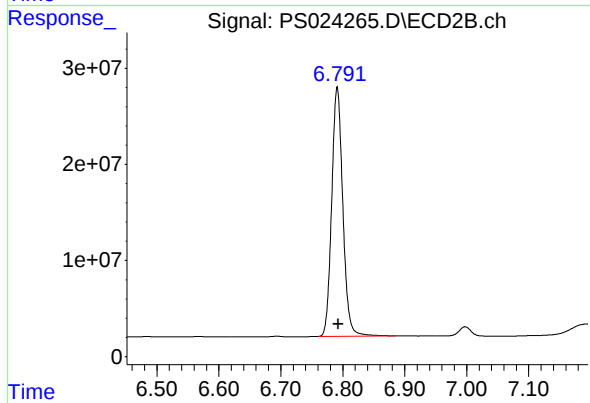

#4 2,4-DCAA


R.T.: 6.791 min
Delta R.T.: -0.002 min
Response: 322484495
Conc: 480.18 ng/ml

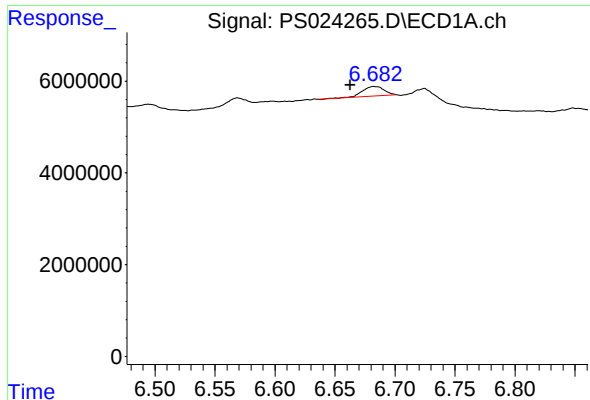

#6 MCPP


R.T.: 6.683 min
Delta R.T.: 0.020 min
Response: 2725330
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

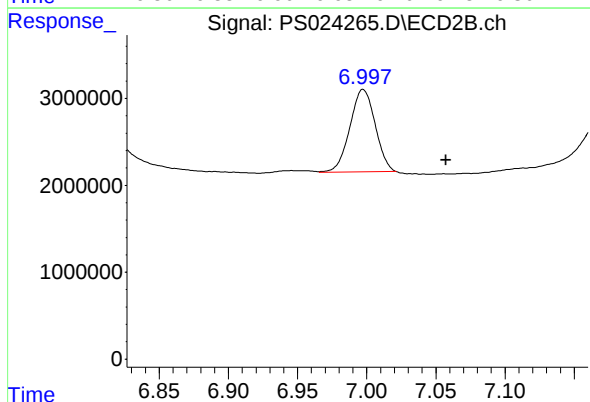


#6 MCPP

R.T.: 6.997 min
Delta R.T.: -0.060 min
Response: 12067995
Conc: 6.30 ug/ml

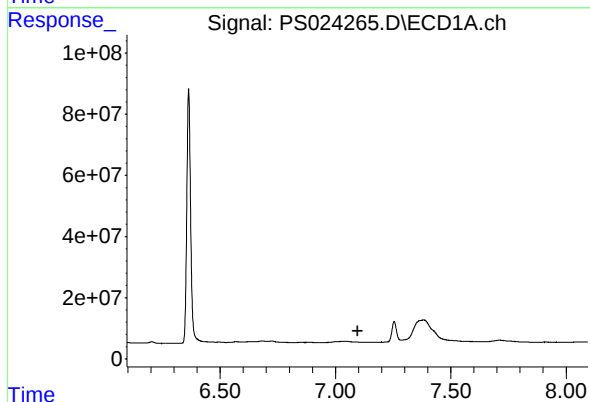


#8 DICHLORPROP

R.T.: 7.123 min
Delta R.T.: 0.028 min
Response: -217626
Conc: N.D.

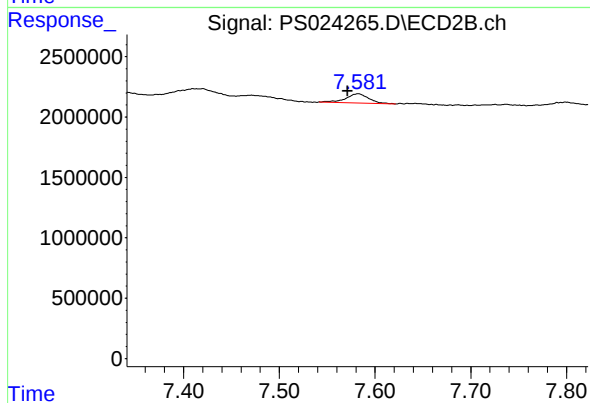

#8 DICHLORPROP


R.T.: 7.582 min
Delta R.T.: 0.011 min
Response: 1252570
Conc: 1.72 ng/ml

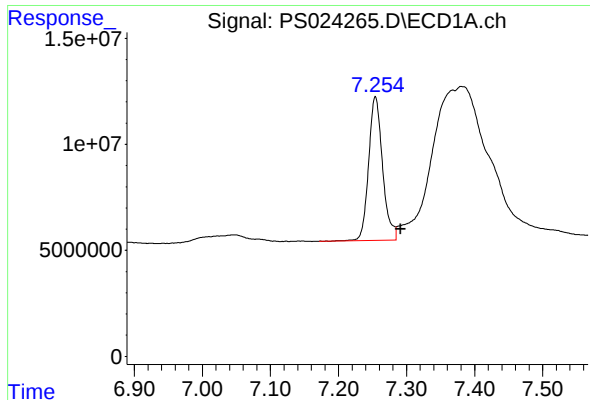

#9 2,4-D


R.T.: 7.254 min
Delta R.T.: -0.037 min
Response: 96824701
Conc: 36.40 ng/ml

Instrument :
ECD_S
ClientSampleId :

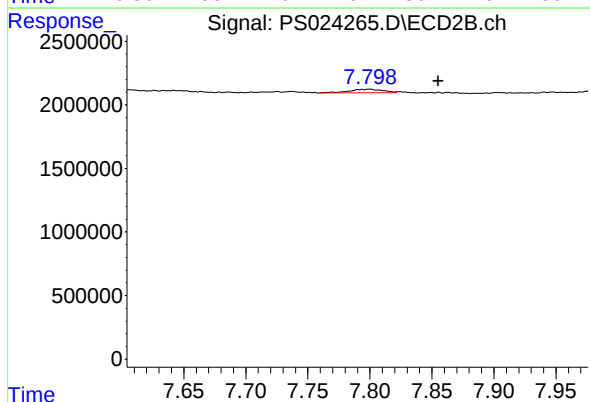


#9 2,4-D

R.T.: 7.800 min
Delta R.T.: -0.056 min
Response: 535059
Conc: N.D.

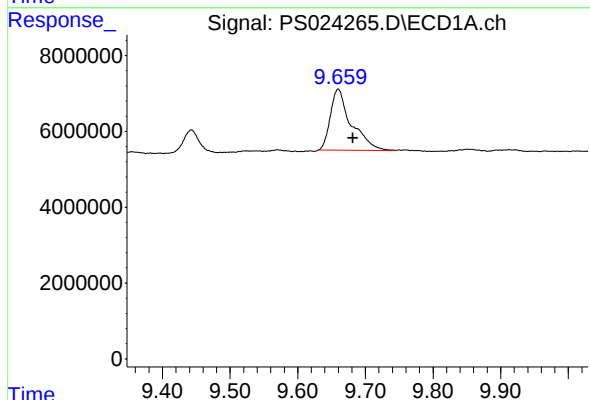


#15 Picloram

R.T.: 9.660 min
Delta R.T.: -0.022 min
Response: 34560660
Conc: 2.12 ng/ml

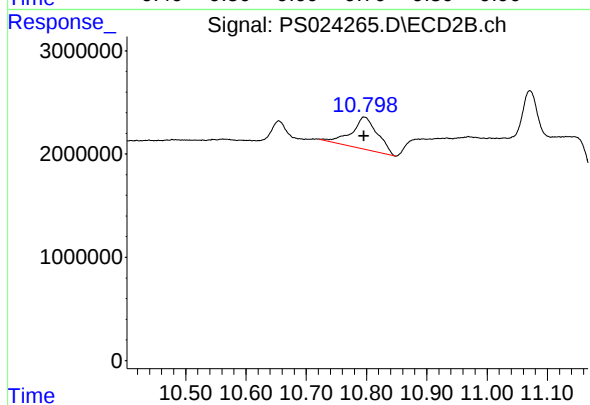

#15 Picloram


R.T.: 10.796 min
Delta R.T.: 0.000 min
Response: 9268982
Conc: 1.56 ng/ml

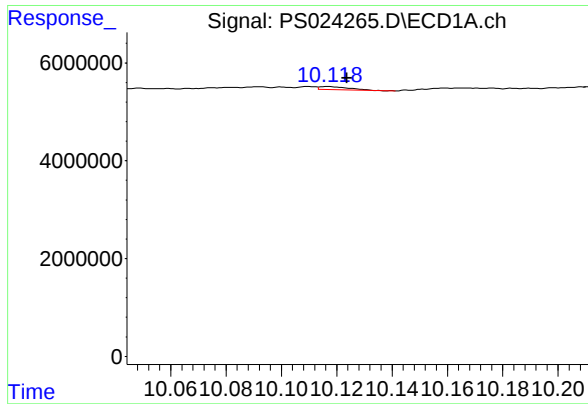

#16 DCPA

R.T.: 10.116 min
Delta R.T.: -0.007 min
Response: 440261
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

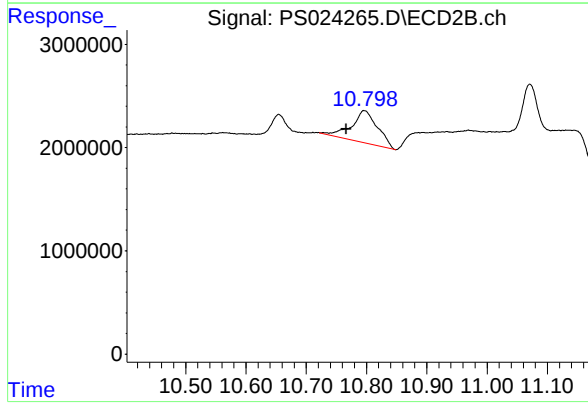

#16 DCPA

R.T.: 10.796 min
Delta R.T.: 0.030 min
Response: 9268982
Conc: 1.81 ng/ml