

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090723\
 Data File : PS024277.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Sep 2023 20:57
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 03:30:17 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082823.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 28 16:48:10 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.363	6.790	965.9E6	325.9E6	484.802	485.277
Target Compounds							
1) T	Dalapon	2.514	2.578	5284607	3457782	2.431	3.279 #
2) T	3,5-DICHL...	5.702	5.934f	6480984	6525	2.132	<MDL #
3) T	4-Nitroph...	6.202	6.337f	11433952	512013	9.203	1.214 #
5) T	DICAMBA	6.493	6.946	860641	510224	<MDL	<MDL #
6) T	MCP	6.685	6.997f	4501668	11725489	<MDL	6.121 #
7) T	MCPA	6.847f	7.202f	1460797	22354070	<MDL	7.647 #
8) T	DICHLORPROP	7.046f	7.582	3512532	4337378	1.545	5.970 #
9) T	2,4-D	7.254	7.797f	91202569	793706	34.288	<MDL #
10) T	Pentachlo...	7.592f	0.000	481691	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.049	8.632	783262	498001	<MDL	<MDL #
12) T	2,4,5-T	8.301	9.049	1001531	757925	<MDL	<MDL #
13) T	2,4-DB	8.823	9.504	125532	699303	<MDL	1.521 #
14) T	DINOSEB	9.851	0.000	759303	0	<MDL	N.D. #
15) T	Picloram	9.658	10.796	29292667	7952937	1.794	1.339 #
16) T	DCPA	10.110	10.796	663229	7952937	<MDL	1.550 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090723\
Data File : PS024277.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Sep 2023 20:57
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 03:30:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082823.M
Quant Title : 8080.M
QLast Update : Mon Aug 28 16:48:10 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

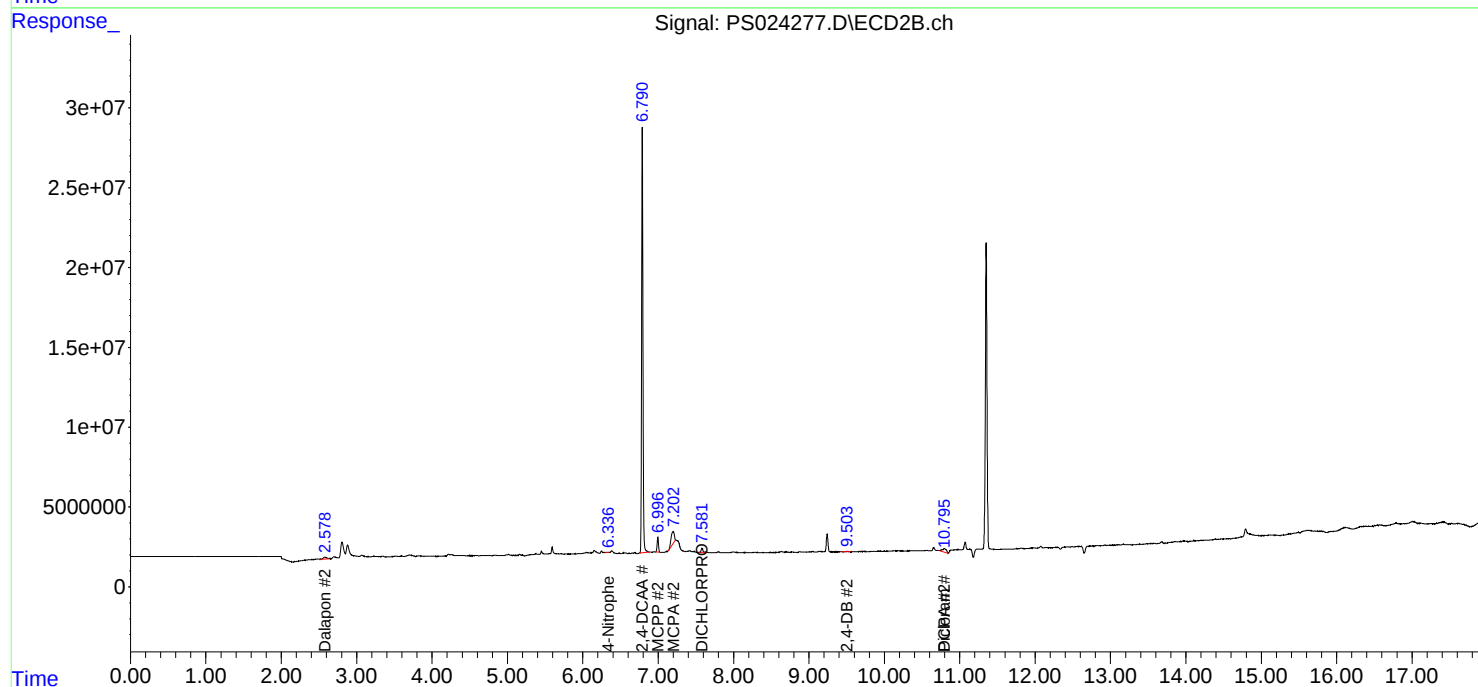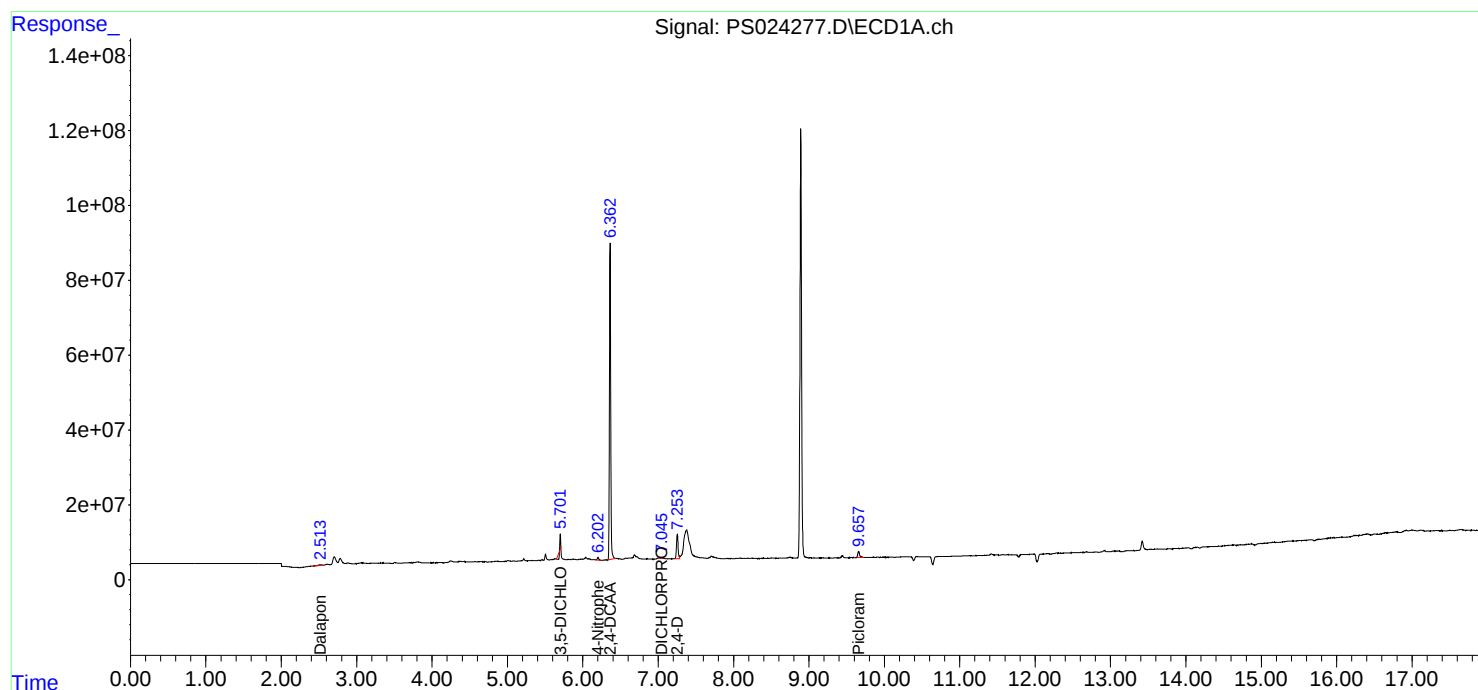


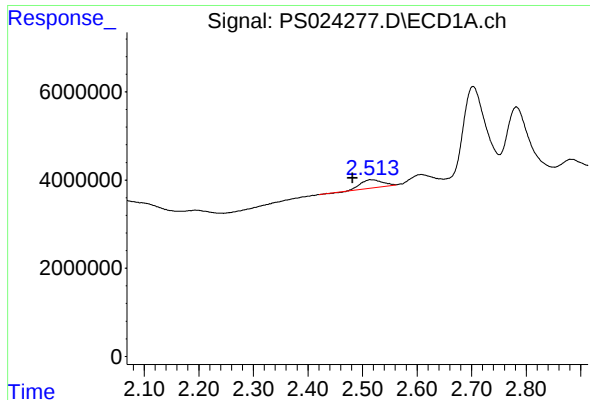

#1 Dalapon


R.T.: 2.514 min
Delta R.T.: 0.032 min
Response: 5284607
Conc: 2.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

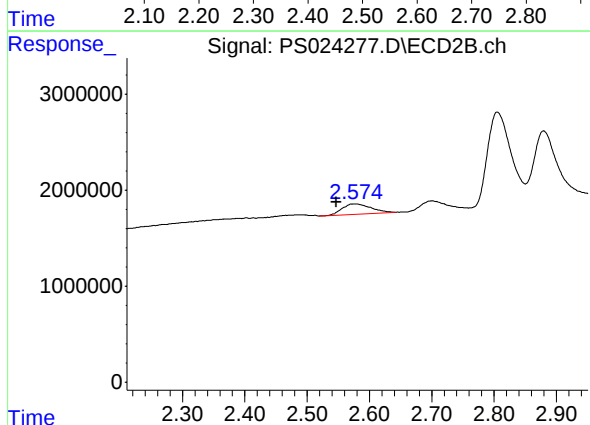


#1 Dalapon

R.T.: 2.578 min
Delta R.T.: 0.031 min
Response: 3457782
Conc: 3.28 ng/ml

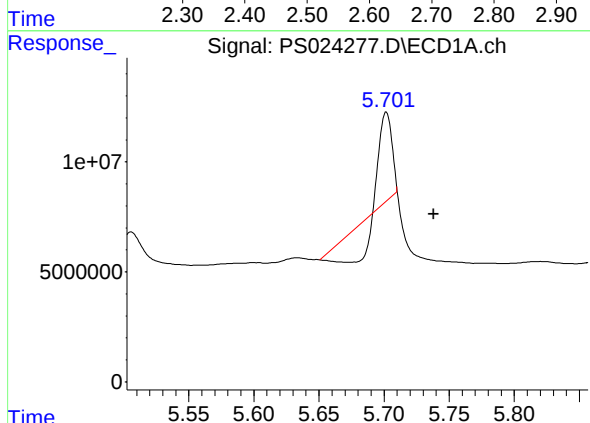


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.702 min
Delta R.T.: -0.036 min
Response: 6480984
Conc: 2.13 ng/ml

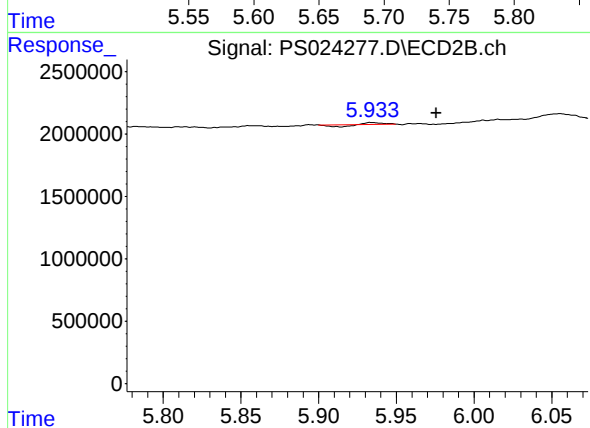

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.934 min
Delta R.T.: -0.042 min
Response: 6525
Conc: N.D.

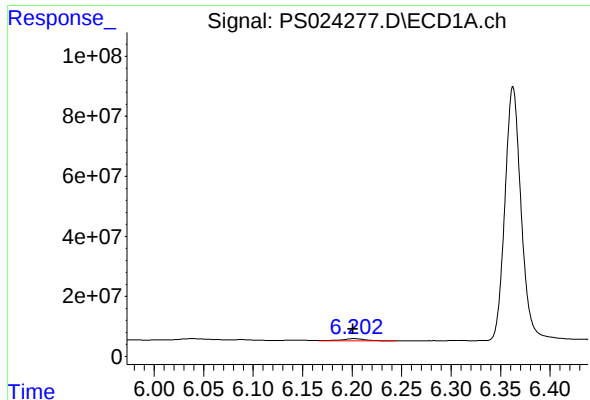

#3 4-Nitrophenol


R.T.: 6.202 min
Delta R.T.: 0.001 min
Response: 11433952
Conc: 9.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

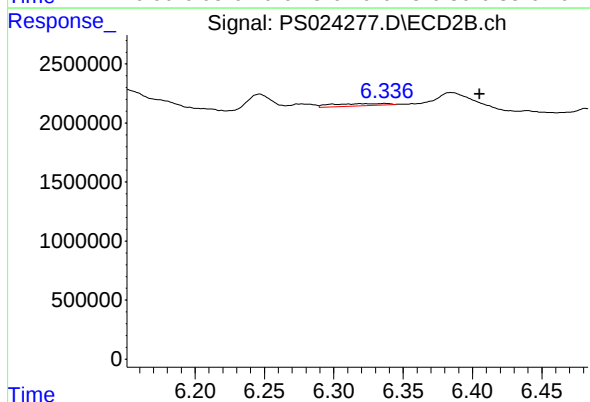


#3 4-Nitrophenol

R.T.: 6.337 min
Delta R.T.: -0.068 min
Response: 512013
Conc: 1.21 ng/ml

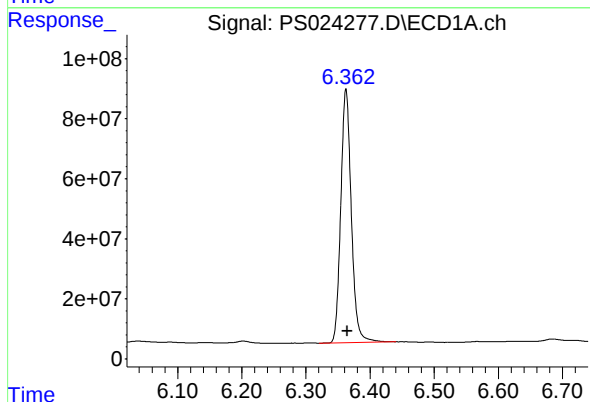


#4 2,4-DCAA

R.T.: 6.363 min
Delta R.T.: -0.002 min
Response: 965880407
Conc: 484.80 ng/ml

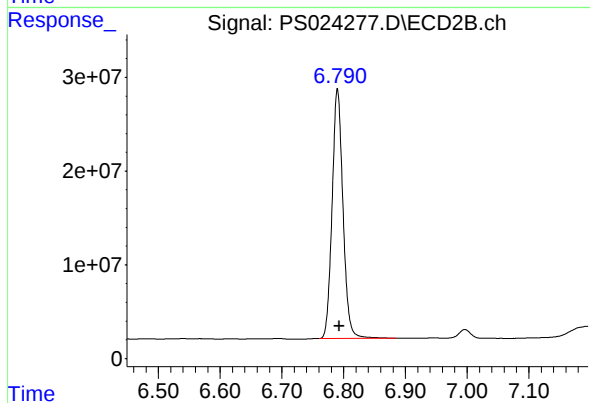

#4 2,4-DCAA


R.T.: 6.790 min
Delta R.T.: -0.003 min
Response: 325907718
Conc: 485.28 ng/ml

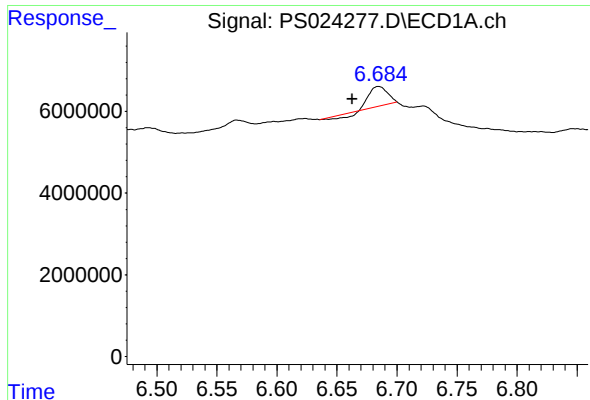

#6 MCPP


R.T.: 6.685 min
Delta R.T.: 0.022 min
Response: 4501668
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

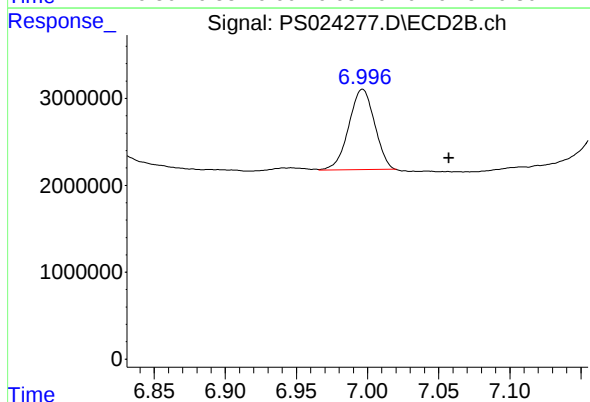


#6 MCPP

R.T.: 6.997 min
Delta R.T.: -0.061 min
Response: 11725489
Conc: 6.12 ug/ml

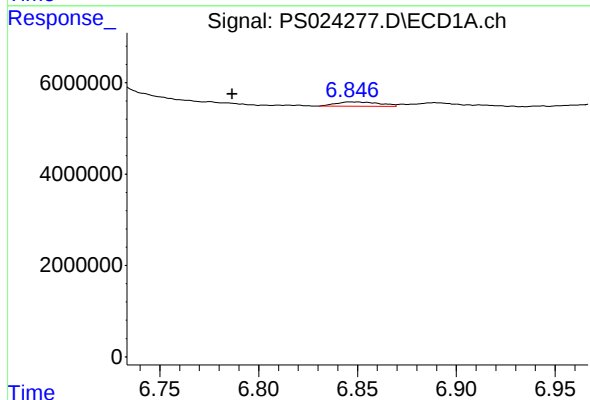


#7 MCPA

R.T.: 6.847 min
Delta R.T.: 0.060 min
Response: 1460797
Conc: N.D.

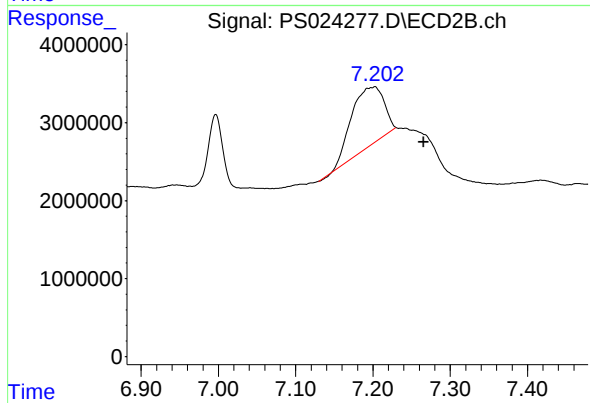

#7 MCPA


R.T.: 7.202 min
Delta R.T.: -0.063 min
Response: 22354070
Conc: 7.65 ug/ml

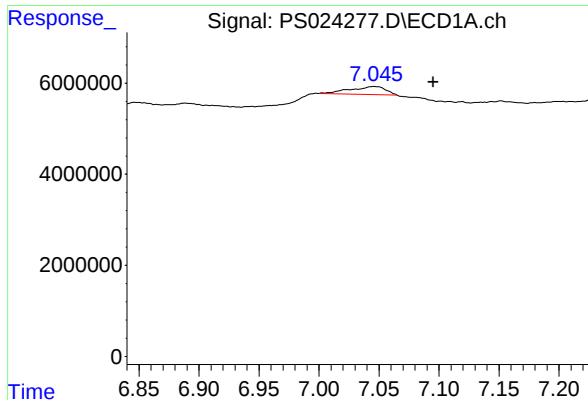

#8 DICHLORPROP


R.T.: 7.046 min
Delta R.T.: -0.049 min
Response: 3512532
Conc: 1.55 ng/ml

Instrument :
ECD_S
ClientSampleId :

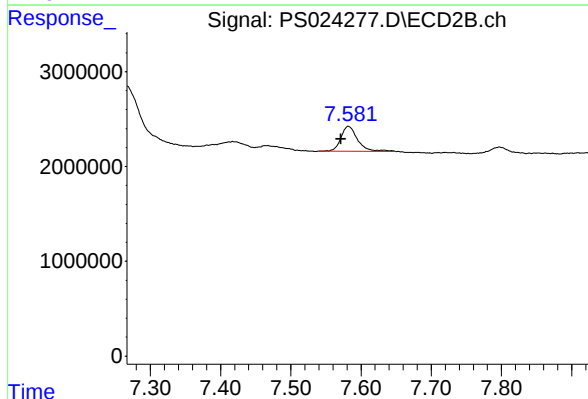


#8 DICHLORPROP

R.T.: 7.582 min
Delta R.T.: 0.011 min
Response: 4337378
Conc: 5.97 ng/ml

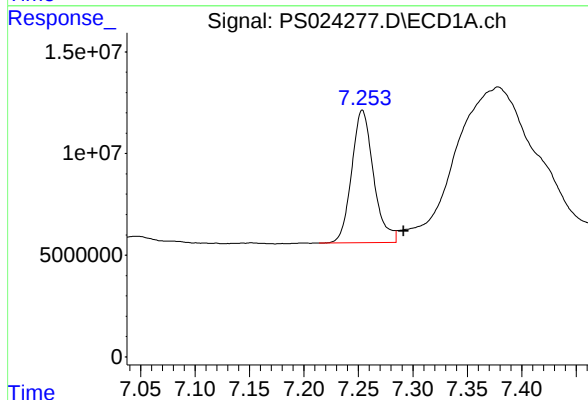


#9 2,4-D

R.T.: 7.254 min
Delta R.T.: -0.038 min
Response: 91202569
Conc: 34.29 ng/ml

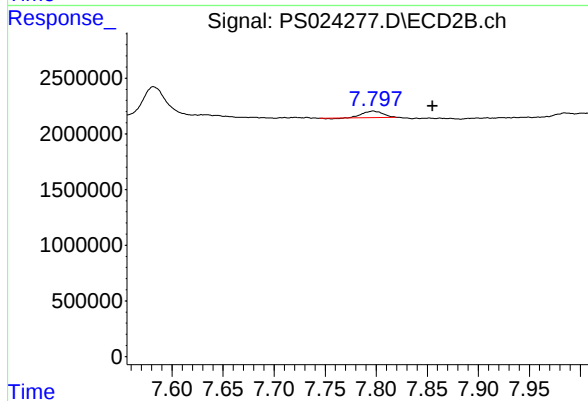

#9 2,4-D


R.T.: 7.797 min
Delta R.T.: -0.058 min
Response: 793706
Conc: N.D.

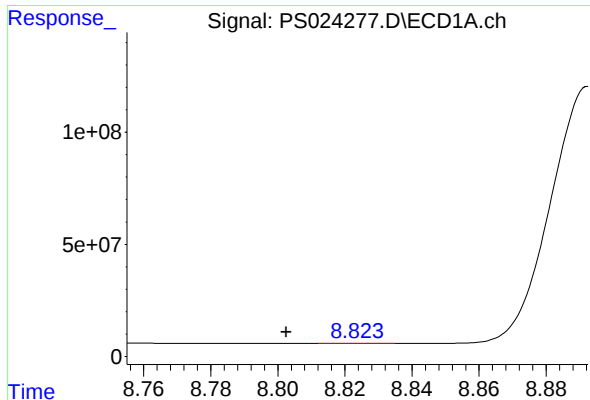

#13 2,4-DB


R.T.: 8.823 min
Delta R.T.: 0.021 min
Response: 125532
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

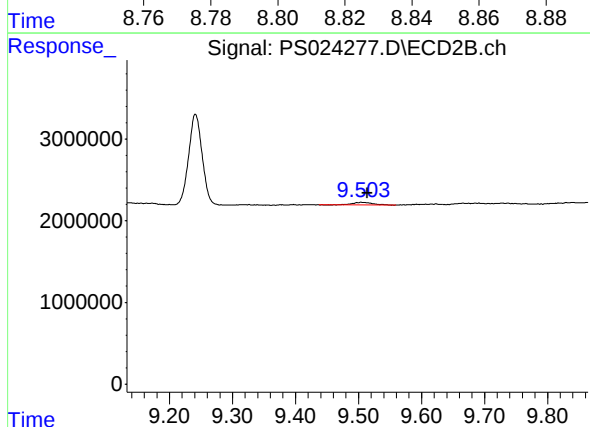


#13 2,4-DB

R.T.: 9.504 min
Delta R.T.: -0.010 min
Response: 699303
Conc: 1.52 ng/ml

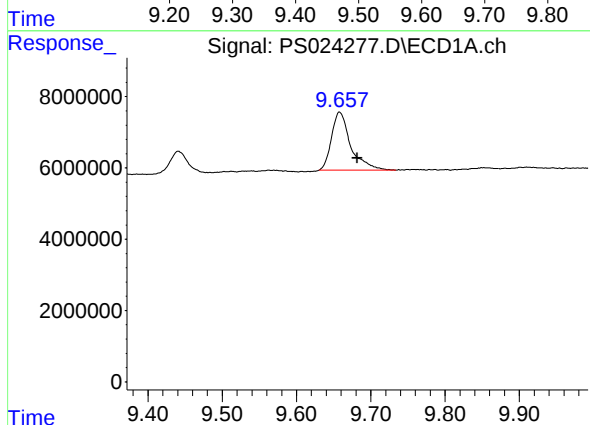


#15 Picloram

R.T.: 9.658 min
Delta R.T.: -0.024 min
Response: 29292667
Conc: 1.79 ng/ml

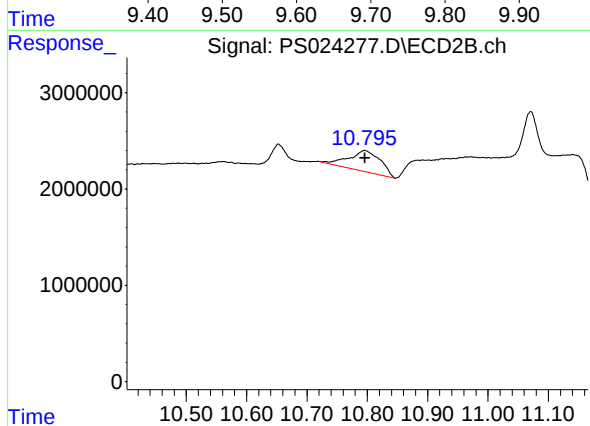

#15 Picloram


R.T.: 10.796 min
Delta R.T.: 0.000 min
Response: 7952937
Conc: 1.34 ng/ml

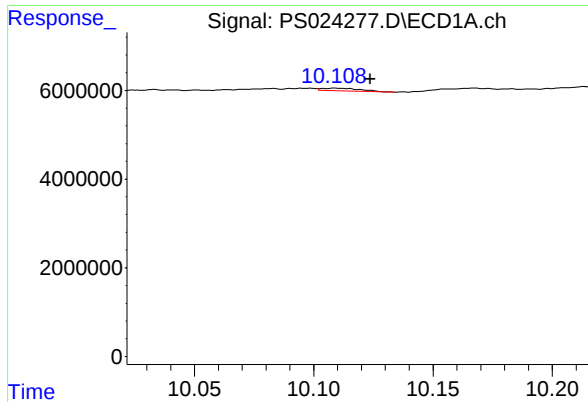

#16 DCPA

R.T.: 10.110 min
Delta R.T.: -0.014 min
Response: 663229
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

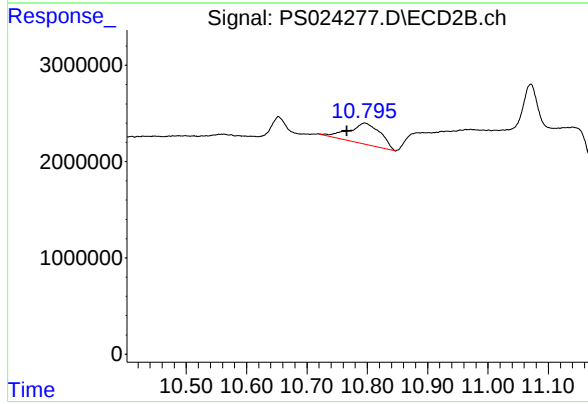

#16 DCPA

R.T.: 10.796 min
Delta R.T.: 0.029 min
Response: 7952937
Conc: 1.55 ng/ml