

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090723\
 Data File : PS024283.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Sep 2023 00:11
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 03:31:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082823.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 28 16:48:10 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.363	6.790	969.4E6	326.3E6	486.548	485.894
Target Compounds							
1) T	Dalapon	2.519	2.577	5361175	3253595	2.467	3.085 #
2) T	3,5-DICHL...	5.702	6.007	9677550	-175285	3.184	N.D. #
3) T	4-Nitroph...	6.203	6.336f	9024418	448529	7.264	1.064 #
5) T	DICAMBA	6.492	6.945	748975	399357	<MDL	<MDL #
6) T	MCPD	6.685	6.996f	5649018	12369966	<MDL	6.457 #
7) T	MCPA	6.851f	7.210f	1350521	18074506	<MDL	6.183 #
8) T	DICHLORPROP	7.047f	7.582	3298977	4795058	1.451	6.600 #
9) T	2,4-D	7.254	7.796f	98781163	907165	37.137	1.018 #
11) T	2,4,5-TP ...	8.043	8.633	976135	792302	<MDL	<MDL #
12) T	2,4,5-T	8.295	9.051f	1128384	792330	<MDL	<MDL #
13) T	2,4-DB	8.746f	9.506	1226514	804247	<MDL	1.750 #
14) T	DINOSEB	9.851	0.000	1118281	0	<MDL	N.D. #
15) T	Picloram	9.659	10.796	31769644	6491268	1.945	1.093 #
16) T	DCPA	10.166f	10.766	719853	1440265	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090723\
Data File : PS024283.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2023 00:11
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 03:31:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082823.M
Quant Title : 8080.M
QLast Update : Mon Aug 28 16:48:10 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

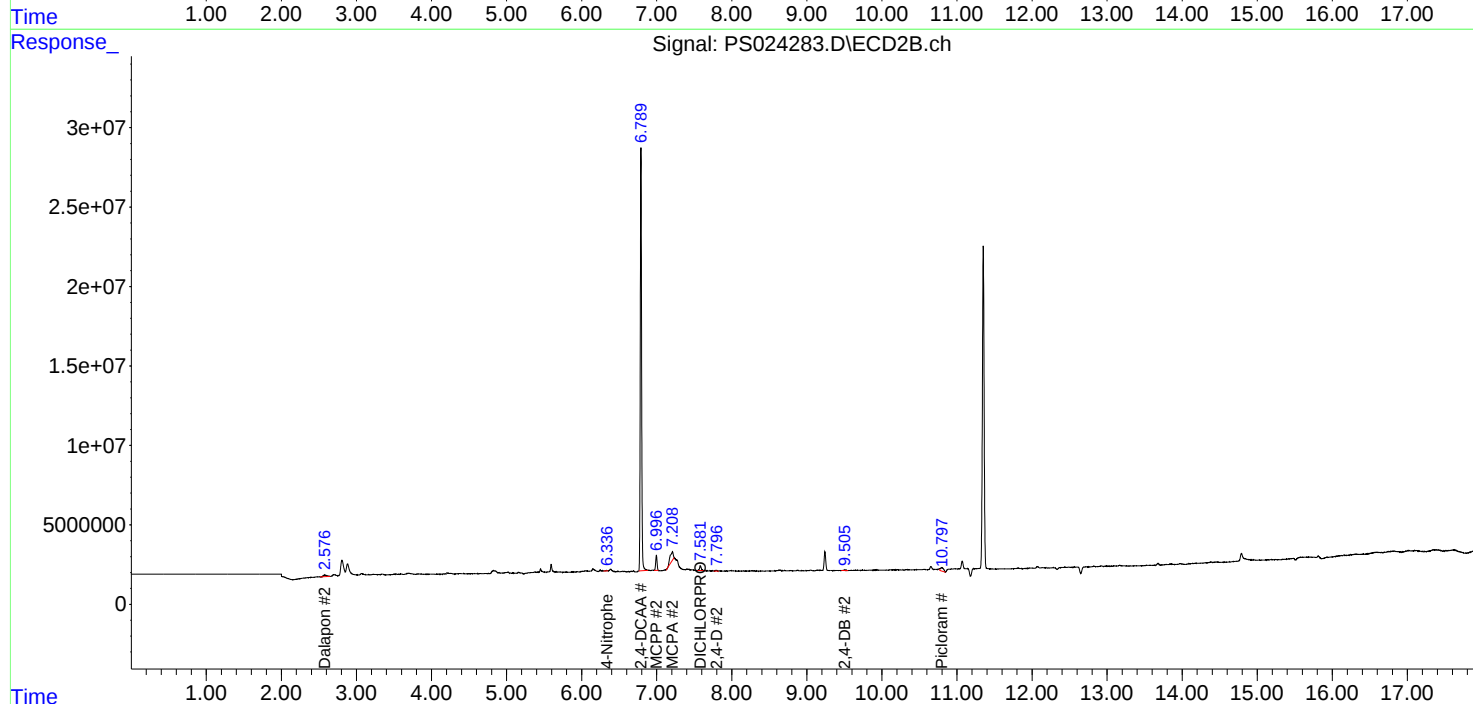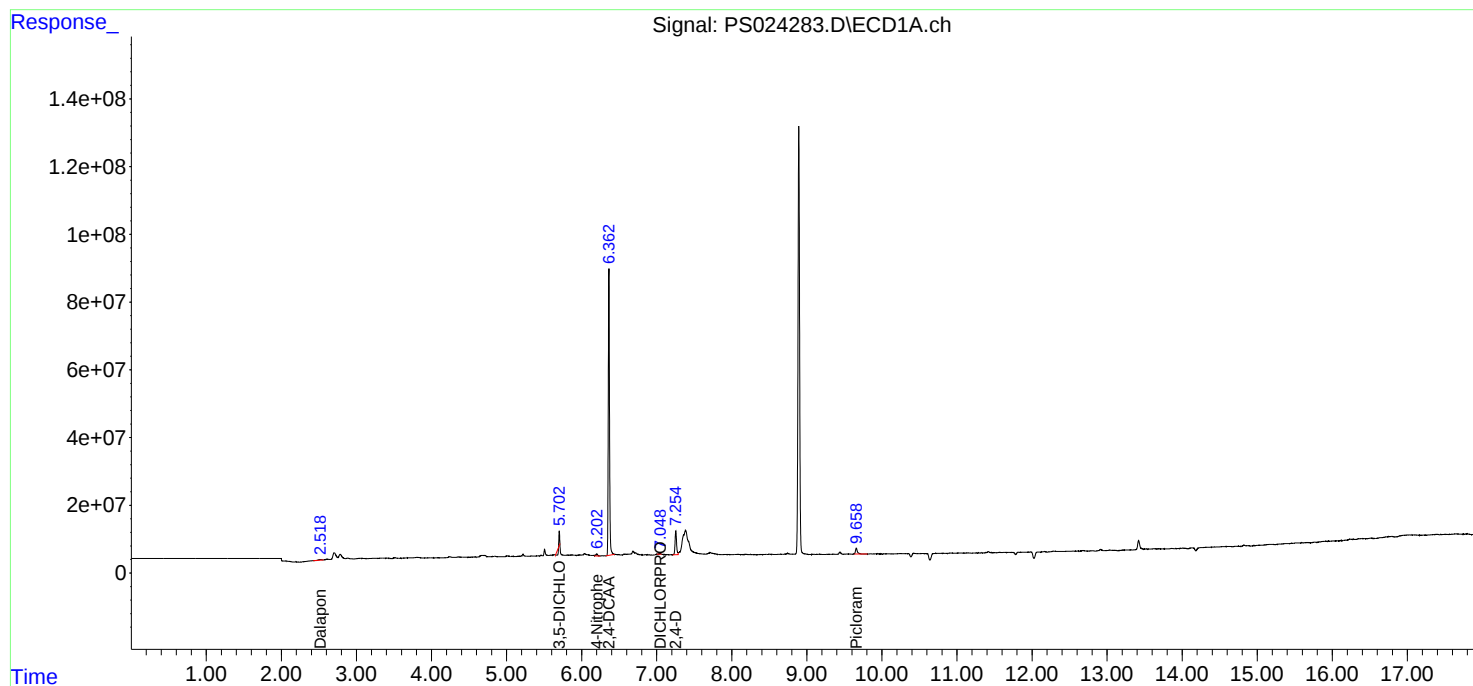


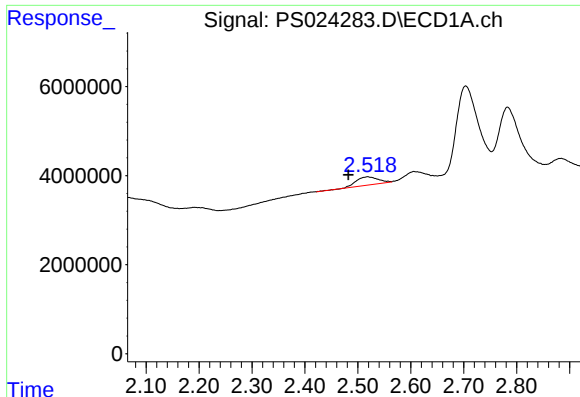

#1 Dalapon


R.T.: 2.519 min
Delta R.T.: 0.037 min
Response: 5361175
Conc: 2.47 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

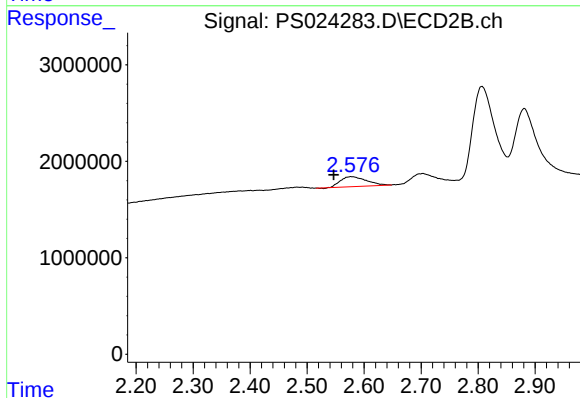


#1 Dalapon

R.T.: 2.577 min
Delta R.T.: 0.030 min
Response: 3253595
Conc: 3.09 ng/ml

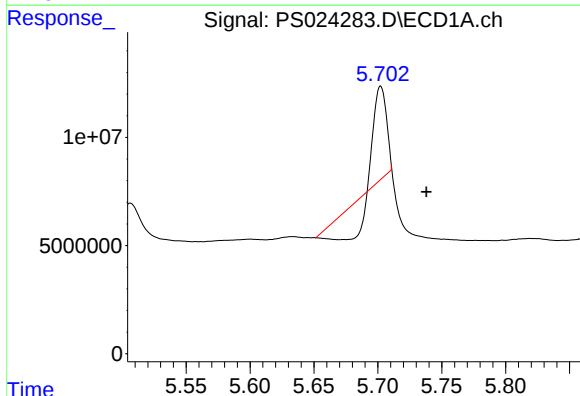


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.702 min
Delta R.T.: -0.036 min
Response: 9677550
Conc: 3.18 ng/ml

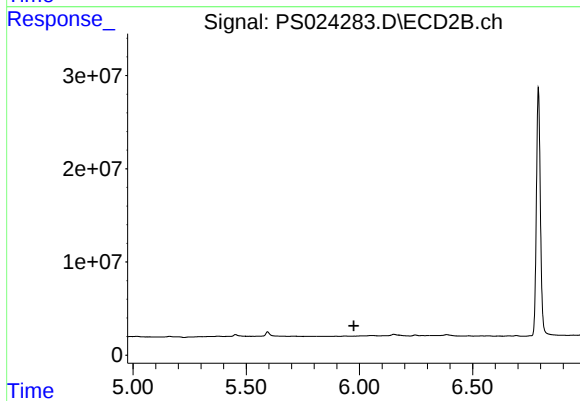

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.007 min
Delta R.T.: 0.032 min
Response: -175285
Conc: N.D.

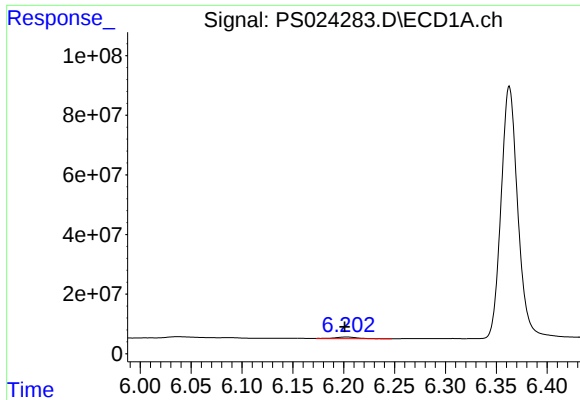

#3 4-Nitrophenol


R.T.: 6.203 min
Delta R.T.: 0.002 min
Response: 9024418
Conc: 7.26 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

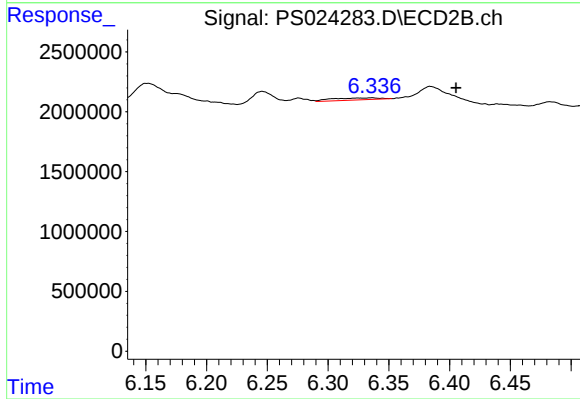


#3 4-Nitrophenol

R.T.: 6.336 min
Delta R.T.: -0.069 min
Response: 448529
Conc: 1.06 ng/ml

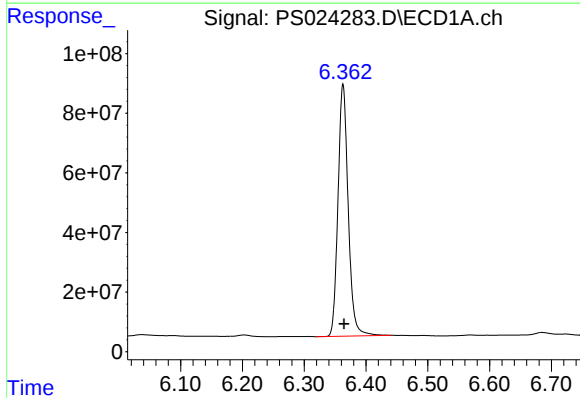


#4 2,4-DCAA

R.T.: 6.363 min
Delta R.T.: -0.002 min
Response: 969360361
Conc: 486.55 ng/ml

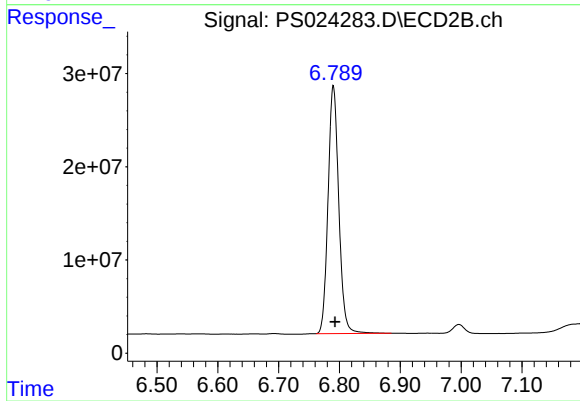

#4 2,4-DCAA


R.T.: 6.790 min
Delta R.T.: -0.003 min
Response: 326322206
Conc: 485.89 ng/ml

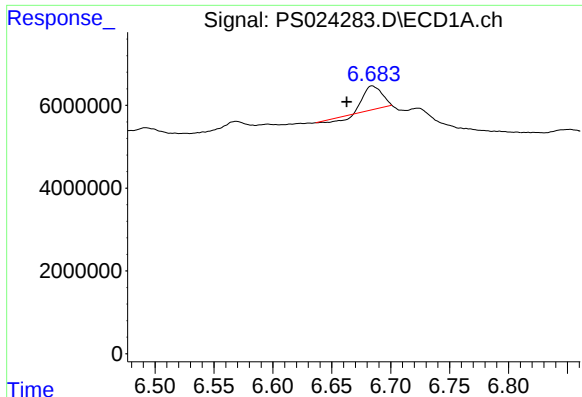

#6 MCP


R.T.: 6.685 min
Delta R.T.: 0.022 min
Response: 5649018
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

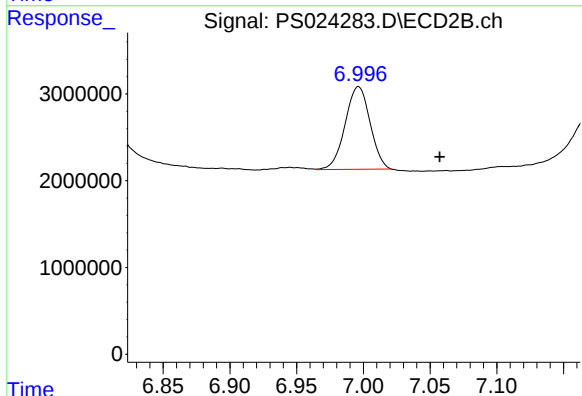


#6 MCP

R.T.: 6.996 min
Delta R.T.: -0.061 min
Response: 12369966
Conc: 6.46 ug/ml

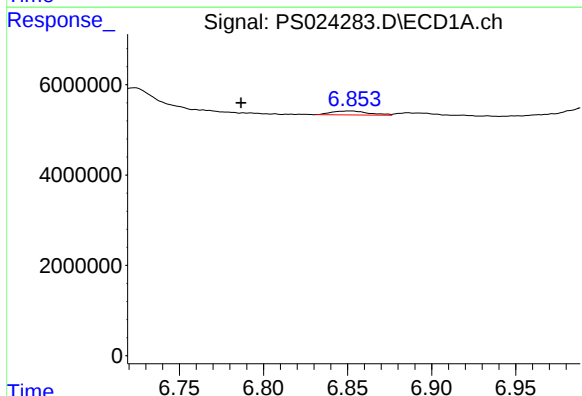


#7 MCP

R.T.: 6.851 min
Delta R.T.: 0.064 min
Response: 1350521
Conc: N.D.

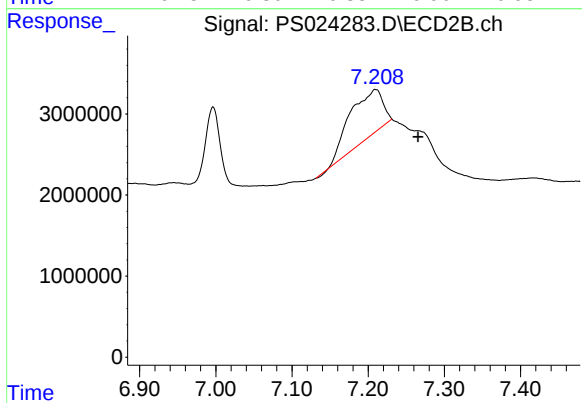

#7 MCP


R.T.: 7.210 min
Delta R.T.: -0.056 min
Response: 18074506
Conc: 6.18 ug/ml

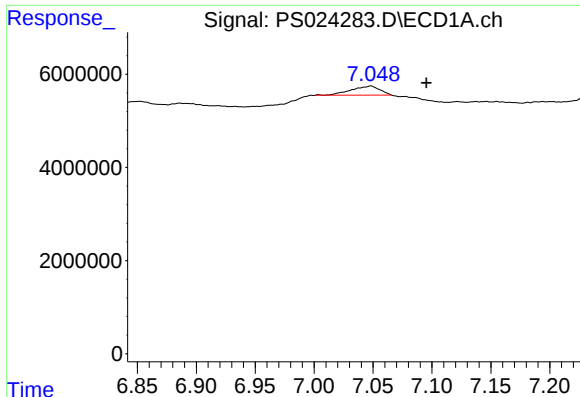

#8 DICHLORPROP


R.T.: 7.047 min
Delta R.T.: -0.048 min
Response: 3298977
Conc: 1.45 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

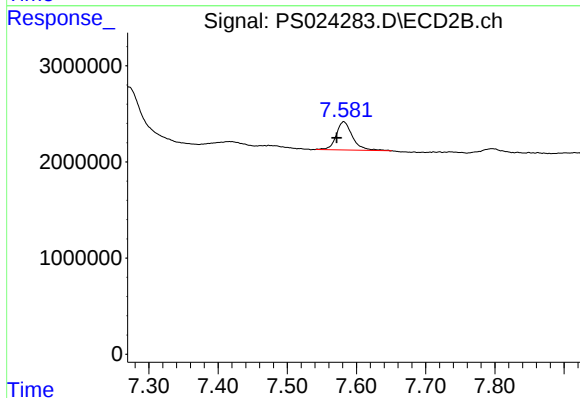


#8 DICHLORPROP

R.T.: 7.582 min
Delta R.T.: 0.010 min
Response: 4795058
Conc: 6.60 ng/ml

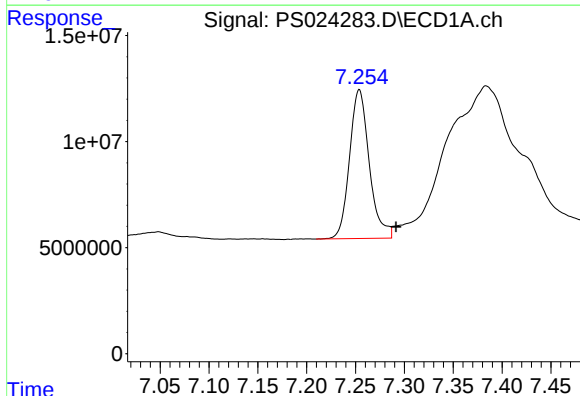


#9 2,4-D

R.T.: 7.254 min
Delta R.T.: -0.038 min
Response: 98781163
Conc: 37.14 ng/ml

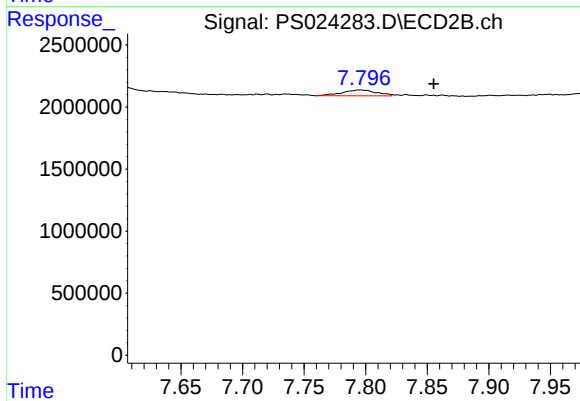

#9 2,4-D


R.T.: 7.796 min
Delta R.T.: -0.060 min
Response: 907165
Conc: 1.02 ng/ml

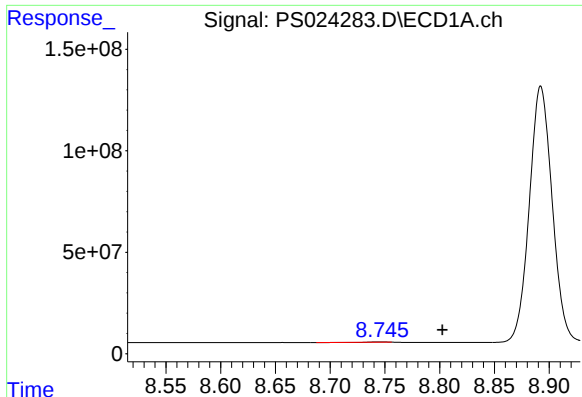

#13 2,4-DB


R.T.: 8.746 min
Delta R.T.: -0.057 min
Response: 1226514
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

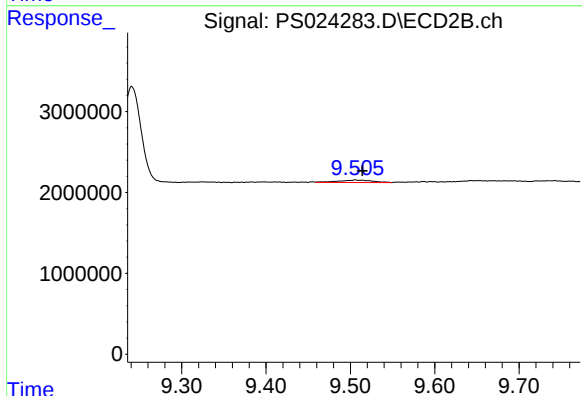


#13 2,4-DB

R.T.: 9.506 min
Delta R.T.: -0.008 min
Response: 804247
Conc: 1.75 ng/ml

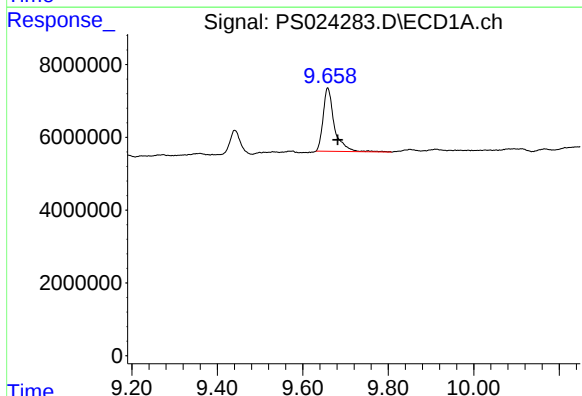

#15 Picloram

R.T.: 9.659 min
Delta R.T.: -0.023 min
Response: 31769644
Conc: 1.95 ng/ml

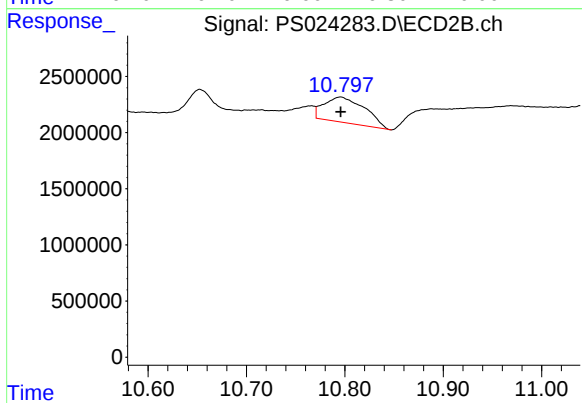

#15 Picloram

R.T.: 10.796 min
Delta R.T.: 0.000 min
Response: 6491268
Conc: 1.09 ng/ml