

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090820\
 Data File : PS012144.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Sep 2020 08:47
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 11:03:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.218	6.914	417.1E6	248.5E6	382.390	464.634
Target Compounds							
9) T	2,4-D	8.400	0.000	98937070	0	87.625	N.D. #
15) T	Picloram	11.052	11.034	13411498	13183294	1.716	2.909 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090820\
Data File : PS012144.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2020 08:47
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 11:03:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

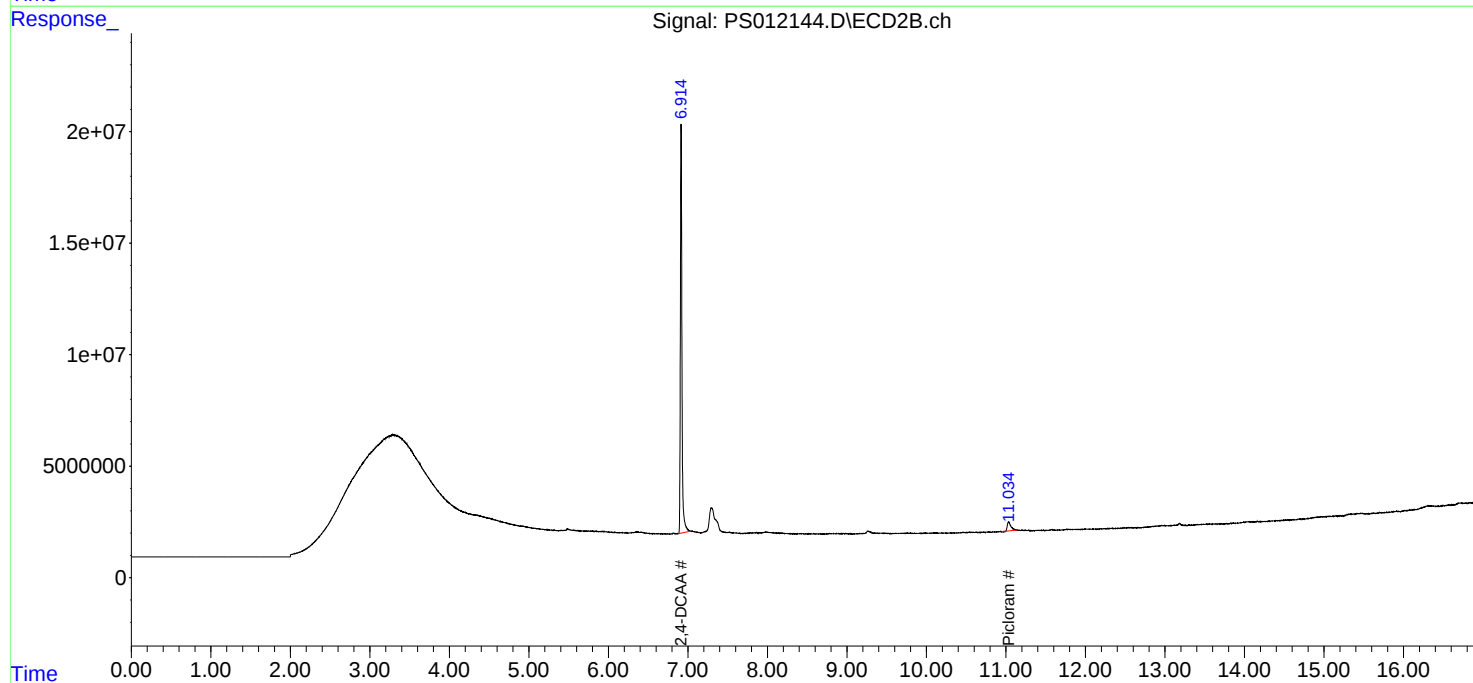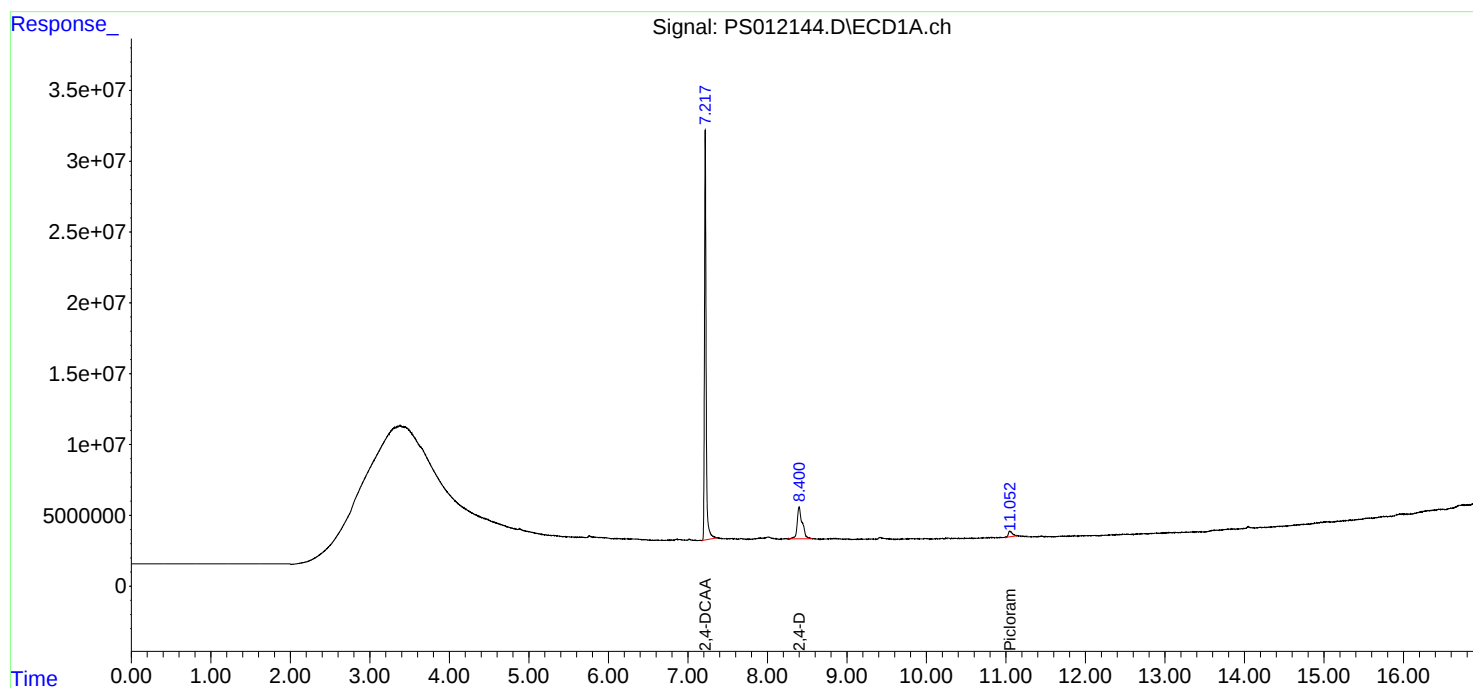


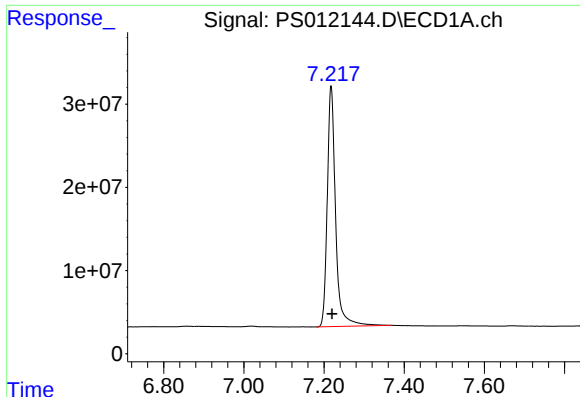

#4 2,4-DCAA


R.T.: 7.218 min
Delta R.T.: -0.002 min
Response: 417098712
Conc: 382.39 ng/ml

Instrument :
ECD_S
ClientSampleId :

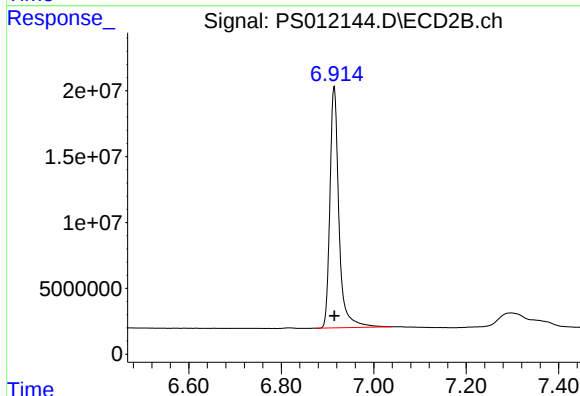


#4 2,4-DCAA

R.T.: 6.914 min
Delta R.T.: 0.000 min
Response: 248480181
Conc: 464.63 ng/ml

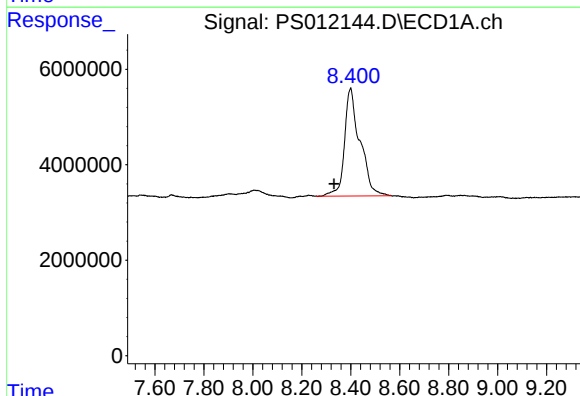


#9 2,4-D

R.T.: 8.400 min
Delta R.T.: 0.068 min
Response: 98937070
Conc: 87.63 ng/ml

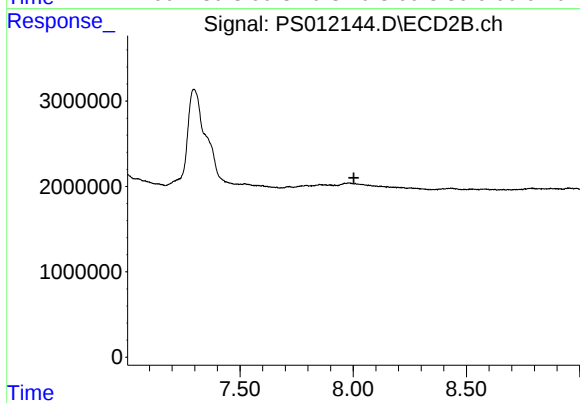

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.003 min
Response: 0
Conc: N.D.

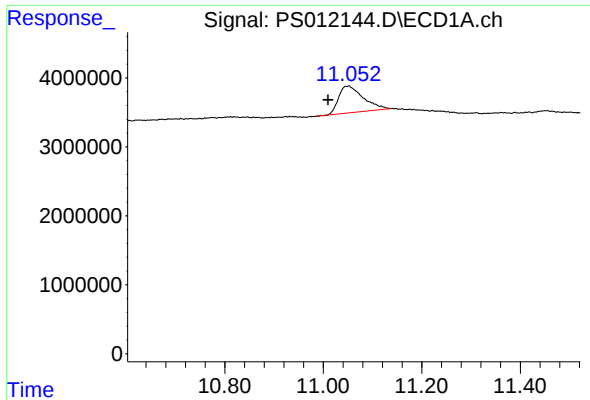

#15 Picloram

R.T.: 11.052 min
Delta R.T.: 0.042 min
Response: 13411498
Conc: 1.72 ng/ml

Instrument :
ECD_S
ClientSampleId :

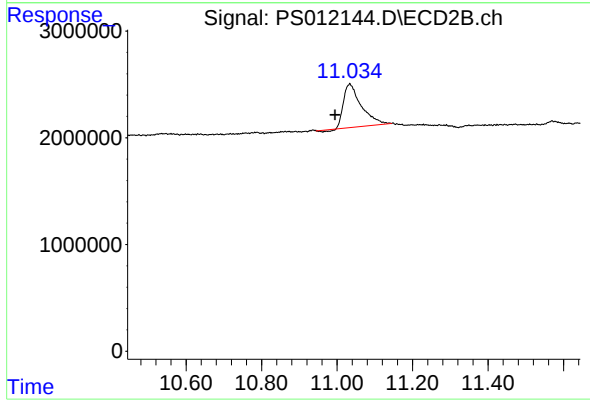

#15 Picloram

R.T.: 11.034 min
Delta R.T.: 0.038 min
Response: 13183294
Conc: 2.91 ng/ml