

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090820\
 Data File : PS012153.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Sep 2020 18:19
 Operator : DD\AJ
 Sample : PB131479TB
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 02:37:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.217	6.914	145.7E6	93318157	133.541	174.496 #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.095	0	52174765	N.D.	63.425
5) T	DICAMBA	7.480	7.048	7568756	11242846	1.848	5.204 #
7) T	MCPA	7.698	0.000	67824347	0	14.911	N.D. #
8) T	DICHLORPROP	0.000	7.738	0	20906179	N.D.	37.026
9) T	2,4-D	8.398	7.942	147.9E6	9412277	131.011	12.812 #
11) T	2,4,5-TP ...	0.000	8.762	0	8487441	N.D.	2.903
12) T	2,4,5-T	9.409	0.000	21942550	0	3.703	N.D. #
15) T	Picloram	11.011	11.016	21708046	17029548	2.778	3.757 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090820\
Data File : PS012153.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2020 18:19
Operator : DD\AJ
Sample : PB131479TB
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 02:37:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

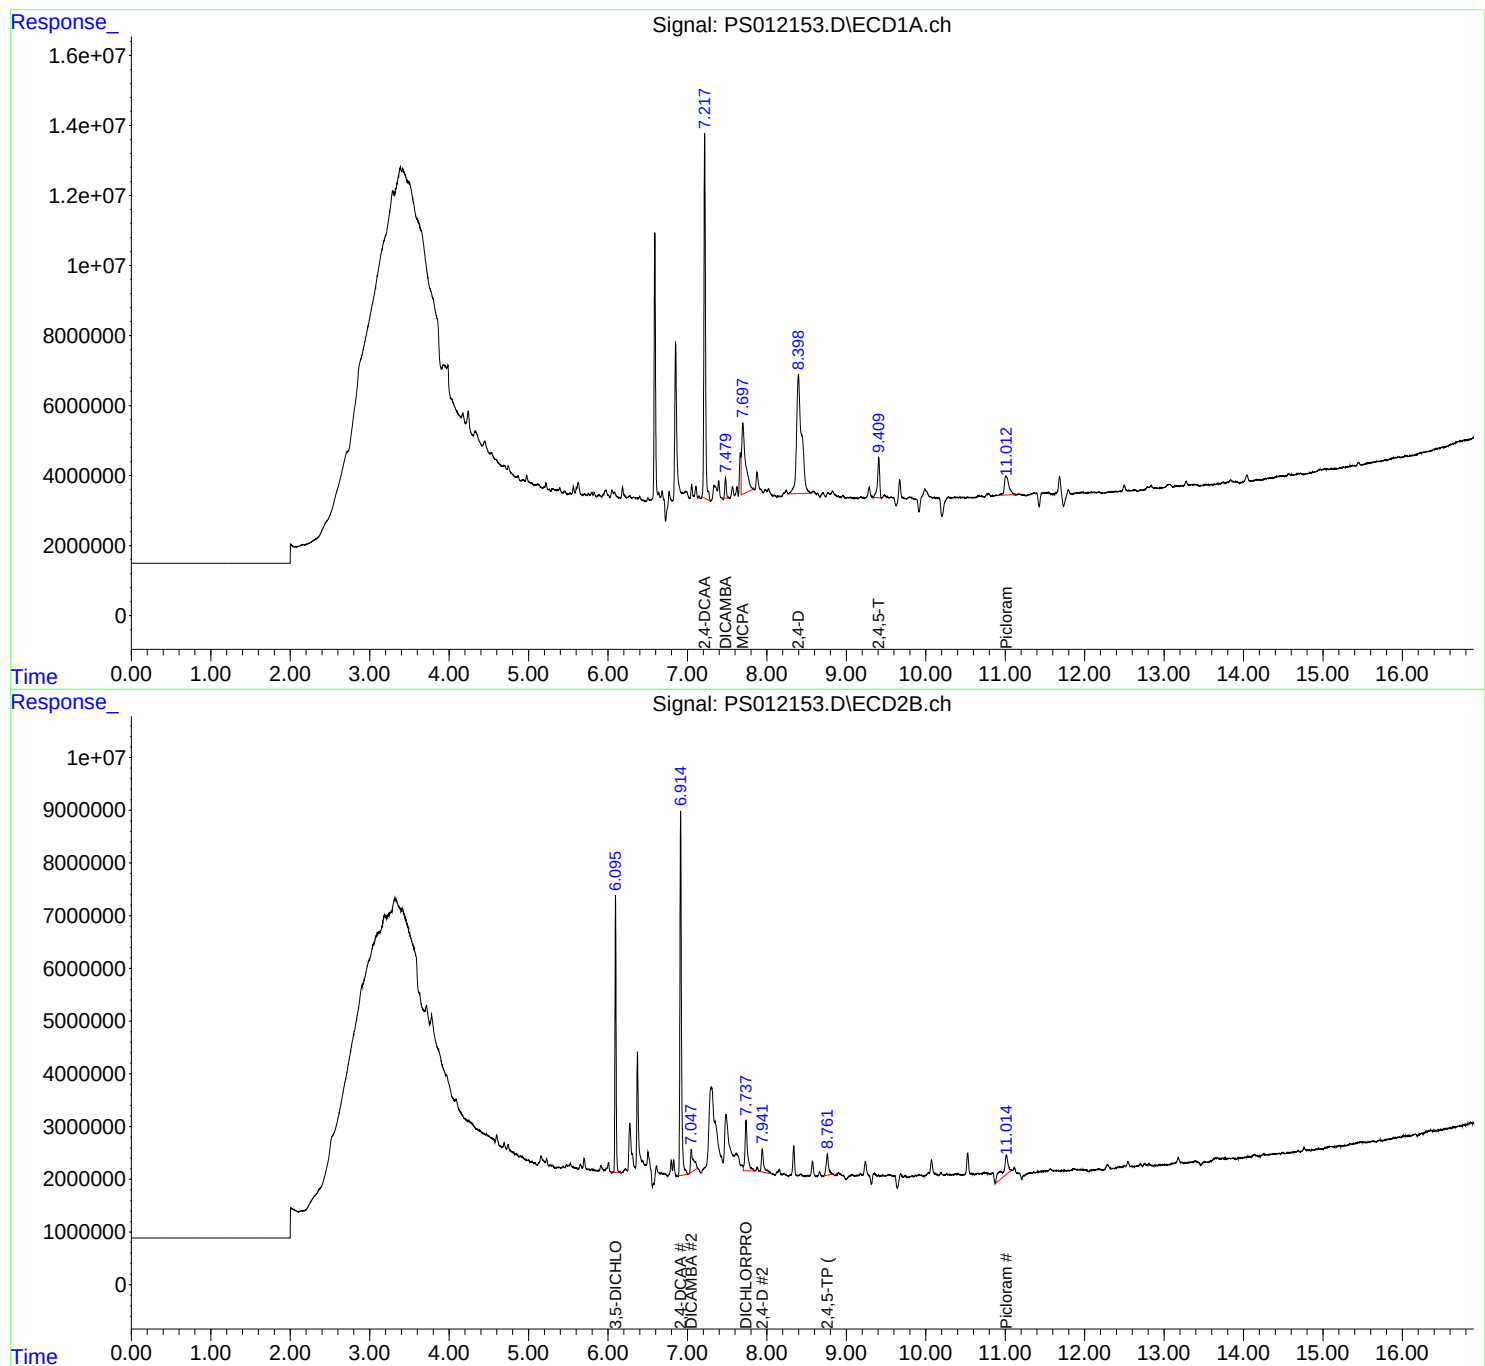


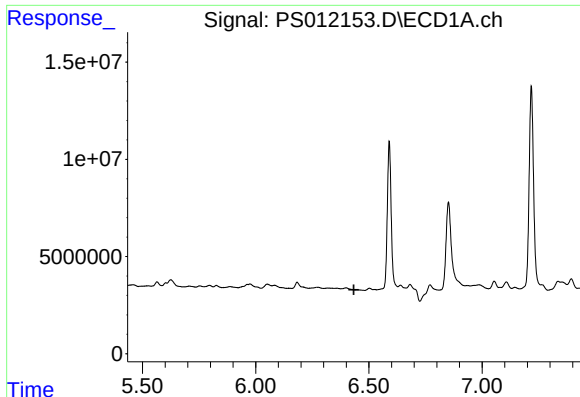

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

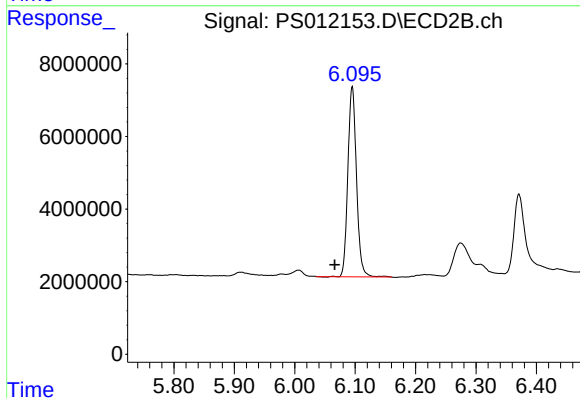


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.095 min
Delta R.T.: 0.029 min
Response: 52174765
Conc: 63.43 ng/ml

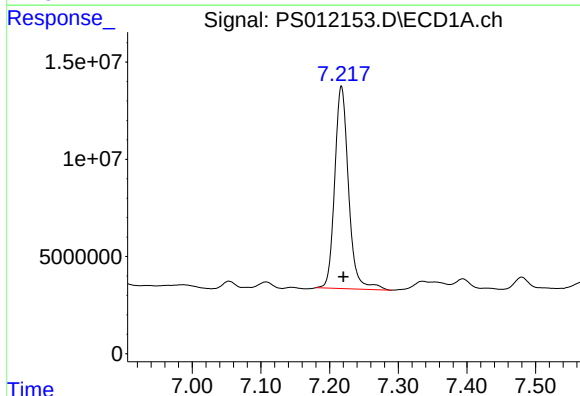


#4 2,4-DCAA

R.T.: 7.217 min
Delta R.T.: -0.003 min
Response: 145661933
Conc: 133.54 ng/ml

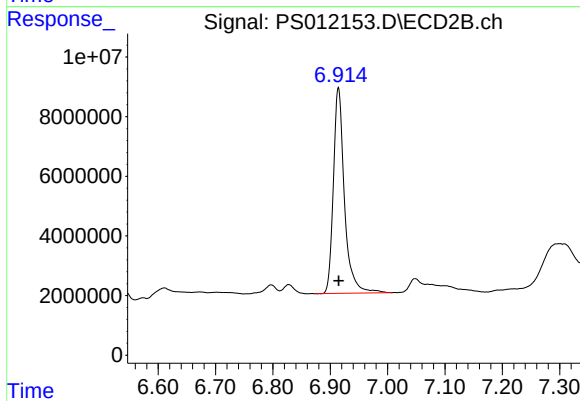

#4 2,4-DCAA


R.T.: 6.914 min
Delta R.T.: 0.000 min
Response: 93318157
Conc: 174.50 ng/ml

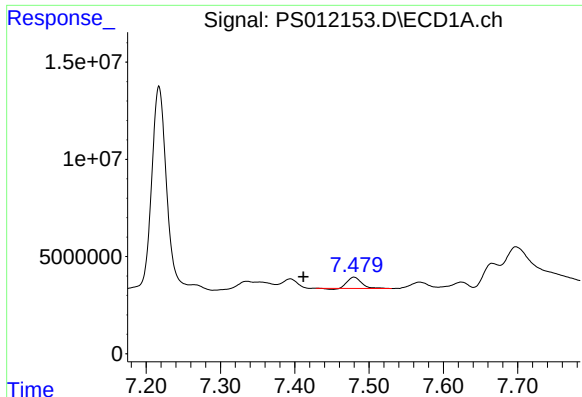

#5 DICAMBA


R.T.: 7.480 min
Delta R.T.: 0.068 min
Response: 7568756
Conc: 1.85 ng/ml

Instrument :
ECD_S
ClientSampleId :

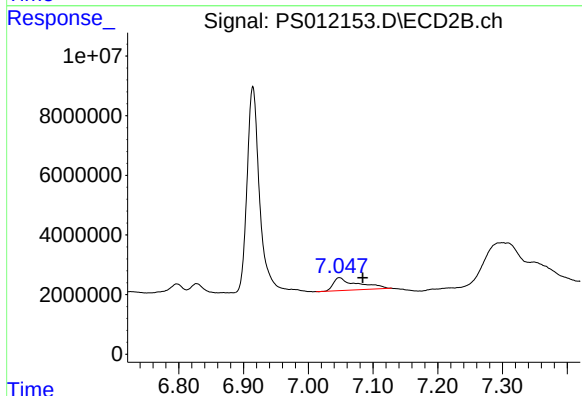


#5 DICAMBA

R.T.: 7.048 min
Delta R.T.: -0.036 min
Response: 11242846
Conc: 5.20 ng/ml

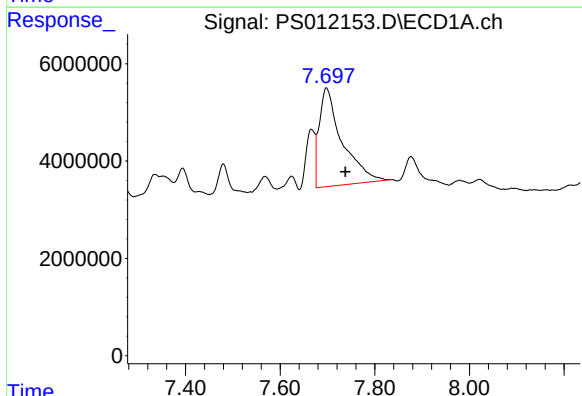


#7 MCPA

R.T.: 7.698 min
Delta R.T.: -0.041 min
Response: 67824347
Conc: 14.91 ug/ml

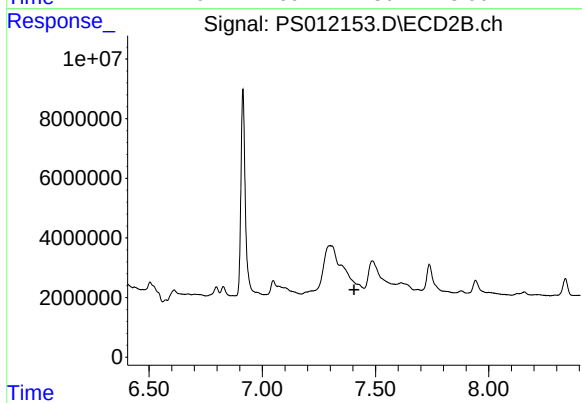

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.405 min
Response: 0
Conc: N.D.

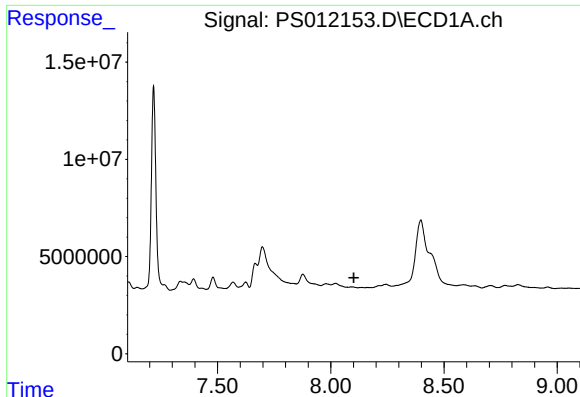

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

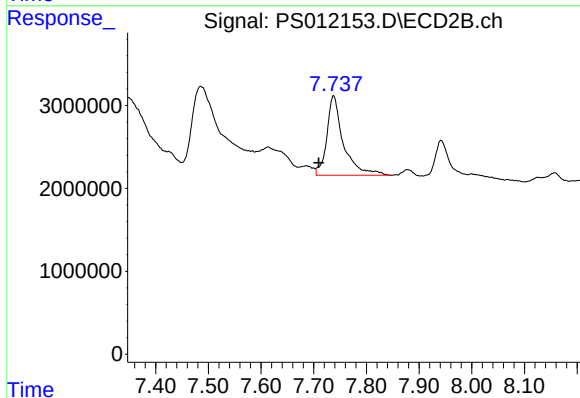


#8 DICHLORPROP

R.T.: 7.738 min
Delta R.T.: 0.028 min
Response: 20906179
Conc: 37.03 ng/ml

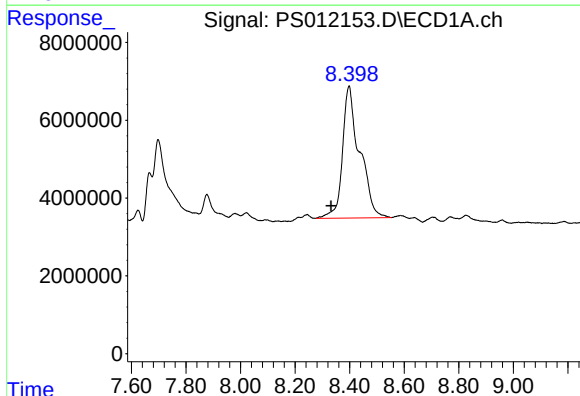


#9 2,4-D

R.T.: 8.398 min
Delta R.T.: 0.066 min
Response: 147923867
Conc: 131.01 ng/ml

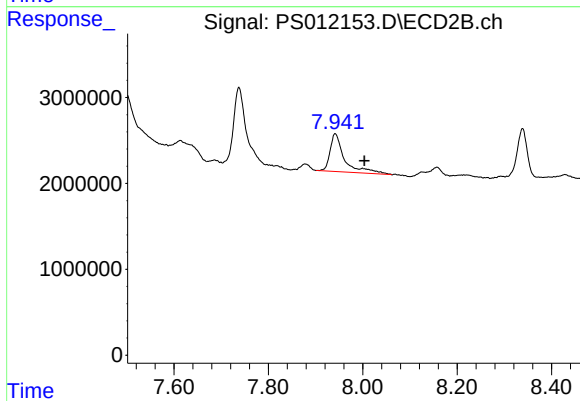

#9 2,4-D


R.T.: 7.942 min
Delta R.T.: -0.061 min
Response: 9412277
Conc: 12.81 ng/ml

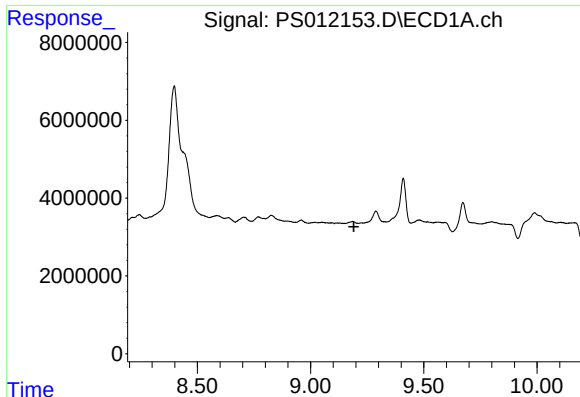

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

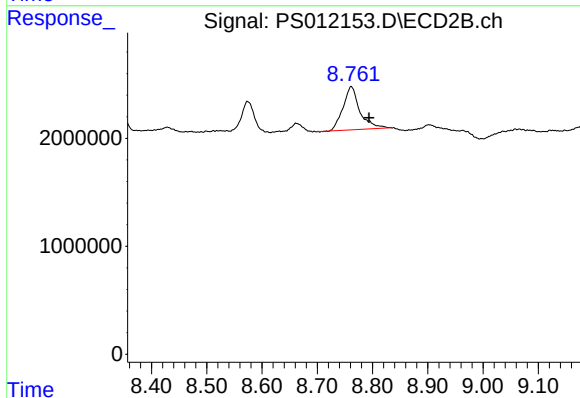


#11 2,4,5-TP (SILVEX)

R.T.: 8.762 min
Delta R.T.: -0.032 min
Response: 8487441
Conc: 2.90 ng/ml

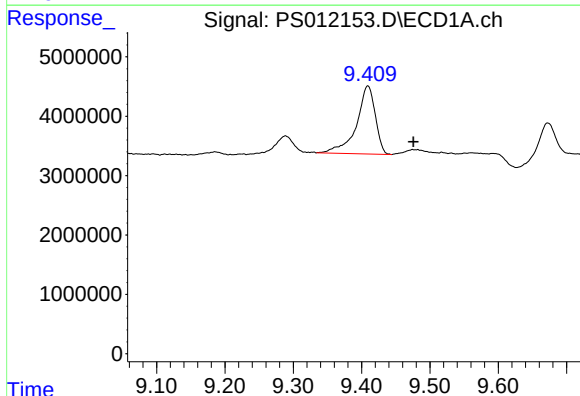


#12 2,4,5-T

R.T.: 9.409 min
Delta R.T.: -0.067 min
Response: 21942550
Conc: 3.70 ng/ml

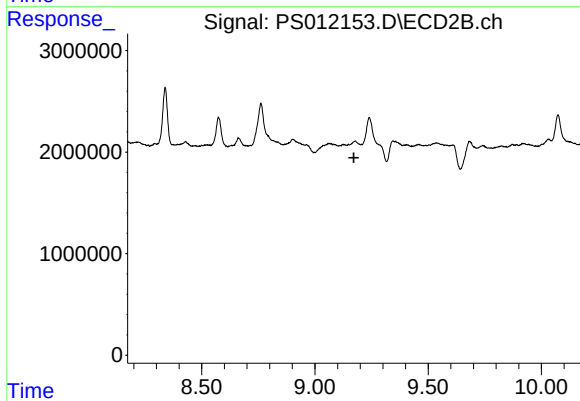

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.172 min
Response: 0
Conc: N.D.

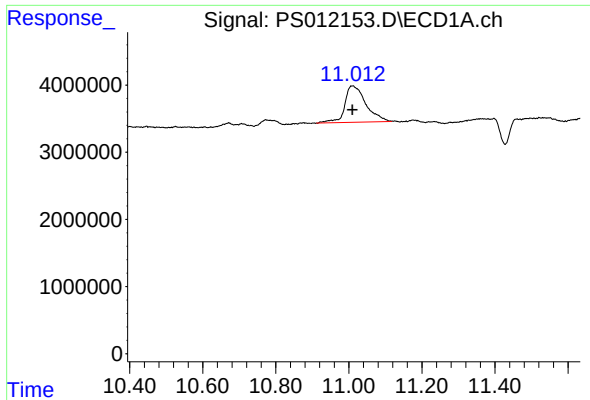

#15 Picloram

R.T.: 11.011 min
Delta R.T.: 0.002 min
Response: 21708046
Conc: 2.78 ng/ml

Instrument :
ECD_S
ClientSampleId :

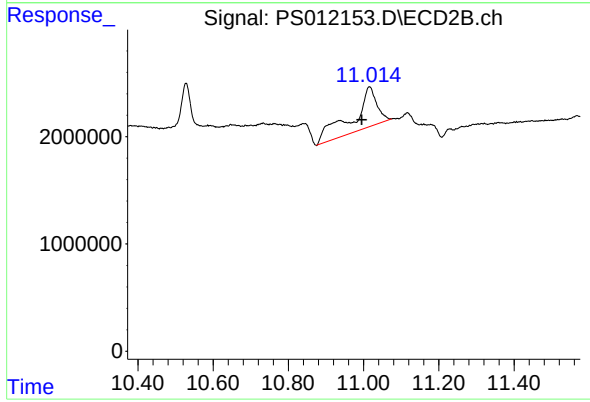

#15 Picloram

R.T.: 11.016 min
Delta R.T.: 0.021 min
Response: 17029548
Conc: 3.76 ng/ml