

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090820\
 Data File : PS012154.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Sep 2020 18:42
 Operator : DD\AJ
 Sample : L3808-11
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 02:37:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.217	6.914	244.5E6	147.1E6	224.154	275.016
Target Compounds							
2) T	3,5-DICHL...	0.000	6.095	0	32334728	N.D.	39.307
3) T	4-Nitroph...	6.985	0.000	2852500	0	4.843	N.D. #
5) T	DICAMBA	0.000	7.047	0	20693551	N.D.	9.578
6) T	MCP	7.627	0.000	10571493	0	3.309	N.D. #
7) T	MCPA	7.689	7.469	181.8E6	96990540	39.979	35.396
8) T	DICHLORPROP	0.000	7.735	0	35112957	N.D.	62.187
9) T	2,4-D	8.396	0.000	141.3E6	0	125.179	N.D. #
11) T	2,4,5-TP ...	0.000	8.761	0	21628597	N.D.	7.398
12) T	2,4,5-T	9.409	9.242	17510280	9922568	2.955	3.352



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090820\
Data File : PS012154.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2020 18:42
Operator : DD\AJ
Sample : L3808-11
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 02:37:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

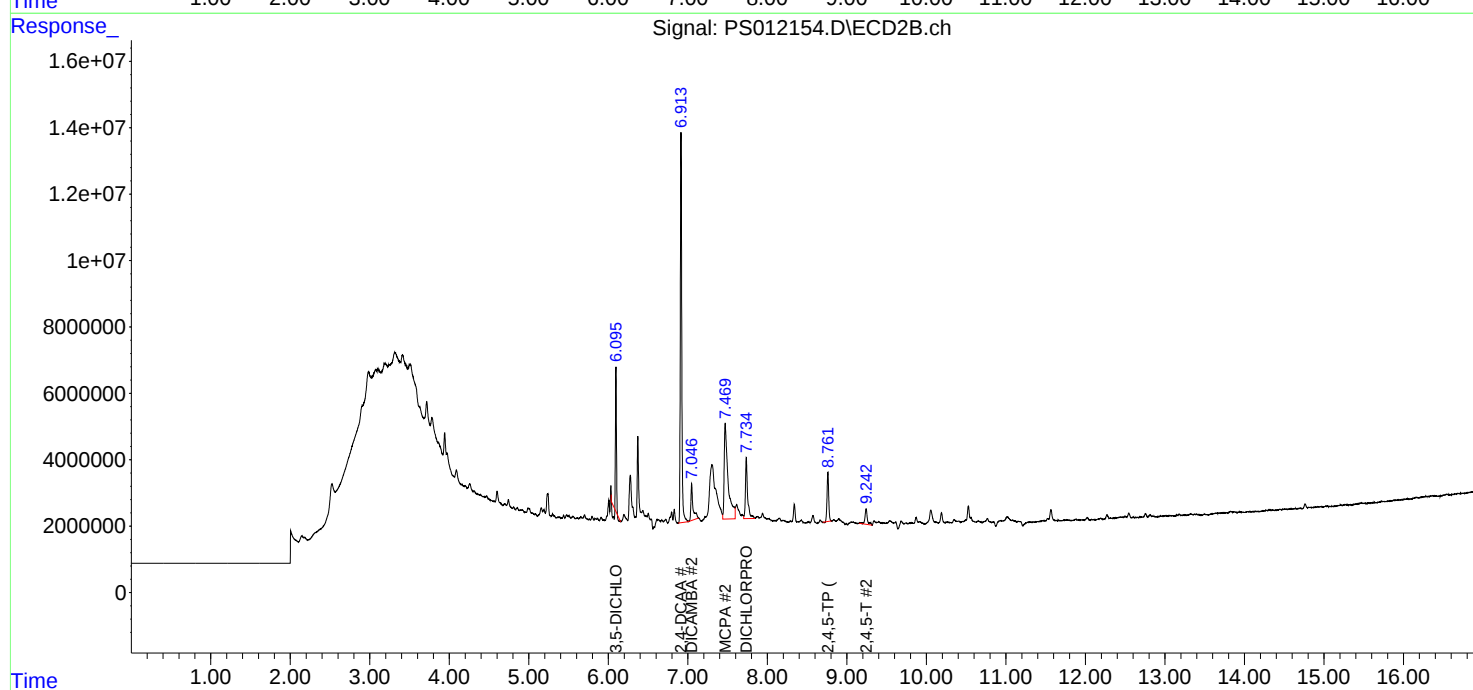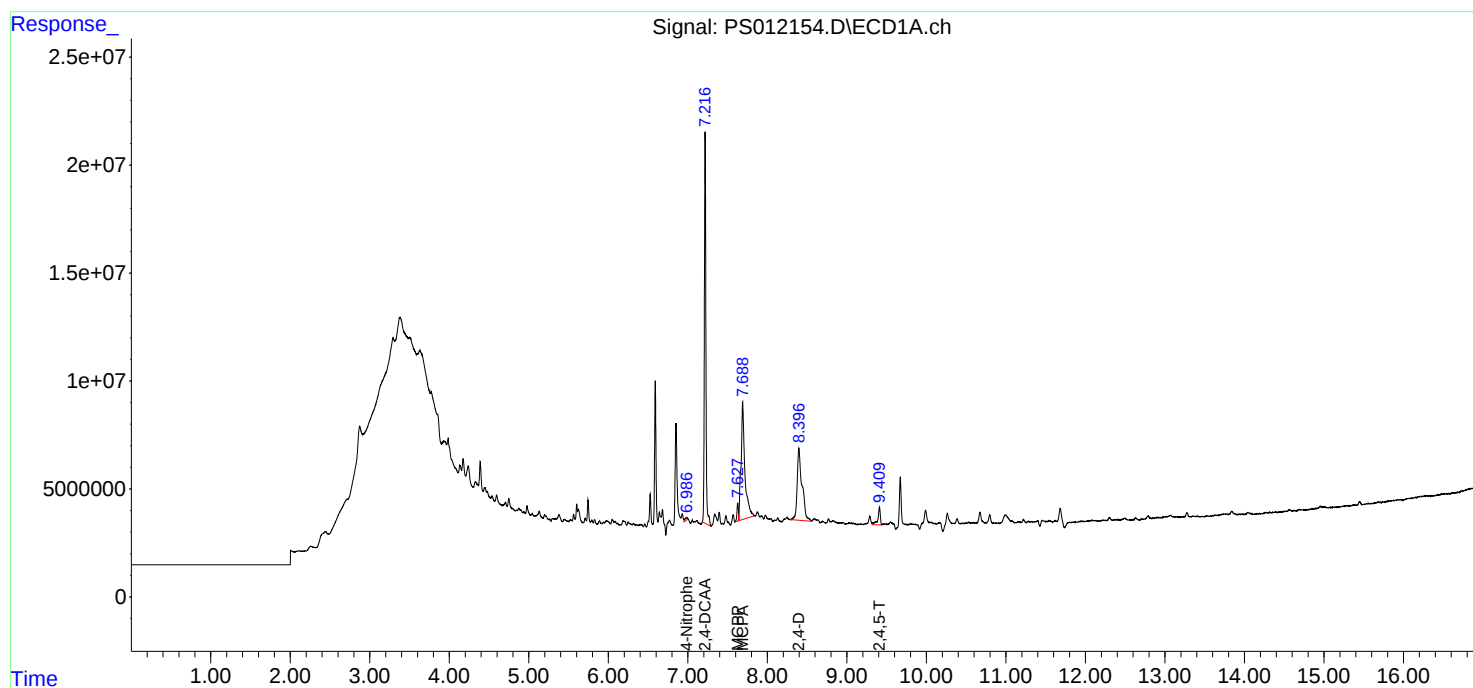


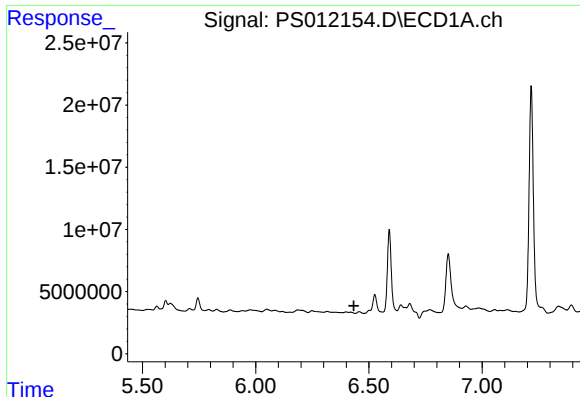

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

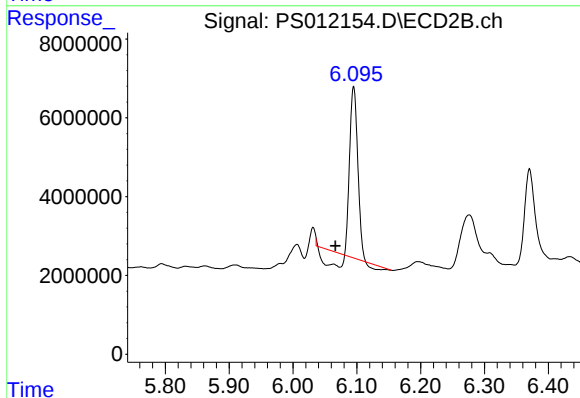


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.095 min
Delta R.T.: 0.029 min
Response: 32334728
Conc: 39.31 ng/ml

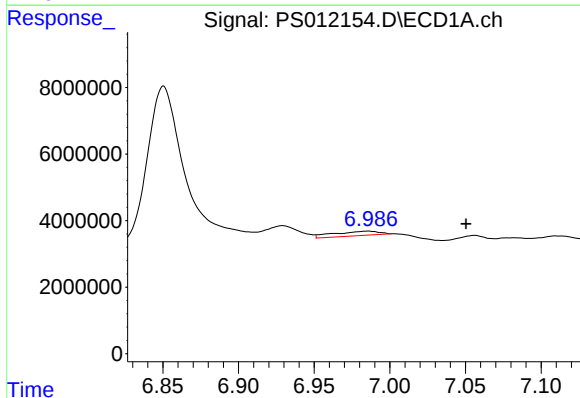


#3 4-Nitrophenol

R.T.: 6.985 min
Delta R.T.: -0.065 min
Response: 2852500
Conc: 4.84 ng/ml

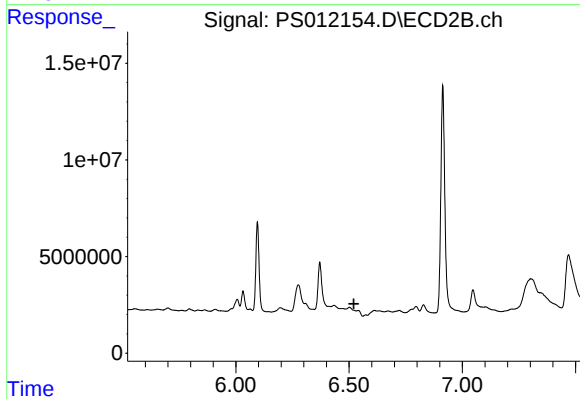

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.521 min
Response: 0
Conc: N.D.

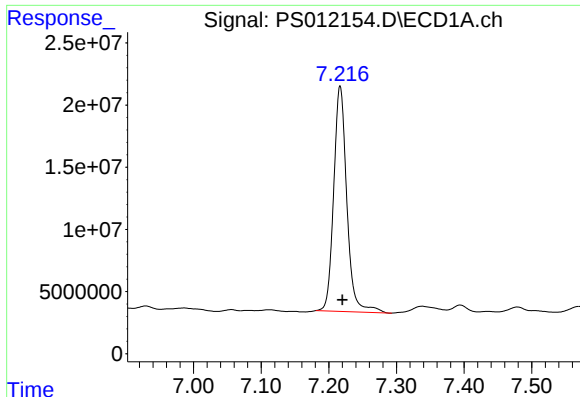

#4 2,4-DCAA


R.T.: 7.217 min
Delta R.T.: -0.003 min
Response: 244500412
Conc: 224.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

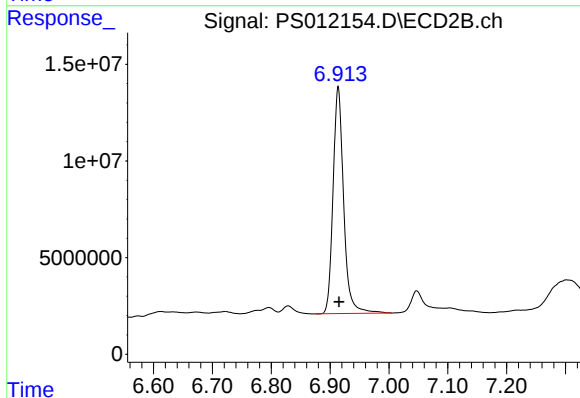


#4 2,4-DCAA

R.T.: 6.914 min
Delta R.T.: -0.001 min
Response: 147074733
Conc: 275.02 ng/ml

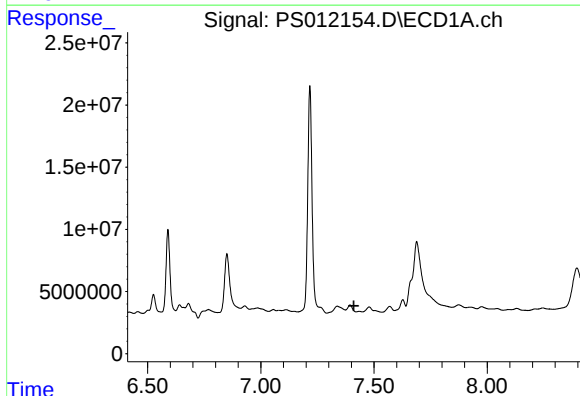


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.412 min
Response: 0
Conc: N.D.

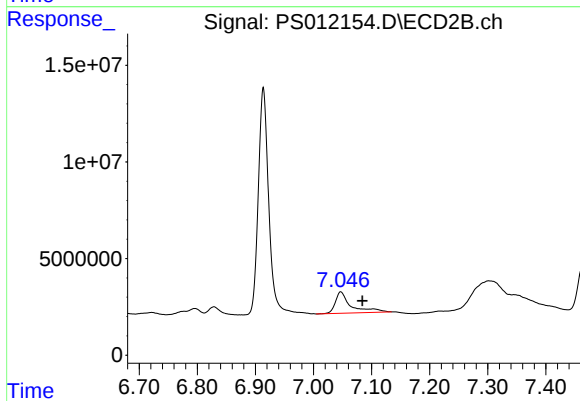

#5 DICAMBA


R.T.: 7.047 min
Delta R.T.: -0.037 min
Response: 20693551
Conc: 9.58 ng/ml

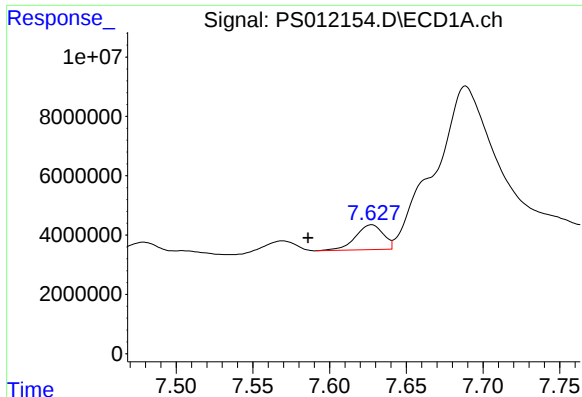

#6 MCPP


R.T.: 7.627 min
Delta R.T.: 0.041 min
Response: 10571493
Conc: 3.31 ug/ml

Instrument :
ECD_S
ClientSampleId :

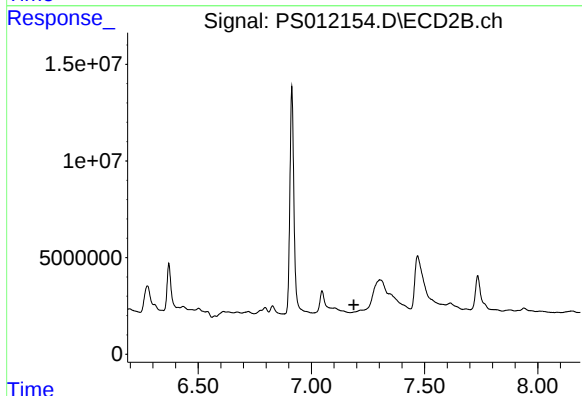


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 7.188 min
Response: 0
Conc: N.D.

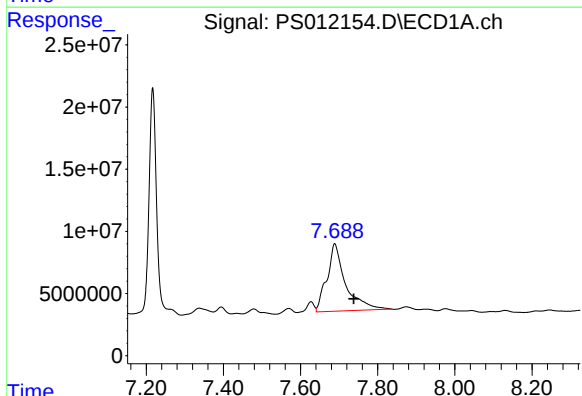


#7 MCPA

R.T.: 7.689 min
Delta R.T.: -0.049 min
Response: 181844041
Conc: 39.98 ug/ml

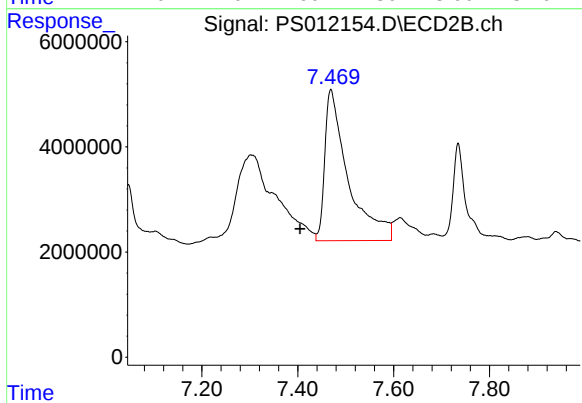

#7 MCPA


R.T.: 7.469 min
Delta R.T.: 0.064 min
Response: 96990540
Conc: 35.40 ug/ml

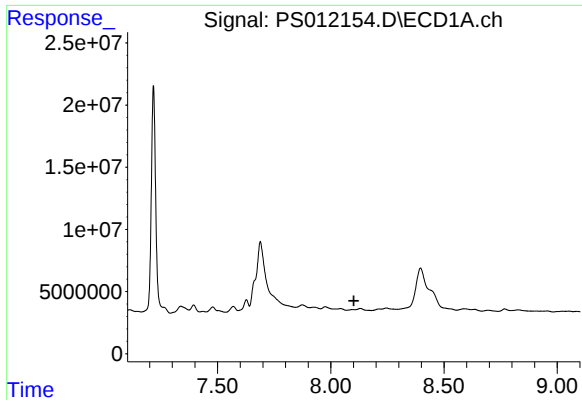

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

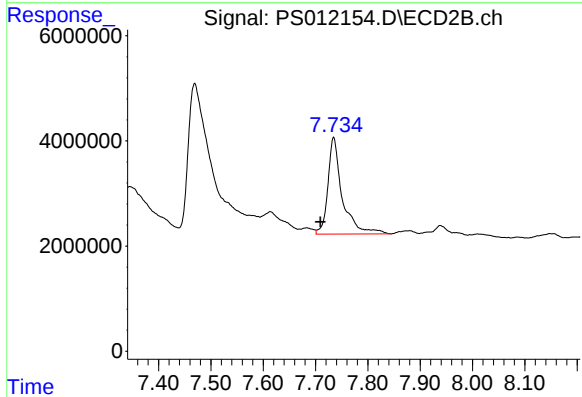


#8 DICHLORPROP

R.T.: 7.735 min
Delta R.T.: 0.025 min
Response: 35112957
Conc: 62.19 ng/ml

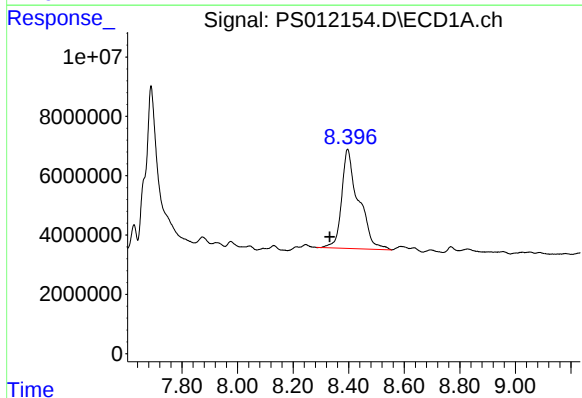


#9 2,4-D

R.T.: 8.396 min
Delta R.T.: 0.064 min
Response: 141339199
Conc: 125.18 ng/ml

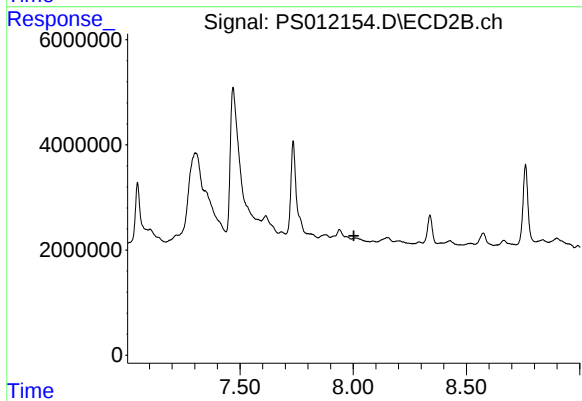

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.003 min
Response: 0
Conc: N.D.

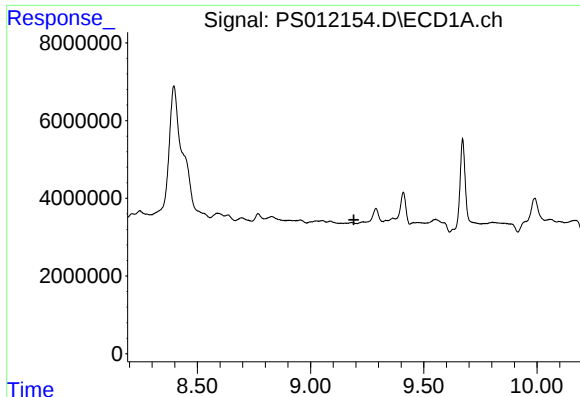

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

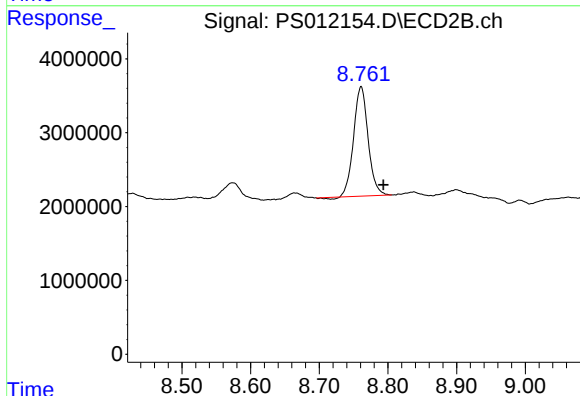


#11 2,4,5-TP (SILVEX)

R.T.: 8.761 min
Delta R.T.: -0.033 min
Response: 21628597
Conc: 7.40 ng/ml

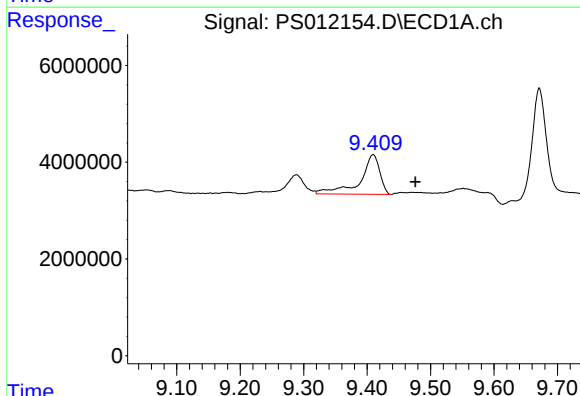

#12 2,4,5-T

R.T.: 9.409 min
Delta R.T.: -0.067 min
Response: 17510280
Conc: 2.95 ng/ml

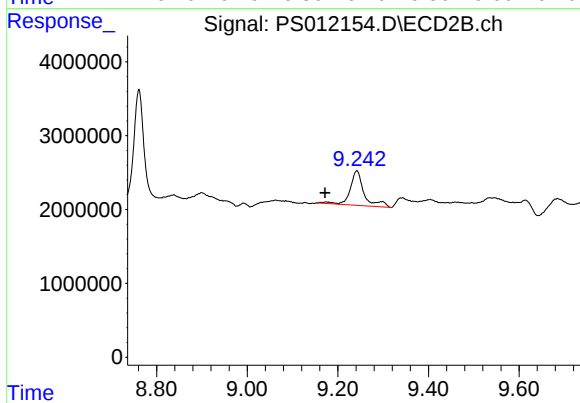

#12 2,4,5-T

R.T.: 9.242 min
Delta R.T.: 0.070 min
Response: 9922568
Conc: 3.35 ng/ml