

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090820\
 Data File : PS012156.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Sep 2020 19:28
 Operator : DD\AJ
 Sample : L3808-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 02:38:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.216	6.913	262.7E6	156.6E6	240.817	292.848
Target Compounds							
2) T	3,5-DICHL...	0.000	6.095	0	32034859	N.D.	38.942
5) T	DICAMBA	7.394	7.047	6188178	12711444	1.511	5.884 #
6) T	MCP	7.627	0.000	11676490	0	3.655	N.D. #
7) T	MCPA	7.691	7.472	176.2E6	74616367	38.738	27.231 #
8) T	DICHLORPROP	0.000	7.735	0	23856187	N.D.	42.251
9) T	2,4-D	8.396	0.000	139.8E6	0	123.857	N.D. #
11) T	2,4,5-TP ...	0.000	8.761	0	21894632	N.D.	7.489
12) T	2,4,5-T	9.409	0.000	10179714	0	1.718	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090820\
Data File : PS012156.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2020 19:28
Operator : DD\AJ
Sample : L3808-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 02:38:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

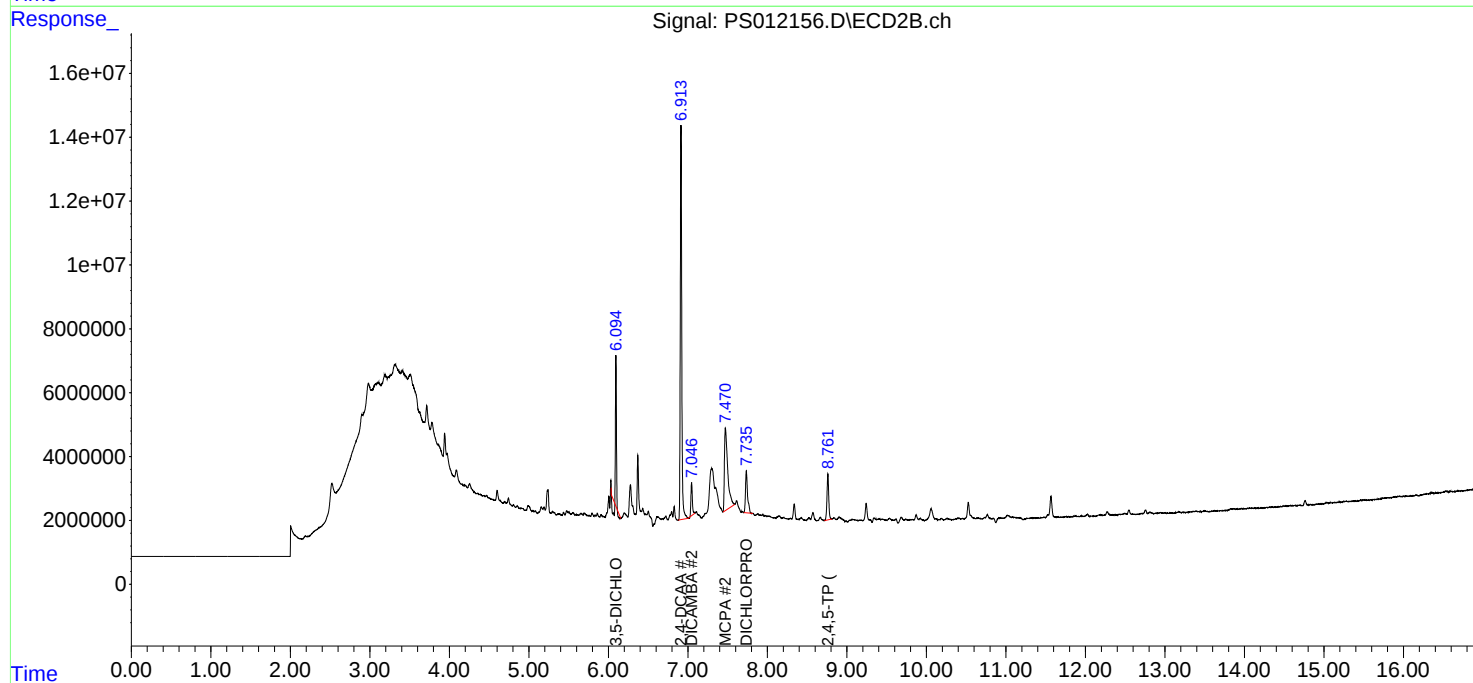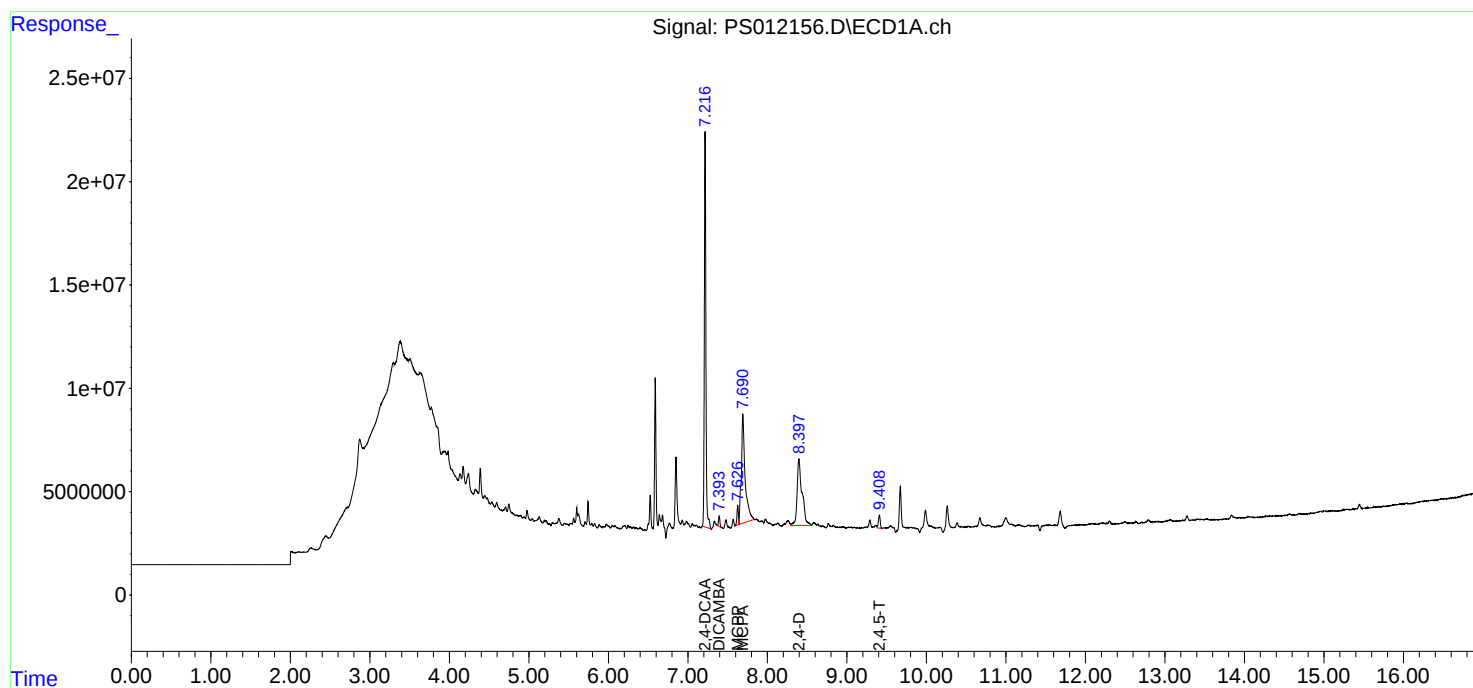


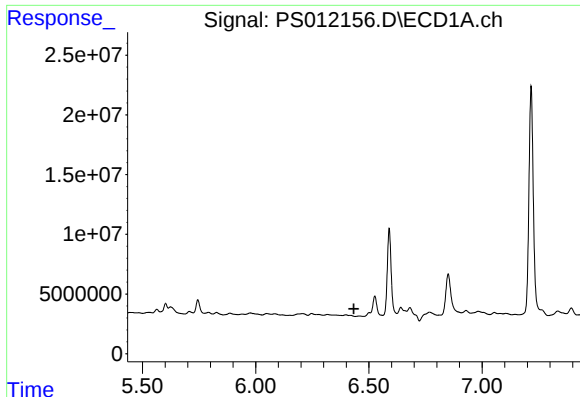

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

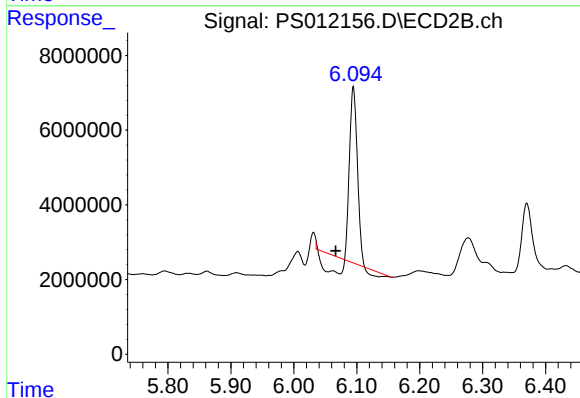


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.095 min
Delta R.T.: 0.028 min
Response: 32034859
Conc: 38.94 ng/ml

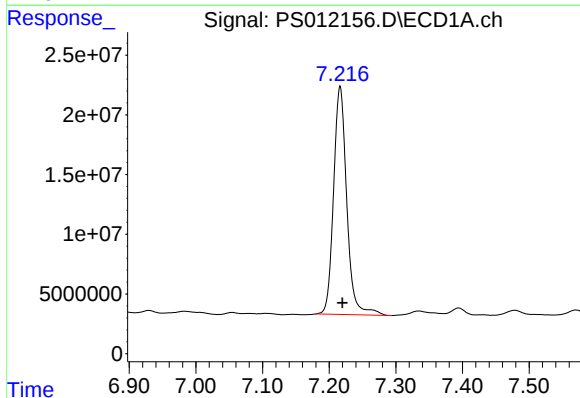


#4 2,4-DCAA

R.T.: 7.216 min
Delta R.T.: -0.004 min
Response: 262675247
Conc: 240.82 ng/ml

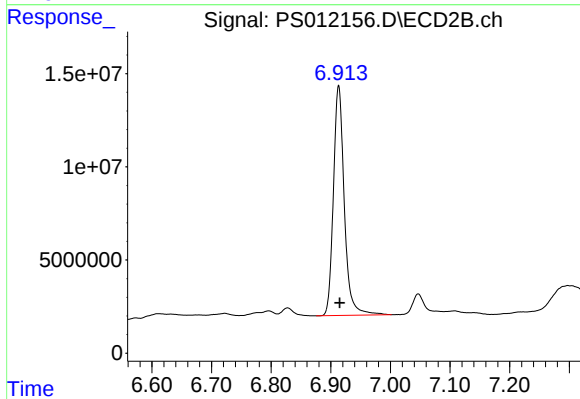

#4 2,4-DCAA


R.T.: 6.913 min
Delta R.T.: -0.002 min
Response: 156611407
Conc: 292.85 ng/ml

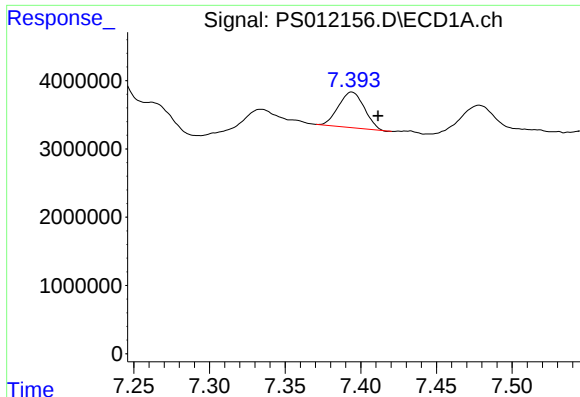

#5 DICAMBA


R.T.: 7.394 min
Delta R.T.: -0.017 min
Response: 6188178
Conc: 1.51 ng/ml

Instrument :
ECD_S
ClientSampleId :

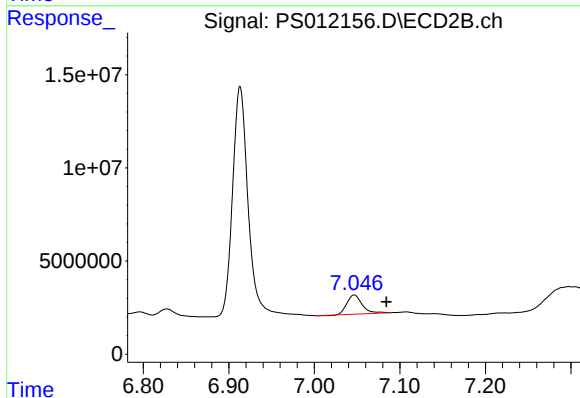


#5 DICAMBA

R.T.: 7.047 min
Delta R.T.: -0.038 min
Response: 12711444
Conc: 5.88 ng/ml

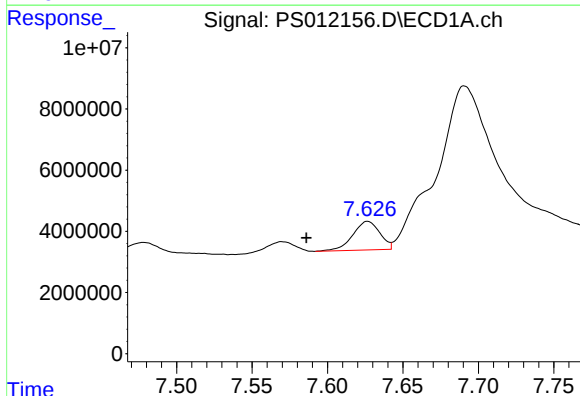


#6 MCP

R.T.: 7.627 min
Delta R.T.: 0.041 min
Response: 11676490
Conc: 3.65 ug/ml

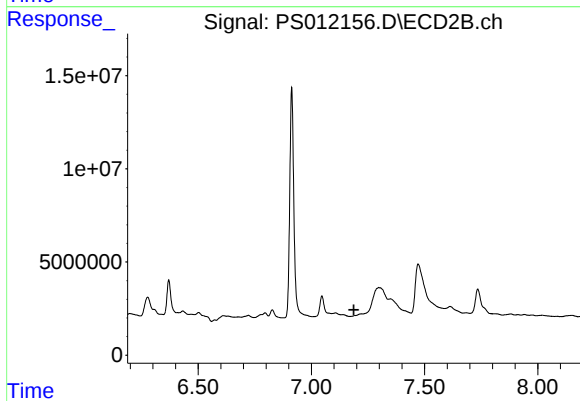

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.188 min
Response: 0
Conc: N.D.

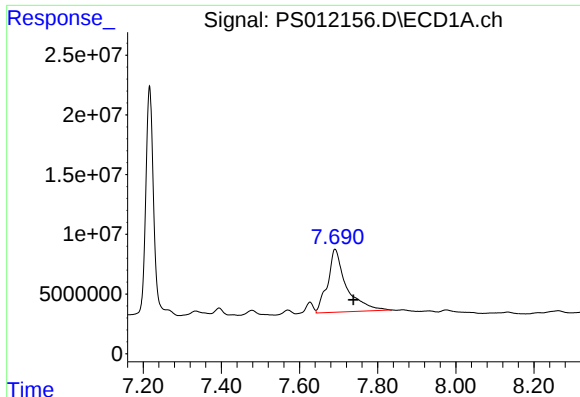

#7 MCPA


R.T.: 7.691 min
Delta R.T.: -0.047 min
Response: 176200189
Conc: 38.74 ug/ml

Instrument :
ECD_S
ClientSampleId :

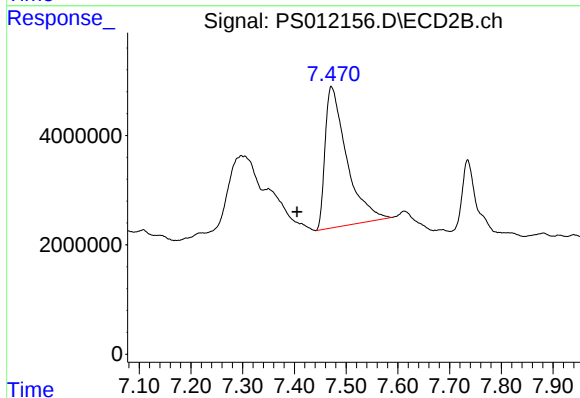


#7 MCPA

R.T.: 7.472 min
Delta R.T.: 0.067 min
Response: 74616367
Conc: 27.23 ug/ml

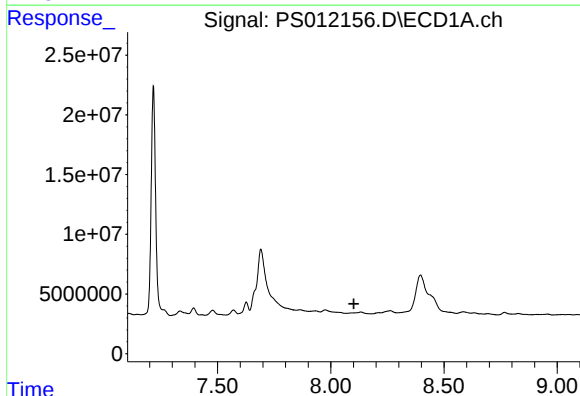


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.102 min
Response: 0
Conc: N.D.

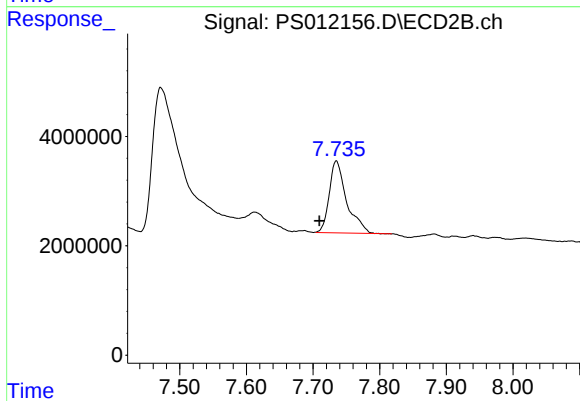

#8 DICHLORPROP


R.T.: 7.735 min
Delta R.T.: 0.026 min
Response: 23856187
Conc: 42.25 ng/ml

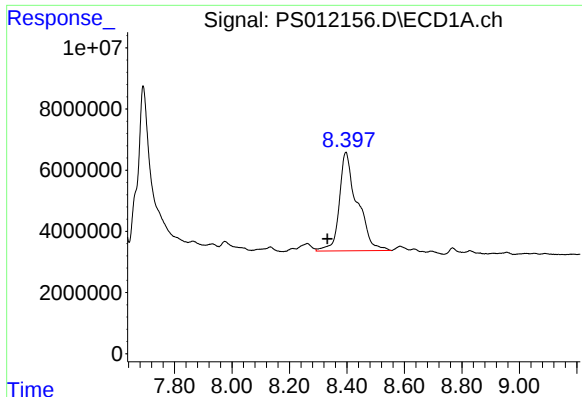

#9 2,4-D


R.T.: 8.396 min
Delta R.T.: 0.064 min
Response: 139845860
Conc: 123.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

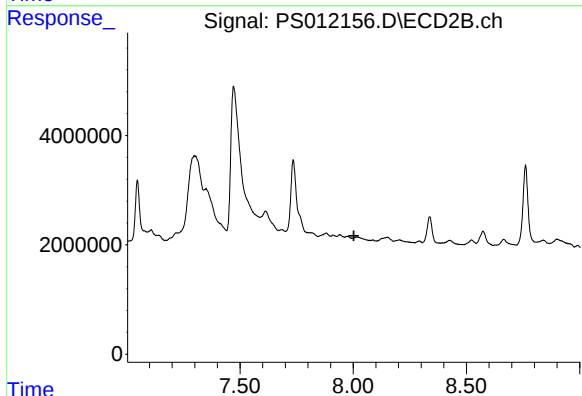


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.003 min
Response: 0
Conc: N.D.

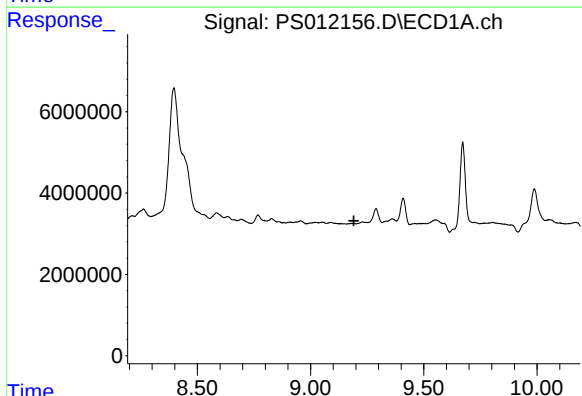


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.191 min
Response: 0
Conc: N.D.

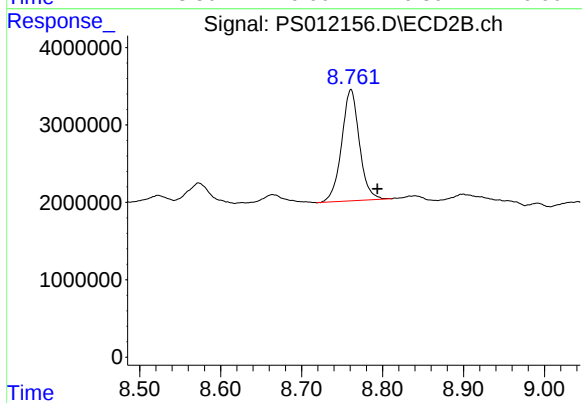

#11 2,4,5-TP (SILVEX)


R.T.: 8.761 min
Delta R.T.: -0.033 min
Response: 21894632
Conc: 7.49 ng/ml

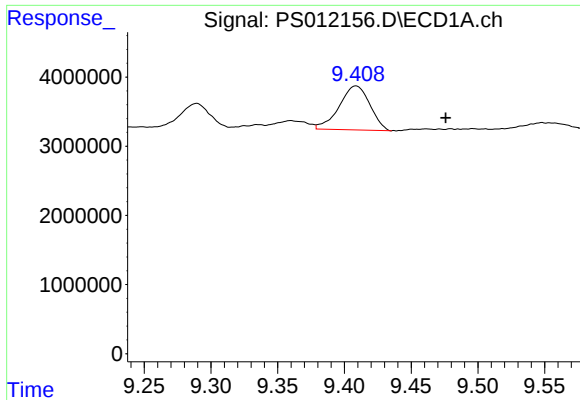

#12 2,4,5-T

R.T.: 9.409 min
Delta R.T.: -0.067 min
Response: 10179714
Conc: 1.72 ng/ml

Instrument :
ECD_S
ClientSampleId :

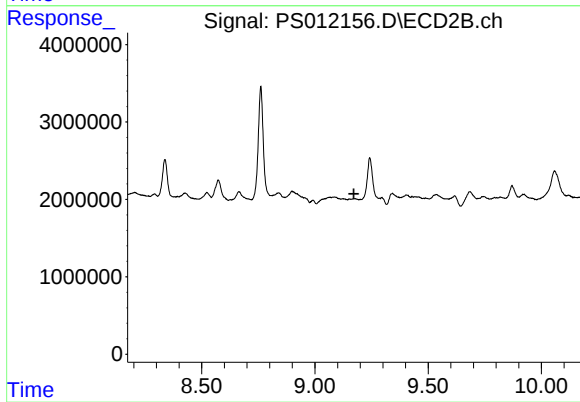

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.172 min
Response: 0
Conc: N.D.