

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090820\
 Data File : PS012157.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Sep 2020 19:51
 Operator : DD\AJ
 Sample : L3864-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 02:38:19 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.217	6.914	168.9E6	105.6E6	154.849	197.522 #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.095	0	59246381	N.D.	72.022
3) T	4-Nitroph...	7.054	0.000	3270050	0	5.551	N.D. #
5) T	DICAMBA	7.394	7.047	5849698	5055458	1.428	2.340 #
7) T	MCPA	7.697	0.000	143.4E6	0	31.528	N.D. #
8) T	DICHLORPROP	0.000	7.738	0	11452524	N.D.	20.283
9) T	2,4-D	8.397	0.000	134.8E6	0	119.399	N.D. #
11) T	2,4,5-TP ...	0.000	8.761	0	8061082	N.D.	2.757
12) T	2,4,5-T	9.410	0.000	21303902	0	3.595	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090820\
Data File : PS012157.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2020 19:51
Operator : DD\AJ
Sample : L3864-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 02:38:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

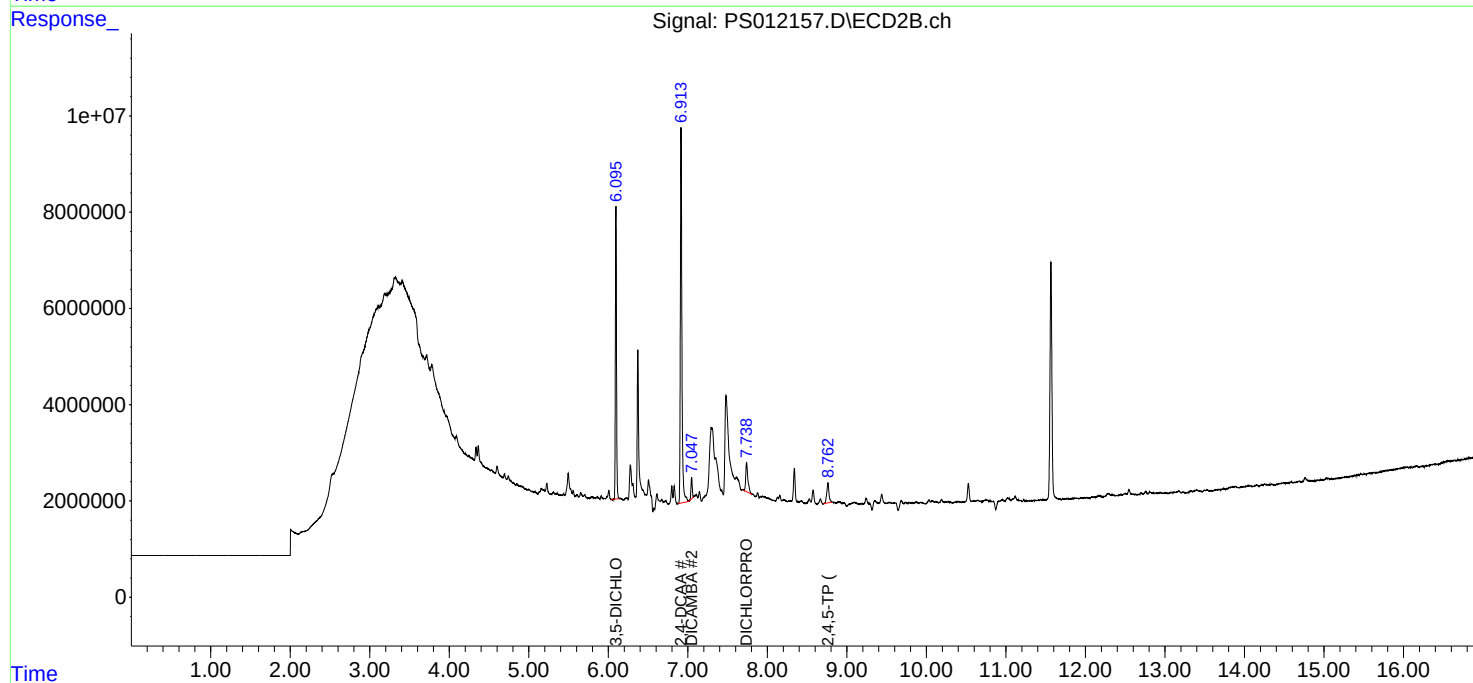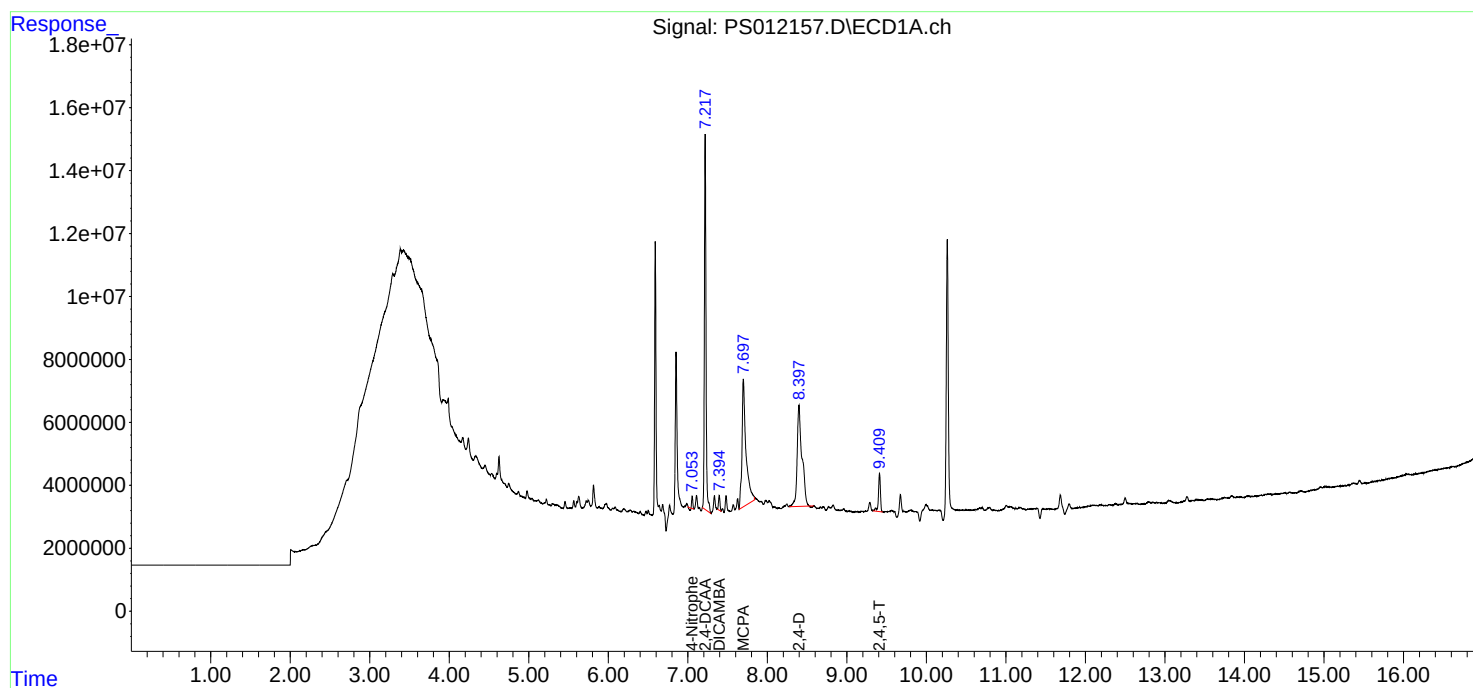


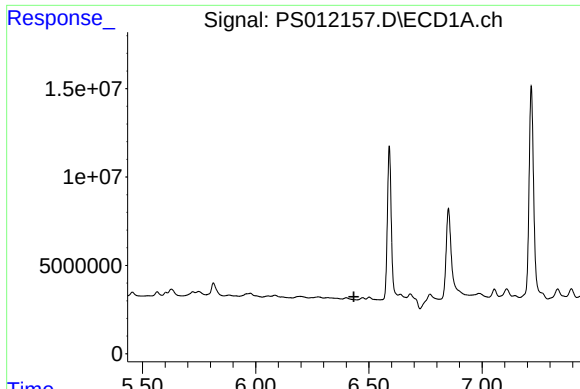

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

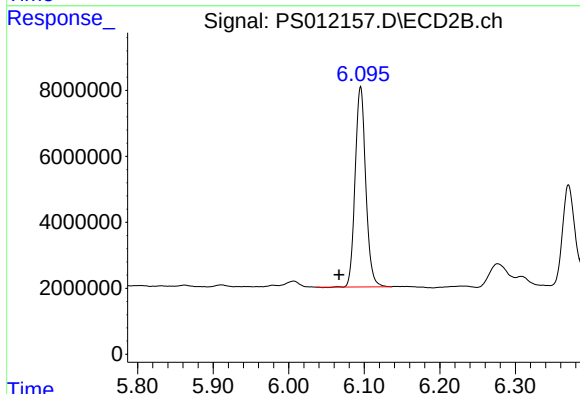


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.095 min
Delta R.T.: 0.029 min
Response: 59246381
Conc: 72.02 ng/ml

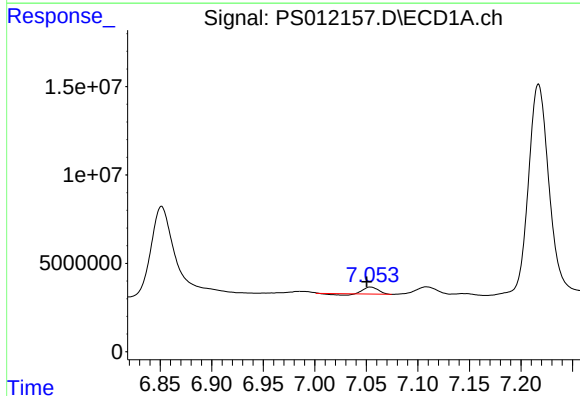


#3 4-Nitrophenol

R.T.: 7.054 min
Delta R.T.: 0.004 min
Response: 3270050
Conc: 5.55 ng/ml

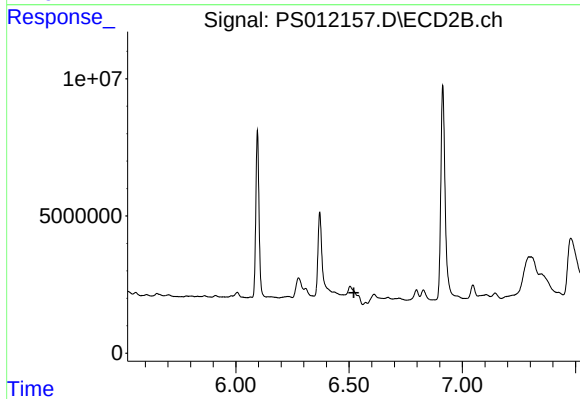

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.521 min
Response: 0
Conc: N.D.

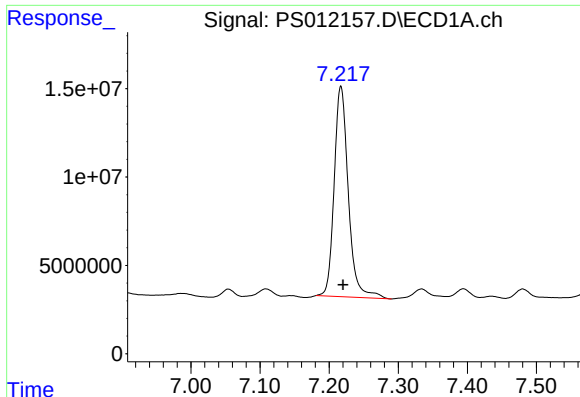

#4 2,4-DCAA


R.T.: 7.217 min
Delta R.T.: -0.003 min
Response: 168903920
Conc: 154.85 ng/ml

Instrument :
ECD_S
ClientSampleId :

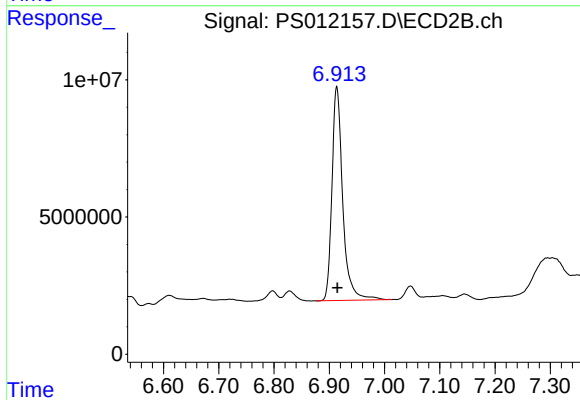


#4 2,4-DCAA

R.T.: 6.914 min
Delta R.T.: -0.001 min
Response: 105631939
Conc: 197.52 ng/ml

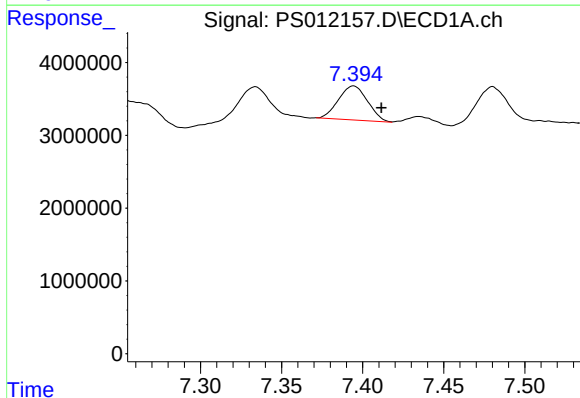


#5 DICAMBA

R.T.: 7.394 min
Delta R.T.: -0.017 min
Response: 5849698
Conc: 1.43 ng/ml

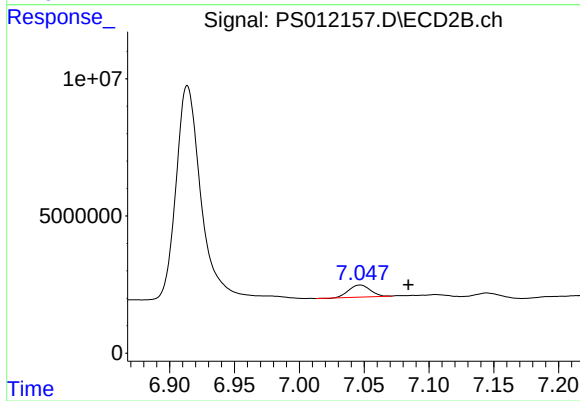

#5 DICAMBA


R.T.: 7.047 min
Delta R.T.: -0.037 min
Response: 5055458
Conc: 2.34 ng/ml

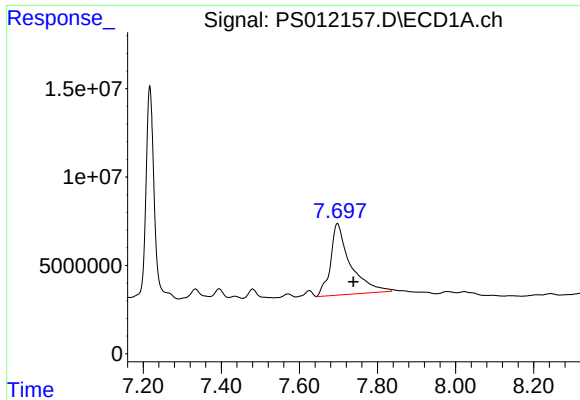

#7 MCPA


R.T.: 7.697 min
Delta R.T.: -0.041 min
Response: 143402850
Conc: 31.53 ug/ml

Instrument :
ECD_S
ClientSampleId :

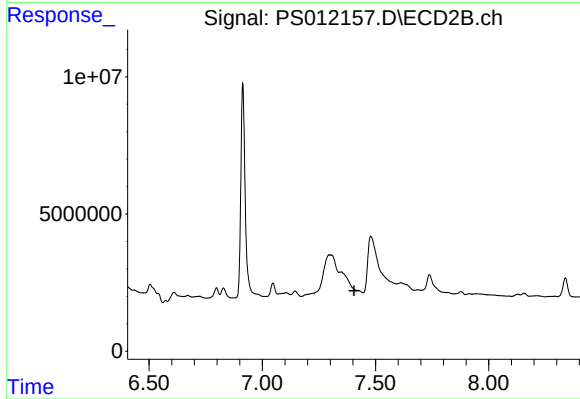


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.405 min
Response: 0
Conc: N.D.

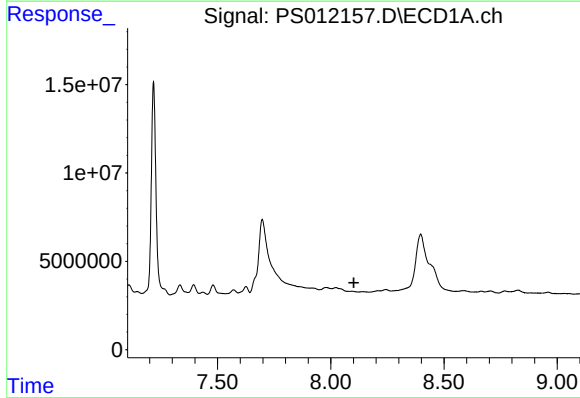


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.102 min
Response: 0
Conc: N.D.

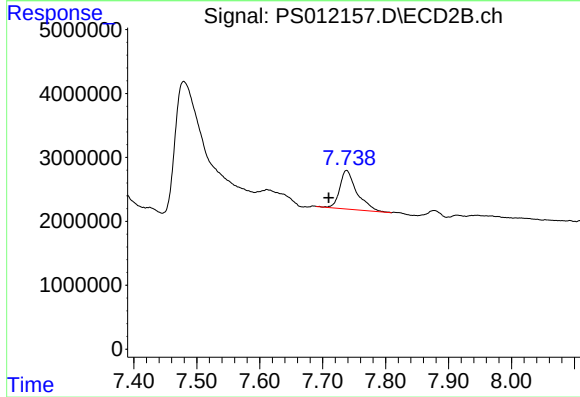

#8 DICHLORPROP


R.T.: 7.738 min
Delta R.T.: 0.029 min
Response: 11452524
Conc: 20.28 ng/ml

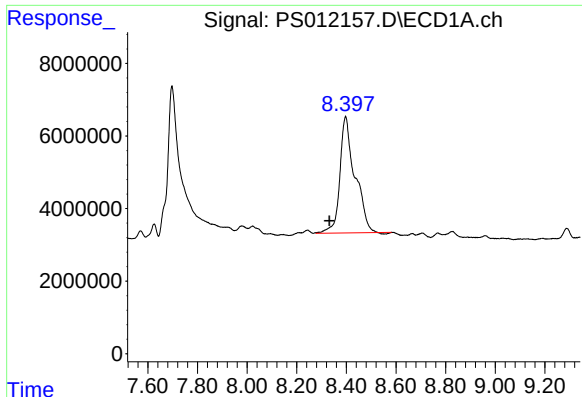

#9 2,4-D


R.T.: 8.397 min
Delta R.T.: 0.065 min
Response: 134812256
Conc: 119.40 ng/ml

Instrument :
ECD_S
ClientSampleId :

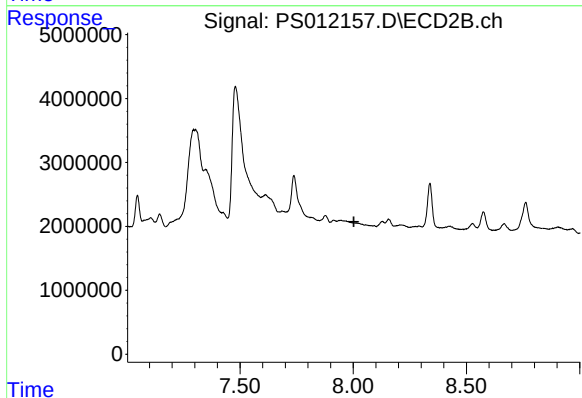


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.003 min
Response: 0
Conc: N.D.

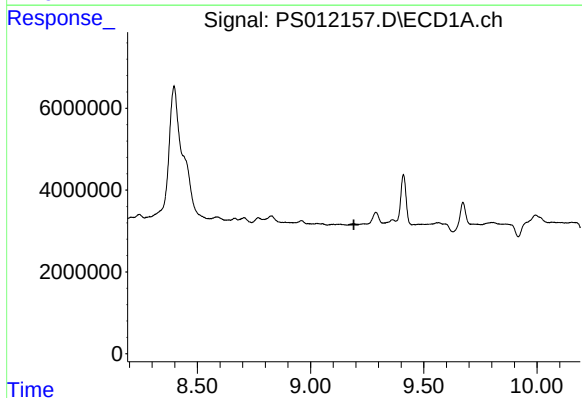


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.191 min
Response: 0
Conc: N.D.

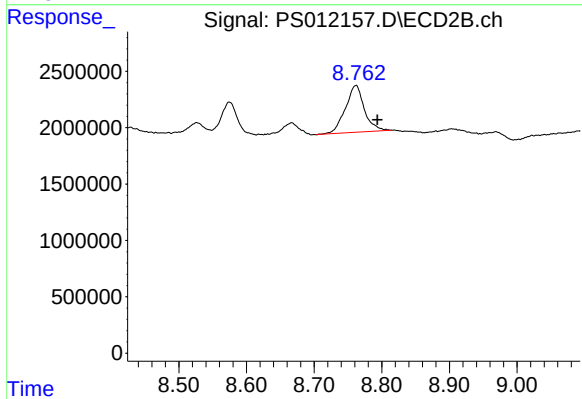

#11 2,4,5-TP (SILVEX)


R.T.: 8.761 min
Delta R.T.: -0.032 min
Response: 8061082
Conc: 2.76 ng/ml

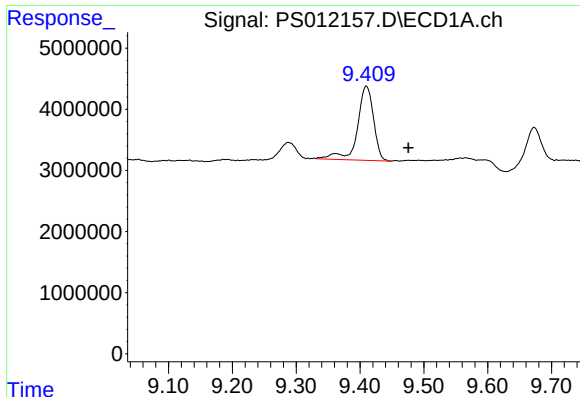

#12 2,4,5-T

R.T.: 9.410 min
Delta R.T.: -0.066 min
Response: 21303902
Conc: 3.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

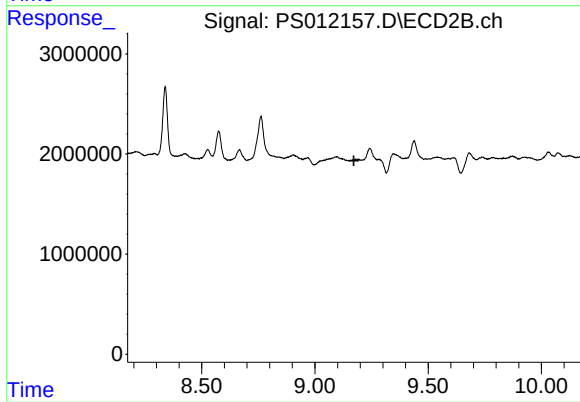

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.172 min
Response: 0
Conc: N.D.