

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090820\
 Data File : PS012160.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Sep 2020 21:00
 Operator : DD\AJ
 Sample : L3872-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 02:39:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.216	6.913	219.2E6	131.6E6	200.920	246.163
Target Compounds							
2) T	3,5-DICHL...	6.455	6.095	7621682	53734443	5.257	65.321 #
3) T	4-Nitroph...	6.985	0.000	3941771	0	6.692	N.D. #
5) T	DICAMBA	7.394	7.047	6248812	10054131	1.526	4.654 #
6) T	MCP	7.626	0.000	7655766	0	2.396	N.D. #
7) T	MCPA	7.684	7.463	341.3E6	211.9E6	75.045	77.346
8) T	DICHLORPROP	0.000	7.733	0	36557916	N.D.	64.746
9) T	2,4-D	8.396	0.000	137.9E6	0	122.146	N.D. #
11) T	2,4,5-TP ...	0.000	8.780	0	266.9E6	N.D.	91.274
12) T	2,4,5-T	9.409	0.000	15251612	0	2.574	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090820\
Data File : PS012160.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2020 21:00
Operator : DD\AJ
Sample : L3872-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 02:39:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

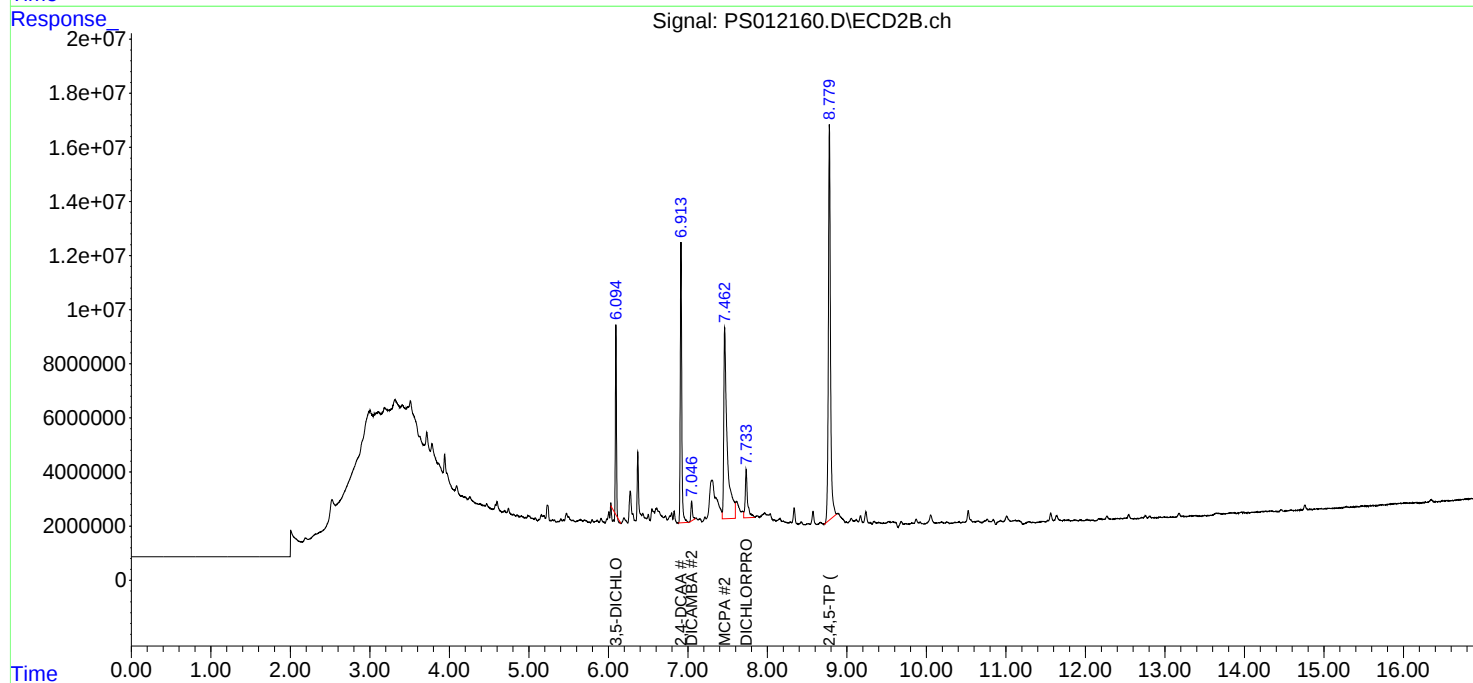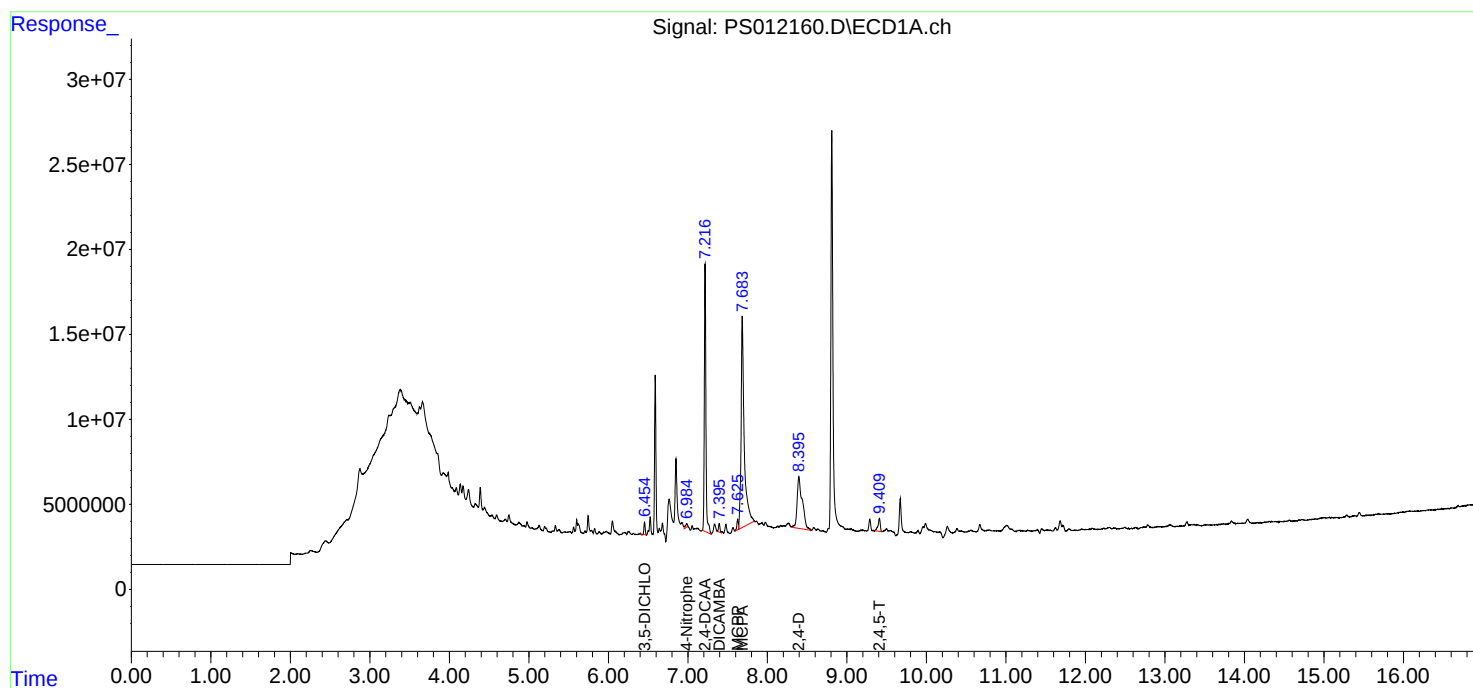


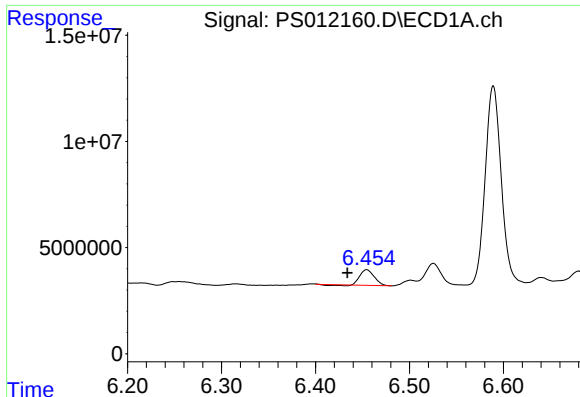

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.455 min
Delta R.T.: 0.021 min
Response: 7621682
Conc: 5.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

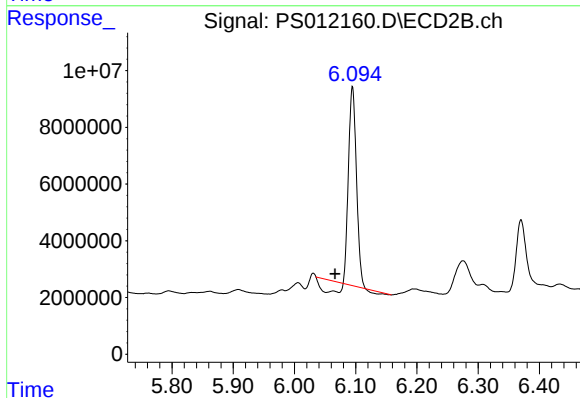


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.095 min
Delta R.T.: 0.028 min
Response: 53734443
Conc: 65.32 ng/ml

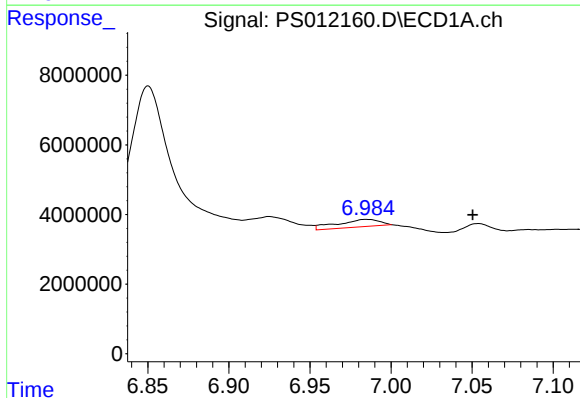


#3 4-Nitrophenol

R.T.: 6.985 min
Delta R.T.: -0.065 min
Response: 3941771
Conc: 6.69 ng/ml

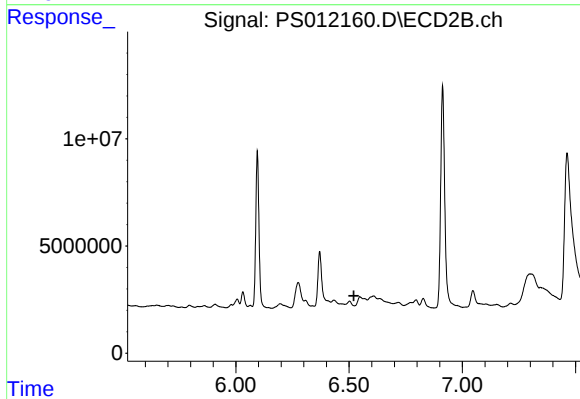

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.521 min
Response: 0
Conc: N.D.

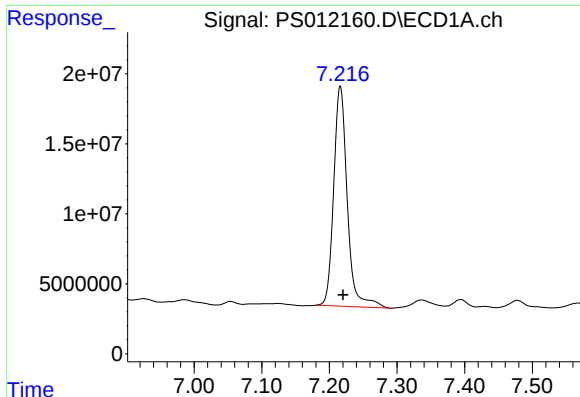

#4 2,4-DCAA


R.T.: 7.216 min
Delta R.T.: -0.004 min
Response: 219157463
Conc: 200.92 ng/ml

Instrument :
ECD_S
ClientSampleId :

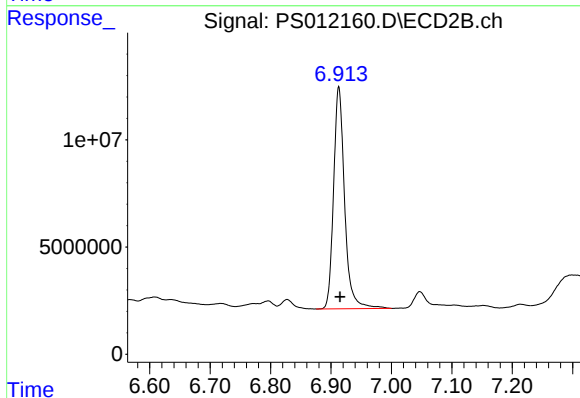


#4 2,4-DCAA

R.T.: 6.913 min
Delta R.T.: -0.002 min
Response: 131644886
Conc: 246.16 ng/ml

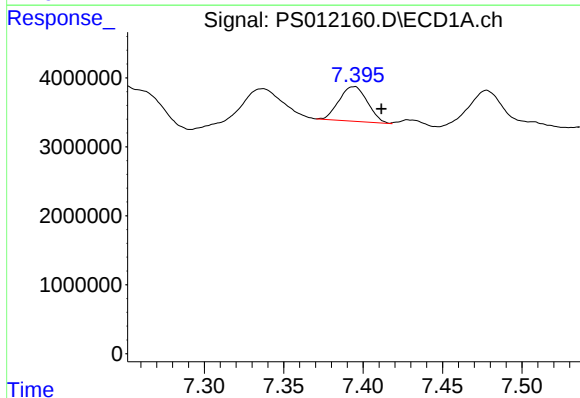


#5 DICAMBA

R.T.: 7.394 min
Delta R.T.: -0.018 min
Response: 6248812
Conc: 1.53 ng/ml

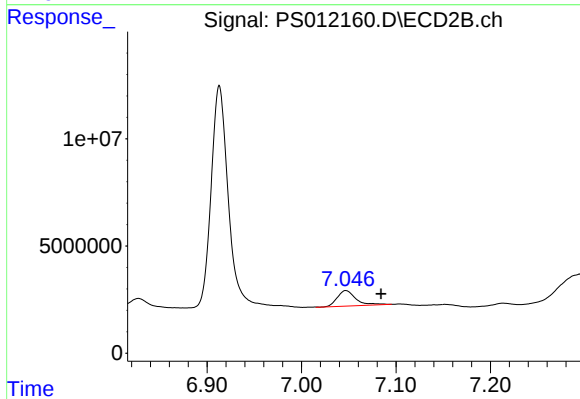

#5 DICAMBA


R.T.: 7.047 min
Delta R.T.: -0.037 min
Response: 10054131
Conc: 4.65 ng/ml

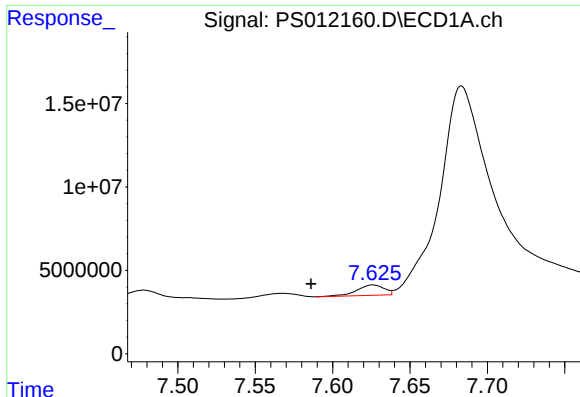

#6 MCPP


R.T.: 7.626 min
Delta R.T.: 0.040 min
Response: 7655766
Conc: 2.40 ug/ml

Instrument :
ECD_S
ClientSampleId :

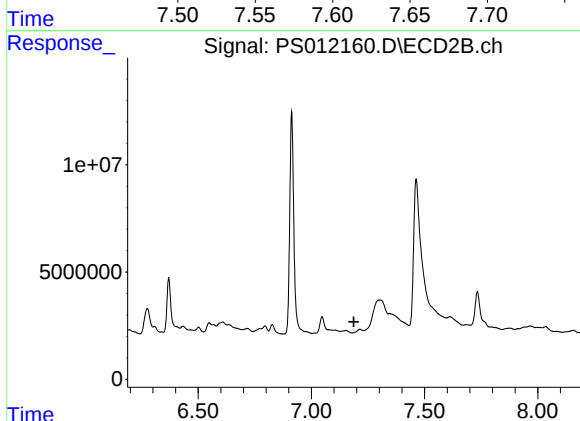


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

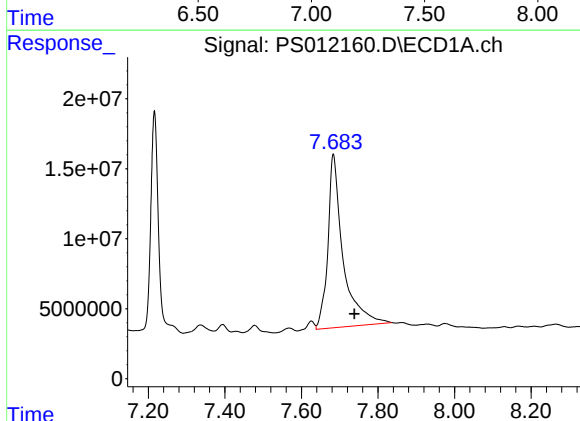


#7 MCPA

R.T.: 7.684 min
Delta R.T.: -0.055 min
Response: 341339358
Conc: 75.04 ug/ml

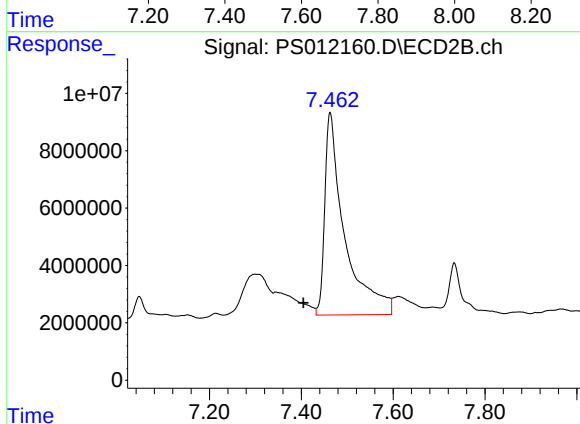

#7 MCPA


R.T.: 7.463 min
Delta R.T.: 0.058 min
Response: 211940257
Conc: 77.35 ug/ml

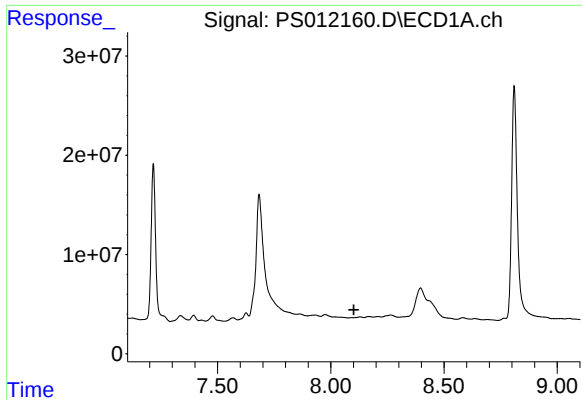

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

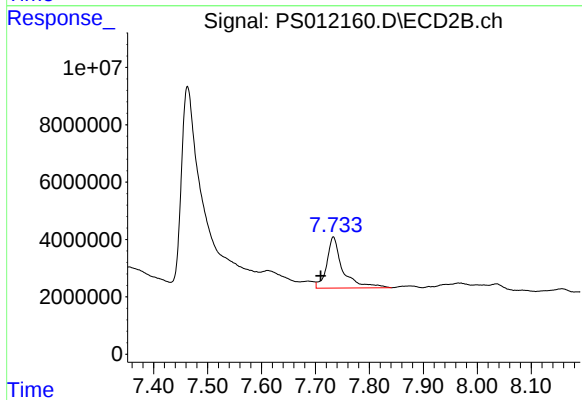


#8 DICHLORPROP

R.T.: 7.733 min
Delta R.T.: 0.024 min
Response: 36557916
Conc: 64.75 ng/ml

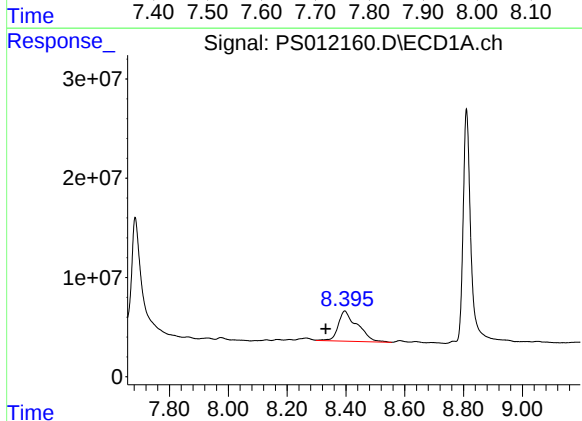


#9 2,4-D

R.T.: 8.396 min
Delta R.T.: 0.064 min
Response: 137913903
Conc: 122.15 ng/ml

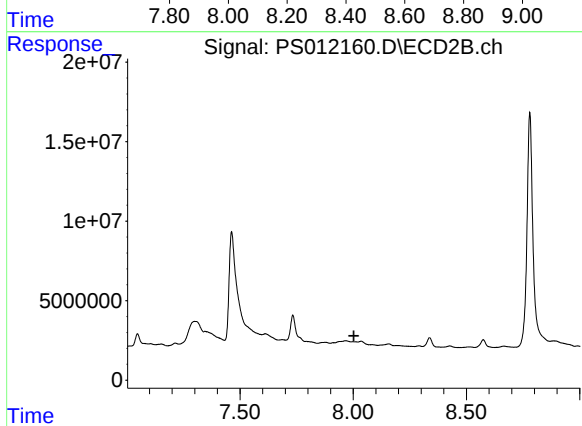

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.003 min
Response: 0
Conc: N.D.

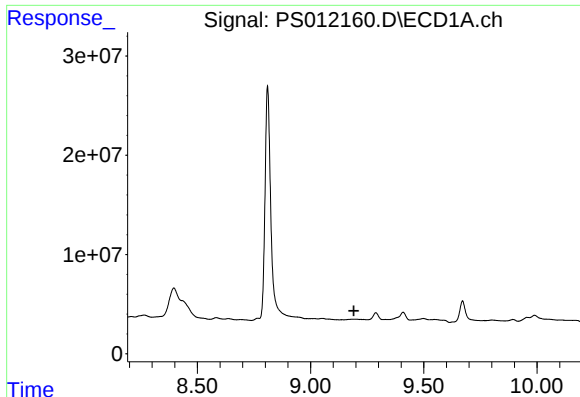

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

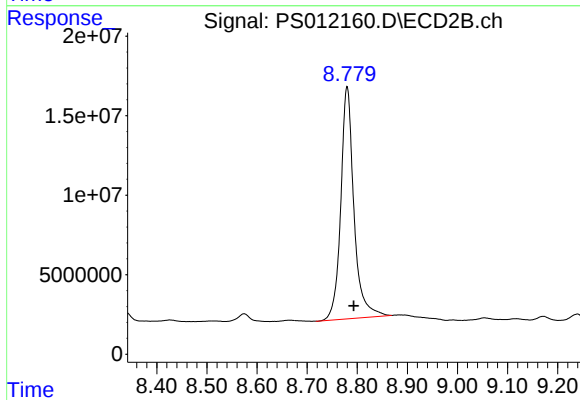


#11 2,4,5-TP (SILVEX)

R.T.: 8.780 min
Delta R.T.: -0.014 min
Response: 266853228
Conc: 91.27 ng/ml

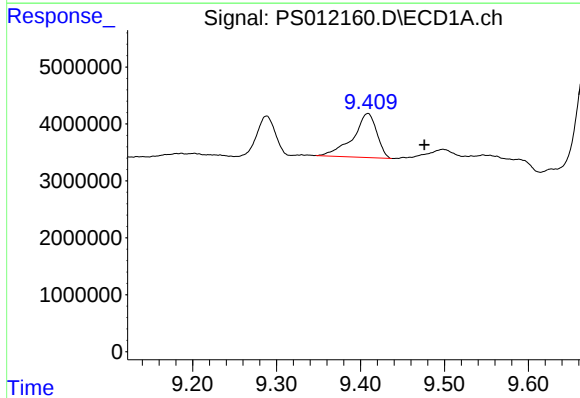

#12 2,4,5-T

R.T.: 9.409 min
Delta R.T.: -0.067 min
Response: 15251612
Conc: 2.57 ng/ml

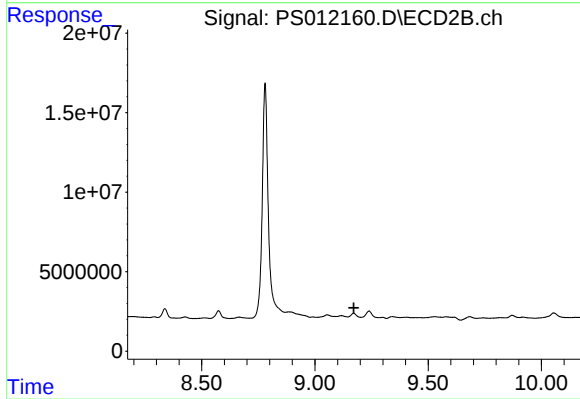

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 9.172 min
Response: 0
Conc: N.D.