

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090820\
 Data File : PS012163.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Sep 2020 22:09
 Operator : DD\AJ
 Sample : L3915-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 02:40:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.216	6.913	259.9E6	165.2E6	238.267	308.879 #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.095	0	36251678	N.D.	44.069
3) T	4-Nitroph...	7.115	6.544	28336628	11177492	48.106	30.656 #
5) T	DICAMBA	7.394	7.047	5270143	17629420	1.287	8.160 #
6) T	MCP	7.566	0.000	6202748	0	1.941	N.D. #
7) T	MCPA	7.689	7.467	218.8E6	127.6E6	48.108	46.575
8) T	DICHLORPROP	8.045	7.734	16783211	18270939	16.705	32.359 #
9) T	2,4-D	8.396	7.936	106.9E6	77504358	94.638	105.496
11) T	2,4,5-TP ...	0.000	8.782	0	58782407	N.D.	20.106
12) T	2,4,5-T	9.408	9.238	43171049	21077850	7.285	7.121
14) T	DINOSEB	0.000	10.057	0	13649270	N.D.	6.420
15) T	Picloram	11.021	11.007	71745558	63018042	9.180	13.904 #
16) T	DCPA	0.000	11.007	0	63018042	N.D.	17.139



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090820\
Data File : PS012163.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2020 22:09
Operator : DD\AJ
Sample : L3915-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 02:40:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

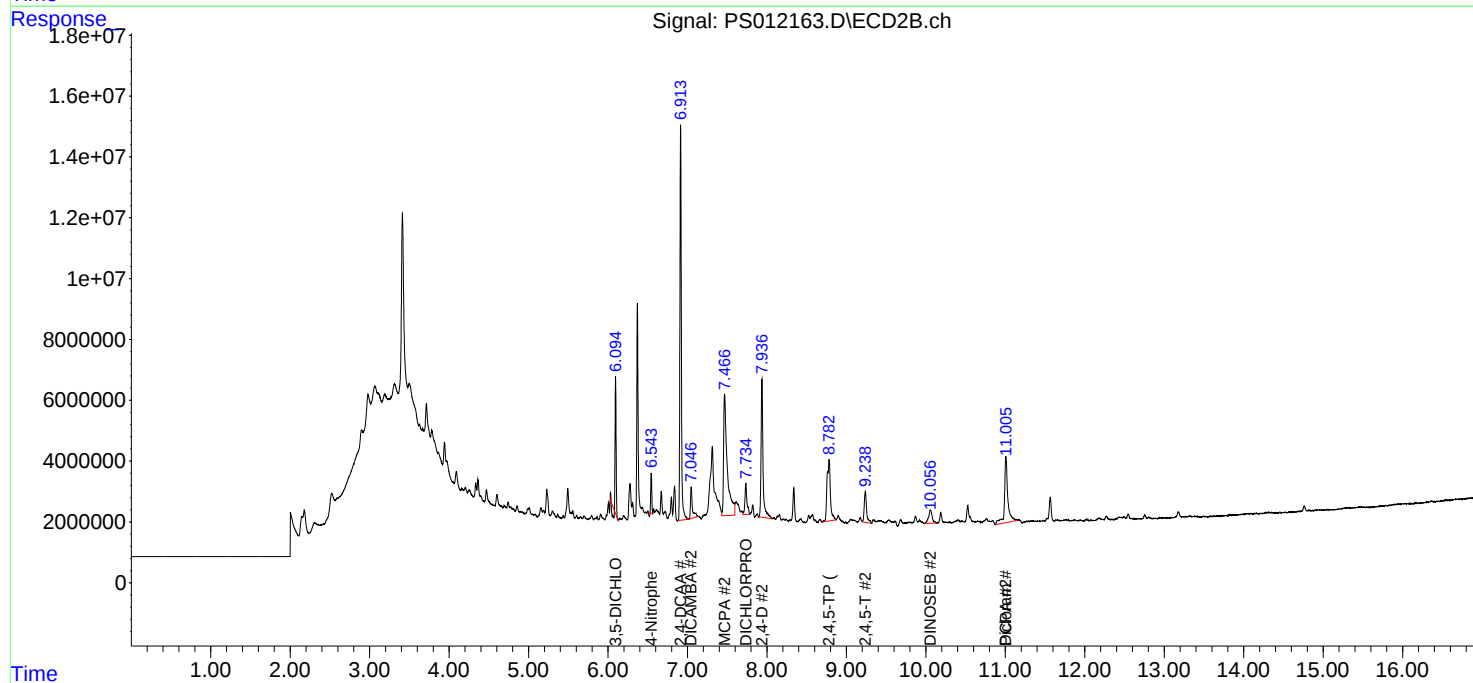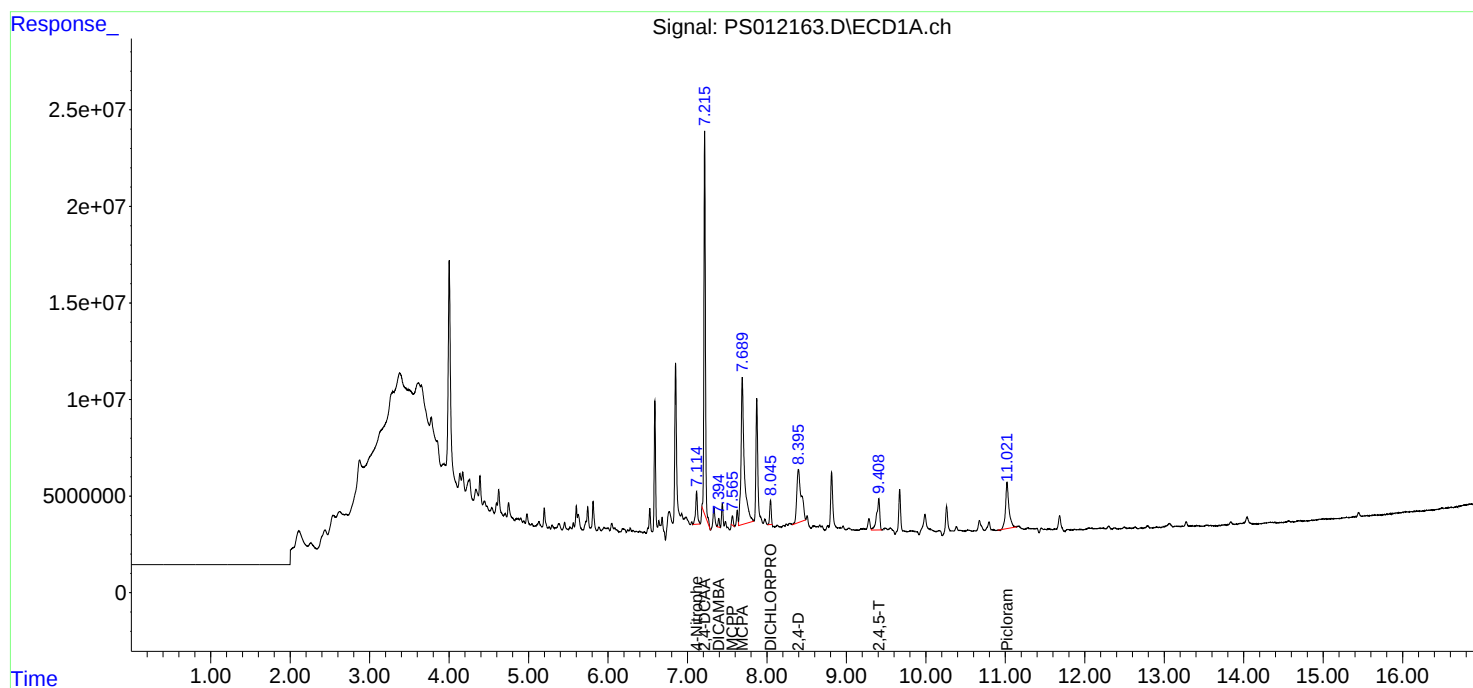


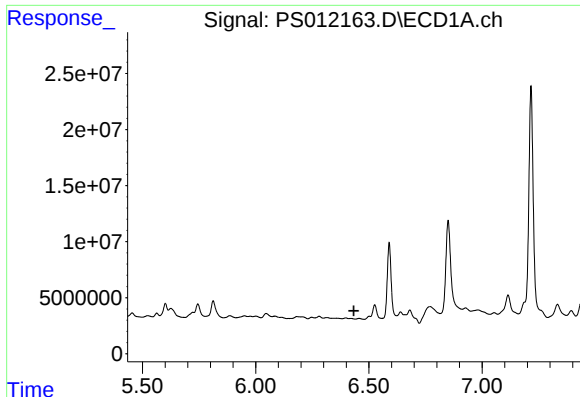

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

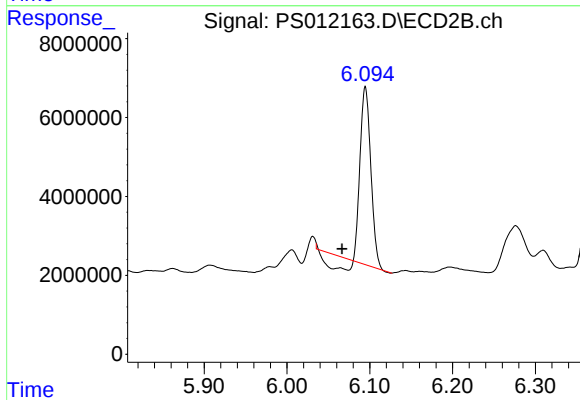


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.095 min
Delta R.T.: 0.028 min
Response: 36251678
Conc: 44.07 ng/ml

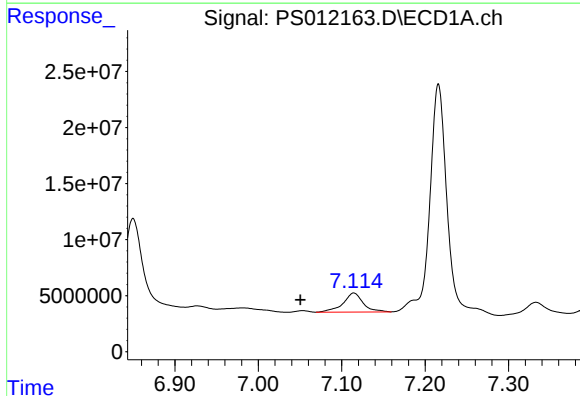


#3 4-Nitrophenol

R.T.: 7.115 min
Delta R.T.: 0.064 min
Response: 28336628
Conc: 48.11 ng/ml

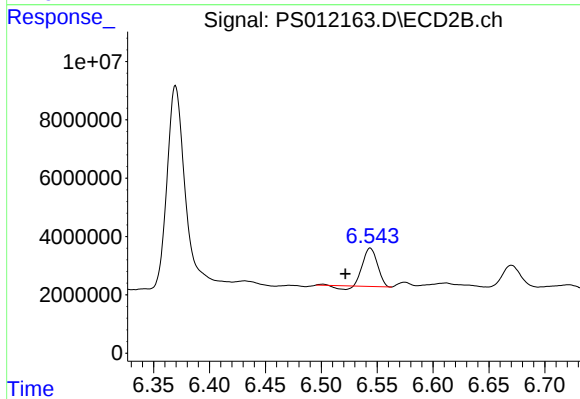

#3 4-Nitrophenol


R.T.: 6.544 min
Delta R.T.: 0.023 min
Response: 11177492
Conc: 30.66 ng/ml

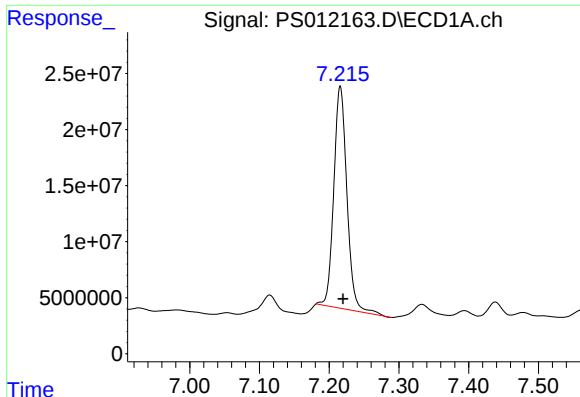

#4 2,4-DCAA


R.T.: 7.216 min
Delta R.T.: -0.004 min
Response: 259893833
Conc: 238.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

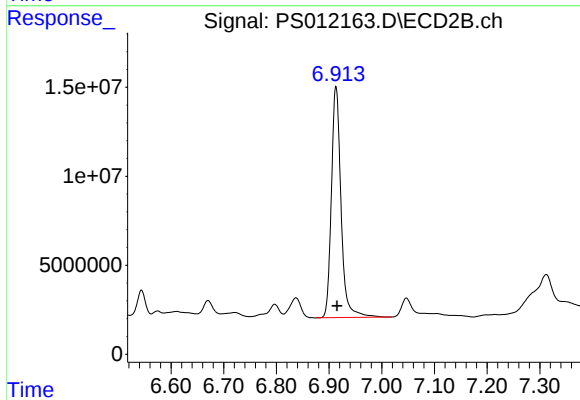


#4 2,4-DCAA

R.T.: 6.913 min
Delta R.T.: -0.002 min
Response: 165184359
Conc: 308.88 ng/ml

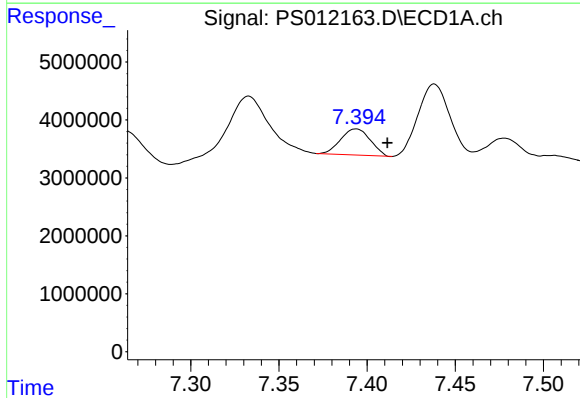


#5 DICAMBA

R.T.: 7.394 min
Delta R.T.: -0.018 min
Response: 5270143
Conc: 1.29 ng/ml

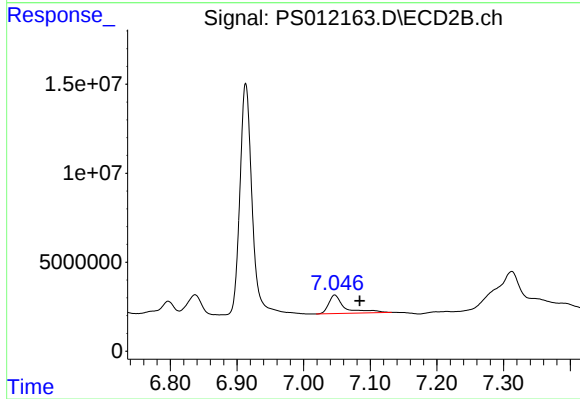

#5 DICAMBA


R.T.: 7.047 min
Delta R.T.: -0.037 min
Response: 17629420
Conc: 8.16 ng/ml

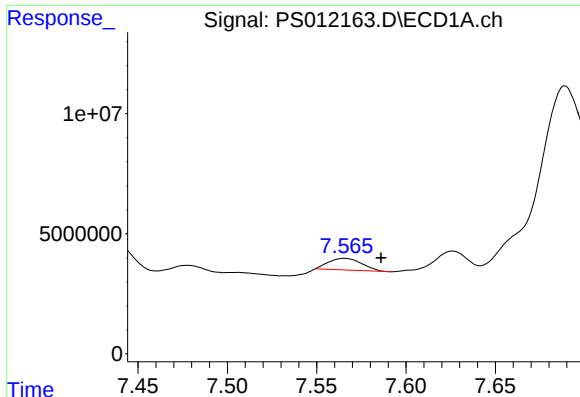

#6 MCPP


R.T.: 7.566 min
Delta R.T.: -0.020 min
Response: 6202748
Conc: 1.94 ug/ml

Instrument :
ECD_S
ClientSampleId :

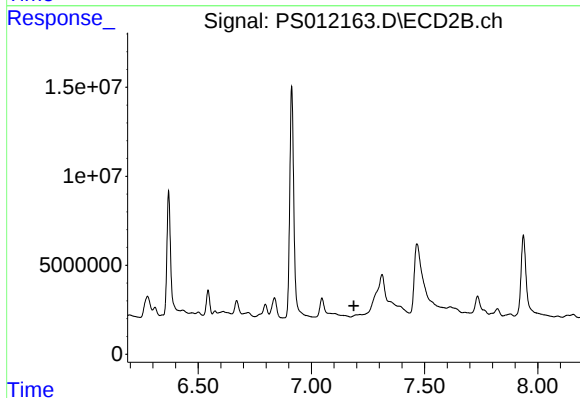


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

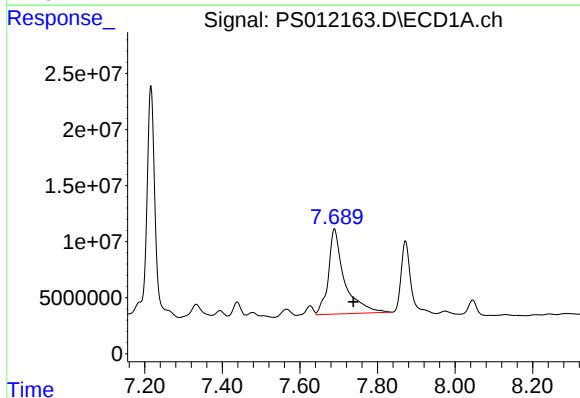


#7 MCPA

R.T.: 7.689 min
Delta R.T.: -0.049 min
Response: 218820645
Conc: 48.11 ug/ml

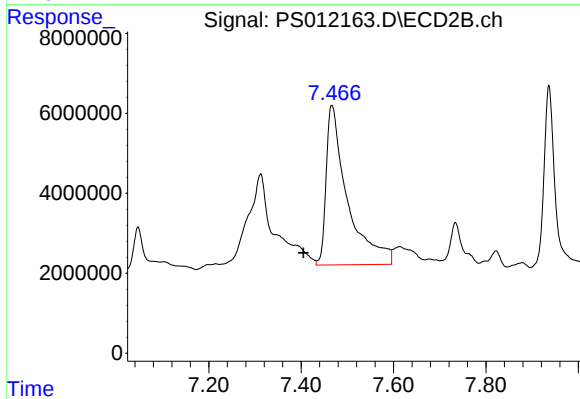

#7 MCPA


R.T.: 7.467 min
Delta R.T.: 0.062 min
Response: 127621055
Conc: 46.57 ug/ml

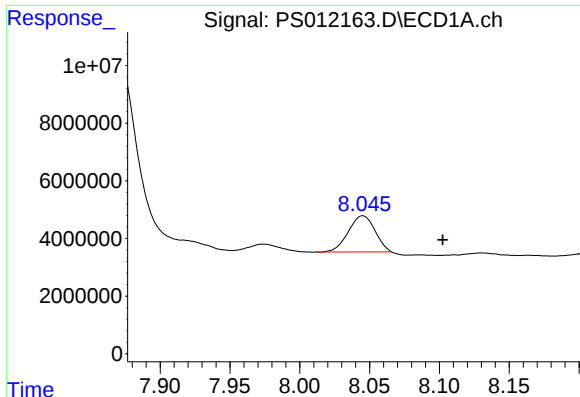

#8 DICHLORPROP


R.T.: 8.045 min
Delta R.T.: -0.057 min
Response: 16783211
Conc: 16.71 ng/ml

Instrument :
ECD_S
ClientSampleId :

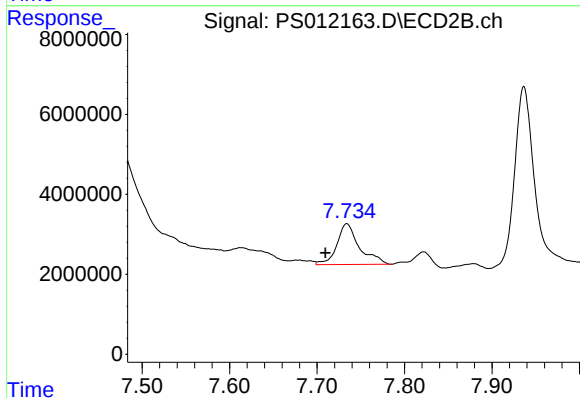


#8 DICHLORPROP

R.T.: 7.734 min
Delta R.T.: 0.025 min
Response: 18270939
Conc: 32.36 ng/ml

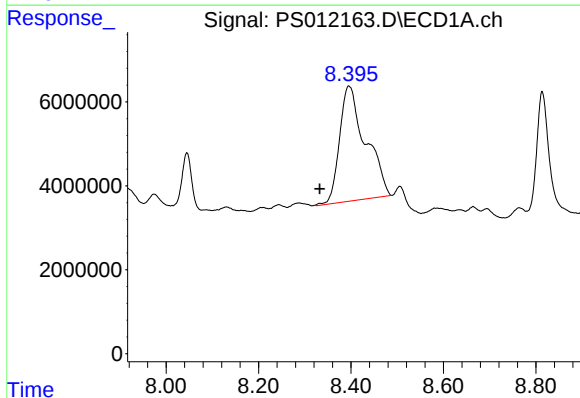


#9 2,4-D

R.T.: 8.396 min
Delta R.T.: 0.064 min
Response: 106855516
Conc: 94.64 ng/ml

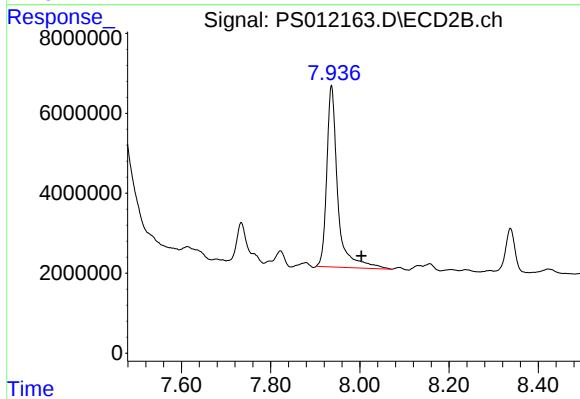

#9 2,4-D


R.T.: 7.936 min
Delta R.T.: -0.067 min
Response: 77504358
Conc: 105.50 ng/ml

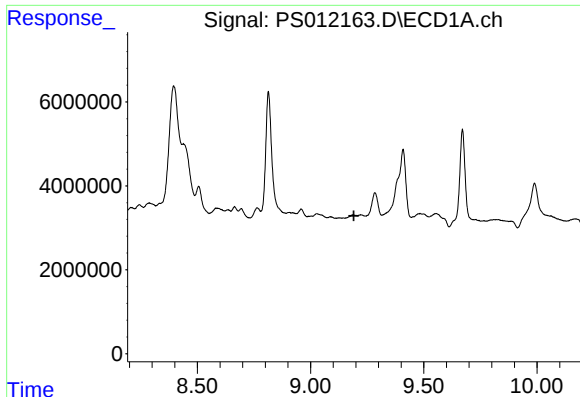

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

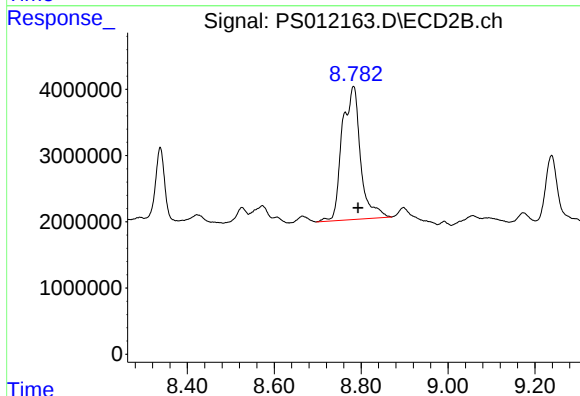


#11 2,4,5-TP (SILVEX)

R.T.: 8.782 min
Delta R.T.: -0.011 min
Response: 58782407
Conc: 20.11 ng/ml

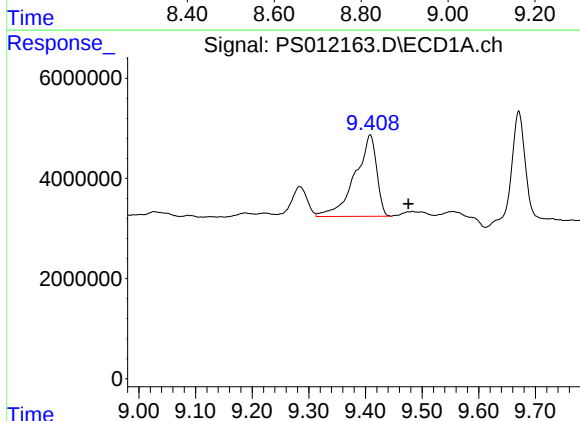


#12 2,4,5-T

R.T.: 9.408 min
Delta R.T.: -0.068 min
Response: 43171049
Conc: 7.29 ng/ml

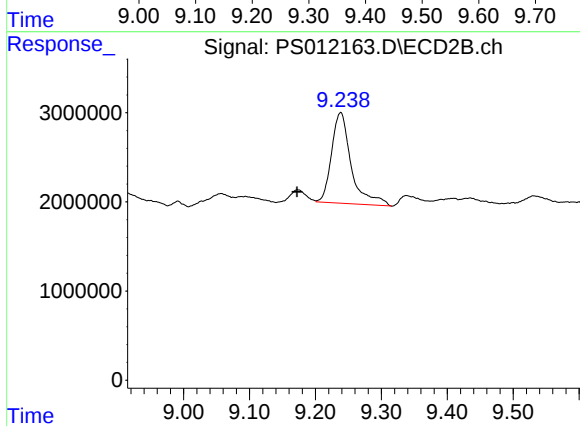

#12 2,4,5-T


R.T.: 9.238 min
Delta R.T.: 0.066 min
Response: 21077850
Conc: 7.12 ng/ml

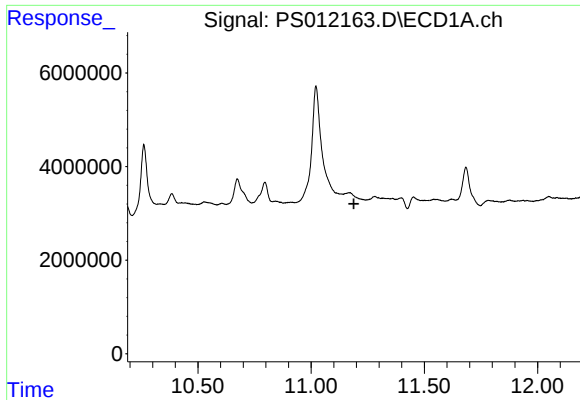

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.189 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

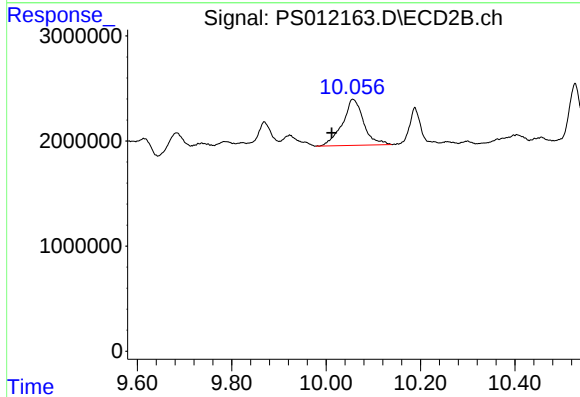


#14 DINOSEB

R.T.: 10.057 min
Delta R.T.: 0.045 min
Response: 13649270
Conc: 6.42 ng/ml

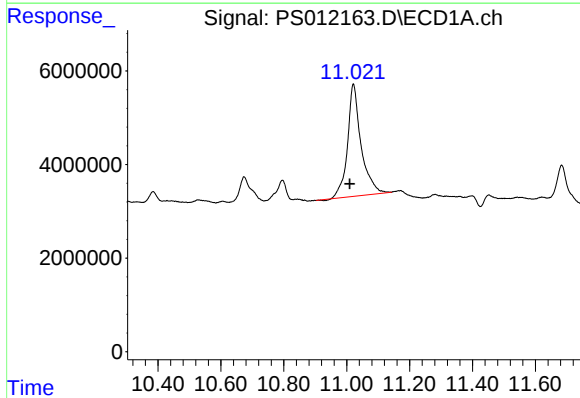


#15 Picloram

R.T.: 11.021 min
Delta R.T.: 0.012 min
Response: 71745558
Conc: 9.18 ng/ml

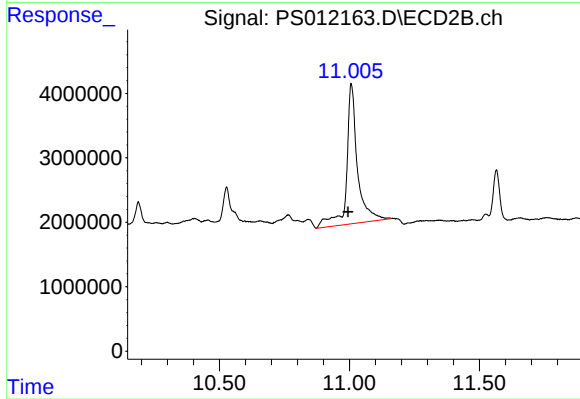

#15 Picloram


R.T.: 11.007 min
Delta R.T.: 0.012 min
Response: 63018042
Conc: 13.90 ng/ml

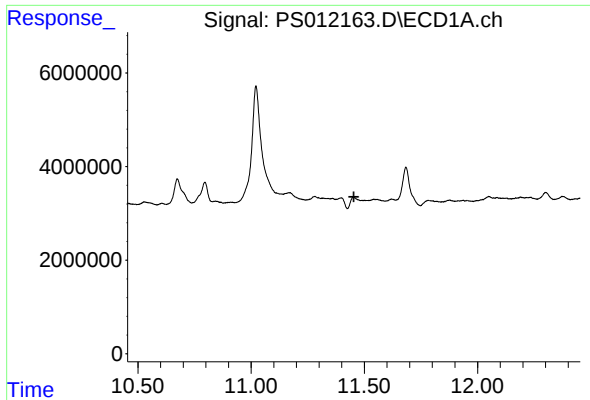

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.454 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

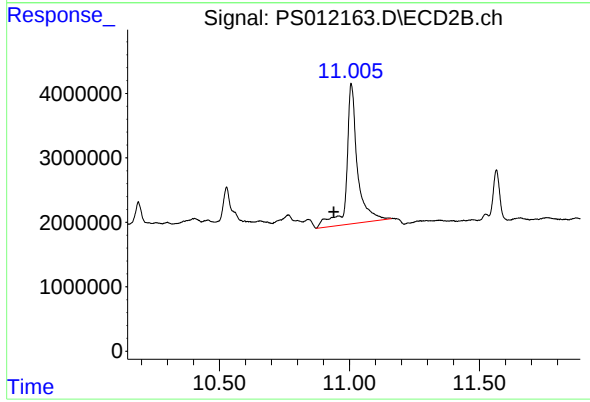

#16 DCPA

R.T.: 11.007 min
Delta R.T.: 0.067 min
Response: 63018042
Conc: 17.14 ng/ml