

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090820\
 Data File : PS012164.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Sep 2020 22:32
 Operator : DD\AJ
 Sample : L3915-06
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 02:40:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.216	6.913	291.6E6	173.8E6	267.324	325.034
Target Compounds							
2) T	3,5-DICHL...	0.000	6.095	0	39912210	N.D.	48.518
3) T	4-Nitroph...	6.982	0.000	2784996	0	4.728	N.D. #
5) T	DICAMBA	7.394	7.047	6604801	12472263	1.613	5.773 #
6) T	MCP	7.626	0.000	11525769	0	3.607	N.D. #
7) T	MCPA	7.690	7.467	197.3E6	111.8E6	43.380	40.795
8) T	DICHLORPROP	0.000	7.735	0	24876556	N.D.	44.058
9) T	2,4-D	8.396	0.000	126.7E6	0	112.242	N.D. #
11) T	2,4,5-TP ...	0.000	8.761	0	34878333	N.D.	11.930
12) T	2,4,5-T	9.409	9.242	16909166	8901628	2.853	3.007
14) T	DINOSEB	0.000	10.057	0	10390484	N.D.	4.888



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090820\
Data File : PS012164.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2020 22:32
Operator : DD\AJ
Sample : L3915-06
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 02:40:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

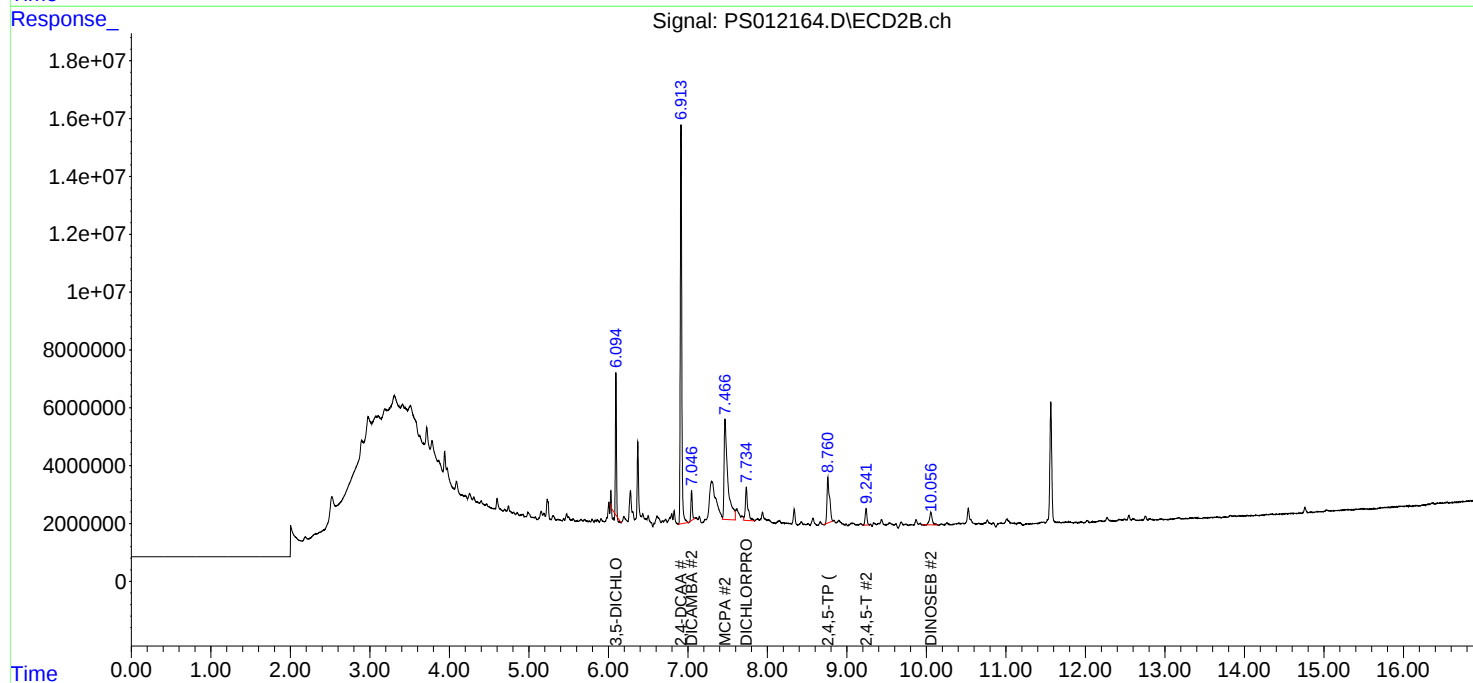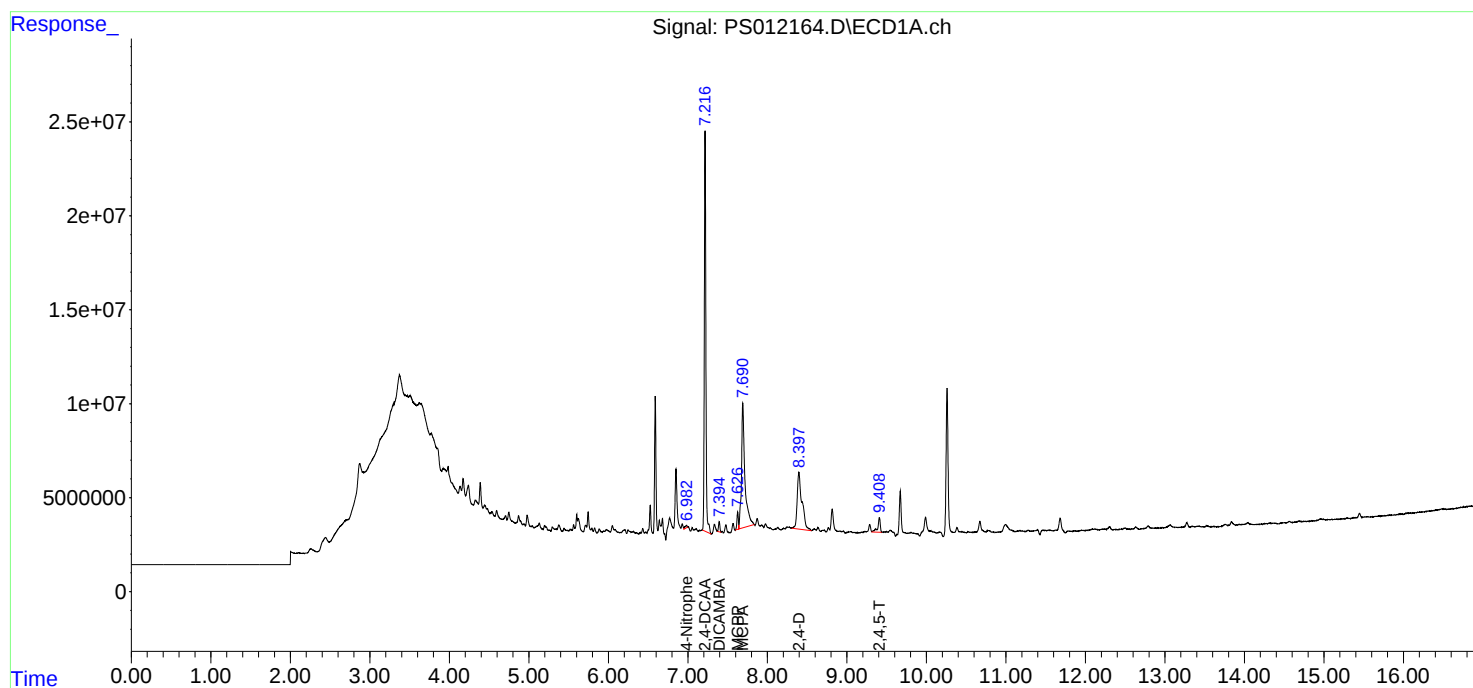


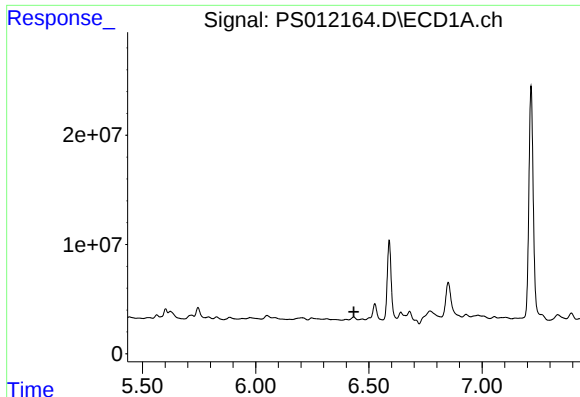

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

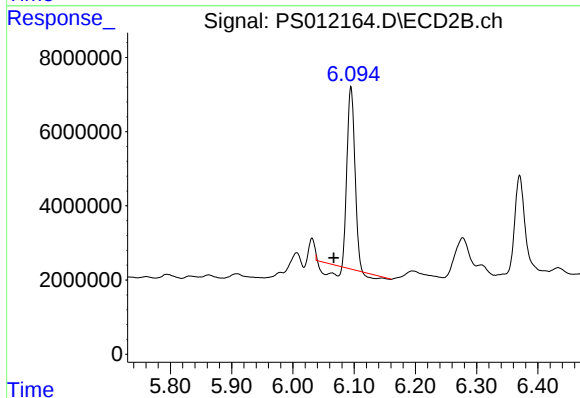


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.095 min
Delta R.T.: 0.028 min
Response: 39912210
Conc: 48.52 ng/ml

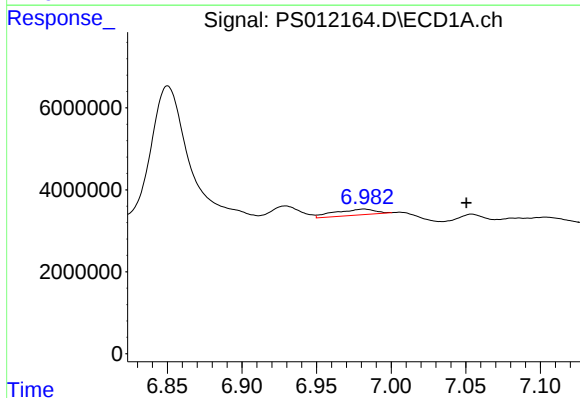


#3 4-Nitrophenol

R.T.: 6.982 min
Delta R.T.: -0.069 min
Response: 2784996
Conc: 4.73 ng/ml

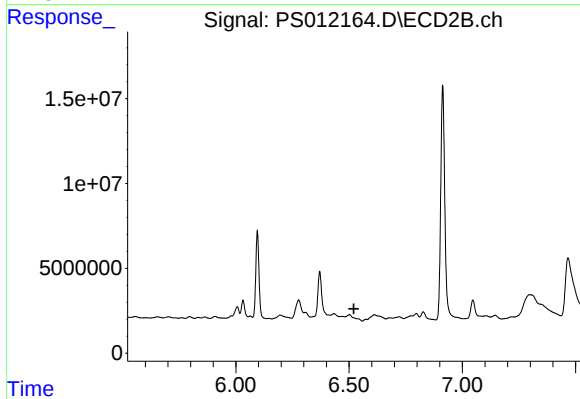

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.521 min
Response: 0
Conc: N.D.

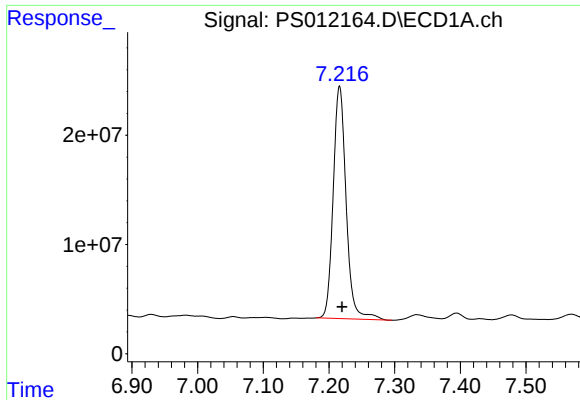

#4 2,4-DCAA


R.T.: 7.216 min
Delta R.T.: -0.004 min
Response: 291588979
Conc: 267.32 ng/ml

Instrument :
ECD_S
ClientSampleId :

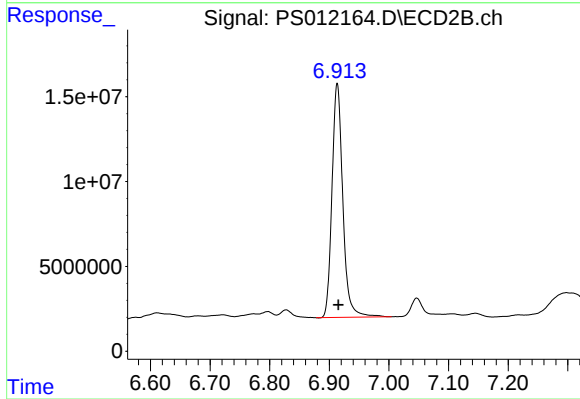


#4 2,4-DCAA

R.T.: 6.913 min
Delta R.T.: -0.002 min
Response: 173823855
Conc: 325.03 ng/ml

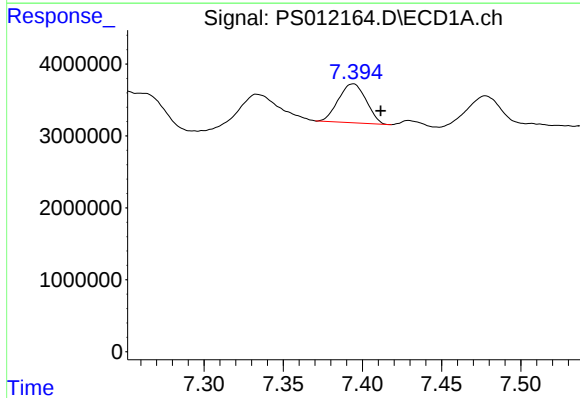


#5 DICAMBA

R.T.: 7.394 min
Delta R.T.: -0.018 min
Response: 6604801
Conc: 1.61 ng/ml

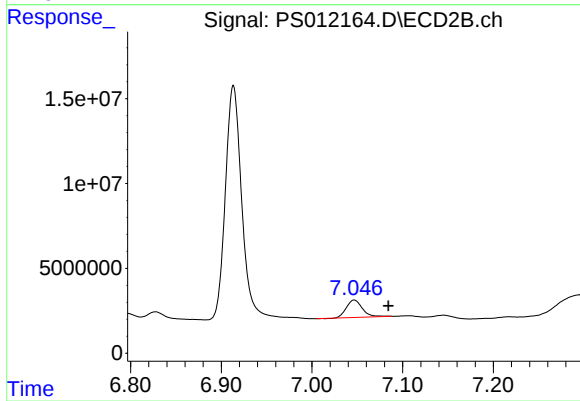

#5 DICAMBA


R.T.: 7.047 min
Delta R.T.: -0.038 min
Response: 12472263
Conc: 5.77 ng/ml

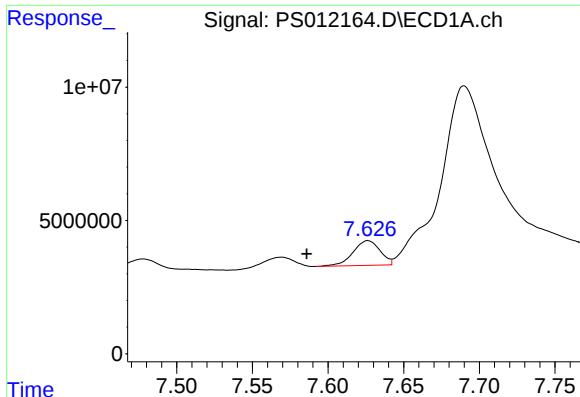

#6 MCPP


R.T.: 7.626 min
Delta R.T.: 0.040 min
Response: 11525769
Conc: 3.61 ug/ml

Instrument :
ECD_S
ClientSampleId :

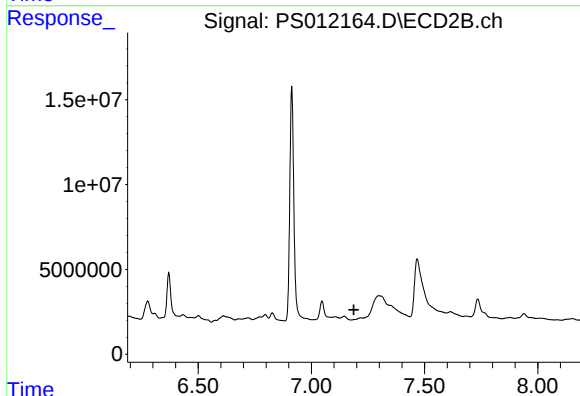


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

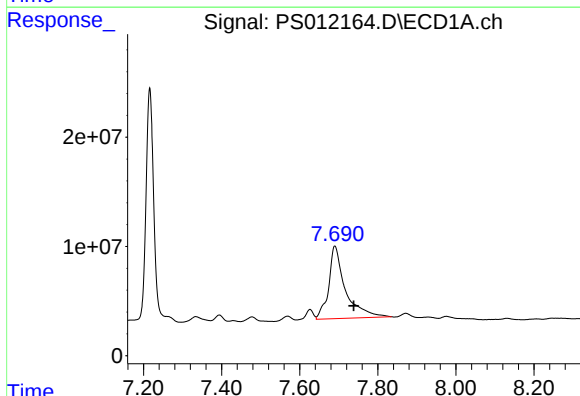


#7 MCPA

R.T.: 7.690 min
Delta R.T.: -0.048 min
Response: 197315439
Conc: 43.38 ug/ml

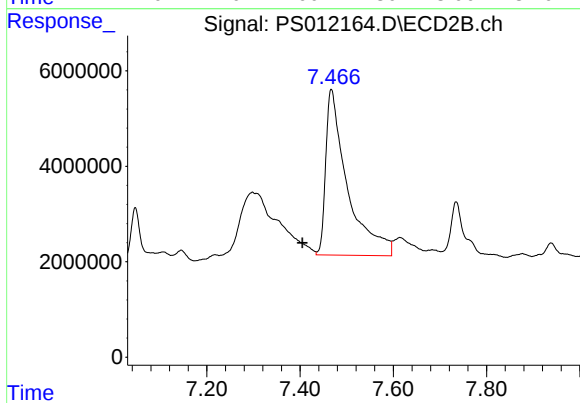

#7 MCPA


R.T.: 7.467 min
Delta R.T.: 0.063 min
Response: 111783663
Conc: 40.79 ug/ml

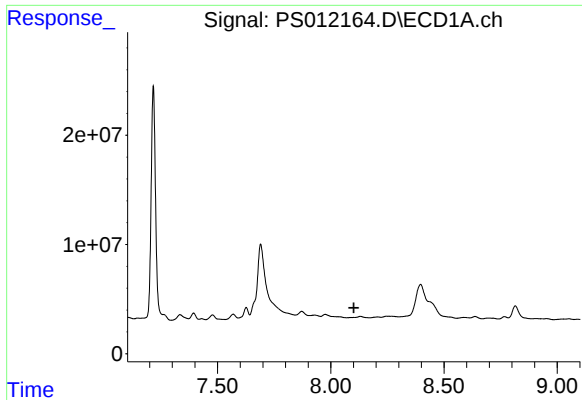

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

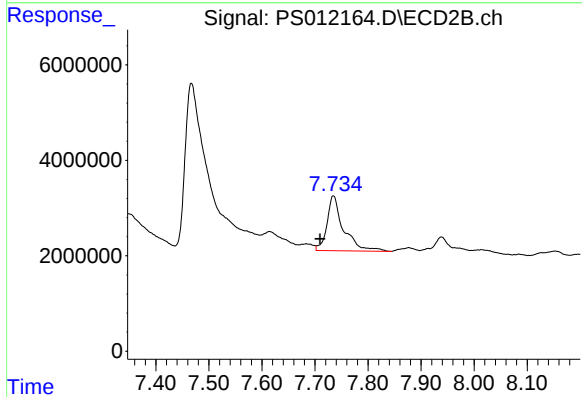


#8 DICHLORPROP

R.T.: 7.735 min
Delta R.T.: 0.025 min
Response: 24876556
Conc: 44.06 ng/ml

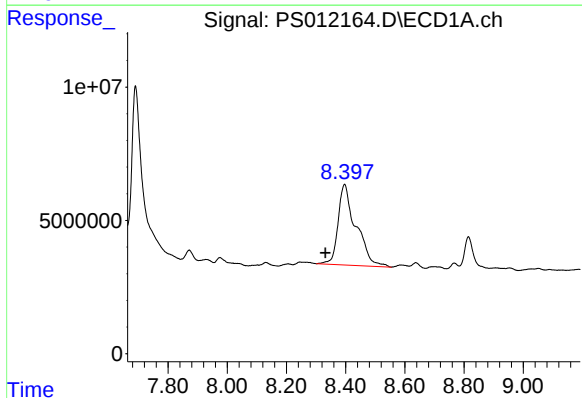


#9 2,4-D

R.T.: 8.396 min
Delta R.T.: 0.064 min
Response: 126731631
Conc: 112.24 ng/ml

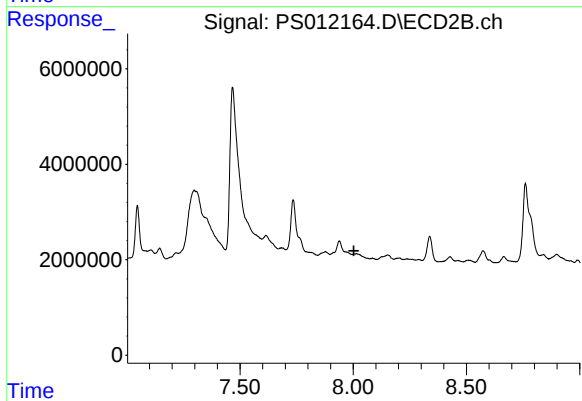

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.003 min
Response: 0
Conc: N.D.

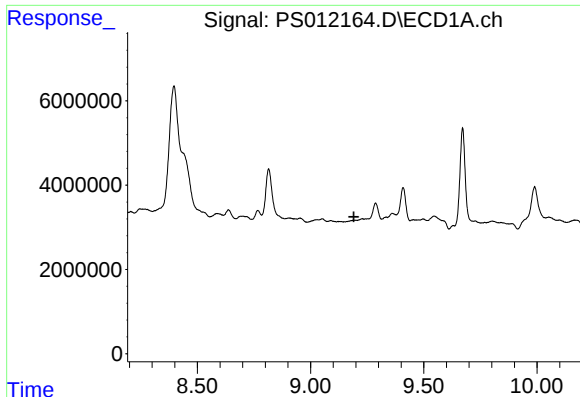

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

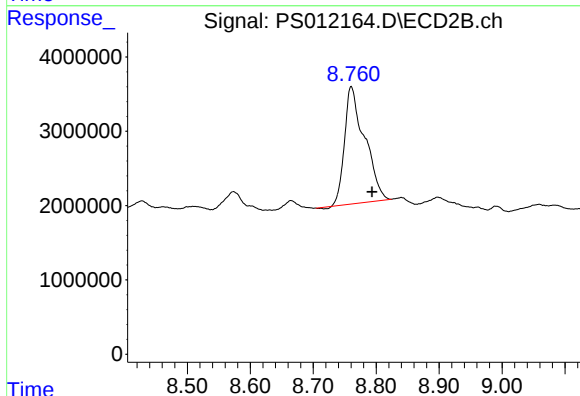


#11 2,4,5-TP (SILVEX)

R.T.: 8.761 min
Delta R.T.: -0.033 min
Response: 34878333
Conc: 11.93 ng/ml

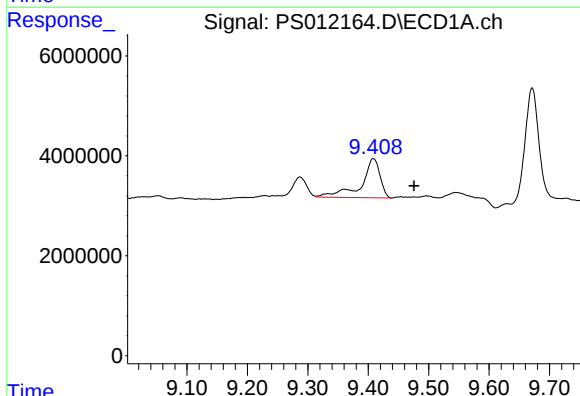


#12 2,4,5-T

R.T.: 9.409 min
Delta R.T.: -0.067 min
Response: 16909166
Conc: 2.85 ng/ml

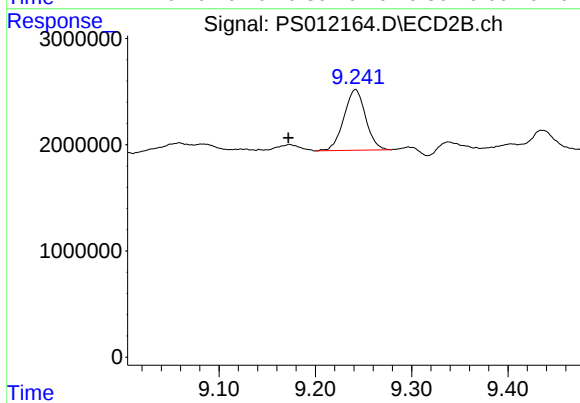

#12 2,4,5-T


R.T.: 9.242 min
Delta R.T.: 0.069 min
Response: 8901628
Conc: 3.01 ng/ml

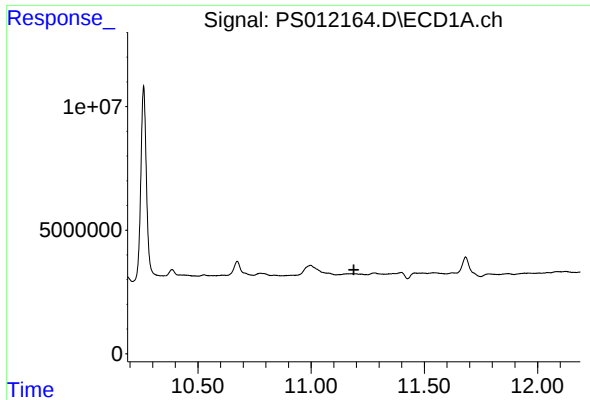

#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 11.189 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

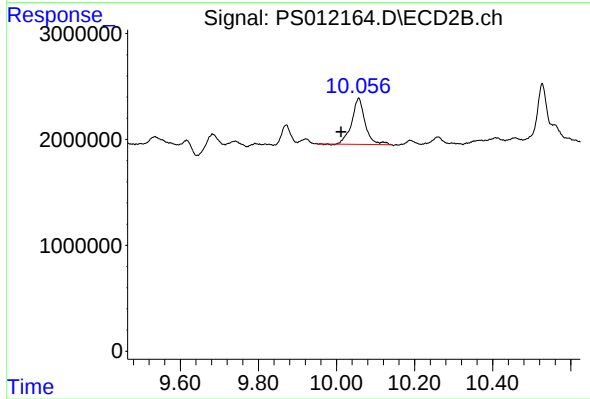

#14 DINOSEB

R.T.: 10.057 min
Delta R.T.: 0.045 min
Response: 10390484
Conc: 4.89 ng/ml