

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090820\
 Data File : PS012165.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Sep 2020 22:55
 Operator : DD\AJ
 Sample : L3915-10
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 02:40:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.216	6.914	269.8E6	164.6E6	247.338	307.723
Target Compounds							
2) T	3,5-DICHL...	0.000	6.095	0	83968980	N.D.	102.075
3) T	4-Nitroph...	7.053	0.000	3579291	0	6.076	N.D. #
5) T	DICAMBA	7.394	7.046	8615189	9308265	2.103	4.308 #
6) T	MCP	7.626	0.000	7571280	0	2.370	N.D. #
7) T	MCPA	7.693	7.469	200.2E6	90001387	44.014	32.846 #
8) T	DICHLORPROP	0.000	7.736	0	23388817	N.D.	41.423
9) T	2,4-D	8.395	0.000	127.3E6	0	112.740	N.D. #
11) T	2,4,5-TP ...	0.000	8.761	0	28867200	N.D.	9.874
12) T	2,4,5-T	9.408	0.000	15794497	0	2.665	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090820\
Data File : PS012165.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2020 22:55
Operator : DD\AJ
Sample : L3915-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 02:40:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

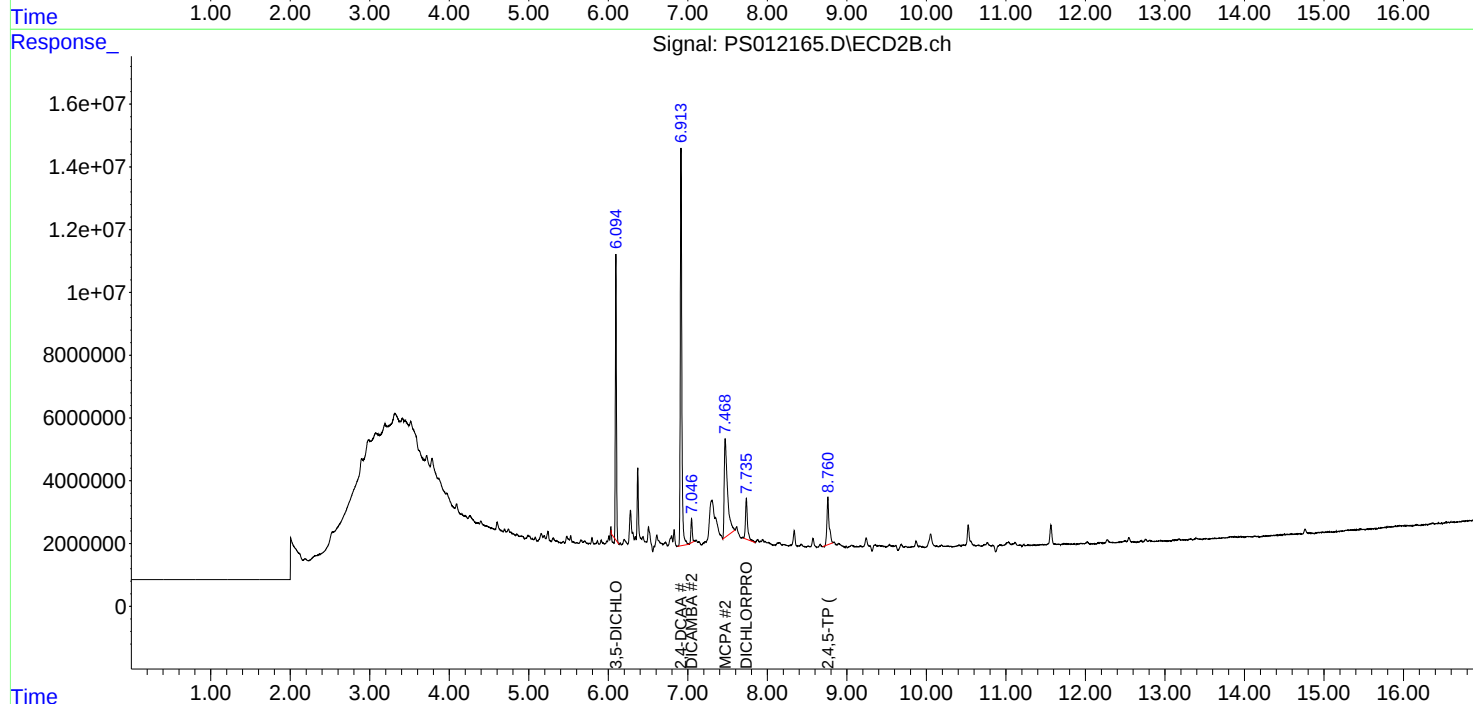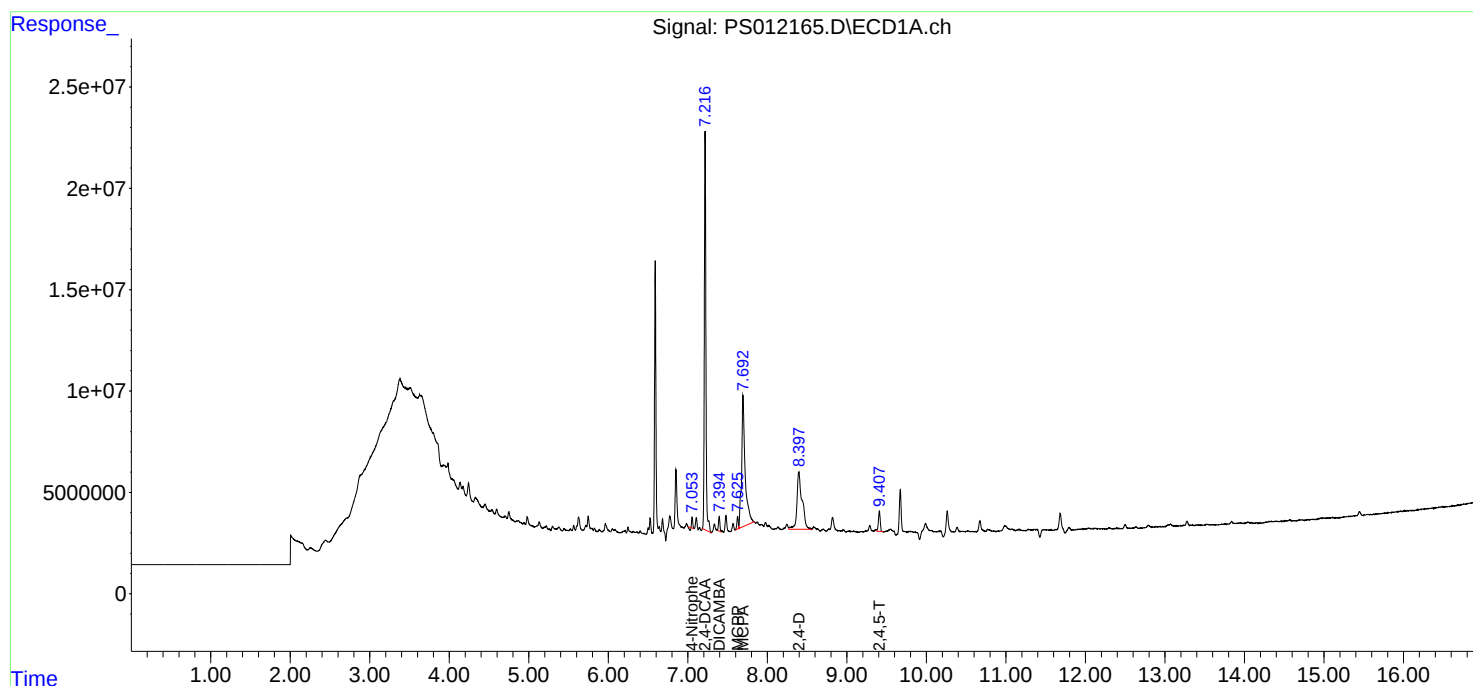


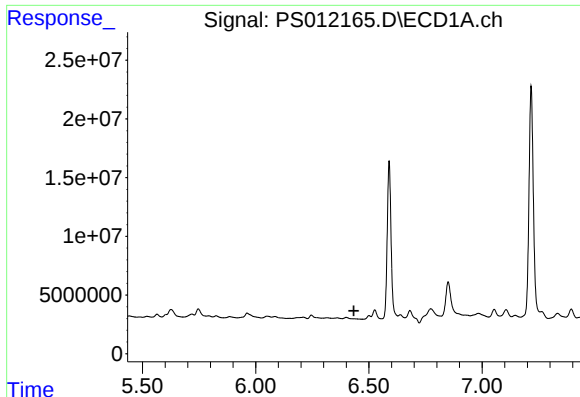

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

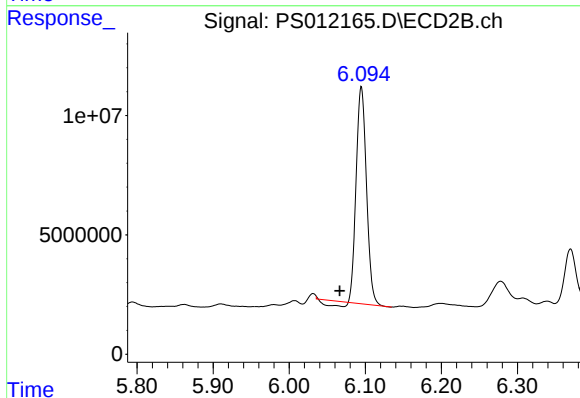


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.095 min
Delta R.T.: 0.028 min
Response: 83968980
Conc: 102.08 ng/ml

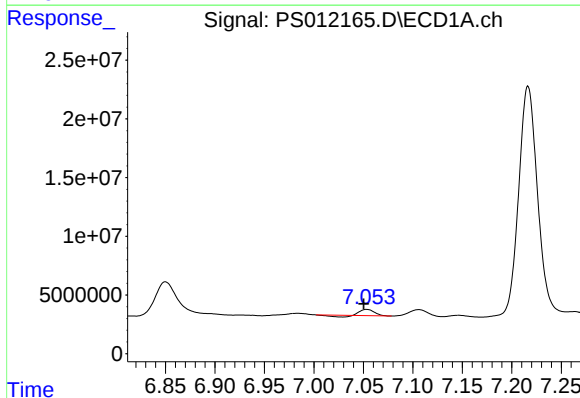


#3 4-Nitrophenol

R.T.: 7.053 min
Delta R.T.: 0.003 min
Response: 3579291
Conc: 6.08 ng/ml

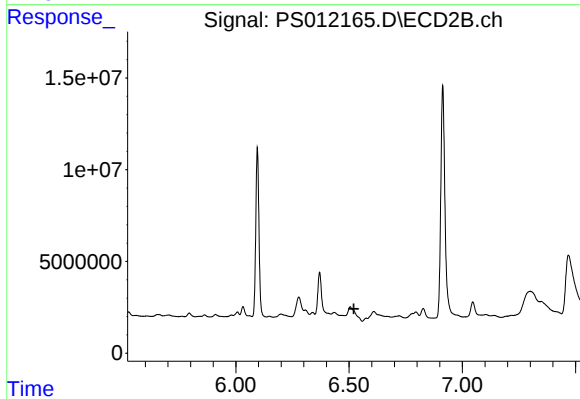

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.521 min
Response: 0
Conc: N.D.

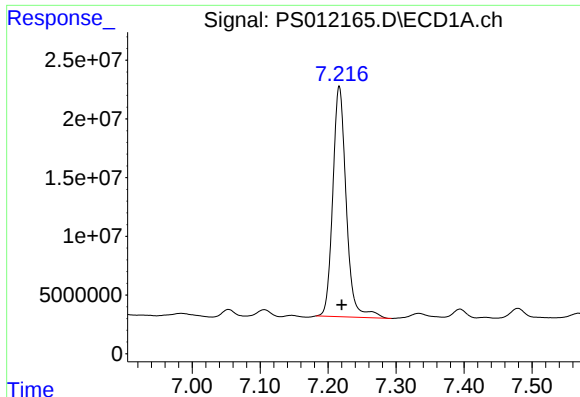

#4 2,4-DCAA


R.T.: 7.216 min
Delta R.T.: -0.004 min
Response: 269788085
Conc: 247.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

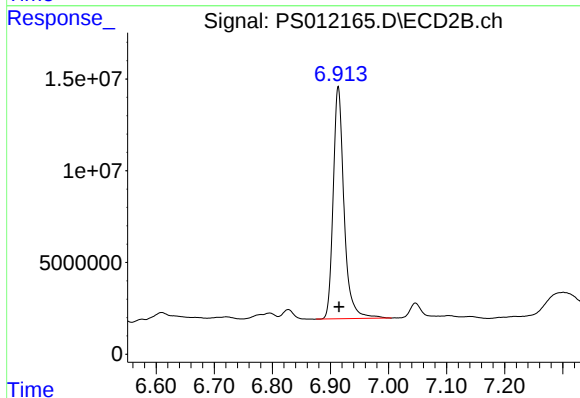


#4 2,4-DCAA

R.T.: 6.914 min
Delta R.T.: -0.001 min
Response: 164566343
Conc: 307.72 ng/ml

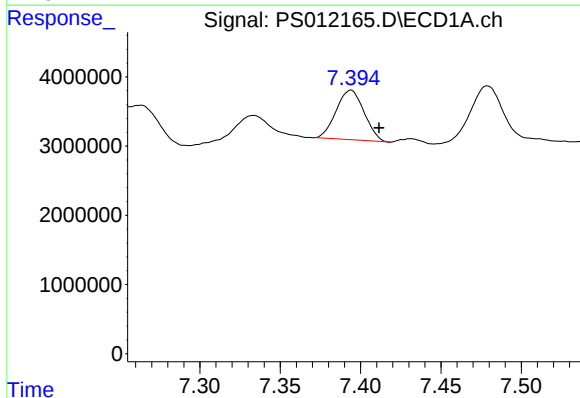


#5 DICAMBA

R.T.: 7.394 min
Delta R.T.: -0.018 min
Response: 8615189
Conc: 2.10 ng/ml

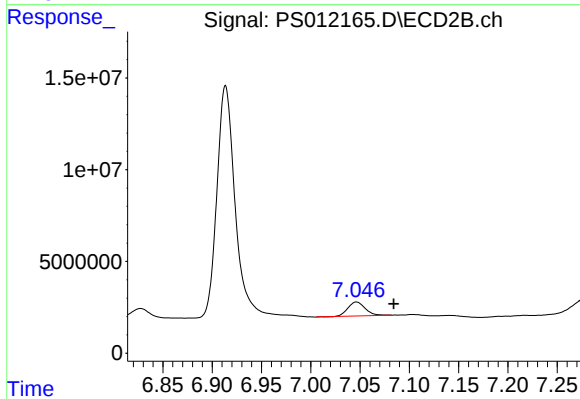

#5 DICAMBA


R.T.: 7.046 min
Delta R.T.: -0.038 min
Response: 9308265
Conc: 4.31 ng/ml

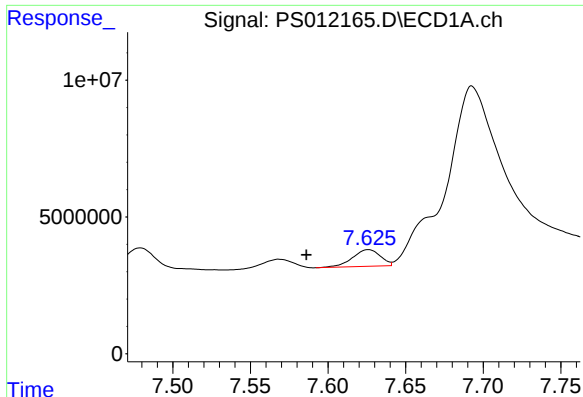

#6 MCPP


R.T.: 7.626 min
Delta R.T.: 0.040 min
Response: 7571280
Conc: 2.37 ug/ml

Instrument :
ECD_S
ClientSampleId :

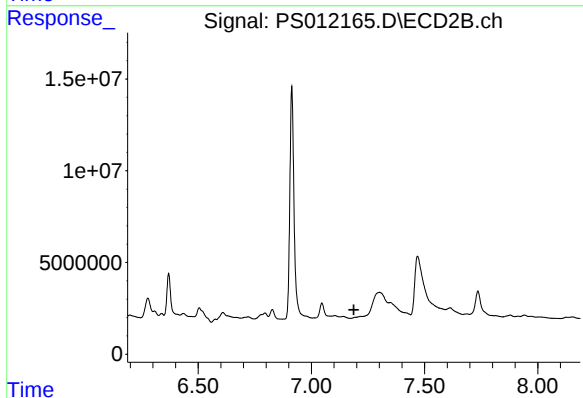


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

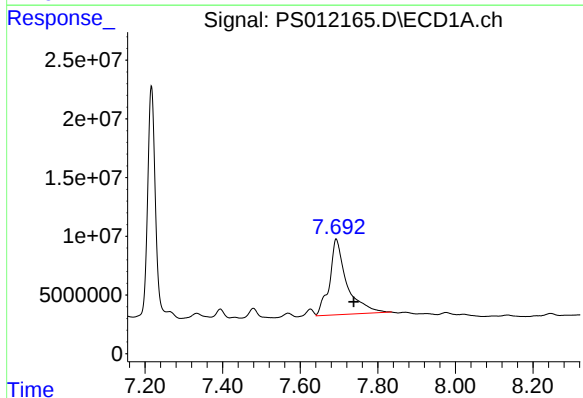


#7 MCPA

R.T.: 7.693 min
Delta R.T.: -0.045 min
Response: 200196727
Conc: 44.01 ug/ml

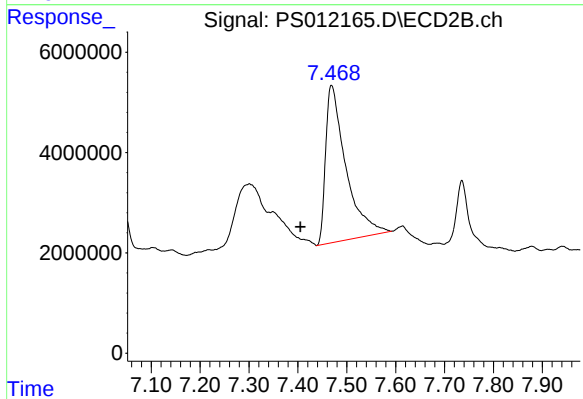

#7 MCPA


R.T.: 7.469 min
Delta R.T.: 0.064 min
Response: 90001387
Conc: 32.85 ug/ml

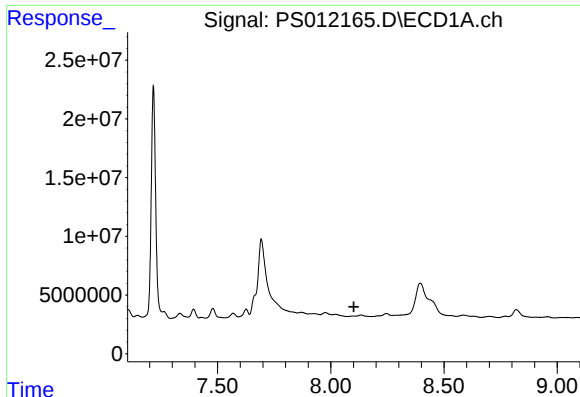

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

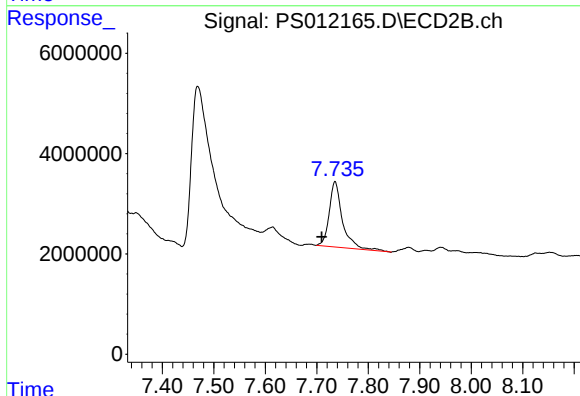


#8 DICHLORPROP

R.T.: 7.736 min
Delta R.T.: 0.026 min
Response: 23388817
Conc: 41.42 ng/ml

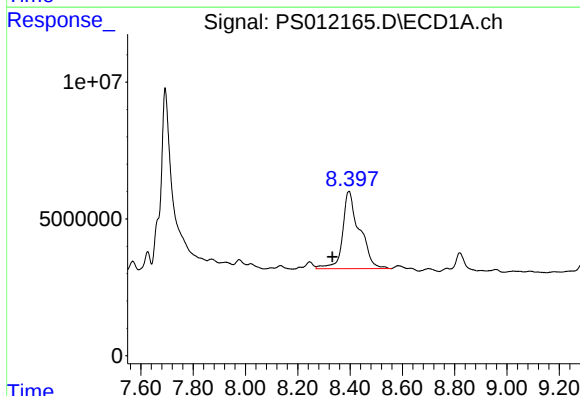


#9 2,4-D

R.T.: 8.395 min
Delta R.T.: 0.063 min
Response: 127293466
Conc: 112.74 ng/ml

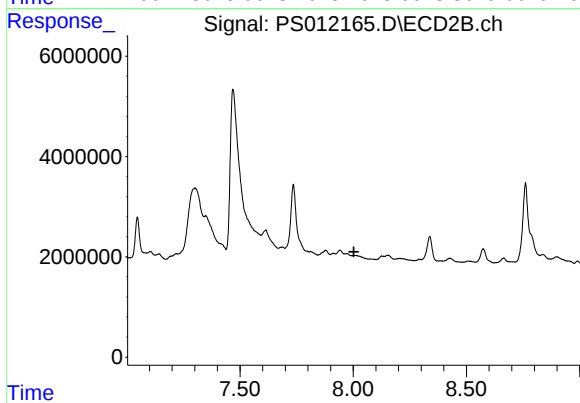

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.003 min
Response: 0
Conc: N.D.

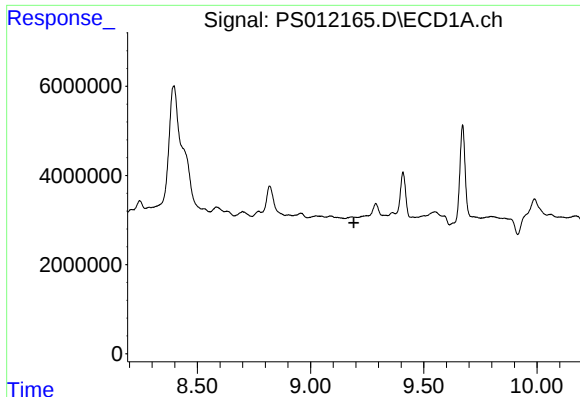

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

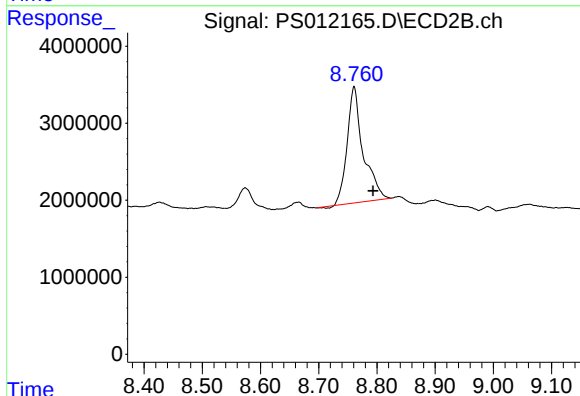


#11 2,4,5-TP (SILVEX)

R.T.: 8.761 min
Delta R.T.: -0.033 min
Response: 28867200
Conc: 9.87 ng/ml

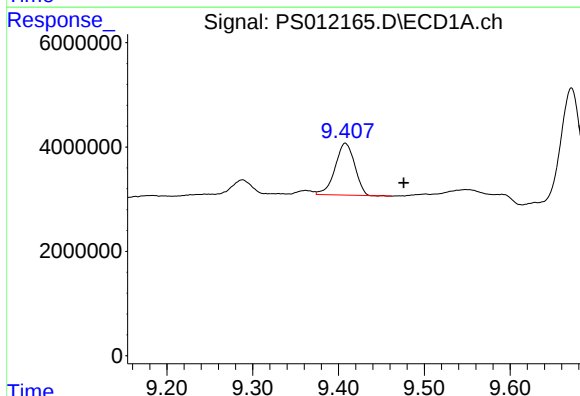

#12 2,4,5-T

R.T.: 9.408 min
Delta R.T.: -0.068 min
Response: 15794497
Conc: 2.67 ng/ml

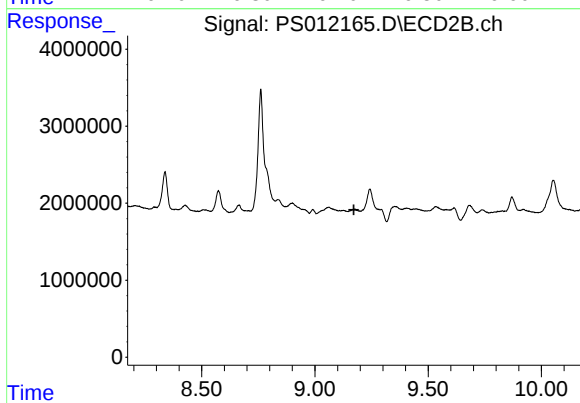

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 9.172 min
Response: 0
Conc: N.D.