

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090820\
 Data File : PS012168.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2020 00:04
 Operator : DD\AJ
 Sample : L3847-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 02:41:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.217	6.914	88473875	56033290	81.112	104.777 #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.095	0	100.7E6	N.D.	122.376
3) T	4-Nitroph...	7.054	0.000	7022292	0	11.922	N.D. #
5) T	DICAMBA	7.394	7.047	9350039	12514092	2.283	5.792 #
6) T	MCP	7.569	0.000	6789502	0	2.125	N.D. #
7) T	MCPA	7.763	7.374	21491172	32052746	4.725	11.697 #
8) T	DICHLORPROP	0.000	7.736	0	15077791	N.D.	26.704
9) T	2,4-D	8.394	0.000	121.0E6	0	107.203	N.D. #
10) T	Pentachlo...	8.699	0.000	12627180	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	8.761	0	23732918	N.D.	8.118
12) T	2,4,5-T	9.410	0.000	44931360	0	7.582	N.D. #
13) T	2,4-DB	9.978	0.000	10848785	0	13.654	N.D. #
15) T	Picloram	0.000	11.018	0	26951758	N.D.	5.946
16) T	DCPA	11.520	0.000	27926694	0	3.673	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090820\
Data File : PS012168.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2020 00:04
Operator : DD\AJ
Sample : L3847-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 02:41:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

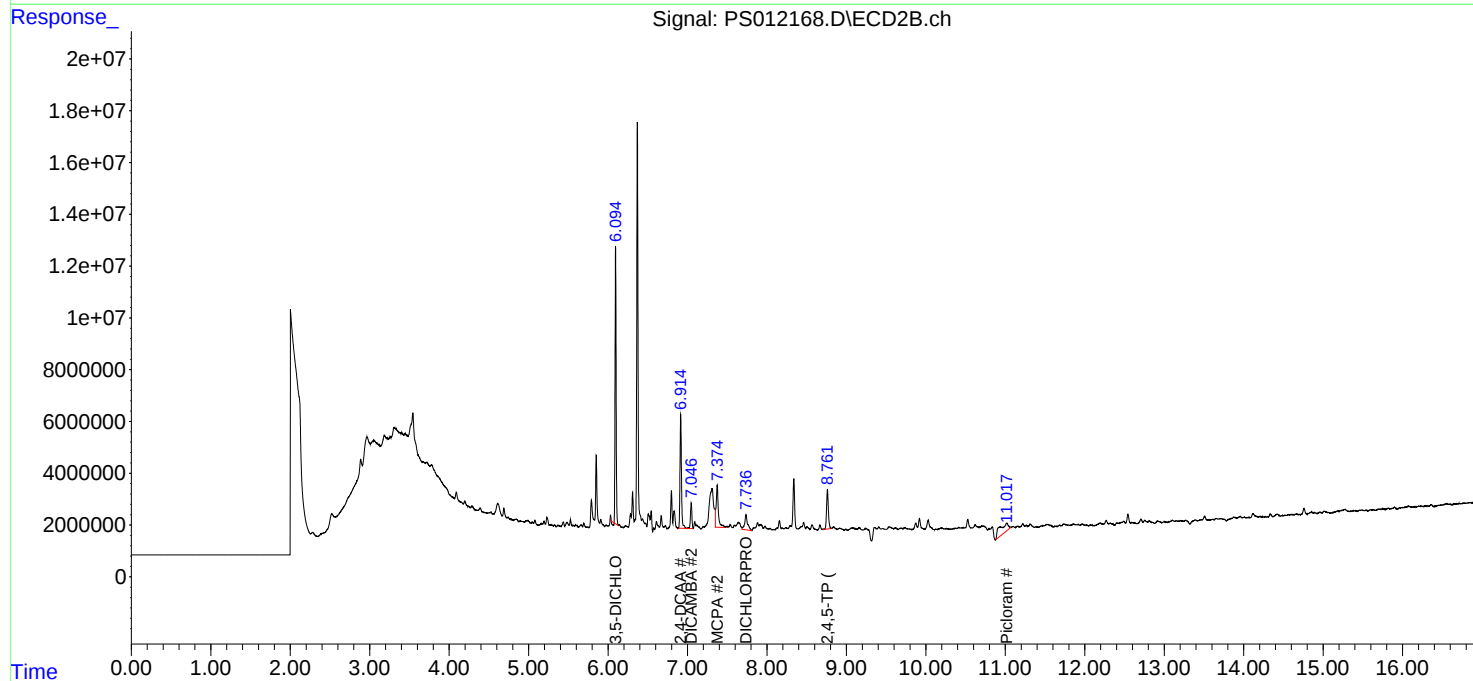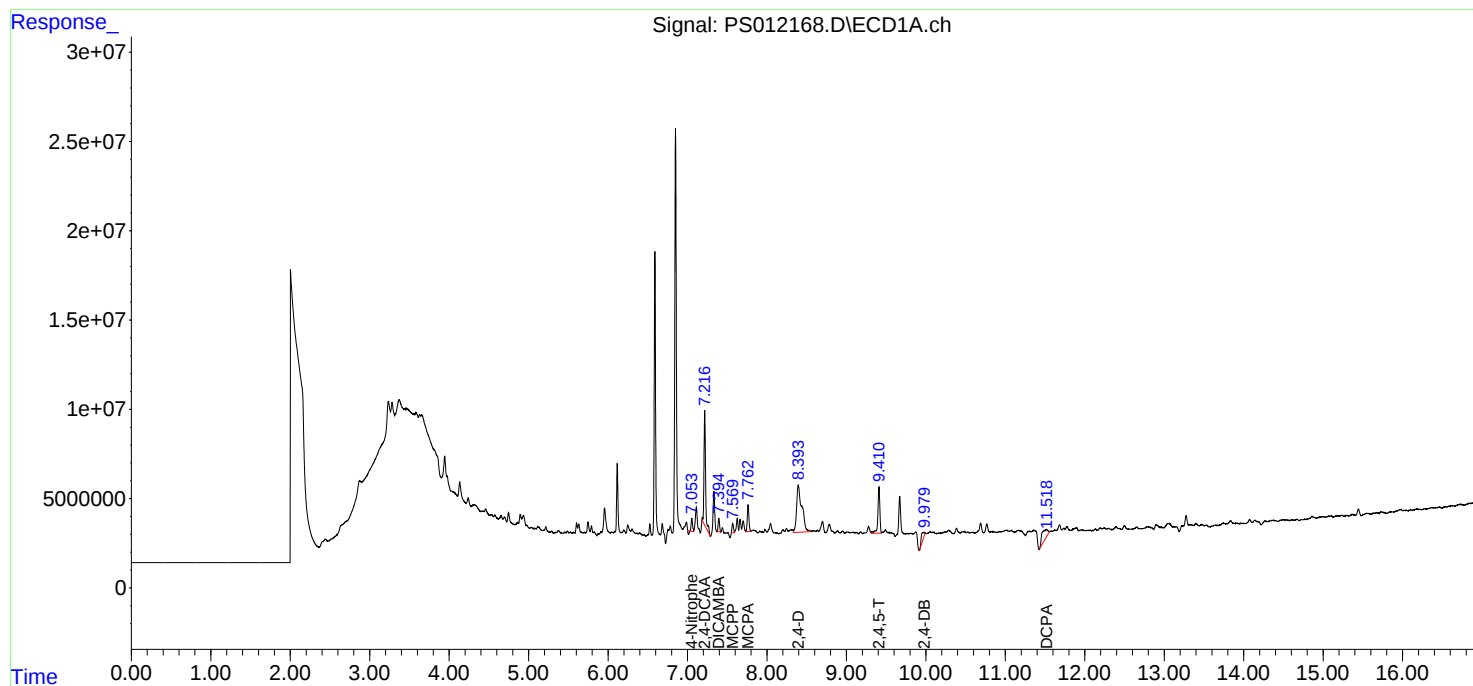


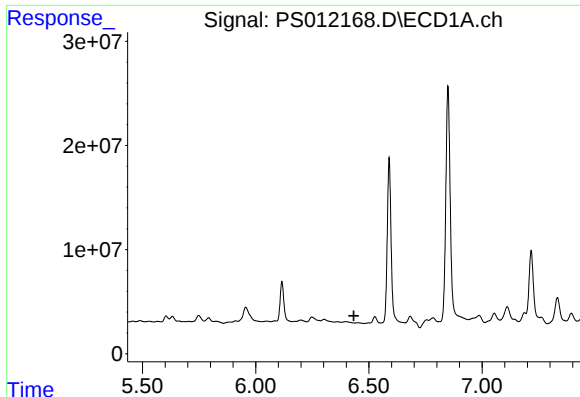

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

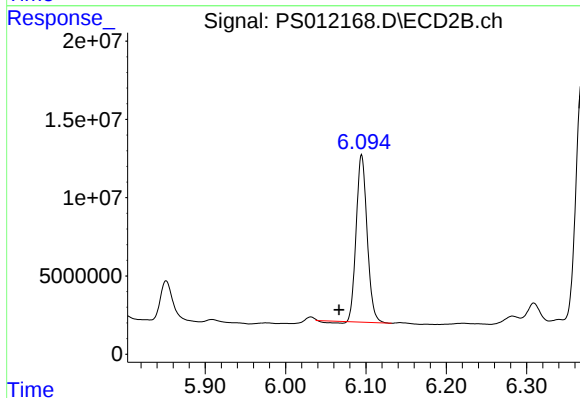


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.095 min
Delta R.T.: 0.028 min
Response: 100669146
Conc: 122.38 ng/ml

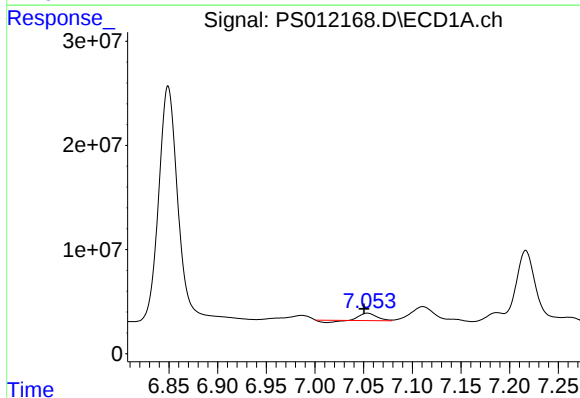


#3 4-Nitrophenol

R.T.: 7.054 min
Delta R.T.: 0.004 min
Response: 7022292
Conc: 11.92 ng/ml

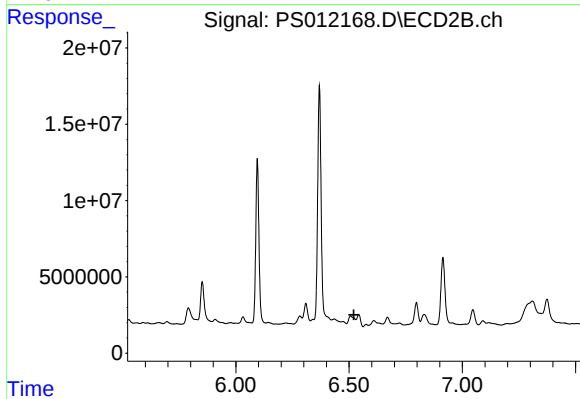

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.521 min
Response: 0
Conc: N.D.

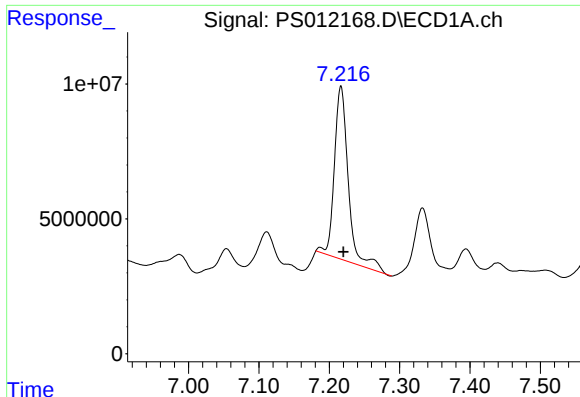

#4 2,4-DCAA


R.T.: 7.217 min
Delta R.T.: -0.003 min
Response: 88473875
Conc: 81.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

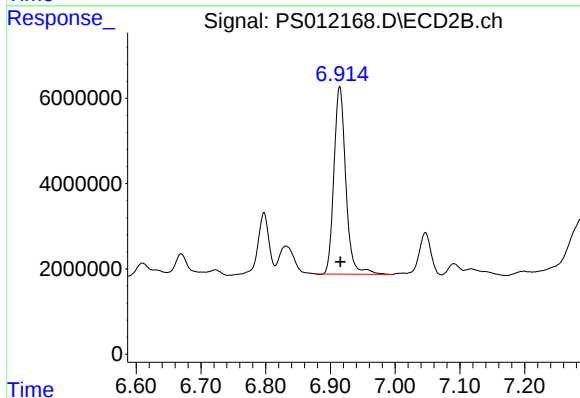


#4 2,4-DCAA

R.T.: 6.914 min
Delta R.T.: 0.000 min
Response: 56033290
Conc: 104.78 ng/ml

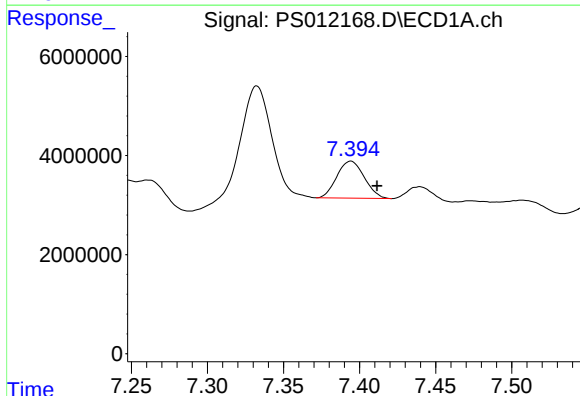


#5 DICAMBA

R.T.: 7.394 min
Delta R.T.: -0.017 min
Response: 9350039
Conc: 2.28 ng/ml

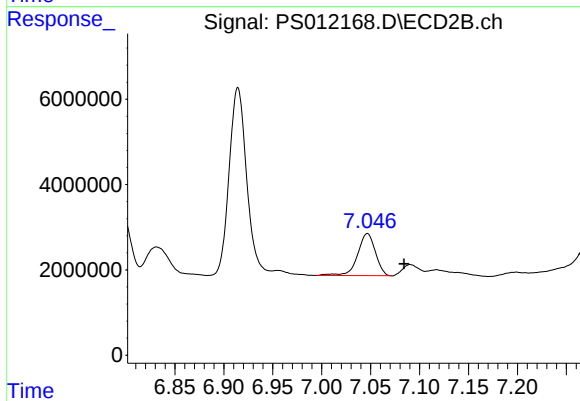

#5 DICAMBA


R.T.: 7.047 min
Delta R.T.: -0.037 min
Response: 12514092
Conc: 5.79 ng/ml

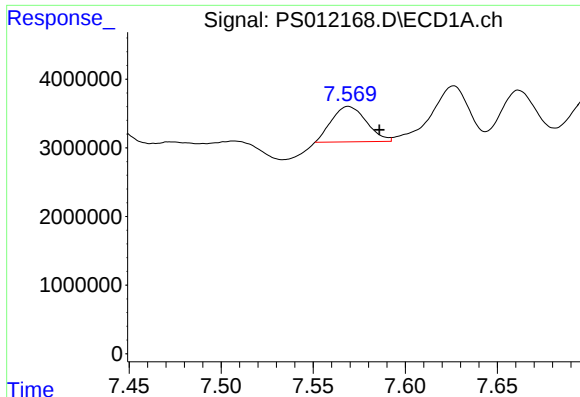

#6 MCPP


R.T.: 7.569 min
Delta R.T.: -0.017 min
Response: 6789502
Conc: 2.12 ug/ml

Instrument :
ECD_S
ClientSampleId :

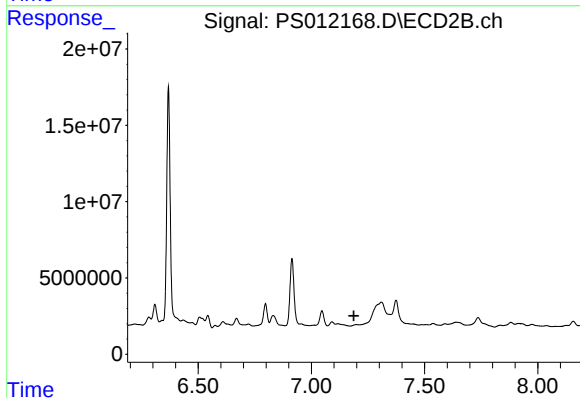


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

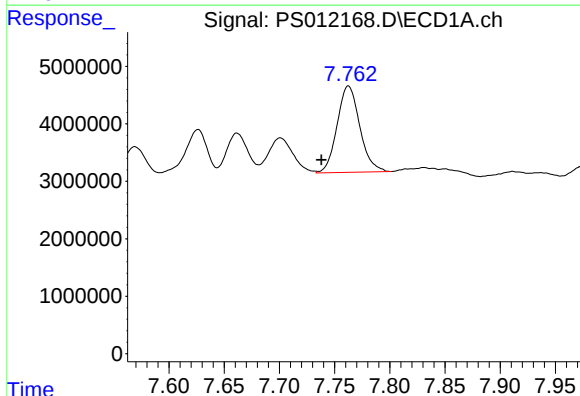


#7 MCPA

R.T.: 7.763 min
Delta R.T.: 0.024 min
Response: 21491172
Conc: 4.72 ug/ml

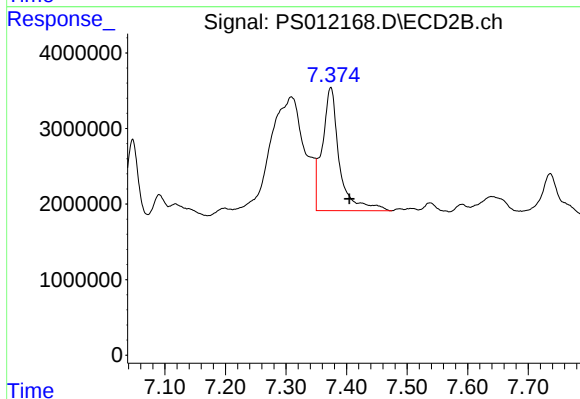

#7 MCPA


R.T.: 7.374 min
Delta R.T.: -0.031 min
Response: 32052746
Conc: 11.70 ug/ml

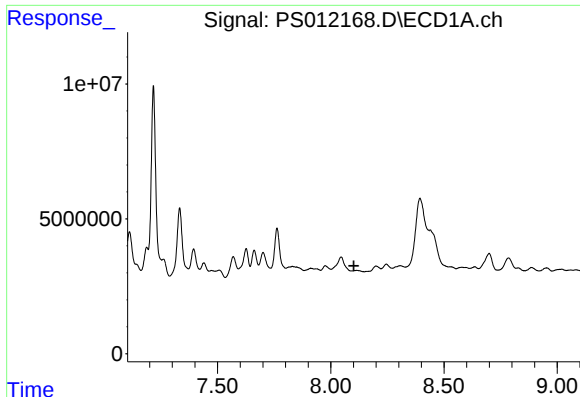

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

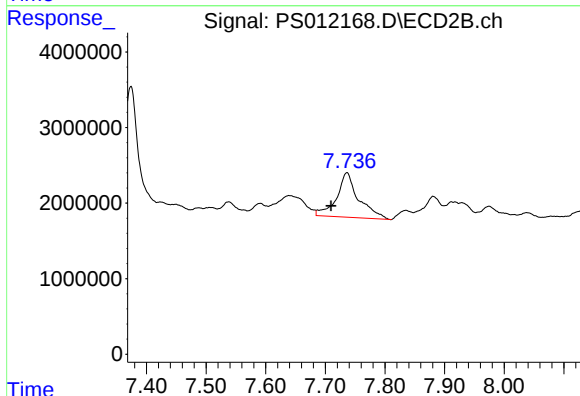


#8 DICHLORPROP

R.T.: 7.736 min
Delta R.T.: 0.027 min
Response: 15077791
Conc: 26.70 ng/ml

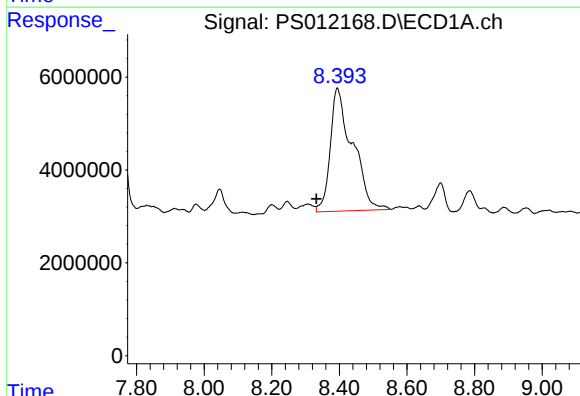


#9 2,4-D

R.T.: 8.394 min
Delta R.T.: 0.062 min
Response: 121042606
Conc: 107.20 ng/ml

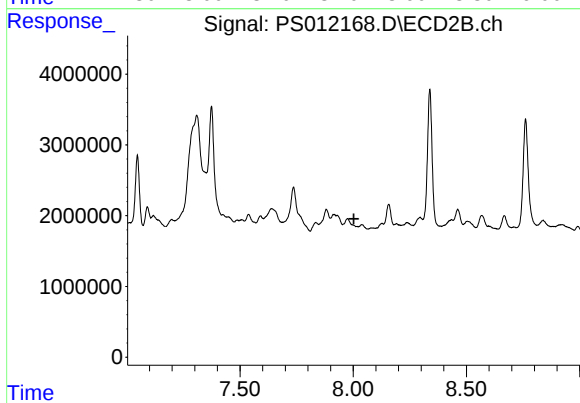

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.003 min
Response: 0
Conc: N.D.

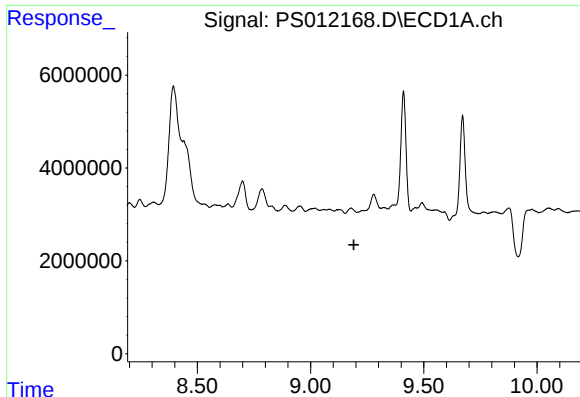

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

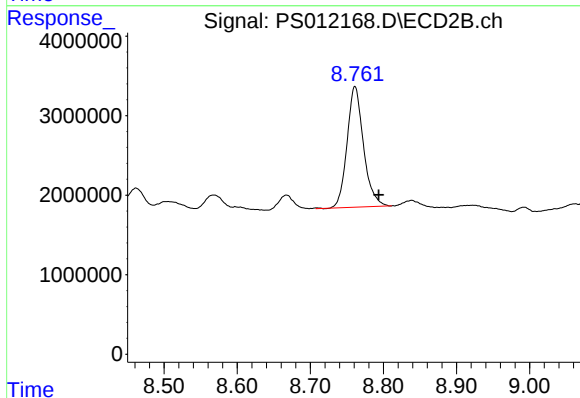


#11 2,4,5-TP (SILVEX)

R.T.: 8.761 min
Delta R.T.: -0.032 min
Response: 23732918
Conc: 8.12 ng/ml

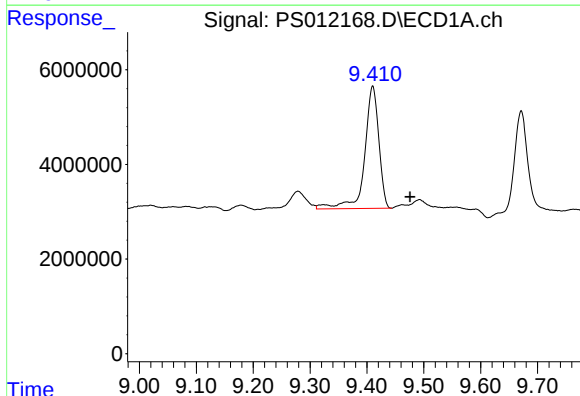


#12 2,4,5-T

R.T.: 9.410 min
Delta R.T.: -0.066 min
Response: 44931360
Conc: 7.58 ng/ml

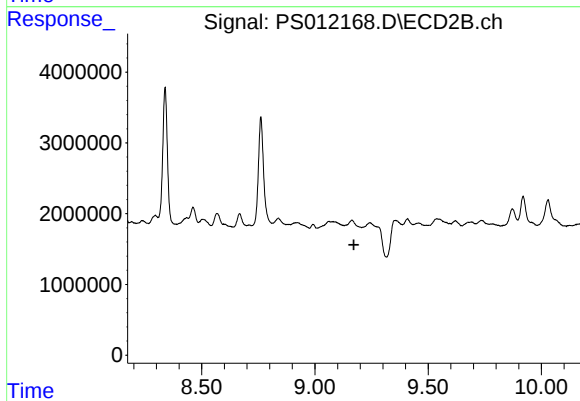

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.172 min
Response: 0
Conc: N.D.

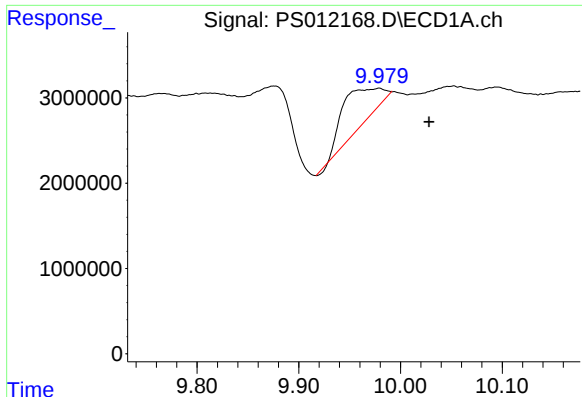

#13 2,4-DB


R.T.: 9.978 min
Delta R.T.: -0.050 min
Response: 10848785
Conc: 13.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

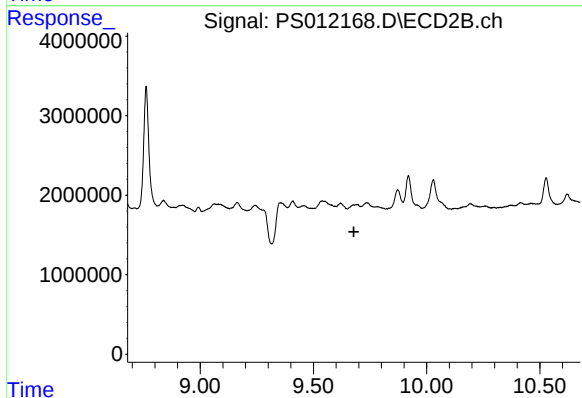


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.679 min
Response: 0
Conc: N.D.

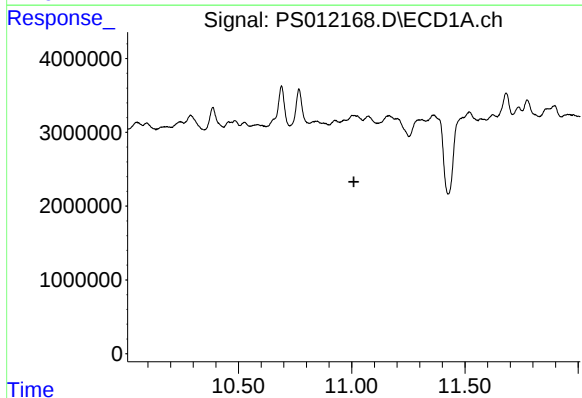


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.009 min
Response: 0
Conc: N.D.

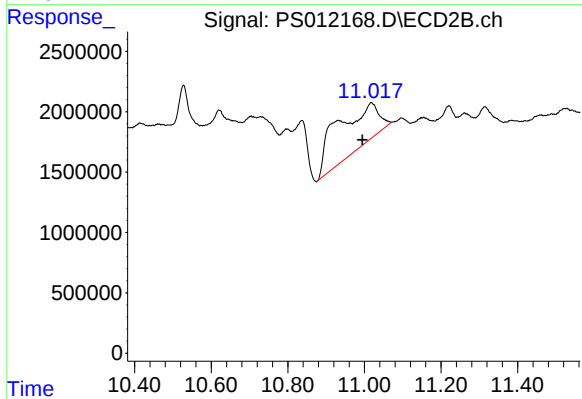

#15 Picloram


R.T.: 11.018 min
Delta R.T.: 0.023 min
Response: 26951758
Conc: 5.95 ng/ml

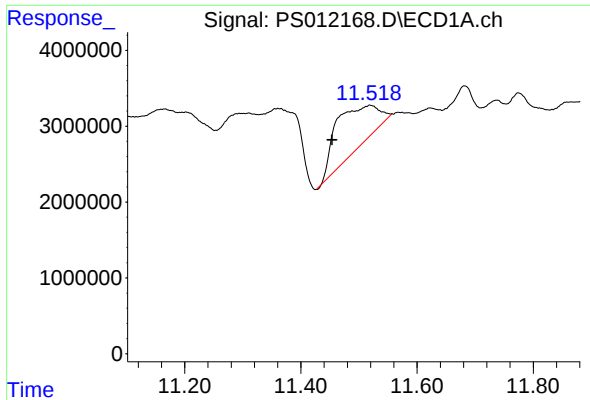

#16 DCPA

R.T.: 11.520 min
Delta R.T.: 0.066 min
Response: 27926694
Conc: 3.67 ng/ml

Instrument :
ECD_S
ClientSampleId :

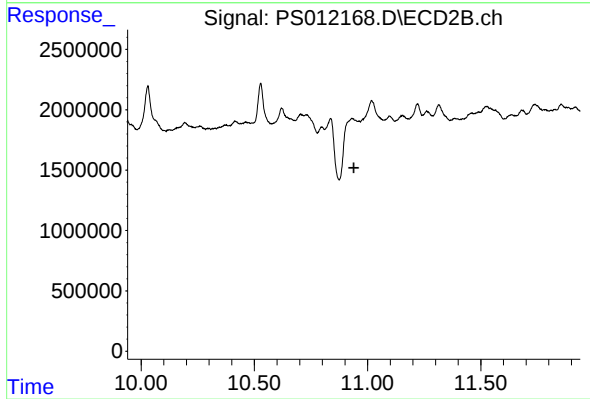

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.940 min
Response: 0
Conc: N.D.