

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090820\
 Data File : PS012146.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Sep 2020 09:57
 Operator : DD\AJ
 Sample : L3871-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TR-05-090220

Manual Integrations
 APPROVED

Ankita
 9/9/2020 10:43:28 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 11:03:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.219	6.912	224.0E6	133.5E6	205.333m	249.609

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090820\
Data File : PS012146.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2020 09:57
Operator : DD\AJ
Sample : L3871-01
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
TR-05-090220


Manual Integrations
APPROVED

Ankita
9/9/2020 10:43:28 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 11:03:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

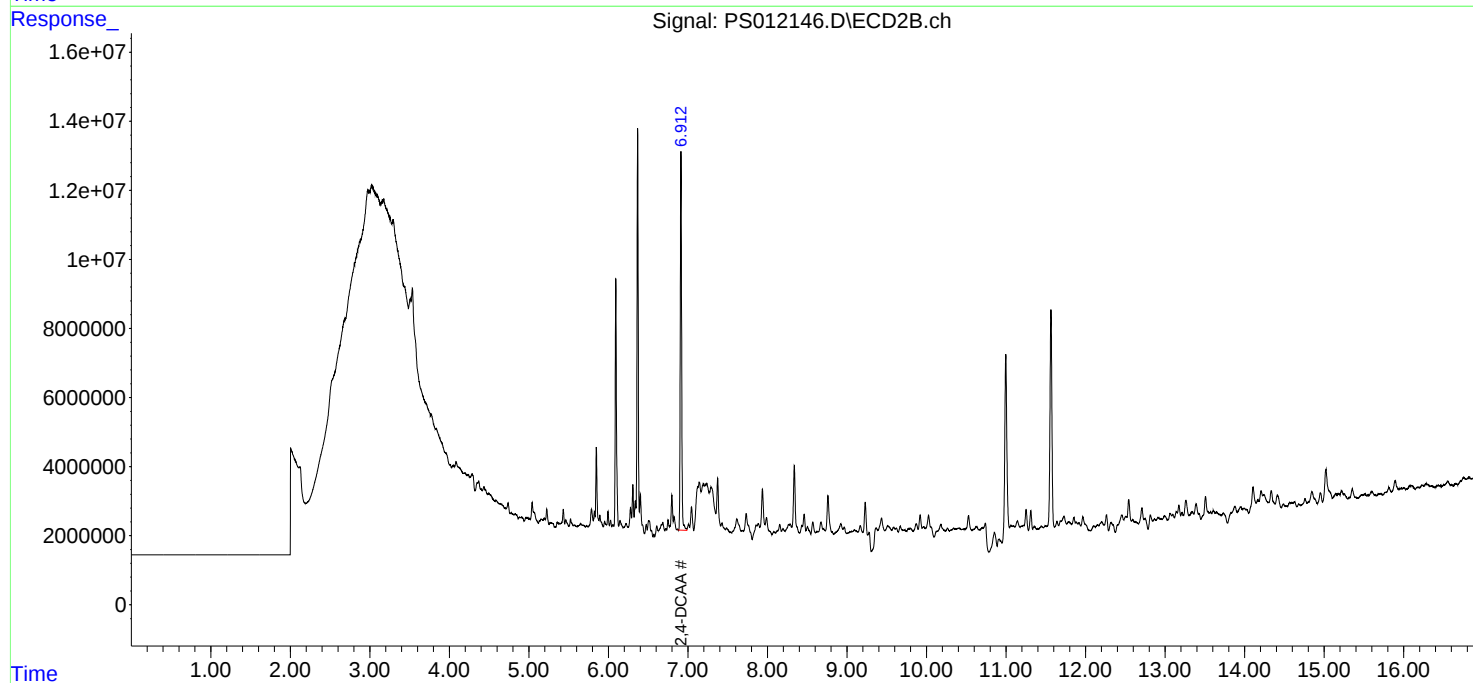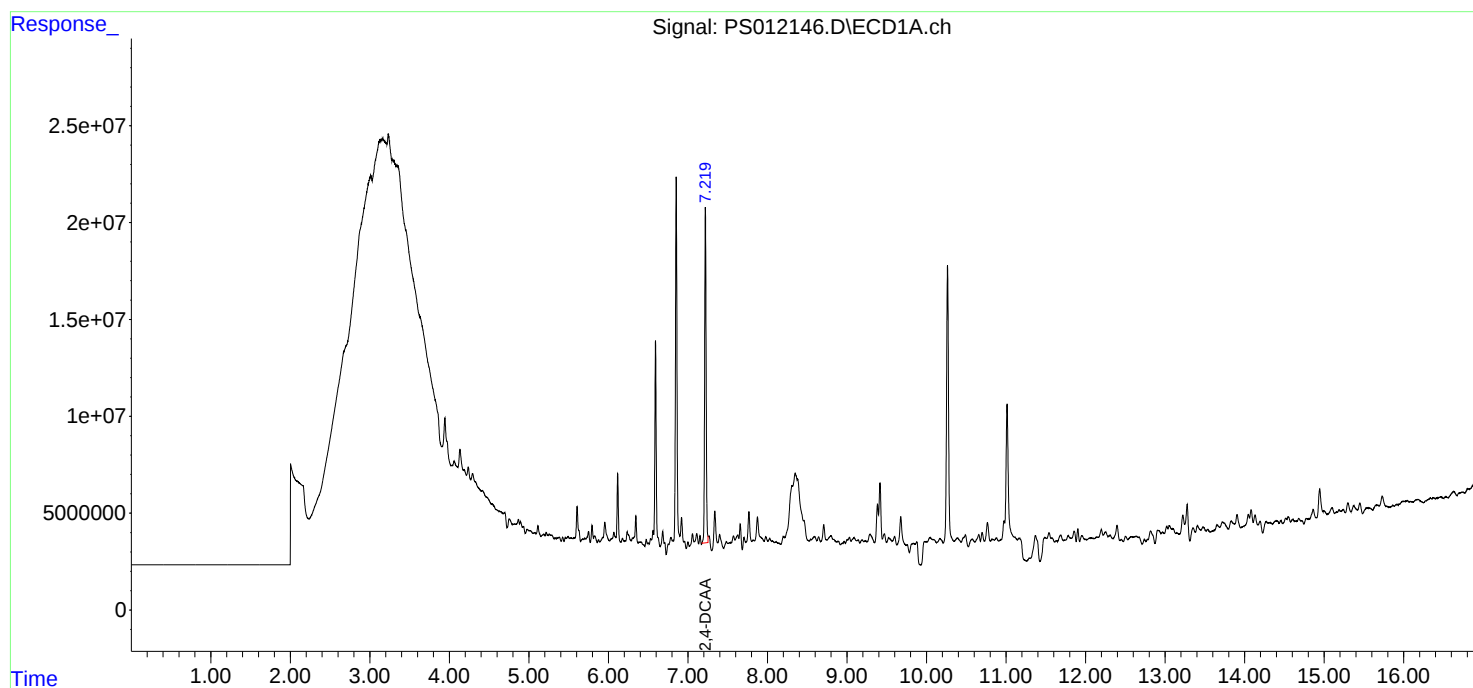

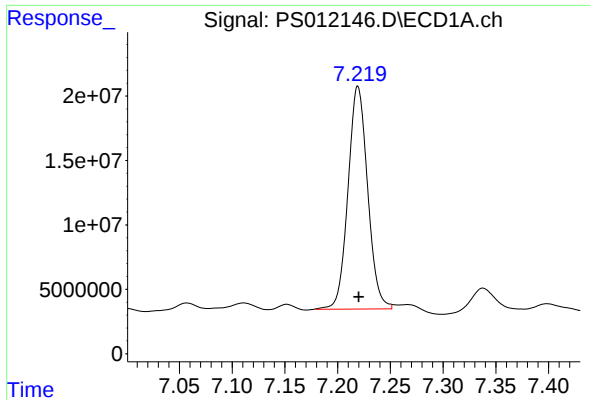


#4 2,4-DCAA

R.T.: 7.219 min
Delta R.T.: -0.001 min
Response: 223970428
Conc: 205.33 ng/ml m

Instrument :
ECD_S
ClientSampleId :
TR-05-090220

Manual Integrations
APPROVED

Ankita
9/9/2020 10:43:28 AM

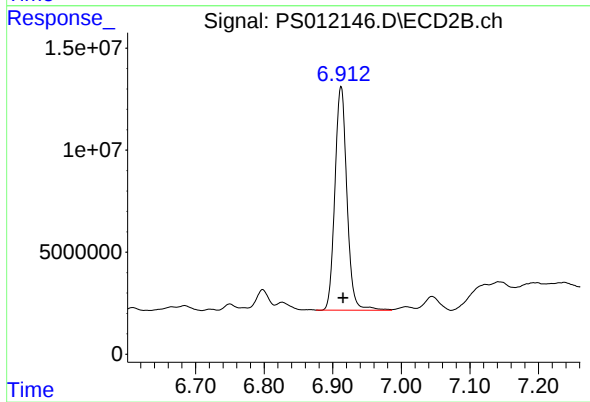

#4 2,4-DCAA

R.T.: 6.912 min
Delta R.T.: -0.003 min
Response: 133487415
Conc: 249.61 ng/ml