

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090825\
 Data File : PS031649.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Sep 2025 20:00
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 03:59:33 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090825.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 09 03:37:51 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.287	7.747	1552.4E6	402.5E6	422.469	476.229
Target Compounds							
1) T	Dalapon	0.000	2.661f	0	59457751	N.D.	21.395
2) T	3,5-DICHL...	6.439	0.000	337704	0	<MDL	N.D. #
6) T	MCP	7.632	0.000	983595	0	<MDL	N.D. #
7) T	MCPA	7.762f	8.235f	5655678	41566574	<MDL	15.548 #
8) T	DICHLORPROP	8.196	0.000	440795	0	<MDL	N.D. #
10) T	Pentachlo...	8.712	9.513	14629634	9292023	<MDL	<MDL #
11) T	2,4,5-TP ...	9.304	9.921f	13019189	12325373	<MDL	<MDL #
12) T	2,4,5-T	9.587	0.000	5736754	0	<MDL	N.D. #
13) T	2,4-DB	10.160	0.000	333505	0	<MDL	N.D. #
14) T	DINOSEB	11.359	11.274	21611502	2887577	1.339	<MDL #
15) T	Picloram	11.179	0.000	718425	0	<MDL	N.D. #
16) T	DCPA	11.656	12.312	18585084	10697463	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090825\
Data File : PS031649.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2025 20:00
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 03:59:33 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090825.M
Quant Title : 8080.M
QLast Update : Tue Sep 09 03:37:51 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

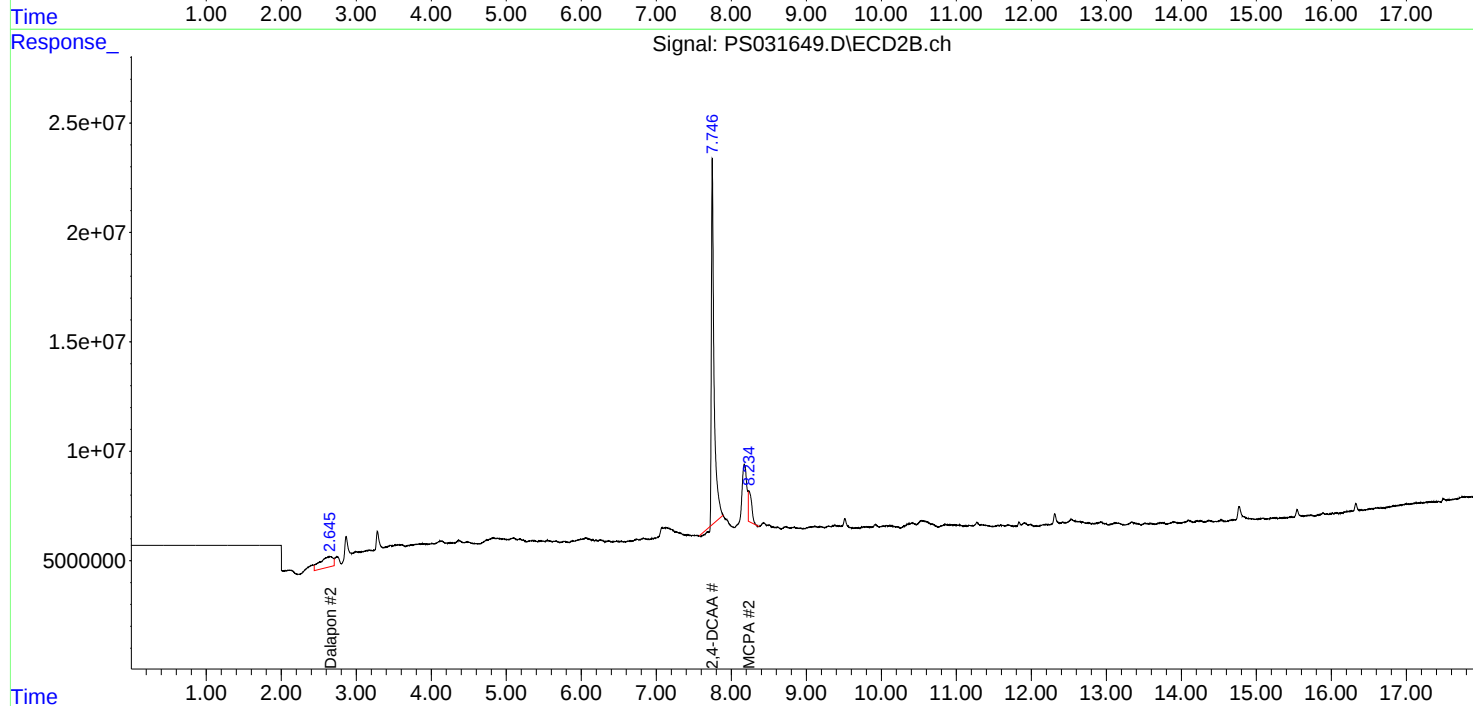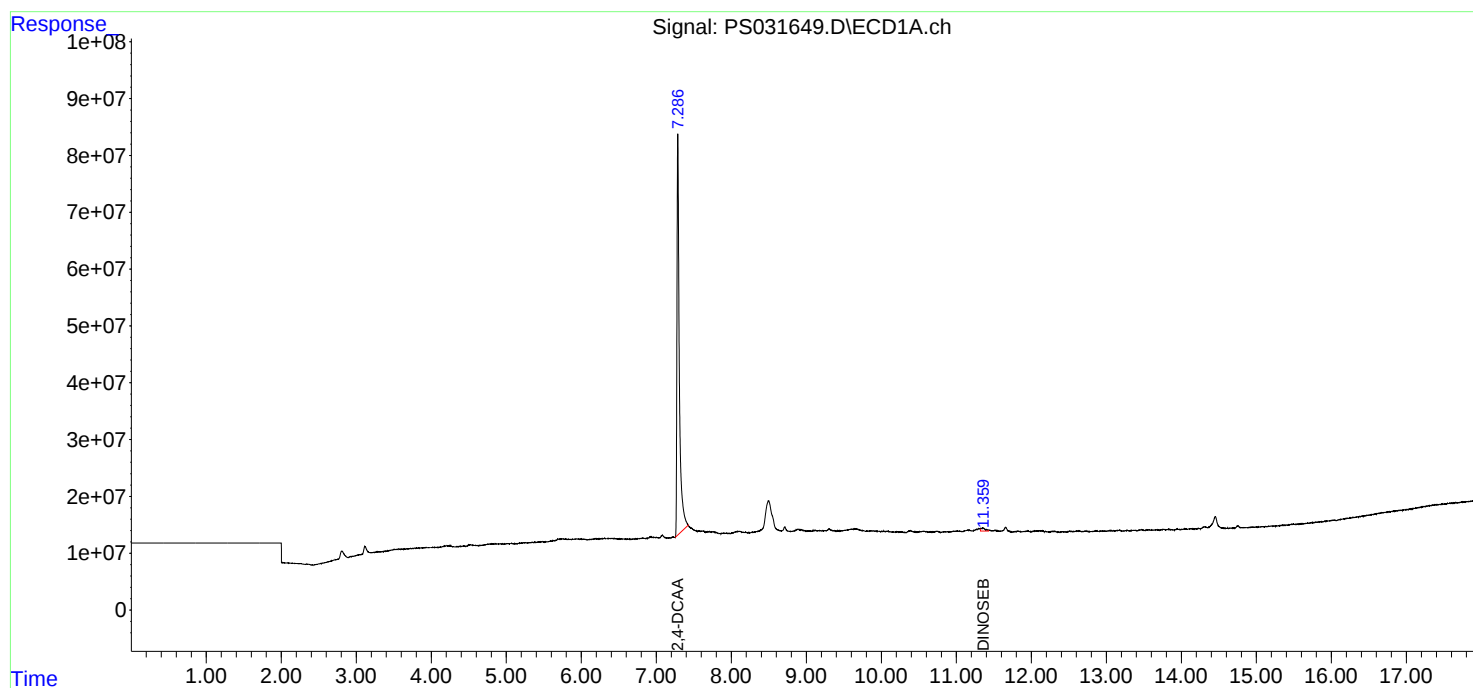


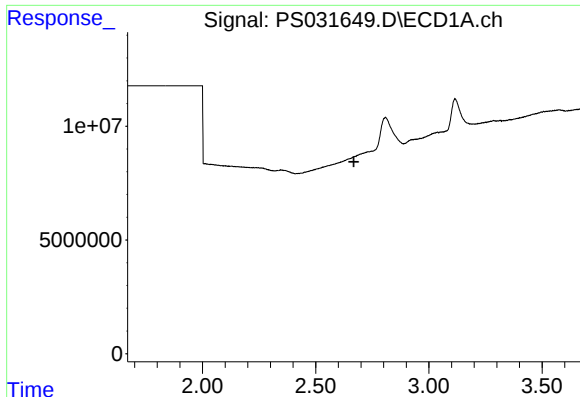

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.669 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

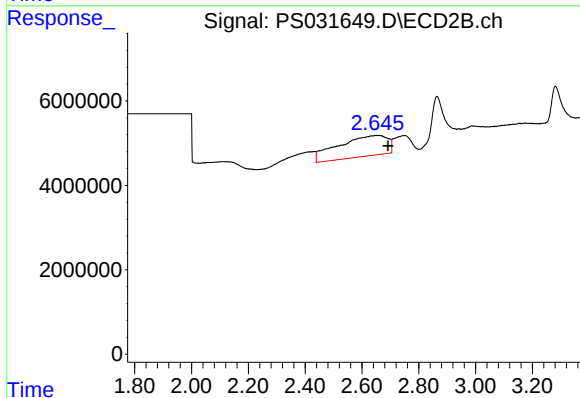


#1 Dalapon

R.T.: 2.661 min
Delta R.T.: -0.032 min
Response: 59457751
Conc: 21.40 ng/ml

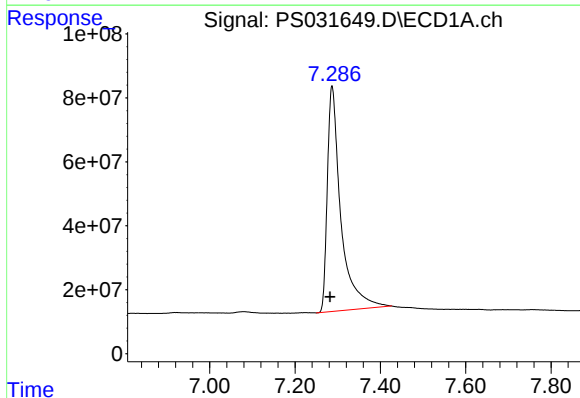


#4 2,4-DCAA

R.T.: 7.287 min
Delta R.T.: 0.005 min
Response: 1552388654
Conc: 422.47 ng/ml

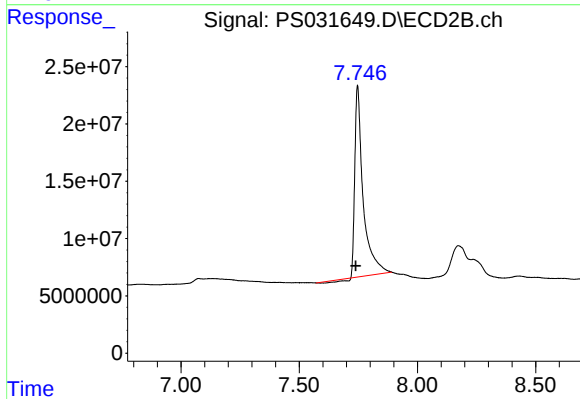

#4 2,4-DCAA


R.T.: 7.747 min
Delta R.T.: 0.008 min
Response: 402505545
Conc: 476.23 ng/ml

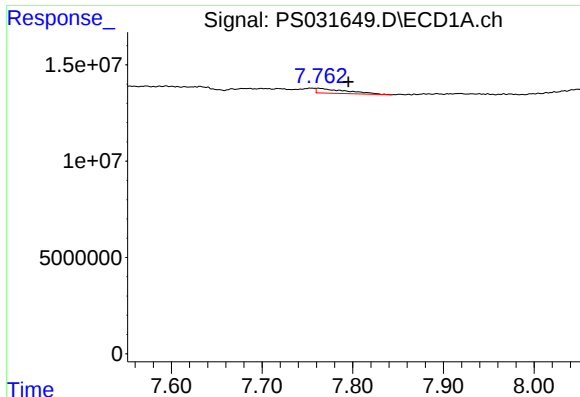

#7 MCPA


R.T.: 7.762 min
Delta R.T.: -0.033 min
Response: 5655678
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

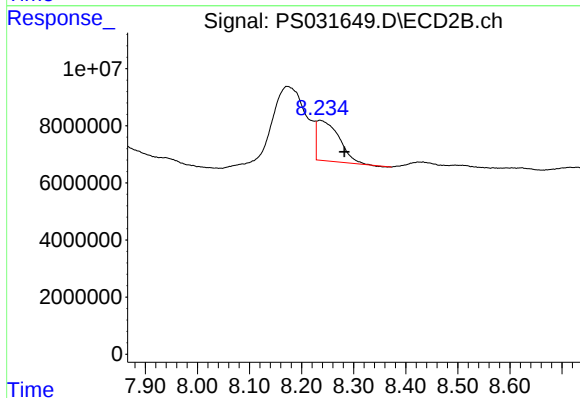


#7 MCPA

R.T.: 8.235 min
Delta R.T.: -0.047 min
Response: 41566574
Conc: 15.55 ug/ml

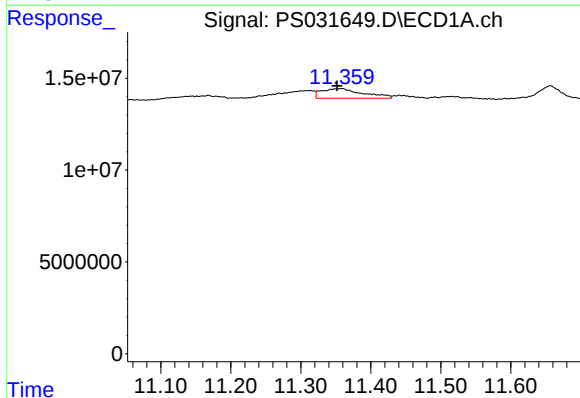

#14 DINOSEB

R.T.: 11.359 min
Delta R.T.: 0.007 min
Response: 21611502
Conc: 1.34 ng/ml

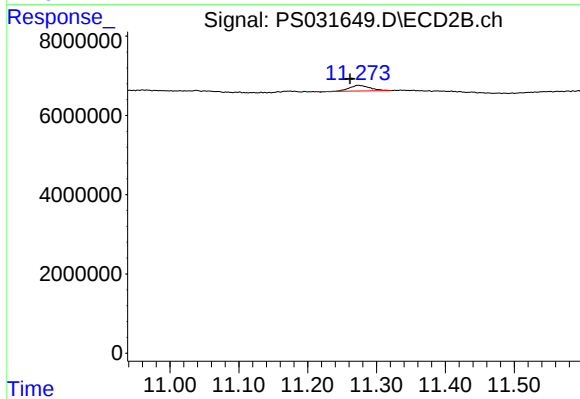

#14 DINOSEB

R.T.: 11.274 min
Delta R.T.: 0.013 min
Response: 2887577
Conc: N.D.