

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090825\
 Data File : PS031664.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2025 02:26
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 04:08:19 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090825.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 09 03:37:51 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.285	7.743	1591.6E6	450.5E6	433.133	533.050
Target Compounds							
1) T	Dalapon	0.000	2.659f	0	64020007	N.D.	23.037
2) T	3,5-DICHL...	6.448	0.000	463677	0	<MDL	N.D. #
7) T	MCPA	7.754f	8.234f	28788389	26847544	2.638	10.042 #
8) T	DICHLORPROP	8.190	8.686f	656248	1422972	<MDL	<MDL #
9) T	2,4-D	0.000	8.996	0	6687792	N.D.	4.486
10) T	Pentachlo...	8.707	9.510	9326814	7386252	<MDL	<MDL #
11) T	2,4,5-TP ...	9.293	9.903	7335626	3180304	<MDL	<MDL #
12) T	2,4,5-T	9.625f	0.000	19843835	0	1.101	N.D. #
13) T	2,4-DB	10.189f	0.000	2678830	0	1.353	N.D. #
14) T	DINOSEB	11.352	0.000	6763504	0	<MDL	N.D. #
15) T	Picloram	11.167	0.000	2382254	0	<MDL	N.D. #
16) T	DCPA	11.652	0.000	10467427	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090825\
Data File : PS031664.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2025 02:26
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 04:08:19 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090825.M
Quant Title : 8080.M
QLast Update : Tue Sep 09 03:37:51 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

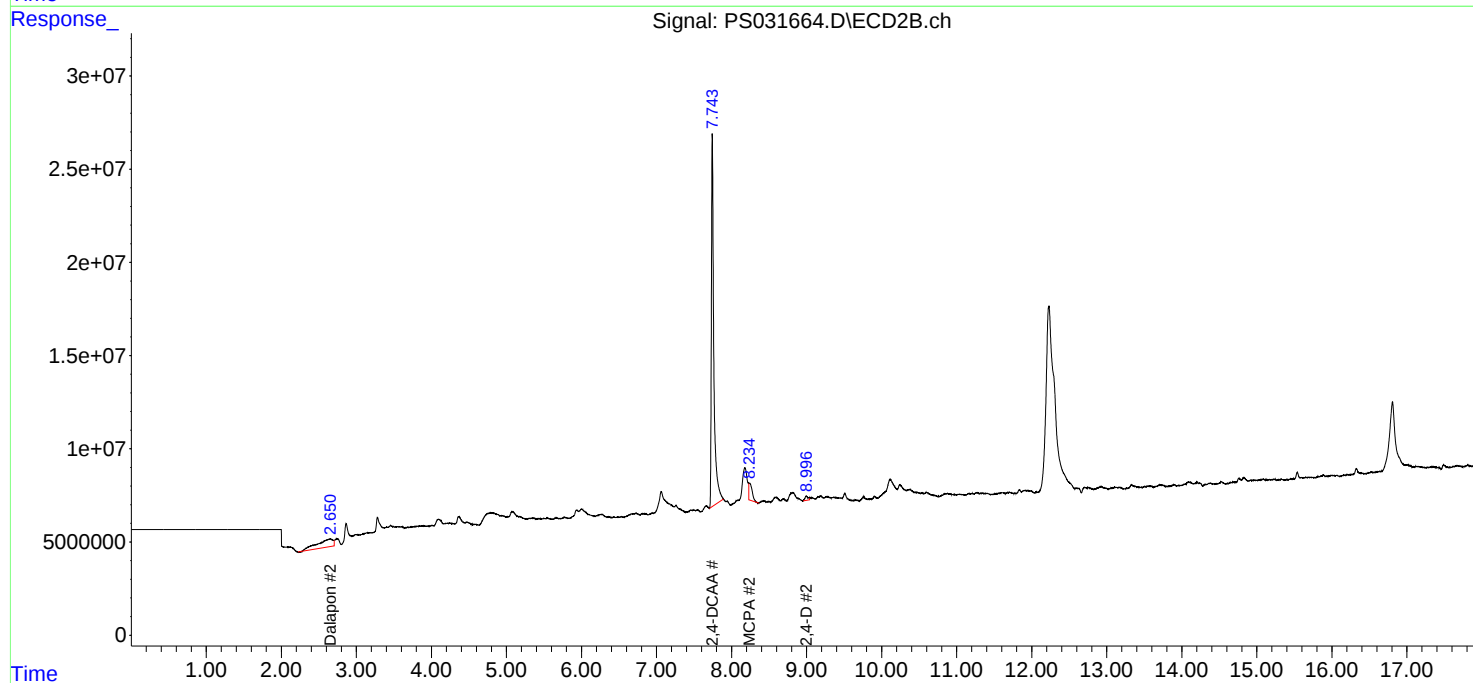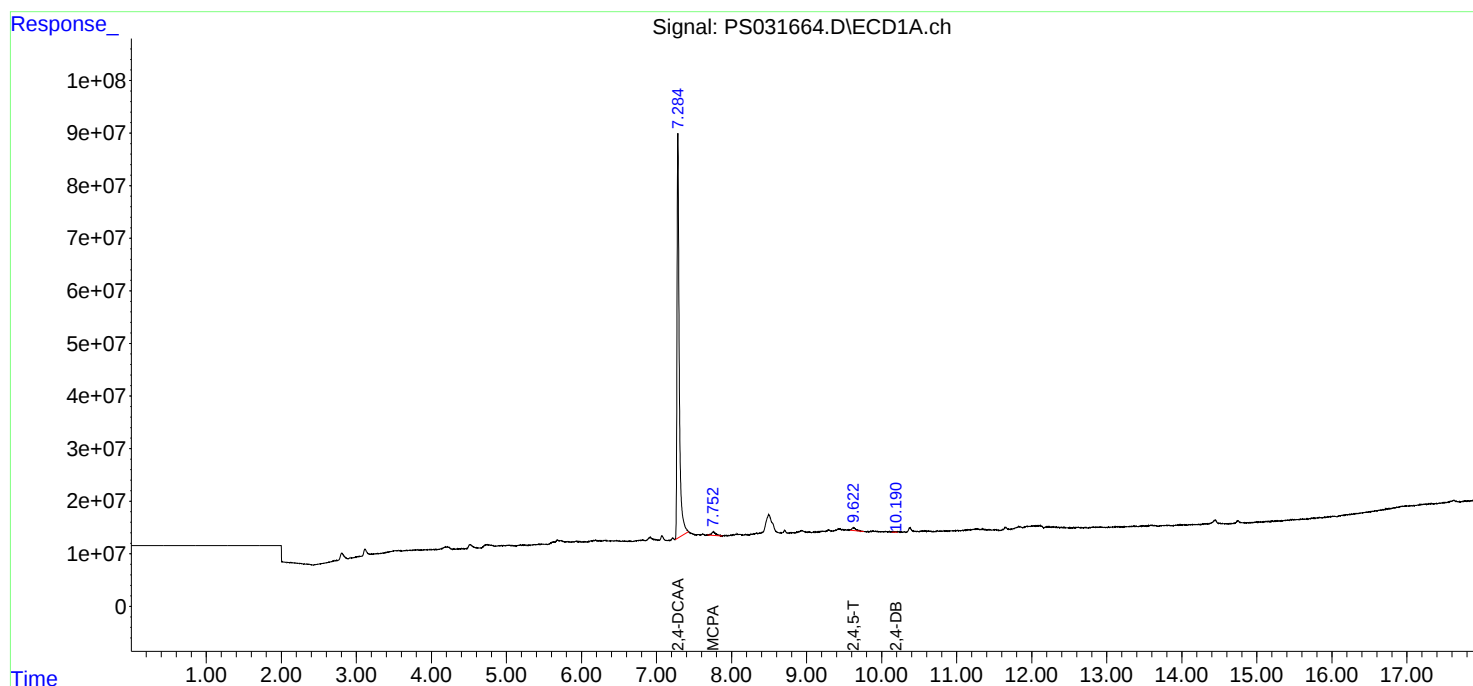


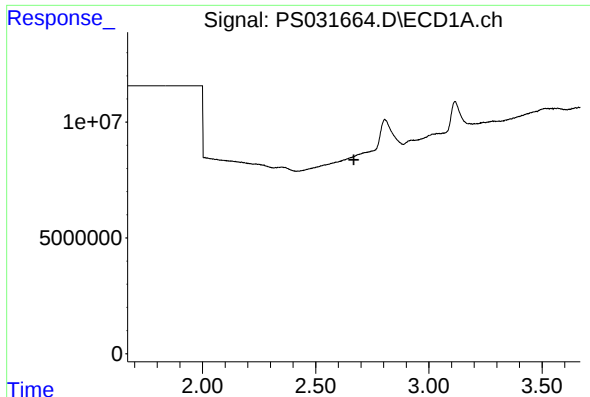

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.669 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

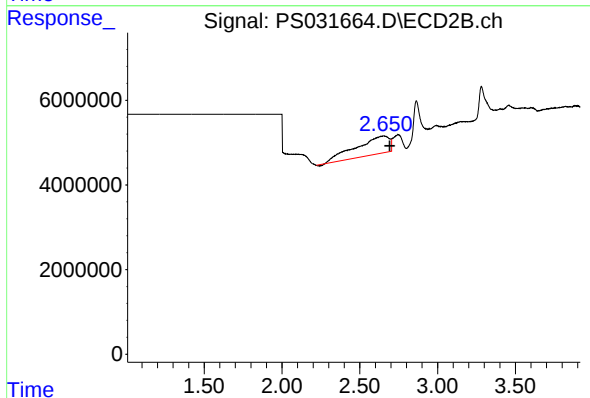


#1 Dalapon

R.T.: 2.659 min
Delta R.T.: -0.034 min
Response: 64020007
Conc: 23.04 ng/ml

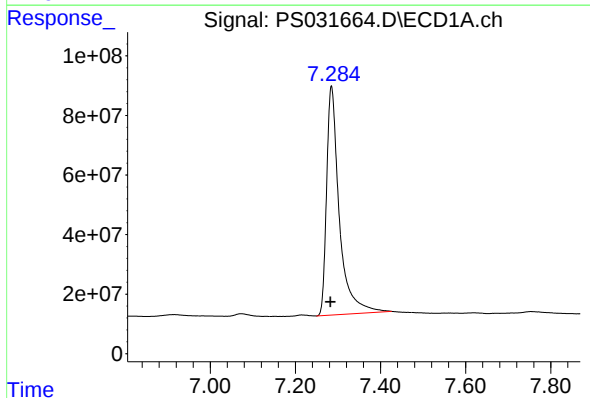


#4 2,4-DCAA

R.T.: 7.285 min
Delta R.T.: 0.003 min
Response: 1591571724
Conc: 433.13 ng/ml

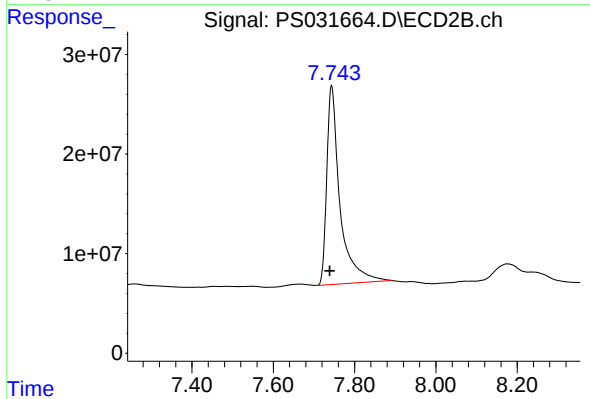

#4 2,4-DCAA


R.T.: 7.743 min
Delta R.T.: 0.005 min
Response: 450530448
Conc: 533.05 ng/ml

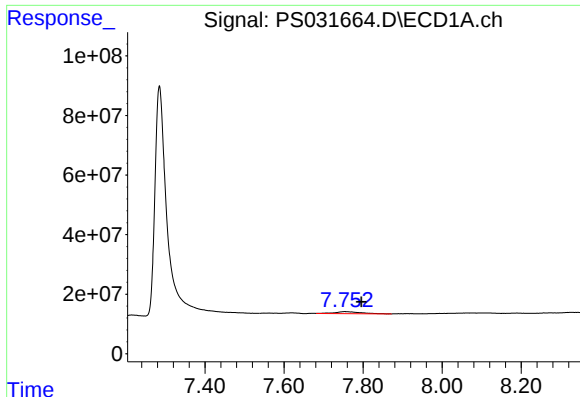

#7 MCPA


R.T.: 7.754 min
Delta R.T.: -0.042 min
Response: 28788389
Conc: 2.64 ug/ml

Instrument :
ECD_S
ClientSampleId :

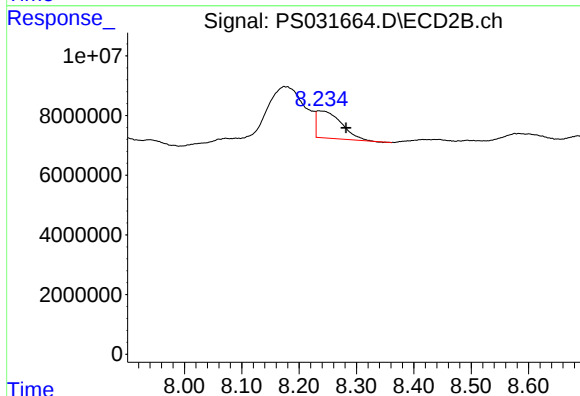


#7 MCPA

R.T.: 8.234 min
Delta R.T.: -0.048 min
Response: 26847544
Conc: 10.04 ug/ml

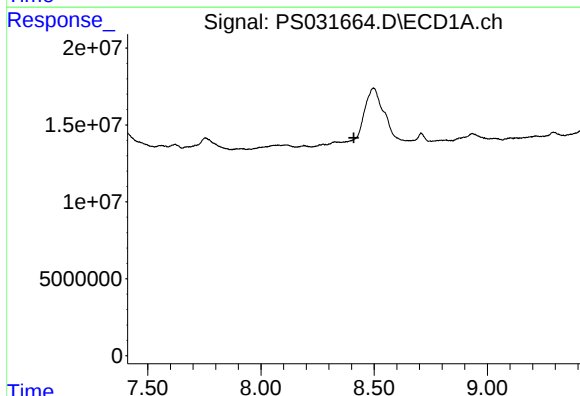


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.410 min
Response: 0
Conc: N.D.

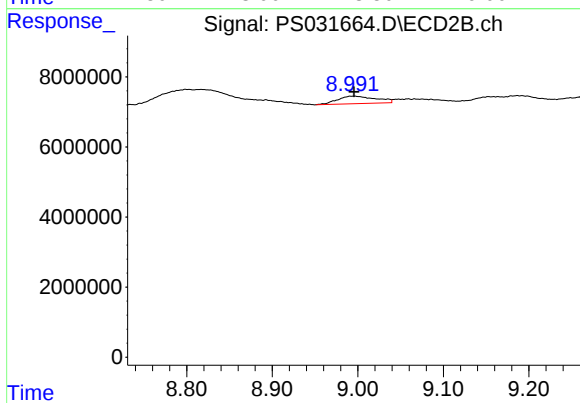

#9 2,4-D


R.T.: 8.996 min
Delta R.T.: 0.000 min
Response: 6687792
Conc: 4.49 ng/ml

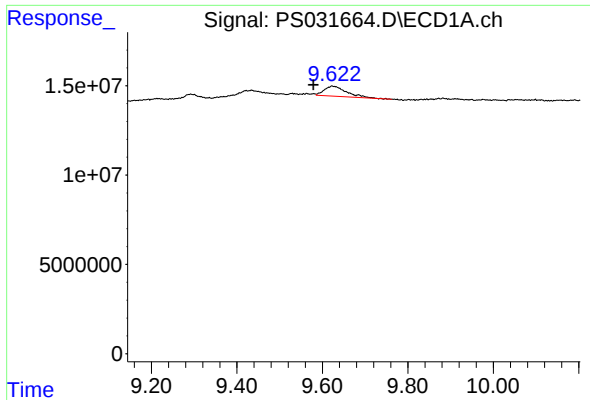

#12 2,4,5-T


R.T.: 9.625 min
Delta R.T.: 0.046 min
Response: 19843835
Conc: 1.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

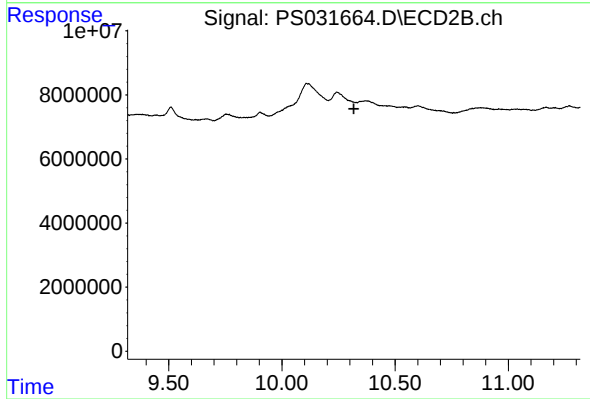


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 10.318 min
Response: 0
Conc: N.D.

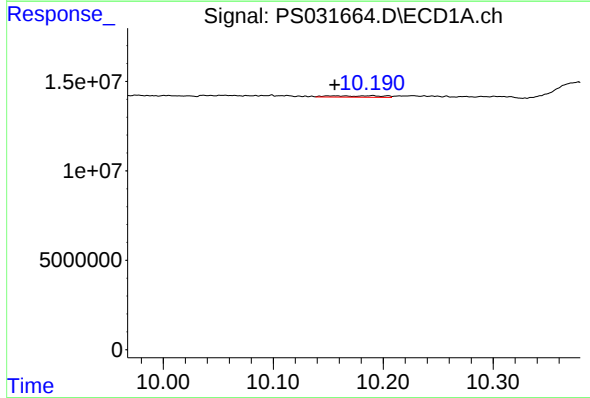

#13 2,4-DB

R.T.: 10.189 min
Delta R.T.: 0.033 min
Response: 2678830
Conc: 1.35 ng/ml

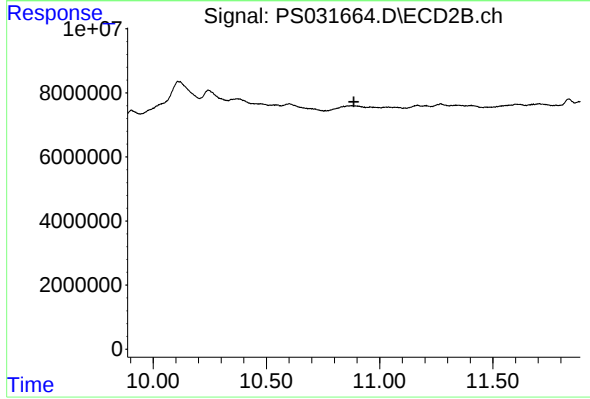

#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.886 min
Response: 0
Conc: N.D.