

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090919\
 Data File : PS006623.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2019 18:12
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 06:31:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 10 06:14:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.502	5.230	300.7E6	170.6E6	386.998	399.425
Target Compounds							
7) T	MCPA	0.000	5.554	0 74380744		N.D.	42.406
9) T	2,4-D	6.564	0.000	153.7E6	0	198.944	N.D. #
10) T	Pentachlo...	6.761	0.000	9947239	0	<MDL	N.D. #
15) T	Picloram	9.067	9.012	47159910	36281570	6.991	9.804 #
16) T	DCPA	0.000	9.012	0 36281570		N.D.	11.517



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090919\
Data File : PS006623.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2019 18:12
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 06:31:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
Quant Title : 8080.M
QLast Update : Tue Sep 10 06:14:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

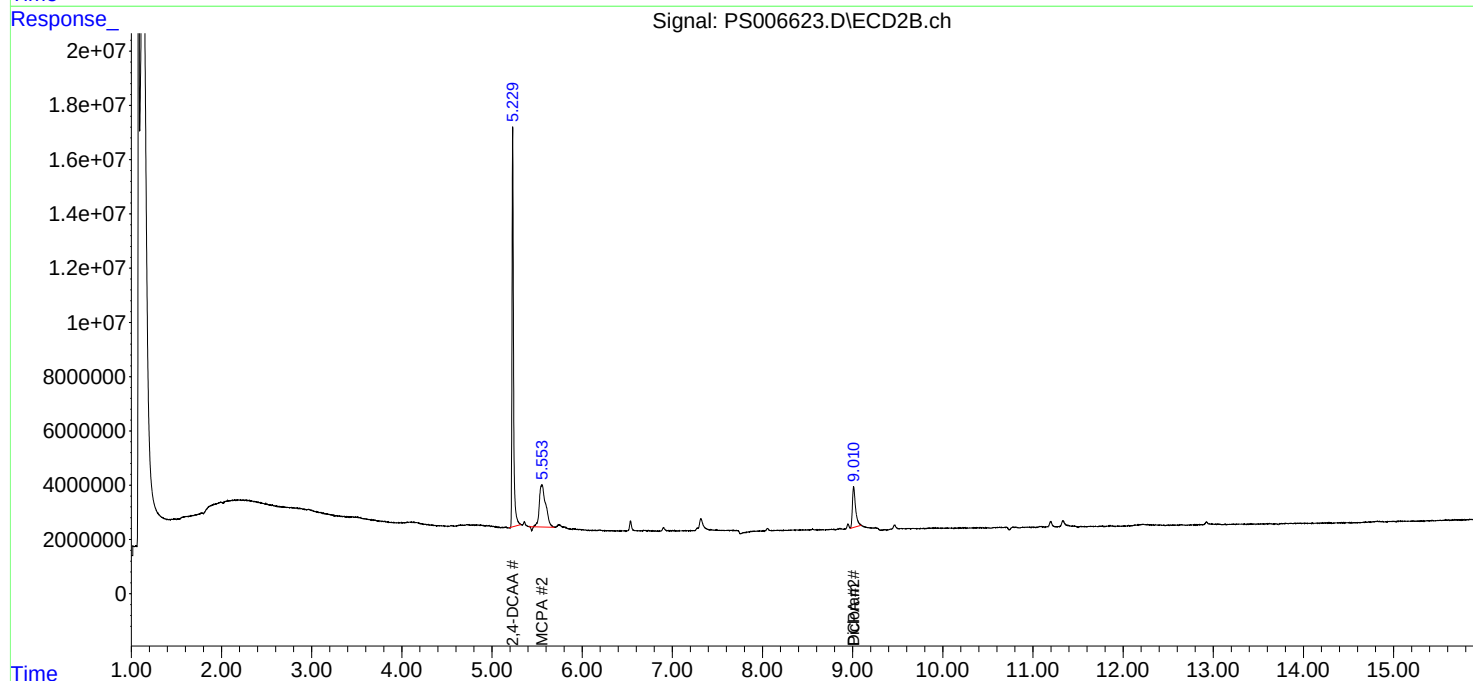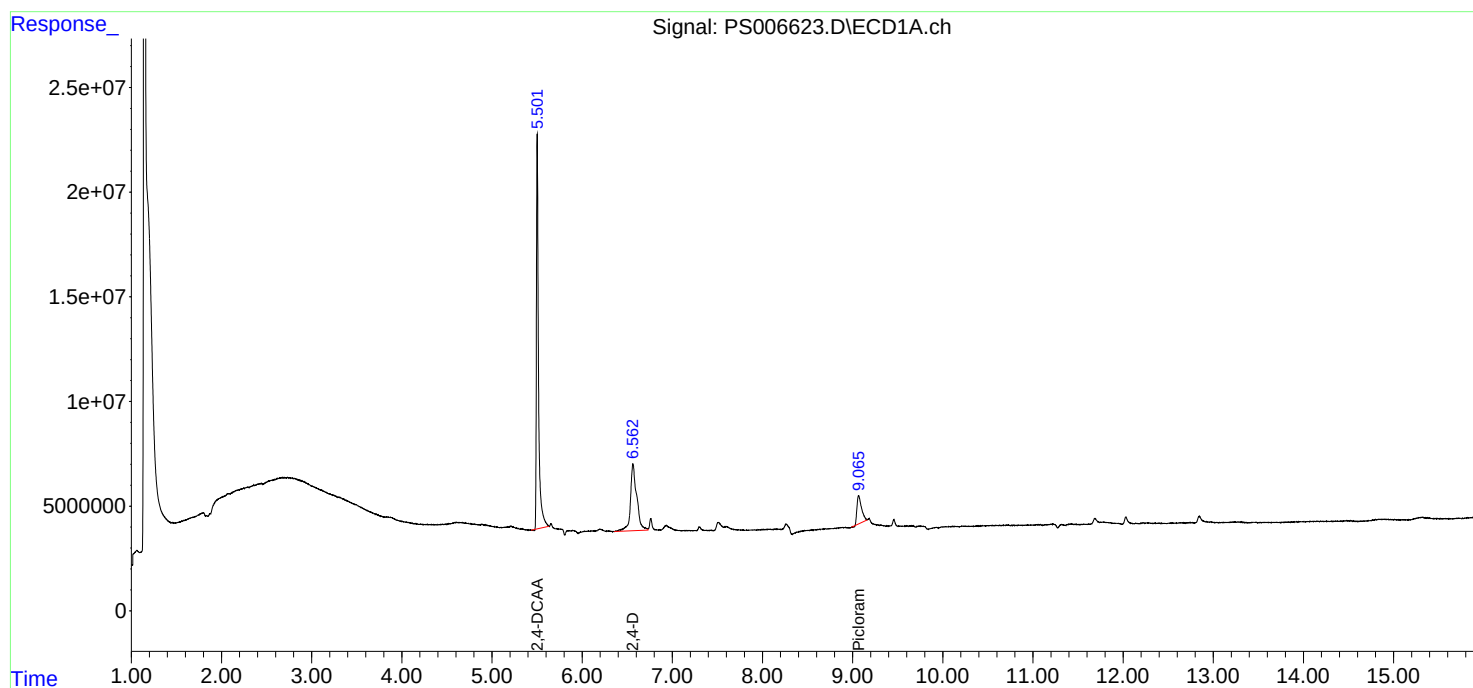


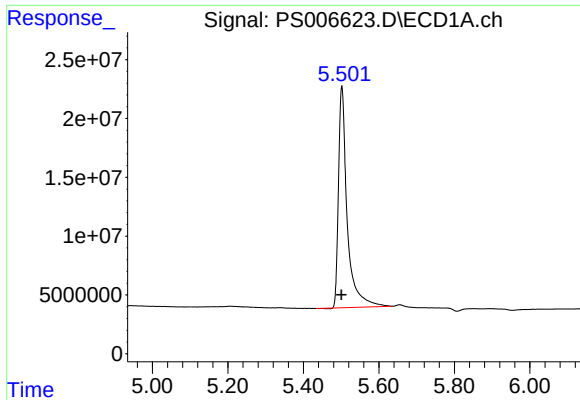

#4 2,4-DCAA


R.T.: 5.502 min
Delta R.T.: 0.001 min
Response: 300653459
Conc: 387.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

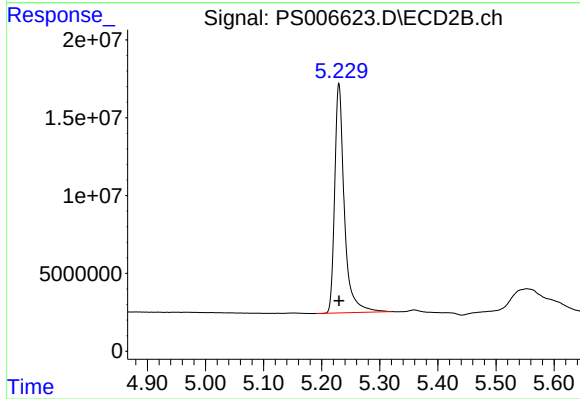


#4 2,4-DCAA

R.T.: 5.230 min
Delta R.T.: 0.000 min
Response: 170555653
Conc: 399.43 ng/ml

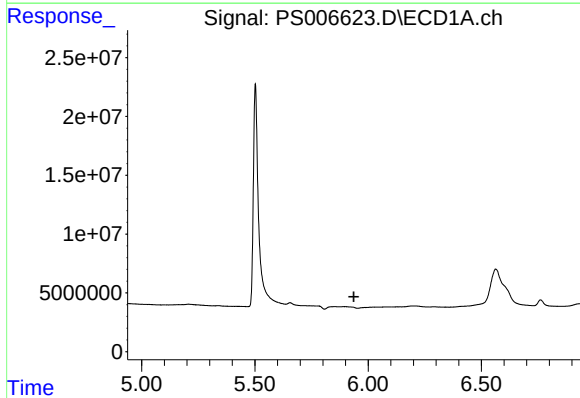


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.937 min
Response: 0
Conc: N.D.

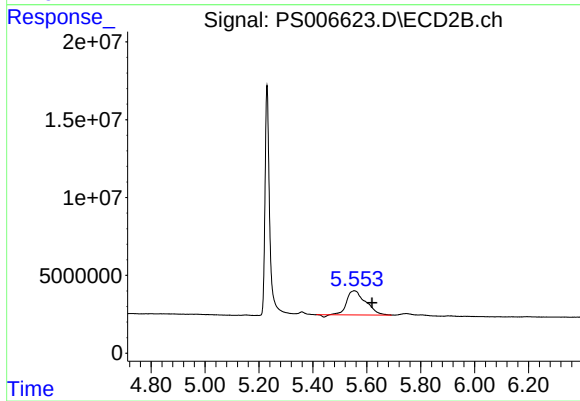

#7 MCPA


R.T.: 5.554 min
Delta R.T.: -0.066 min
Response: 74380744
Conc: 42.41 ug/ml

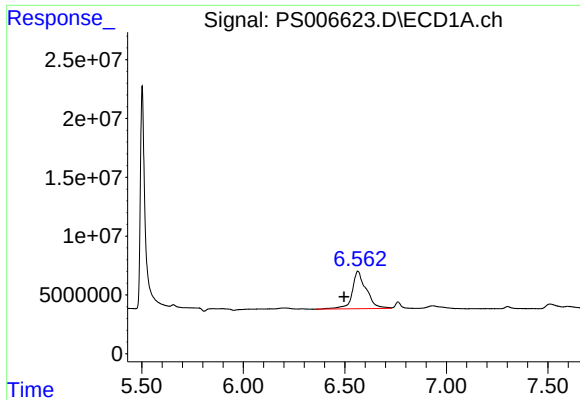

#9 2,4-D


R.T.: 6.564 min
Delta R.T.: 0.067 min
Response: 153708407
Conc: 198.94 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

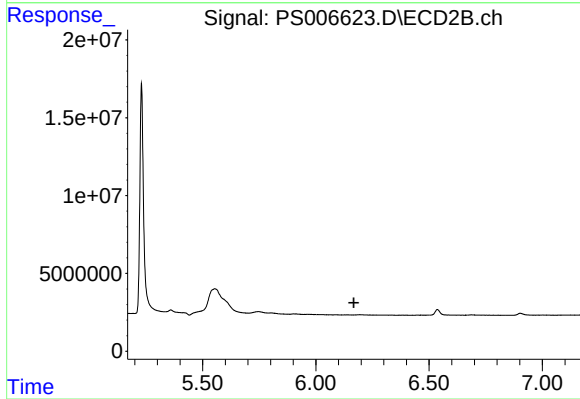


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 6.168 min
Response: 0
Conc: N.D.

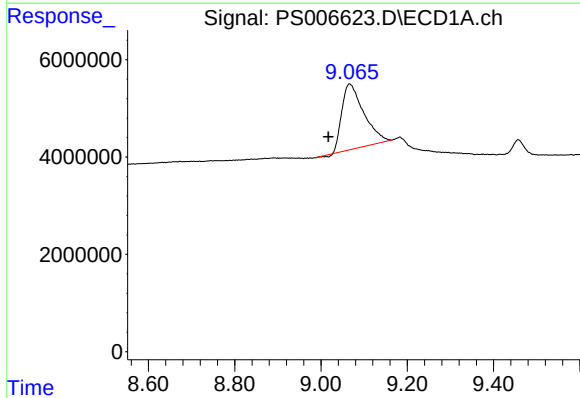


#15 Picloram

R.T.: 9.067 min
Delta R.T.: 0.049 min
Response: 47159910
Conc: 6.99 ng/ml

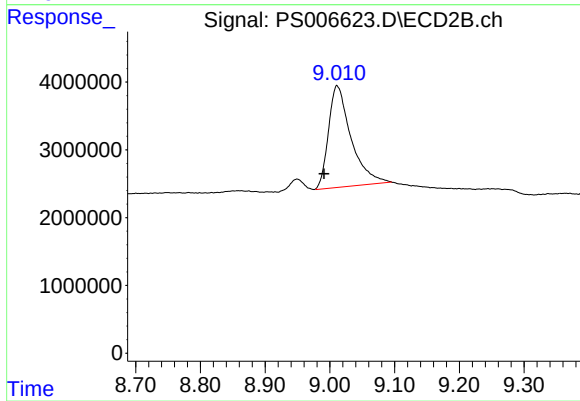

#15 Picloram


R.T.: 9.012 min
Delta R.T.: 0.020 min
Response: 36281570
Conc: 9.80 ng/ml

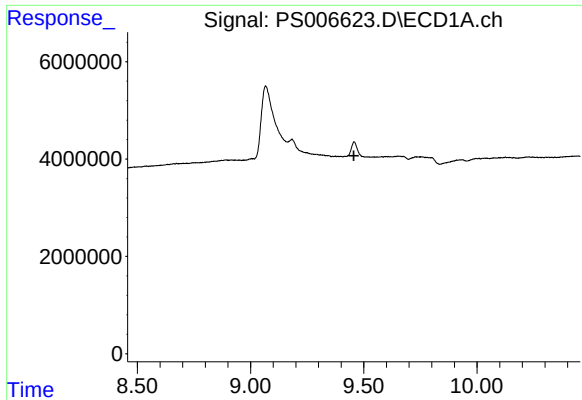

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.456 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

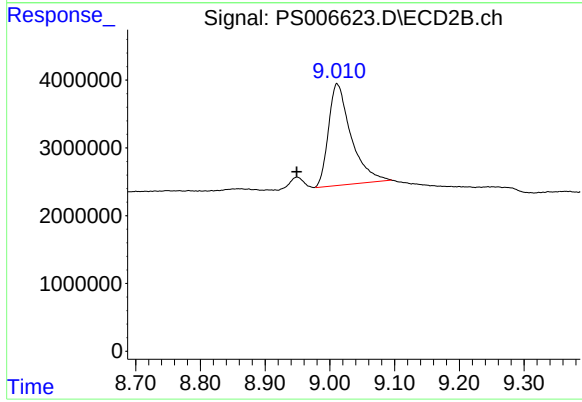

#16 DCPA

R.T.: 9.012 min
Delta R.T.: 0.063 min
Response: 36281570
Conc: 11.52 ng/ml