

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090919\
 Data File : PS006625.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2019 18:55
 Operator : SM\AJ
 Sample : PB122925BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB122925BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 06:32:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 10 06:14:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.482	5.211	648.0E6	382.0E6	834.160	894.502
Target Compounds							
1) T	Dalapon	2.026	1.739	64489756	36109212	65.981	70.657
2) T	3,5-DICHL...	0.000	4.540	0	15767812	N.D.	29.132
7) T	MCPA	5.958	5.589	15289479	24731589	5.410	14.100 #
9) T	2,4-D	6.547	0.000	145.8E6	0	188.696	N.D. #
10) T	Pentachlo...	6.744	0.000	13925134	0	1.250	N.D. #
11) T	2,4,5-TP ...	0.000	6.838	0	6224718	N.D.	2.734
15) T	Picloram	9.041	8.992	120.2E6	46724029	17.811	12.626 #
16) T	DCPA	9.439	8.992	105.9E6	46724029	18.754	14.832



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090919\
Data File : PS006625.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2019 18:55
Operator : SM\AJ
Sample : PB122925BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
PB122925BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 06:32:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
Quant Title : 8080.M
QLast Update : Tue Sep 10 06:14:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

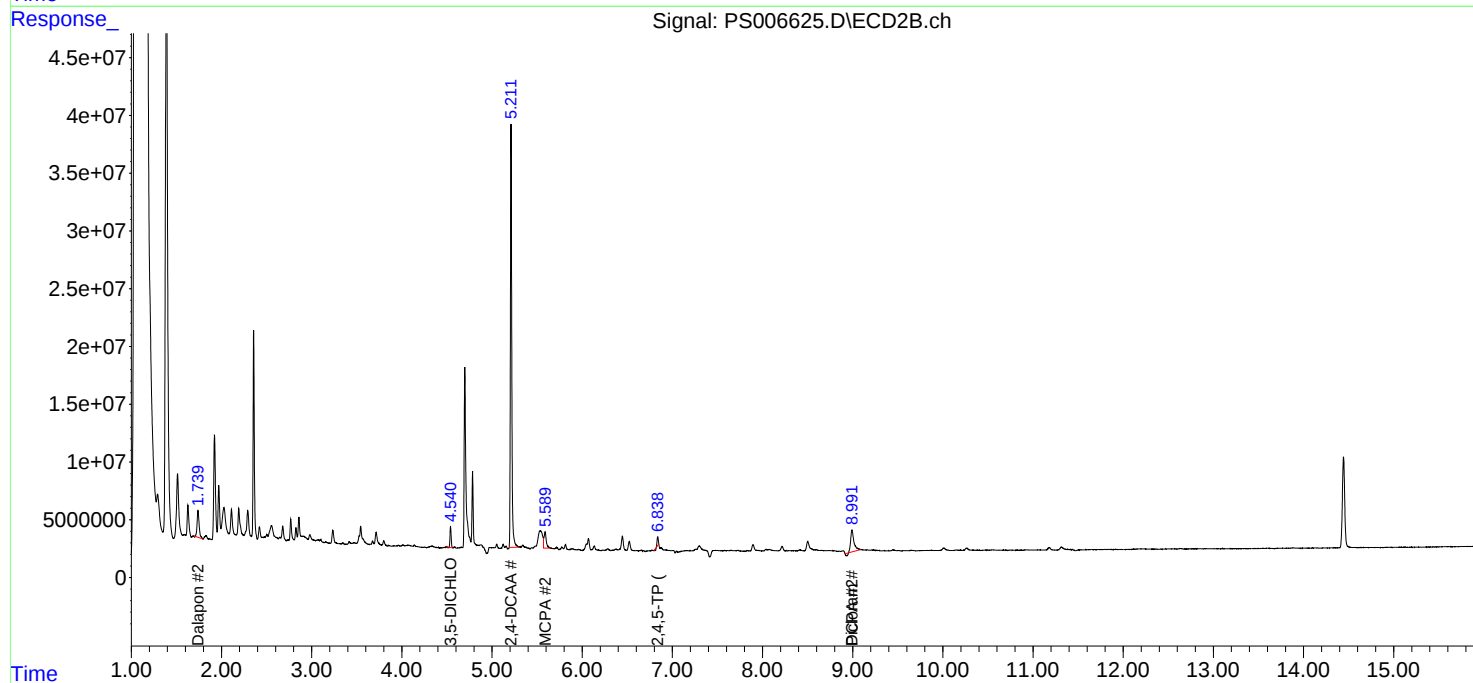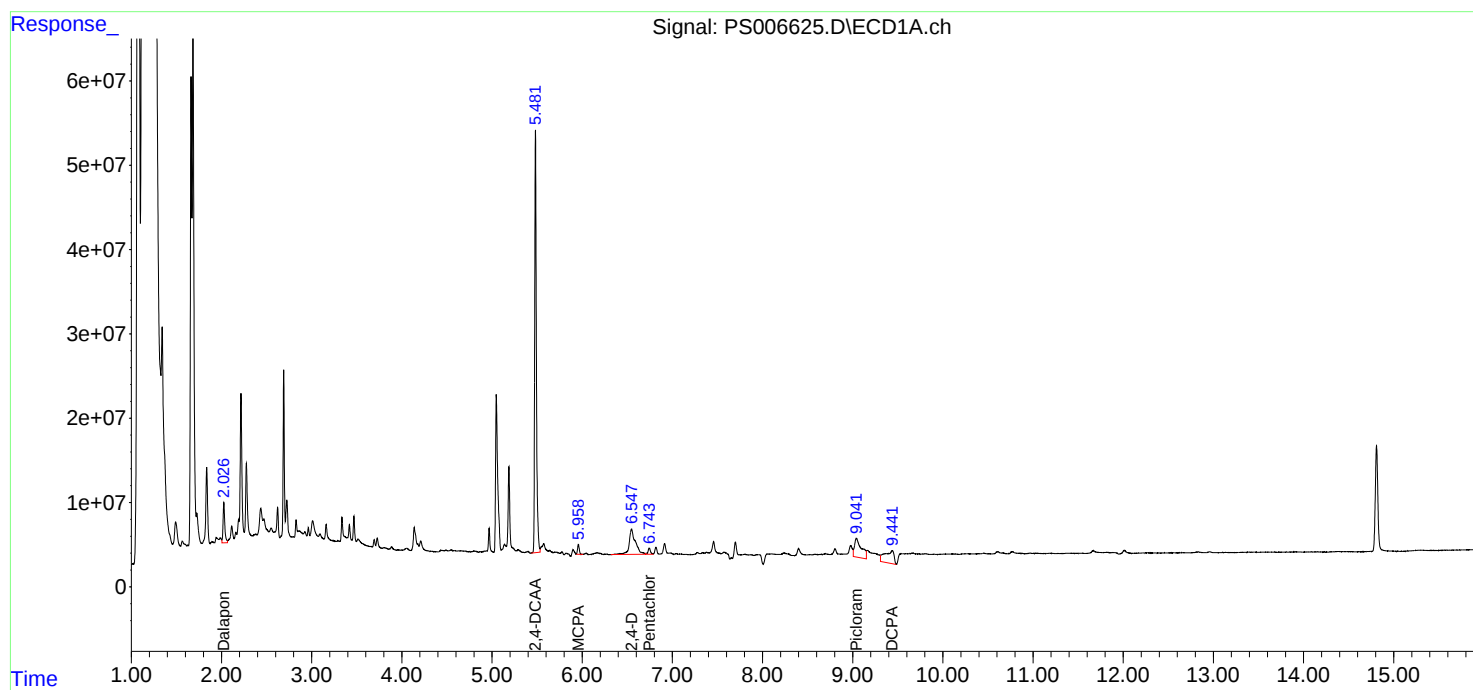


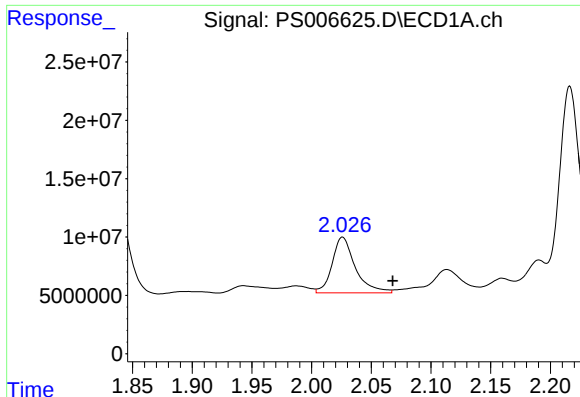

#1 Dalapon


R.T.: 2.026 min
Delta R.T.: -0.042 min
Response: 64489756
Conc: 65.98 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB122925BL

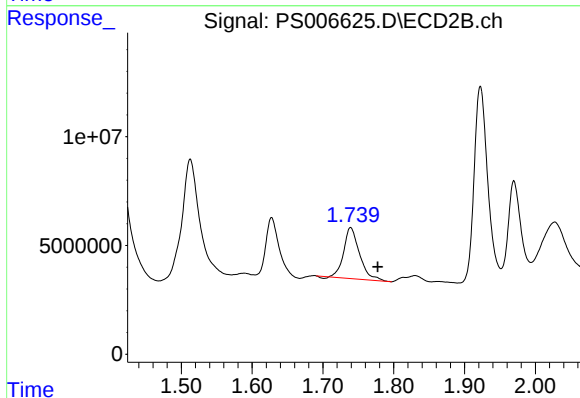


#1 Dalapon

R.T.: 1.739 min
Delta R.T.: -0.038 min
Response: 36109212
Conc: 70.66 ng/ml

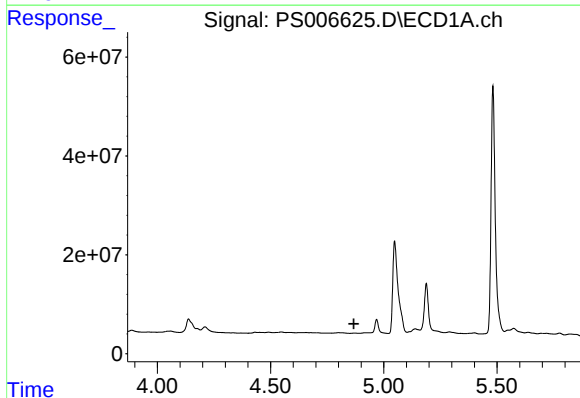


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.868 min
Response: 0
Conc: N.D.

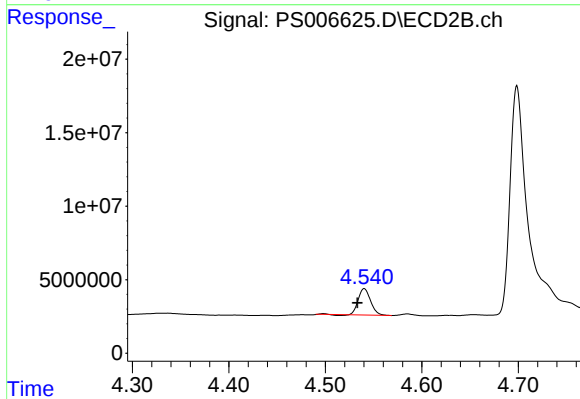

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.540 min
Delta R.T.: 0.007 min
Response: 15767812
Conc: 29.13 ng/ml

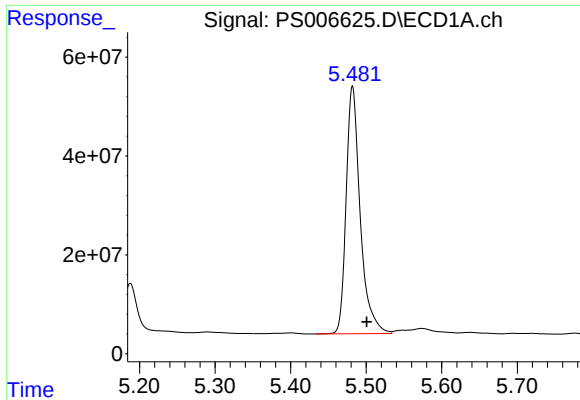

#4 2,4-DCAA


R.T.: 5.482 min
Delta R.T.: -0.019 min
Response: 648046885
Conc: 834.16 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB122925BL

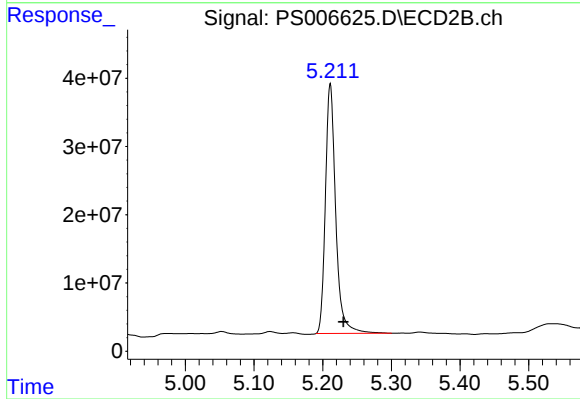


#4 2,4-DCAA

R.T.: 5.211 min
Delta R.T.: -0.019 min
Response: 381954455
Conc: 894.50 ng/ml

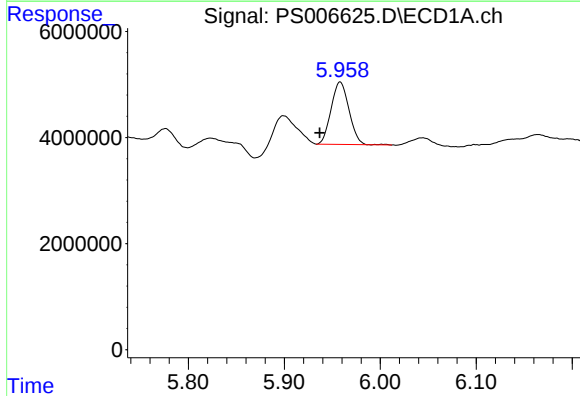


#7 MCPA

R.T.: 5.958 min
Delta R.T.: 0.021 min
Response: 15289479
Conc: 5.41 ug/ml

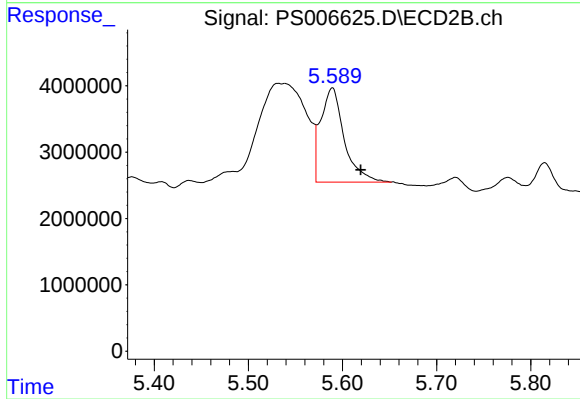

#7 MCPA


R.T.: 5.589 min
Delta R.T.: -0.030 min
Response: 24731589
Conc: 14.10 ug/ml

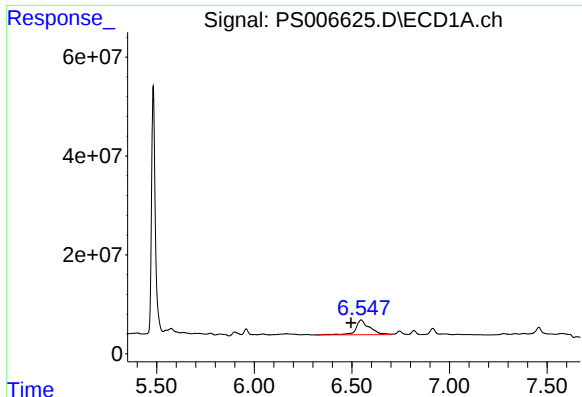

#9 2,4-D


R.T.: 6.547 min
Delta R.T.: 0.050 min
Response: 145790670
Conc: 188.70 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB122925BL

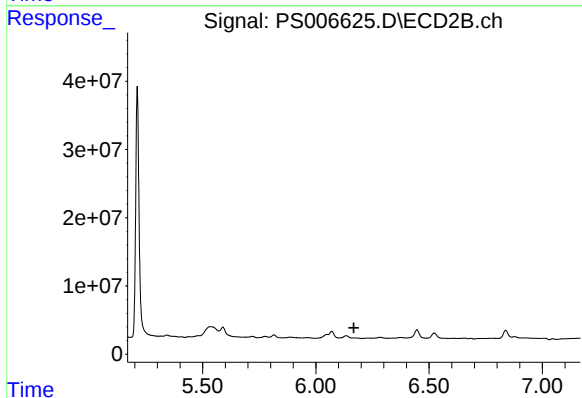


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.168 min
Response: 0
Conc: N.D.

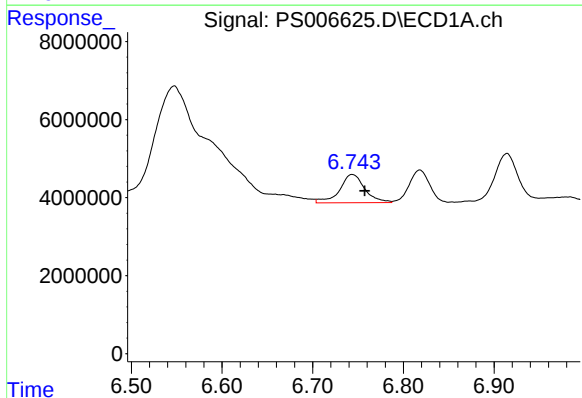


#10 Pentachlorophenol

R.T.: 6.744 min
Delta R.T.: -0.014 min
Response: 13925134
Conc: 1.25 ng/ml

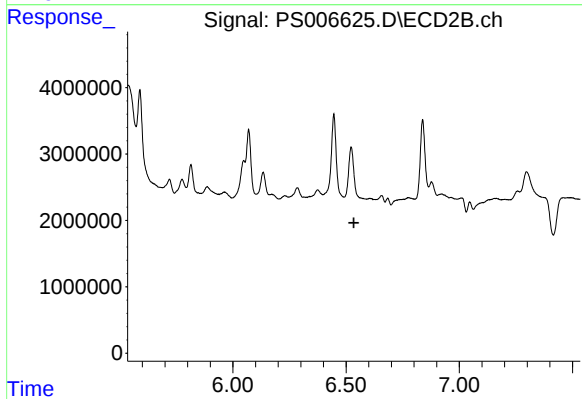

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 6.535 min
Response: 0
Conc: N.D.

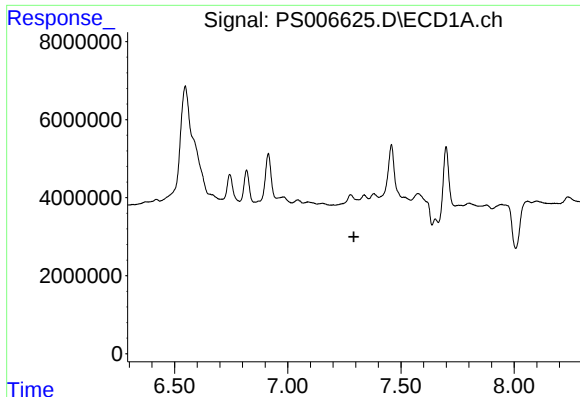

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.292 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB122925BL

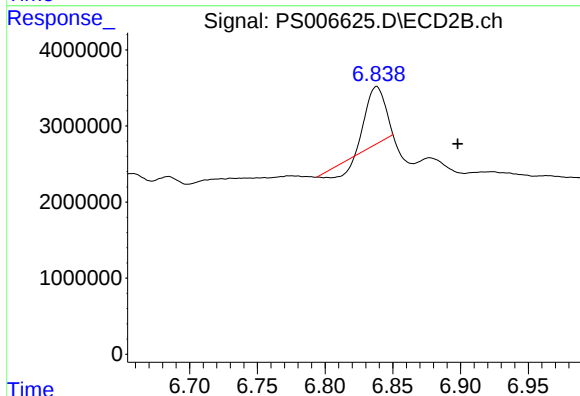


#11 2,4,5-TP (SILVEX)

R.T.: 6.838 min
Delta R.T.: -0.060 min
Response: 6224718
Conc: 2.73 ng/ml

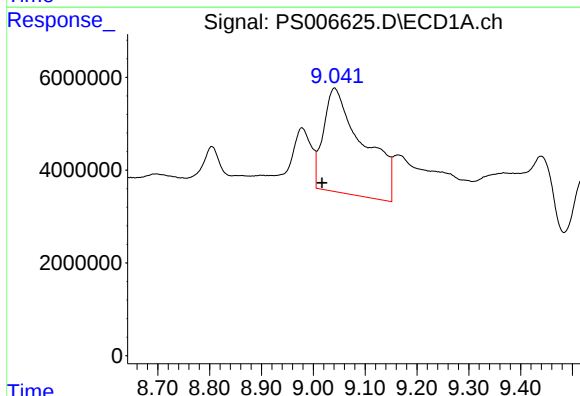


#15 Picloram

R.T.: 9.041 min
Delta R.T.: 0.024 min
Response: 120150275
Conc: 17.81 ng/ml

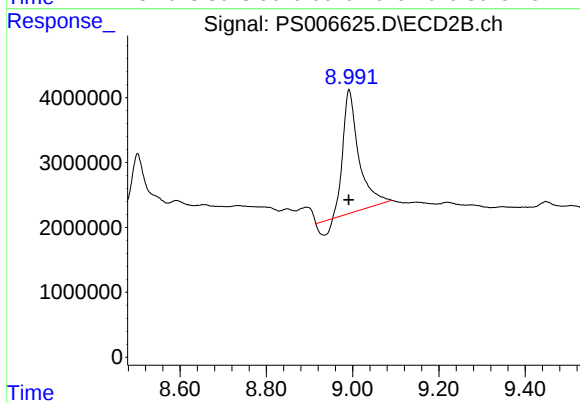

#15 Picloram


R.T.: 8.992 min
Delta R.T.: 0.000 min
Response: 46724029
Conc: 12.63 ng/ml

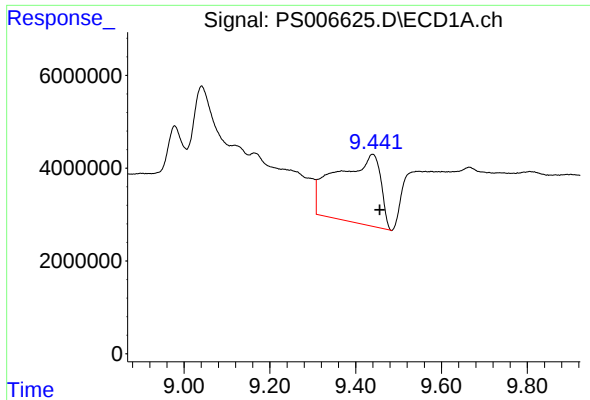

#16 DCPA

R.T.: 9.439 min
Delta R.T.: -0.017 min
Response: 105946178
Conc: 18.75 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB122925BL

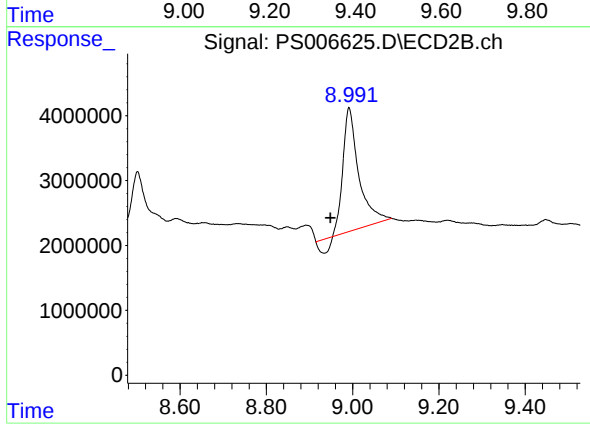

#16 DCPA

R.T.: 8.992 min
Delta R.T.: 0.043 min
Response: 46724029
Conc: 14.83 ng/ml