

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090919\
 Data File : PS006632.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2019 21:30
 Operator : SM\AJ
 Sample : K4661-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HD-01-090519

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 06:34:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 10 06:14:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.524	5.253	380.4E6	223.9E6	489.593	524.273
Target Compounds							
1) T	Dalapon	2.068	1.782	70492227	67355401	72.122	131.798 #
2) T	3,5-DICHL...	0.000	4.582	0	38476700	N.D.	71.088
5) T	DICAMBA	5.617	0.000	14228927	0	4.936	N.D. #
6) T	MCPD	5.793	0.000	6080969	0	3.197	N.D. #
7) T	MCPA	0.000	5.575	0	69993227	N.D.	39.905
9) T	2,4-D	0.000	6.175	0	17307696	N.D.	36.285
11) T	2,4,5-TP ...	0.000	6.874	0	21338490	N.D.	9.374
12) T	2,4,5-T	7.505	0.000	21965808	0	4.714	N.D. #
15) T	Picloram	9.011	0.000	51903316	0	7.694	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090919\
Data File : PS006632.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2019 21:30
Operator : SM\AJ
Sample : K4661-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HD-01-090519

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 06:34:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
Quant Title : 8080.M
QLast Update : Tue Sep 10 06:14:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

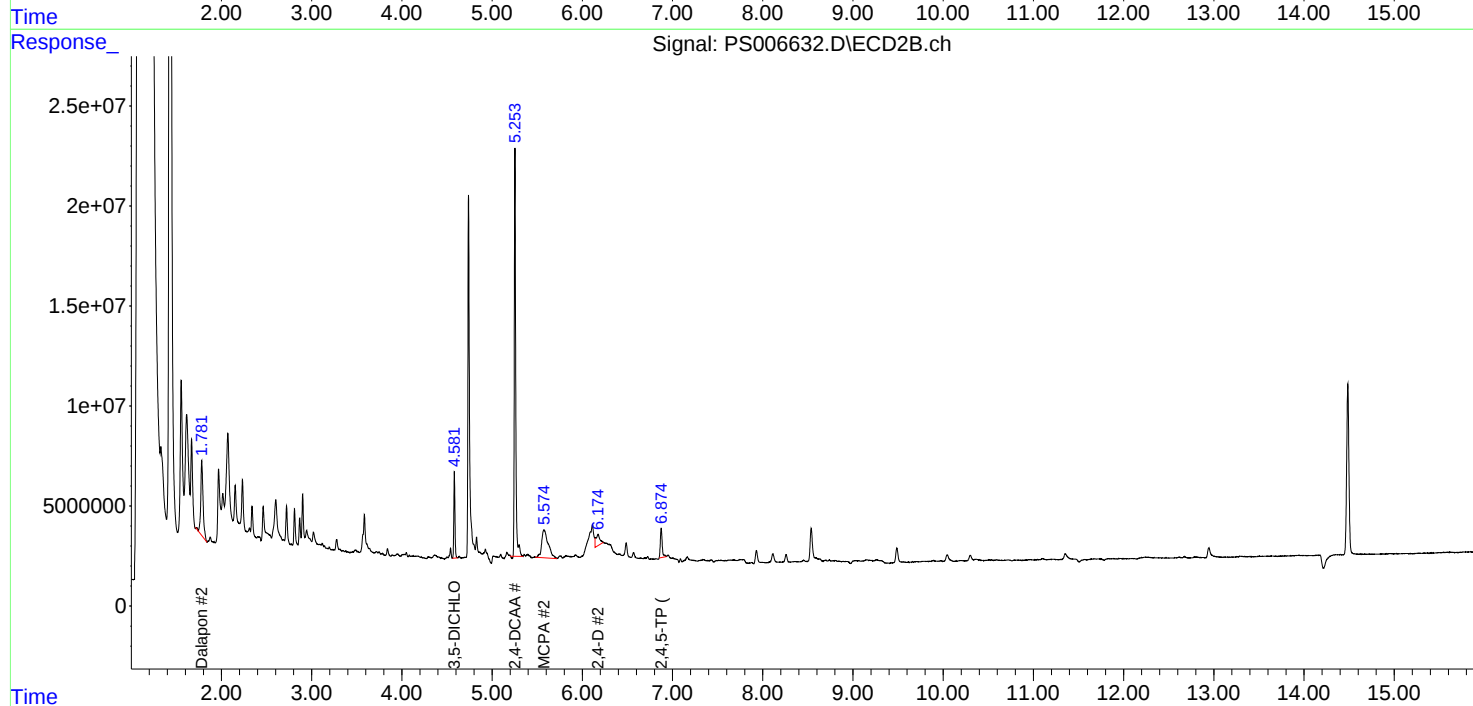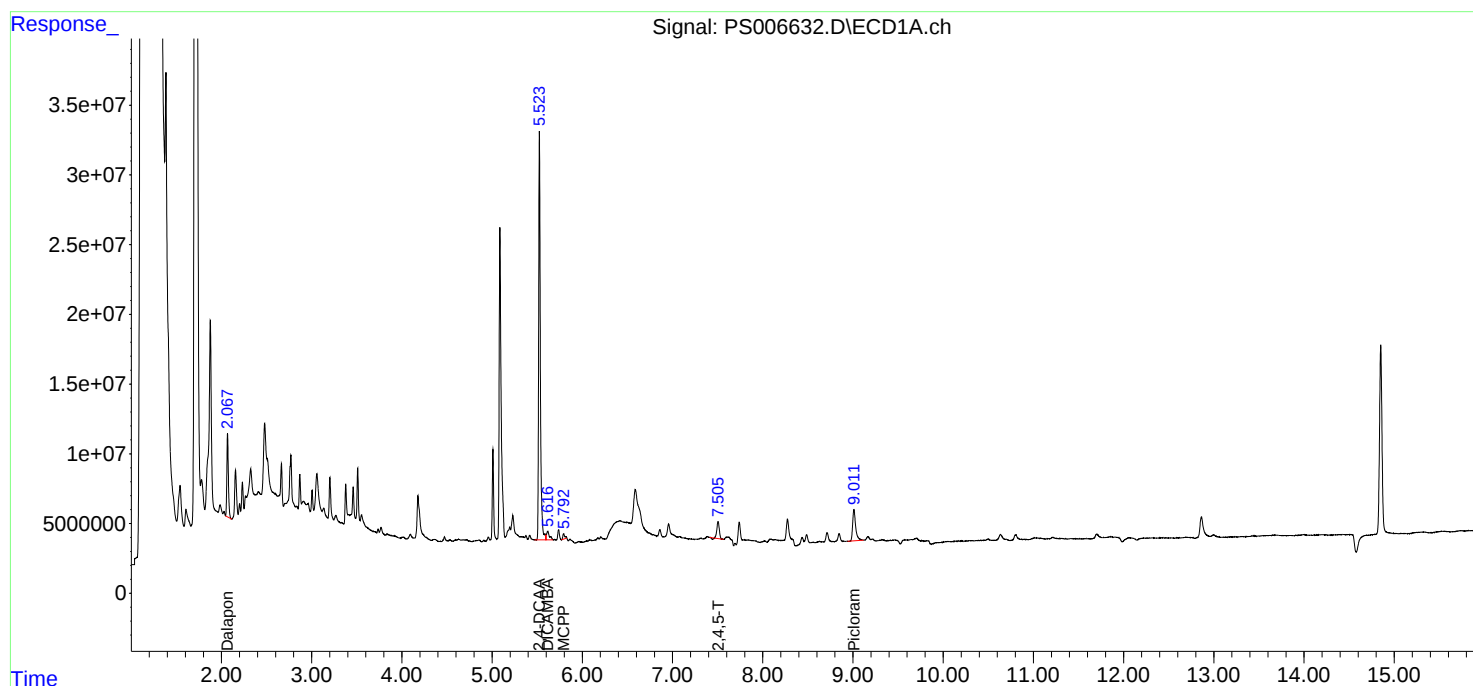


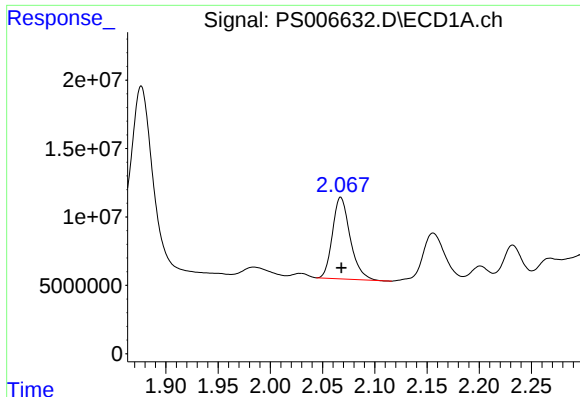

#1 Dalapon


R.T.: 2.068 min
Delta R.T.: 0.000 min
Response: 70492227
Conc: 72.12 ng/ml

Instrument :
ECD_S
ClientSampleId :
HD-01-090519

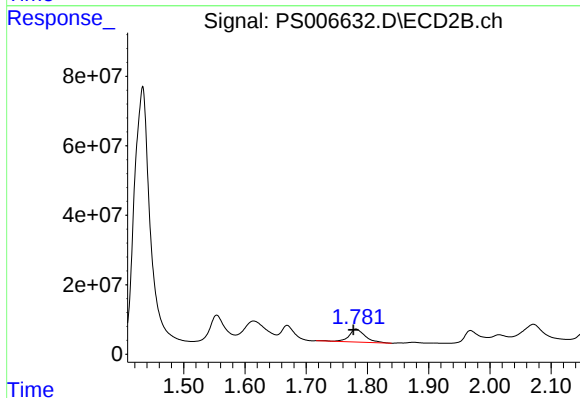


#1 Dalapon

R.T.: 1.782 min
Delta R.T.: 0.004 min
Response: 67355401
Conc: 131.80 ng/ml

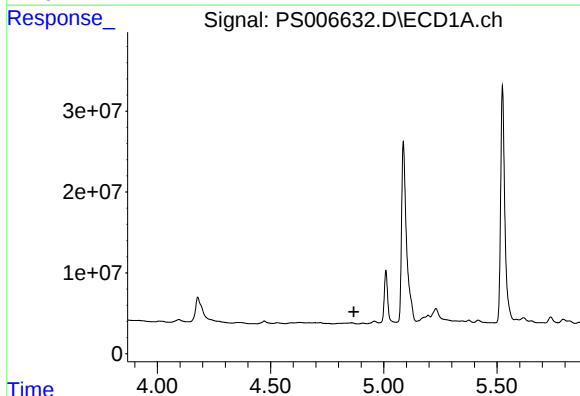


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.868 min
Response: 0
Conc: N.D.

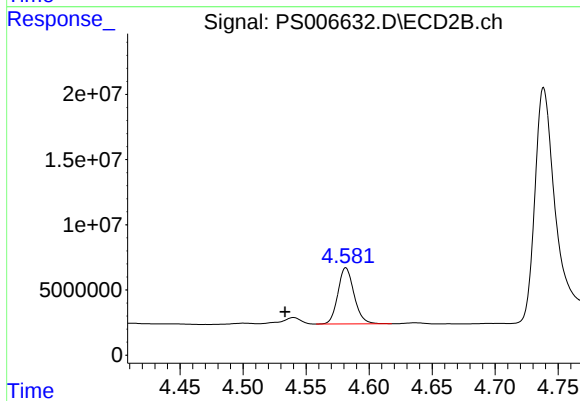

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.582 min
Delta R.T.: 0.048 min
Response: 38476700
Conc: 71.09 ng/ml

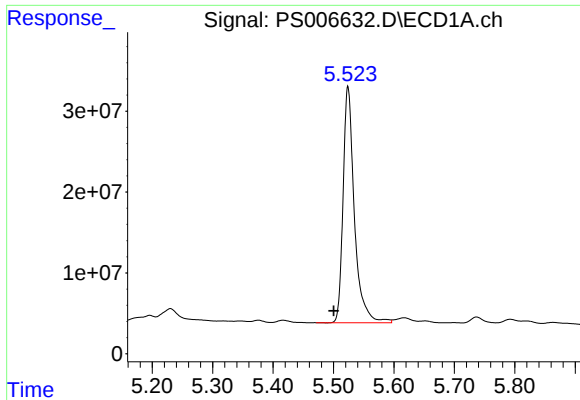

#4 2,4-DCAA


R.T.: 5.524 min
Delta R.T.: 0.024 min
Response: 380357604
Conc: 489.59 ng/ml

Instrument :
ECD_S
ClientSampleId :
HD-01-090519

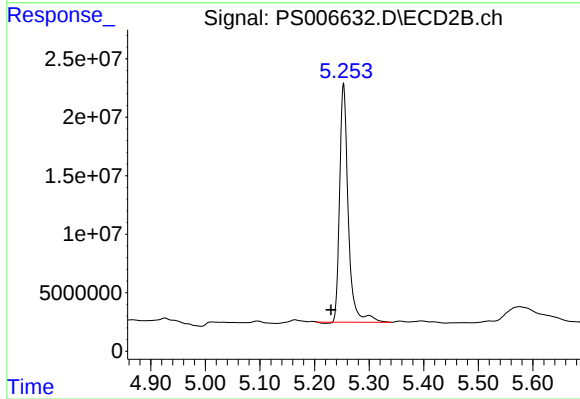


#4 2,4-DCAA

R.T.: 5.253 min
Delta R.T.: 0.023 min
Response: 223866014
Conc: 524.27 ng/ml

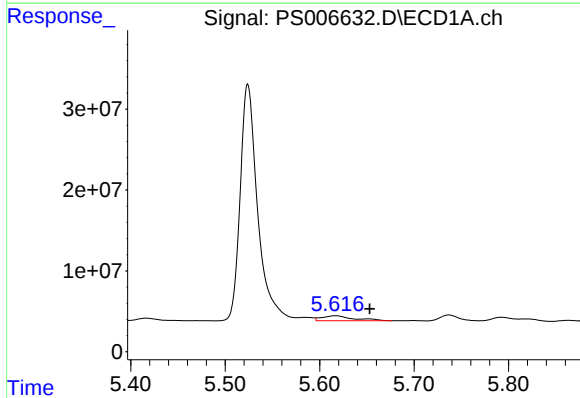


#5 DICAMBA

R.T.: 5.617 min
Delta R.T.: -0.036 min
Response: 14228927
Conc: 4.94 ng/ml

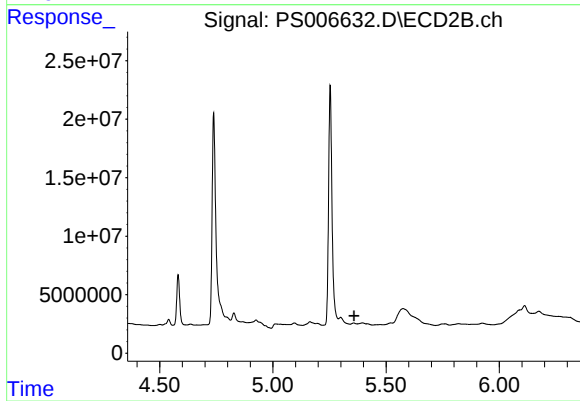

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.358 min
Response: 0
Conc: N.D.

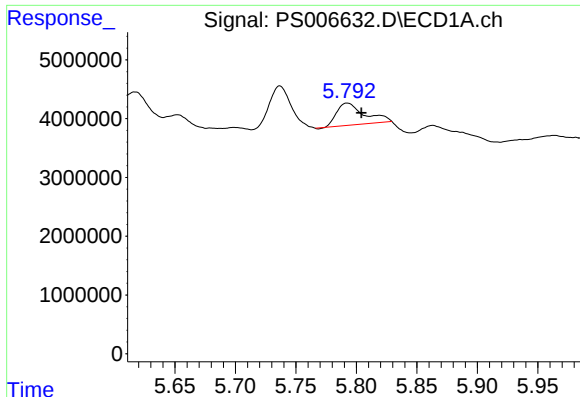

#6 MCPP


R.T.: 5.793 min
Delta R.T.: -0.012 min
Response: 6080969
Conc: 3.20 ug/ml

Instrument :
ECD_S
ClientSampleId :
HD-01-090519

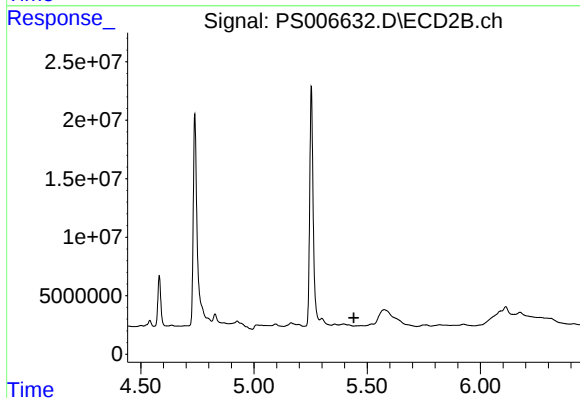


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 5.441 min
Response: 0
Conc: N.D.

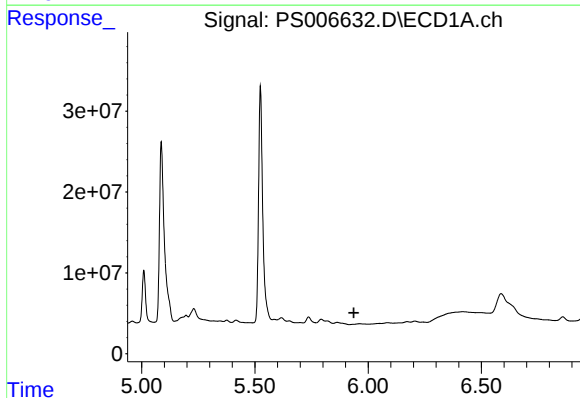


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.937 min
Response: 0
Conc: N.D.

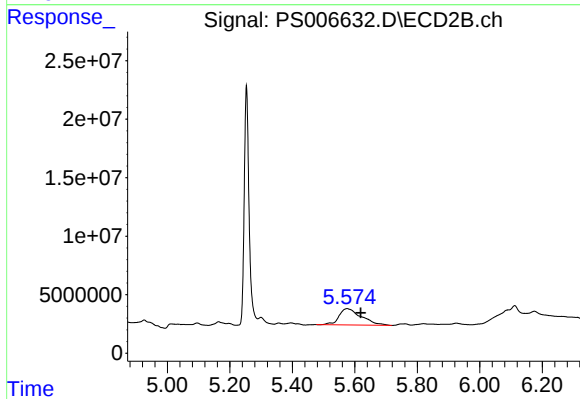

#7 MCPA


R.T.: 5.575 min
Delta R.T.: -0.044 min
Response: 69993227
Conc: 39.90 ug/ml

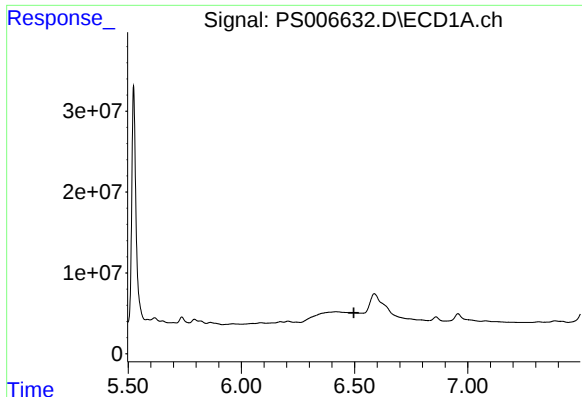

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.497 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HD-01-090519

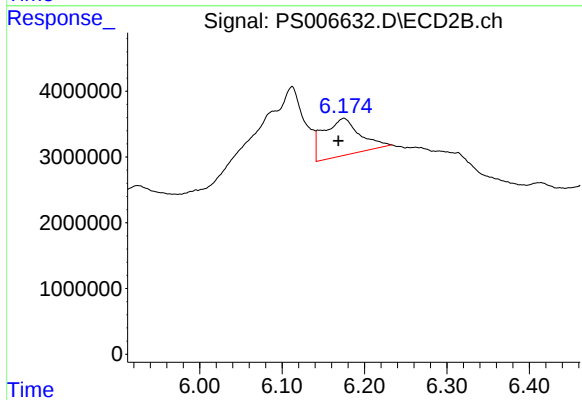


#9 2,4-D

R.T.: 6.175 min
Delta R.T.: 0.007 min
Response: 17307696
Conc: 36.29 ng/ml

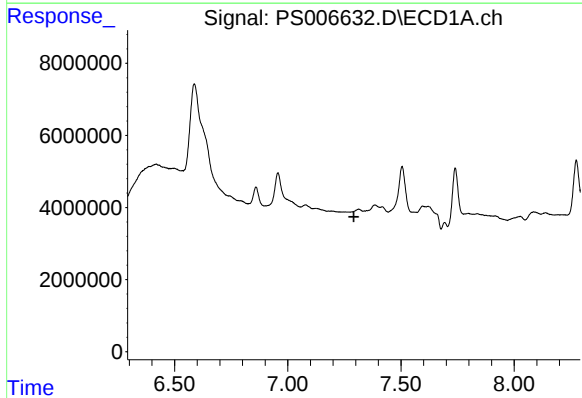


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.292 min
Response: 0
Conc: N.D.

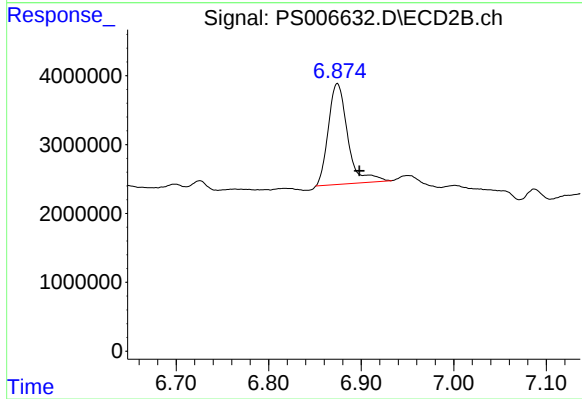

#11 2,4,5-TP (SILVEX)


R.T.: 6.874 min
Delta R.T.: -0.024 min
Response: 21338490
Conc: 9.37 ng/ml

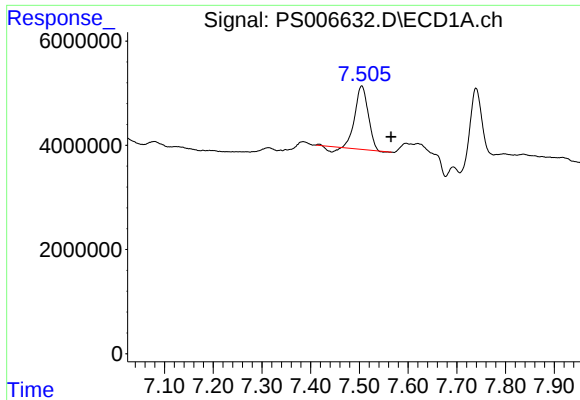

#12 2,4,5-T


R.T.: 7.505 min
Delta R.T.: -0.061 min
Response: 21965808
Conc: 4.71 ng/ml

Instrument :
ECD_S
ClientSampleId :
HD-01-090519

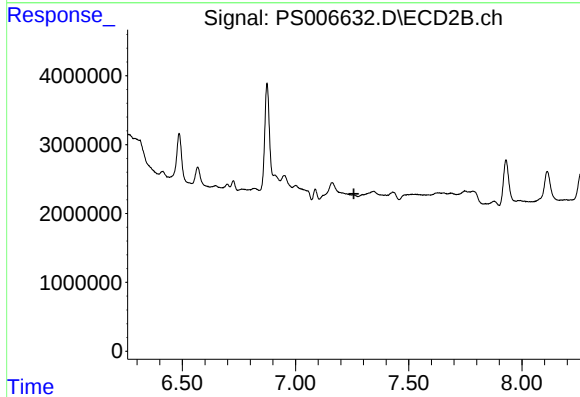


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.258 min
Response: 0
Conc: N.D.

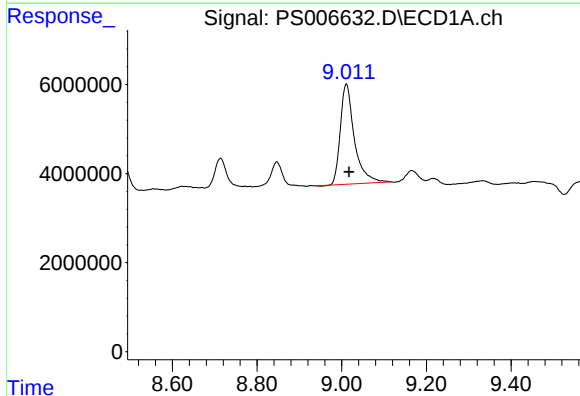

#15 Picloram

R.T.: 9.011 min
Delta R.T.: -0.006 min
Response: 51903316
Conc: 7.69 ng/ml

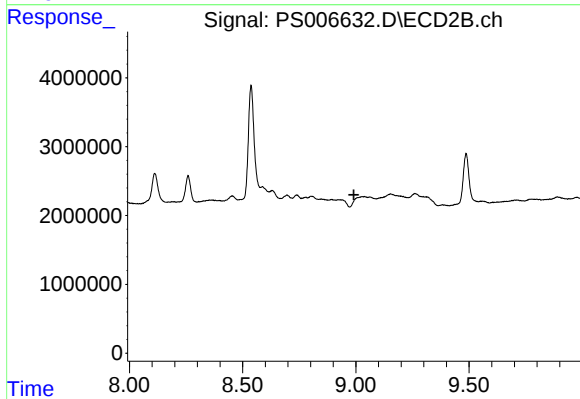

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 8.991 min
Response: 0
Conc: N.D.