

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090919\
 Data File : PS006634.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2019 22:13
 Operator : SM\AJ
 Sample : K4663-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 OK-03-090519

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 06:35:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 10 06:14:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.499	5.228	369.1E6	218.7E6	475.043	512.205
Target Compounds							
1) T	Dalapon	2.042	1.757	75480991	81373533	77.226	159.229 #
2) T	3,5-DICHL...	4.883	4.556	4527805	31759572	4.574	58.678 #
5) T	DICAMBA	5.712	0.000	1523492	0	<MDL	N.D. #
9) T	2,4-D	6.564	6.151	358.1E6	14815039	463.534	31.060 #
15) T	Picloram	8.987	0.000	57209426	0	8.481	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090919\
Data File : PS006634.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2019 22:13
Operator : SM\AJ
Sample : K4663-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
OK-03-090519

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 06:35:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
Quant Title : 8080.M
QLast Update : Tue Sep 10 06:14:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

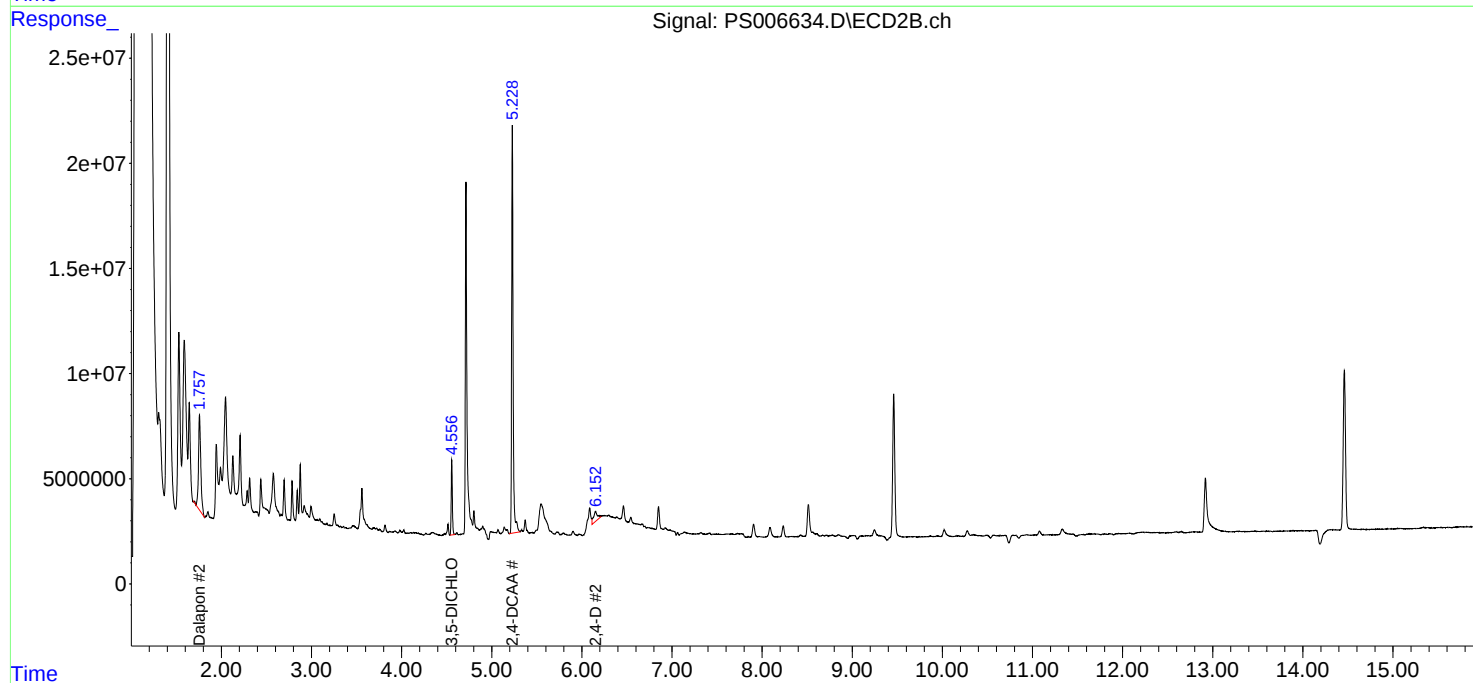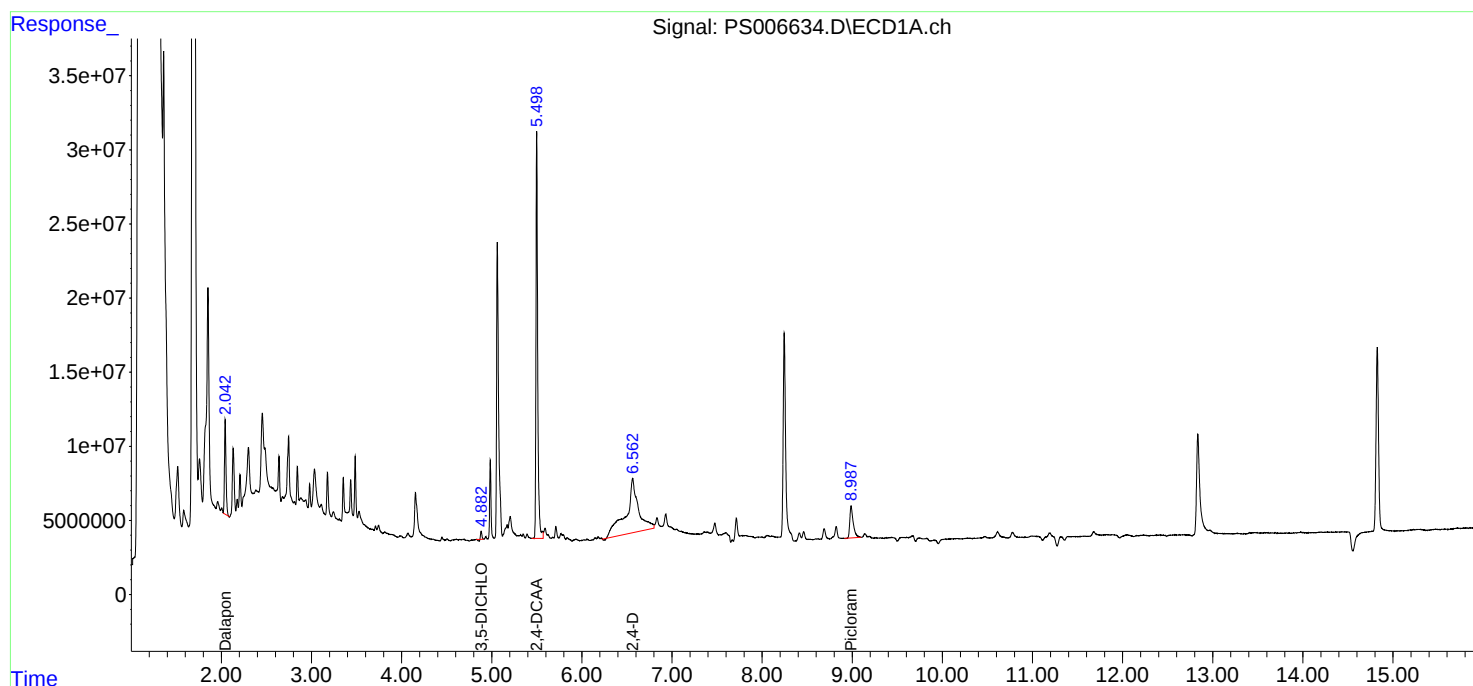


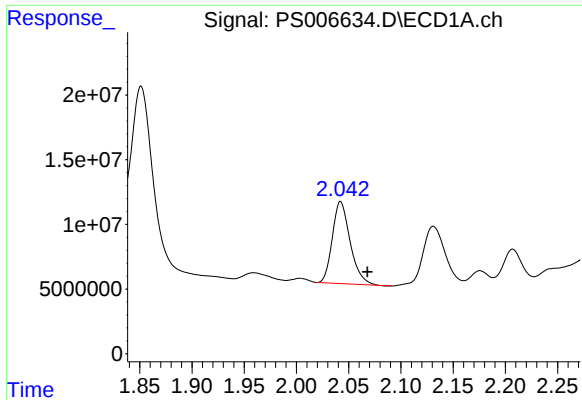

#1 Dalapon


R.T.: 2.042 min
Delta R.T.: -0.026 min
Response: 75480991
Conc: 77.23 ng/ml

Instrument :
ECD_S
ClientSampleId :
OK-03-090519

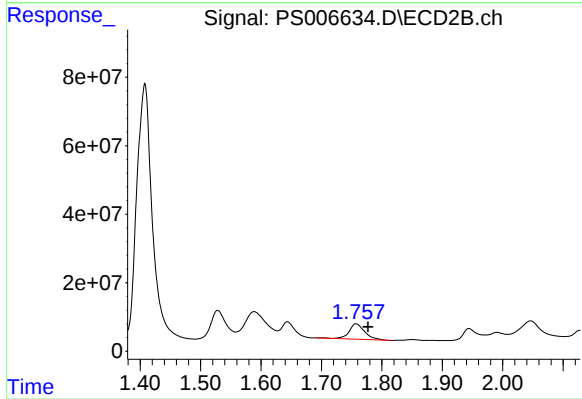


#1 Dalapon

R.T.: 1.757 min
Delta R.T.: -0.020 min
Response: 81373533
Conc: 159.23 ng/ml

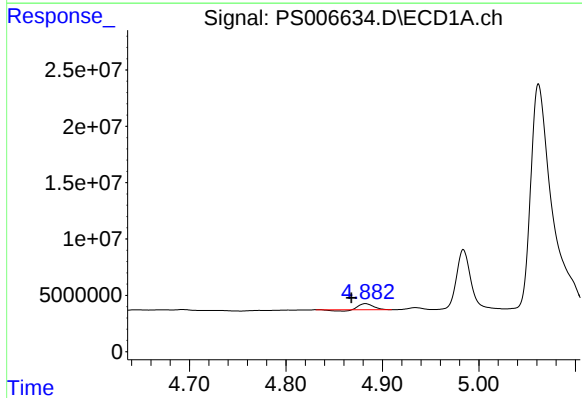


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.883 min
Delta R.T.: 0.014 min
Response: 4527805
Conc: 4.57 ng/ml

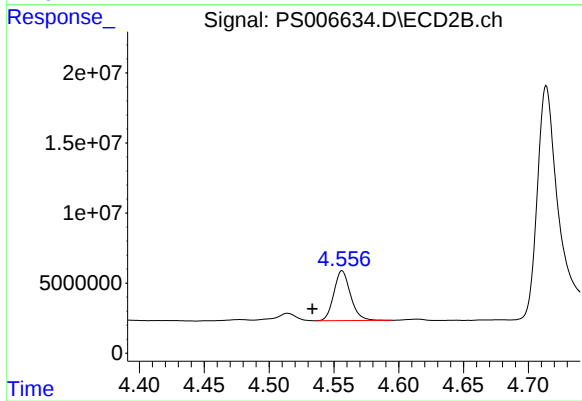

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.556 min
Delta R.T.: 0.023 min
Response: 31759572
Conc: 58.68 ng/ml

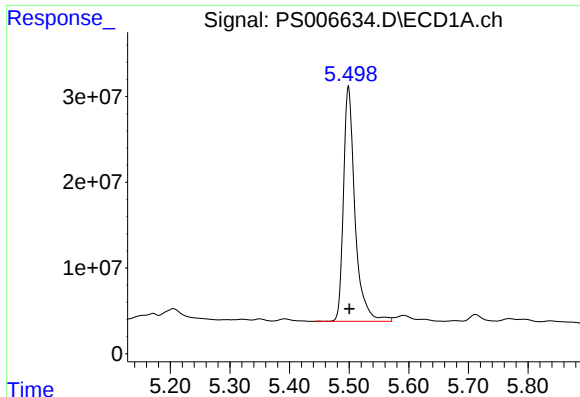

#4 2,4-DCAA


R.T.: 5.499 min
Delta R.T.: -0.002 min
Response: 369054179
Conc: 475.04 ng/ml

Instrument :
ECD_S
ClientSampleId :
OK-03-090519

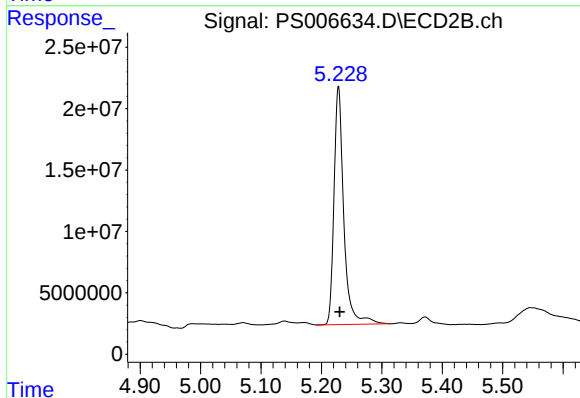


#4 2,4-DCAA

R.T.: 5.228 min
Delta R.T.: -0.002 min
Response: 218712850
Conc: 512.21 ng/ml

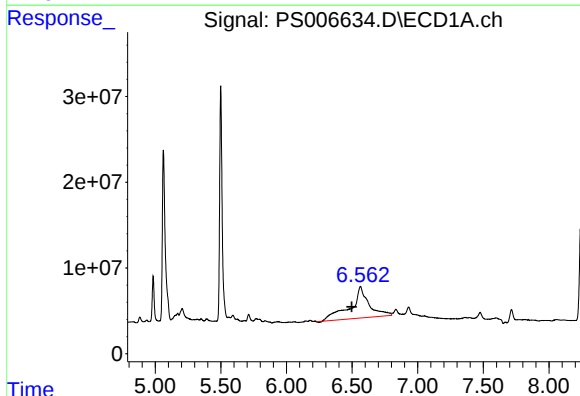


#9 2,4-D

R.T.: 6.564 min
Delta R.T.: 0.067 min
Response: 358136853
Conc: 463.53 ng/ml

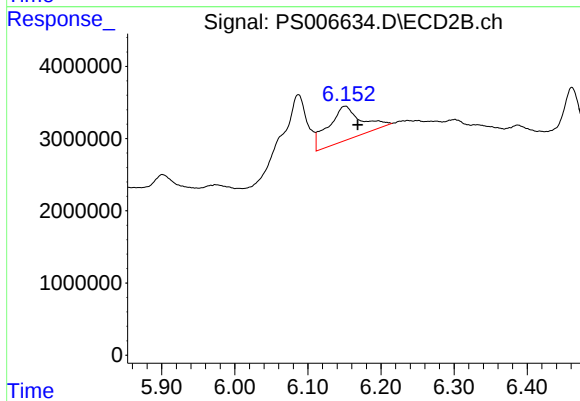

#9 2,4-D


R.T.: 6.151 min
Delta R.T.: -0.017 min
Response: 14815039
Conc: 31.06 ng/ml

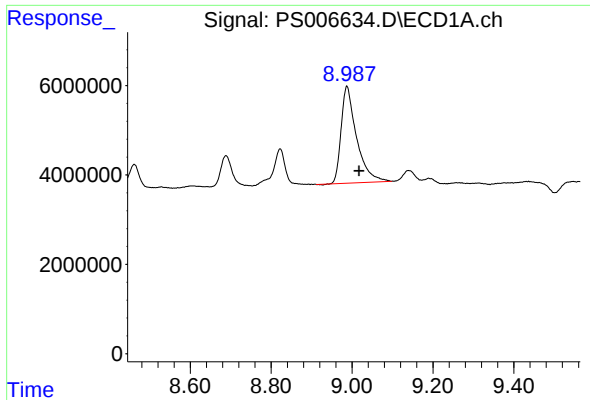

#15 Picloram

R.T.: 8.987 min
Delta R.T.: -0.030 min
Response: 57209426
Conc: 8.48 ng/ml

Instrument :
ECD_S
ClientSampleId :
OK-03-090519

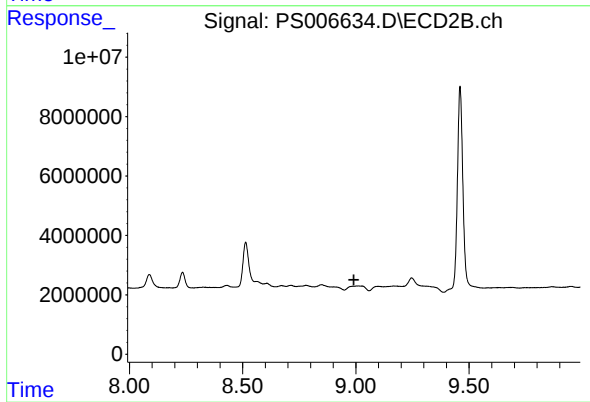

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 8.991 min
Response: 0
Conc: N.D.