

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090919\
 Data File : PS006638.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2019 23:41
 Operator : SM\AJ
 Sample : K4669-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TR-05-090519

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 06:36:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 10 06:14:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.484	5.213	430.7E6	251.1E6	554.398	587.994
Target Compounds							
1) T	Dalapon	2.028	1.742	80783181	83147505	82.651	162.700 #
2) T	3,5-DICHL...	0.000	4.542	0	34261133	N.D.	63.300
5) T	DICAMBA	5.696	0.000	8971017	0	3.112	N.D. #
9) T	2,4-D	6.549	0.000	89822537	0	116.257	N.D. #
10) T	Pentachlo...	6.819	0.000	7804520	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	6.836	0	8239728	N.D.	3.620
15) T	Picloram	8.972	0.000	57478846	0	8.521	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090919\
Data File : PS006638.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2019 23:41
Operator : SM\AJ
Sample : K4669-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
TR-05-090519

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 06:36:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
Quant Title : 8080.M
QLast Update : Tue Sep 10 06:14:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

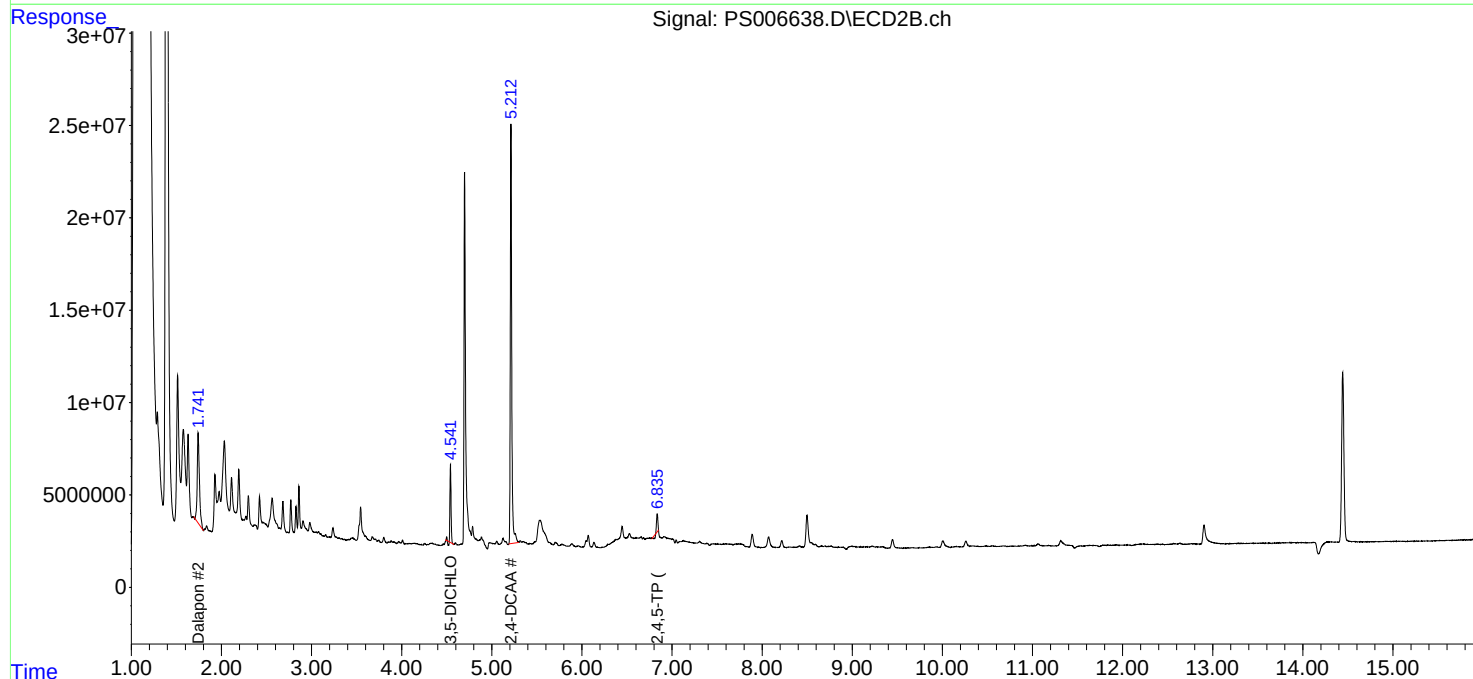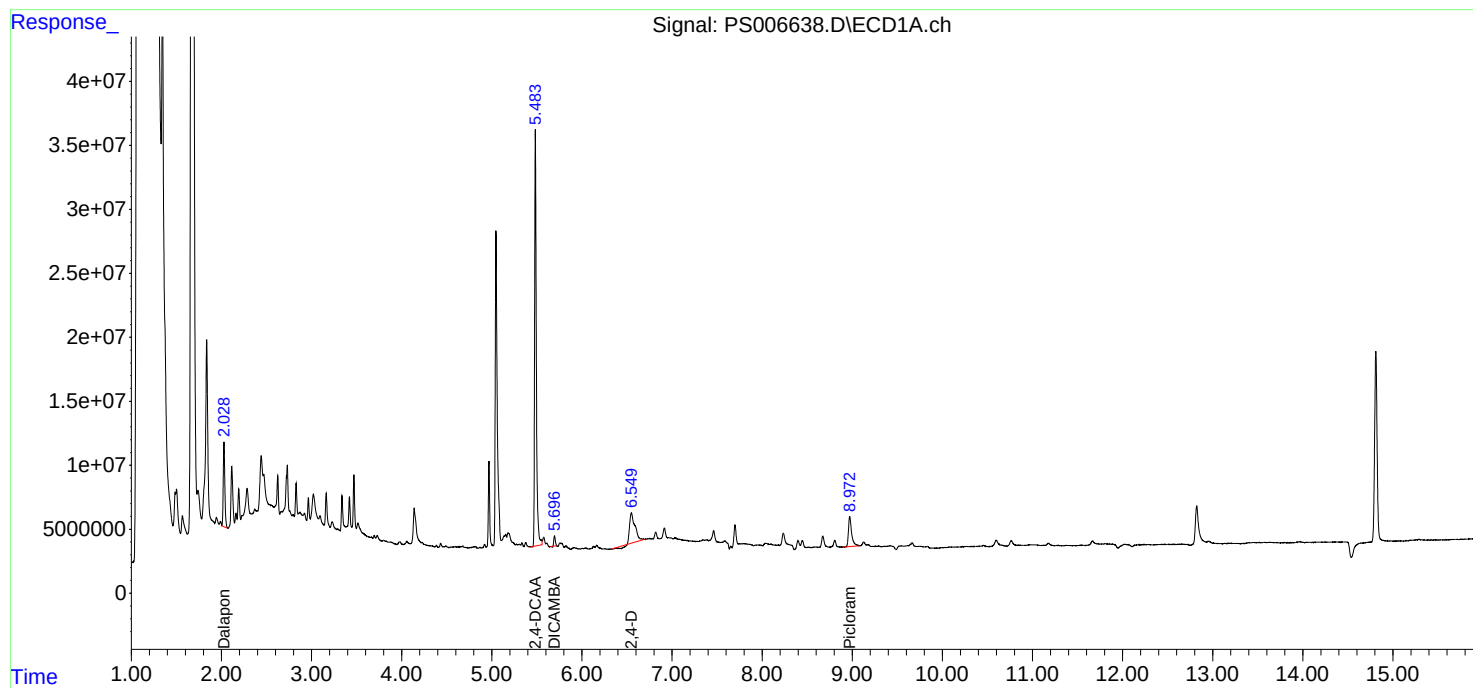


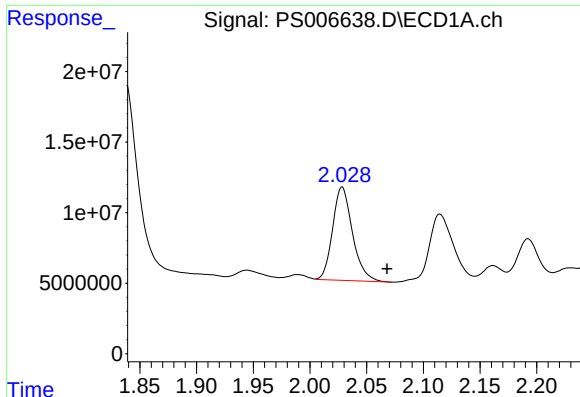

#1 Dalapon


R.T.: 2.028 min
Delta R.T.: -0.040 min
Response: 80783181
Conc: 82.65 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR-05-090519

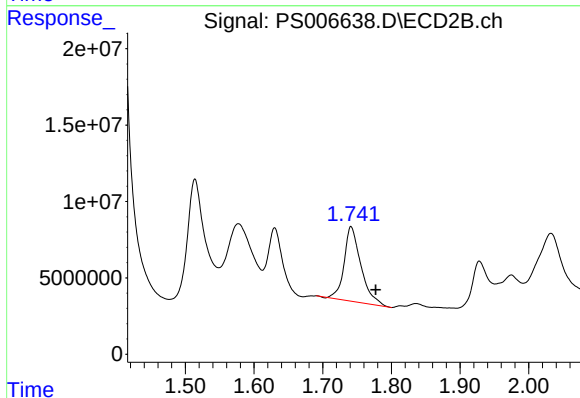


#1 Dalapon

R.T.: 1.742 min
Delta R.T.: -0.036 min
Response: 83147505
Conc: 162.70 ng/ml

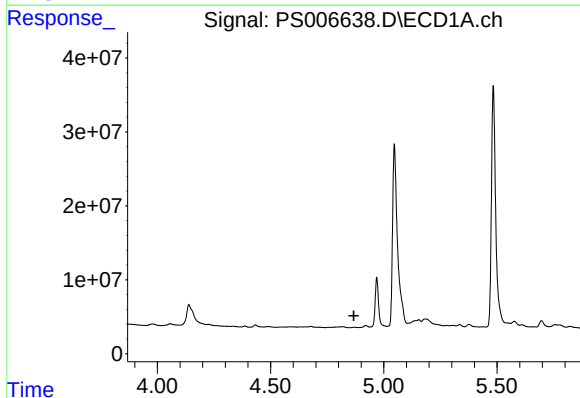


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.868 min
Response: 0
Conc: N.D.

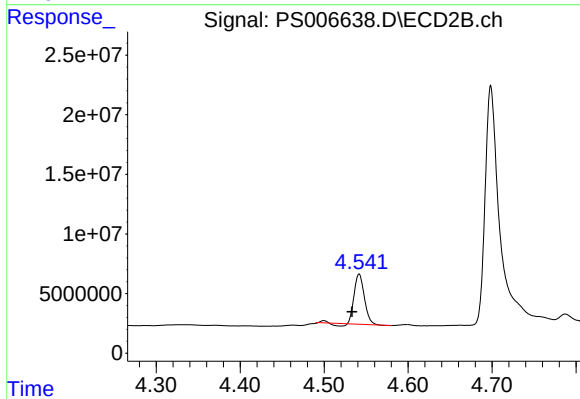

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.542 min
Delta R.T.: 0.008 min
Response: 34261133
Conc: 63.30 ng/ml

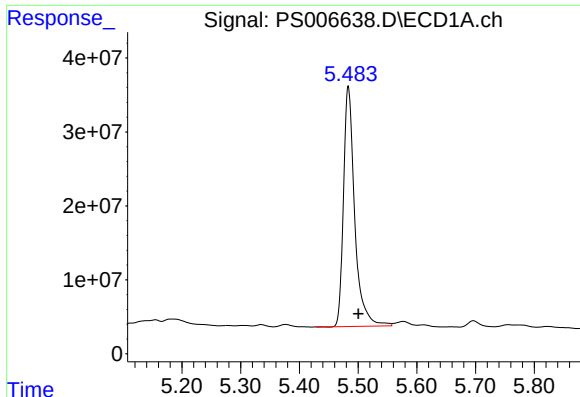

#4 2,4-DCAA


R.T.: 5.484 min
Delta R.T.: -0.017 min
Response: 430703997
Conc: 554.40 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR-05-090519

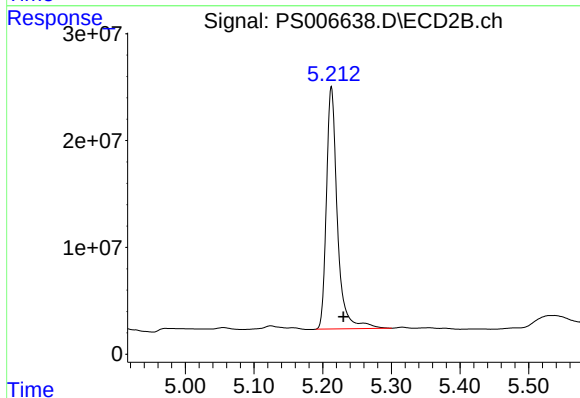


#4 2,4-DCAA

R.T.: 5.213 min
Delta R.T.: -0.017 min
Response: 251074863
Conc: 587.99 ng/ml

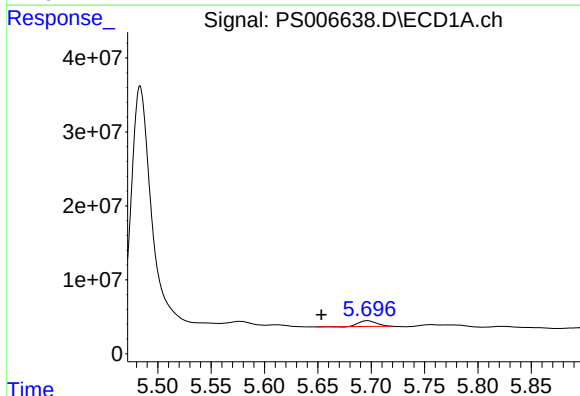


#5 DICAMBA

R.T.: 5.696 min
Delta R.T.: 0.043 min
Response: 8971017
Conc: 3.11 ng/ml

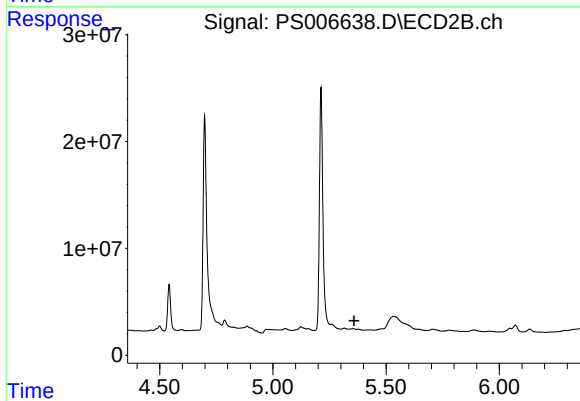

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.358 min
Response: 0
Conc: N.D.

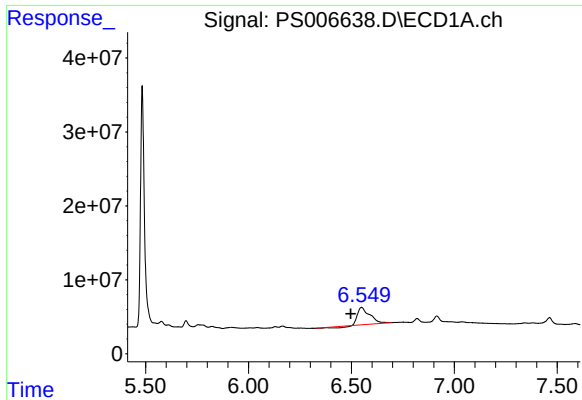

#9 2,4-D


R.T.: 6.549 min
Delta R.T.: 0.052 min
Response: 89822537
Conc: 116.26 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR-05-090519

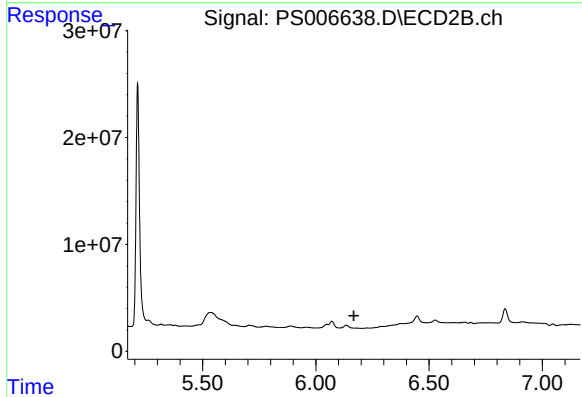


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.168 min
Response: 0
Conc: N.D.

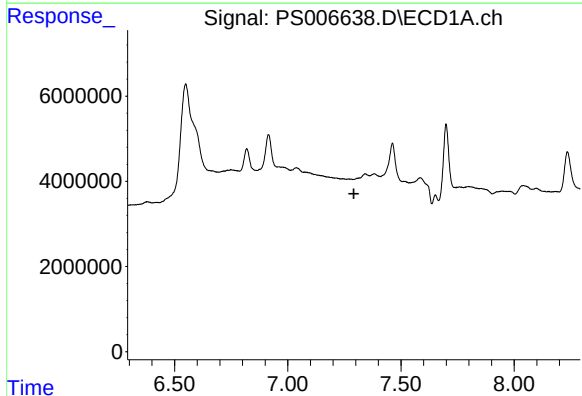


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.292 min
Response: 0
Conc: N.D.

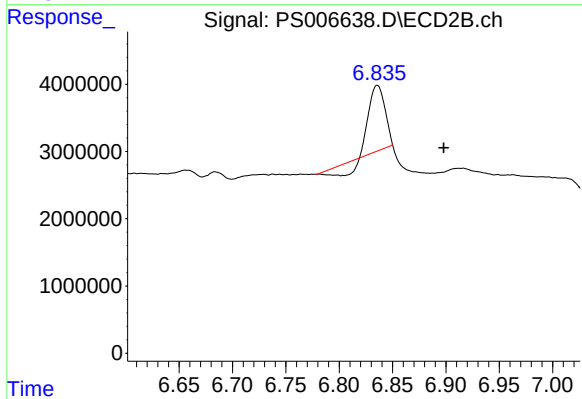

#11 2,4,5-TP (SILVEX)


R.T.: 6.836 min
Delta R.T.: -0.062 min
Response: 8239728
Conc: 3.62 ng/ml

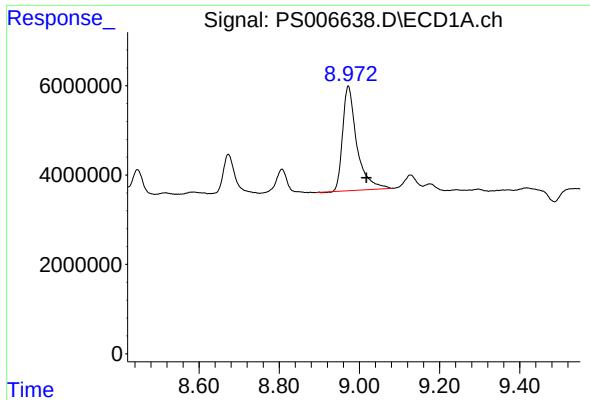

#15 Picloram

R.T.: 8.972 min
Delta R.T.: -0.045 min
Response: 57478846
Conc: 8.52 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR-05-090519

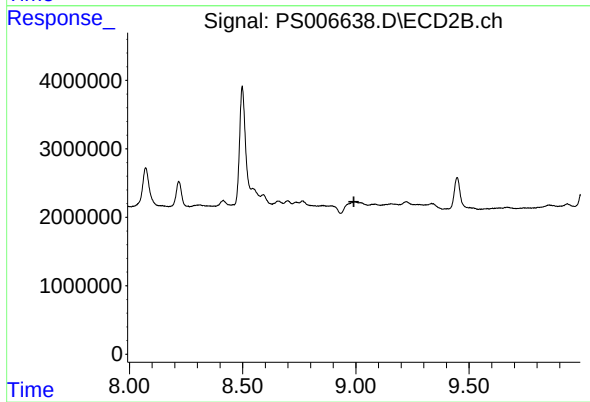

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 8.991 min
Response: 0
Conc: N.D.