

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090919\
 Data File : PS006641.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2019 00:47
 Operator : SM\AJ
 Sample : PB122893BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB122893BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 06:37:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 10 06:14:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.482	5.211	400.4E6	223.2E6	515.391	522.653
Target Compounds							
1) T	Dalapon	2.027	1.738	64530717	51967697	66.023	101.688 #
2) T	3,5-DICHL...	0.000	4.540	0	33801002	N.D.	62.450
7) T	MCPA	5.957	5.587	11230413	18883592	3.974	10.766 #
9) T	2,4-D	6.545	0.000	121.4E6	0	157.078	N.D. #
11) T	2,4,5-TP ...	0.000	6.837	0	4239936	N.D.	1.863
15) T	Picloram	8.981	0.000	29897554	0	4.432	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090919\
Data File : PS006641.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2019 00:47
Operator : SM\AJ
Sample : PB122893BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB122893BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 06:37:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
Quant Title : 8080.M
QLast Update : Tue Sep 10 06:14:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

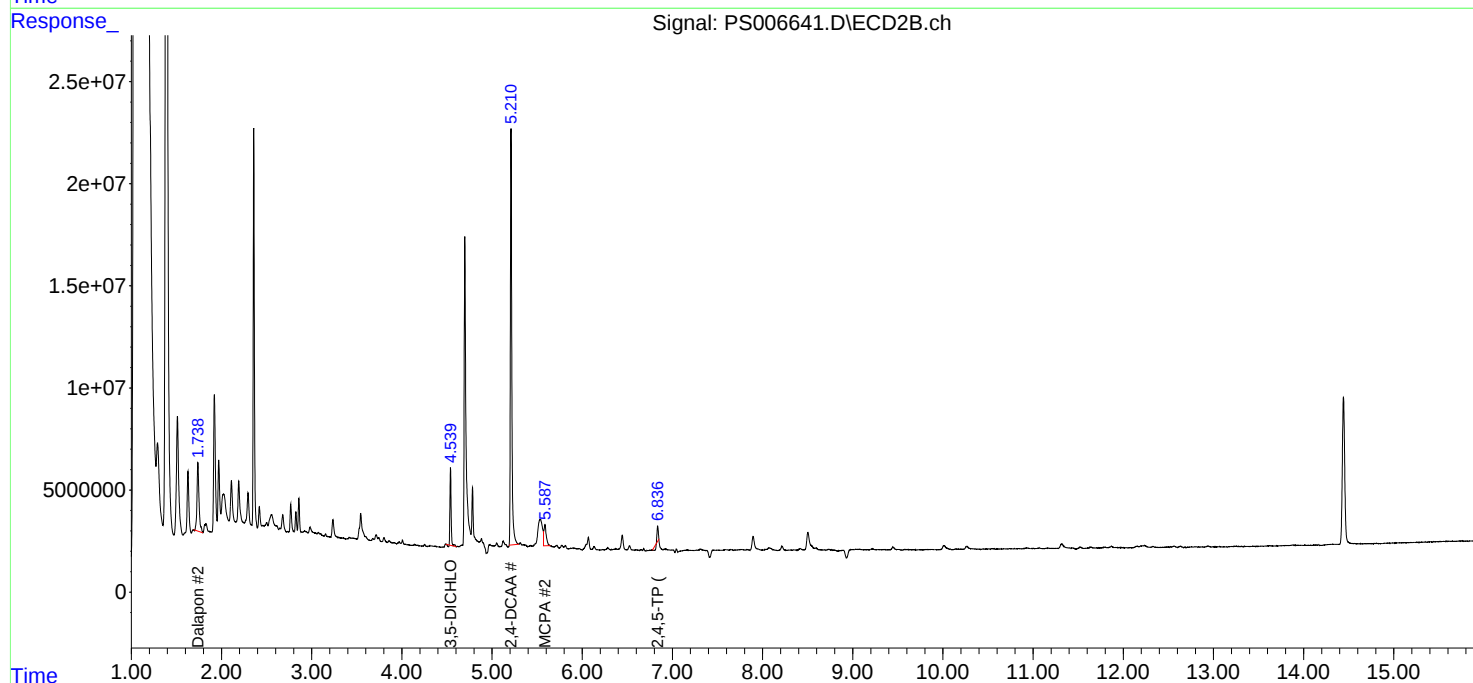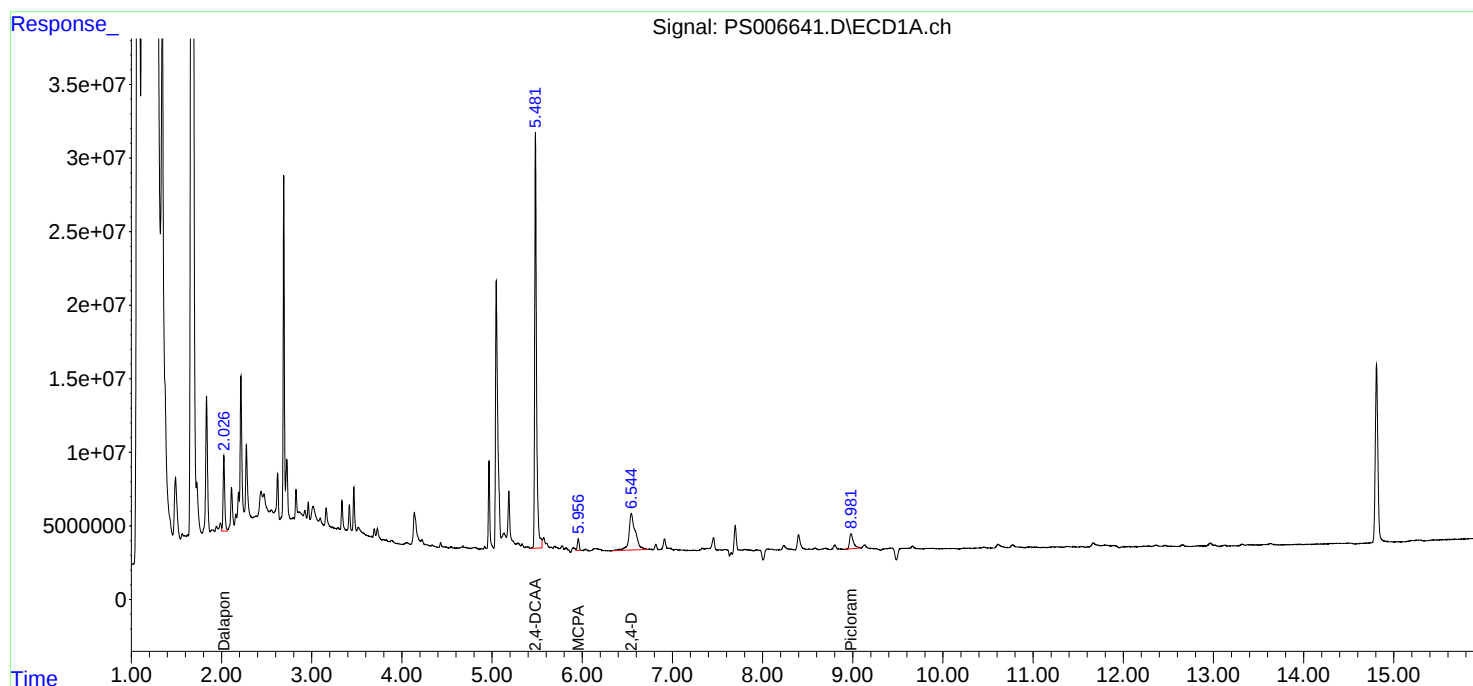


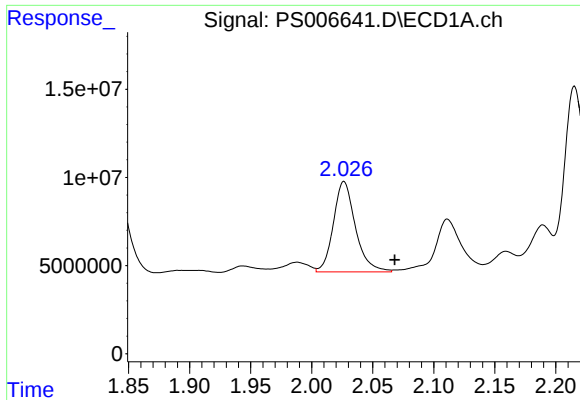

#1 Dalapon


R.T.: 2.027 min
Delta R.T.: -0.041 min
Response: 64530717
Conc: 66.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB122893BL

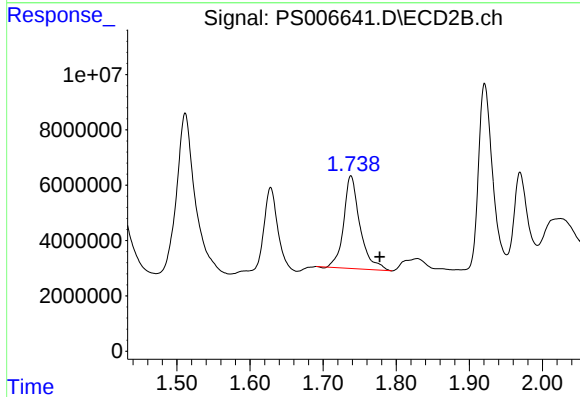


#1 Dalapon

R.T.: 1.738 min
Delta R.T.: -0.039 min
Response: 51967697
Conc: 101.69 ng/ml

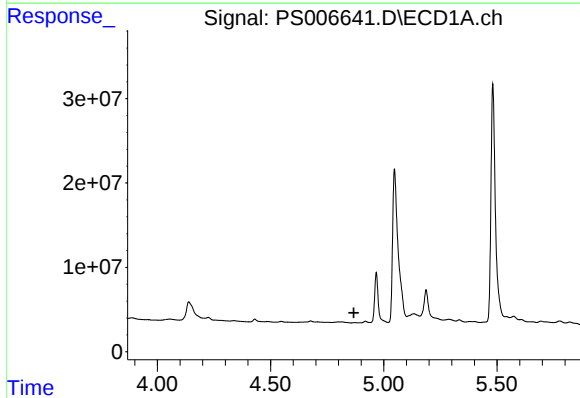


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.868 min
Response: 0
Conc: N.D.

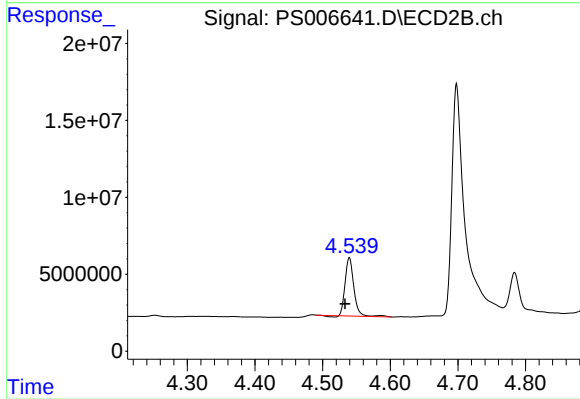

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.540 min
Delta R.T.: 0.006 min
Response: 33801002
Conc: 62.45 ng/ml

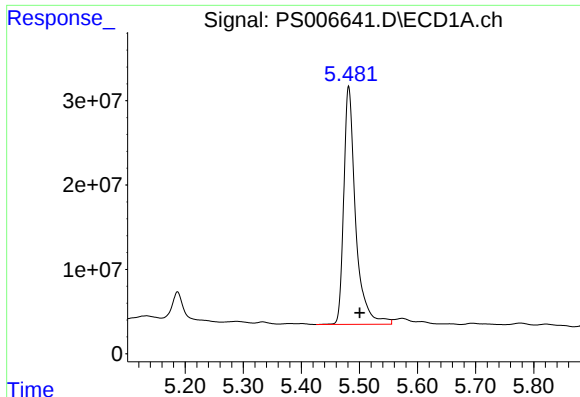

#4 2,4-DCAA


R.T.: 5.482 min
Delta R.T.: -0.019 min
Response: 400399621
Conc: 515.39 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB122893BL

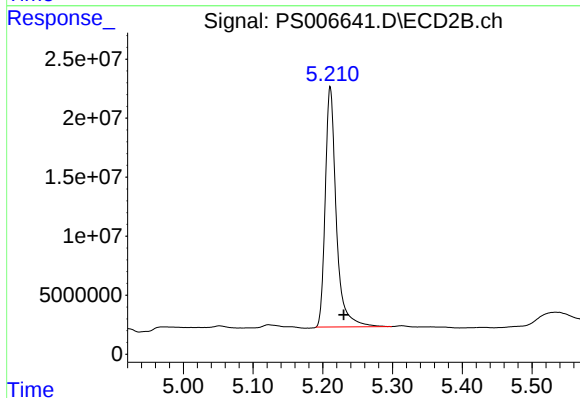


#4 2,4-DCAA

R.T.: 5.211 min
Delta R.T.: -0.019 min
Response: 223174079
Conc: 522.65 ng/ml

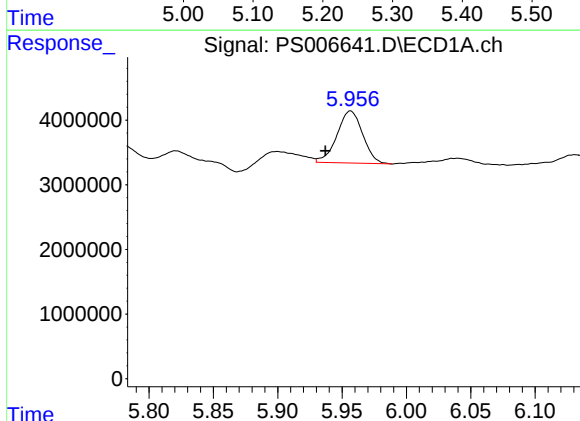


#7 MCPA

R.T.: 5.957 min
Delta R.T.: 0.020 min
Response: 11230413
Conc: 3.97 ug/ml

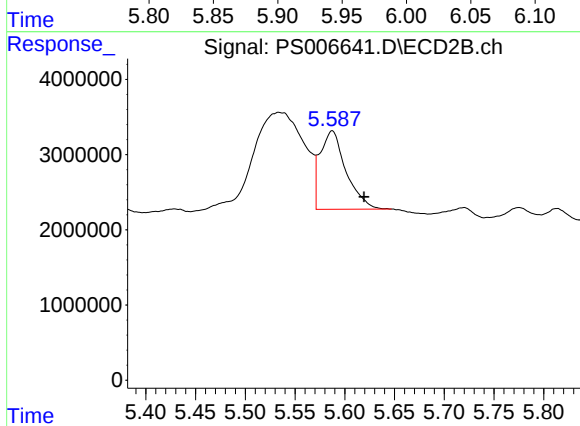

#7 MCPA


R.T.: 5.587 min
Delta R.T.: -0.032 min
Response: 18883592
Conc: 10.77 ug/ml

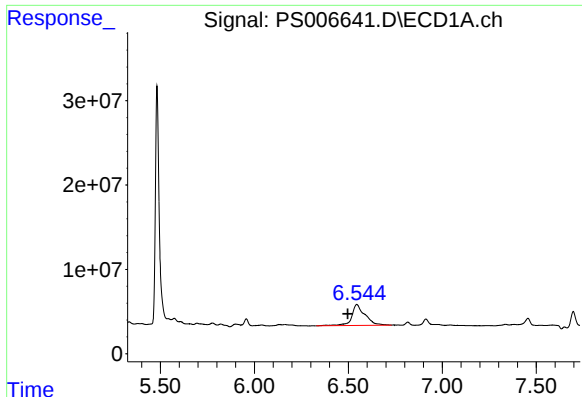

#9 2,4-D


R.T.: 6.545 min
Delta R.T.: 0.048 min
Response: 121362301
Conc: 157.08 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB122893BL

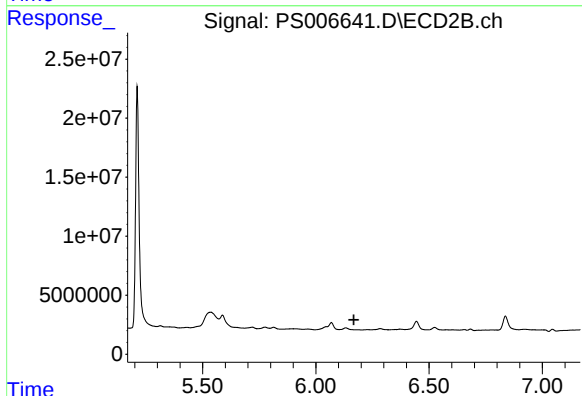


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.168 min
Response: 0
Conc: N.D.

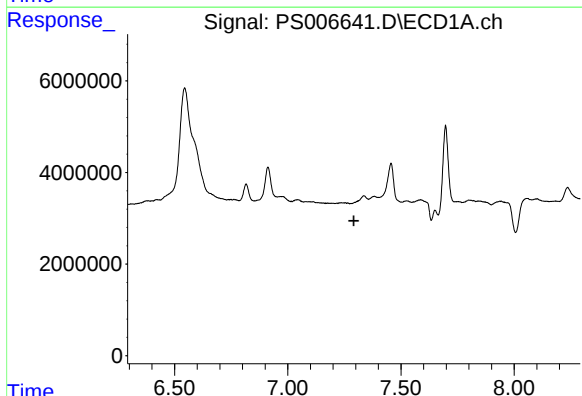


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.292 min
Response: 0
Conc: N.D.

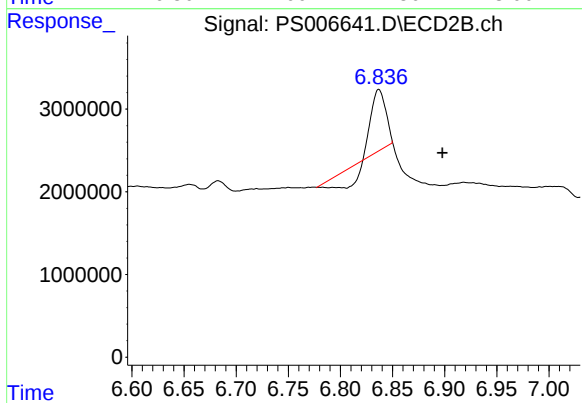

#11 2,4,5-TP (SILVEX)


R.T.: 6.837 min
Delta R.T.: -0.061 min
Response: 4239936
Conc: 1.86 ng/ml

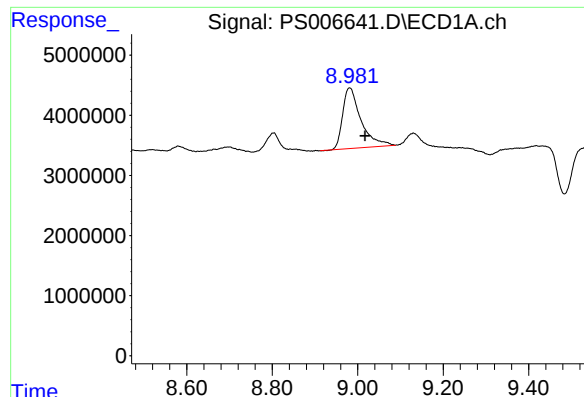

#15 Picloram

R.T.: 8.981 min
Delta R.T.: -0.036 min
Response: 29897554
Conc: 4.43 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB122893BL

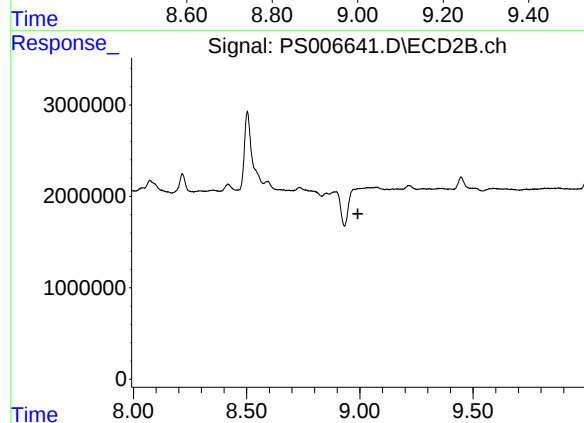

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 8.991 min
Response: 0
Conc: N.D.