

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090919\
 Data File : PS006643.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2019 01:31
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 06:38:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 10 06:14:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.487	5.214	299.9E6	171.8E6	386.073	402.420
Target Compounds							
9) T	2,4-D	6.546	0.000	123.1E6	0	159.271	N.D. #
15) T	Picloram	9.072	9.004	50703221	26101529	7.516	7.053
16) T	DCPA	0.000	9.004	0	26101529	N.D.	8.286



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090919\
Data File : PS006643.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2019 01:31
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 06:38:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
Quant Title : 8080.M
QLast Update : Tue Sep 10 06:14:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

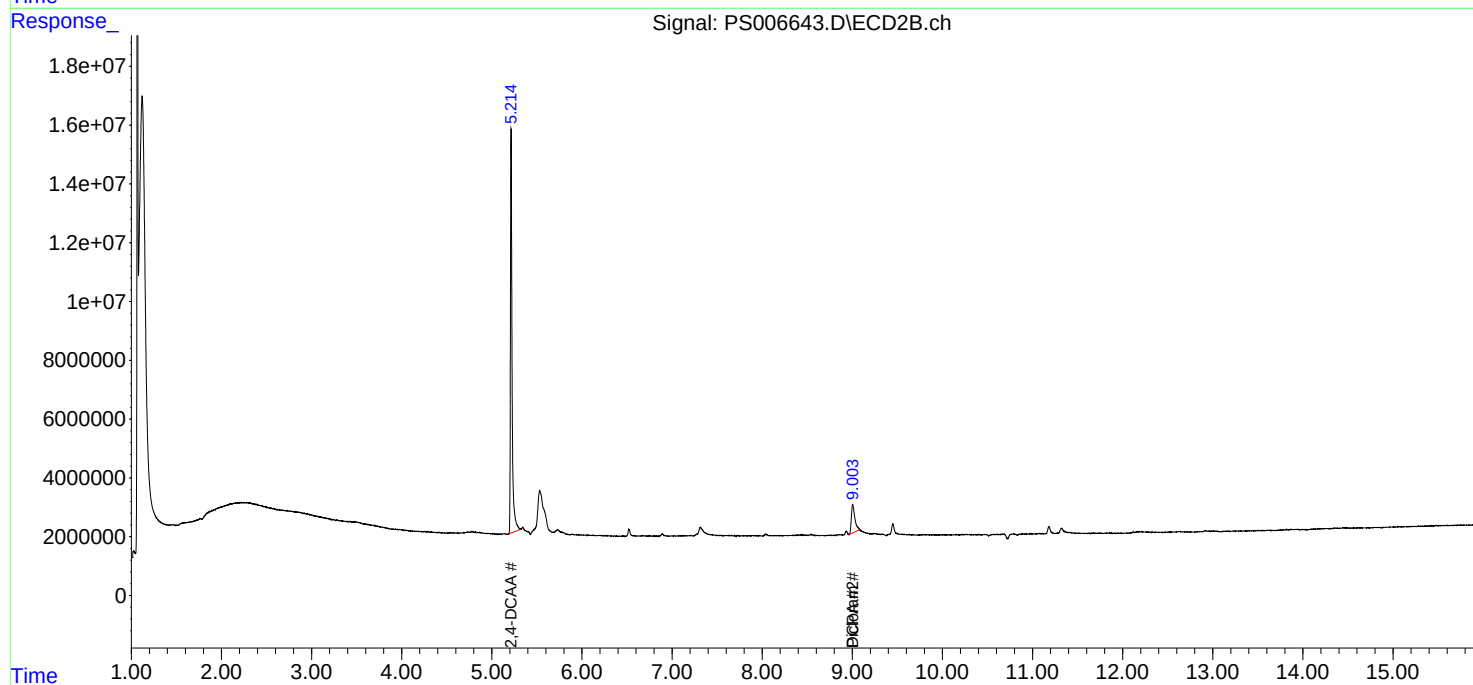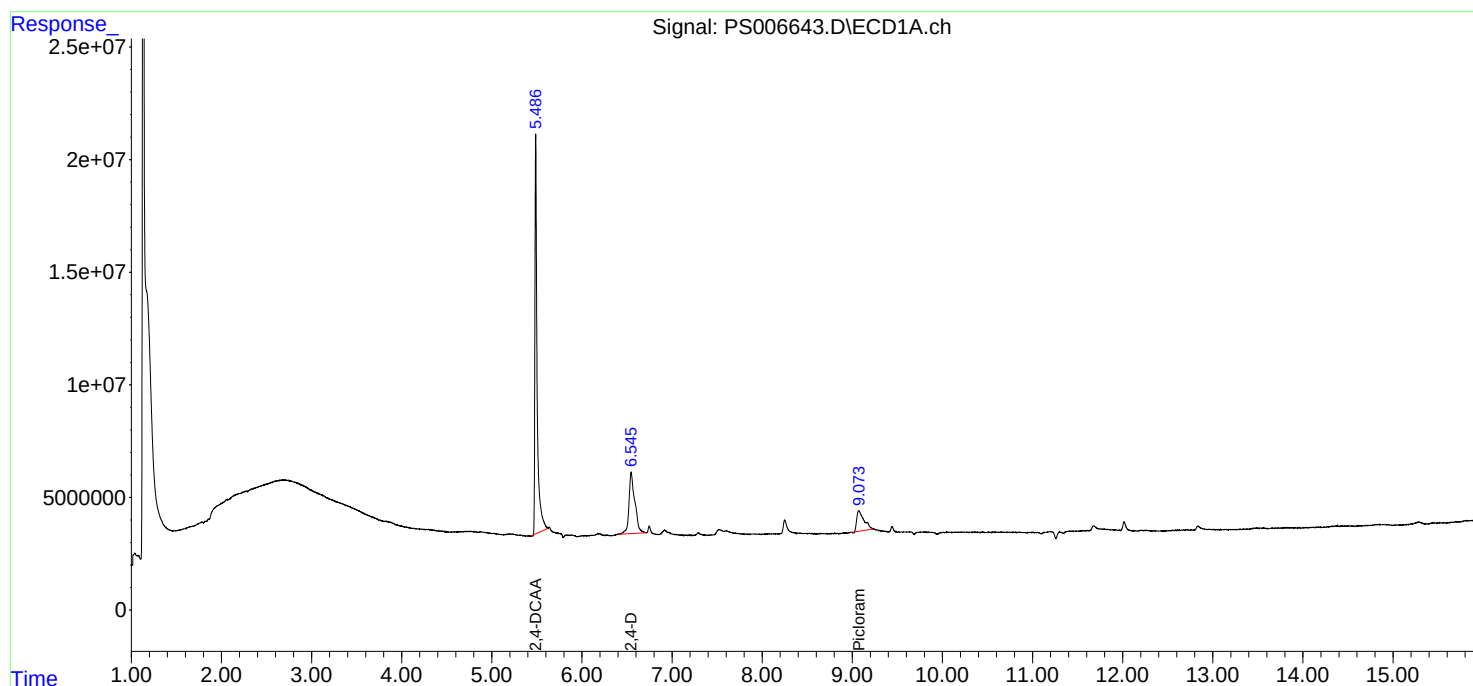


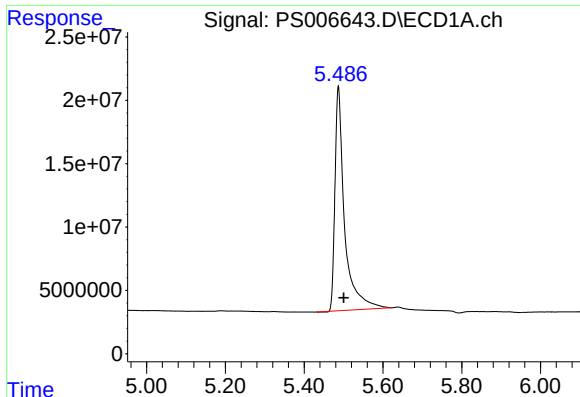

#4 2,4-DCAA


R.T.: 5.487 min
Delta R.T.: -0.014 min
Response: 299934134
Conc: 386.07 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

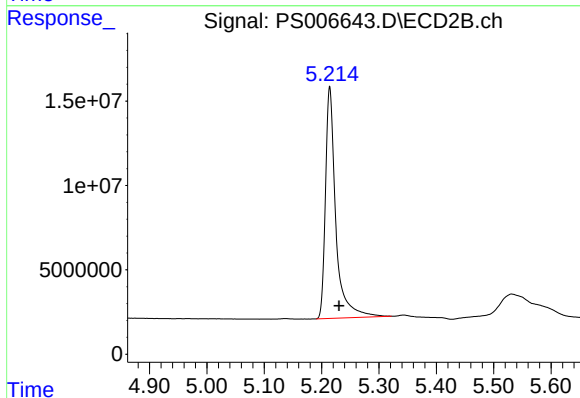


#4 2,4-DCAA

R.T.: 5.214 min
Delta R.T.: -0.016 min
Response: 171834182
Conc: 402.42 ng/ml

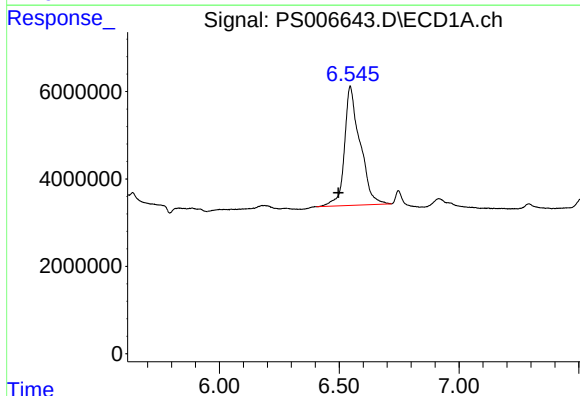


#9 2,4-D

R.T.: 6.546 min
Delta R.T.: 0.049 min
Response: 123056828
Conc: 159.27 ng/ml

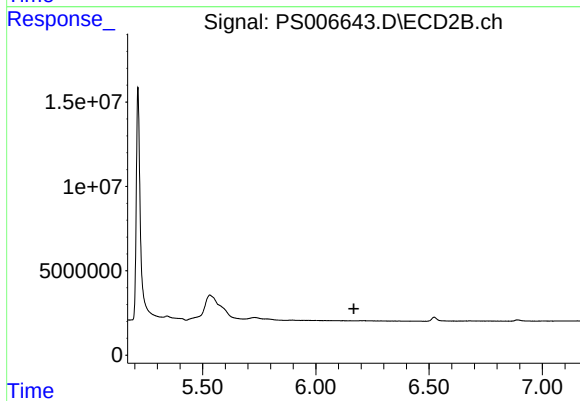

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.168 min
Response: 0
Conc: N.D.

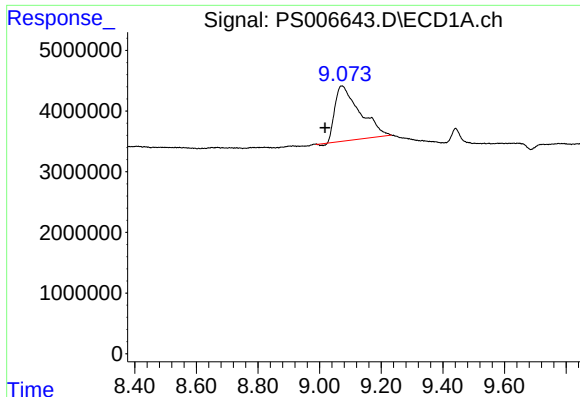

#15 Picloram


R.T.: 9.072 min
Delta R.T.: 0.055 min
Response: 50703221
Conc: 7.52 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

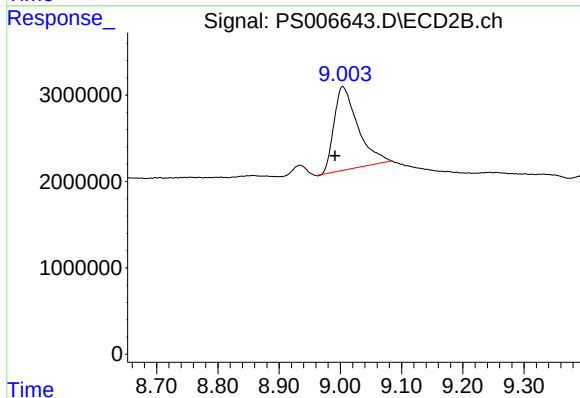


#15 Picloram

R.T.: 9.004 min
Delta R.T.: 0.013 min
Response: 26101529
Conc: 7.05 ng/ml

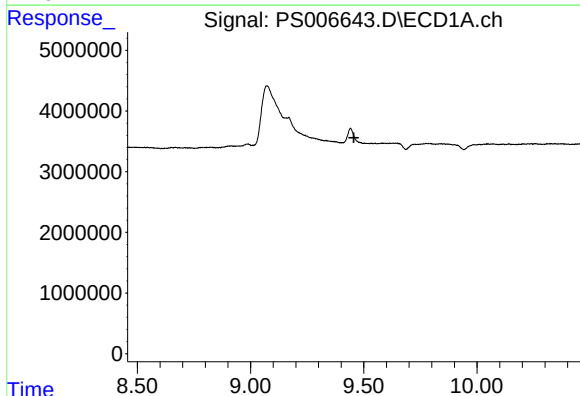

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.456 min
Response: 0
Conc: N.D.

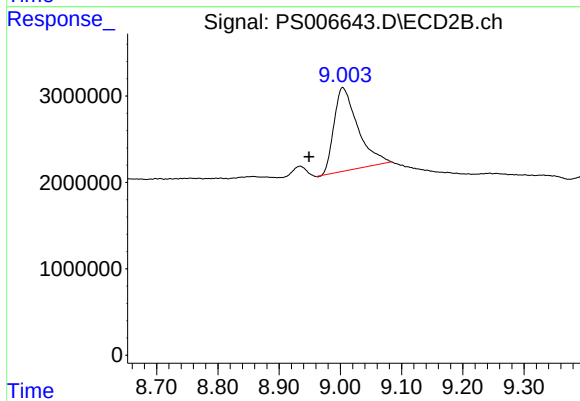

#16 DCPA

R.T.: 9.004 min
Delta R.T.: 0.055 min
Response: 26101529
Conc: 8.29 ng/ml