

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090919\
 Data File : PS006653.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2019 05:11
 Operator : SM\AJ
 Sample : K4762-01
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 STOCK-PILE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 06:42:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 10 06:14:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.483	5.214	203.9E6	113.6E6	262.416	266.048
Target Compounds							
1) T	Dalapon	2.030	1.742	90261568	96555756	92.349	188.937 #
2) T	3,5-DICHL...	4.866	4.542	9577943	40536475	9.675	74.894 #
3) T	4-Nitroph...	5.404	0.000	10916624	0	30.762	N.D. #
5) T	DICAMBA	5.648	0.000	9776781	0	3.391	N.D. #
7) T	MCPA	5.961	5.591	20156878	19003713	7.132	10.834 #
8) T	DICHLORPROP	6.306	0.000	5343279	0	7.513	N.D. #
9) T	2,4-D	6.498	0.000	36990095	0	47.876	N.D. #
10) T	Pentachlo...	6.740	6.520	34831541	23326876	3.127	3.872
11) T	2,4,5-TP ...	0.000	6.835	0	9617387	N.D.	4.225
13) T	2,4-DB	8.117	0.000	55492098	0	91.187	N.D. #
15) T	Picloram	9.024	0.000	17872273	0	2.649	N.D. #
16) T	DCPA	9.449	0.000	76176543	0	13.485	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090919\
Data File : PS006653.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2019 05:11
Operator : SM\AJ
Sample : K4762-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleID :
STOCK-PILE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 06:42:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
Quant Title : 8080.M
QLast Update : Tue Sep 10 06:14:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

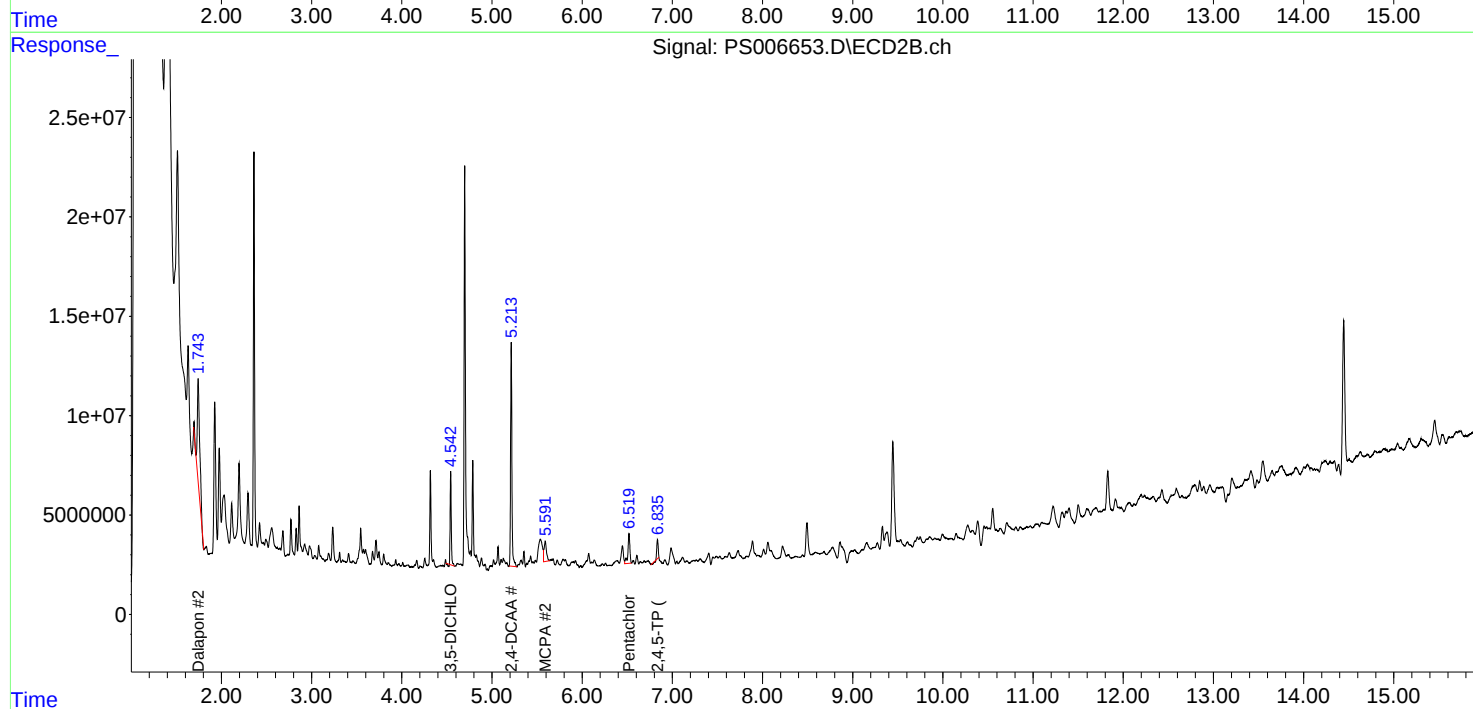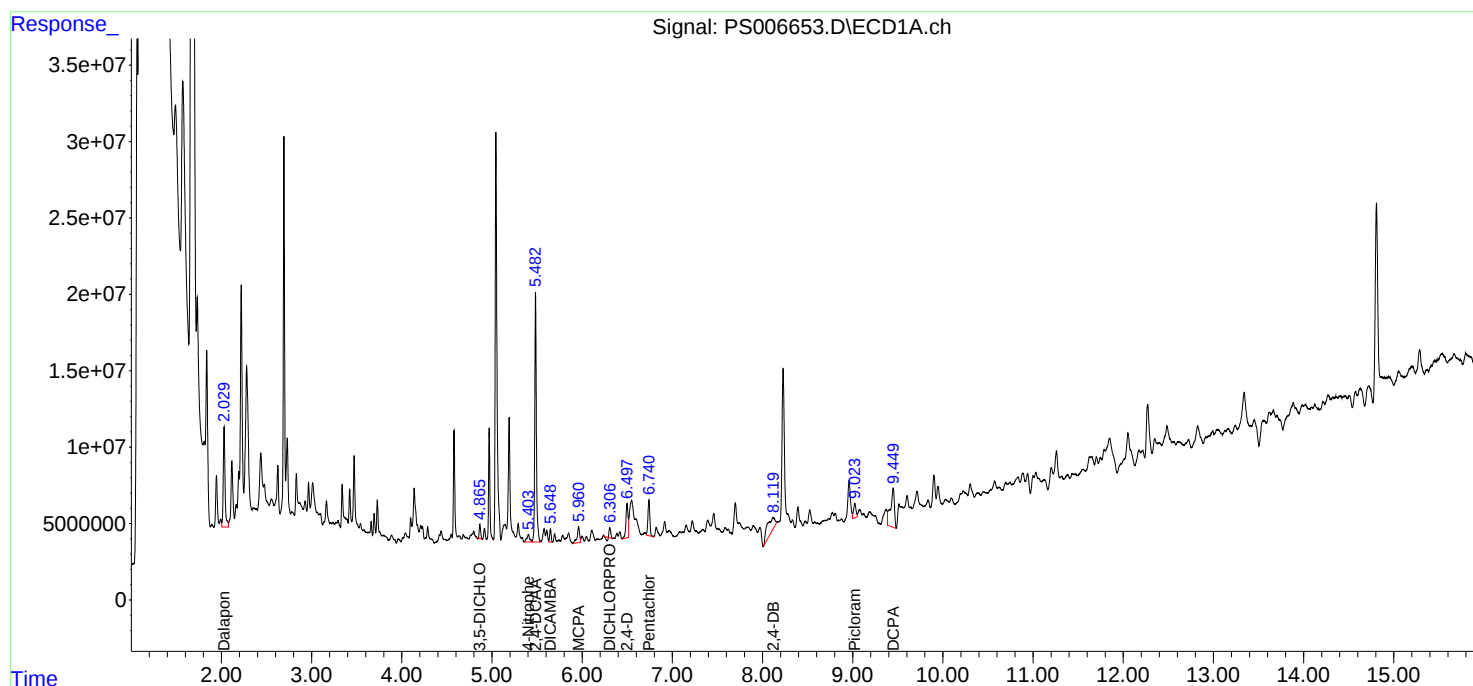


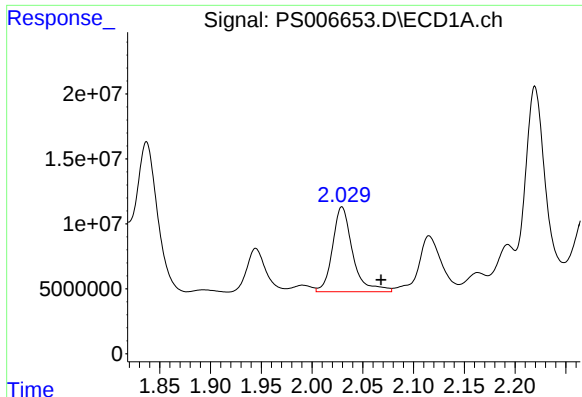

#1 Dalapon


R.T.: 2.030 min
Delta R.T.: -0.038 min
Response: 90261568
Conc: 92.35 ng/ml

Instrument :
ECD_S
ClientSampleId :
STOCK-PILE

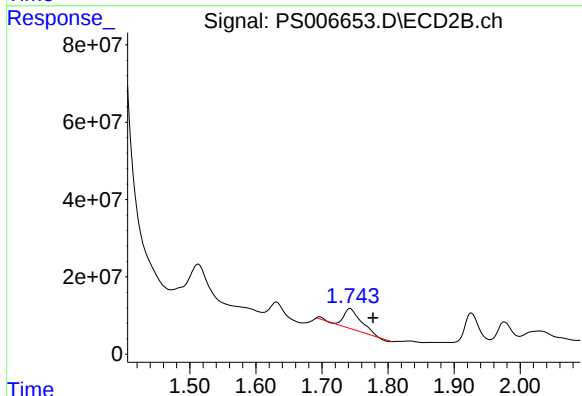


#1 Dalapon

R.T.: 1.742 min
Delta R.T.: -0.035 min
Response: 96555756
Conc: 188.94 ng/ml

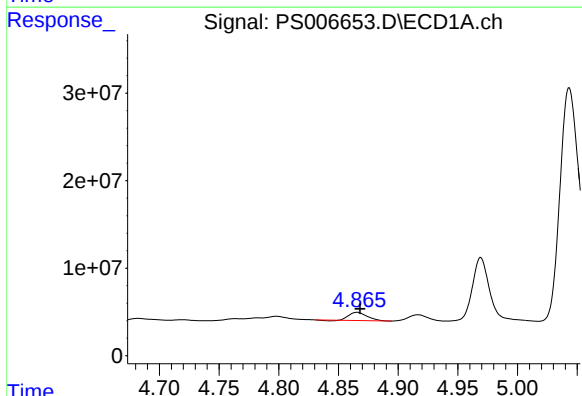


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.866 min
Delta R.T.: -0.002 min
Response: 9577943
Conc: 9.67 ng/ml

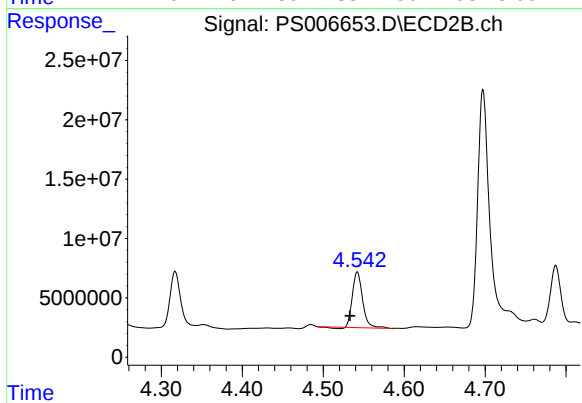

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.542 min
Delta R.T.: 0.009 min
Response: 40536475
Conc: 74.89 ng/ml

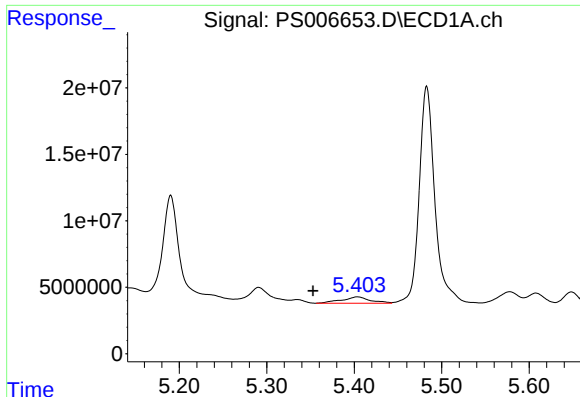

#3 4-Nitrophenol


R.T.: 5.404 min
Delta R.T.: 0.051 min
Response: 10916624
Conc: 30.76 ng/ml

Instrument :
ECD_S
ClientSampleId :
STOCK-PILE

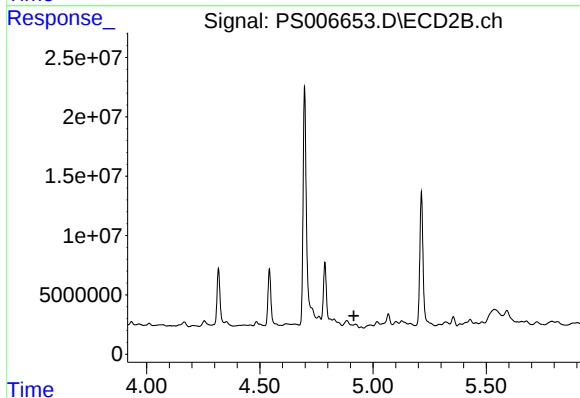


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 4.915 min
Response: 0
Conc: N.D.

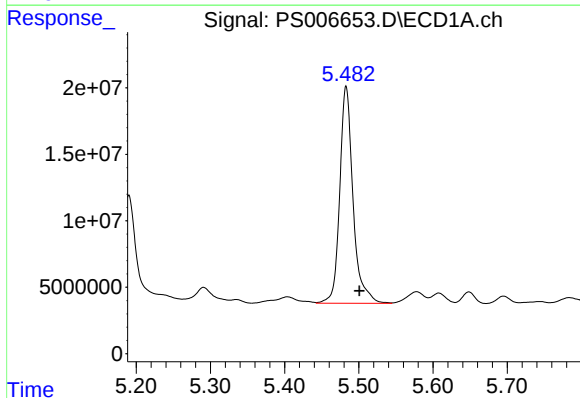


#4 2,4-DCAA

R.T.: 5.483 min
Delta R.T.: -0.018 min
Response: 203867092
Conc: 262.42 ng/ml

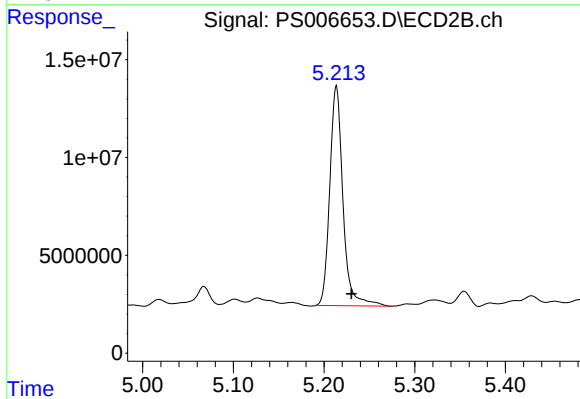

#4 2,4-DCAA


R.T.: 5.214 min
Delta R.T.: -0.017 min
Response: 113602952
Conc: 266.05 ng/ml

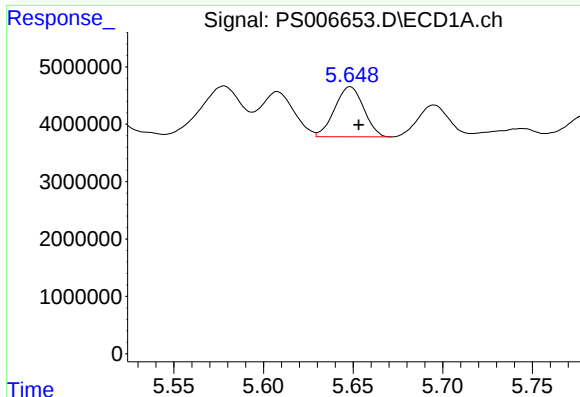

#5 DICAMBA


R.T.: 5.648 min
Delta R.T.: -0.005 min
Response: 9776781
Conc: 3.39 ng/ml

Instrument :
ECD_S
ClientSampleId :
STOCK-PILE

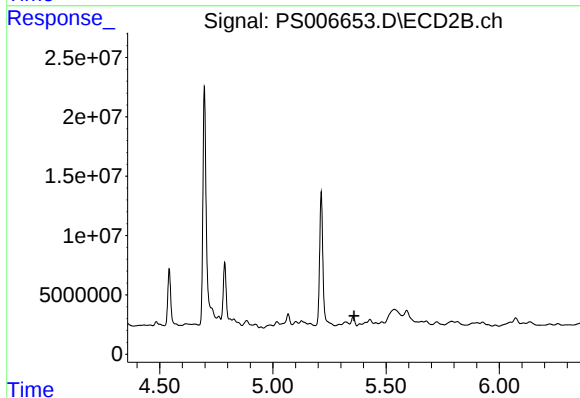


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.358 min
Response: 0
Conc: N.D.

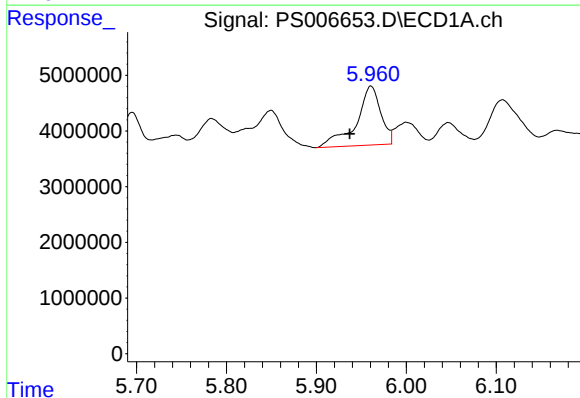


#7 MCPA

R.T.: 5.961 min
Delta R.T.: 0.024 min
Response: 20156878
Conc: 7.13 ug/ml

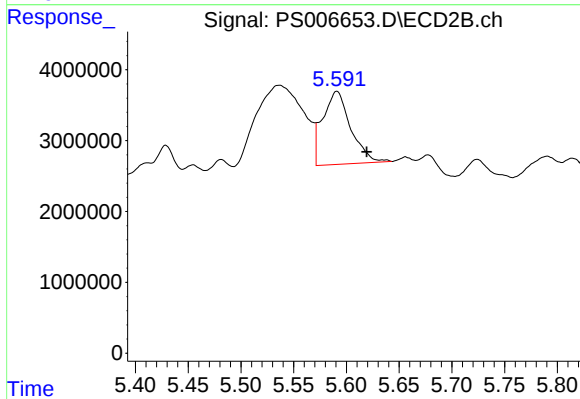

#7 MCPA


R.T.: 5.591 min
Delta R.T.: -0.028 min
Response: 19003713
Conc: 10.83 ug/ml

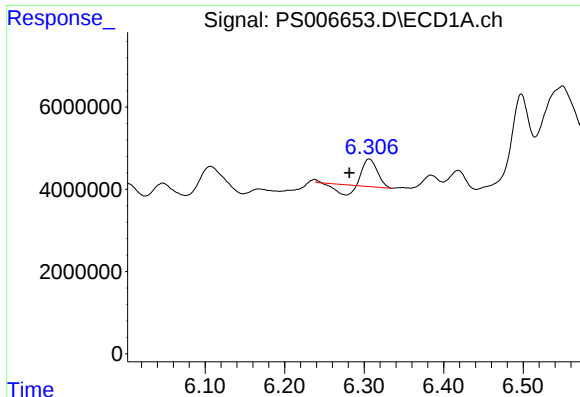

#8 DICHLORPROP


R.T.: 6.306 min
Delta R.T.: 0.025 min
Response: 5343279
Conc: 7.51 ng/ml

Instrument :
ECD_S
ClientSampleId :
STOCK-PILE

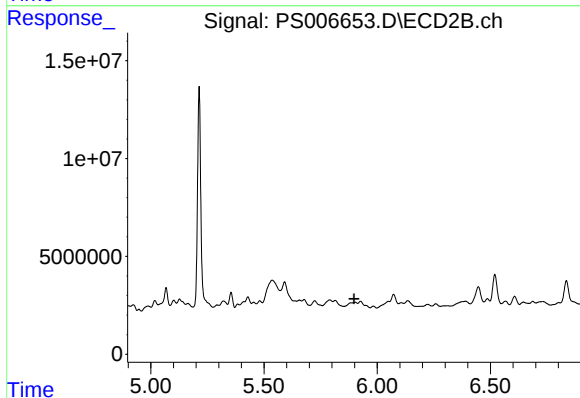


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 5.897 min
Response: 0
Conc: N.D.

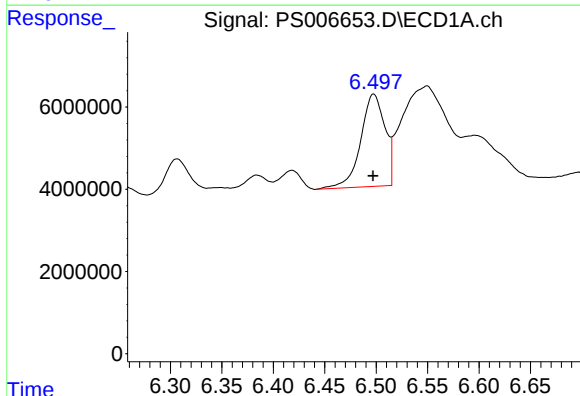


#9 2,4-D

R.T.: 6.498 min
Delta R.T.: 0.000 min
Response: 36990095
Conc: 47.88 ng/ml

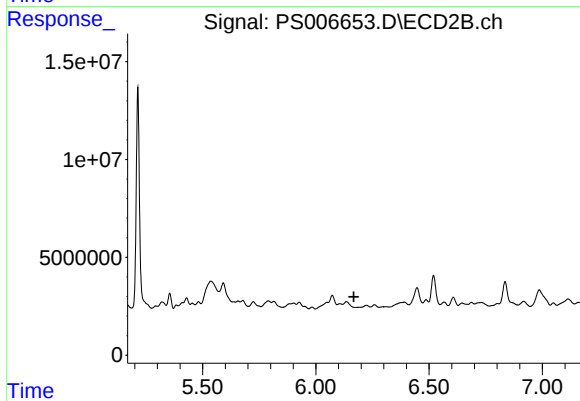

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 6.168 min
Response: 0
Conc: N.D.

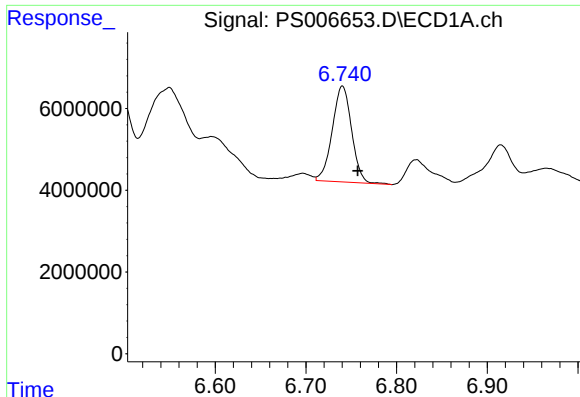

#10 Pentachlorophenol


R.T.: 6.740 min
Delta R.T.: -0.017 min
Response: 34831541
Conc: 3.13 ng/ml

Instrument :
ECD_S
ClientSampleId :
STOCK-PILE

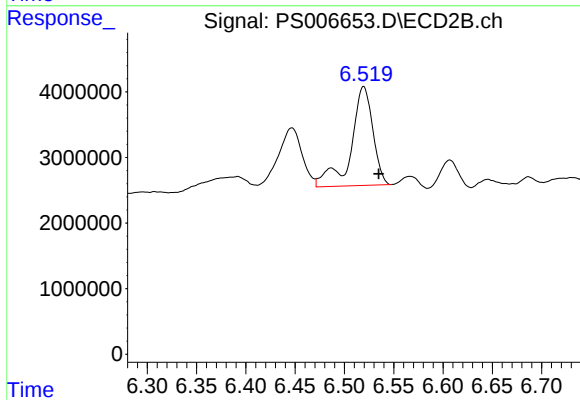


#10 Pentachlorophenol

R.T.: 6.520 min
Delta R.T.: -0.015 min
Response: 23326876
Conc: 3.87 ng/ml

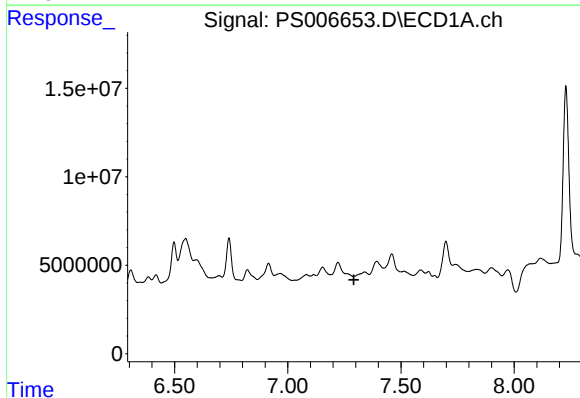


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.292 min
Response: 0
Conc: N.D.

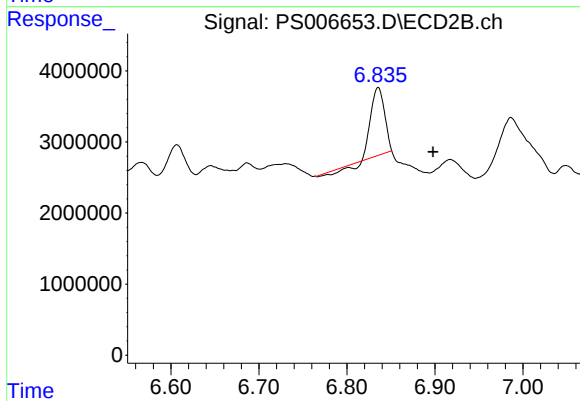

#11 2,4,5-TP (SILVEX)


R.T.: 6.835 min
Delta R.T.: -0.062 min
Response: 9617387
Conc: 4.22 ng/ml

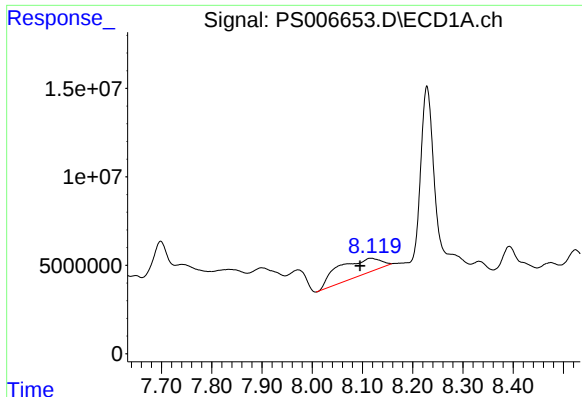

#13 2,4-DB


R.T.: 8.117 min
Delta R.T.: 0.022 min
Response: 55492098
Conc: 91.19 ng/ml

Instrument :
ECD_S
ClientSampleId :
STOCK-PILE

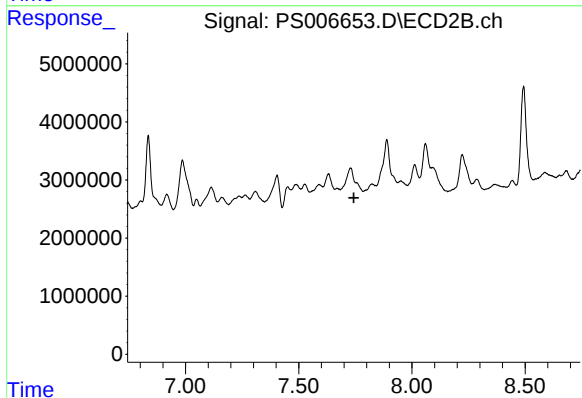


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 7.744 min
Response: 0
Conc: N.D.

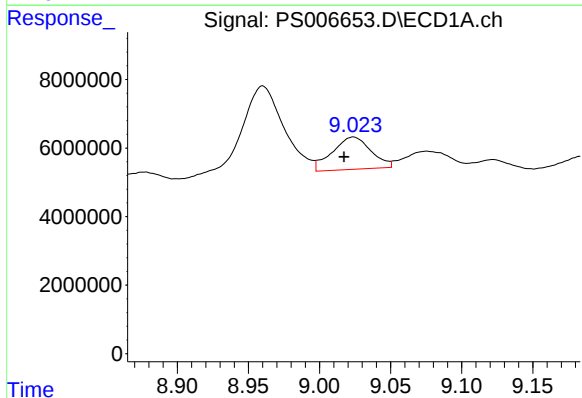


#15 Picloram

R.T.: 9.024 min
Delta R.T.: 0.006 min
Response: 17872273
Conc: 2.65 ng/ml

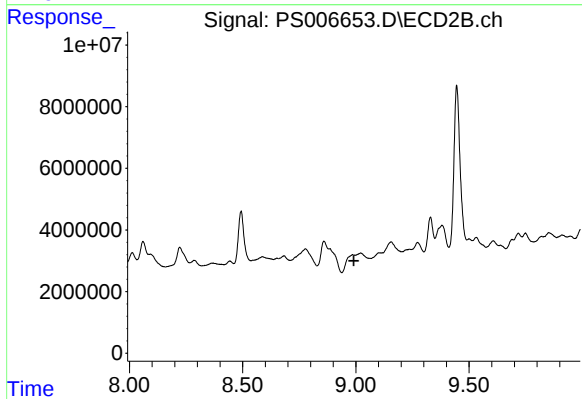

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 8.991 min
Response: 0
Conc: N.D.

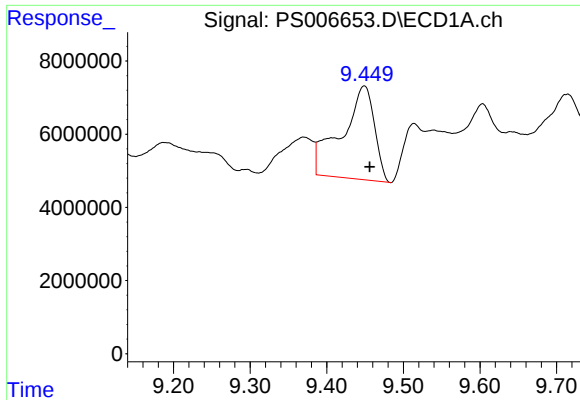

#16 DCPA

R.T.: 9.449 min
Delta R.T.: -0.007 min
Response: 76176543
Conc: 13.48 ng/ml

Instrument :
ECD_S
ClientSampleId :
STOCK-PILE

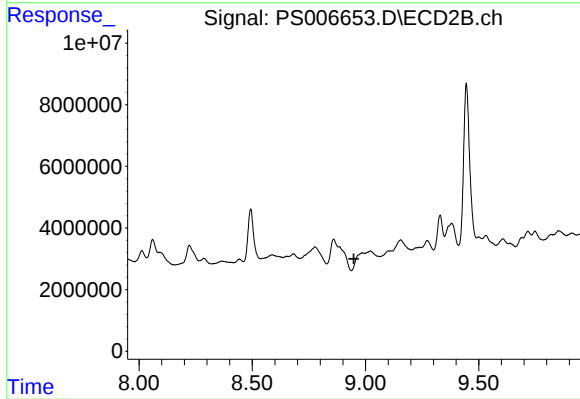

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 8.949 min
Response: 0
Conc: N.D.