

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090920\
 Data File : PS012174.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2020 09:17
 Operator : DD\AJ
 Sample : L3864-07
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CL-01-090320

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 10:46:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.217	6.914	257.8E6	157.9E6	236.341	295.308
Target Compounds							
2) T	3,5-DICHL...	0.000	6.095	0	57814196	N.D.	70.281
5) T	DICAMBA	7.480	7.047	7026259	4035452	1.715	1.868
7) T	MCPA	7.705	0.000	98152923	0	21.579	N.D. #
9) T	2,4-D	8.398	7.941	110.9E6	79336031	98.180	107.990
11) T	2,4,5-TP ...	0.000	8.762	0	10000755	N.D.	3.421
12) T	2,4,5-T	9.407	9.239	34477875	18123191	5.818	6.123
15) T	Picloram	11.027	11.012	93190306	82718987	11.924	18.250 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090920\
Data File : PS012174.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2020 09:17
Operator : DD\AJ
Sample : L3864-07
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CL-01-090320

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 10:46:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

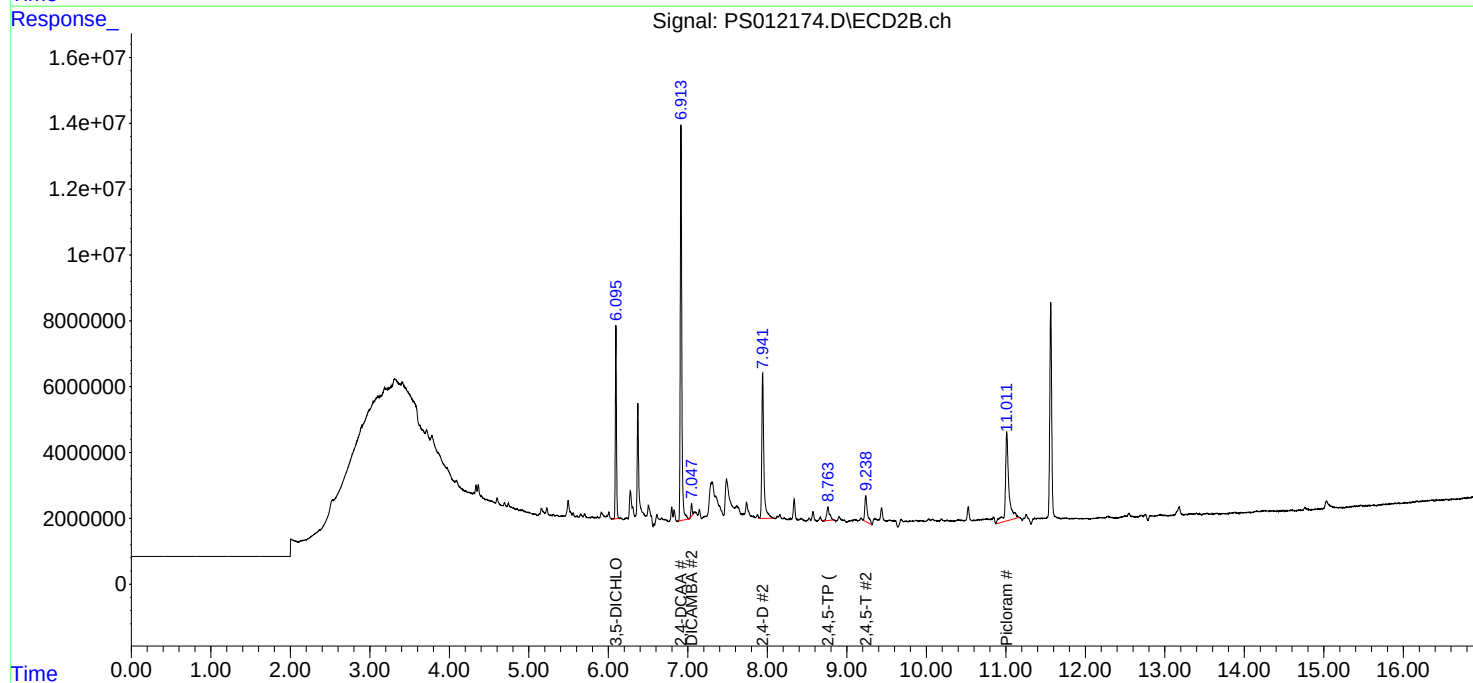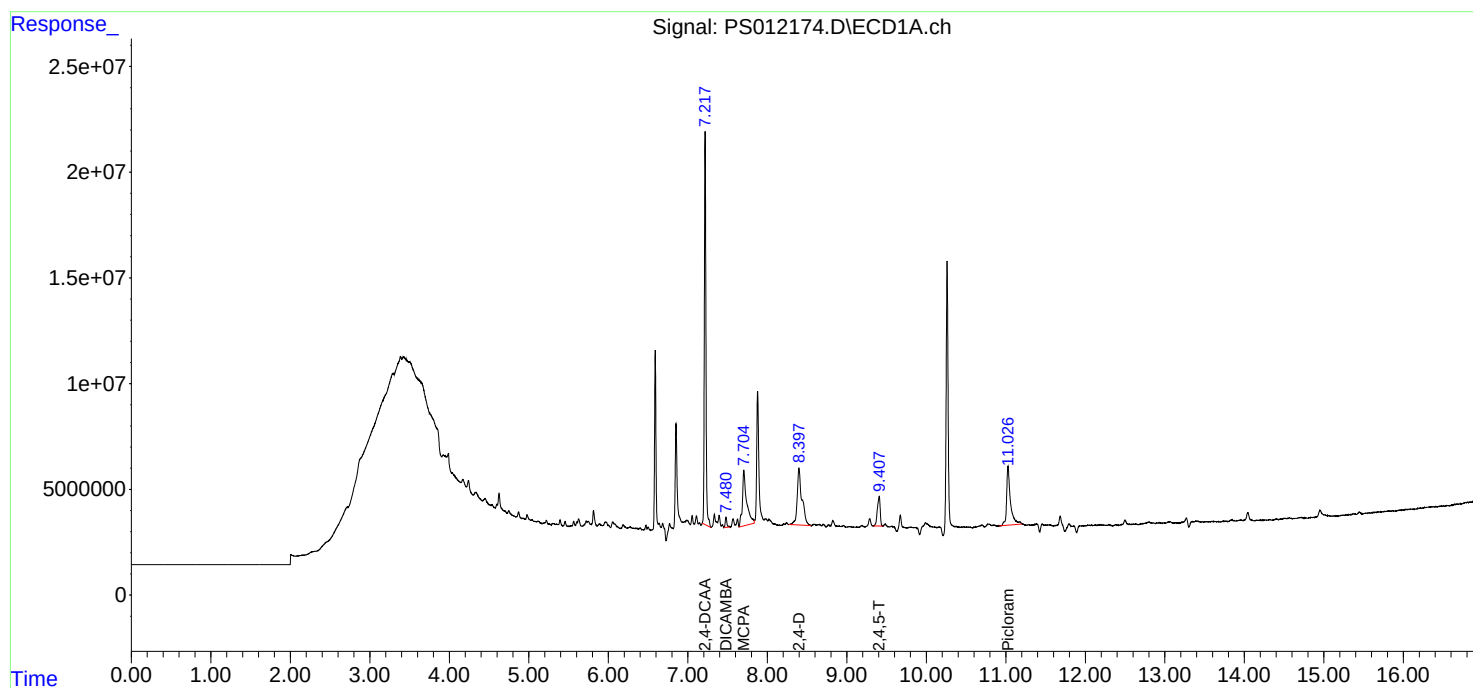


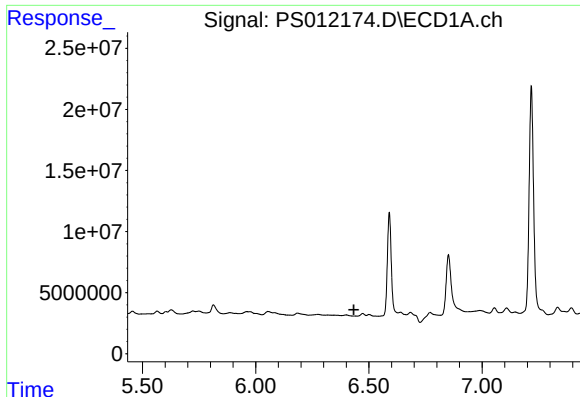

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-01-090320

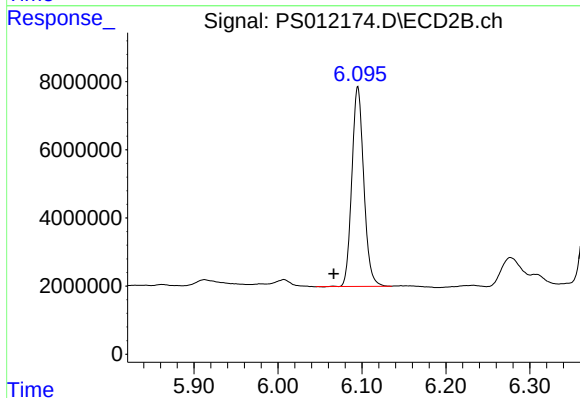


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.095 min
Delta R.T.: 0.029 min
Response: 57814196
Conc: 70.28 ng/ml

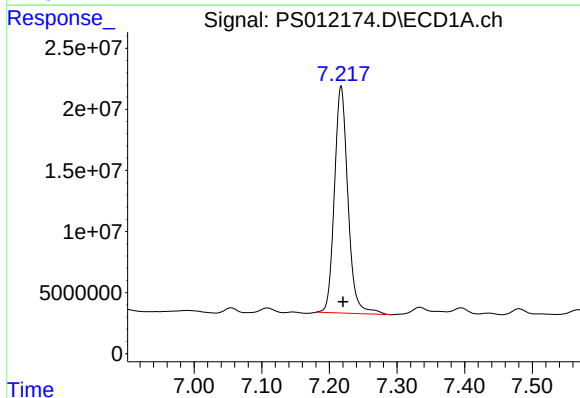


#4 2,4-DCAA

R.T.: 7.217 min
Delta R.T.: -0.003 min
Response: 257793808
Conc: 236.34 ng/ml

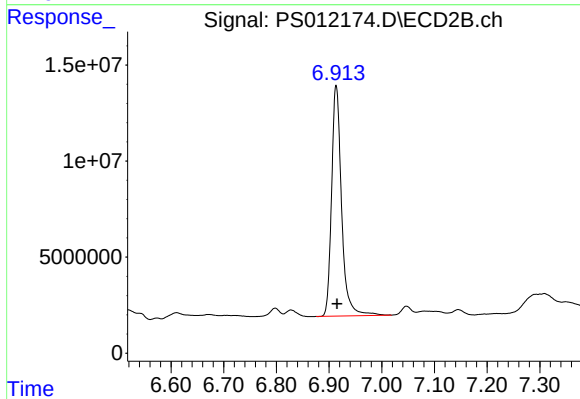

#4 2,4-DCAA


R.T.: 6.914 min
Delta R.T.: -0.001 min
Response: 157927060
Conc: 295.31 ng/ml

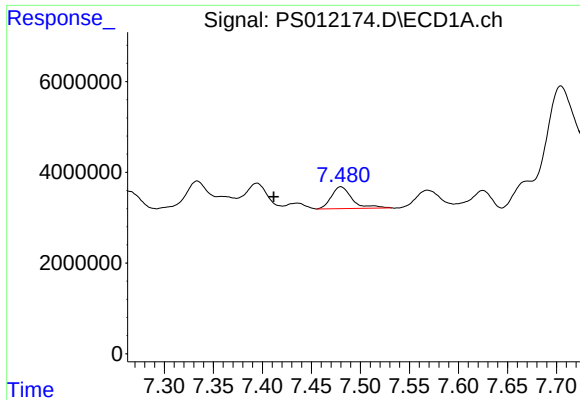

#5 DICAMBA


R.T.: 7.480 min
Delta R.T.: 0.069 min
Response: 7026259
Conc: 1.72 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-01-090320

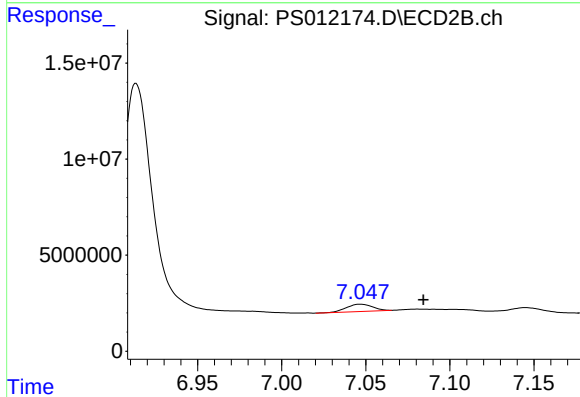


#5 DICAMBA

R.T.: 7.047 min
Delta R.T.: -0.037 min
Response: 4035452
Conc: 1.87 ng/ml

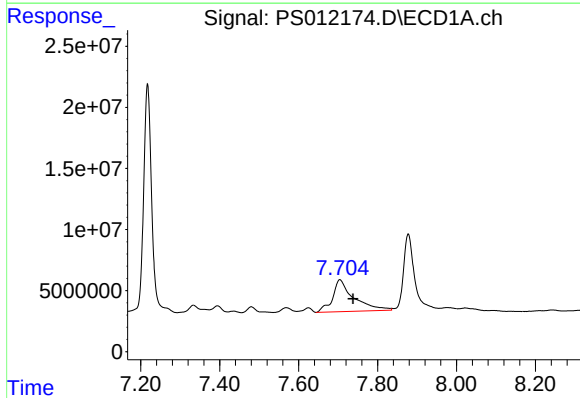


#7 MCPA

R.T.: 7.705 min
Delta R.T.: -0.034 min
Response: 98152923
Conc: 21.58 ug/ml

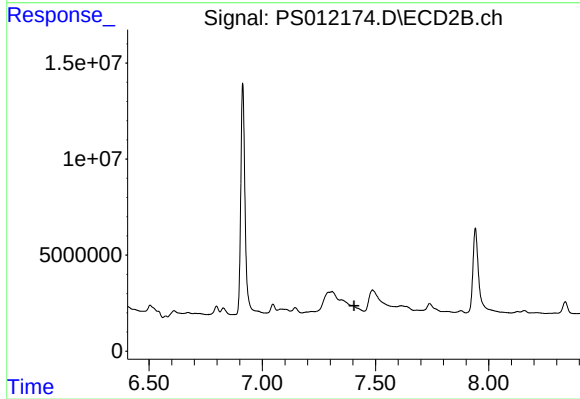

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.405 min
Response: 0
Conc: N.D.

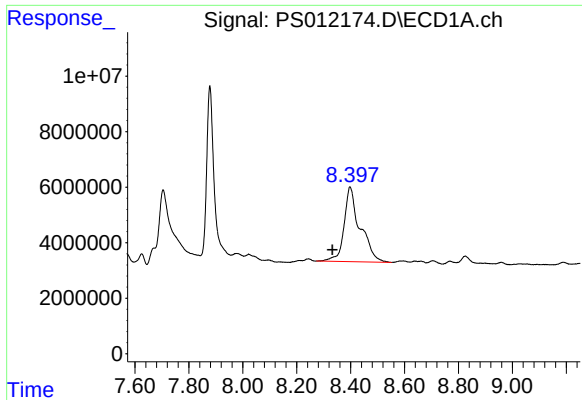

#9 2,4-D


R.T.: 8.398 min
Delta R.T.: 0.066 min
Response: 110854010
Conc: 98.18 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-01-090320

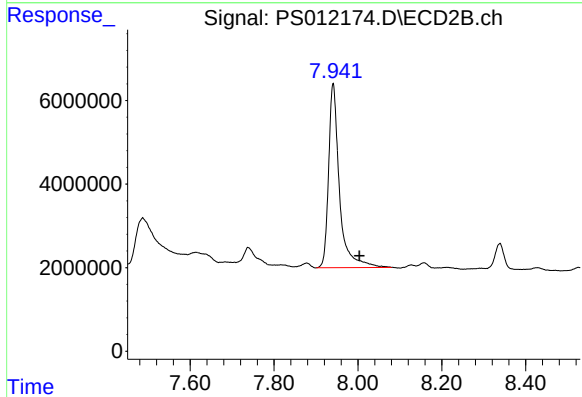


#9 2,4-D

R.T.: 7.941 min
Delta R.T.: -0.062 min
Response: 79336031
Conc: 107.99 ng/ml

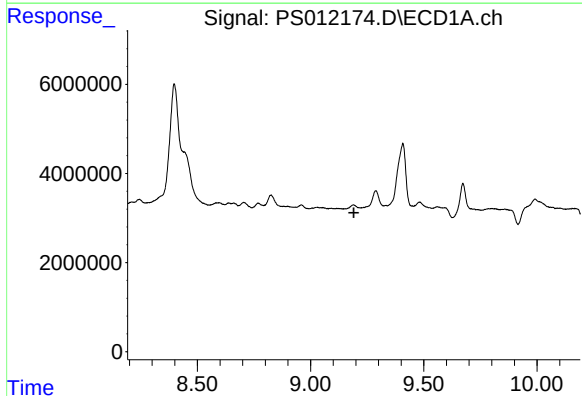


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.191 min
Response: 0
Conc: N.D.

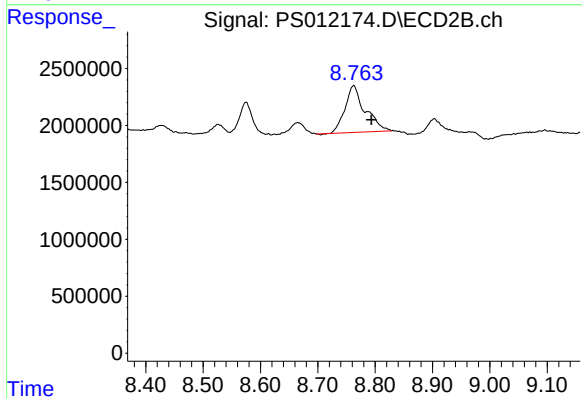

#11 2,4,5-TP (SILVEX)


R.T.: 8.762 min
Delta R.T.: -0.031 min
Response: 10000755
Conc: 3.42 ng/ml

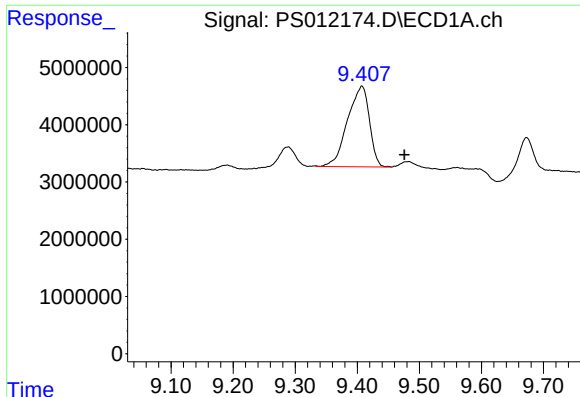

#12 2,4,5-T


R.T.: 9.407 min
Delta R.T.: -0.069 min
Response: 34477875
Conc: 5.82 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-01-090320

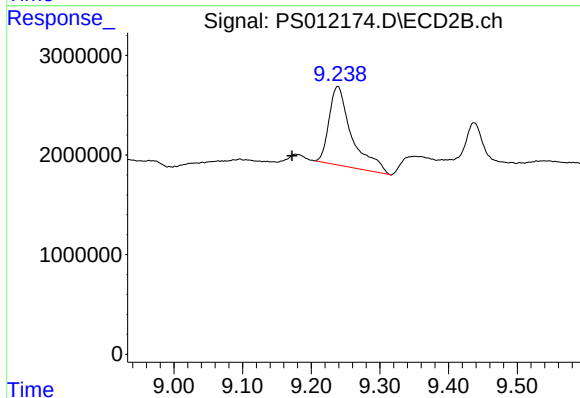


#12 2,4,5-T

R.T.: 9.239 min
Delta R.T.: 0.066 min
Response: 18123191
Conc: 6.12 ng/ml

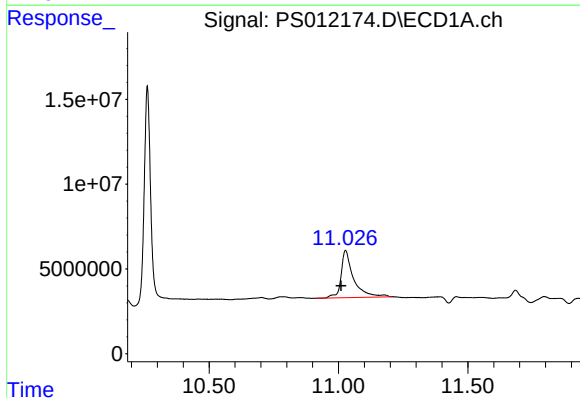

#15 Picloram

R.T.: 11.027 min
Delta R.T.: 0.018 min
Response: 93190306
Conc: 11.92 ng/ml

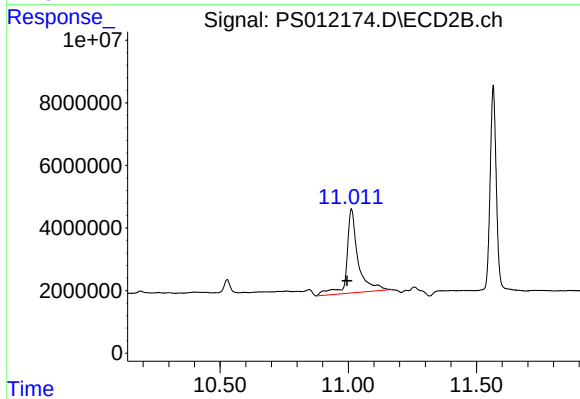

#15 Picloram

R.T.: 11.012 min
Delta R.T.: 0.017 min
Response: 82718987
Conc: 18.25 ng/ml