

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090920\
 Data File : PS012178.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2020 10:49
 Operator : DD\AJ
 Sample : PB131479TB
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 11:38:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.218	6.914	272.8E6	165.6E6	250.097	309.612
Target Compounds							
2) T	3,5-DICHL...	0.000	6.095	0 49054076		N.D.	59.632
5) T	DICAMBA	7.480	0.000	10331882	0	2.522	N.D. #
7) T	MCPA	7.700	0.000	202.6E6	0	44.535	N.D. #
8) T	DICHLORPROP	0.000	7.740	0 14155457		N.D.	25.070
9) T	2,4-D	8.399	0.000	117.9E6	0	104.414	N.D. #
11) T	2,4,5-TP ...	0.000	8.788	0 59382455		N.D.	20.311
12) T	2,4,5-T	9.410	0.000	18869679	0	3.184	N.D. #
15) T	Picloram	10.974	0.000	45219678	0	5.786	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090920\
Data File : PS012178.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2020 10:49
Operator : DD\AJ
Sample : PB131479TB
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 11:38:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

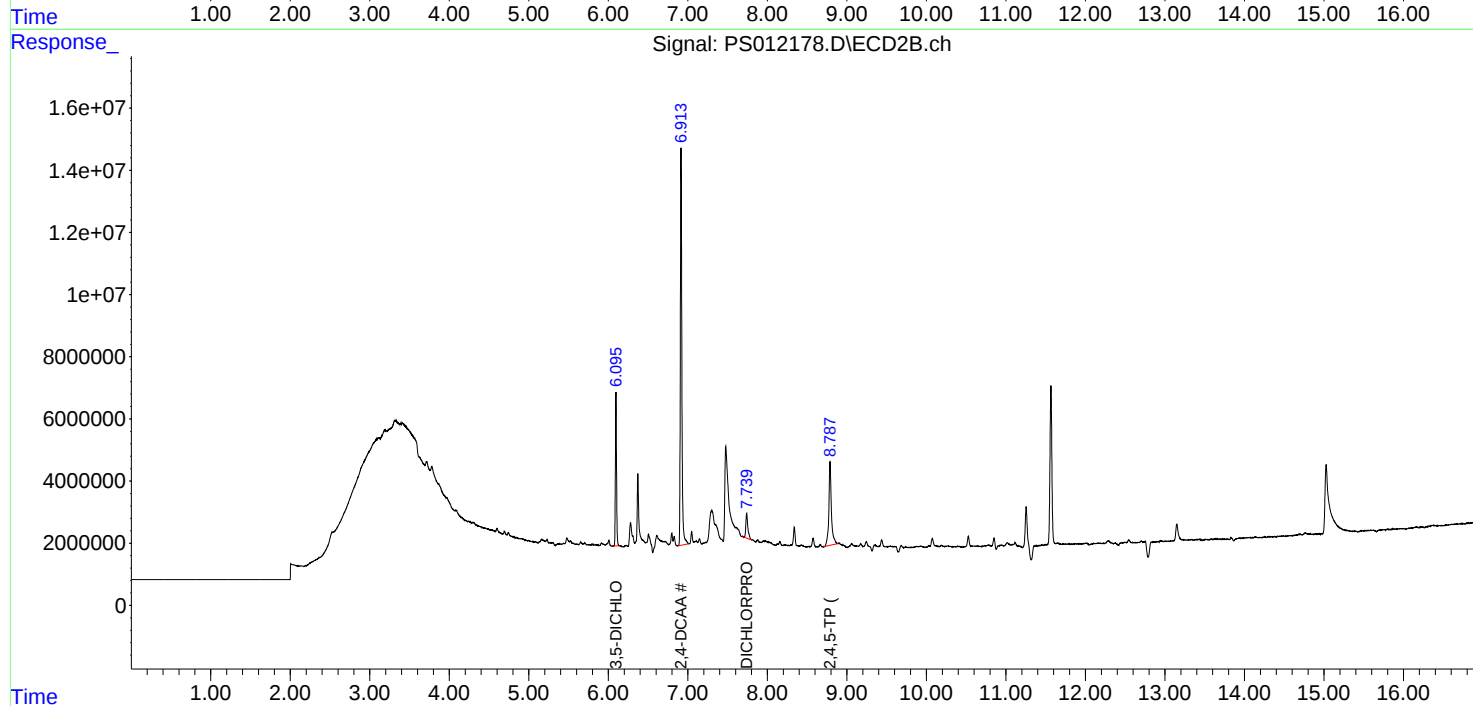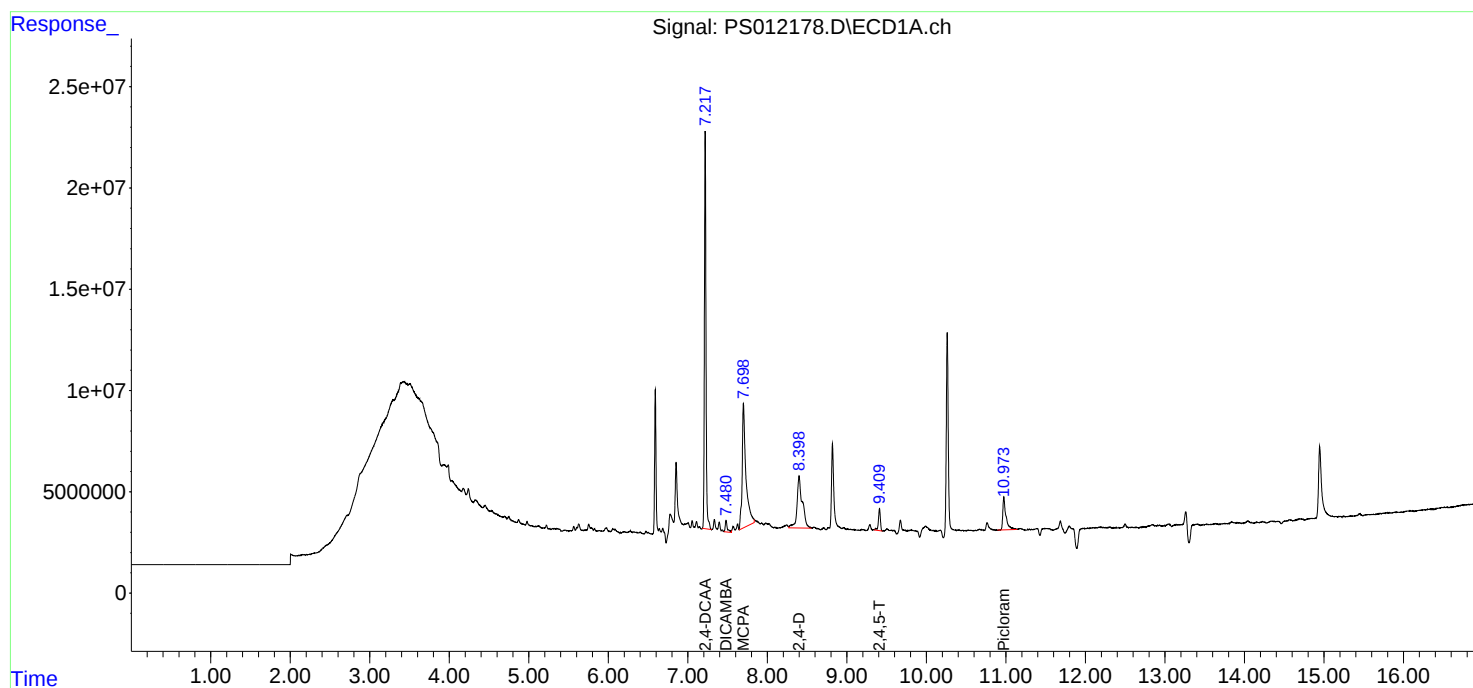


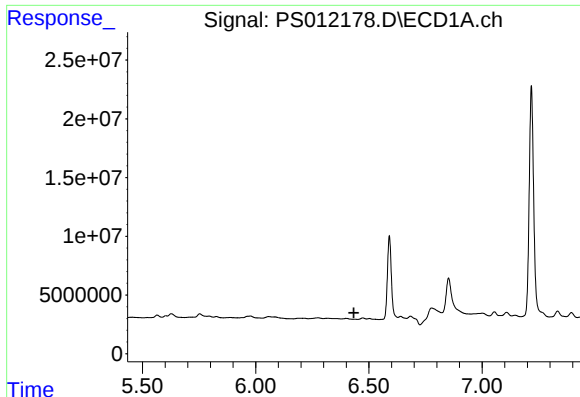

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

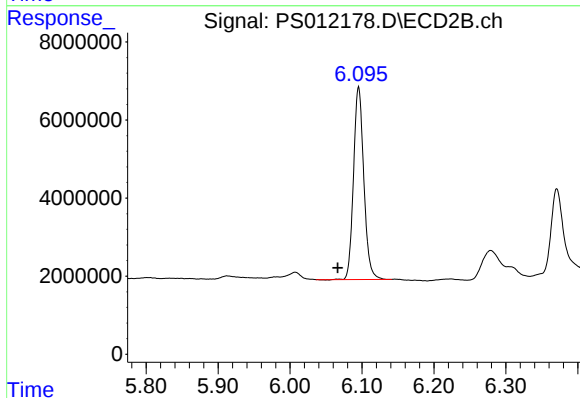


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.095 min
Delta R.T.: 0.029 min
Response: 49054076
Conc: 59.63 ng/ml

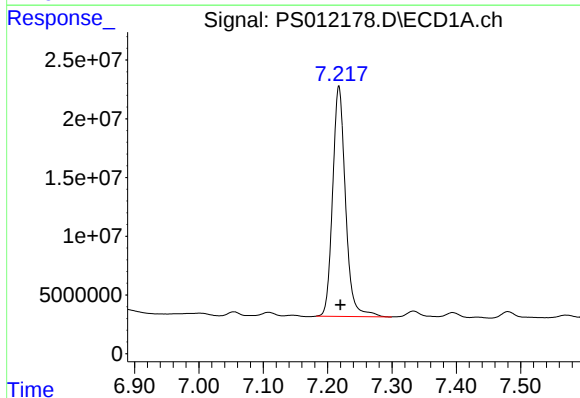


#4 2,4-DCAA

R.T.: 7.218 min
Delta R.T.: -0.002 min
Response: 272797965
Conc: 250.10 ng/ml

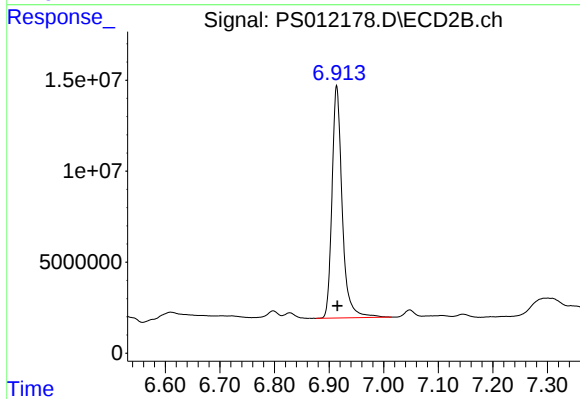

#4 2,4-DCAA


R.T.: 6.914 min
Delta R.T.: -0.001 min
Response: 165576178
Conc: 309.61 ng/ml

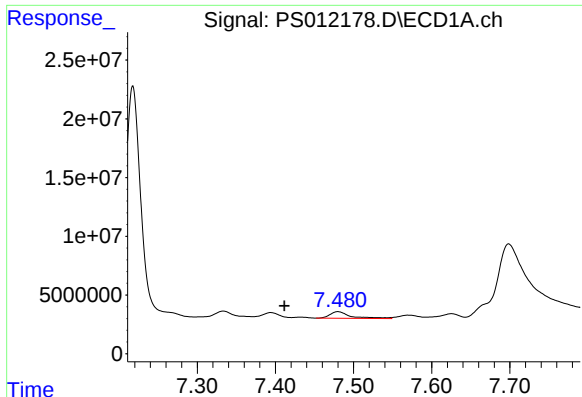

#5 DICAMBA


R.T.: 7.480 min
Delta R.T.: 0.069 min
Response: 10331882
Conc: 2.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

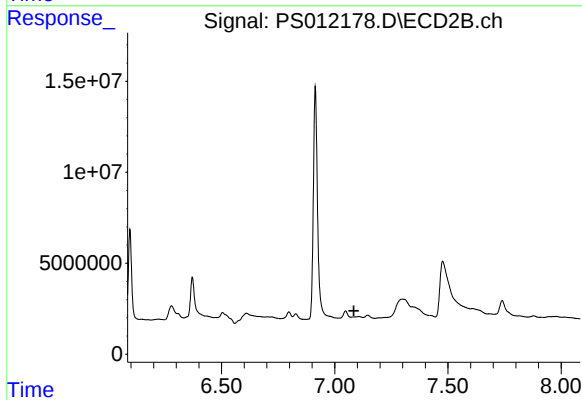


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.084 min
Response: 0
Conc: N.D.

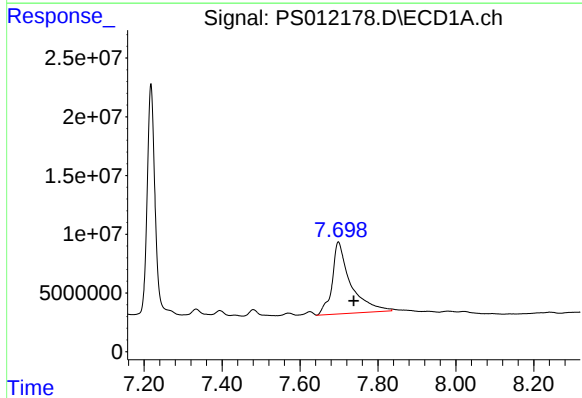


#7 MCPA

R.T.: 7.700 min
Delta R.T.: -0.038 min
Response: 202566507
Conc: 44.53 ug/ml

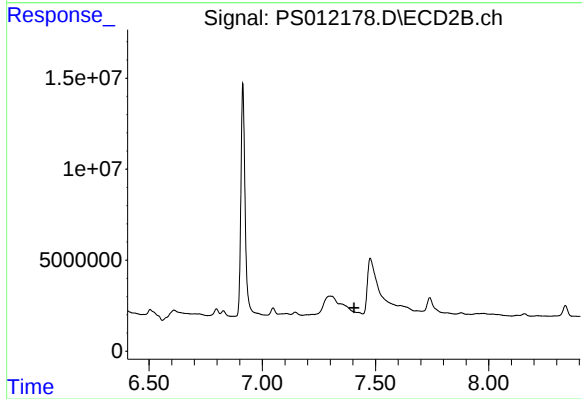

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.405 min
Response: 0
Conc: N.D.

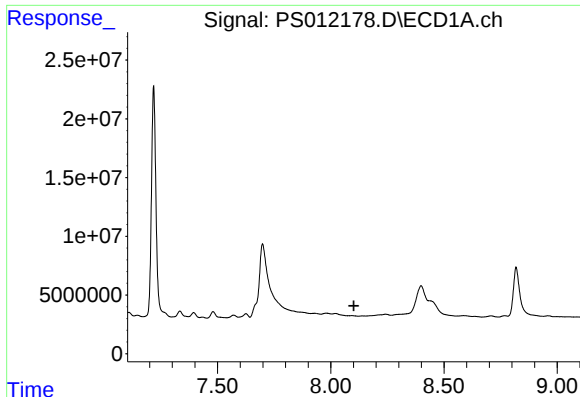

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

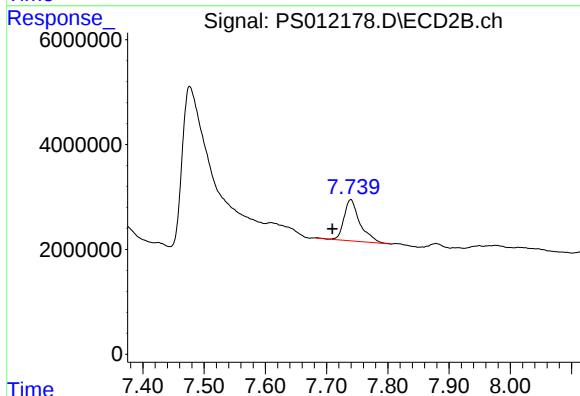


#8 DICHLORPROP

R.T.: 7.740 min
Delta R.T.: 0.030 min
Response: 14155457
Conc: 25.07 ng/ml

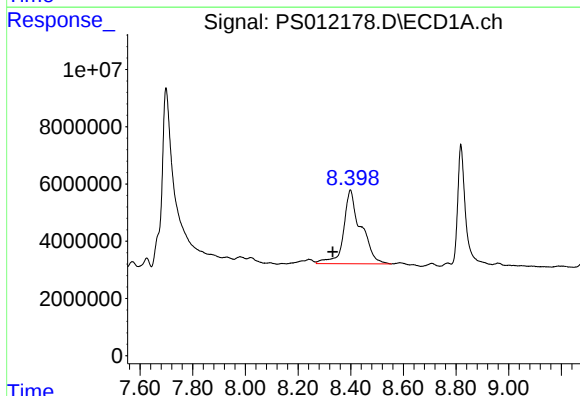


#9 2,4-D

R.T.: 8.399 min
Delta R.T.: 0.066 min
Response: 117893168
Conc: 104.41 ng/ml

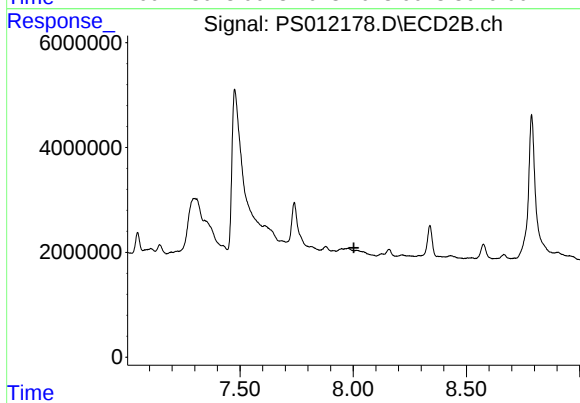

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.003 min
Response: 0
Conc: N.D.

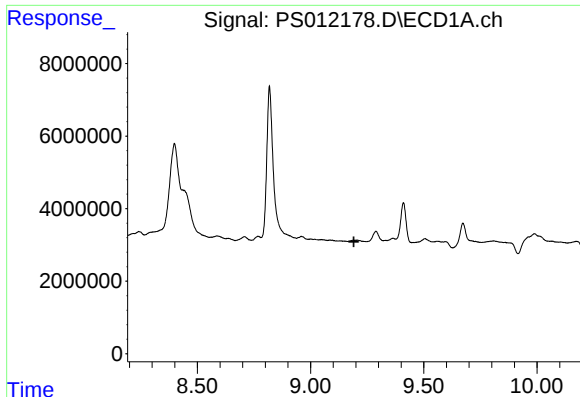

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

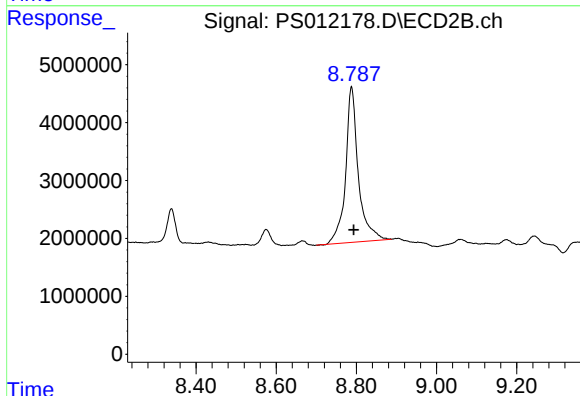


#11 2,4,5-TP (SILVEX)

R.T.: 8.788 min
Delta R.T.: -0.006 min
Response: 59382455
Conc: 20.31 ng/ml

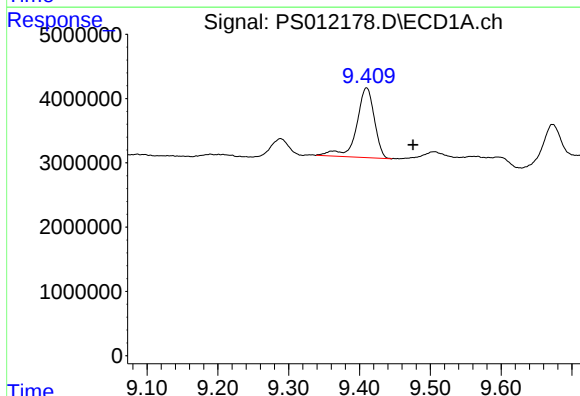


#12 2,4,5-T

R.T.: 9.410 min
Delta R.T.: -0.066 min
Response: 18869679
Conc: 3.18 ng/ml

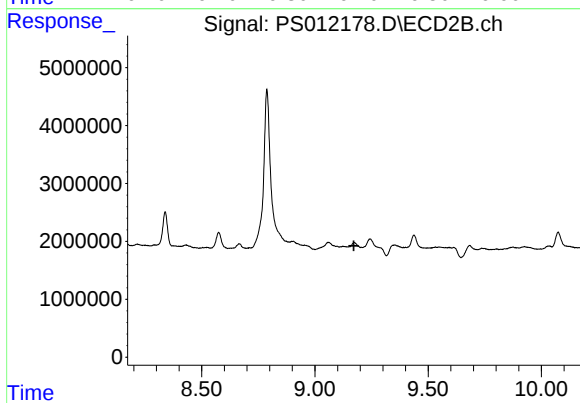

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 9.172 min
Response: 0
Conc: N.D.

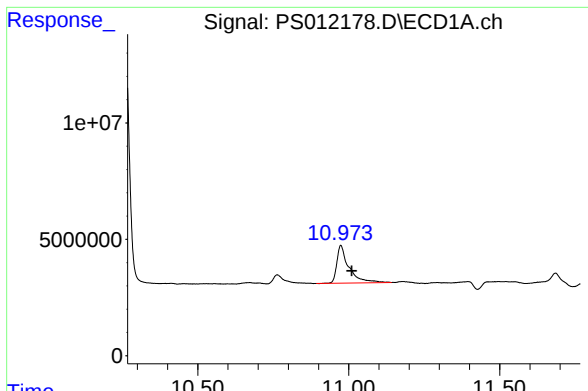

#15 Picloram


R.T.: 10.974 min

Delta R.T.: -0.035 min

Response: 45219678

Conc: 5.79 ng/ml

Instrument :
ECD_S
ClientSampleId :

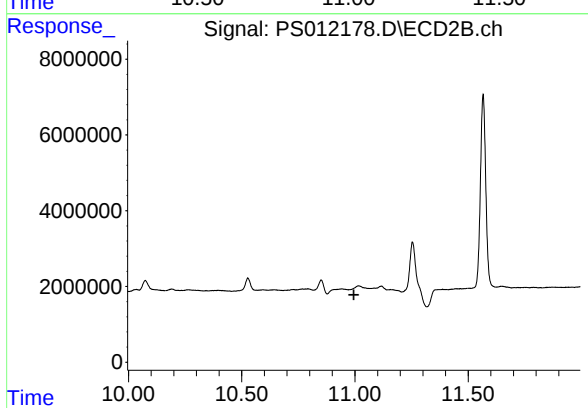

#15 Picloram

R.T.: 0.000 min

Exp R.T. : 10.995 min

Response: 0

Conc: N.D.