

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090920\
 Data File : PS012190.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2020 20:37
 Operator : DD\AJ
 Sample : L3919-17MSD
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-15MSD

Manual Integrations
 APPROVED

Ankita
 9/10/2020 10:21:27 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 01:20:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.199	6.911	7872053	5954006	7.217m	11.133m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090920\
Data File : PS012190.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2020 20:37
Operator : DD\AJ
Sample : L3919-17MSD
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
TP-15MSD


Manual Integrations
APPROVED

Ankita
9/10/2020 10:21:27 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 01:20:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

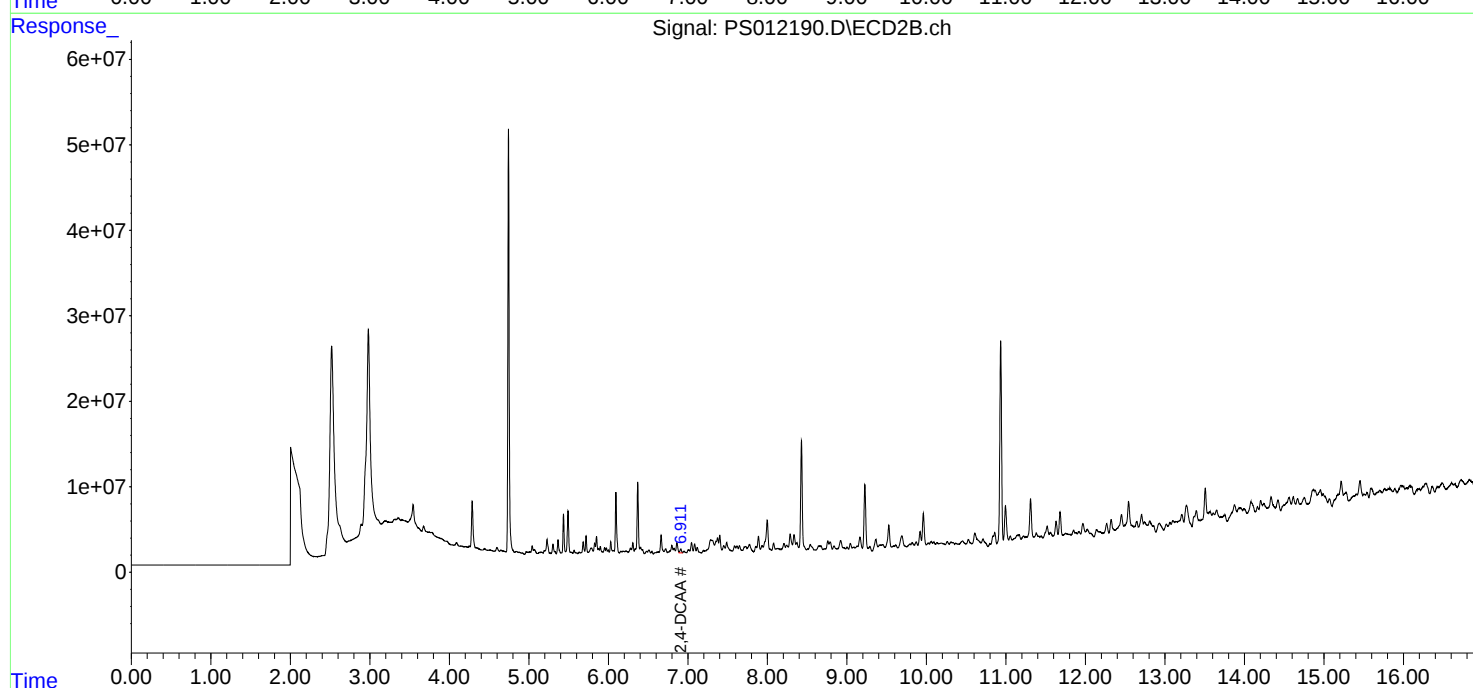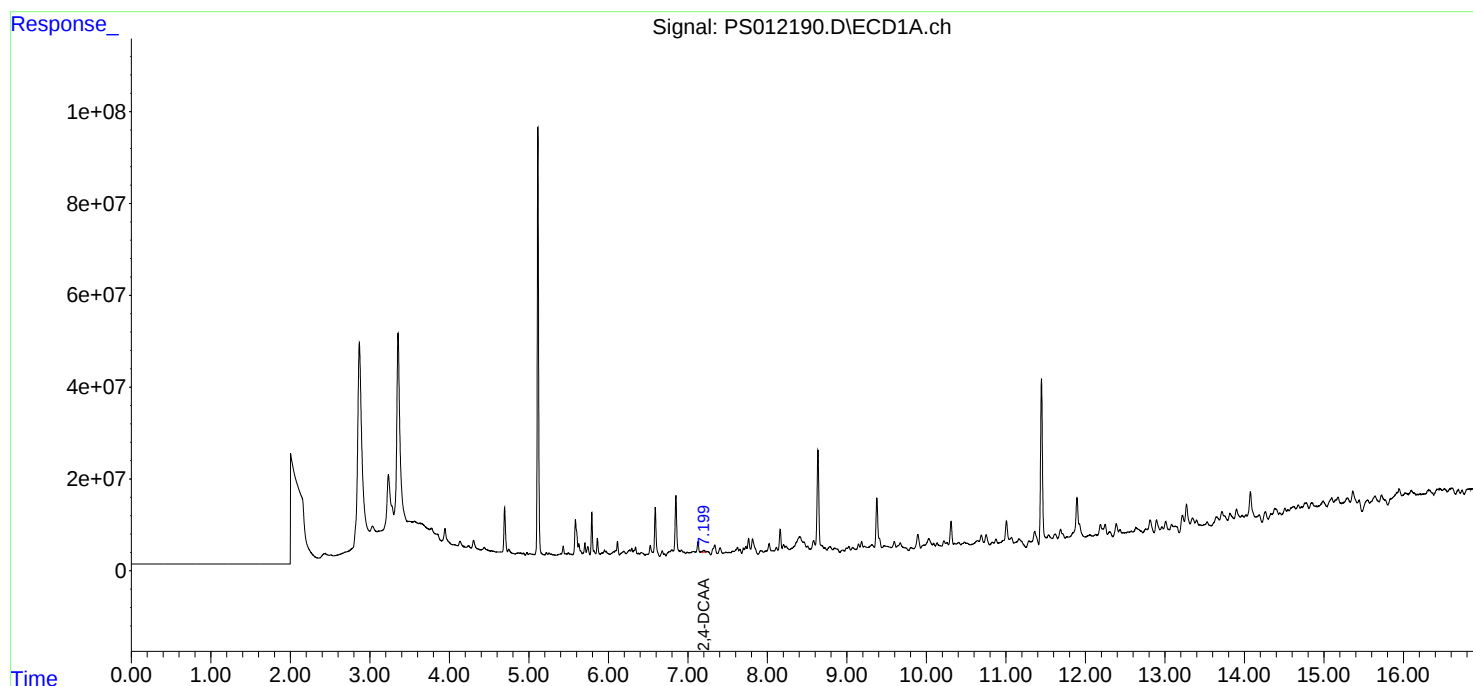

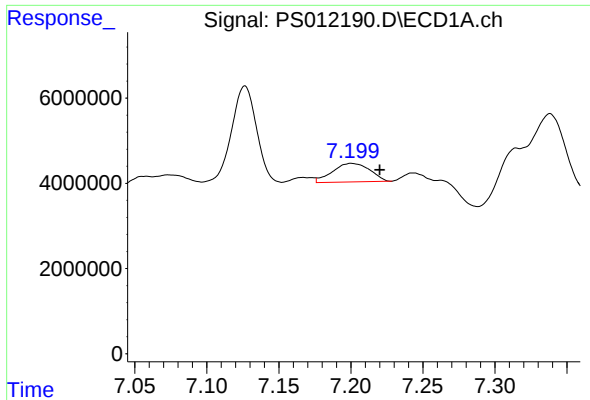


#4 2,4-DCAA

R.T.: 7.199 min
Delta R.T.: -0.021 min
Response: 7872053
Conc: 7.22 ng/ml m

Instrument :
ECD_S
ClientSampleId :
TP-15MSD

Manual Integrations
APPROVED

Ankita
9/10/2020 10:21:27 AM

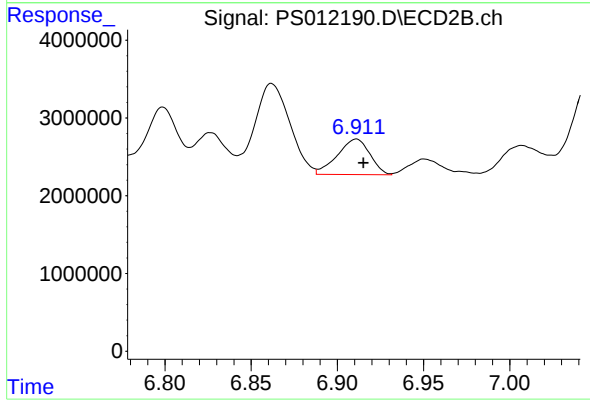

#4 2,4-DCAA

R.T.: 6.911 min
Delta R.T.: -0.004 min
Response: 5954006
Conc: 11.13 ng/ml m