

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091018\
 Data File : PS001680.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2018 18:12
 Operator : EI\SJ
 Sample : J4776-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 02:43:34 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 23 02:55:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.502	10.999	76147738	73845609	412.500	364.616
Target Compounds							
1) T	Dalapon	2.923	2.403	10407523	14434651	41.402	60.313 #
2) T	3,5-DICHL...	0.000	9.087	0	5710916	N.D.	22.347 #
5) T	DICAMBA	0.000	11.242	0	17451328	N.D.	24.883 #
6) T	MCP	12.191	0.000	21268904	0	42.271	N.D. #
15) T	Picloram	17.015	16.879	2978378	-336957	2.126	N.D. #
16) T	DCPA	0.000	16.935	0	3901307	N.D.	2.733 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091018\
Data File : PS001680.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2018 18:12
Operator : EI\SJ
Sample : J4776-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 02:43:34 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
Quant Title : 8080.M
QLast Update : Thu Aug 23 02:55:24 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

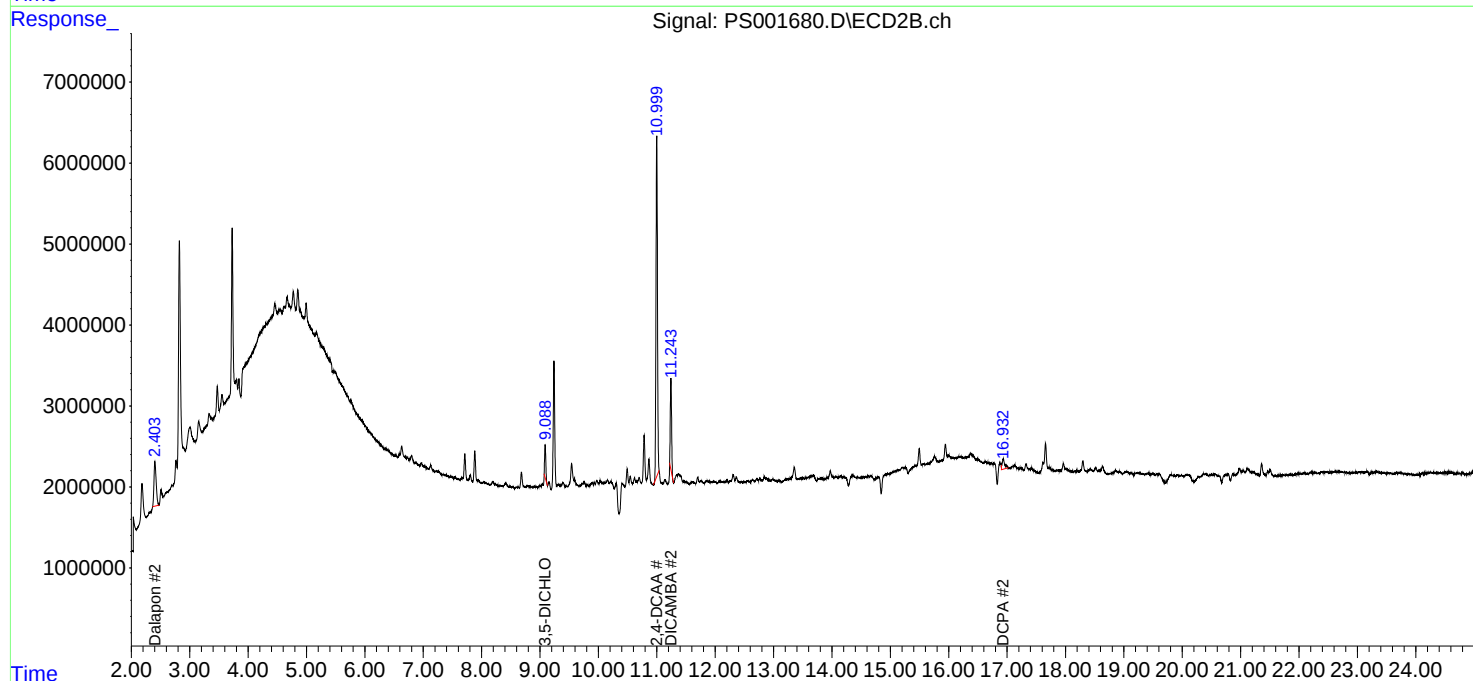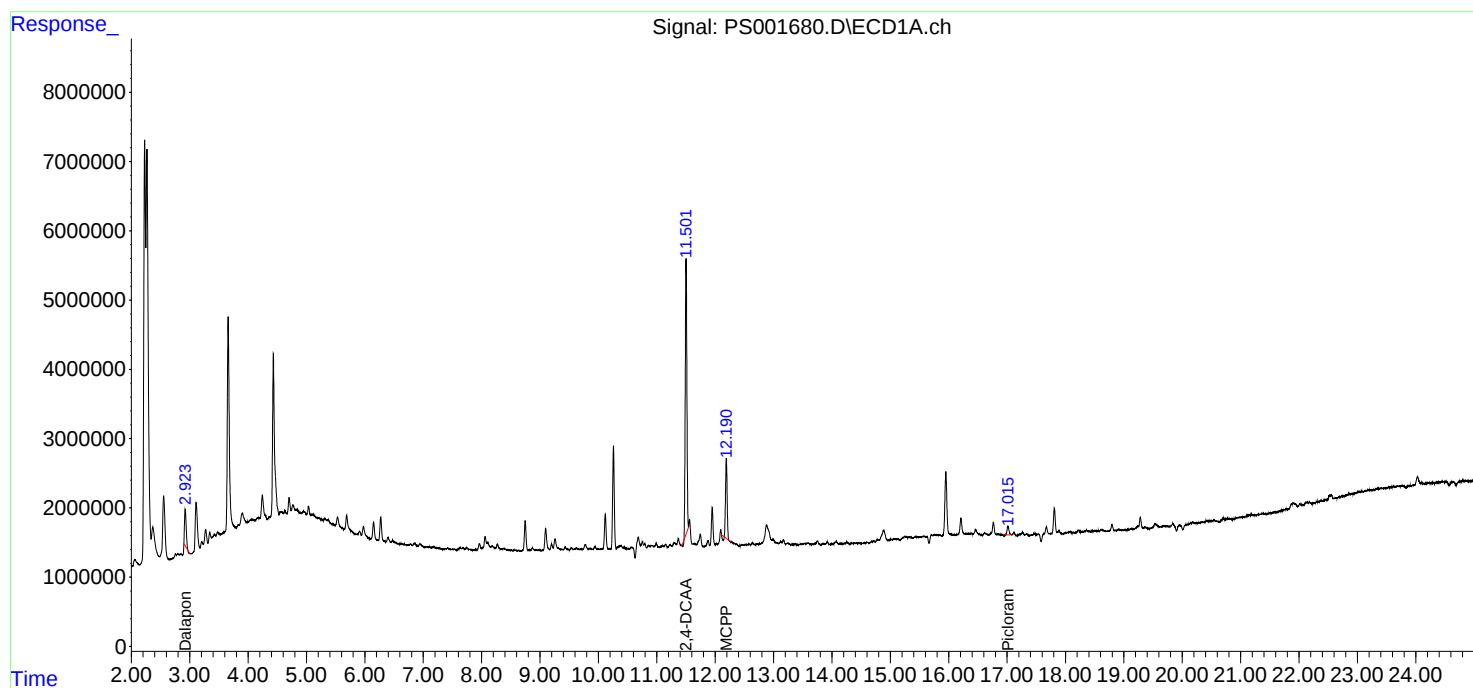


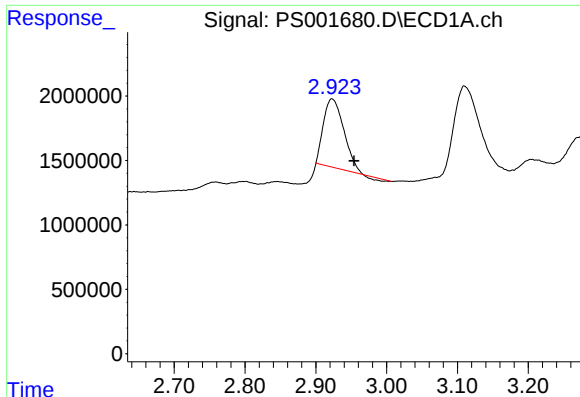

#1 Dalapon


R.T.: 2.923 min
Delta R.T.: -0.031 min
Response: 10407523
Conc: 41.40 ng/ml

Instrument :
ECD_S
ClientSampleId :

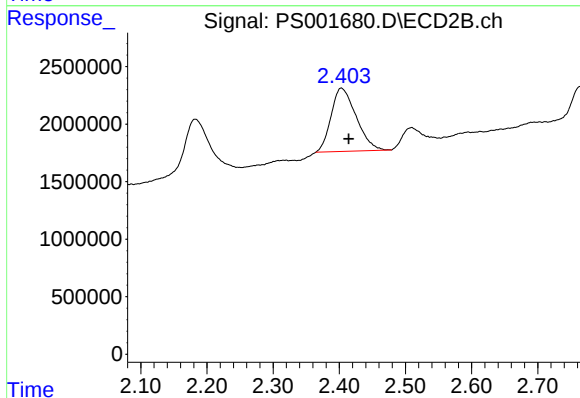


#1 Dalapon

R.T.: 2.403 min
Delta R.T.: -0.011 min
Response: 14434651
Conc: 60.31 ng/ml

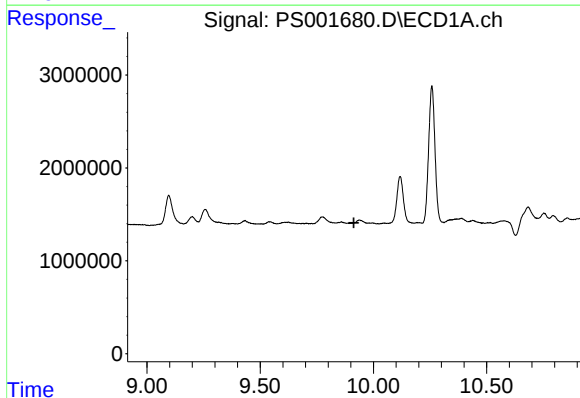


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.914 min
Response: 0
Conc: N.D.

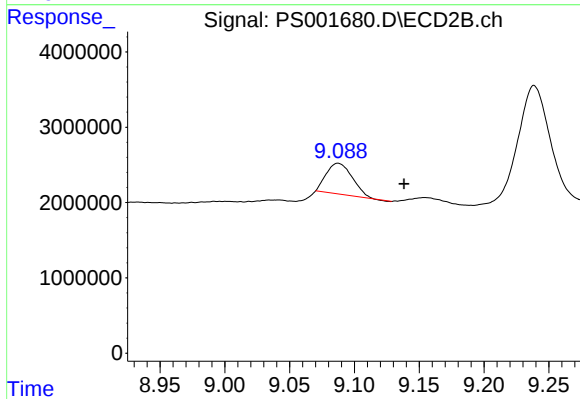

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.087 min
Delta R.T.: -0.051 min
Response: 5710916
Conc: 22.35 ng/ml

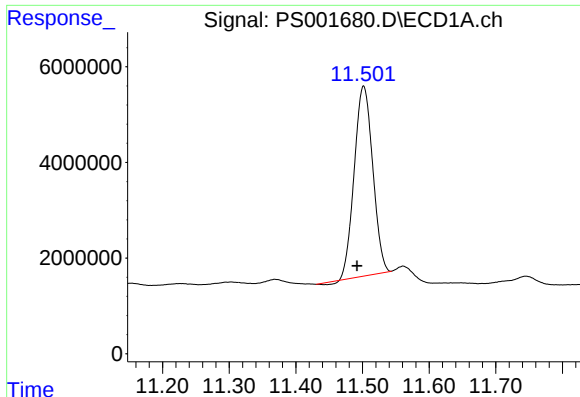

#4 2,4-DCAA


R.T.: 11.502 min
Delta R.T.: 0.010 min
Response: 76147738
Conc: 412.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

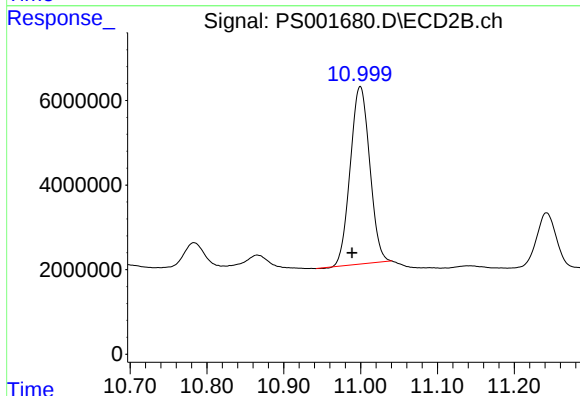


#4 2,4-DCAA

R.T.: 10.999 min
Delta R.T.: 0.011 min
Response: 73845609
Conc: 364.62 ng/ml

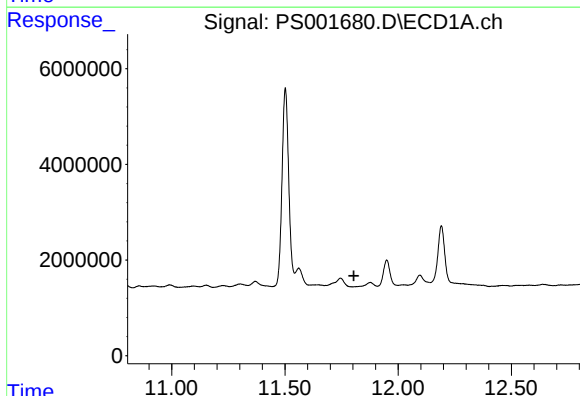


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.805 min
Response: 0
Conc: N.D.

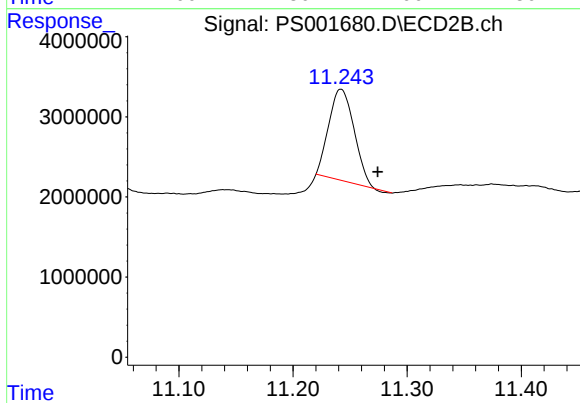

#5 DICAMBA


R.T.: 11.242 min
Delta R.T.: -0.032 min
Response: 17451328
Conc: 24.88 ng/ml

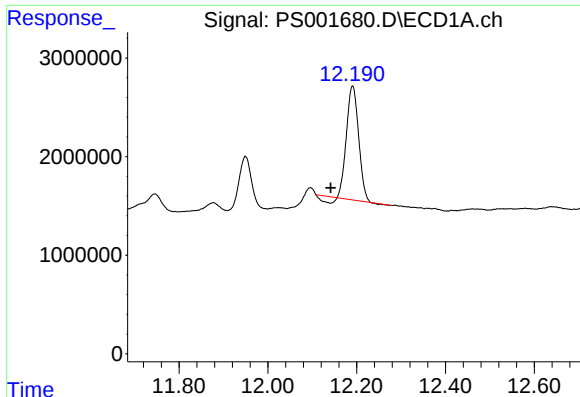

#6 MCP


R.T.: 12.191 min
Delta R.T.: 0.049 min
Response: 21268904
Conc: 42.27 ug/ml

Instrument :
ECD_S
ClientSampleId :

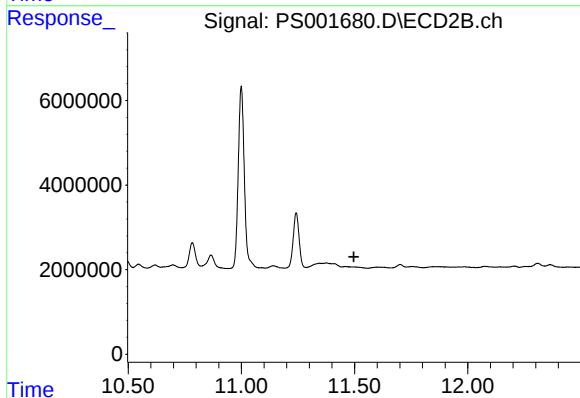


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.497 min
Response: 0
Conc: N.D.

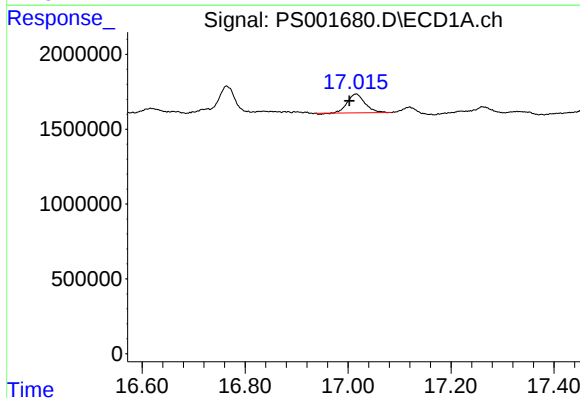


#15 Picloram

R.T.: 17.015 min
Delta R.T.: 0.012 min
Response: 2978378
Conc: 2.13 ng/ml

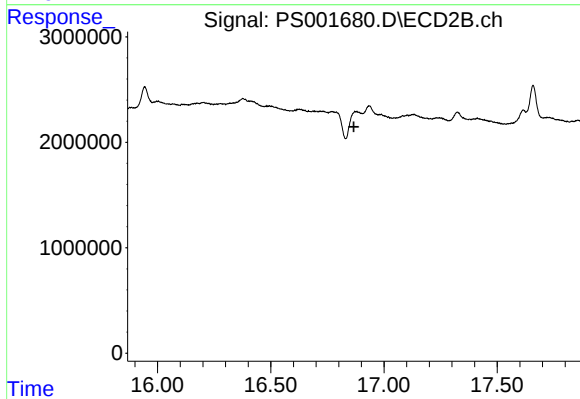

#15 Picloram


R.T.: 16.879 min
Delta R.T.: 0.011 min
Response: -336957
Conc: N.D.

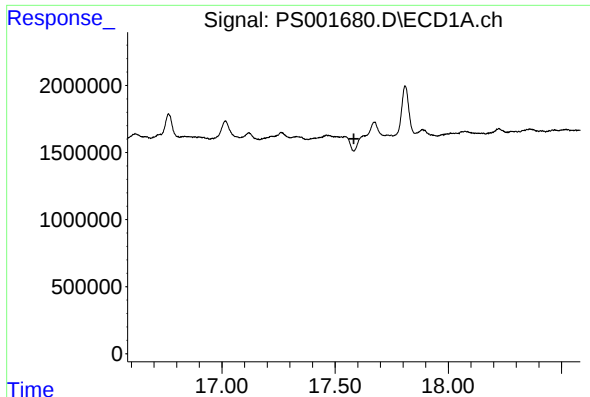

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.583 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

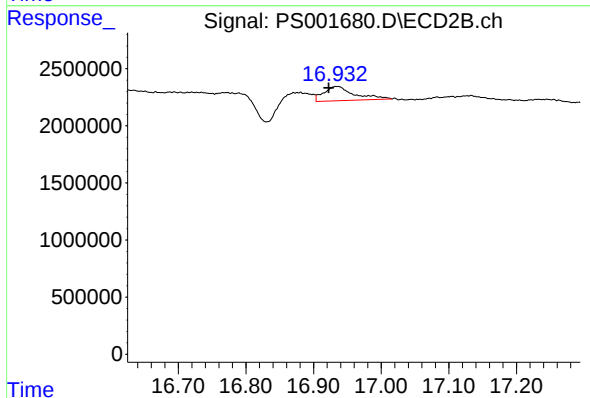

#16 DCPA

R.T.: 16.935 min
Delta R.T.: 0.012 min
Response: 3901307
Conc: 2.73 ng/ml