

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091018\
 Data File : PS001683.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2018 19:45
 Operator : EI\SJ
 Sample : J4777-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 02:43:59 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 23 02:55:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.464	10.964	85782903	88606370	464.695	437.498
Target Compounds							
1) T	Dalapon	2.885	0.000	5800668	0	23.076	N.D. #
2) T	3,5-DICHL...	0.000	9.203	0	33402560	N.D.	130.706 #
5) T	DICAMBA	0.000	11.206	0	4637158	N.D.	6.612 #
6) T	MCP	12.152	0.000	13476716	0	26.784	N.D. #
15) T	Picloram	0.000	16.896	0	5611981	N.D.	4.304 #
16) T	DCPA	0.000	16.896	0	5611981	N.D.	3.931 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091018\
Data File : PS001683.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2018 19:45
Operator : EI\SJ
Sample : J4777-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 02:43:59 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
Quant Title : 8080.M
QLast Update : Thu Aug 23 02:55:24 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

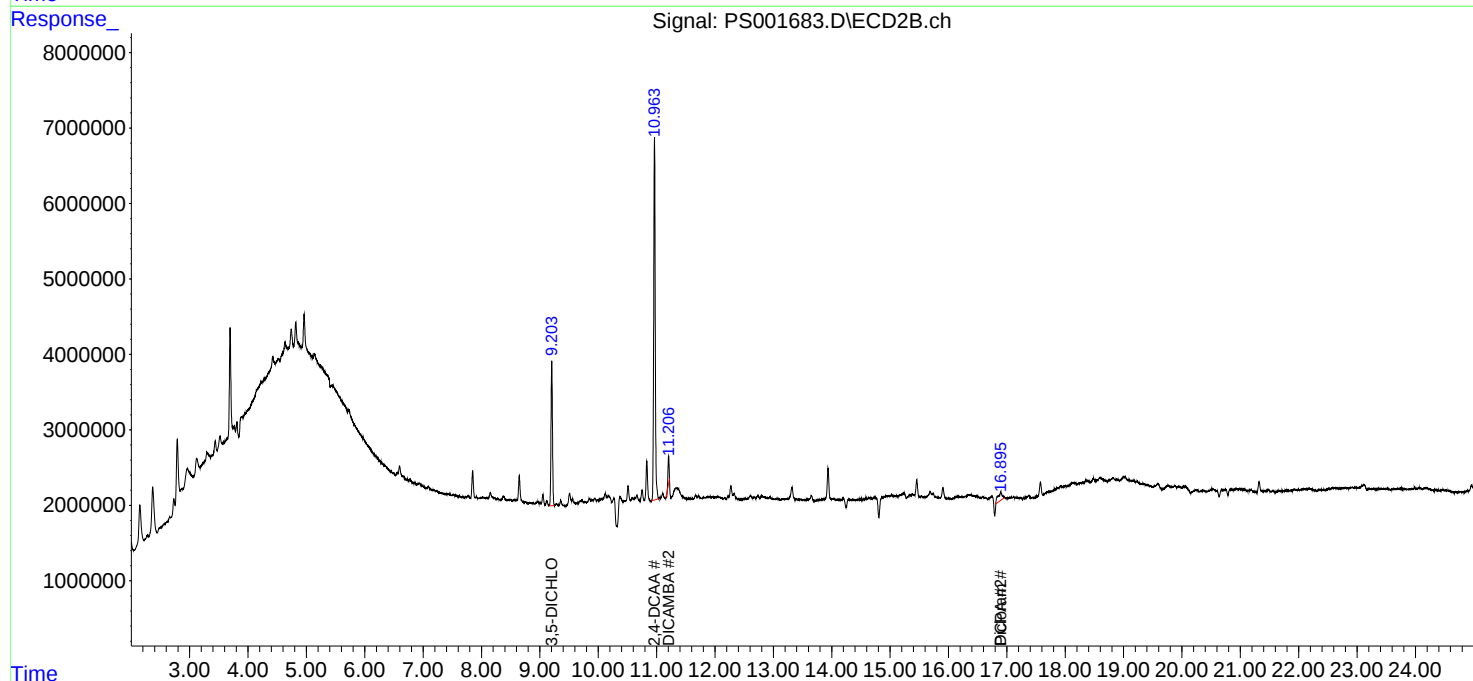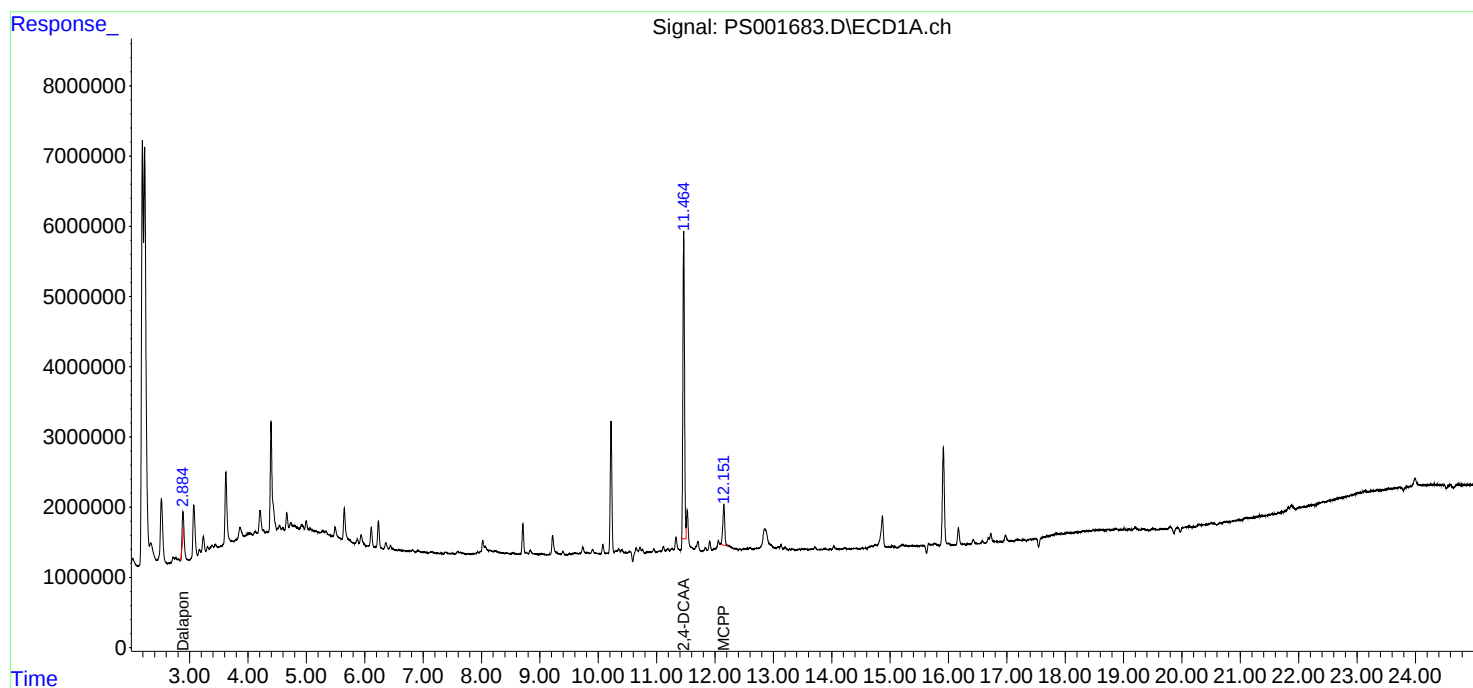


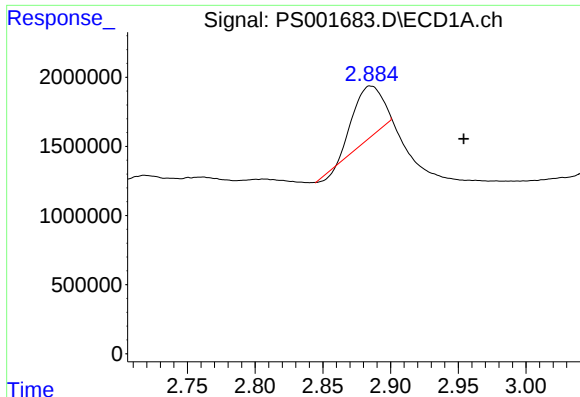

#1 Dalapon


R.T.: 2.885 min
Delta R.T.: -0.069 min
Response: 5800668
Conc: 23.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

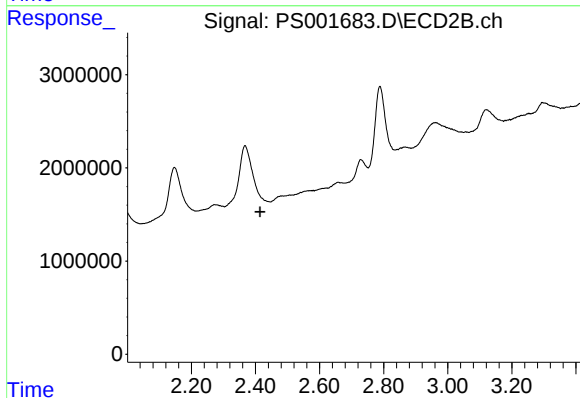


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.414 min
Response: 0
Conc: N.D.

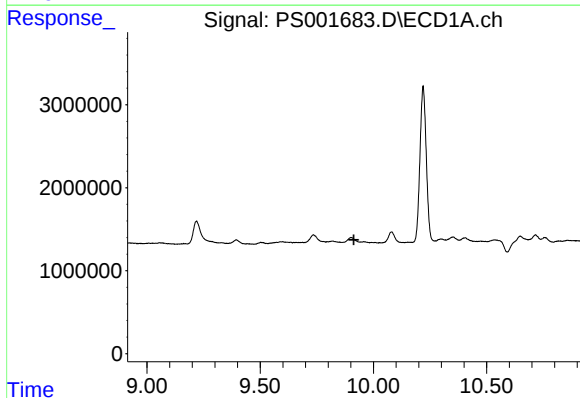


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.914 min
Response: 0
Conc: N.D.

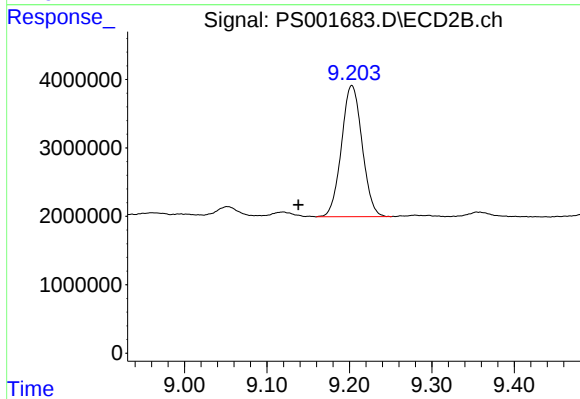

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.203 min
Delta R.T.: 0.065 min
Response: 33402560
Conc: 130.71 ng/ml

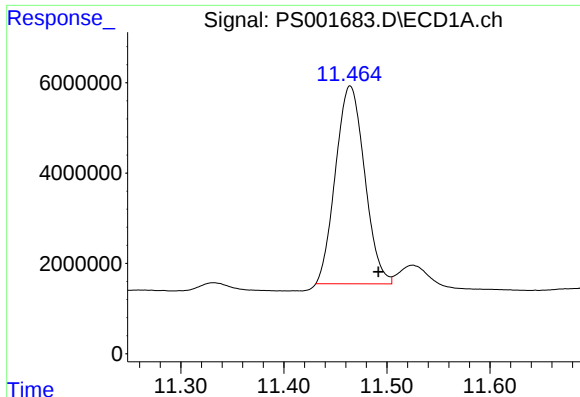

#4 2,4-DCAA


R.T.: 11.464 min
Delta R.T.: -0.027 min
Response: 85782903
Conc: 464.69 ng/ml

Instrument :
ECD_S
ClientSampleId :

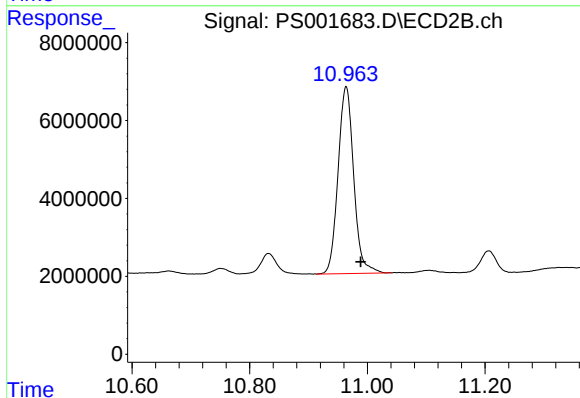


#4 2,4-DCAA

R.T.: 10.964 min
Delta R.T.: -0.025 min
Response: 88606370
Conc: 437.50 ng/ml

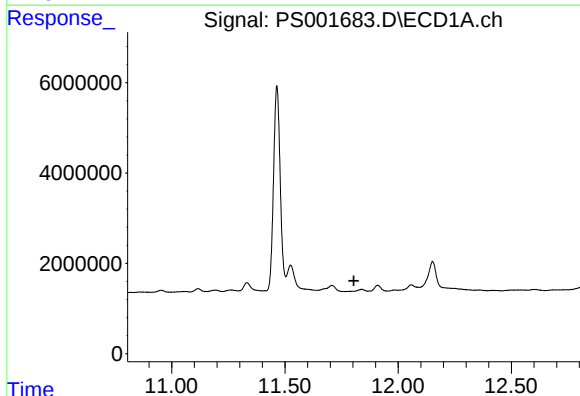


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.805 min
Response: 0
Conc: N.D.

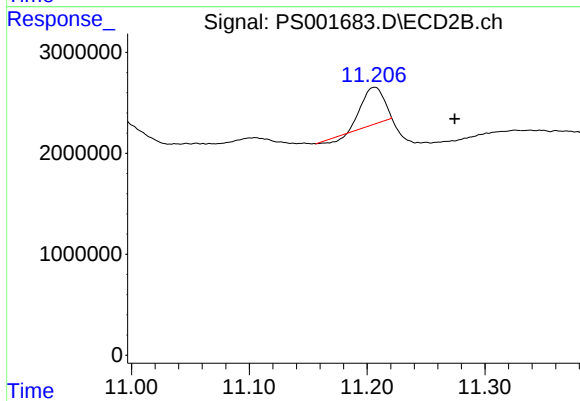

#5 DICAMBA


R.T.: 11.206 min
Delta R.T.: -0.068 min
Response: 4637158
Conc: 6.61 ng/ml

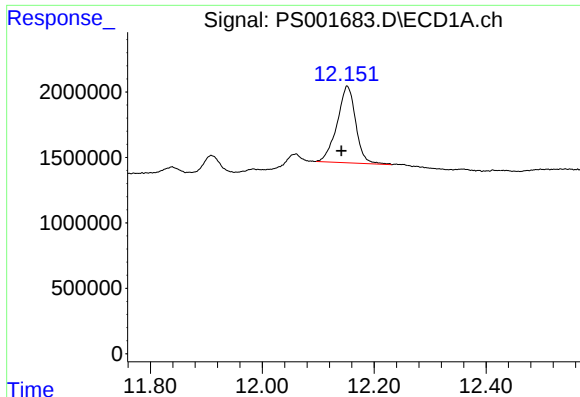

#6 MCPP


R.T.: 12.152 min
Delta R.T.: 0.010 min
Response: 13476716
Conc: 26.78 ug/ml

Instrument :
ECD_S
ClientSampleId :

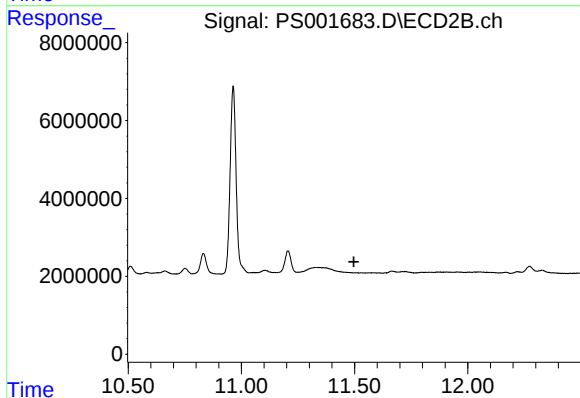


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.497 min
Response: 0
Conc: N.D.

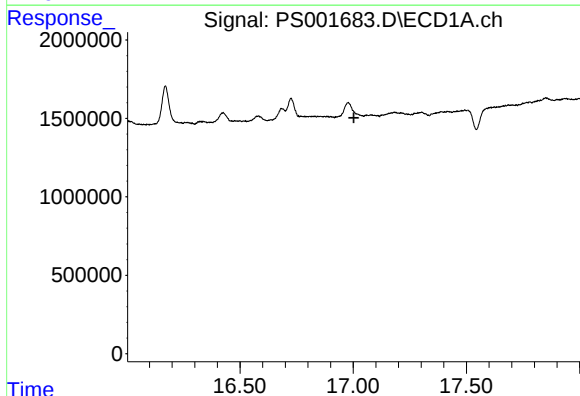


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 17.003 min
Response: 0
Conc: N.D.

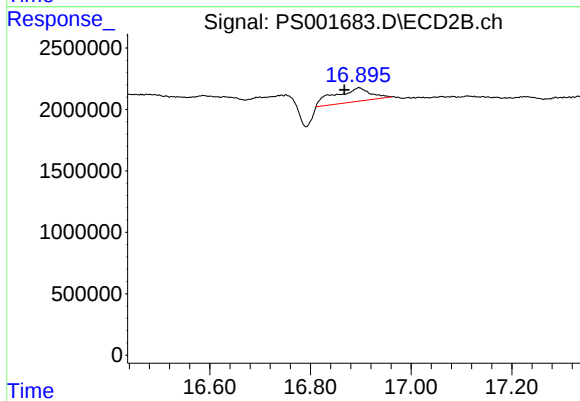

#15 Picloram


R.T.: 16.896 min
Delta R.T.: 0.029 min
Response: 5611981
Conc: 4.30 ng/ml

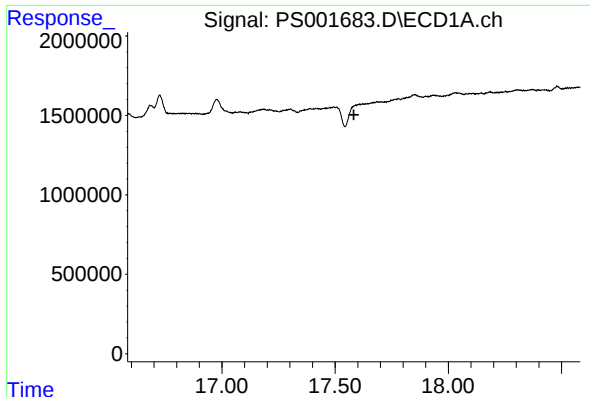

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.583 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

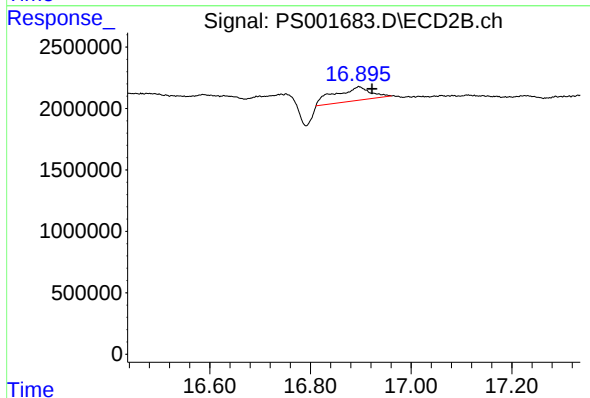

#16 DCPA

R.T.: 16.896 min
Delta R.T.: -0.026 min
Response: 5611981
Conc: 3.93 ng/ml