

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091018\
 Data File : PS001685.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2018 20:48
 Operator : EI\SJ
 Sample : J4777-10
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 02:44:16 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 23 02:55:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.472	10.971	90850046	89737306	492.144	443.082
Target Compounds							
5) T	DICAMBA	0.000	11.213	0	3938837	N.D.	5.616 #
6) T	MCPD	12.161	0.000	14042094	0	27.908	N.D. #
15) T	Picloram	0.000	16.906	0	10413920	N.D.	7.986 #
16) T	DCPA	0.000	16.906	0	10413920	N.D.	7.294 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091018\
Data File : PS001685.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2018 20:48
Operator : EI\SJ
Sample : J4777-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 02:44:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
Quant Title : 8080.M
QLast Update : Thu Aug 23 02:55:24 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

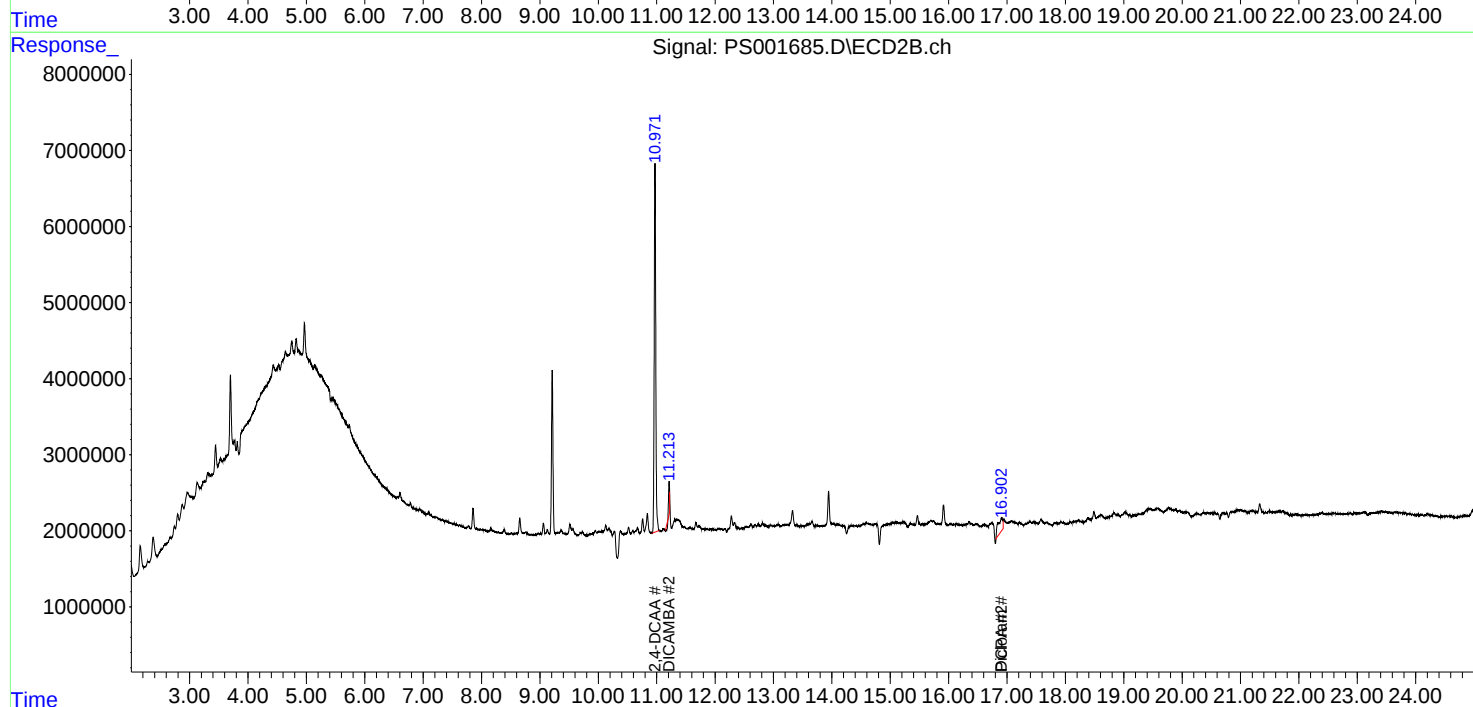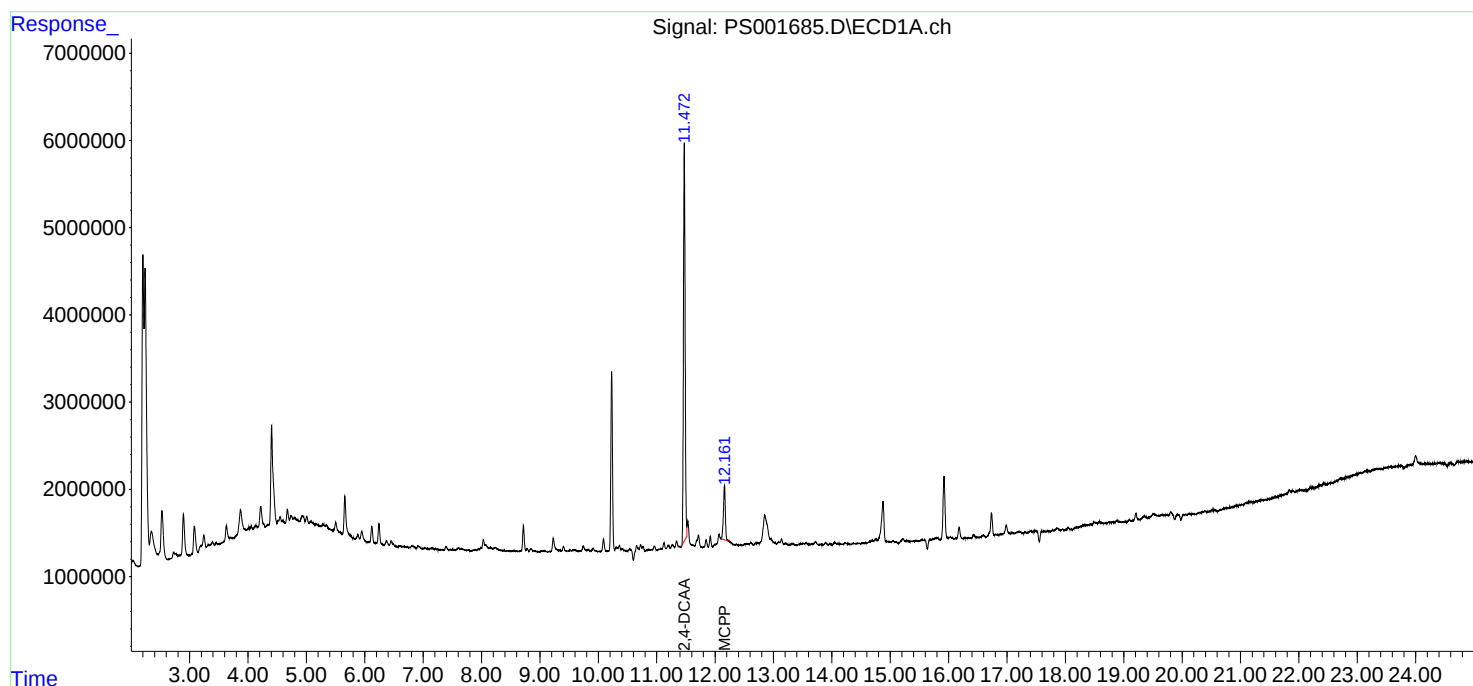


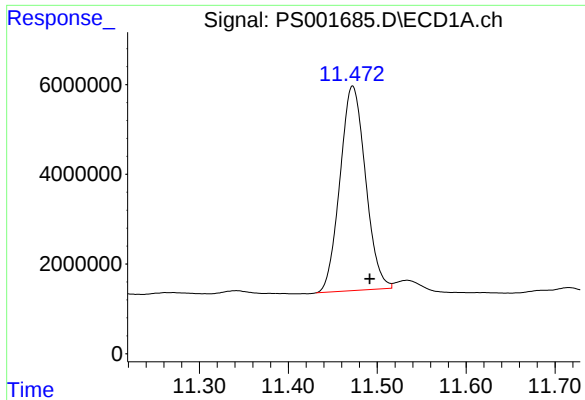

#4 2,4-DCAA


R.T.: 11.472 min
Delta R.T.: -0.019 min
Response: 90850046
Conc: 492.14 ng/ml

Instrument :
ECD_S
ClientSampleId :

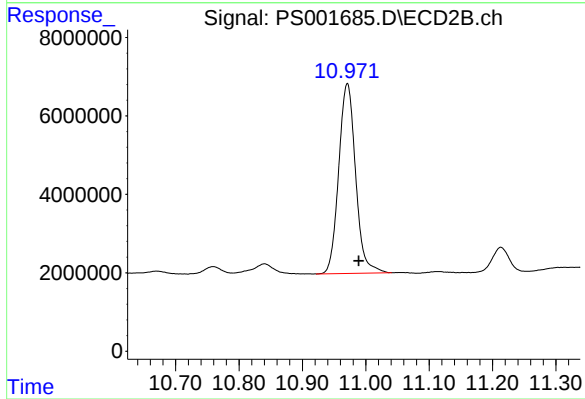


#4 2,4-DCAA

R.T.: 10.971 min
Delta R.T.: -0.018 min
Response: 89737306
Conc: 443.08 ng/ml

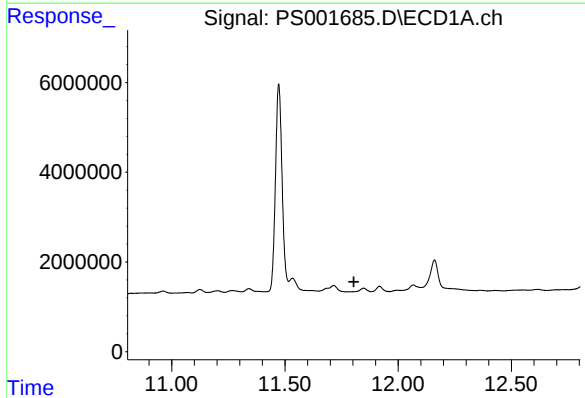


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.805 min
Response: 0
Conc: N.D.

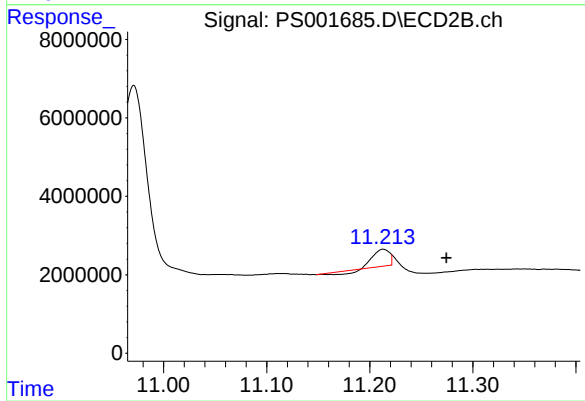

#5 DICAMBA


R.T.: 11.213 min
Delta R.T.: -0.061 min
Response: 3938837
Conc: 5.62 ng/ml

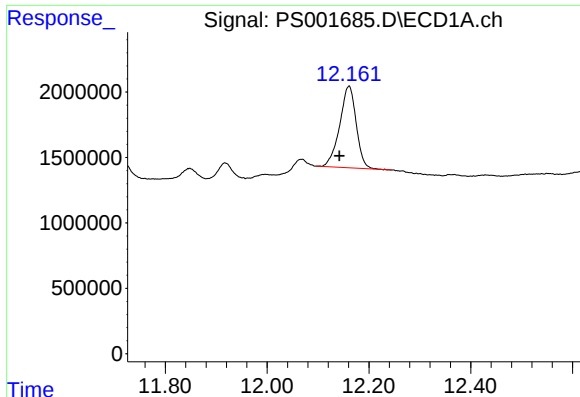

#6 MCP


R.T.: 12.161 min
Delta R.T.: 0.019 min
Response: 14042094
Conc: 27.91 ug/ml

Instrument :
ECD_S
ClientSampleId :

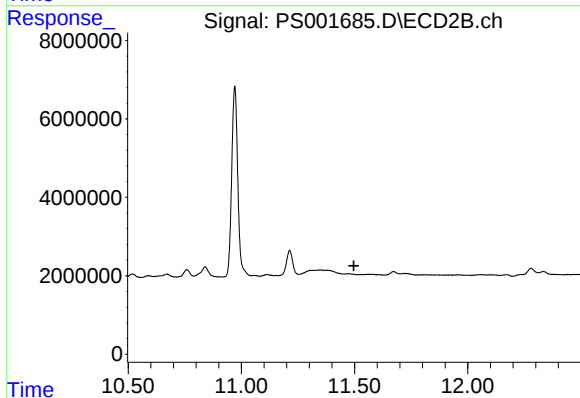


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.497 min
Response: 0
Conc: N.D.

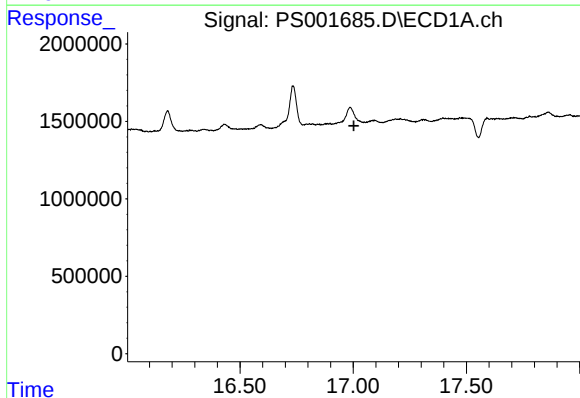


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 17.003 min
Response: 0
Conc: N.D.

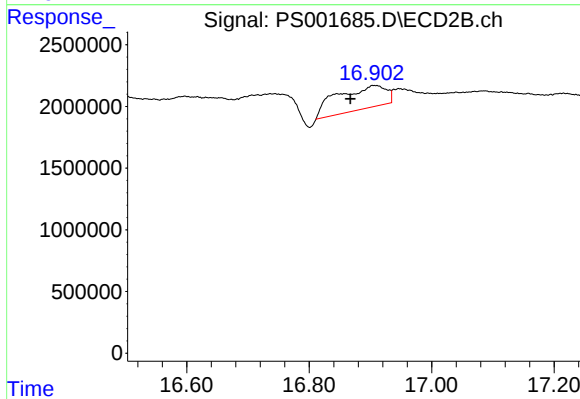

#15 Picloram


R.T.: 16.906 min
Delta R.T.: 0.039 min
Response: 10413920
Conc: 7.99 ng/ml

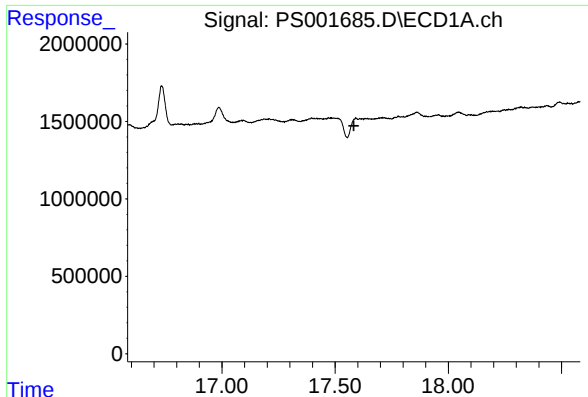

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.583 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

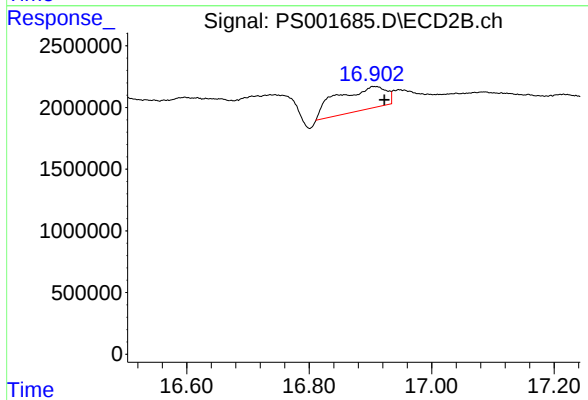

#16 DCPA

R.T.: 16.906 min
Delta R.T.: -0.016 min
Response: 10413920
Conc: 7.29 ng/ml