

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091019\
 Data File : PS006657.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2019 08:50
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 03:12:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 10 06:14:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.488	5.216	318.9E6	172.0E6	410.431	402.789
Target Compounds							
9) T	2,4-D	6.552	0.000	88529722	0	114.583	N.D. #
15) T	Picloram	9.037	8.991	107.2E6	52285889	15.889	14.129
16) T	DCPA	0.000	8.991	0	52285889	N.D.	16.597



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091019\
Data File : PS006657.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2019 08:50
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 03:12:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
Quant Title : 8080.M
QLast Update : Tue Sep 10 06:14:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

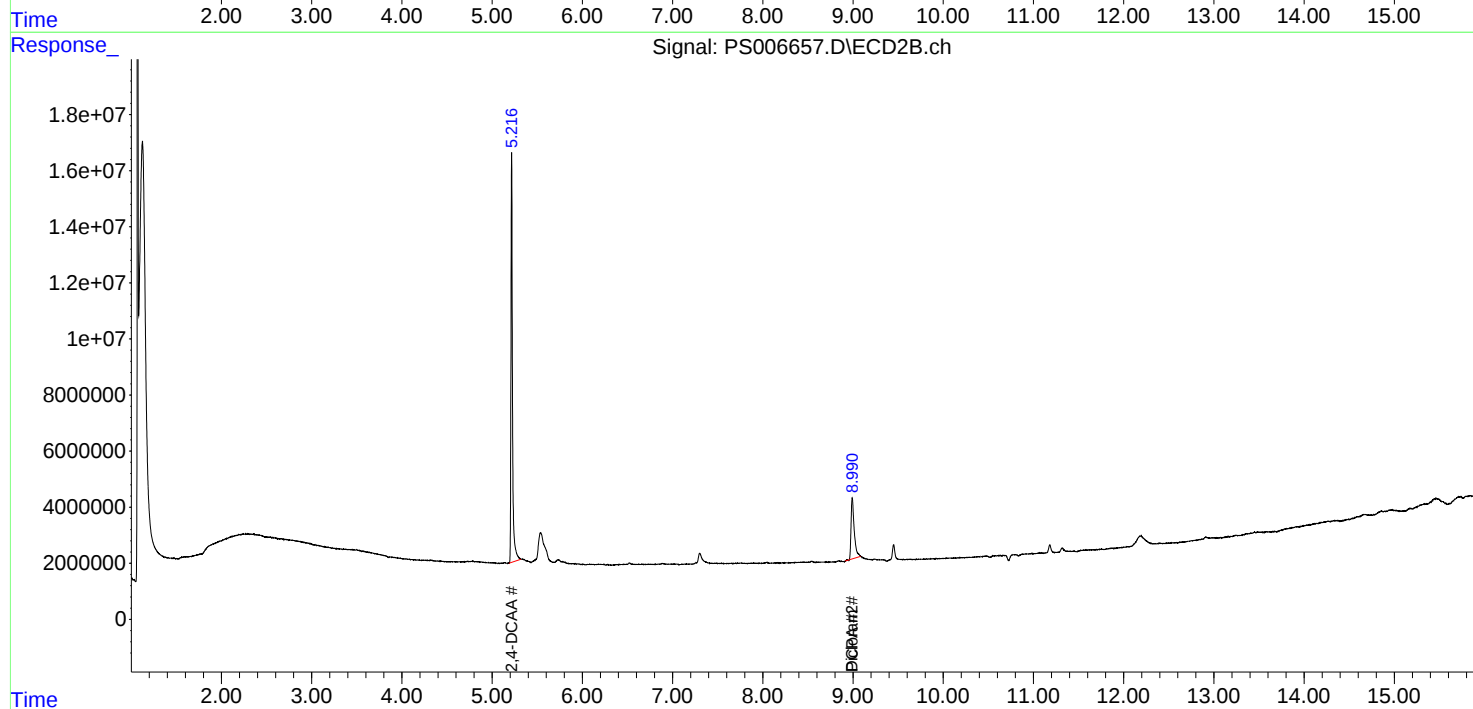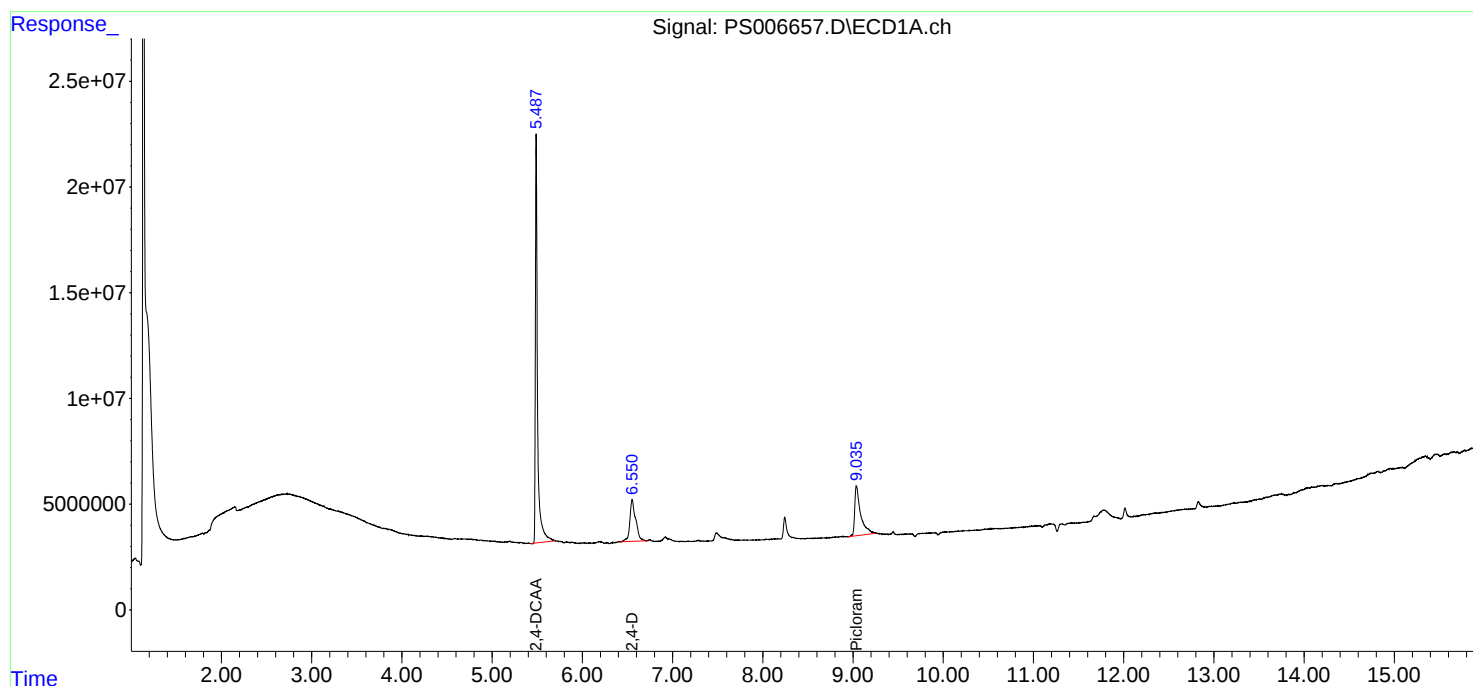


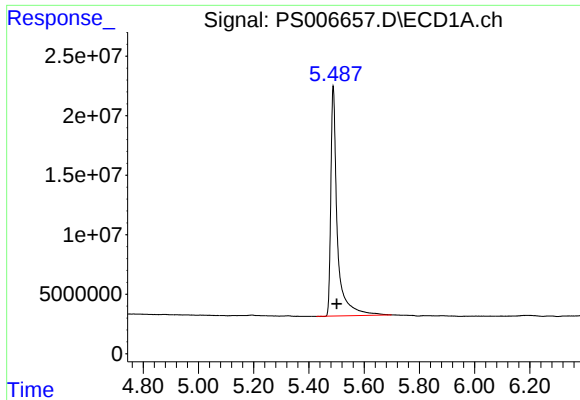

#4 2,4-DCAA


R.T.: 5.488 min
Delta R.T.: -0.012 min
Response: 318858102
Conc: 410.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

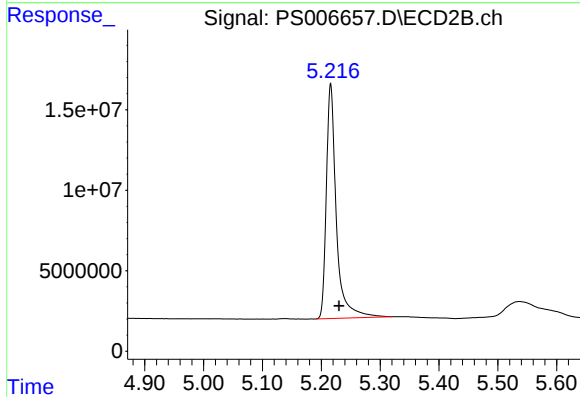


#4 2,4-DCAA

R.T.: 5.216 min
Delta R.T.: -0.014 min
Response: 171992072
Conc: 402.79 ng/ml

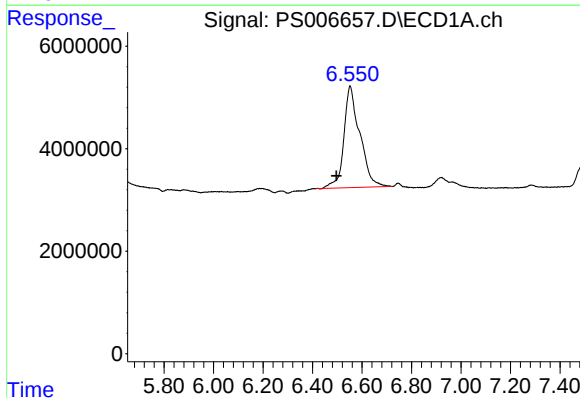


#9 2,4-D

R.T.: 6.552 min
Delta R.T.: 0.055 min
Response: 88529722
Conc: 114.58 ng/ml

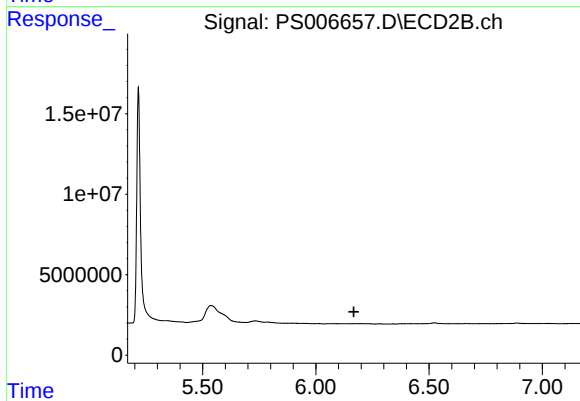

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.168 min
Response: 0
Conc: N.D.

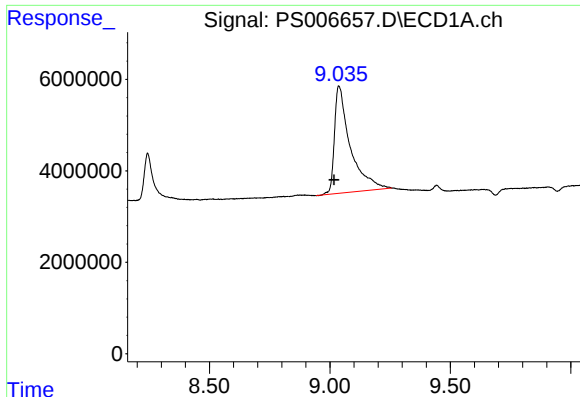

#15 Picloram


R.T.: 9.037 min
Delta R.T.: 0.020 min
Response: 107179287
Conc: 15.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

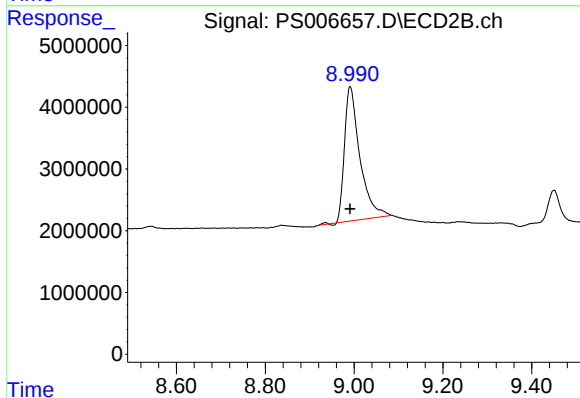


#15 Picloram

R.T.: 8.991 min
Delta R.T.: 0.000 min
Response: 52285889
Conc: 14.13 ng/ml

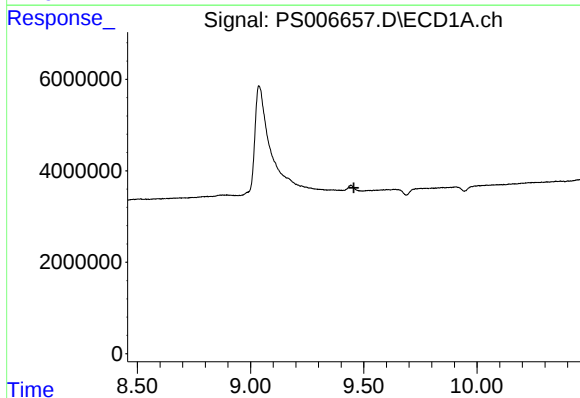

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.456 min
Response: 0
Conc: N.D.

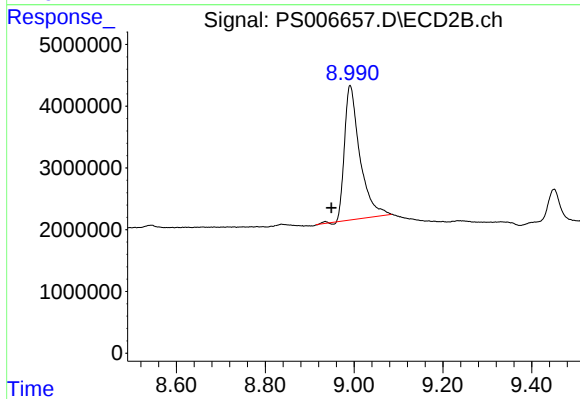

#16 DCPA

R.T.: 8.991 min
Delta R.T.: 0.043 min
Response: 52285889
Conc: 16.60 ng/ml