

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091019\
 Data File : PS006659.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2019 10:27
 Operator : SM\AJ
 Sample : PB122925BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 03:12:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 10 06:14:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.502	5.227	417.3E6	238.2E6	537.205	557.882
Target Compounds							
1) T	Dalapon	2.045	1.754	142.0E6	72697700	145.298	142.252
2) T	3,5-DICHL...	0.000	4.554	0	38391450	N.D.	70.931
5) T	DICAMBA	5.597	0.000	5330987	0	1.849	N.D. #
8) T	DICHLORPROP	6.287	0.000	36016874	0	50.645	N.D. #
10) T	Pentachlo...	6.763	0.000	14139487	0	1.269	N.D. #
15) T	Picloram	9.039	8.999	56792590	34422698	8.419	9.302
16) T	DCPA	0.000	8.999	0	34422698	N.D.	10.927



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091019\
Data File : PS006659.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2019 10:27
Operator : SM\AJ
Sample : PB122925BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 03:12:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
Quant Title : 8080.M
QLast Update : Tue Sep 10 06:14:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

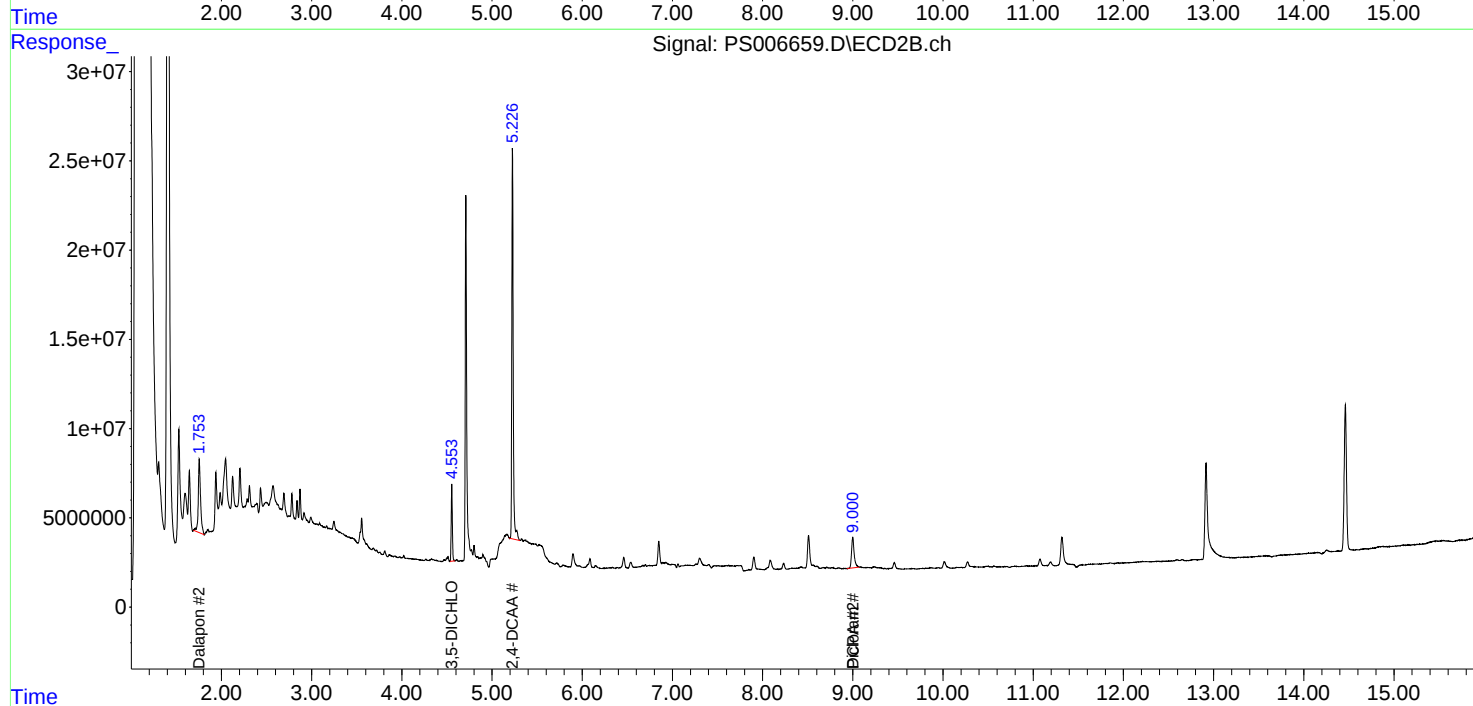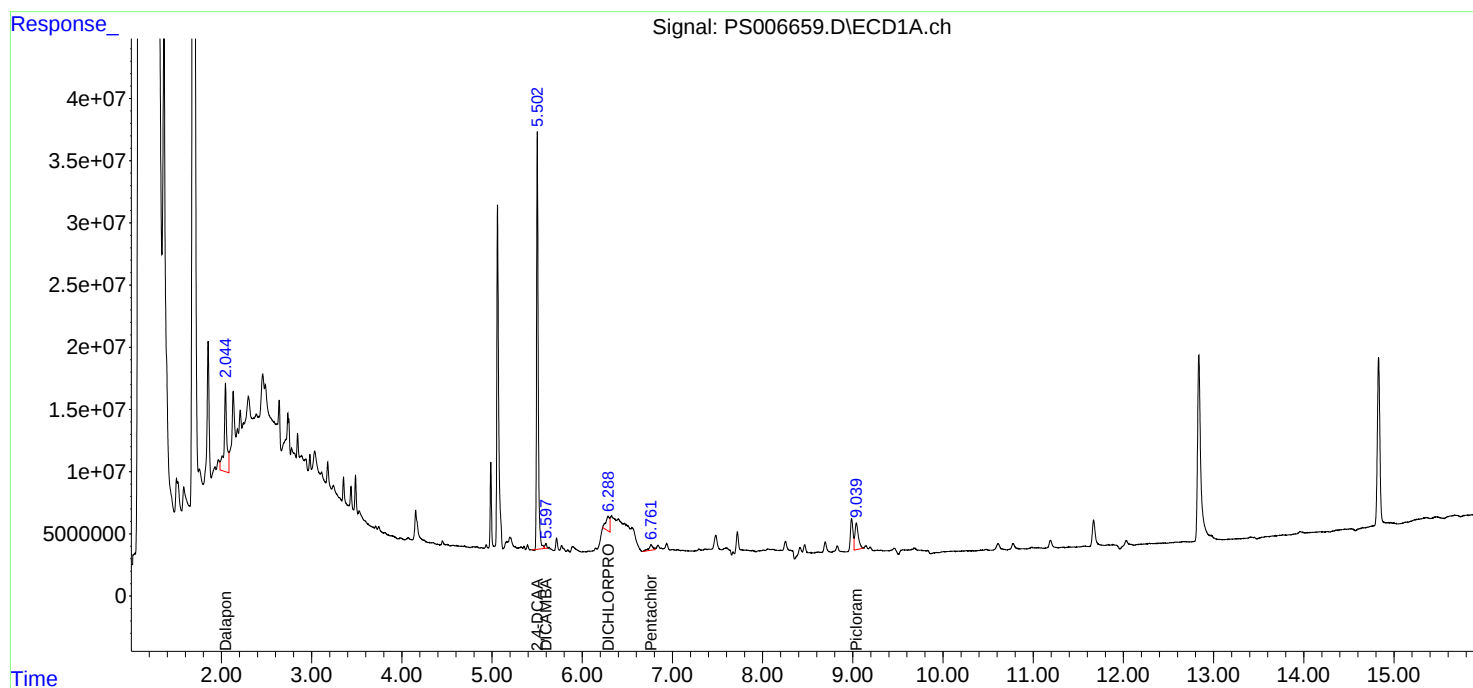


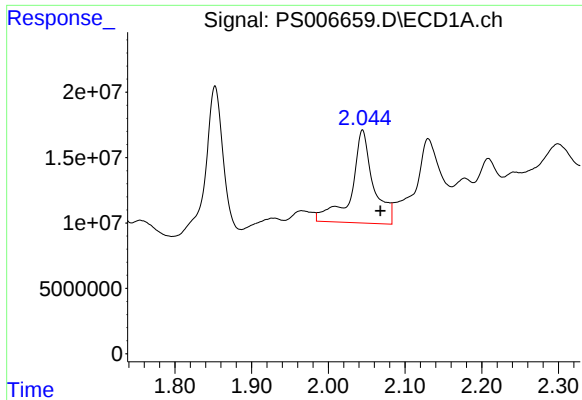

#1 Dalapon


R.T.: 2.045 min
Delta R.T.: -0.023 min
Response: 142014198
Conc: 145.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

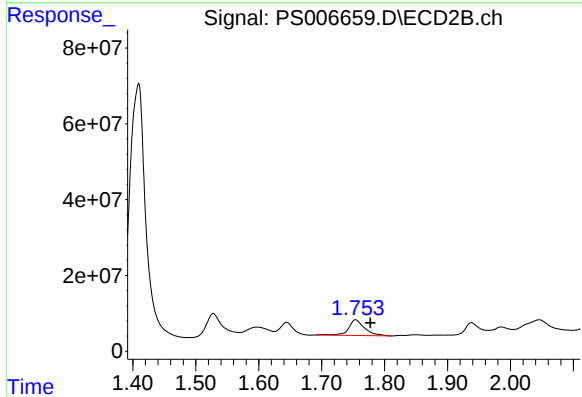


#1 Dalapon

R.T.: 1.754 min
Delta R.T.: -0.023 min
Response: 72697700
Conc: 142.25 ng/ml

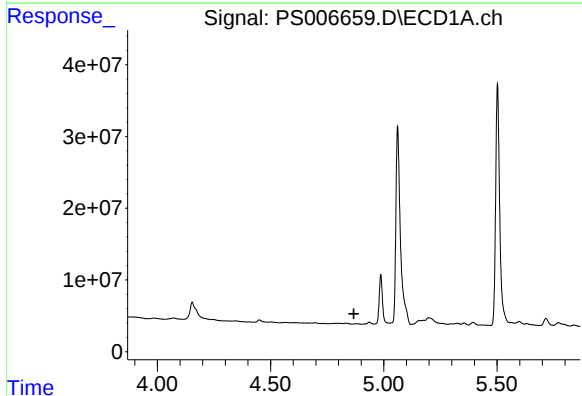


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.868 min
Response: 0
Conc: N.D.

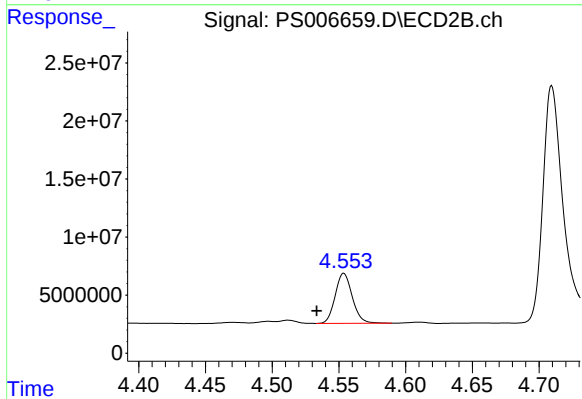

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.554 min
Delta R.T.: 0.020 min
Response: 38391450
Conc: 70.93 ng/ml

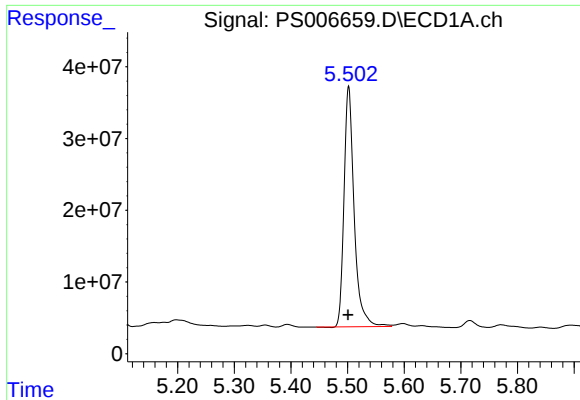

#4 2,4-DCAA


R.T.: 5.502 min
Delta R.T.: 0.001 min
Response: 417346957
Conc: 537.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

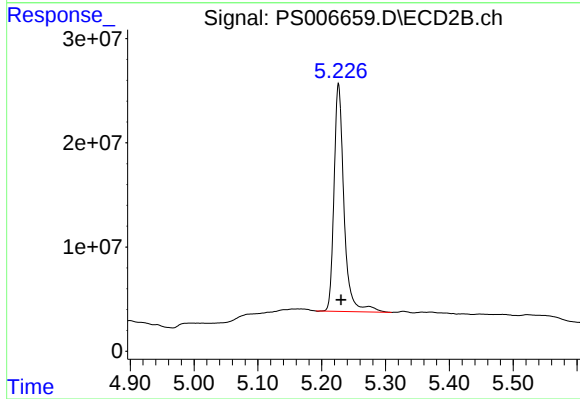


#4 2,4-DCAA

R.T.: 5.227 min
Delta R.T.: -0.004 min
Response: 238217197
Conc: 557.88 ng/ml

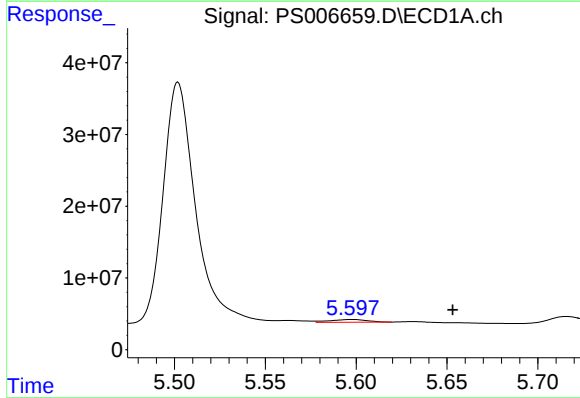


#5 DICAMBA

R.T.: 5.597 min
Delta R.T.: -0.056 min
Response: 5330987
Conc: 1.85 ng/ml

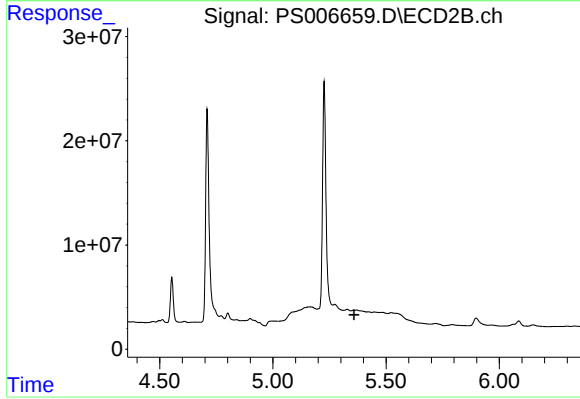

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 5.358 min
Response: 0
Conc: N.D.

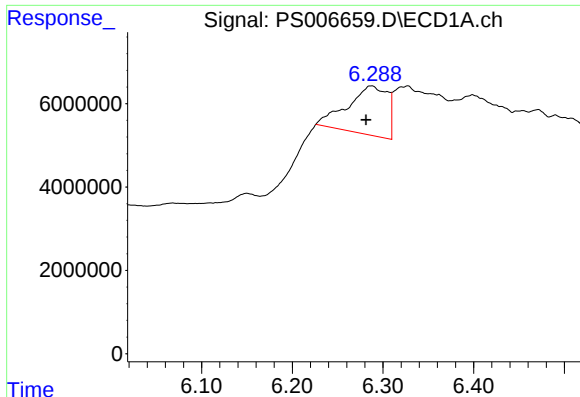

#8 DICHLORPROP


R.T.: 6.287 min
Delta R.T.: 0.006 min
Response: 36016874
Conc: 50.64 ng/ml

Instrument :
ECD_S
ClientSampleId :

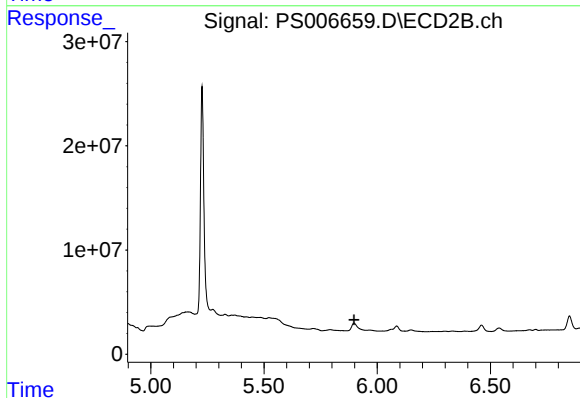


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 5.897 min
Response: 0
Conc: N.D.

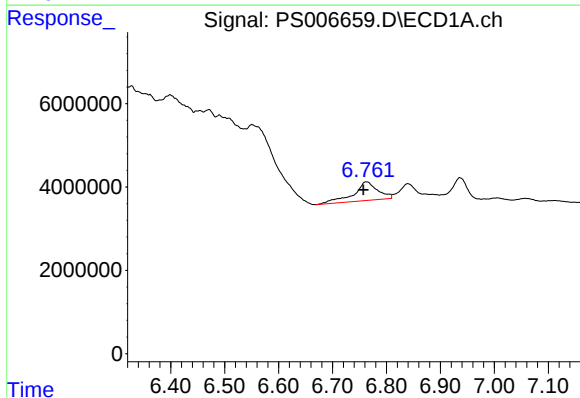


#10 Pentachlorophenol

R.T.: 6.763 min
Delta R.T.: 0.006 min
Response: 14139487
Conc: 1.27 ng/ml

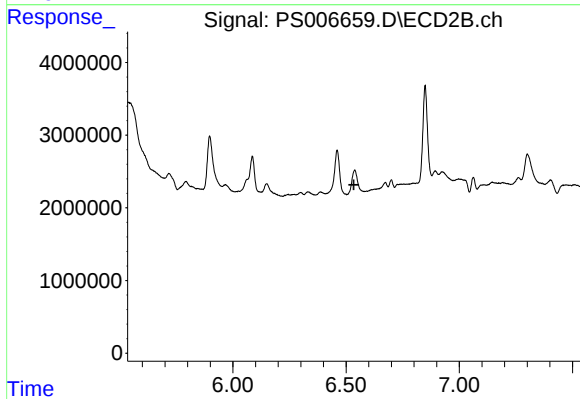

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 6.535 min
Response: 0
Conc: N.D.

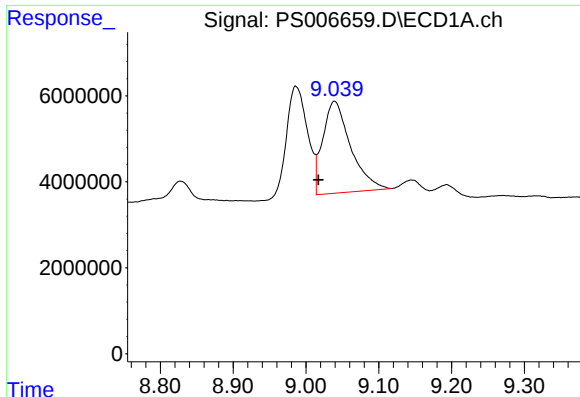

#15 Picloram


R.T.: 9.039 min
Delta R.T.: 0.022 min
Response: 56792590
Conc: 8.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

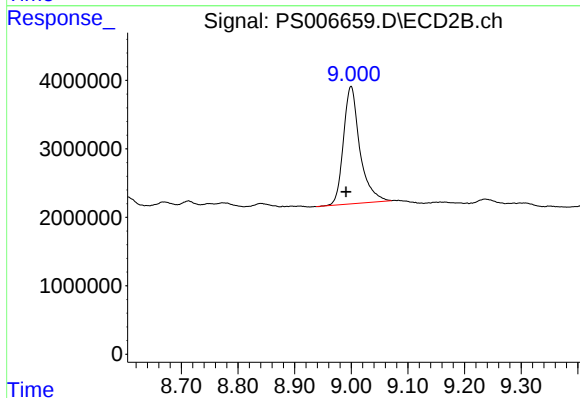


#15 Picloram

R.T.: 8.999 min
Delta R.T.: 0.008 min
Response: 34422698
Conc: 9.30 ng/ml

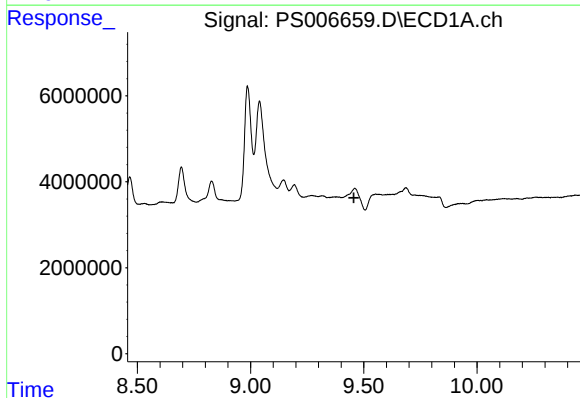

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.456 min
Response: 0
Conc: N.D.

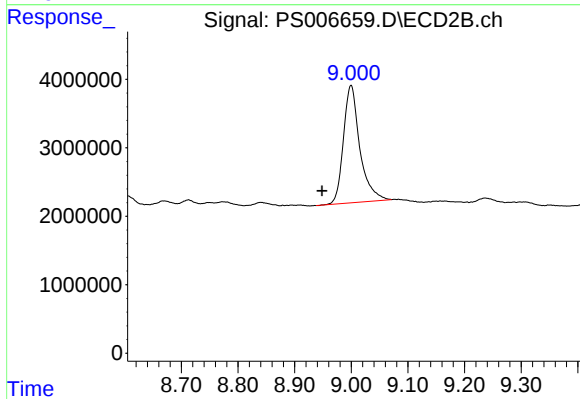

#16 DCPA

R.T.: 8.999 min
Delta R.T.: 0.051 min
Response: 34422698
Conc: 10.93 ng/ml